

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091019\
 Data File : PS006660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2019 10:49
 Operator : SM\AJ
 Sample : K4658-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 03:13:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.214	376.2E6	219.7E6	484.227	514.424
Target Compounds							
1) T	Dalapon	2.030	1.743	77835600	59734137	79.635	116.885 #
2) T	3,5-DICHL...	4.868	4.542	10548237	29099477	10.655	53.763 #
5) T	DICAMBA	5.699	0.000	6628288	0	2.299	N.D. #
9) T	2,4-D	6.551	0.000	91226872	0	118.074	N.D. #
10) T	Pentachlo...	6.822	0.000	5864471	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.837	0	6880052	N.D.	3.022
15) T	Picloram	8.970	0.000	50420251	0	7.474	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091019\
Data File : PS006660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2019 10:49
Operator : SM\AJ
Sample : K4658-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:13:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

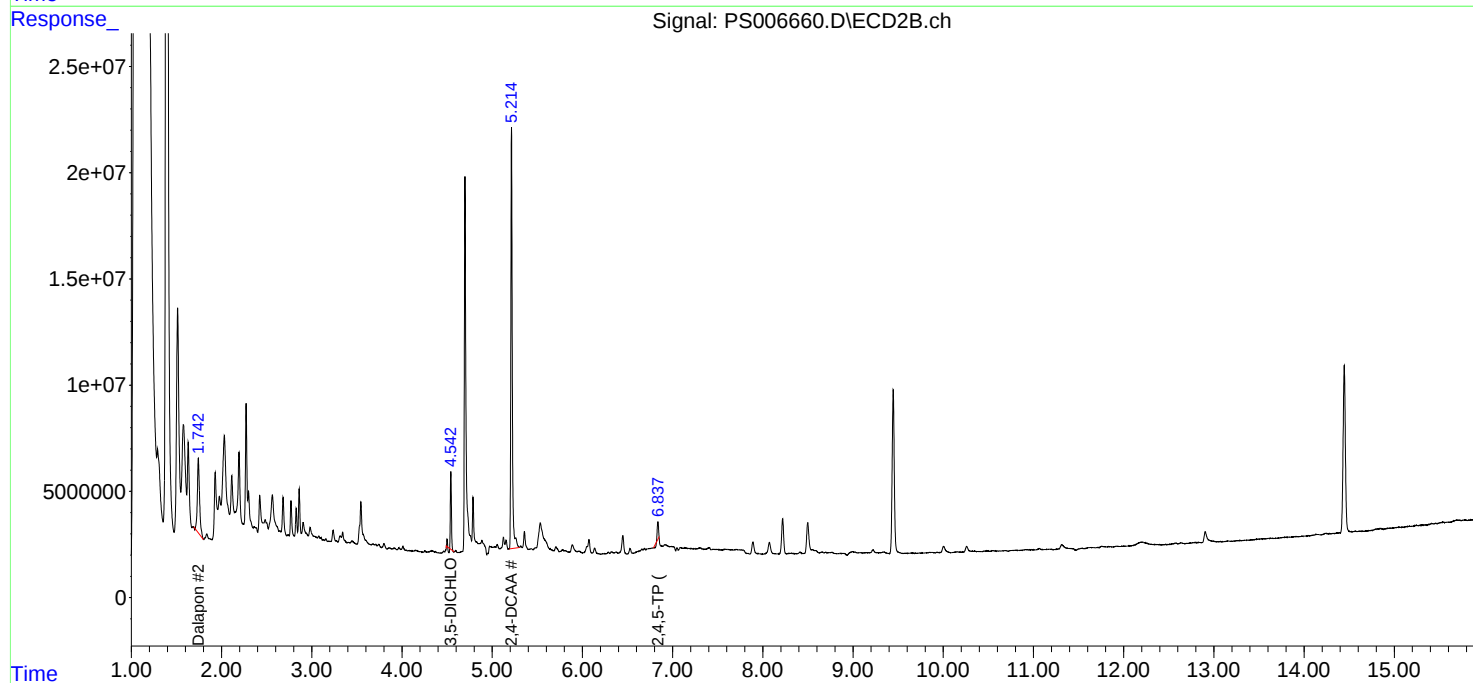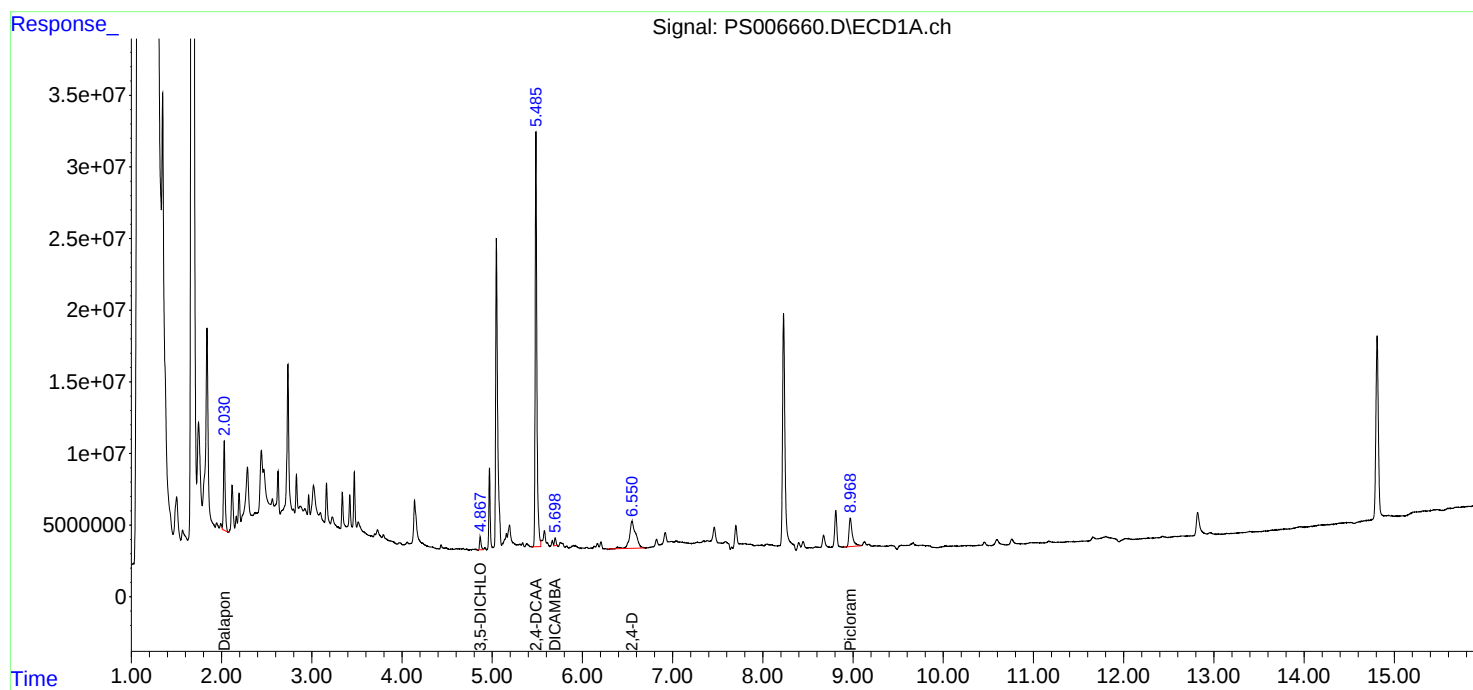


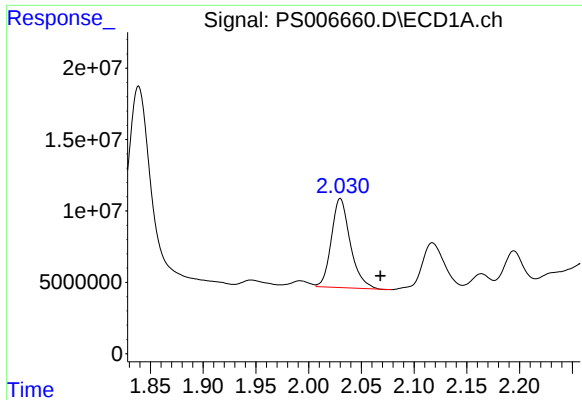

#1 Dalapon


R.T.: 2.030 min
Delta R.T.: -0.038 min
Response: 77835600
Conc: 79.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

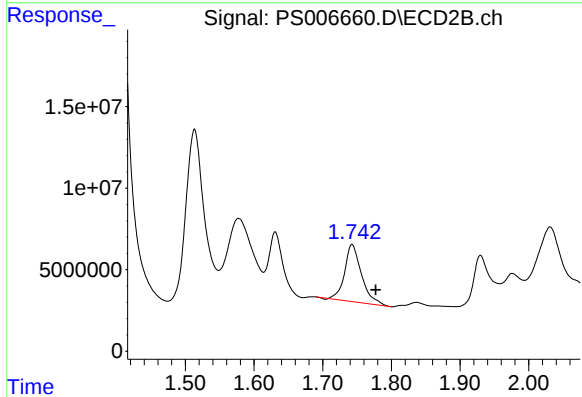


#1 Dalapon

R.T.: 1.743 min
Delta R.T.: -0.035 min
Response: 59734137
Conc: 116.89 ng/ml

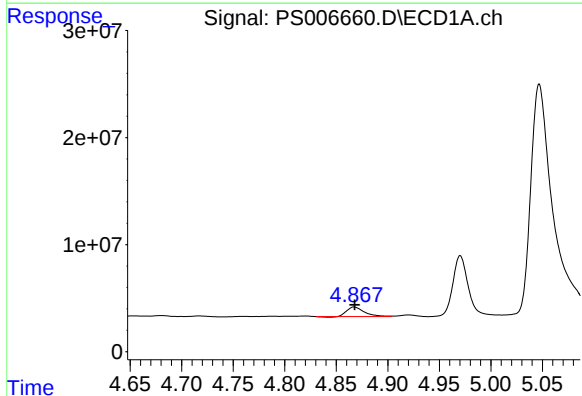


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 10548237
Conc: 10.65 ng/ml

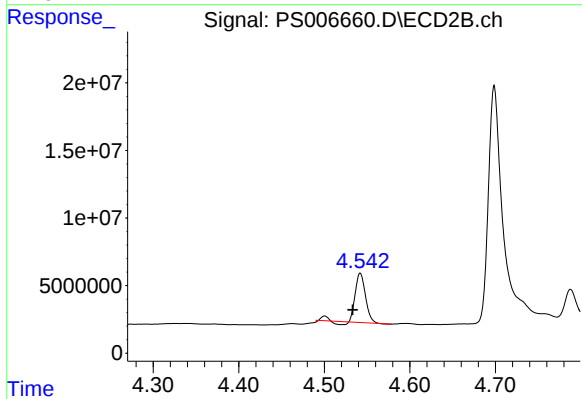

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.542 min
Delta R.T.: 0.009 min
Response: 29099477
Conc: 53.76 ng/ml

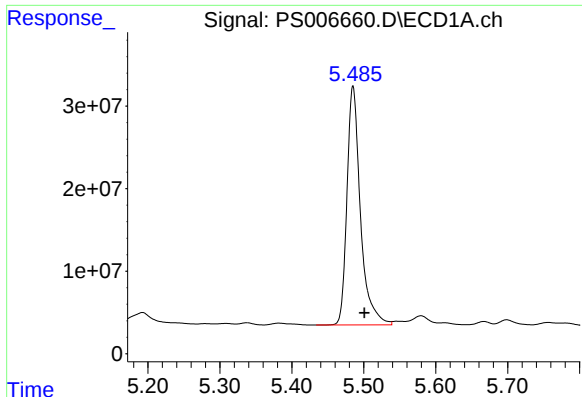

#4 2,4-DCAA


R.T.: 5.485 min
Delta R.T.: -0.015 min
Response: 376189007
Conc: 484.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

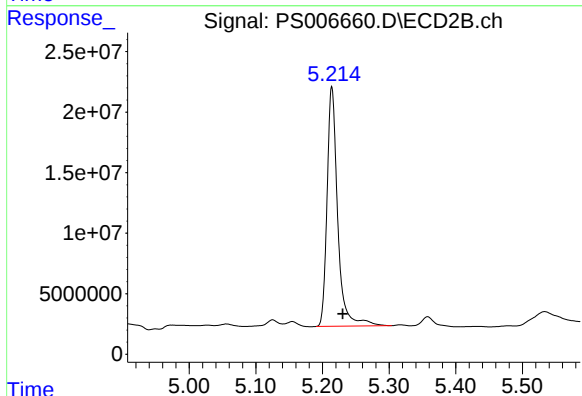


#4 2,4-DCAA

R.T.: 5.214 min
Delta R.T.: -0.016 min
Response: 219660386
Conc: 514.42 ng/ml

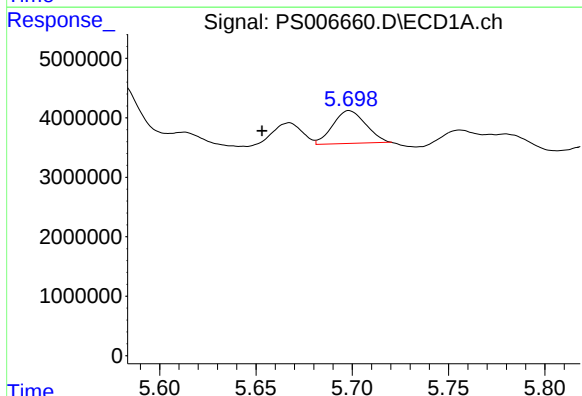


#5 DICAMBA

R.T.: 5.699 min
Delta R.T.: 0.045 min
Response: 6628288
Conc: 2.30 ng/ml

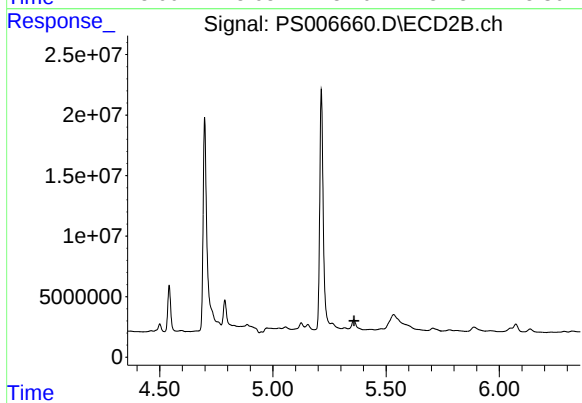

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.358 min
Response: 0
Conc: N.D.

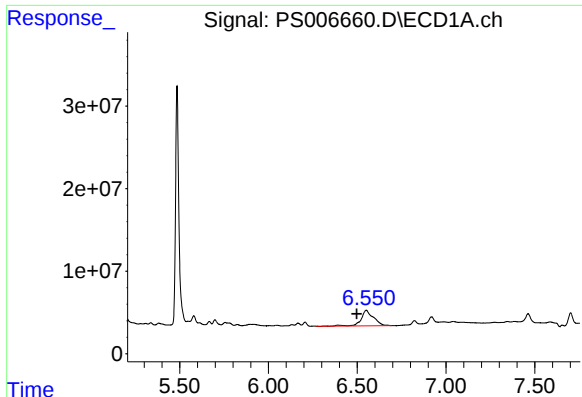

#9 2,4-D


R.T.: 6.551 min
Delta R.T.: 0.054 min
Response: 91226872
Conc: 118.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

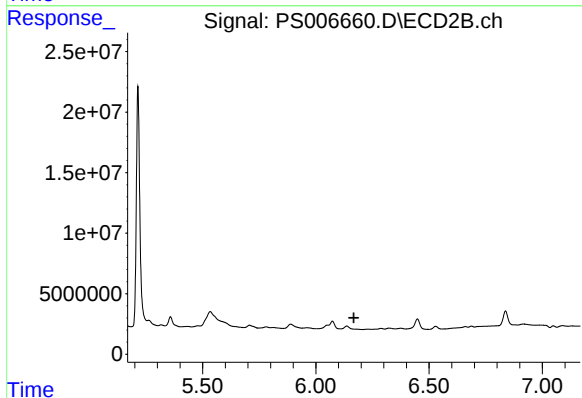


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

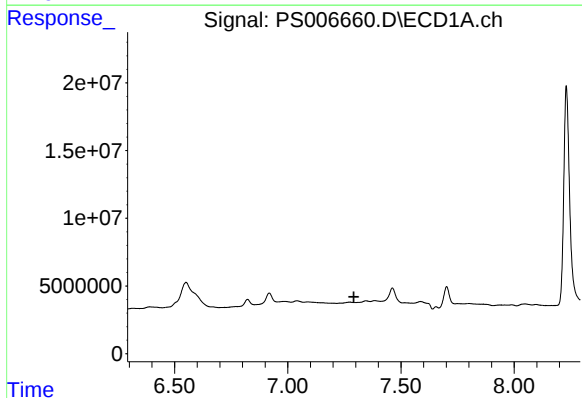


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.292 min
Response: 0
Conc: N.D.

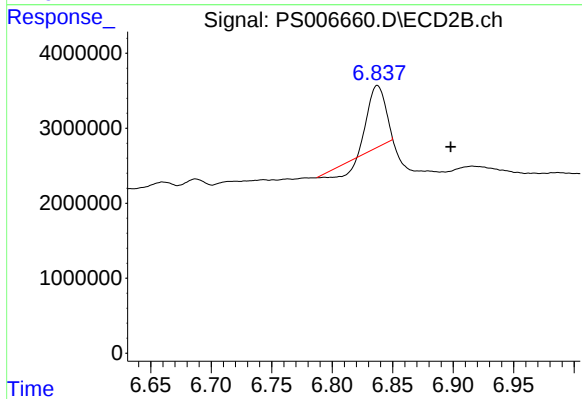

#11 2,4,5-TP (SILVEX)


R.T.: 6.837 min
Delta R.T.: -0.060 min
Response: 6880052
Conc: 3.02 ng/ml

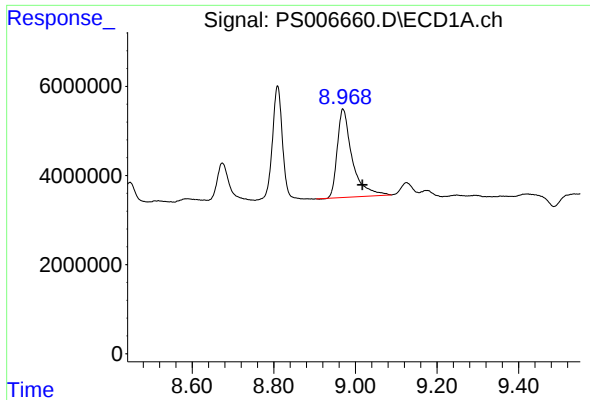

#15 Picloram

R.T.: 8.970 min
Delta R.T.: -0.047 min
Response: 50420251
Conc: 7.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

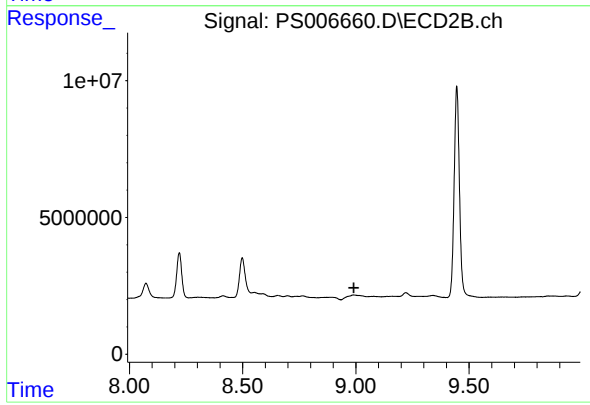

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.