

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
 Data File : PS012209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2020 18:49
 Operator : DD\AJ
 Sample : L3931-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 01:08:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	253.3E6	150.4E6	232.198	281.197
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	54166179	N.D.	65.846
3) T	4-Nitroph...	6.984	0.000	4208417	0	7.145	N.D. #
5) T	DICAMBA	7.394	7.047	6306412	11272454	1.540	5.218 #
6) T	MCP	7.626	0.000	8261773	0	2.586	N.D. #
7) T	MCPA	7.696	7.468	165.2E6	83988898	36.322	30.651
8) T	DICHLORPROP	0.000	7.736	0	15721855	N.D.	27.844
9) T	2,4-D	8.396	0.000	128.2E6	0	113.499	N.D. #
11) T	2,4,5-TP ...	0.000	8.784	0	97584831	N.D.	33.378
12) T	2,4,5-T	9.409	9.241	20281889	9043831	3.423	3.055
15) T	Picloram	11.014	0.000	20518558	0	2.625	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
Data File : PS012209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2020 18:49
Operator : DD\AJ
Sample : L3931-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 01:08:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

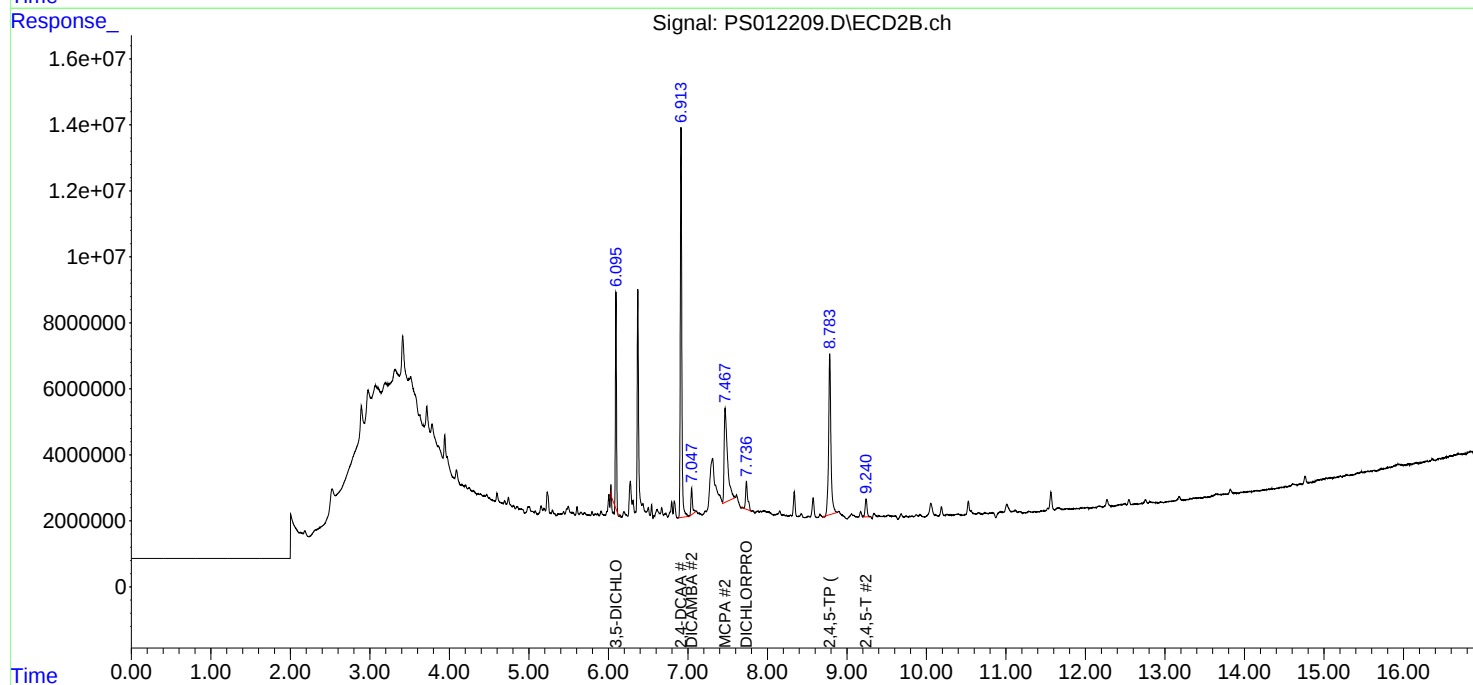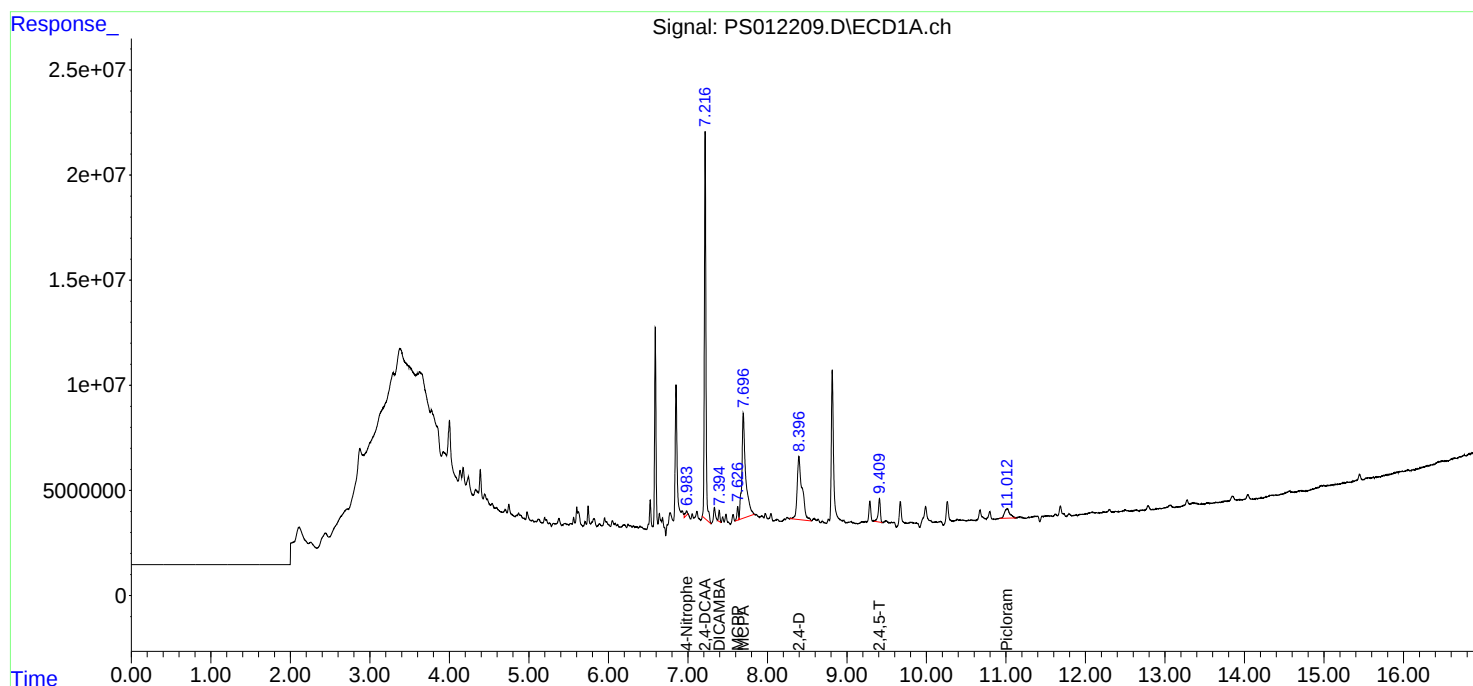


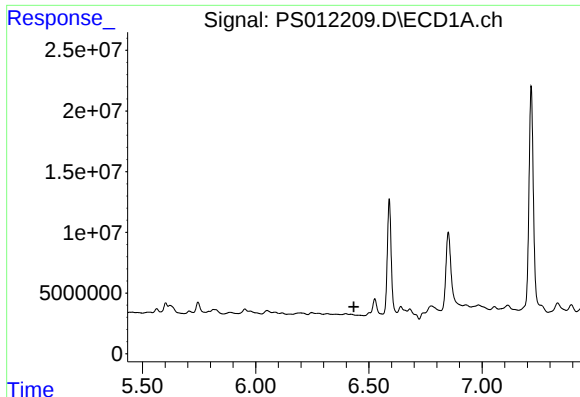

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

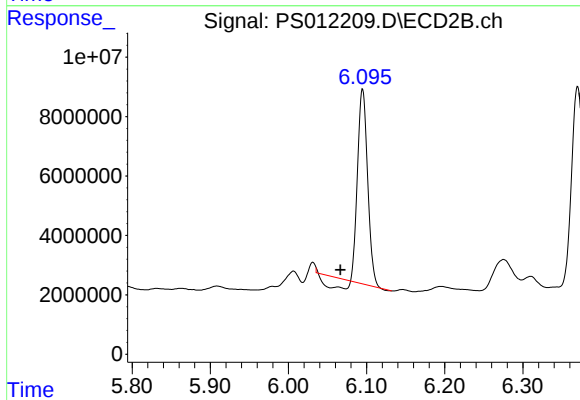


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 54166179
Conc: 65.85 ng/ml

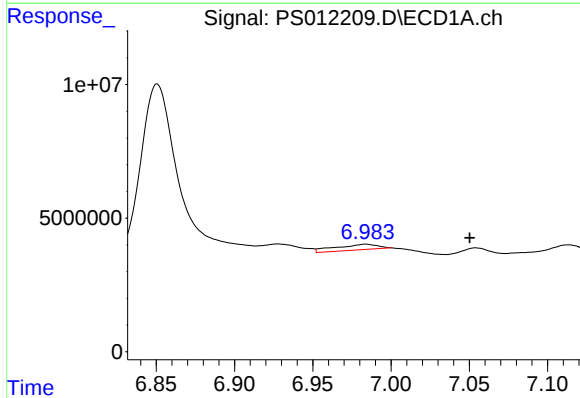


#3 4-Nitrophenol

R.T.: 6.984 min
Delta R.T.: -0.067 min
Response: 4208417
Conc: 7.14 ng/ml

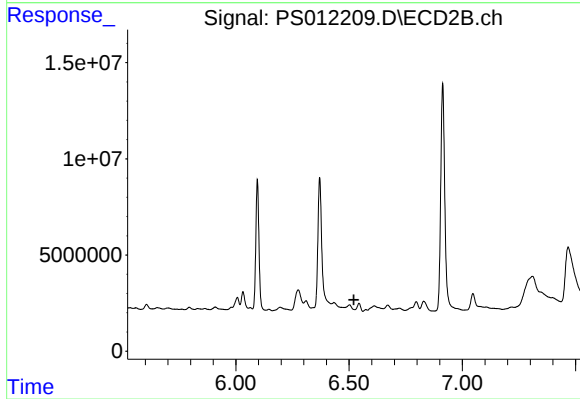

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

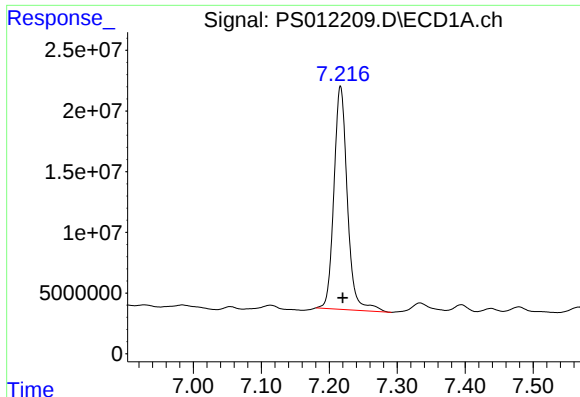

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 253273972
Conc: 232.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

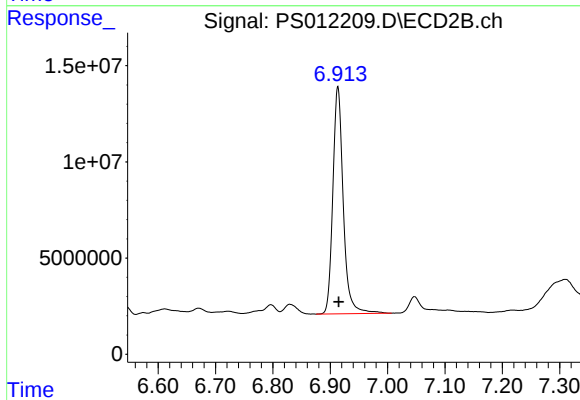


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 150380675
Conc: 281.20 ng/ml

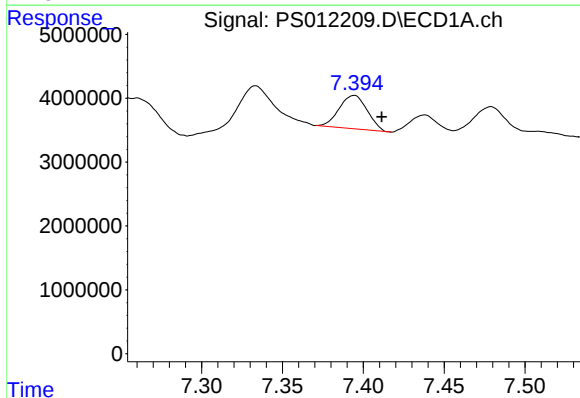


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.018 min
Response: 6306412
Conc: 1.54 ng/ml

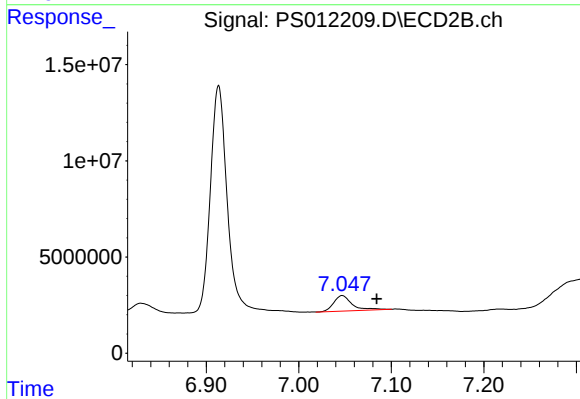

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 11272454
Conc: 5.22 ng/ml

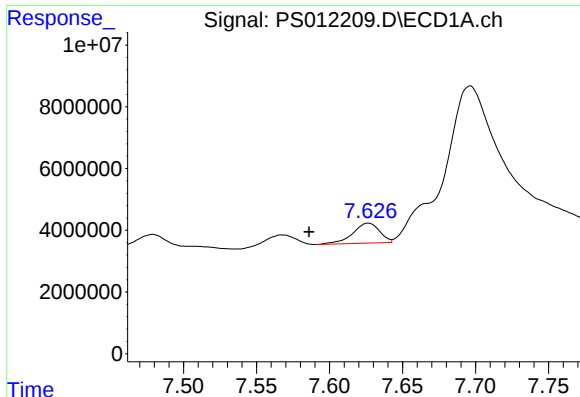

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.040 min
Response: 8261773
Conc: 2.59 ug/ml

Instrument :
ECD_S
ClientSampleId :

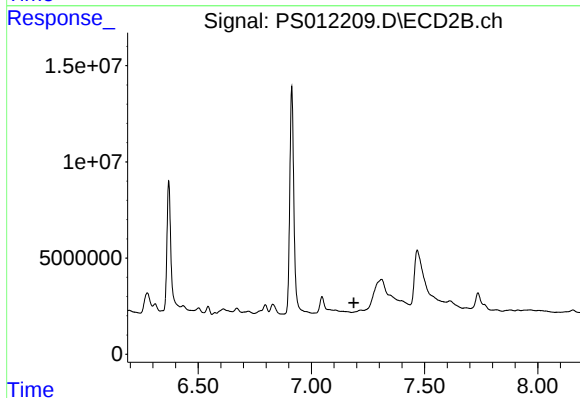


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

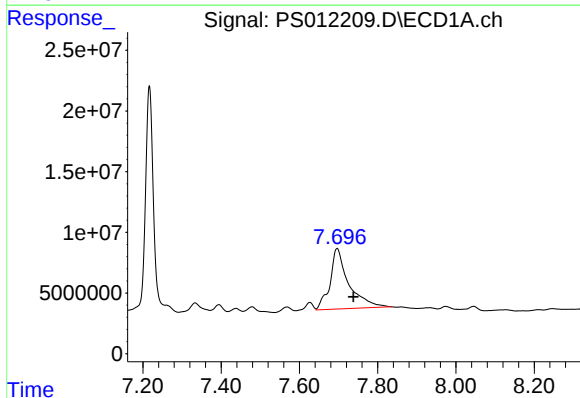


#7 MCPA

R.T.: 7.696 min
Delta R.T.: -0.042 min
Response: 165210679
Conc: 36.32 ug/ml

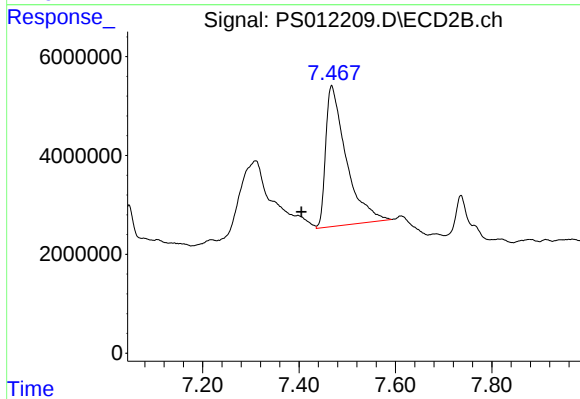

#7 MCPA


R.T.: 7.468 min
Delta R.T.: 0.063 min
Response: 83988898
Conc: 30.65 ug/ml

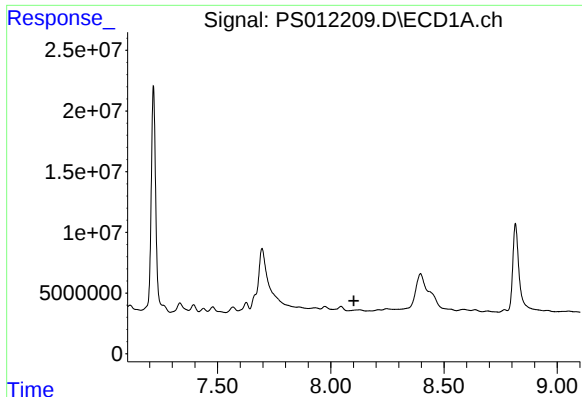

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

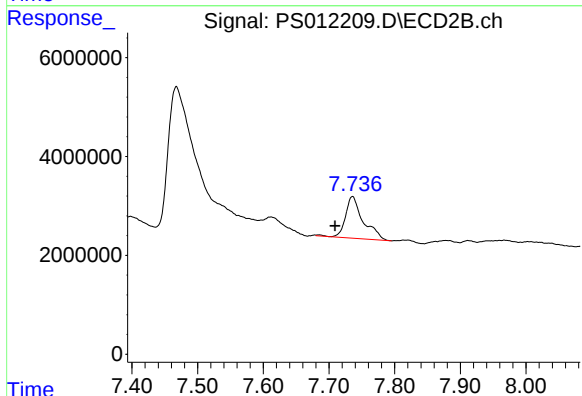


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.026 min
Response: 15721855
Conc: 27.84 ng/ml

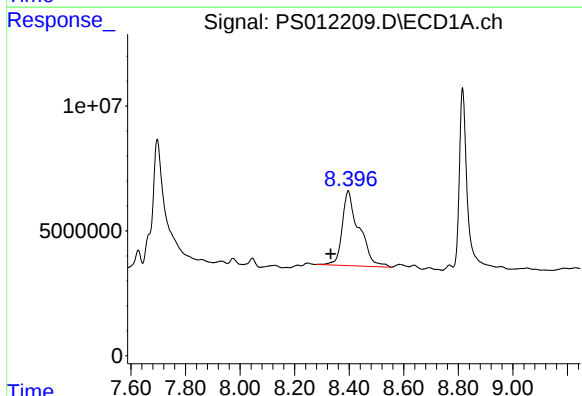


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 128150580
Conc: 113.50 ng/ml

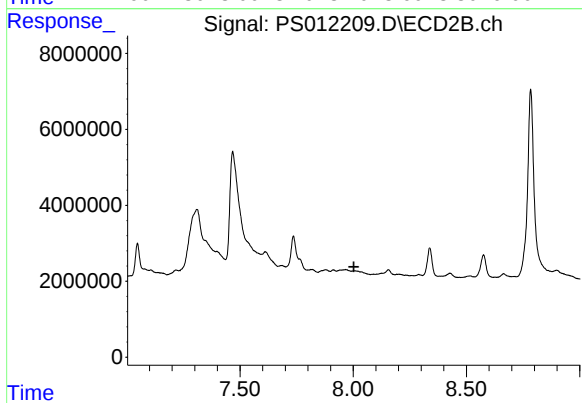

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

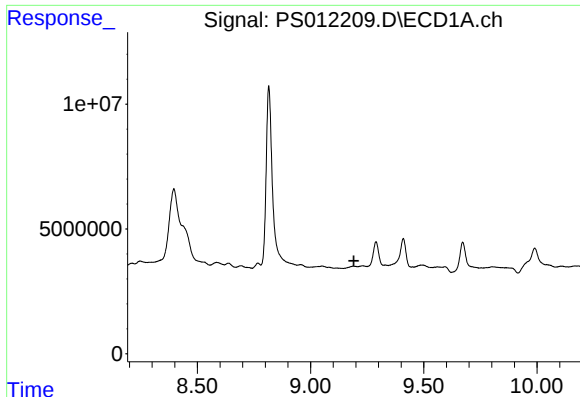

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

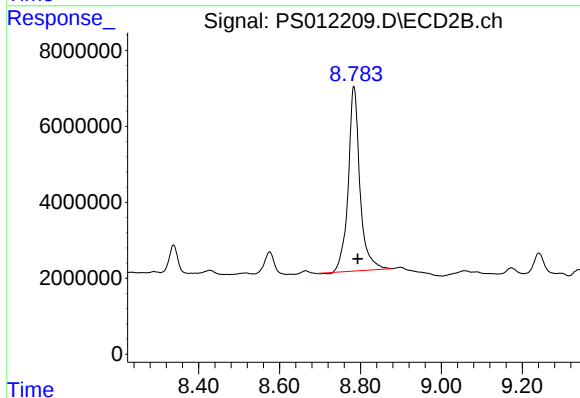


#11 2,4,5-TP (SILVEX)

R.T.: 8.784 min
Delta R.T.: -0.010 min
Response: 97584831
Conc: 33.38 ng/ml

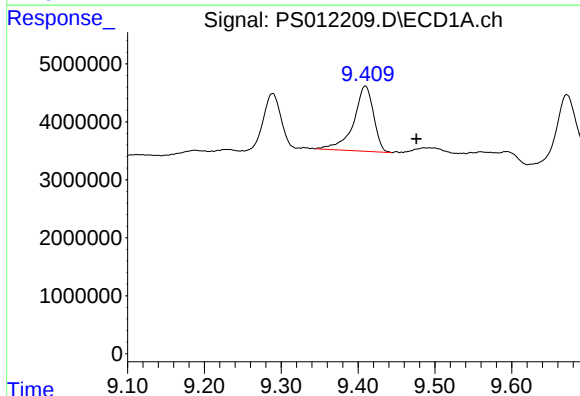


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.067 min
Response: 20281889
Conc: 3.42 ng/ml

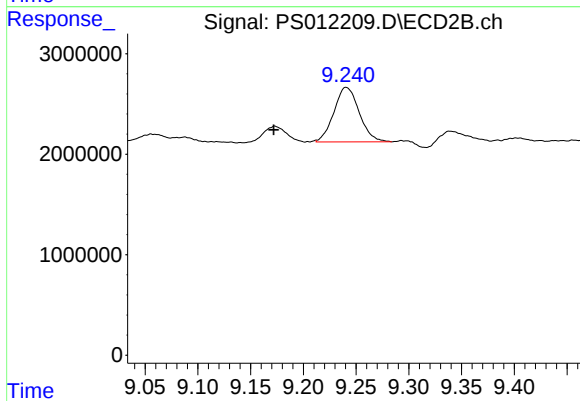

#12 2,4,5-T


R.T.: 9.241 min
Delta R.T.: 0.069 min
Response: 9043831
Conc: 3.06 ng/ml

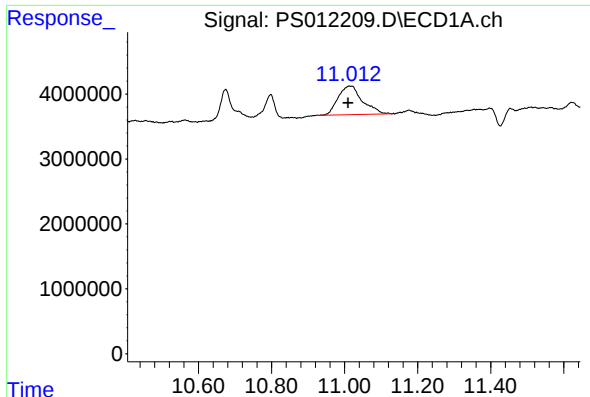

#15 Picloram

R.T.: 11.014 min
Delta R.T.: 0.005 min
Response: 20518558
Conc: 2.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

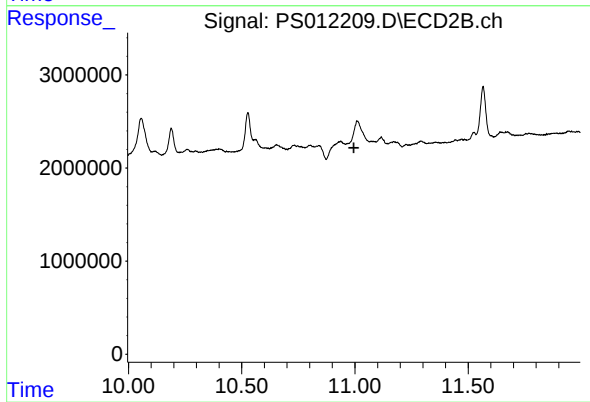

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.