

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
 Data File : PS012212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2020 19:58
 Operator : DD\AJ
 Sample : L3939-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 01:09:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	420.8E6	246.0E6	385.822	460.069
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	38231753	N.D.	46.476
3) T	4-Nitroph...	6.983	0.000	2849797	0	4.838	N.D. #
5) T	DICAMBA	7.394	7.047	7157044	11287582	1.747	5.225 #
6) T	MCP	7.626	0.000	12284550	0	3.845	N.D. #
7) T	MCPA	7.719	0.000	46333568	0	10.187	N.D. #
9) T	2,4-D	8.396	0.000	128.4E6	0	113.744	N.D. #
11) T	2,4,5-TP ...	0.000	8.762	0	14313894	N.D.	4.896
12) T	2,4,5-T	9.410	0.000	13950511	0	2.354	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
Data File : PS012212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2020 19:58
Operator : DD\AJ
Sample : L3939-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 01:09:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

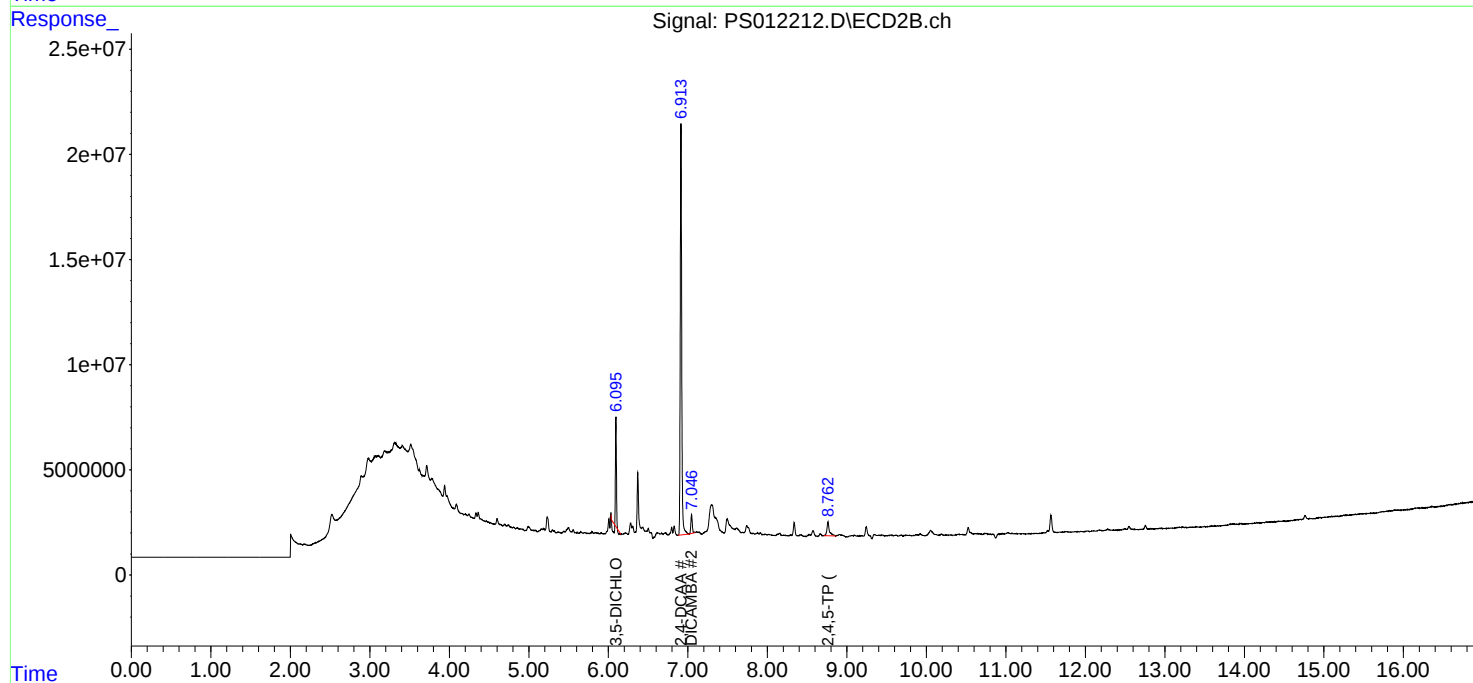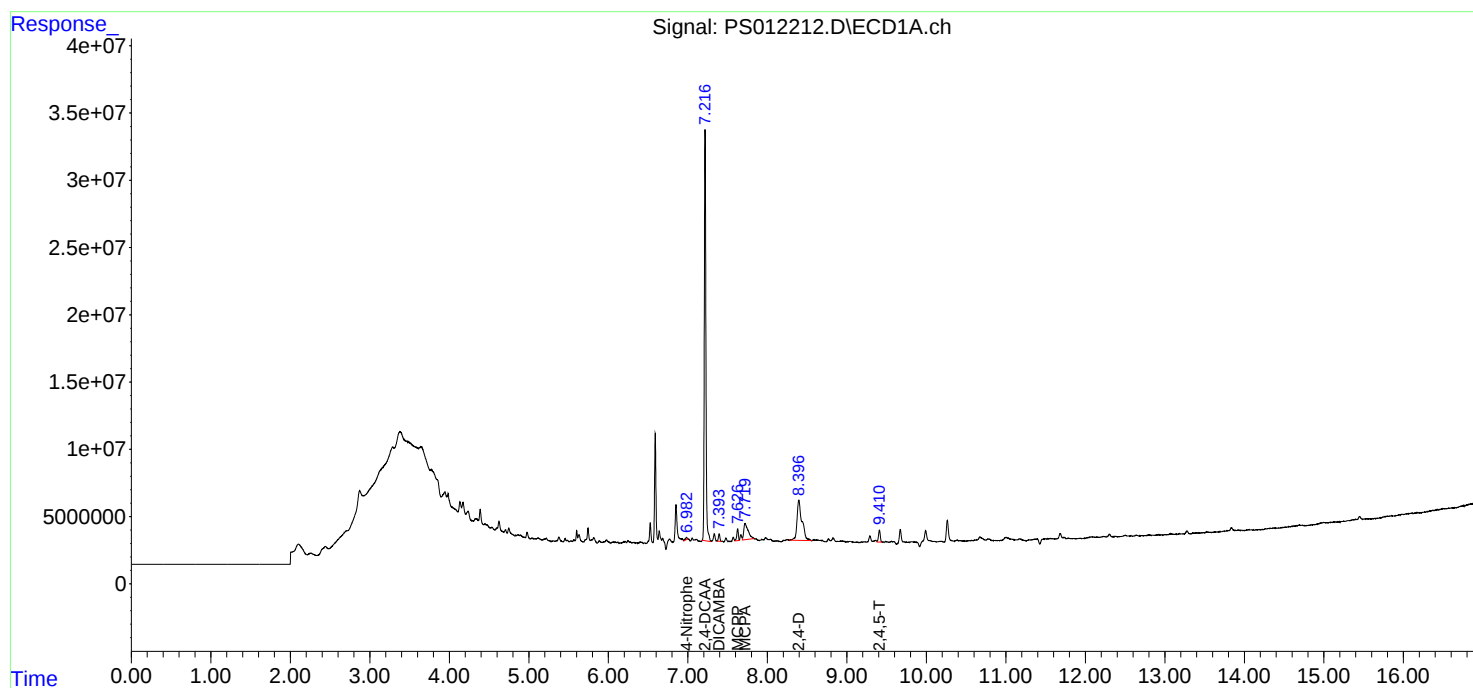


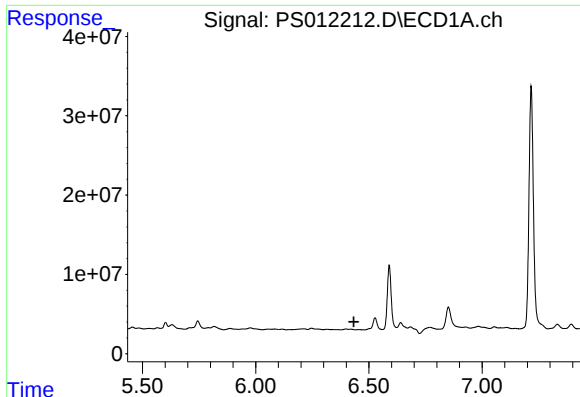

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

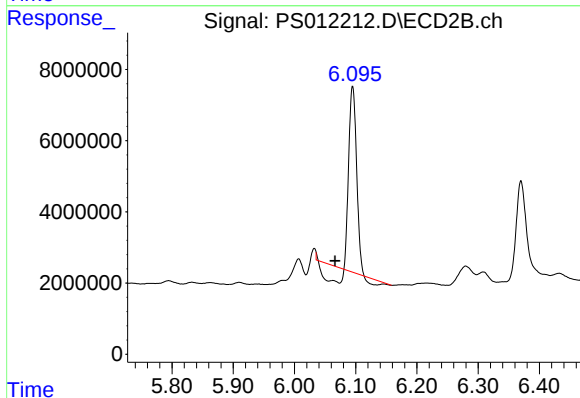


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 38231753
Conc: 46.48 ng/ml

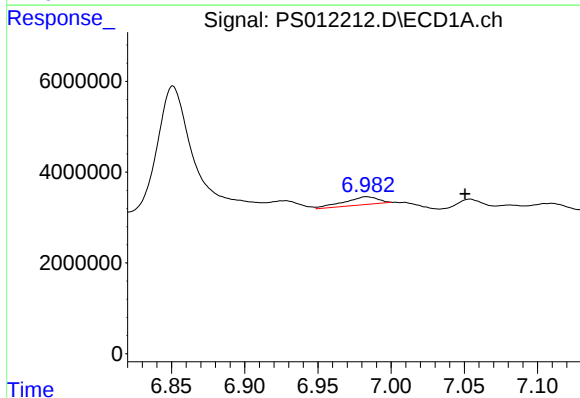


#3 4-Nitrophenol

R.T.: 6.983 min
Delta R.T.: -0.067 min
Response: 2849797
Conc: 4.84 ng/ml

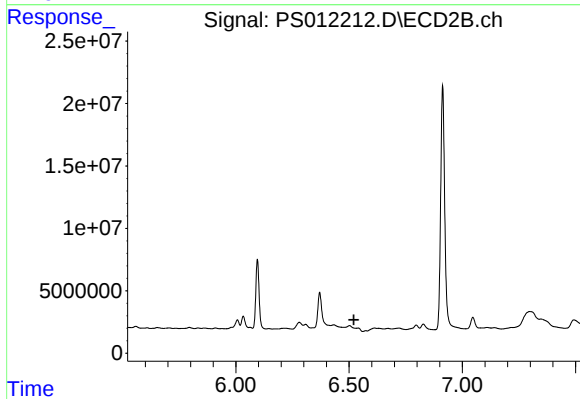

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

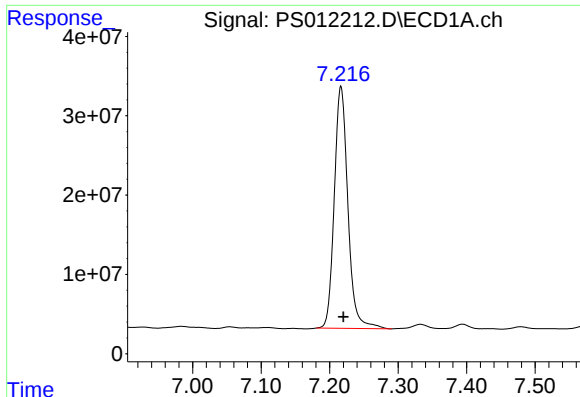

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.004 min
Response: 420842440
Conc: 385.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

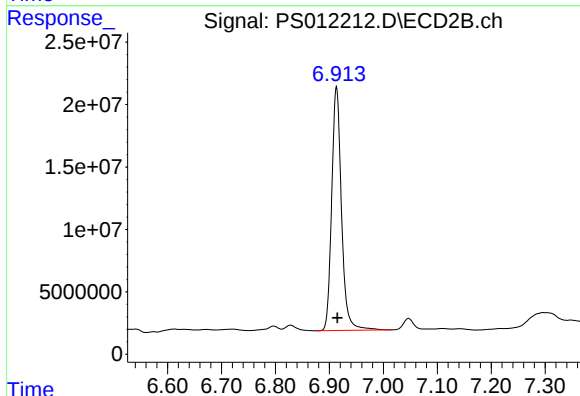


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 246038777
Conc: 460.07 ng/ml

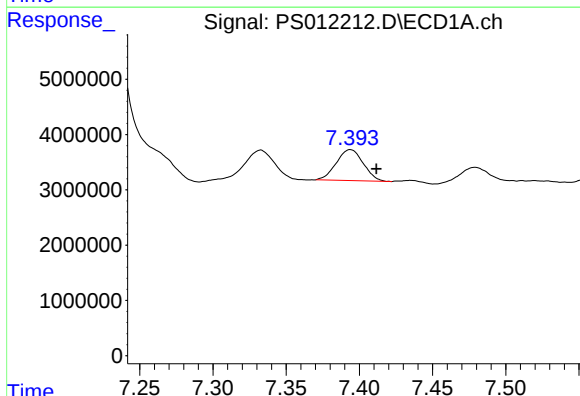


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.018 min
Response: 7157044
Conc: 1.75 ng/ml

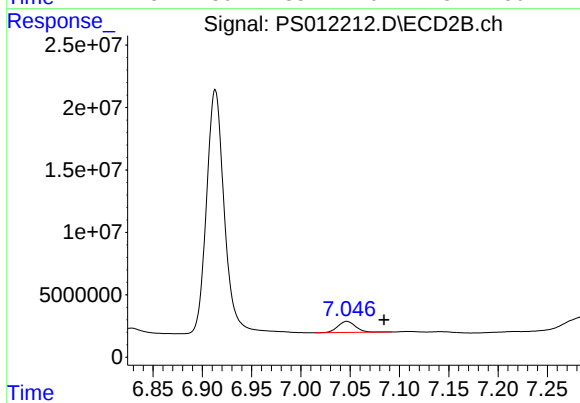

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.038 min
Response: 11287582
Conc: 5.22 ng/ml

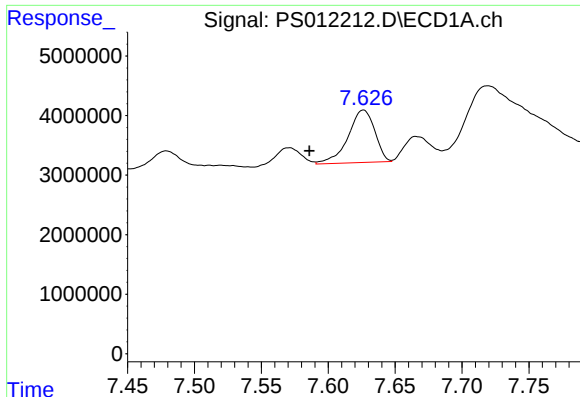

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.040 min
Response: 12284550
Conc: 3.84 ug/ml

Instrument :
ECD_S
ClientSampleId :

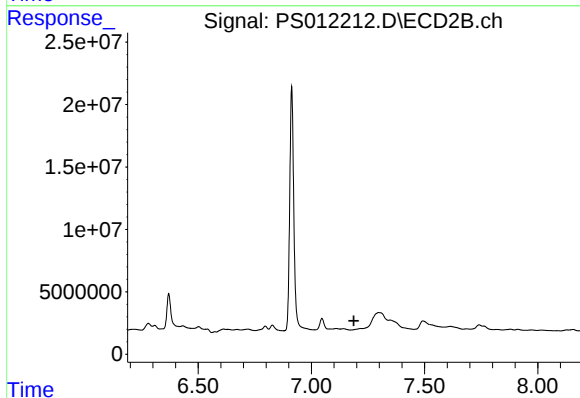


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

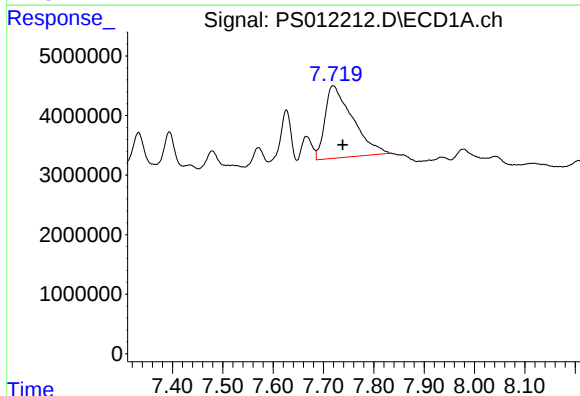


#7 MCPA

R.T.: 7.719 min
Delta R.T.: -0.019 min
Response: 46333568
Conc: 10.19 ug/ml

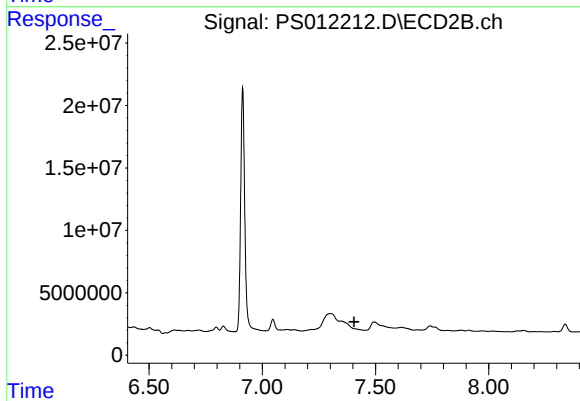

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

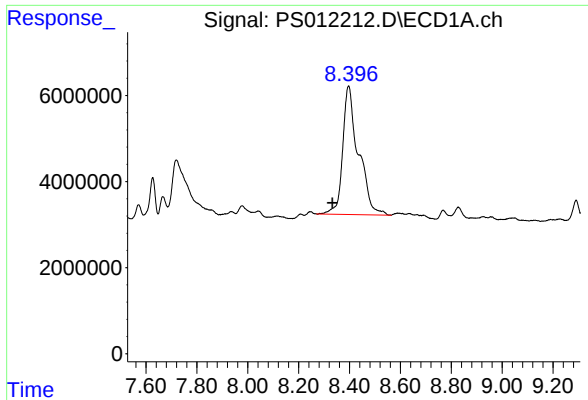

#9 2,4-D


R.T.: 8.396 min
Delta R.T.: 0.064 min
Response: 128427027
Conc: 113.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

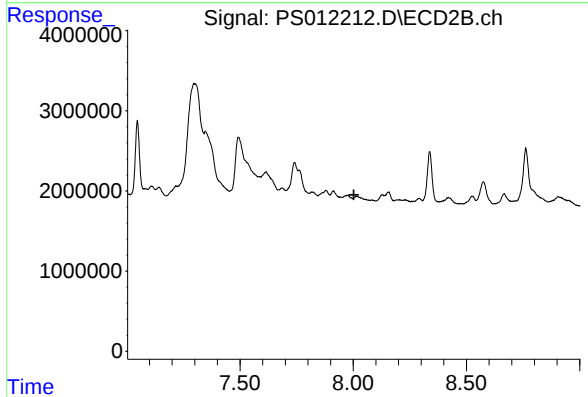


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

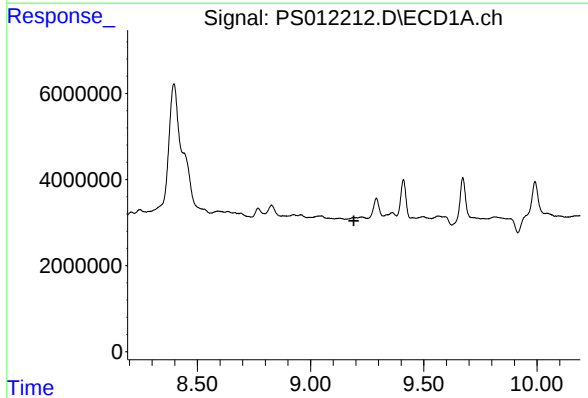


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

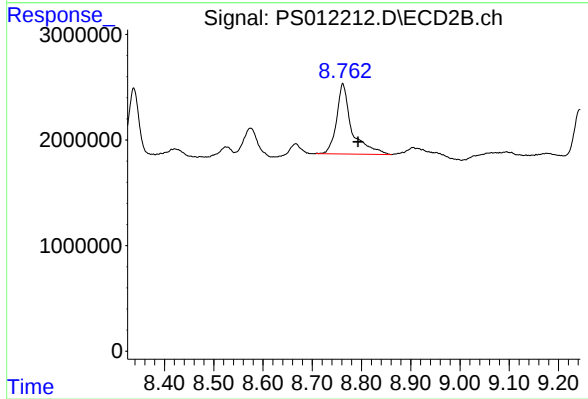

#11 2,4,5-TP (SILVEX)


R.T.: 8.762 min
Delta R.T.: -0.031 min
Response: 14313894
Conc: 4.90 ng/ml

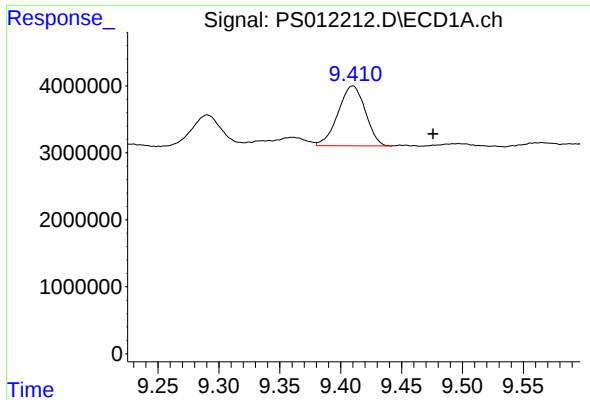

#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.066 min
Response: 13950511
Conc: 2.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

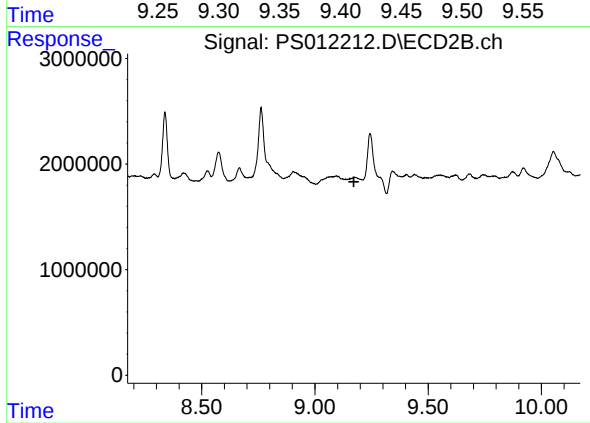

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.