

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
 Data File : PS012218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 09:24
 Operator : DD\AJ
 Sample : L3932-02RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 10:54:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.912	340.7E6	199.3E6	312.375	372.586
Target Compounds							
2) T	3,5-DICHL...	0.000	6.093	0	39705589	N.D.	48.267
3) T	4-Nitroph...	6.987	0.000	4200906	0	7.132	N.D. #
5) T	DICAMBA	0.000	7.081	0	8796800	N.D.	4.072
6) T	MCP	7.571	0.000	5562200	0	1.741	N.D. #
7) T	MCPA	7.700	0.000	129.1E6	0	28.388	N.D. #
8) T	DICHLORPROP	0.000	7.736	0	14160951	N.D.	25.080
9) T	2,4-D	8.343	7.939	111.4E6	59652238	98.625	81.197
11) T	2,4,5-TP ...	0.000	8.760	0	14420306	N.D.	4.932
12) T	2,4,5-T	9.410	9.237	17707772	24548862	2.988	8.293 #
15) T	Picloram	11.026	11.006	93128890	65097639	11.916	14.363
16) T	DCPA	0.000	11.006	0	65097639	N.D.	17.704



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
Data File : PS012218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 09:24
Operator : DD\AJ
Sample : L3932-02RE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 10:54:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

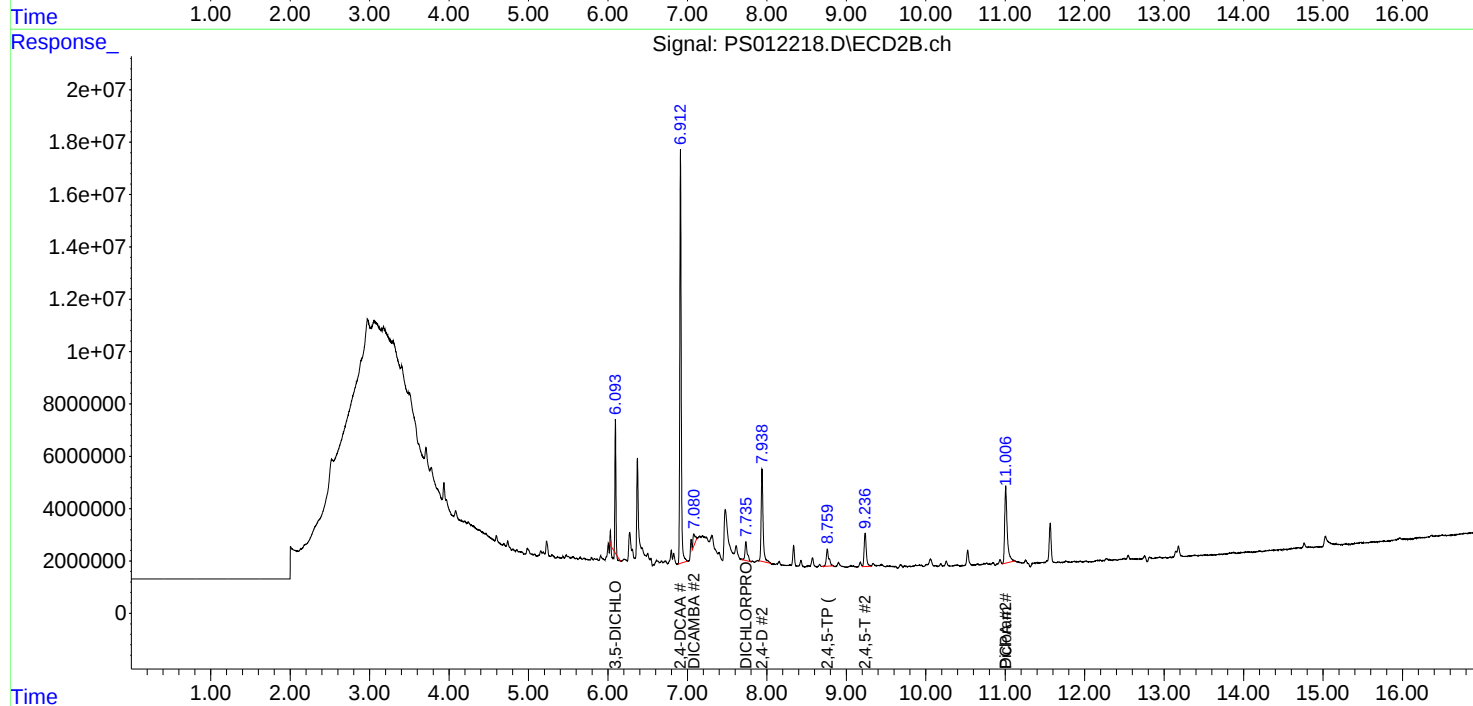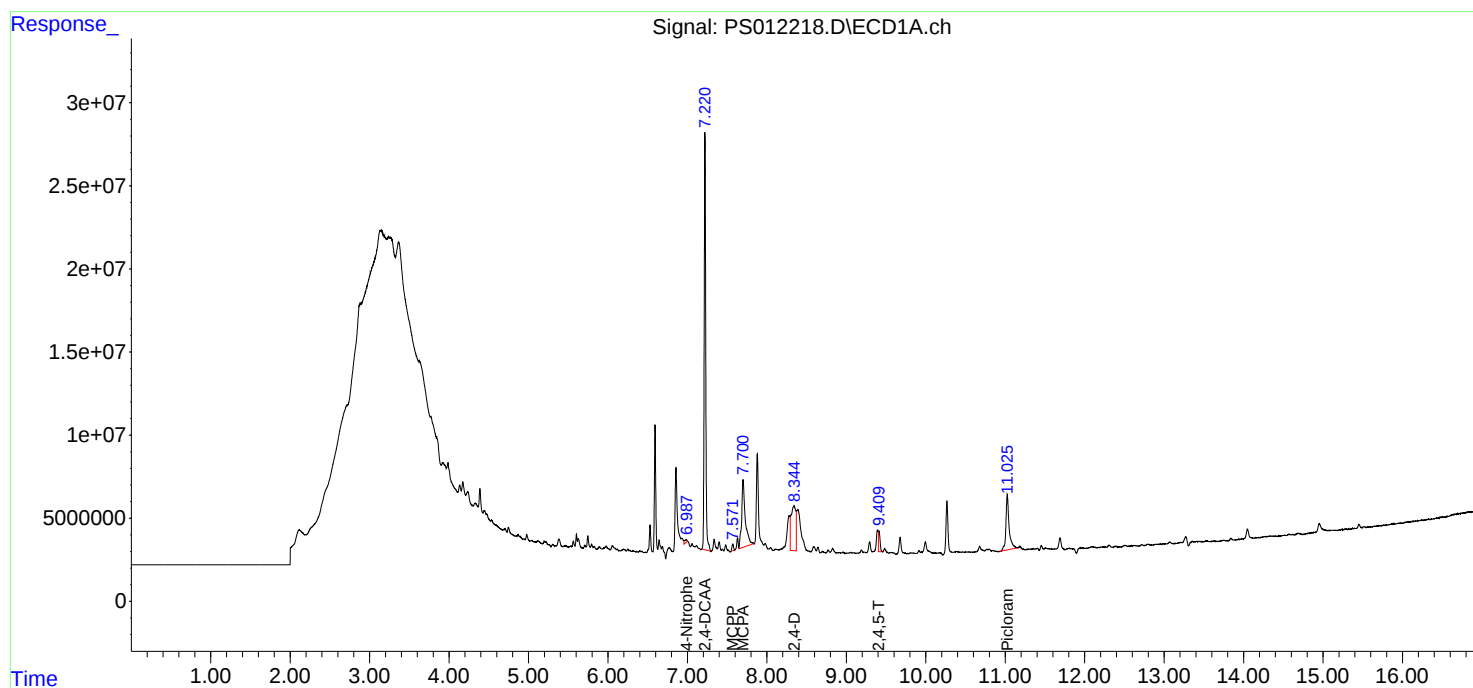


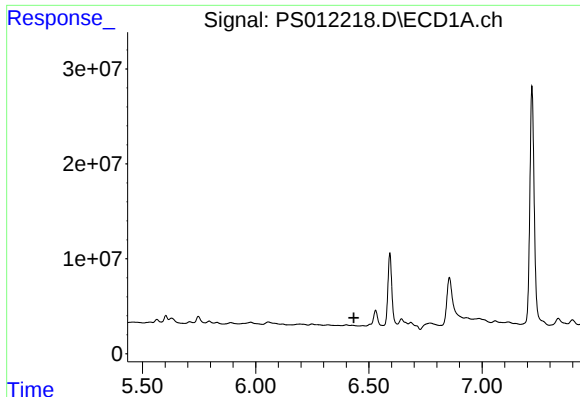

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

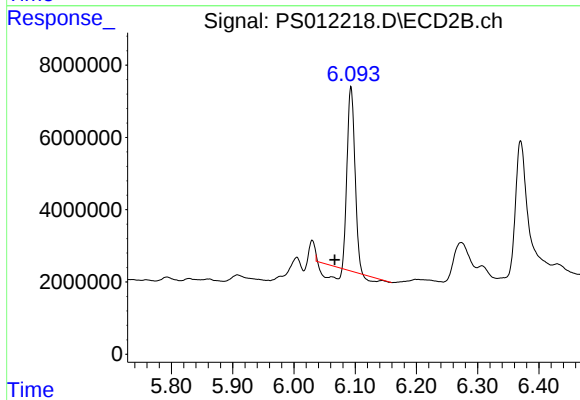


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.093 min
Delta R.T.: 0.027 min
Response: 39705589
Conc: 48.27 ng/ml

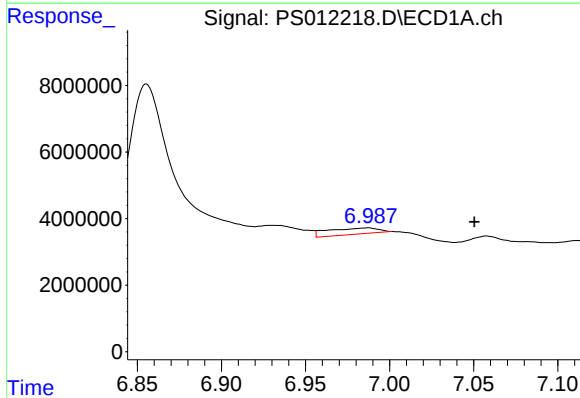


#3 4-Nitrophenol

R.T.: 6.987 min
Delta R.T.: -0.063 min
Response: 4200906
Conc: 7.13 ng/ml

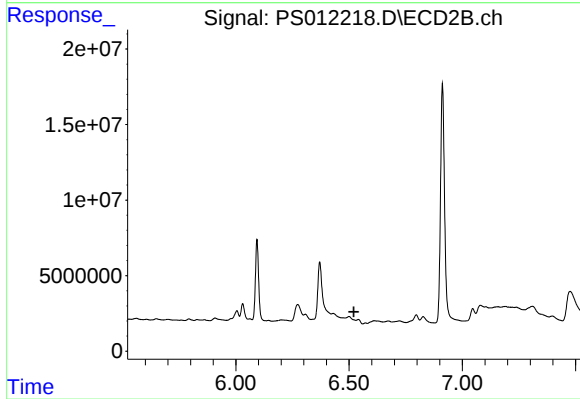

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

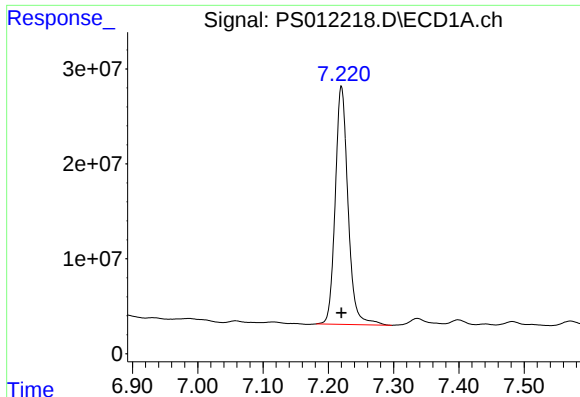

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 340729204
Conc: 312.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

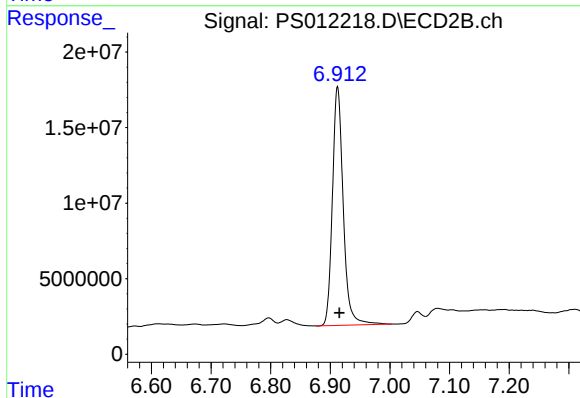


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: -0.003 min
Response: 199253906
Conc: 372.59 ng/ml

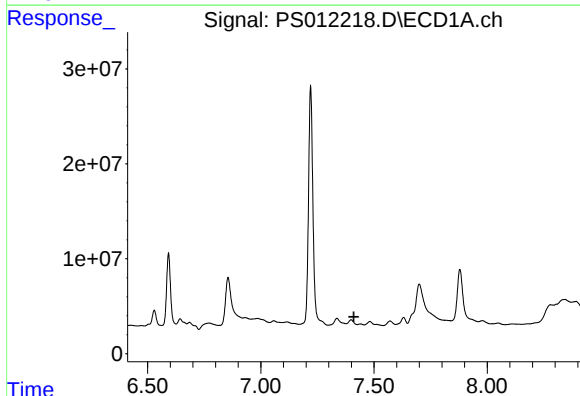


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

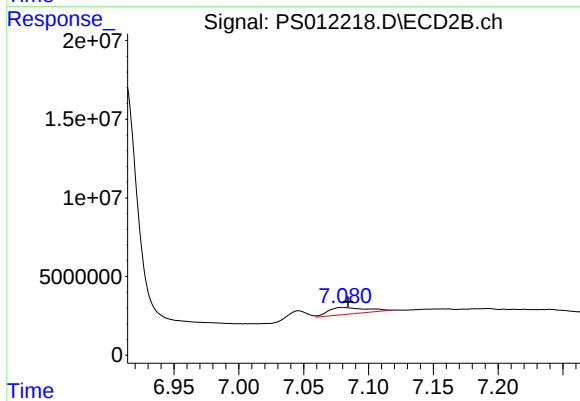

#5 DICAMBA


R.T.: 7.081 min
Delta R.T.: -0.004 min
Response: 8796800
Conc: 4.07 ng/ml

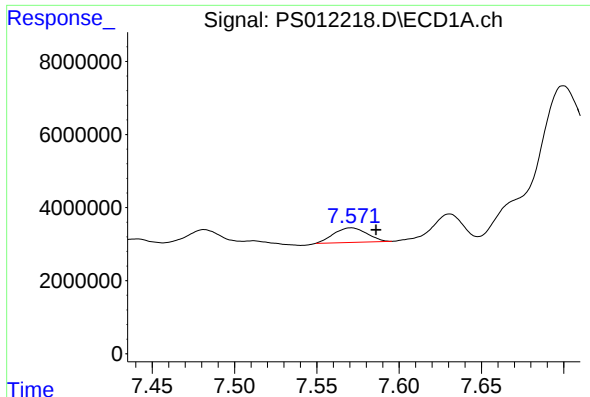

#6 MCPP


R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 5562200
Conc: 1.74 ug/ml

Instrument :
ECD_S
ClientSampleId :

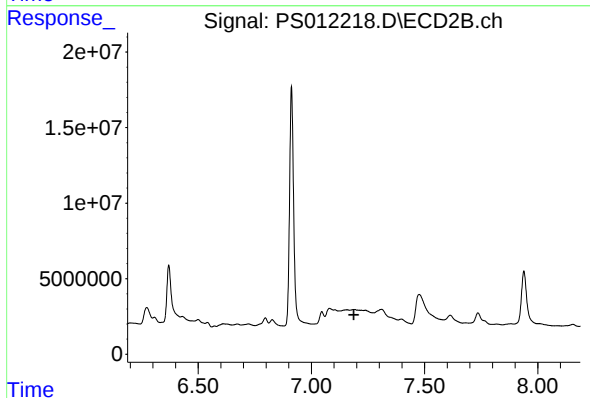


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

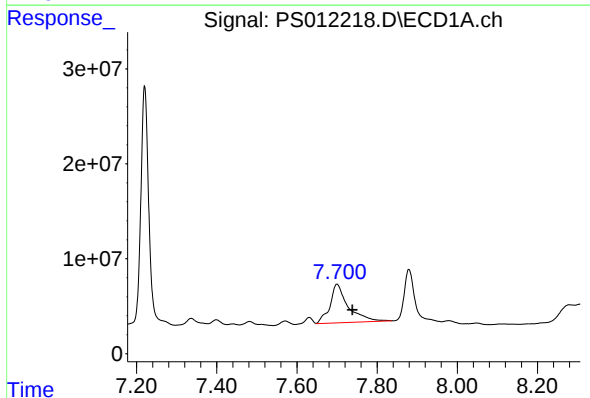


#7 MCPA

R.T.: 7.700 min
Delta R.T.: -0.038 min
Response: 129121964
Conc: 28.39 ug/ml

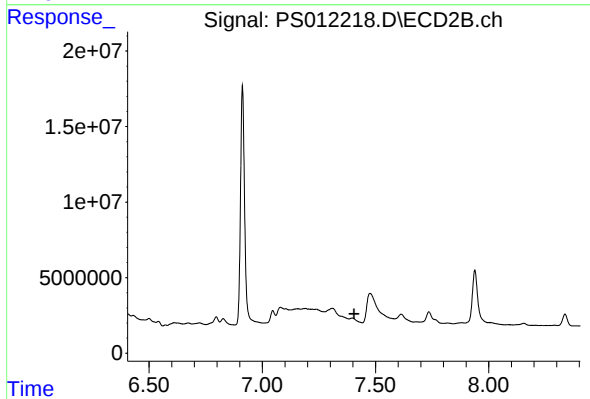

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

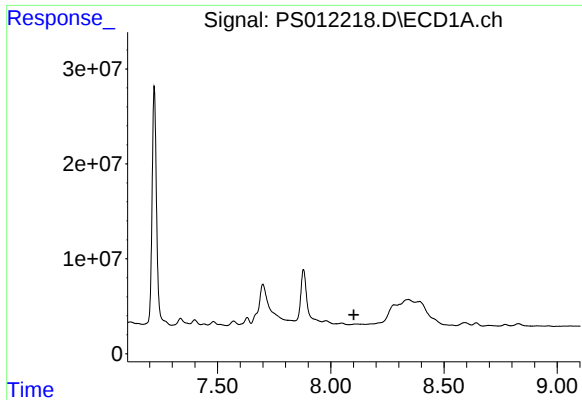

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

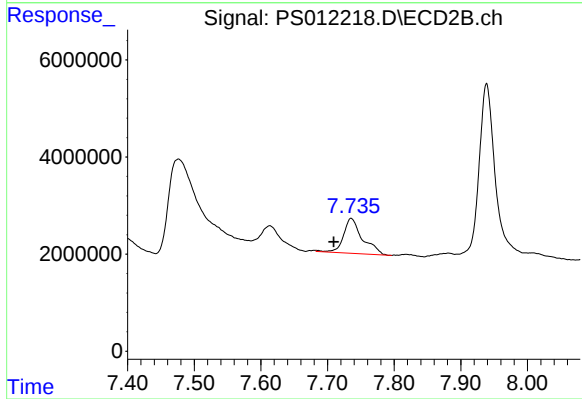


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.026 min
Response: 14160951
Conc: 25.08 ng/ml

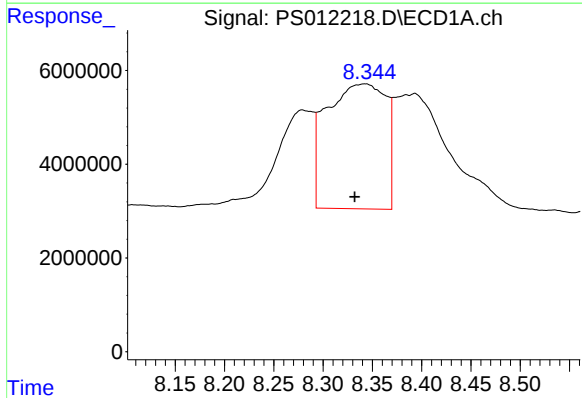


#9 2,4-D

R.T.: 8.343 min
Delta R.T.: 0.011 min
Response: 111356748
Conc: 98.62 ng/ml

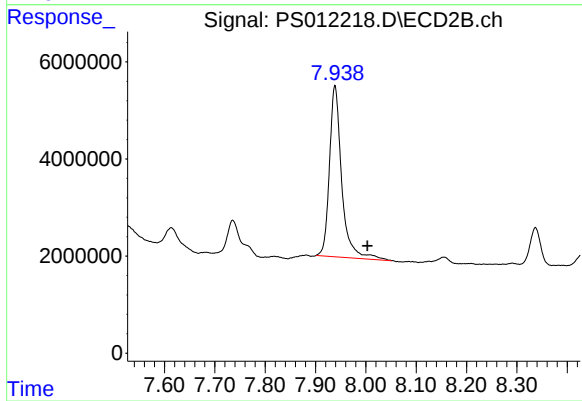

#9 2,4-D


R.T.: 7.939 min
Delta R.T.: -0.064 min
Response: 59652238
Conc: 81.20 ng/ml

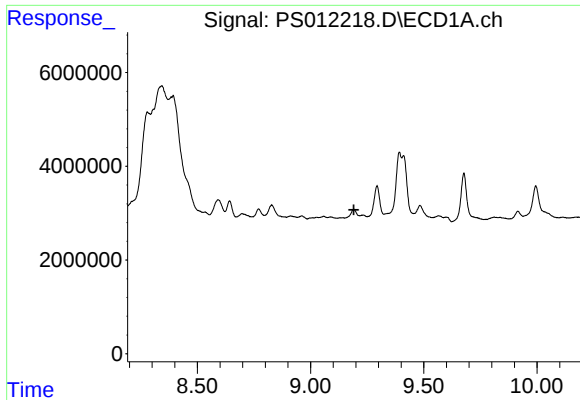

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

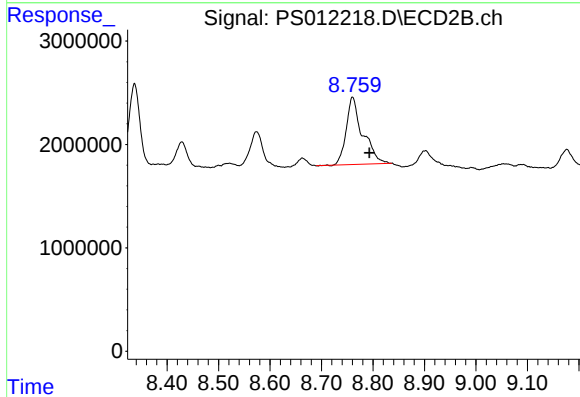


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: -0.033 min
Response: 14420306
Conc: 4.93 ng/ml

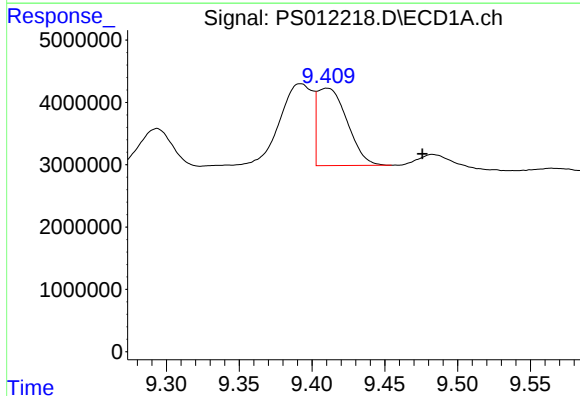


#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.066 min
Response: 17707772
Conc: 2.99 ng/ml

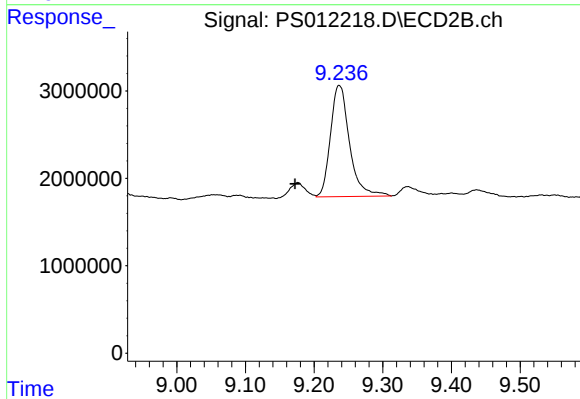

#12 2,4,5-T


R.T.: 9.237 min
Delta R.T.: 0.065 min
Response: 24548862
Conc: 8.29 ng/ml

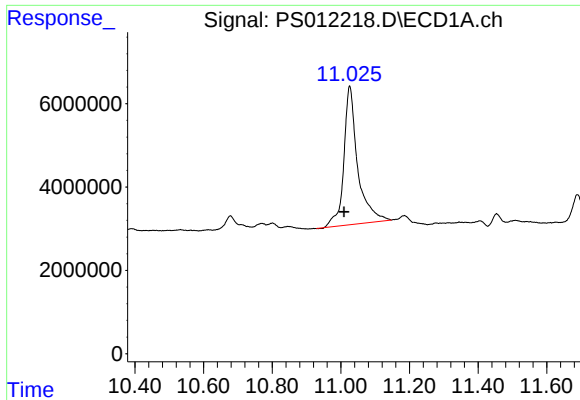

#15 Picloram


R.T.: 11.026 min
Delta R.T.: 0.016 min
Response: 93128890
Conc: 11.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

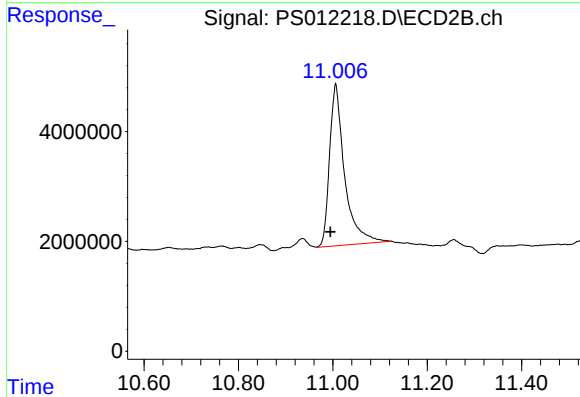


#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.011 min
Response: 65097639
Conc: 14.36 ng/ml

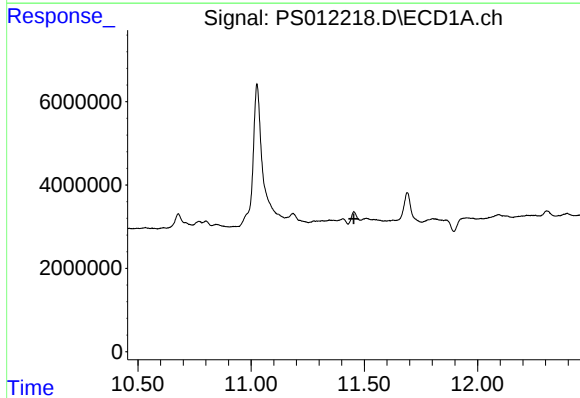

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.454 min
Response: 0
Conc: N.D.

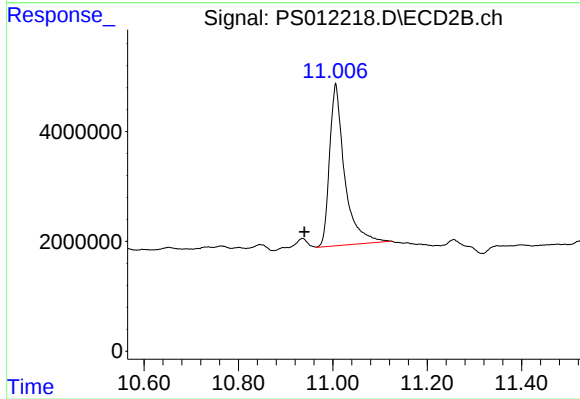

#16 DCPA

R.T.: 11.006 min
Delta R.T.: 0.066 min
Response: 65097639
Conc: 17.70 ng/ml