

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
 Data File : PS012221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 10:32
 Operator : DD\AJ
 Sample : PB131518TB
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 10:55:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	343.6E6	203.6E6	315.027	380.742
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	46774556	N.D.	56.860
3) T	4-Nitroph...	6.984	0.000	3049922	0	5.178	N.D. #
5) T	DICAMBA	7.396	7.048	8047177	7476235	1.965	3.460 #
6) T	MCP	7.628	0.000	8489566	0	2.657	N.D. #
7) T	MCPA	7.701	0.000	127.7E6	0	28.064	N.D. #
8) T	DICHLORPROP	0.000	7.738	0	25574950	N.D.	45.295
9) T	2,4-D	8.397	0.000	78892901	0	69.873	N.D. #
11) T	2,4,5-TP ...	0.000	8.787	0	123.2E6	N.D.	42.126
12) T	2,4,5-T	9.409	0.000	18505641	0	3.123	N.D. #
15) T	Picloram	11.034	11.019	24781763	10623239	3.171	2.344 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091020\
Data File : PS012221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 10:32
Operator : DD\AJ
Sample : PB131518TB
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 10:55:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

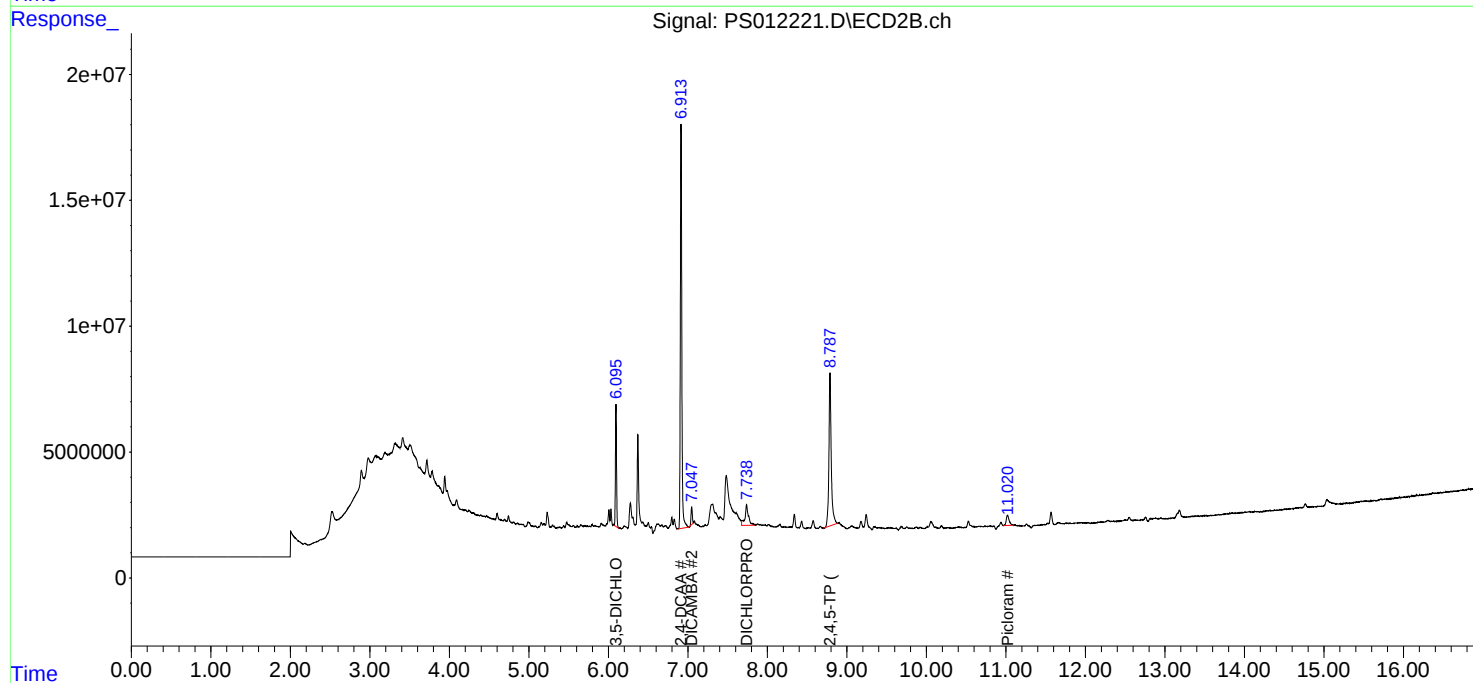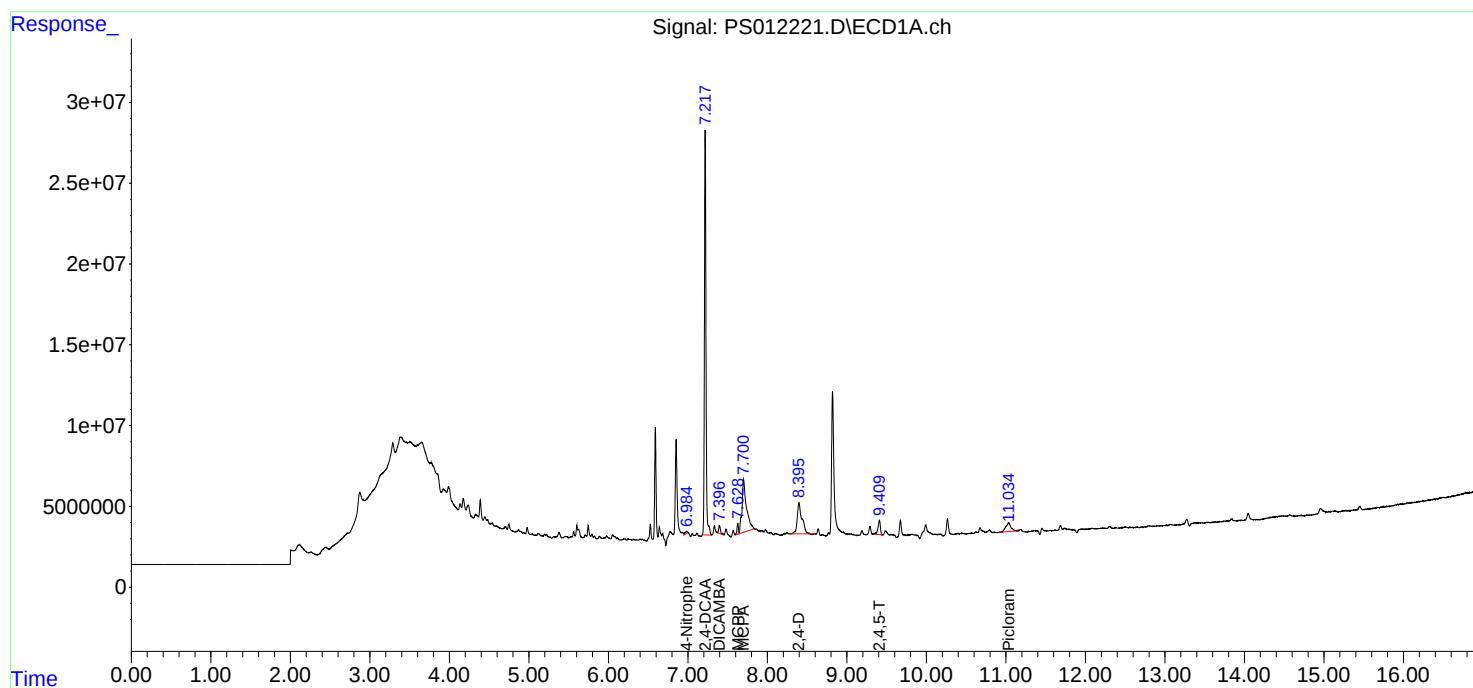


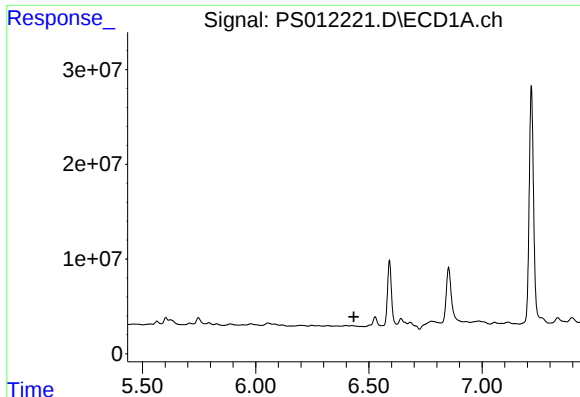

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

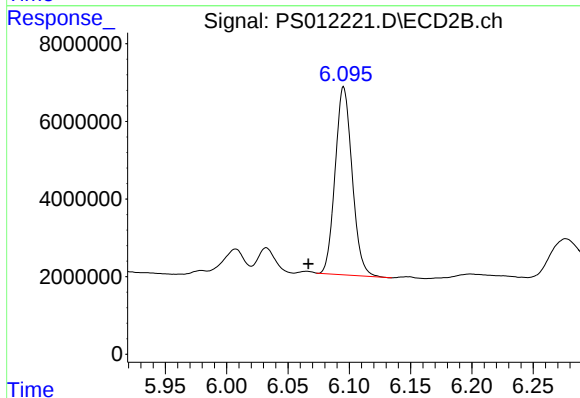


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 46774556
Conc: 56.86 ng/ml

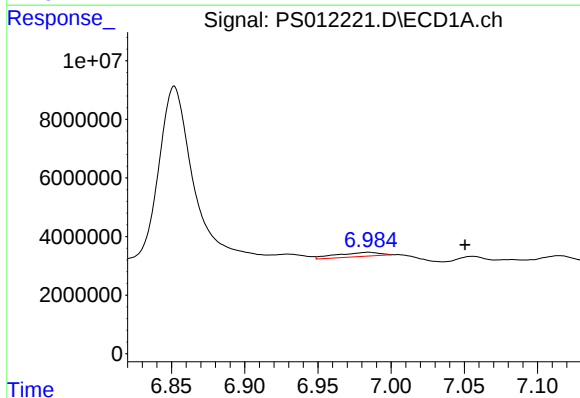


#3 4-Nitrophenol

R.T.: 6.984 min
Delta R.T.: -0.066 min
Response: 3049922
Conc: 5.18 ng/ml

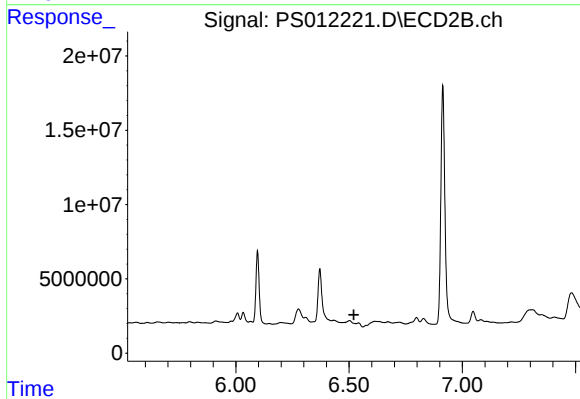

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

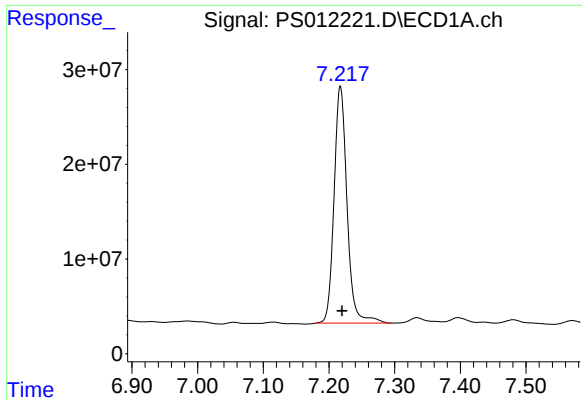

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: -0.003 min
Response: 343622054
Conc: 315.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

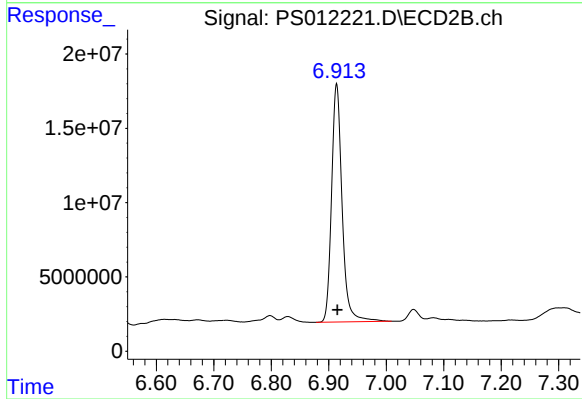


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 203615723
Conc: 380.74 ng/ml

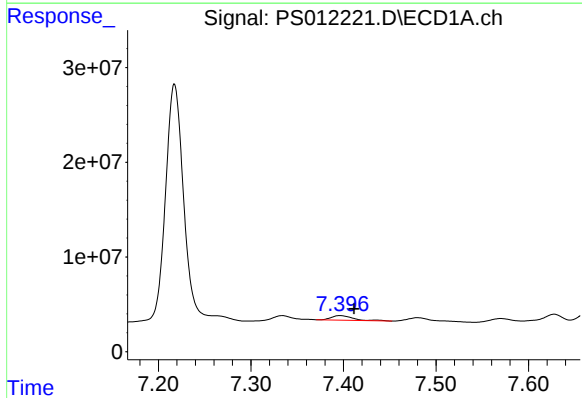


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 8047177
Conc: 1.96 ng/ml

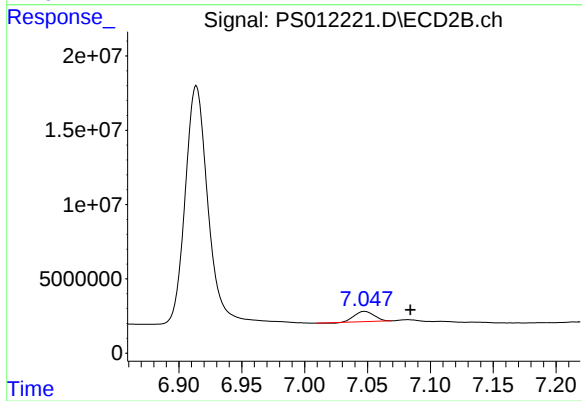

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 7476235
Conc: 3.46 ng/ml

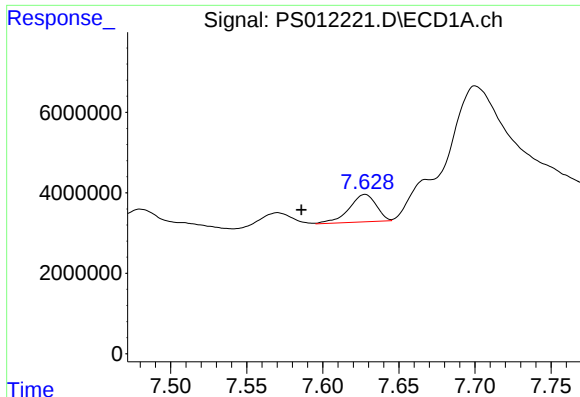

#6 MCPP


R.T.: 7.628 min
Delta R.T.: 0.042 min
Response: 8489566
Conc: 2.66 ug/ml

Instrument :
ECD_S
ClientSampleId :

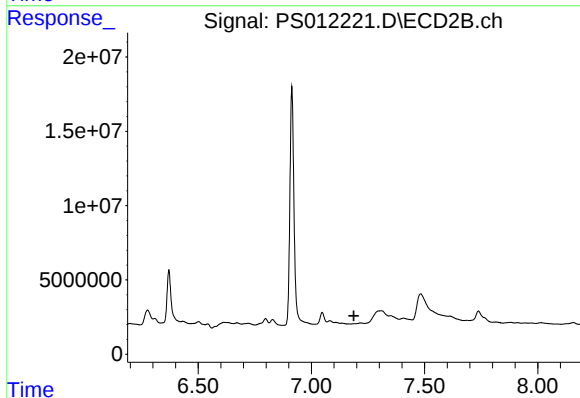


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

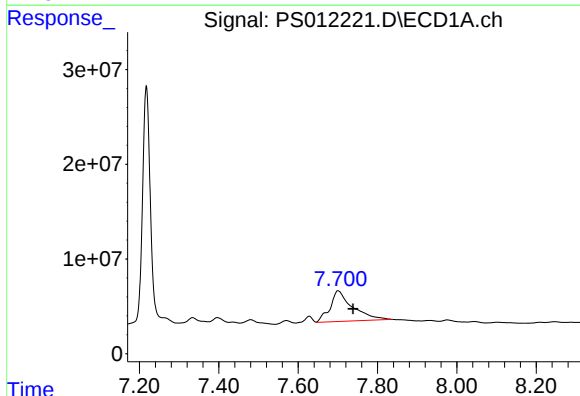


#7 MCPA

R.T.: 7.701 min
Delta R.T.: -0.037 min
Response: 127650154
Conc: 28.06 ug/ml

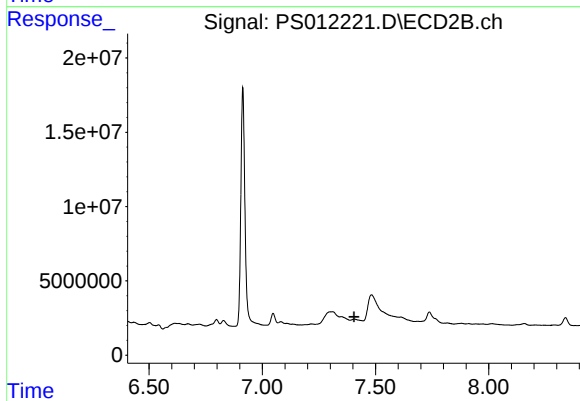

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

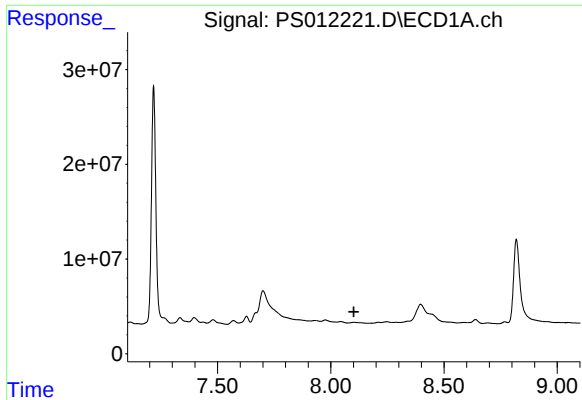

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

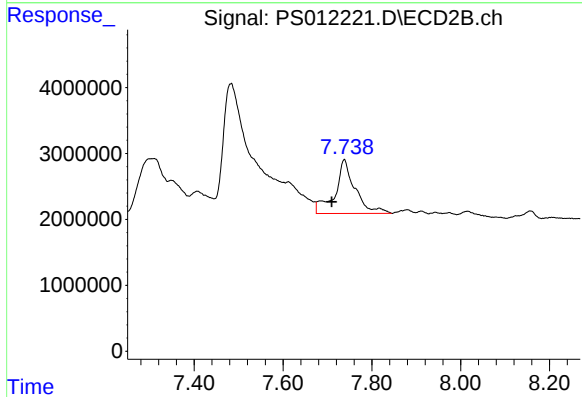


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.028 min
Response: 25574950
Conc: 45.29 ng/ml

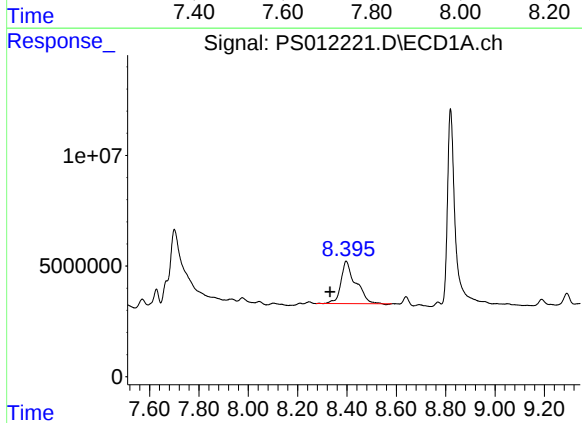


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.065 min
Response: 78892901
Conc: 69.87 ng/ml

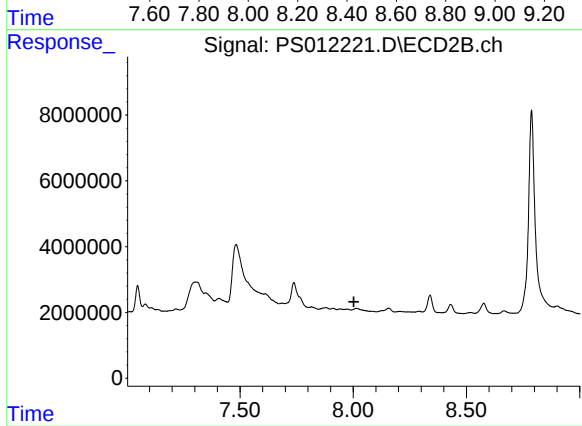

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

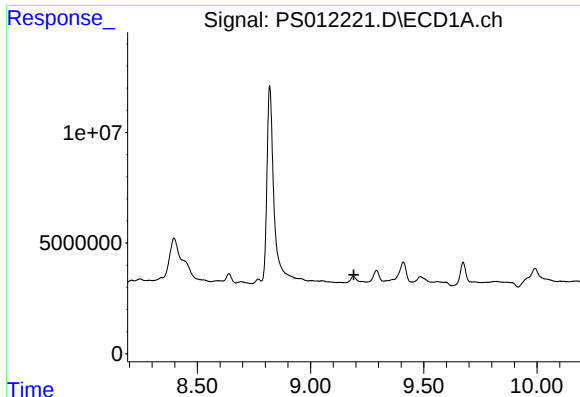

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

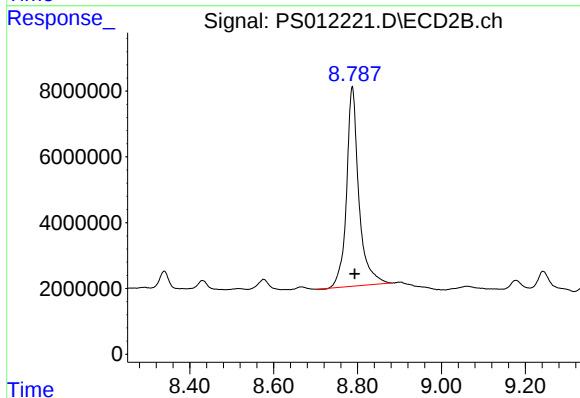


#11 2,4,5-TP (SILVEX)

R.T.: 8.787 min
Delta R.T.: -0.006 min
Response: 123162257
Conc: 42.13 ng/ml

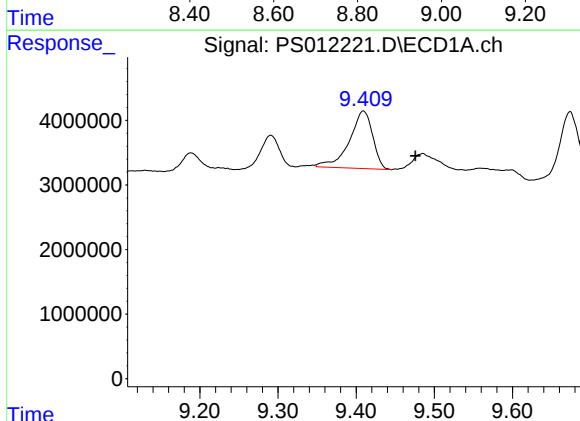


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.067 min
Response: 18505641
Conc: 3.12 ng/ml

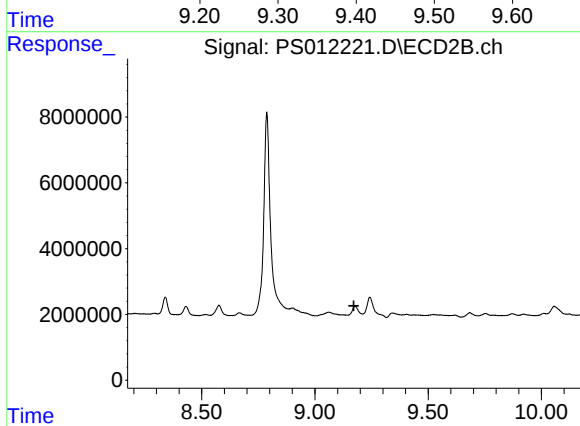

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

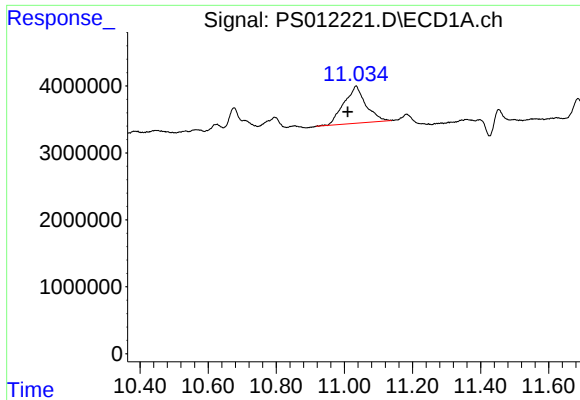

#15 Picloram

R.T.: 11.034 min
Delta R.T.: 0.025 min
Response: 24781763
Conc: 3.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

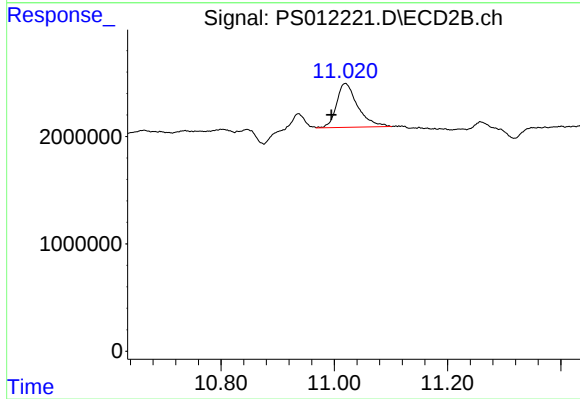

#15 Picloram

R.T.: 11.019 min
Delta R.T.: 0.024 min
Response: 10623239
Conc: 2.34 ng/ml