

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
 Data File : PS001693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2018 16:43
 Operator : EI\SJ
 Sample : PB112753BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 00:50:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.488	10.977	100.1E6	98971041	542.439	488.674
Target Compounds							
6) T	MCP	12.177	0.000	17189838	0	34.164	N.D. #
15) T	Picloram	17.009	16.919	9046194	29084658	6.459	22.305 #
16) T	DCPA	0.000	16.919	0	29084658	N.D.	20.371 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
Data File : PS001693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2018 16:43
Operator : EI\SJ
Sample : PB112753BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:50:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

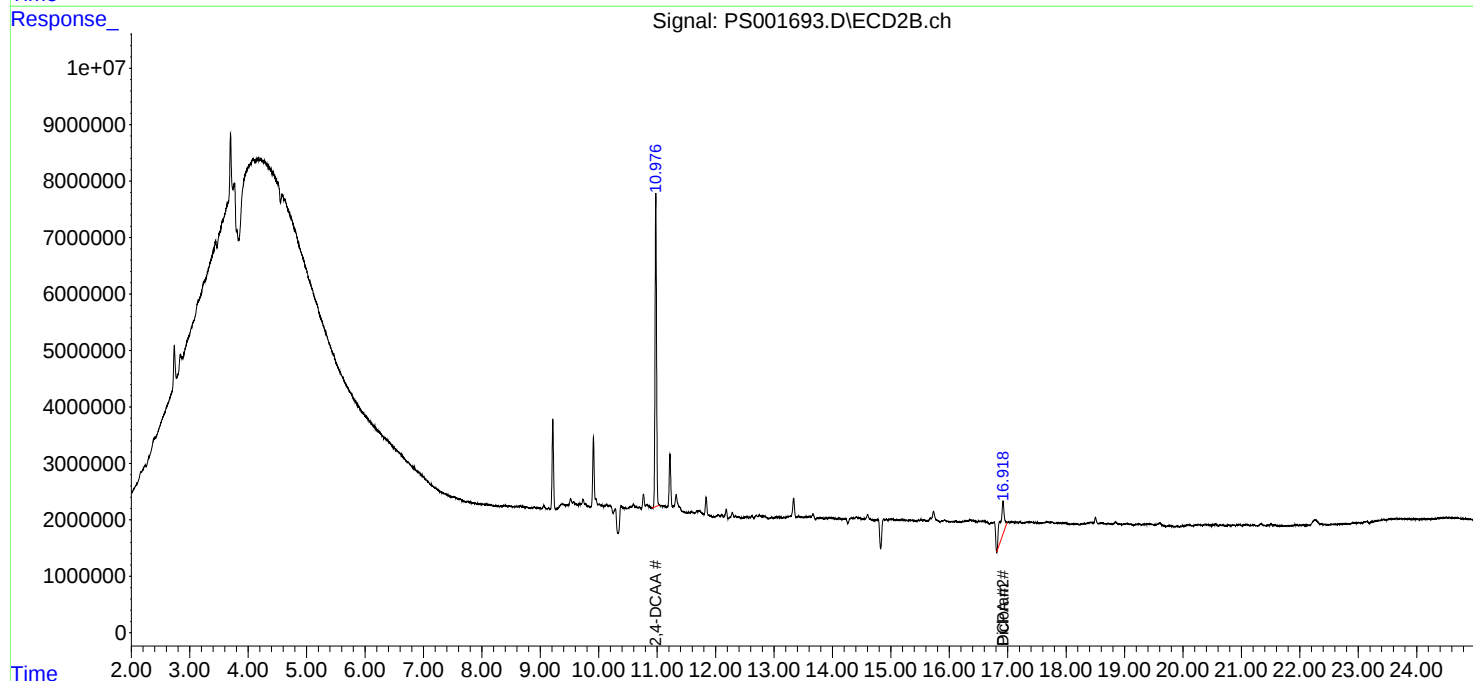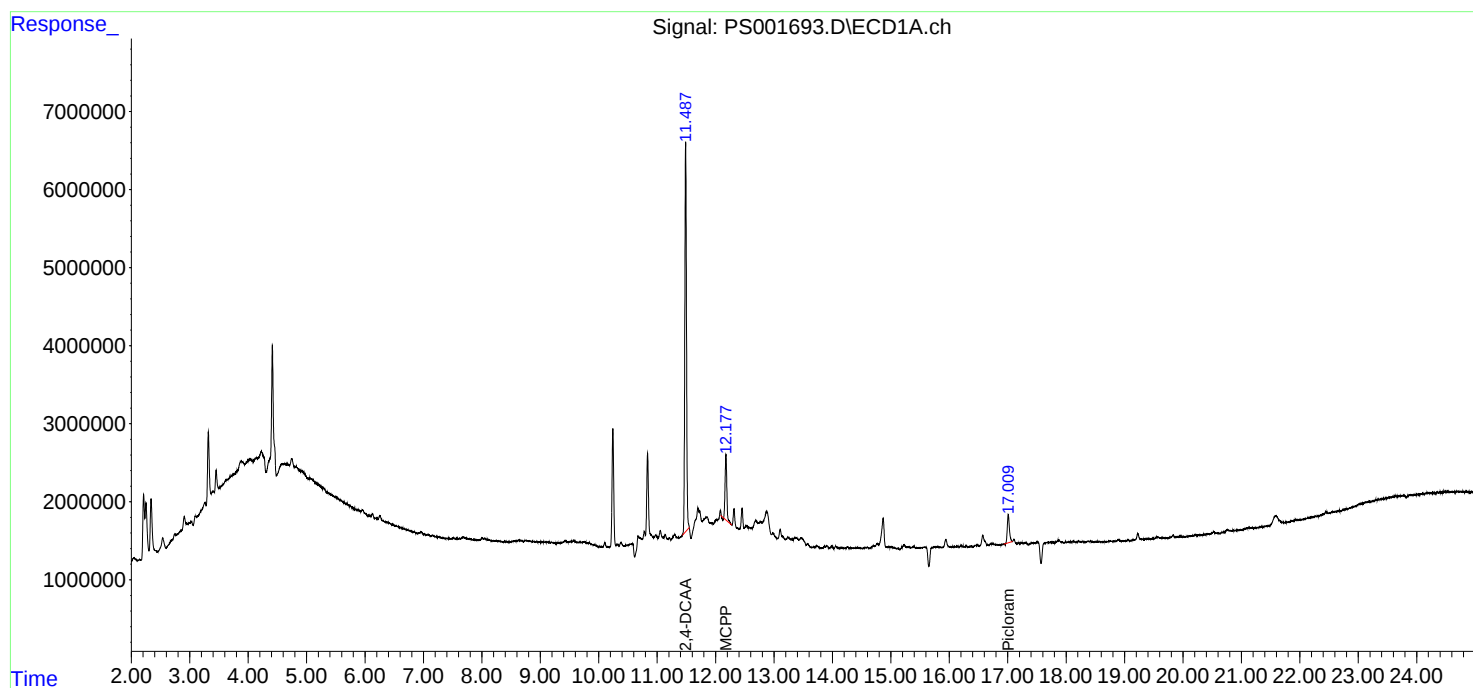


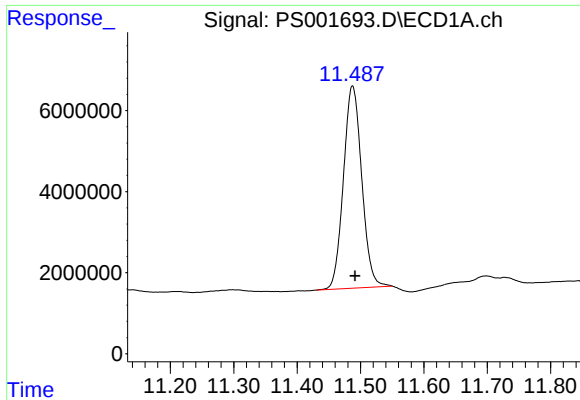

#4 2,4-DCAA


R.T.: 11.488 min
Delta R.T.: -0.004 min
Response: 100134414
Conc: 542.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

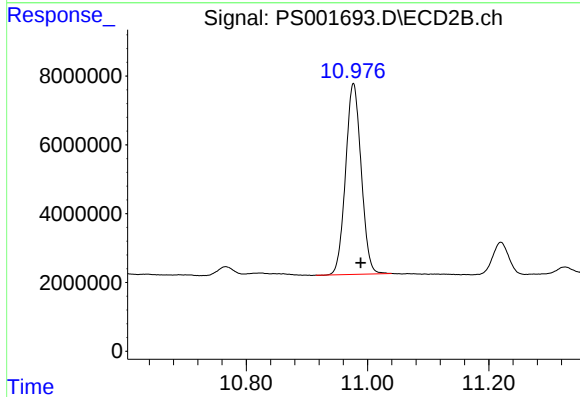


#4 2,4-DCAA

R.T.: 10.977 min
Delta R.T.: -0.012 min
Response: 98971041
Conc: 488.67 ng/ml

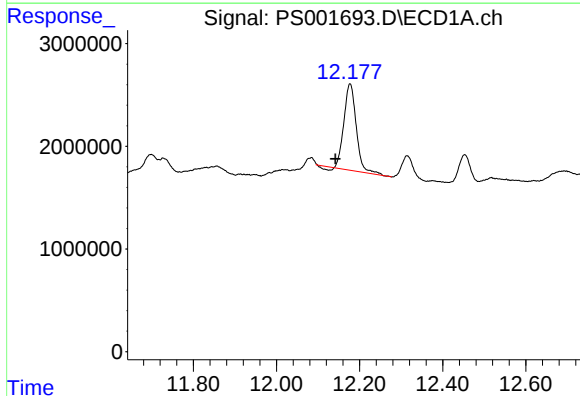


#6 MCP

R.T.: 12.177 min
Delta R.T.: 0.035 min
Response: 17189838
Conc: 34.16 ug/ml

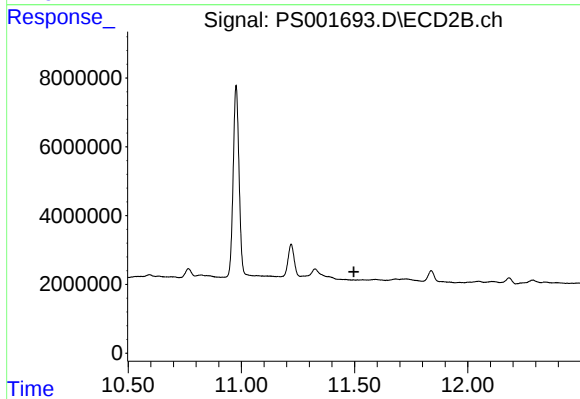

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

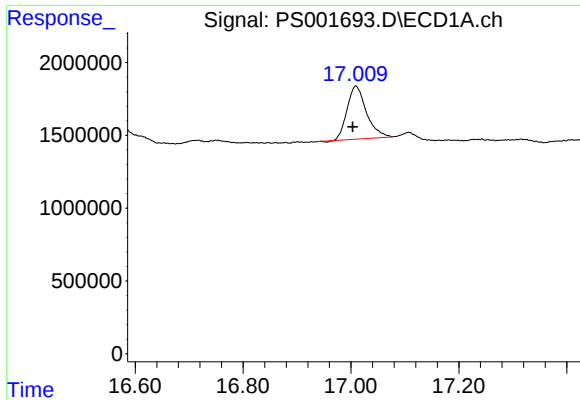

#15 Picloram


R.T.: 17.009 min
Delta R.T.: 0.006 min
Response: 9046194
Conc: 6.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

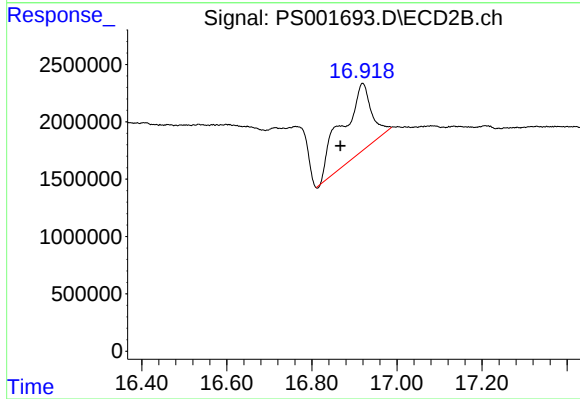


#15 Picloram

R.T.: 16.919 min
Delta R.T.: 0.052 min
Response: 29084658
Conc: 22.30 ng/ml

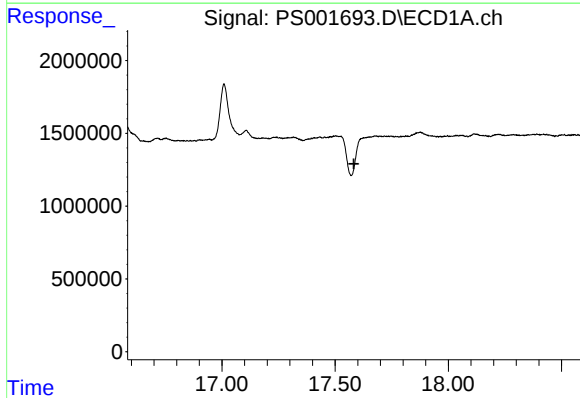

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

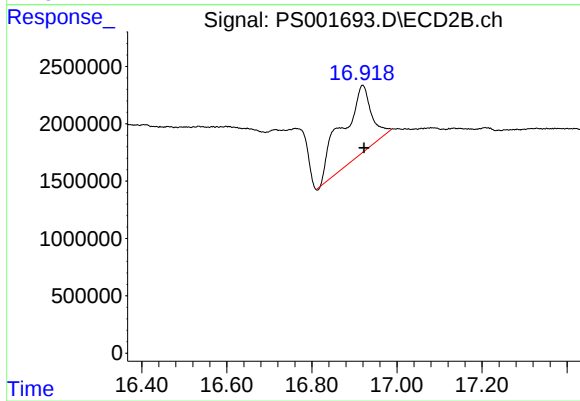

#16 DCPA

R.T.: 16.919 min
Delta R.T.: -0.003 min
Response: 29084658
Conc: 20.37 ng/ml