

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
 Data File : PS001695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2018 17:45
 Operator : EI\SJ
 Sample : J4782-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 00:50:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.482	10.980	41315259	46765828	223.809	230.908
Target Compounds							
1) T	Dalapon	2.945	2.465	2878851	4803926	11.452	20.073 #
3) T	4-Nitroph...	0.000	10.134	0	5486227	N.D.	52.050 #
6) T	MCP	12.167	0.000	20171278	0	40.089	N.D. #
10) T	Pentachlo...	13.725	13.414	9500750	2099124	3.810	0.776 #
13) T	2,4-DB	15.786	15.238	1396951	3037923	10.400	22.909 #
14) T	DINOSEB	0.000	15.672	0	5199849	N.D.	7.031 #
15) T	Picloram	16.994	16.859	4728658	12111589	3.376	9.288 #
16) T	DCPA	0.000	16.916	0	13059687	N.D.	9.147 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
Data File : PS001695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2018 17:45
Operator : EI\SJ
Sample : J4782-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:50:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

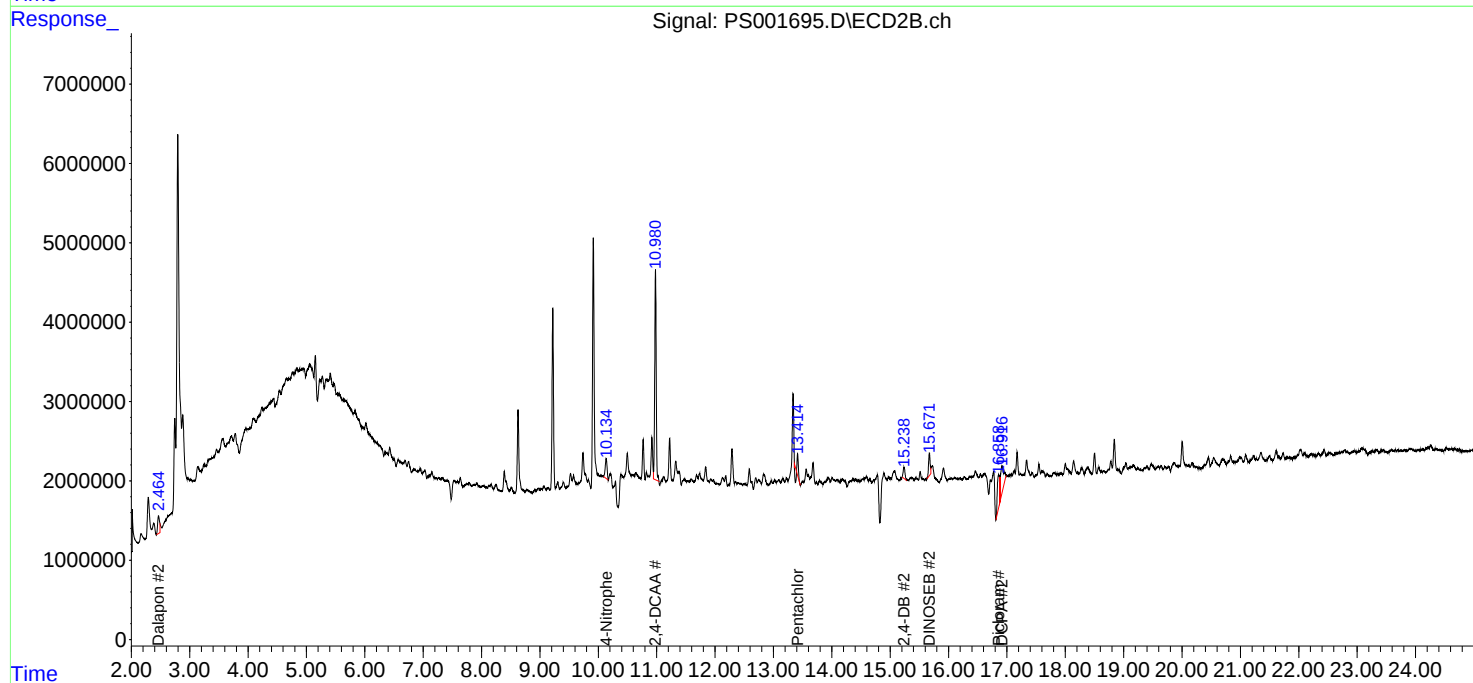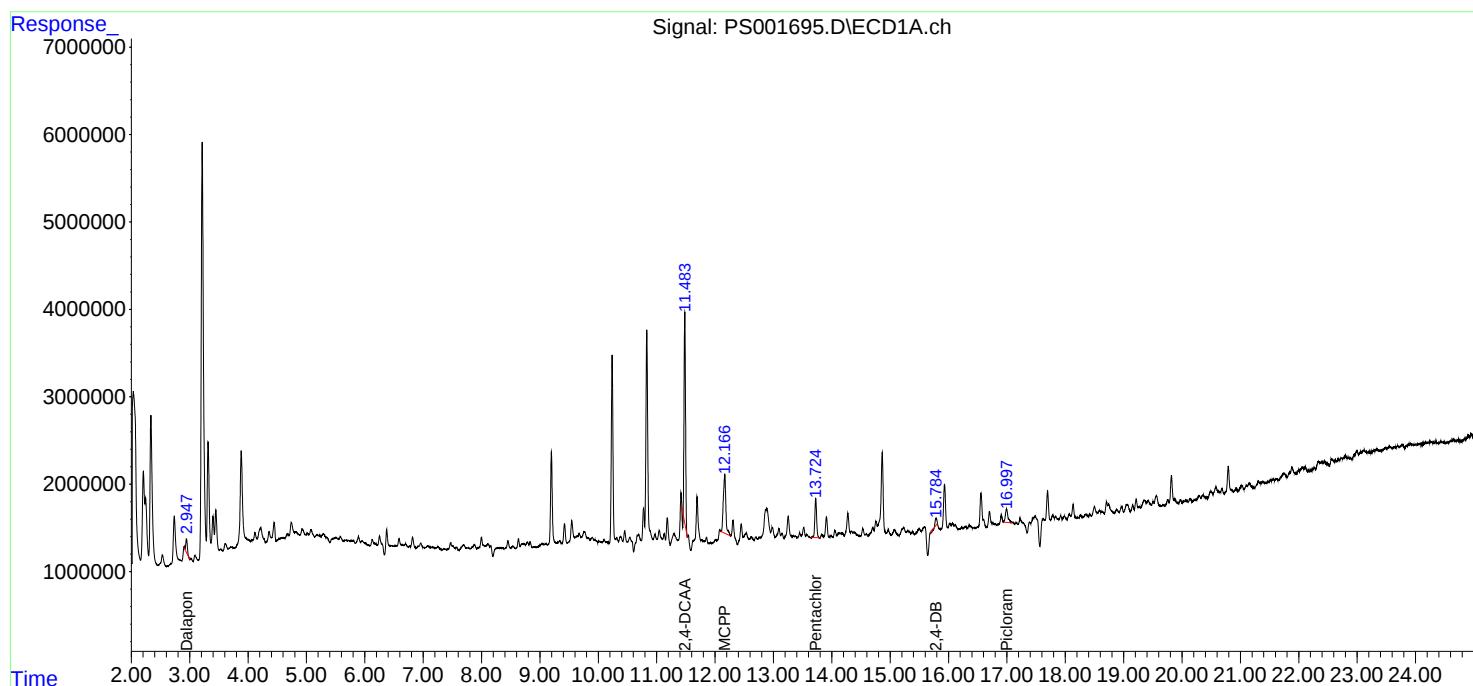


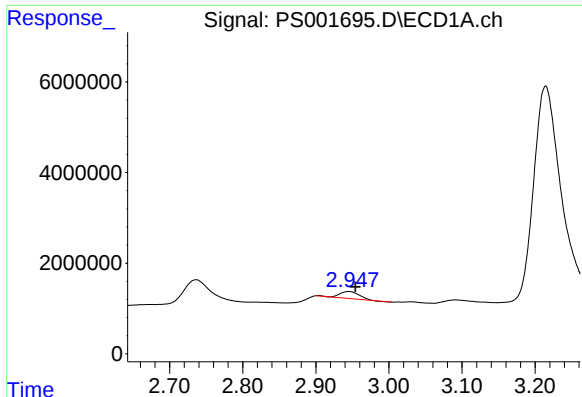

#1 Dalapon


R.T.: 2.945 min
Delta R.T.: -0.009 min
Response: 2878851
Conc: 11.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

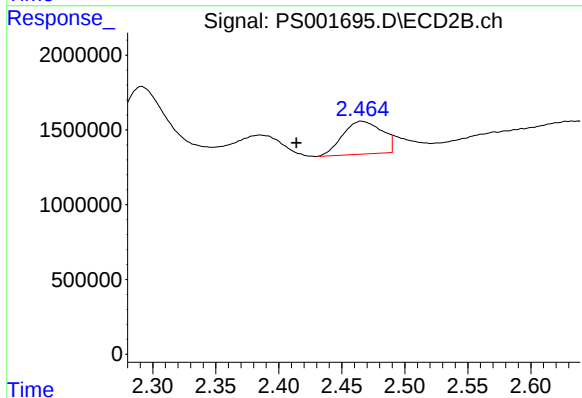


#1 Dalapon

R.T.: 2.465 min
Delta R.T.: 0.051 min
Response: 4803926
Conc: 20.07 ng/ml

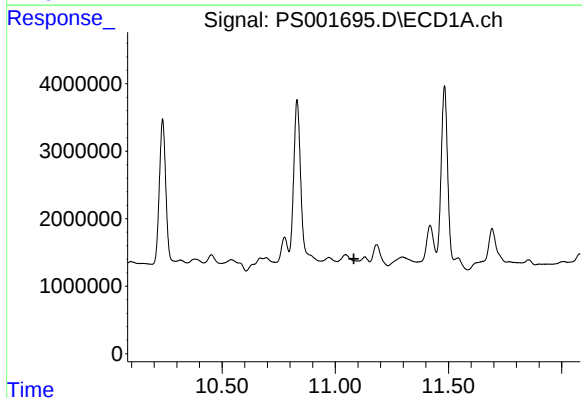


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.082 min
Response: 0
Conc: N.D.

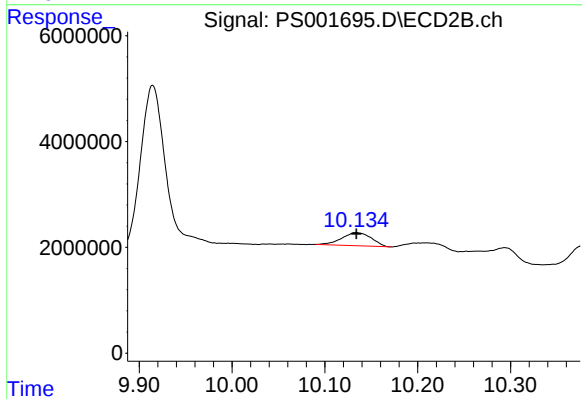

#3 4-Nitrophenol


R.T.: 10.134 min
Delta R.T.: 0.000 min
Response: 5486227
Conc: 52.05 ng/ml

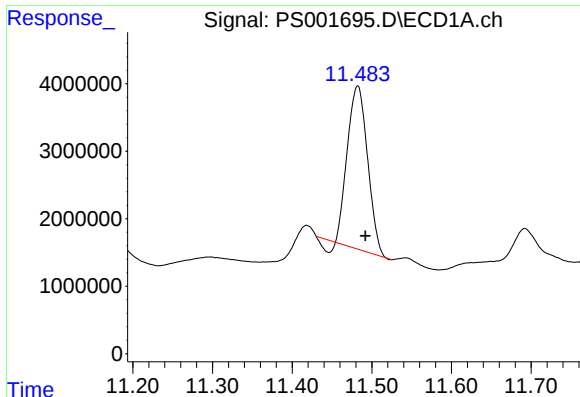

#4 2,4-DCAA


R.T.: 11.482 min
Delta R.T.: -0.010 min
Response: 41315259
Conc: 223.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

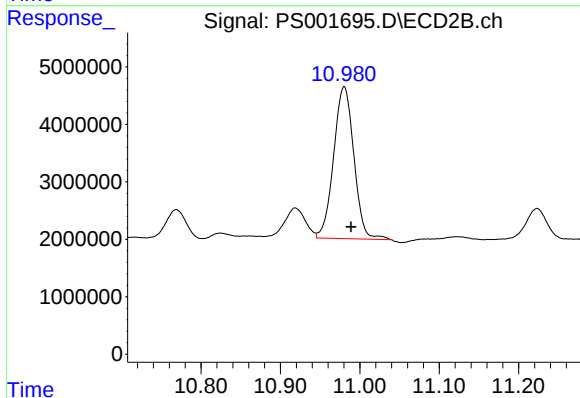


#4 2,4-DCAA

R.T.: 10.980 min
Delta R.T.: -0.009 min
Response: 46765828
Conc: 230.91 ng/ml

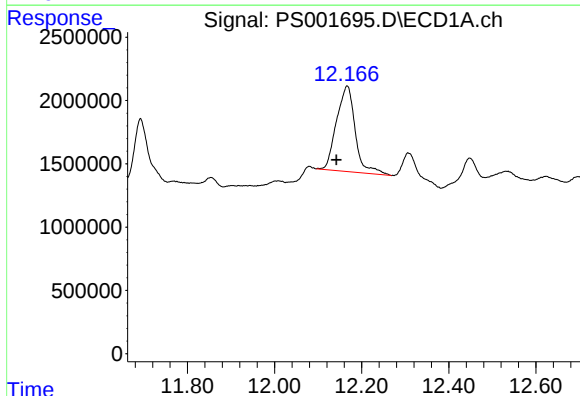


#6 MCP

R.T.: 12.167 min
Delta R.T.: 0.025 min
Response: 20171278
Conc: 40.09 ug/ml

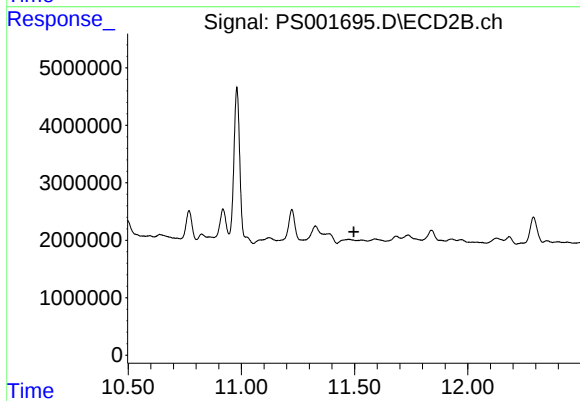

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

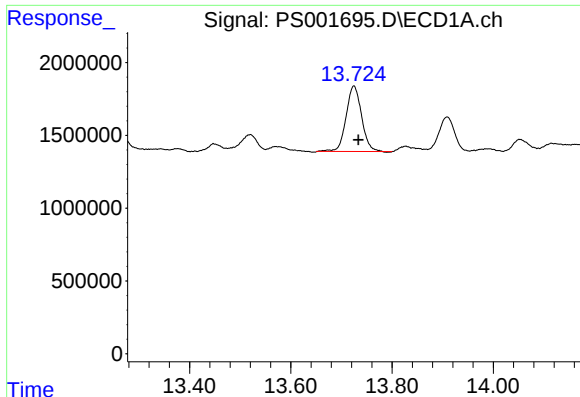

#10 Pentachlorophenol


R.T.: 13.725 min
Delta R.T.: -0.009 min
Response: 9500750
Conc: 3.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

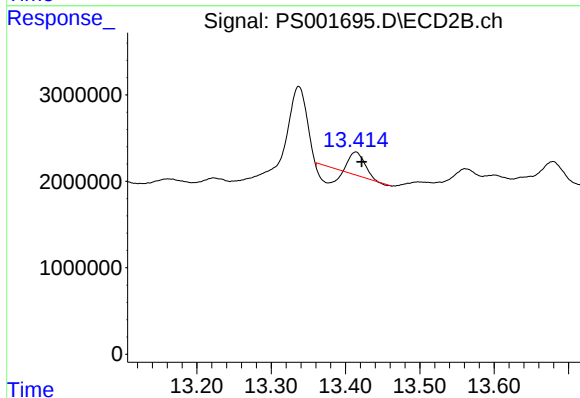


#10 Pentachlorophenol

R.T.: 13.414 min
Delta R.T.: -0.008 min
Response: 2099124
Conc: 0.78 ng/ml

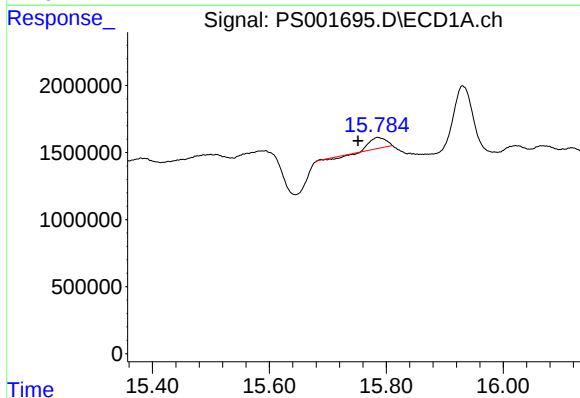


#13 2,4-DB

R.T.: 15.786 min
Delta R.T.: 0.034 min
Response: 1396951
Conc: 10.40 ng/ml

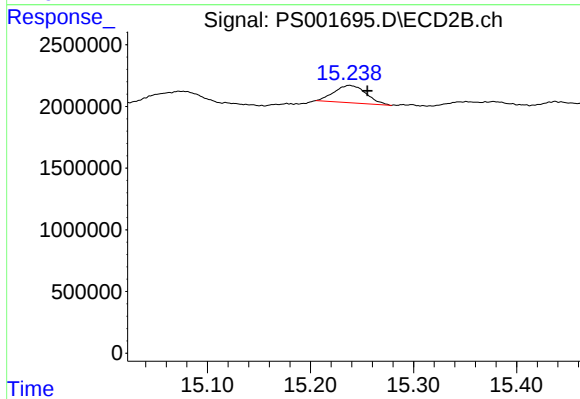

#13 2,4-DB


R.T.: 15.238 min
Delta R.T.: -0.017 min
Response: 3037923
Conc: 22.91 ng/ml

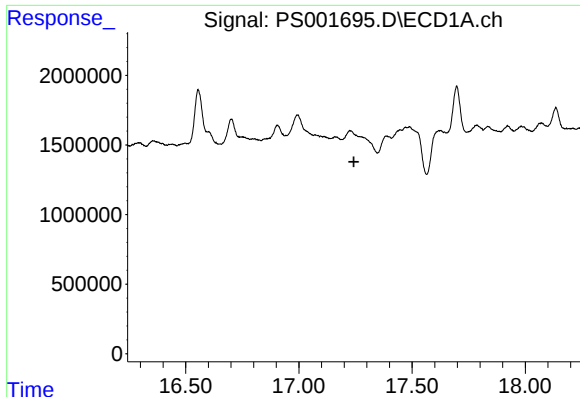

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

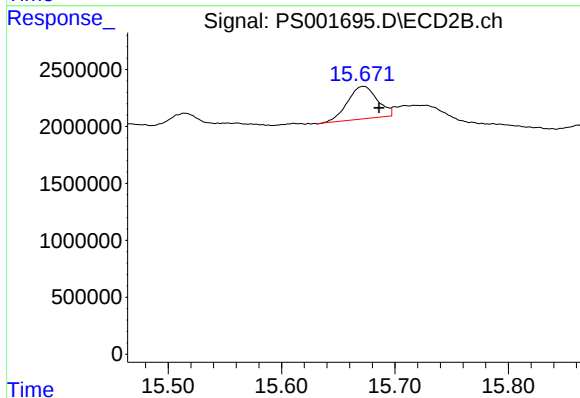


#14 DINOSEB

R.T.: 15.672 min
Delta R.T.: -0.014 min
Response: 5199849
Conc: 7.03 ng/ml

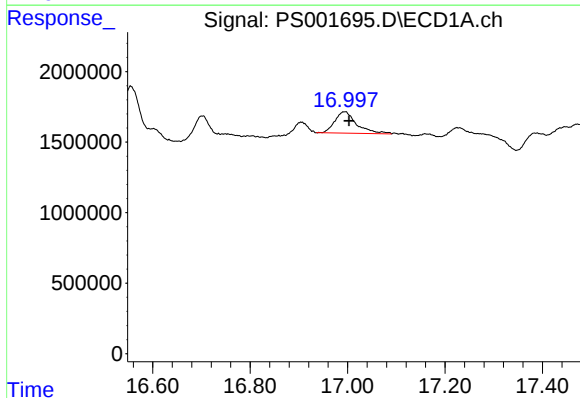


#15 Picloram

R.T.: 16.994 min
Delta R.T.: -0.009 min
Response: 4728658
Conc: 3.38 ng/ml

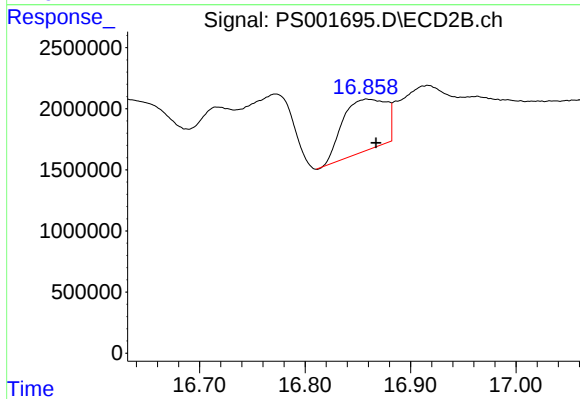

#15 Picloram


R.T.: 16.859 min
Delta R.T.: -0.008 min
Response: 12111589
Conc: 9.29 ng/ml

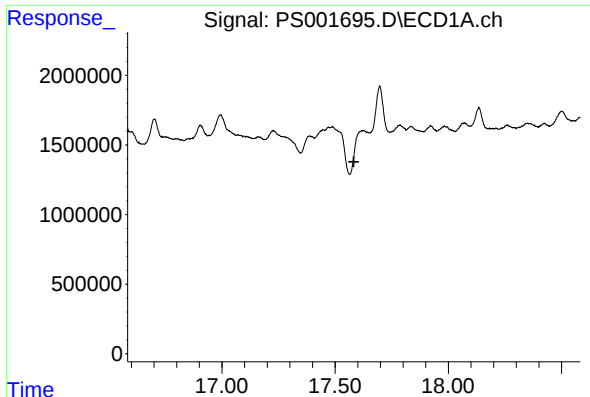

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

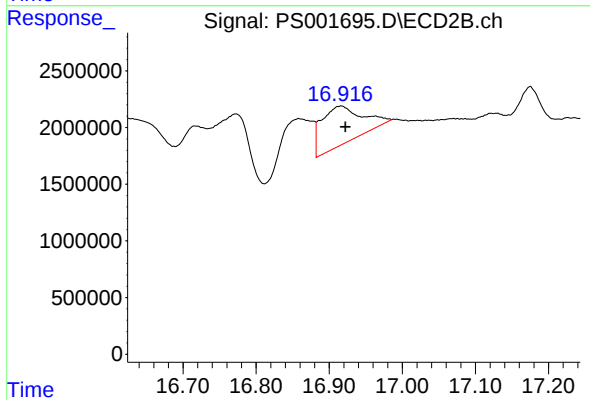

#16 DCPA

R.T.: 16.916 min
Delta R.T.: -0.007 min
Response: 13059687
Conc: 9.15 ng/ml