

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS091118\  
 Data File : PS001703.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 11 Sep 2018 21:53  
 Operator : EI\SJ  
 Sample : J4836-01  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 12 00:52:02 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS082218.M  
 Quant Title : 8080.M  
 QLast Update : Thu Aug 23 02:55:24 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|--------------|--------|--------|----------|----------|---------|----------|
| -----                       |              |        |        |          |          |         |          |
| System Monitoring Compounds |              |        |        |          |          |         |          |
| 4) S                        | 2,4-DCAA     | 11.479 | 10.978 | 58477473 | 58883399 | 316.779 | 290.739  |
| Target Compounds            |              |        |        |          |          |         |          |
| 6) T                        | MCP          | 12.168 | 0.000  | 27548648 | 0        | 54.751  | N.D. #   |
| 10) T                       | Pentachlo... | 13.725 | 0.000  | 3743172  | 0        | 1.501   | N.D. #   |
| 14) T                       | DINOSEB      | 0.000  | 15.727 | 0        | 4487883  | N.D.    | 6.068 #  |
| 15) T                       | Picloram     | 16.984 | 16.859 | 6072179  | 13569254 | 4.335   | 10.406 # |
| 16) T                       | DCPA         | 0.000  | 16.913 | 0        | 19195764 | N.D.    | 13.445 # |
| -----                       |              |        |        |          |          |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS091118\  
Data File : PS001703.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 11 Sep 2018 21:53  
Operator : EI\SJ  
Sample : J4836-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 12 00:52:02 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS082218.M  
Quant Title : 8080.M  
QLast Update : Thu Aug 23 02:55:24 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

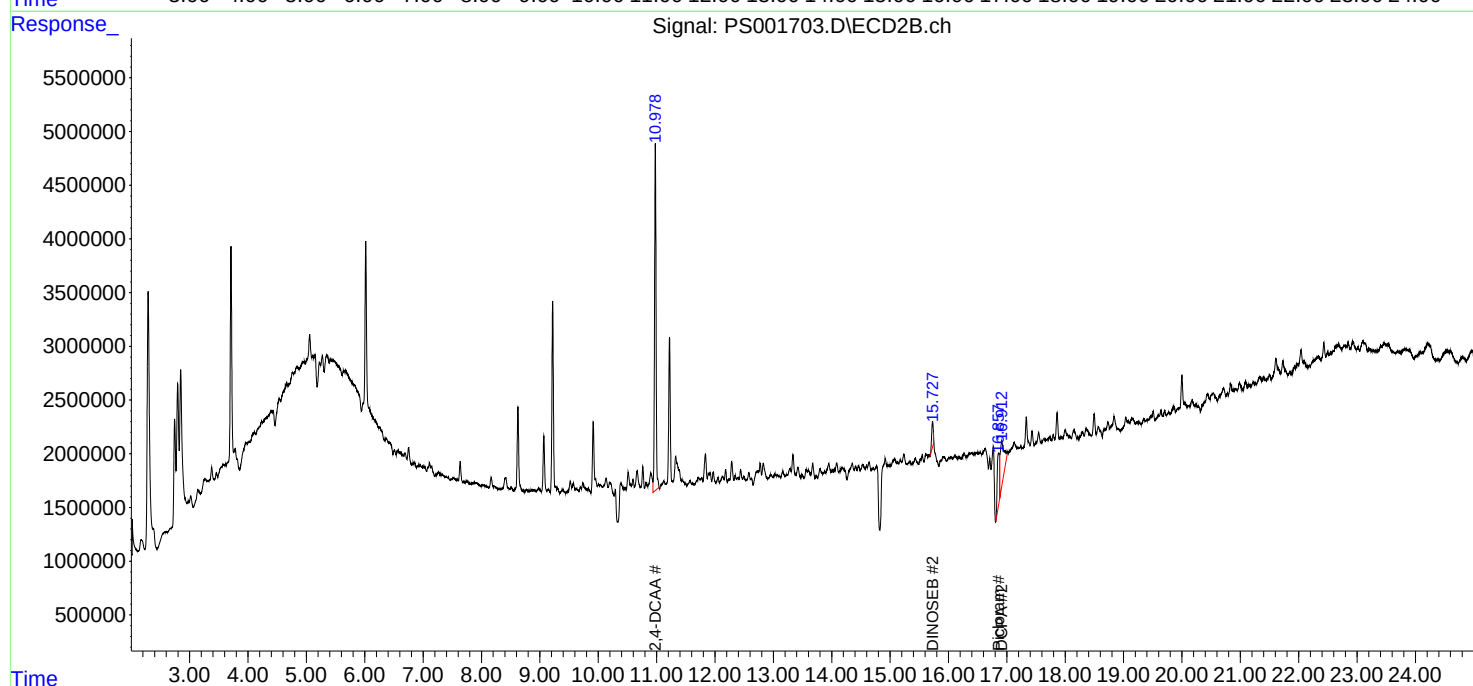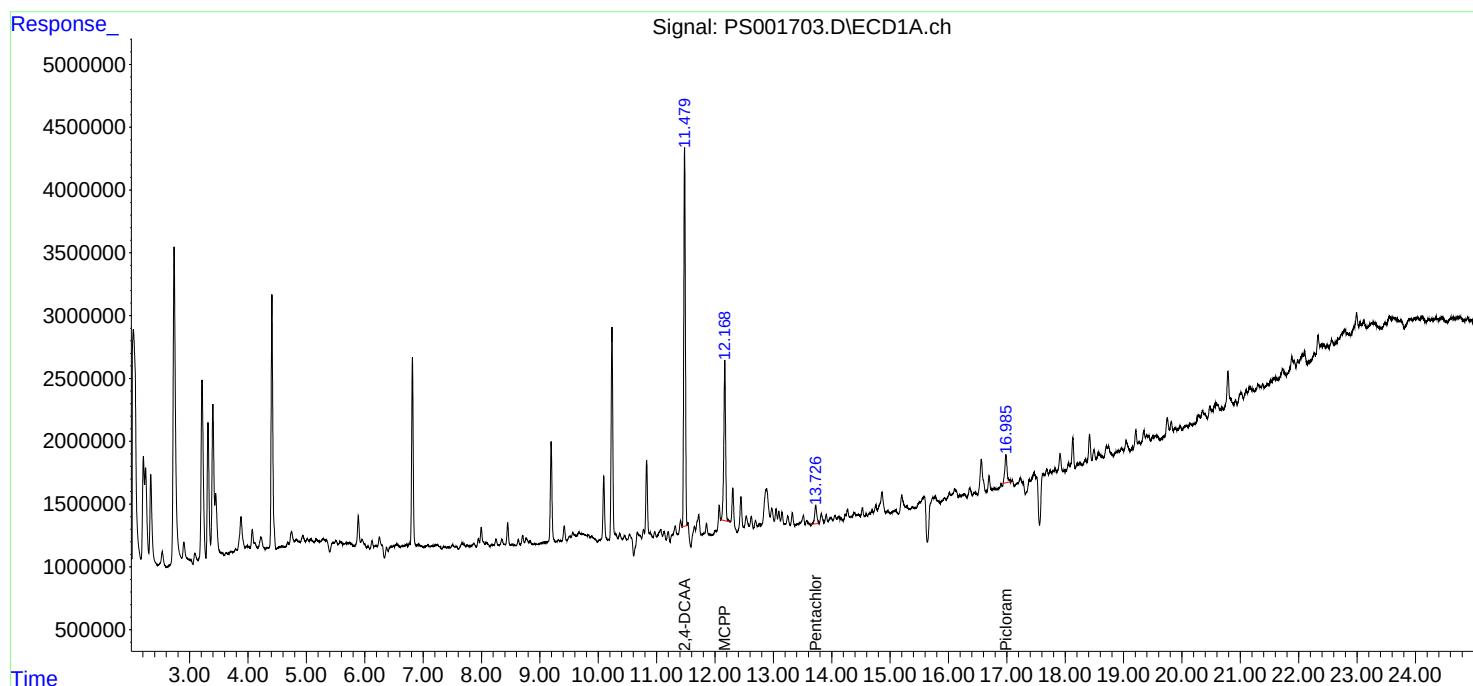


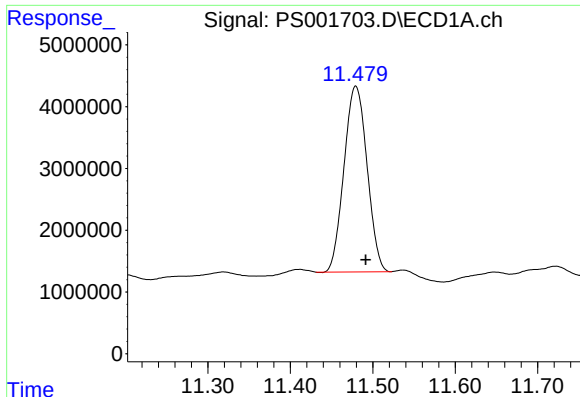

#4 2,4-DCAA


R.T.: 11.479 min  
Delta R.T.: -0.012 min  
Response: 58477473  
Conc: 316.78 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

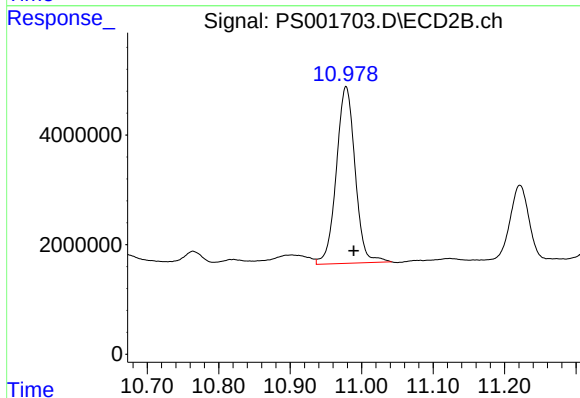


#4 2,4-DCAA

R.T.: 10.978 min  
Delta R.T.: -0.011 min  
Response: 58883399  
Conc: 290.74 ng/ml

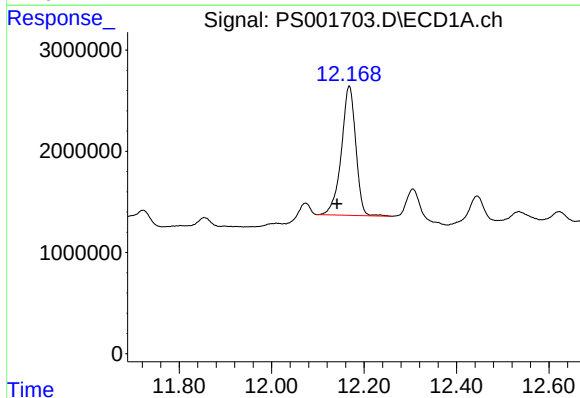


#6 MCP

R.T.: 12.168 min  
Delta R.T.: 0.026 min  
Response: 27548648  
Conc: 54.75 ug/ml

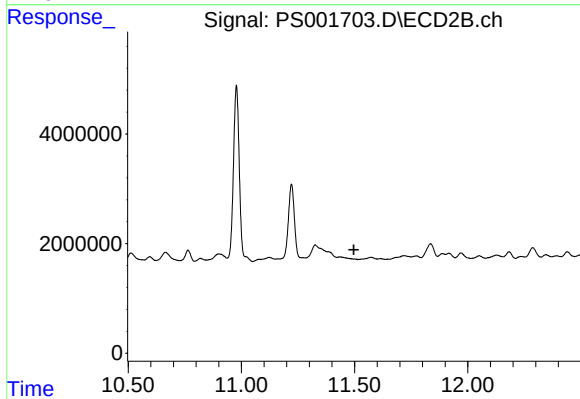

#6 MCP


R.T.: 0.000 min  
Exp R.T.: 11.497 min  
Response: 0  
Conc: N.D.

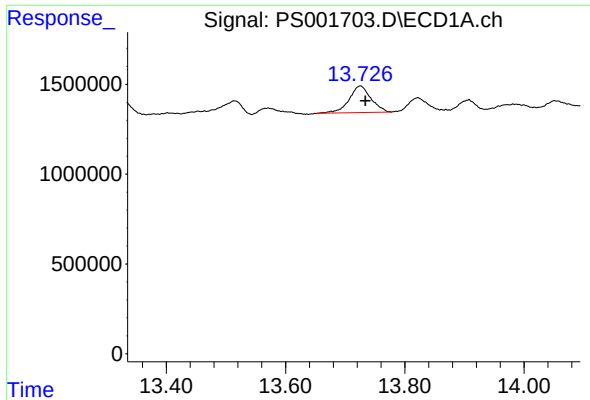

#10 Pentachlorophenol


R.T.: 13.725 min  
Delta R.T.: -0.009 min  
Response: 3743172  
Conc: 1.50 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

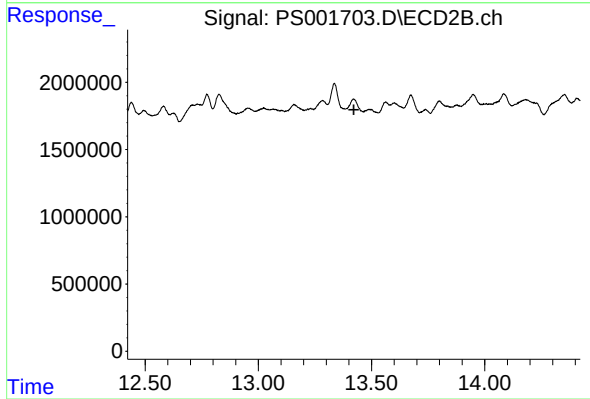


#10 Pentachlorophenol

R.T.: 0.000 min  
Exp R.T. : 13.422 min  
Response: 0  
Conc: N.D.

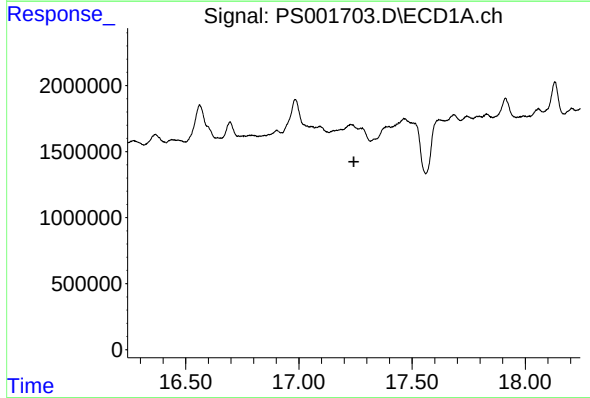


#14 DINOSEB

R.T.: 0.000 min  
Exp R.T. : 17.243 min  
Response: 0  
Conc: N.D.

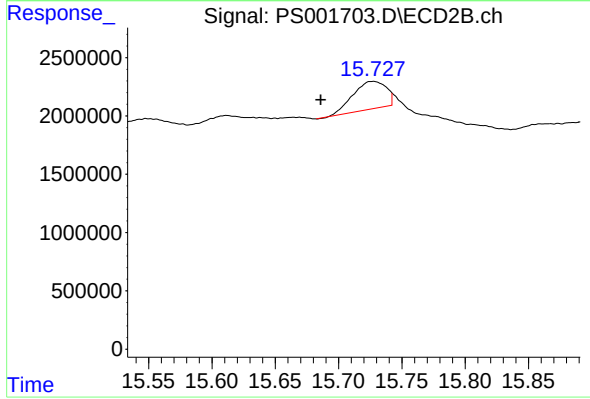

#14 DINOSEB


R.T.: 15.727 min  
Delta R.T.: 0.041 min  
Response: 4487883  
Conc: 6.07 ng/ml

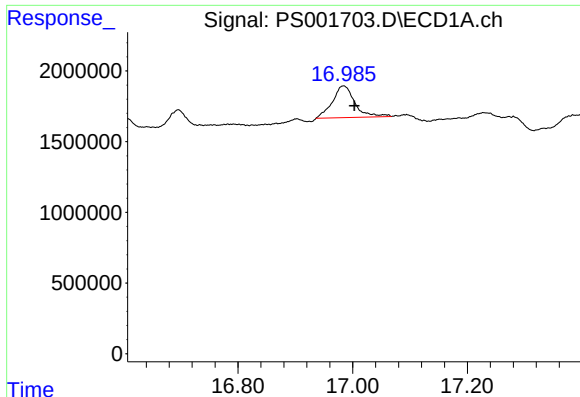

#15 Picloram


R.T.: 16.984 min  
Delta R.T.: -0.019 min  
Response: 6072179  
Conc: 4.34 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

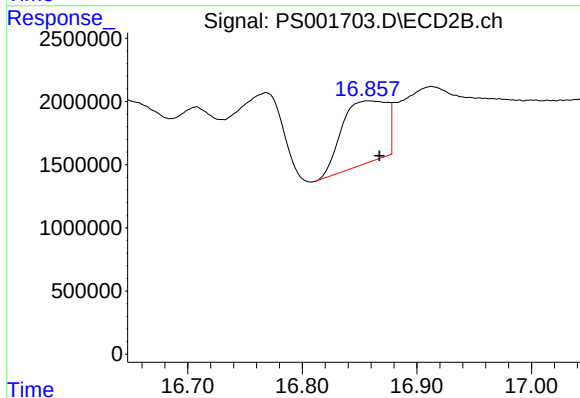


#15 Picloram

R.T.: 16.859 min  
Delta R.T.: -0.009 min  
Response: 13569254  
Conc: 10.41 ng/ml

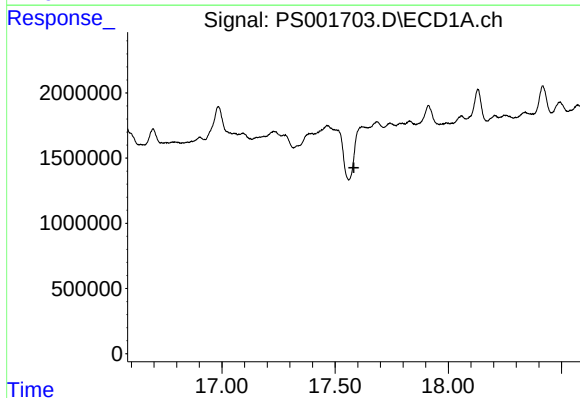

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 17.583 min  
Response: 0  
Conc: N.D.

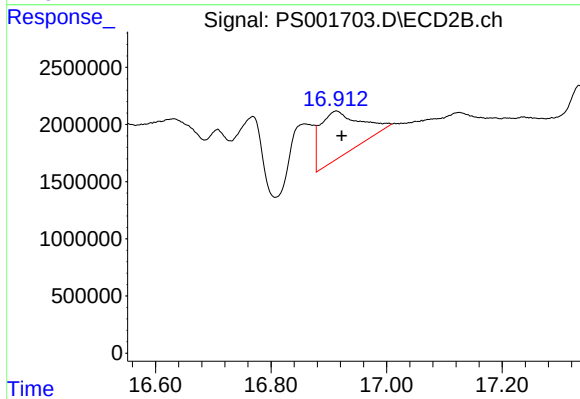

#16 DCPA

R.T.: 16.913 min  
Delta R.T.: -0.010 min  
Response: 19195764  
Conc: 13.44 ng/ml