

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
 Data File : PS001704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2018 22:24
 Operator : EI\SJ
 Sample : J4836-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 00:52:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.499	10.998	61463221	54906699	332.953	271.104
Target Compounds							
2) T	3,5-DICHL...	0.000	9.088	0	4603536	N.D.	18.014 #
3) T	4-Nitroph...	11.082	0.000	2900745	0	23.527	N.D. #
5) T	DICAMBA	0.000	11.242	0	12197291	N.D.	17.391 #
6) T	MCP	12.188	0.000	19322201	0	38.402	N.D. #
7) T	MCPA	12.325	11.858	1795585	2391322	2.151	3.281 #
8) T	DICHLORPROP	12.994	0.000	1700414	0	9.004	N.D. #
9) T	2,4-D	0.000	12.848	0	3448845	N.D.	13.922 #
10) T	Pentachlo...	13.744	0.000	5049769	0	2.025	N.D. #
13) T	2,4-DB	15.747	15.190	7328693	1041975	54.560	7.857 #
15) T	Picloram	0.000	16.874	0	7263661	N.D.	5.570 #
16) T	DCPA	0.000	16.938	0	14852998	N.D.	10.403 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
Data File : PS001704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2018 22:24
Operator : EI\SJ
Sample : J4836-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:52:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

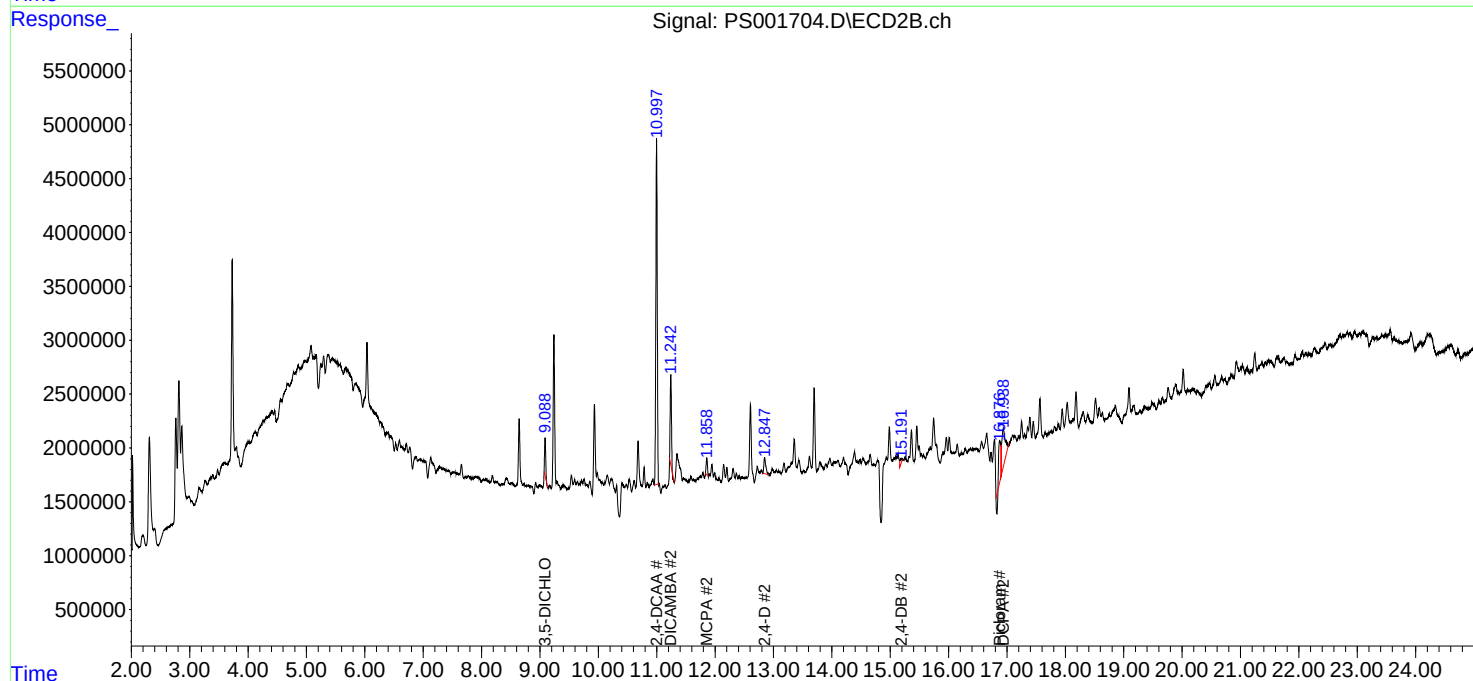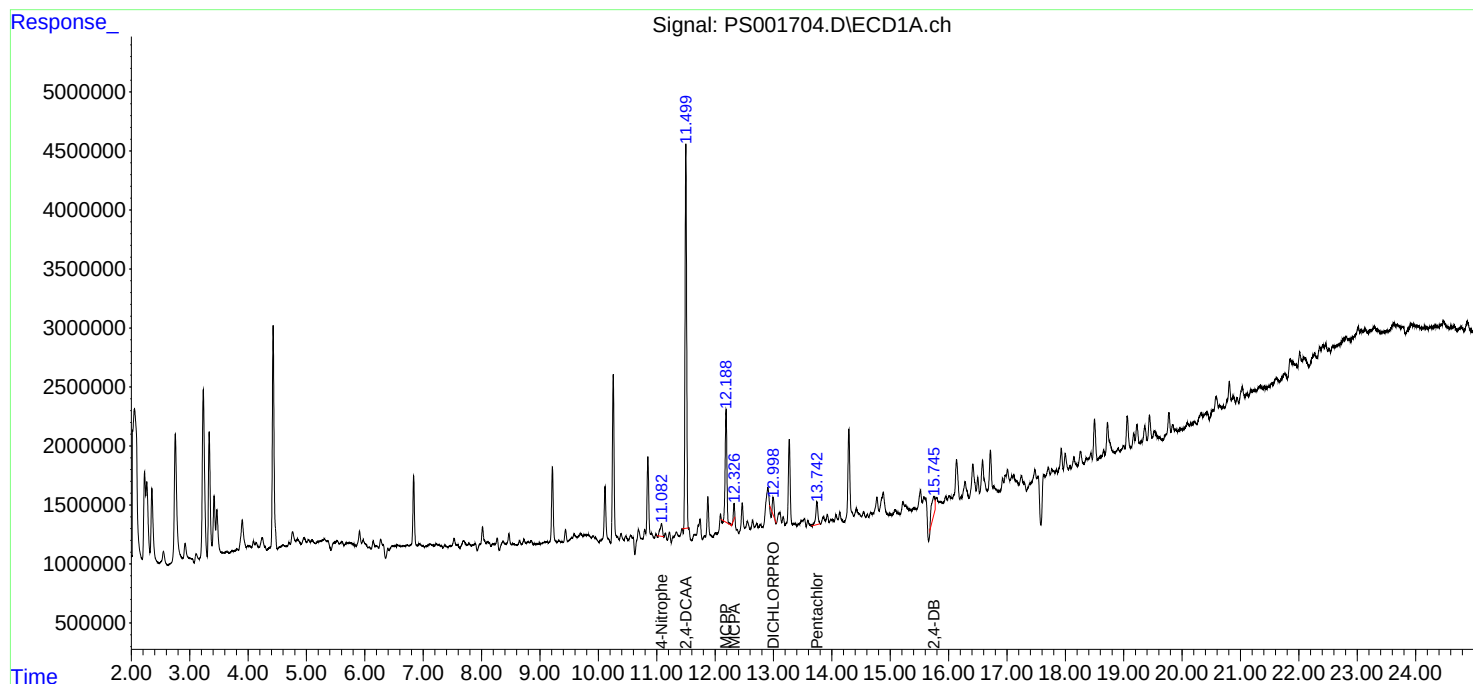


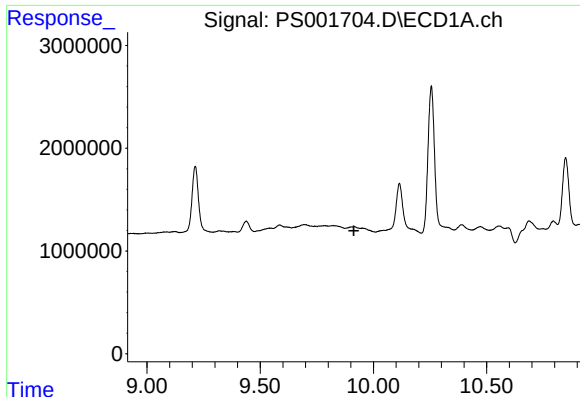

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

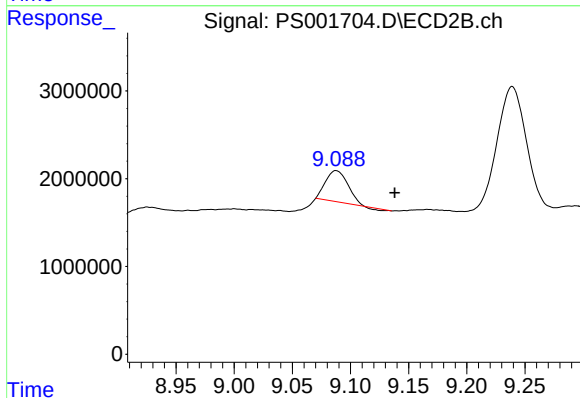


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.088 min
Delta R.T.: -0.050 min
Response: 4603536
Conc: 18.01 ng/ml

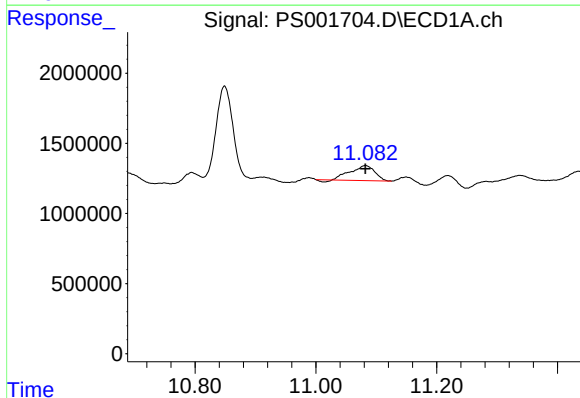


#3 4-Nitrophenol

R.T.: 11.082 min
Delta R.T.: 0.000 min
Response: 2900745
Conc: 23.53 ng/ml

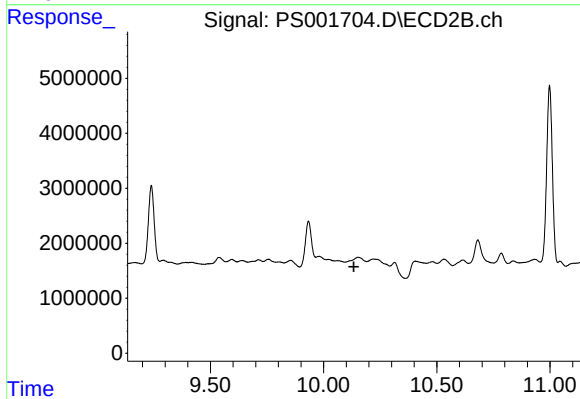

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.134 min
Response: 0
Conc: N.D.

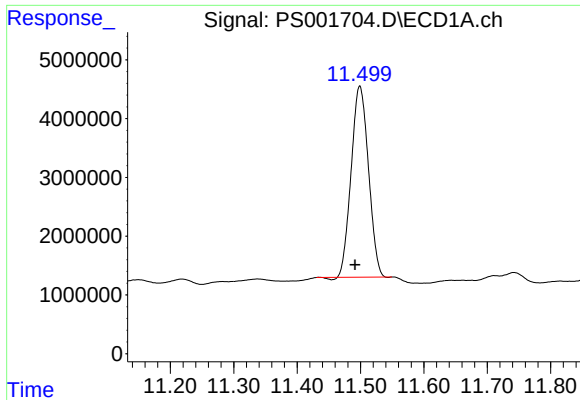

#4 2,4-DCAA


R.T.: 11.499 min
Delta R.T.: 0.007 min
Response: 61463221
Conc: 332.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

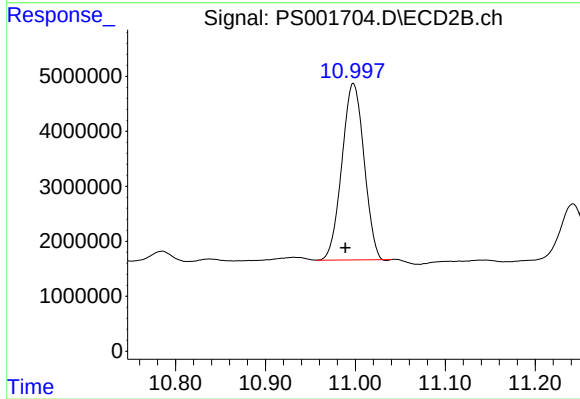


#4 2,4-DCAA

R.T.: 10.998 min
Delta R.T.: 0.009 min
Response: 54906699
Conc: 271.10 ng/ml

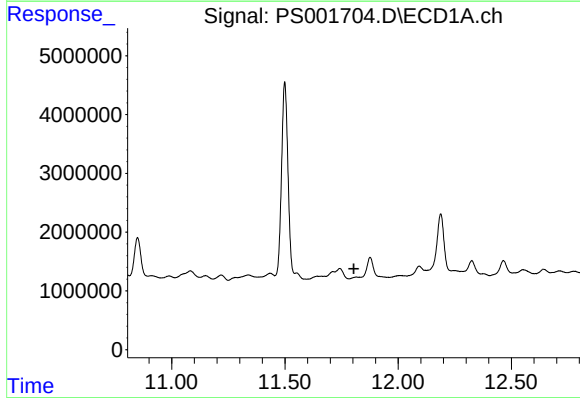


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

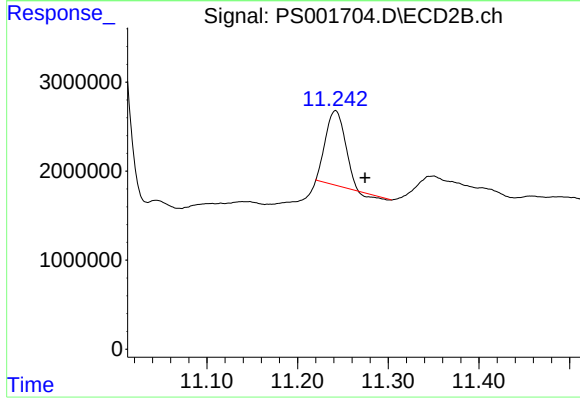

#5 DICAMBA


R.T.: 11.242 min
Delta R.T.: -0.033 min
Response: 12197291
Conc: 17.39 ng/ml

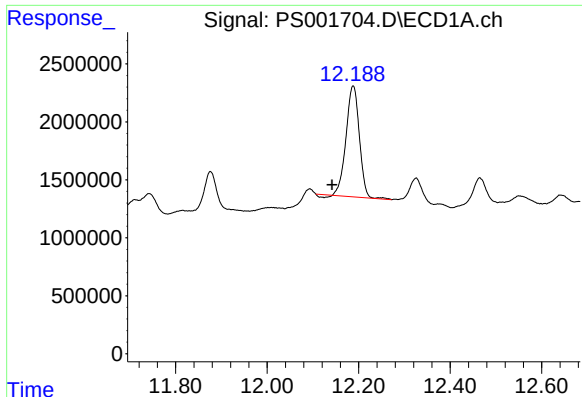

#6 MCP


R.T.: 12.188 min
Delta R.T.: 0.046 min
Response: 19322201
Conc: 38.40 ug/ml

Instrument :
ECD_S
ClientSampleId :

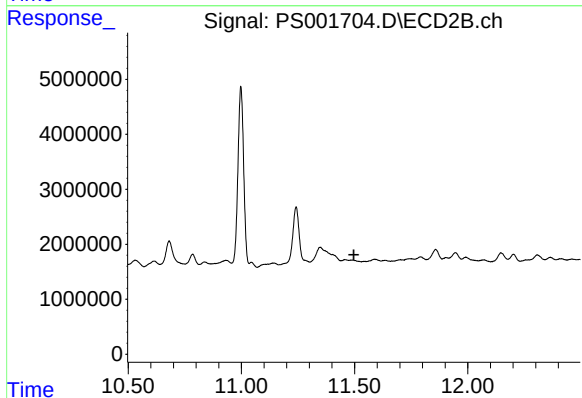


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

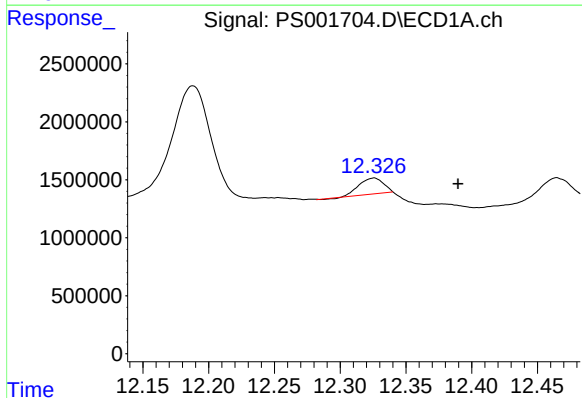


#7 MCP

R.T.: 12.325 min
Delta R.T.: -0.064 min
Response: 1795585
Conc: 2.15 ug/ml

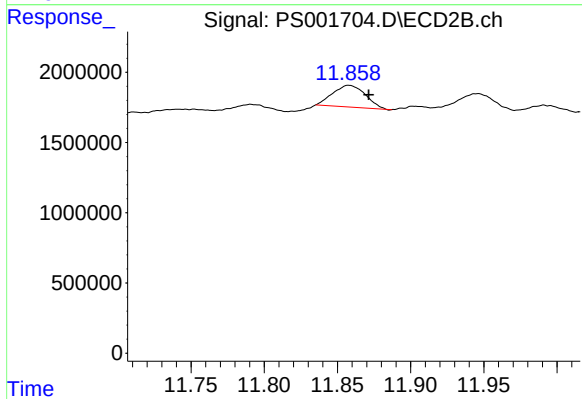

#7 MCP


R.T.: 11.858 min
Delta R.T.: -0.013 min
Response: 2391322
Conc: 3.28 ug/ml

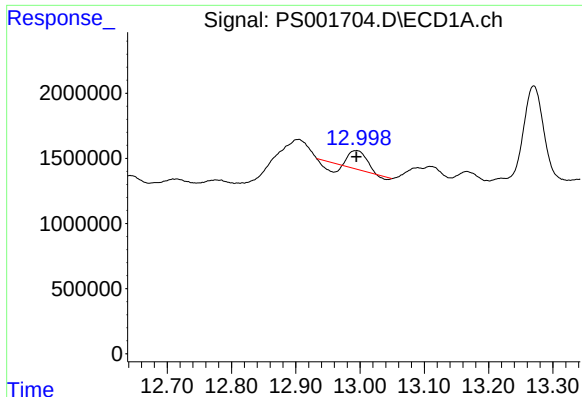

#8 DICHLORPROP


R.T.: 12.994 min
Delta R.T.: 0.000 min
Response: 1700414
Conc: 9.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

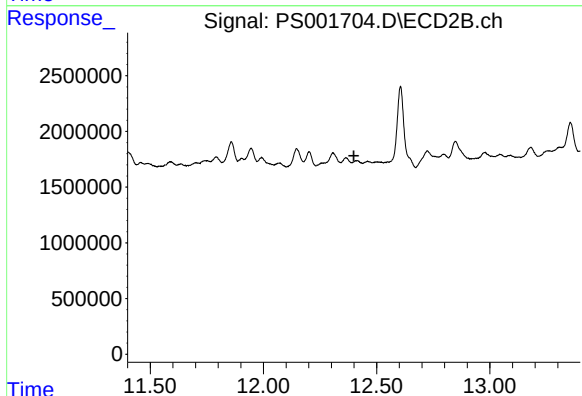


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.399 min
Response: 0
Conc: N.D.

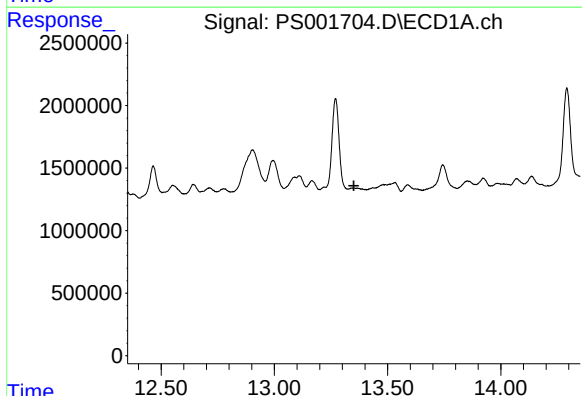


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.352 min
Response: 0
Conc: N.D.

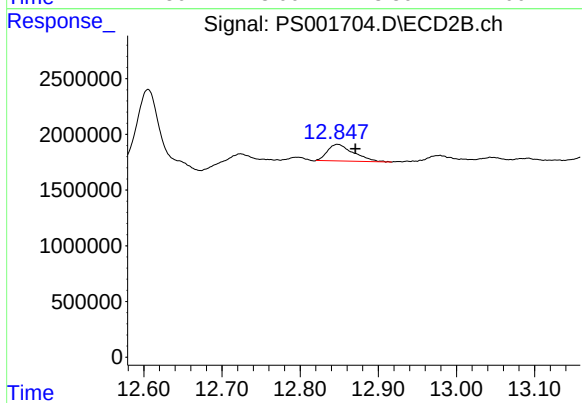

#9 2,4-D


R.T.: 12.848 min
Delta R.T.: -0.023 min
Response: 3448845
Conc: 13.92 ng/ml

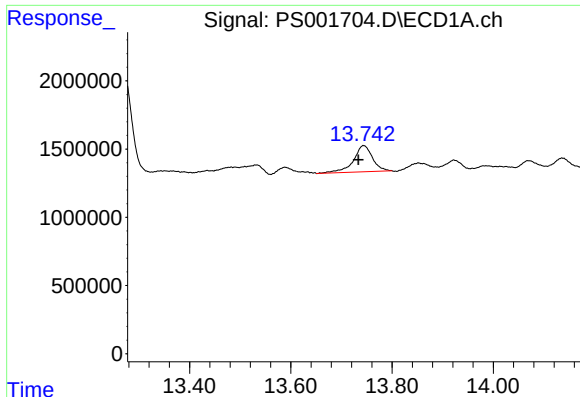

#10 Pentachlorophenol


R.T.: 13.744 min
Delta R.T.: 0.010 min
Response: 5049769
Conc: 2.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

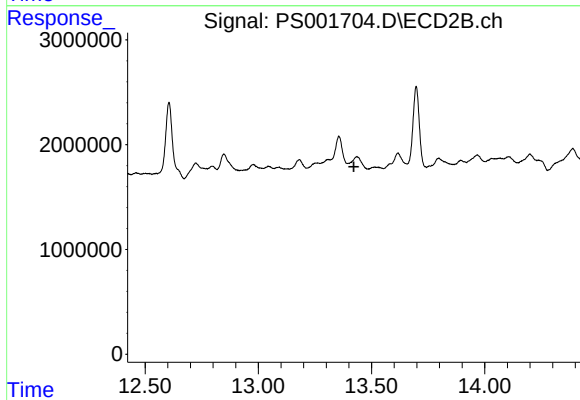


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.422 min
Response: 0
Conc: N.D.

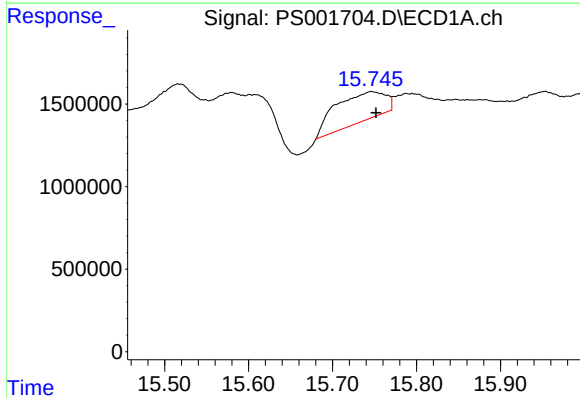


#13 2,4-DB

R.T.: 15.747 min
Delta R.T.: -0.005 min
Response: 7328693
Conc: 54.56 ng/ml

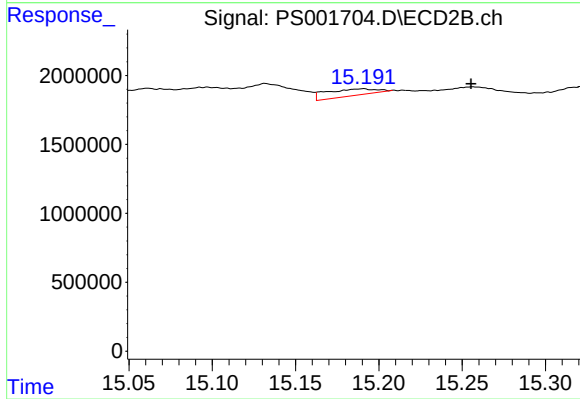

#13 2,4-DB


R.T.: 15.190 min
Delta R.T.: -0.066 min
Response: 1041975
Conc: 7.86 ng/ml

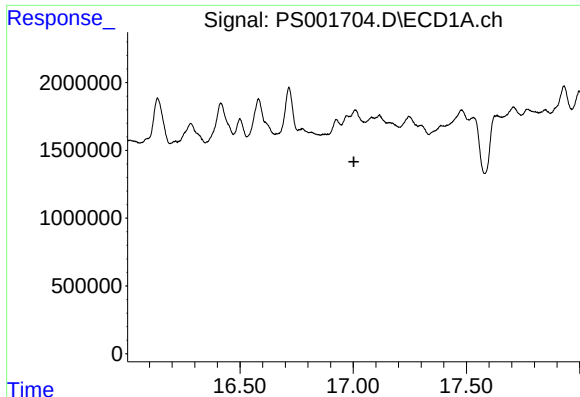

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

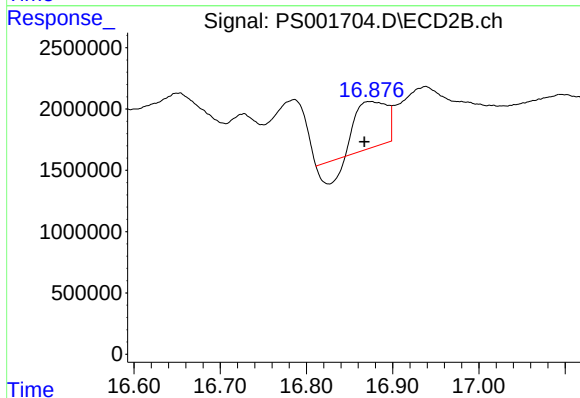


#15 Picloram

R.T.: 16.874 min
Delta R.T.: 0.006 min
Response: 7263661
Conc: 5.57 ng/ml

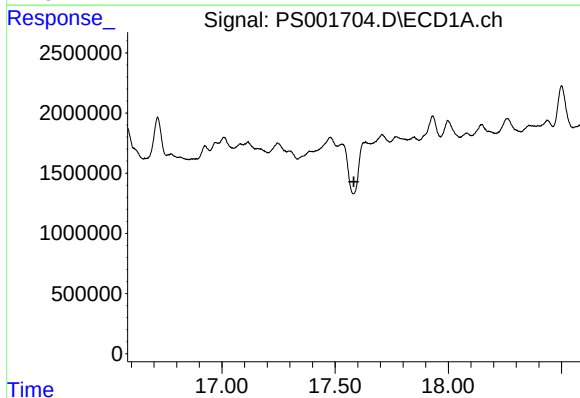

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

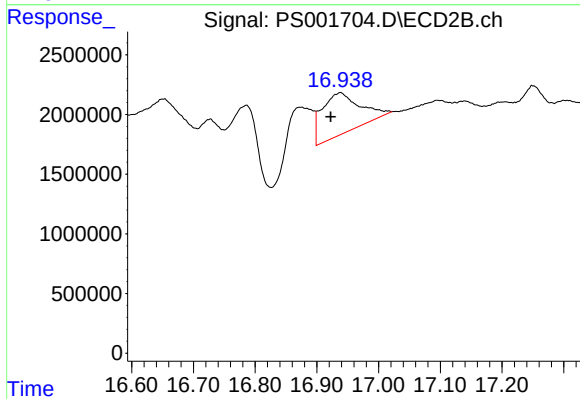

#16 DCPA

R.T.: 16.938 min
Delta R.T.: 0.015 min
Response: 14852998
Conc: 10.40 ng/ml