

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
 Data File : PS001707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2018 23:57
 Operator : EI\SJ
 Sample : J4847-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 00:52:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.481	10.980	56204195	56814190	304.464	280.522
Target Compounds							
6) T	MCP	12.170	0.000	28908437	0	57.454	N.D. #
10) T	Pentachlo...	13.726	0.000	2927968	0	1.174	N.D. #
13) T	2,4-DB	15.793	0.000	809824	0	6.029	N.D. #
15) T	Picloram	16.986	16.860	5440425	12020441	3.884	9.218 #
16) T	DCPA	0.000	16.915	0	11283183	N.D.	7.903 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091118\
Data File : PS001707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2018 23:57
Operator : EI\SJ
Sample : J4847-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 00:52:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

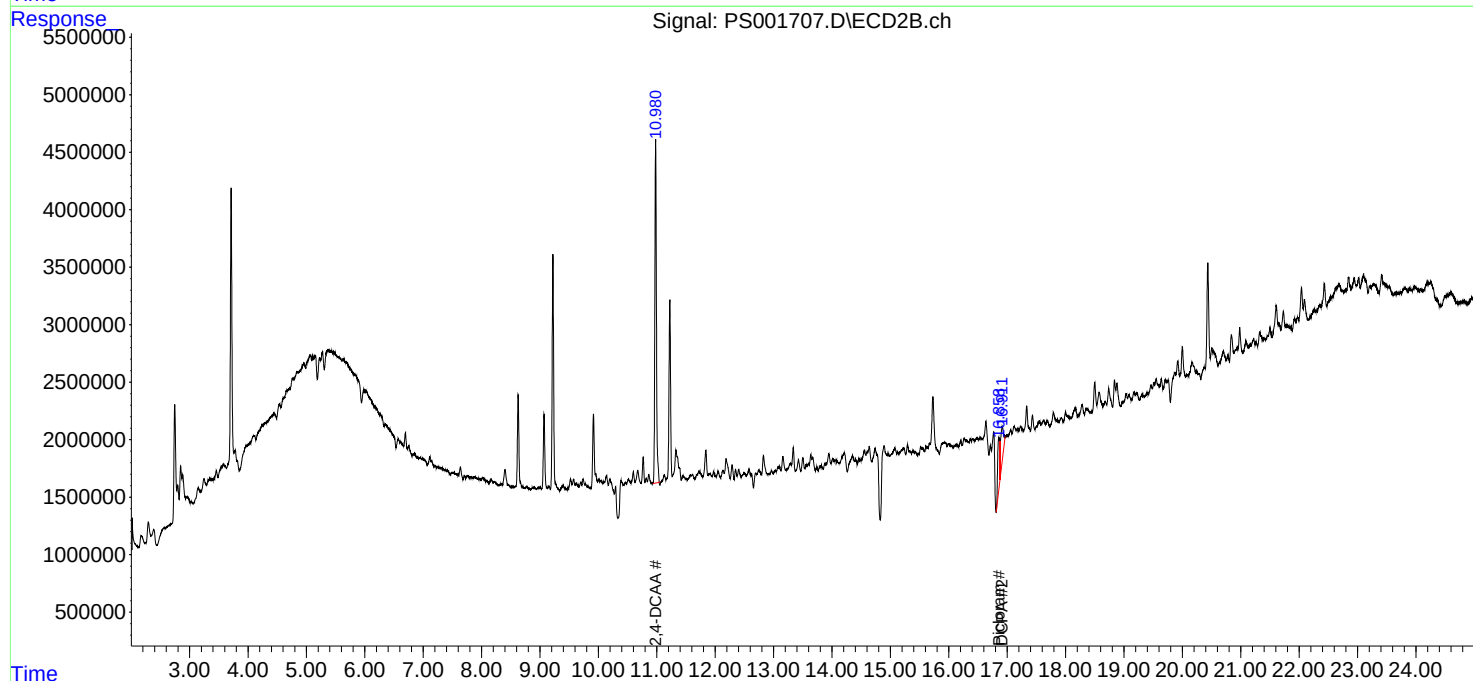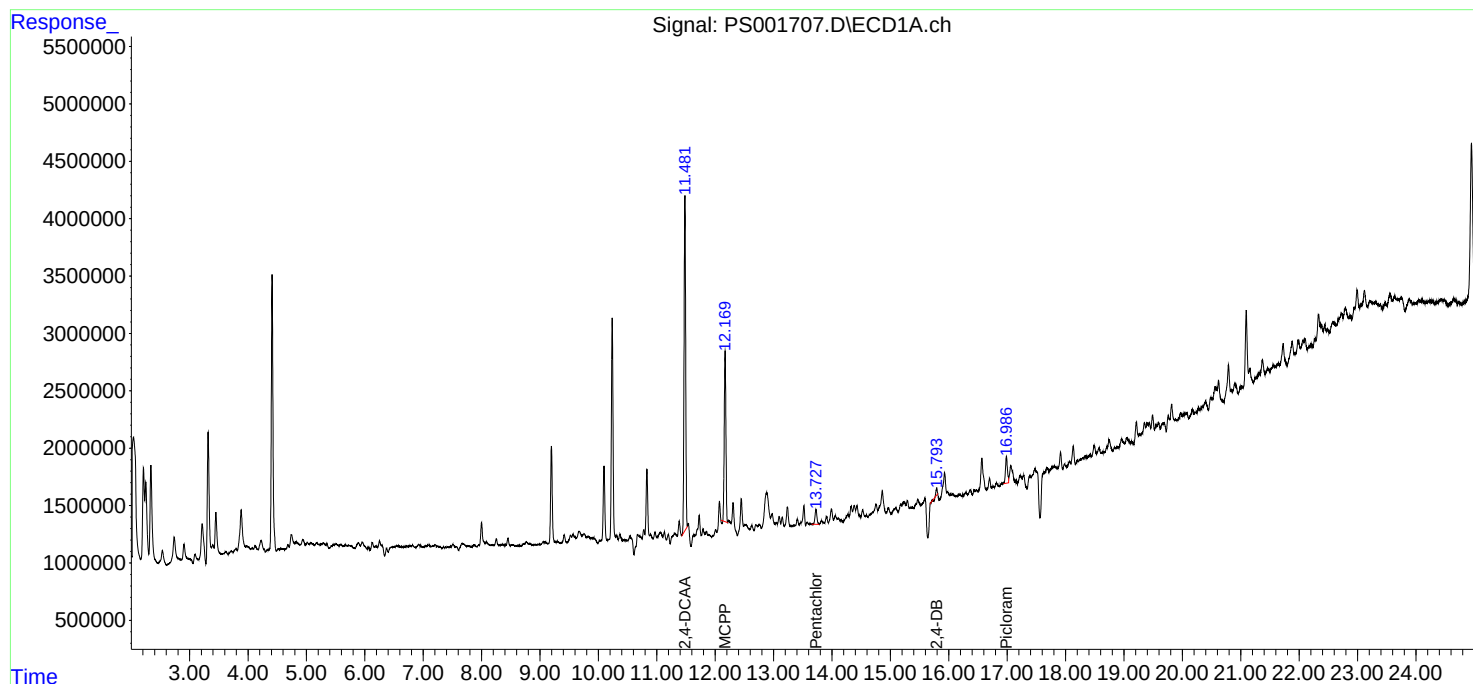


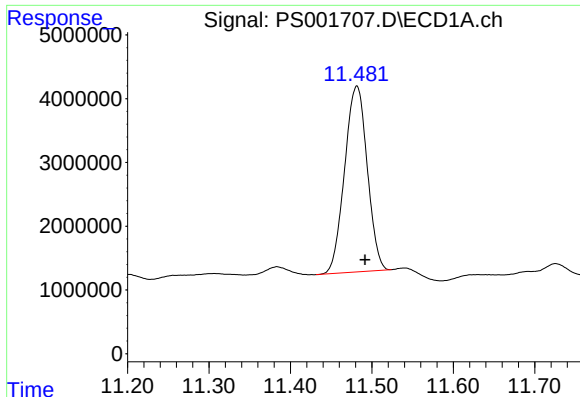

#4 2,4-DCAA


R.T.: 11.481 min
Delta R.T.: -0.010 min
Response: 56204195
Conc: 304.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

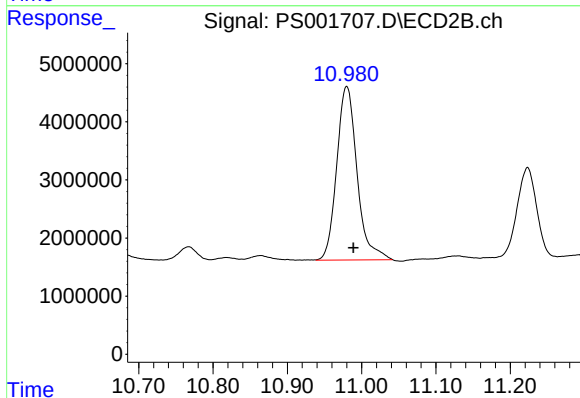


#4 2,4-DCAA

R.T.: 10.980 min
Delta R.T.: -0.009 min
Response: 56814190
Conc: 280.52 ng/ml

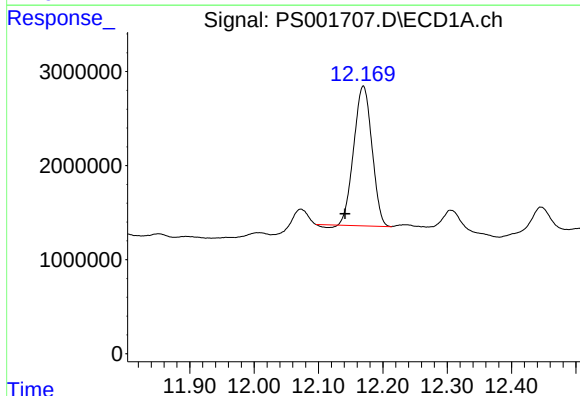


#6 MCP

R.T.: 12.170 min
Delta R.T.: 0.028 min
Response: 28908437
Conc: 57.45 ug/ml

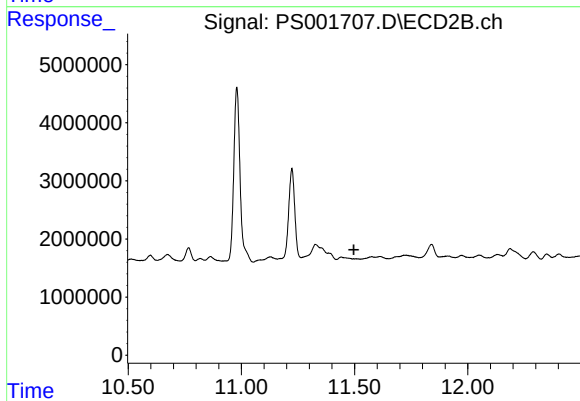

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

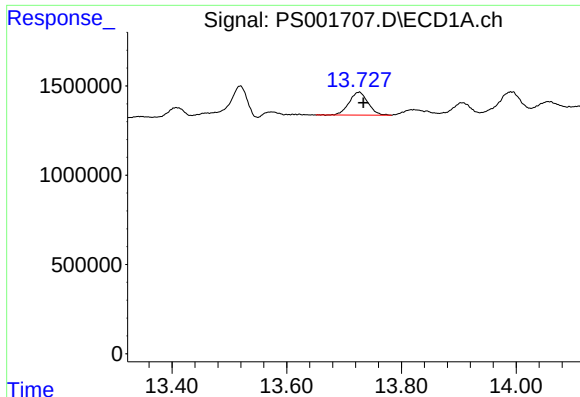

#10 Pentachlorophenol


R.T.: 13.726 min
Delta R.T.: -0.008 min
Response: 2927968
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

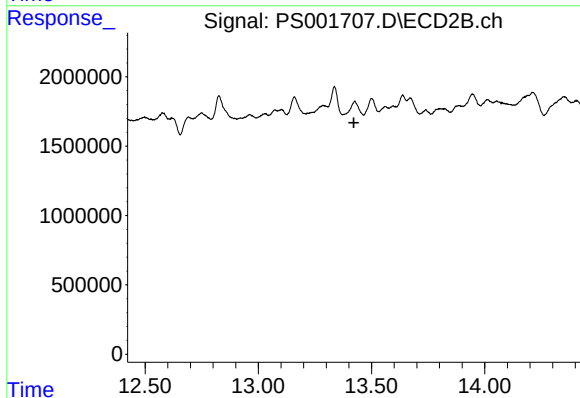


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.422 min
Response: 0
Conc: N.D.

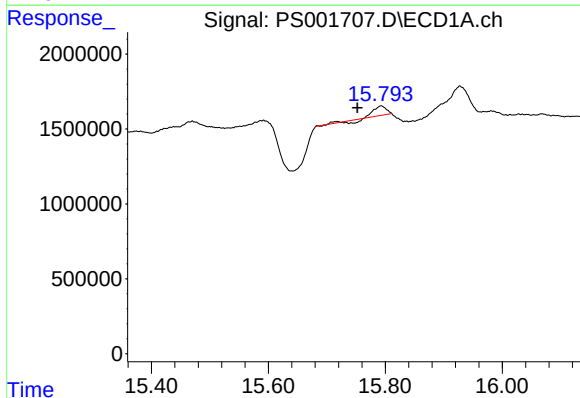


#13 2,4-DB

R.T.: 15.793 min
Delta R.T.: 0.041 min
Response: 809824
Conc: 6.03 ng/ml

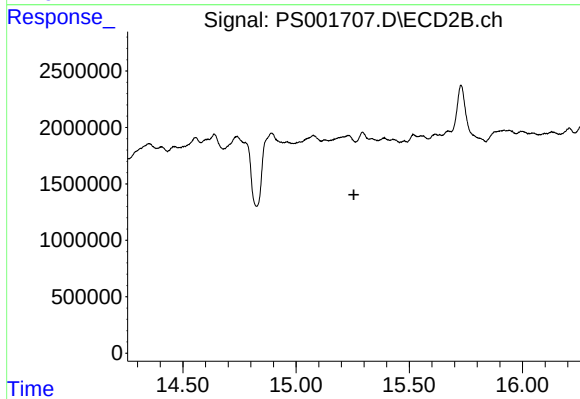

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.255 min
Response: 0
Conc: N.D.

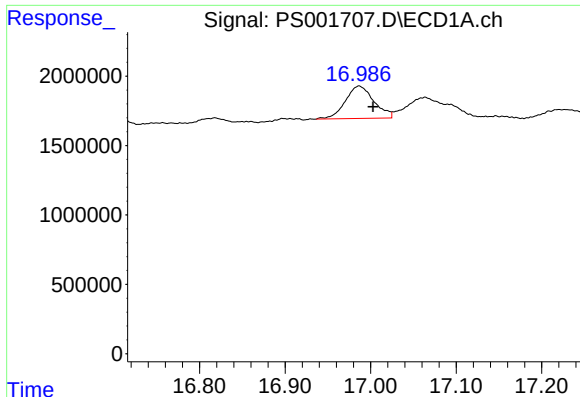

#15 Picloram


R.T.: 16.986 min
Delta R.T.: -0.017 min
Response: 5440425
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

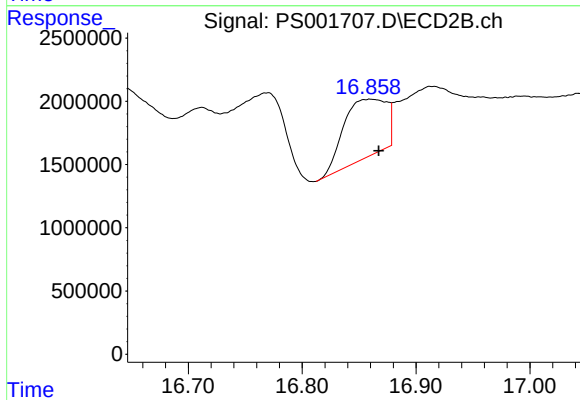


#15 Picloram

R.T.: 16.860 min
Delta R.T.: -0.007 min
Response: 12020441
Conc: 9.22 ng/ml

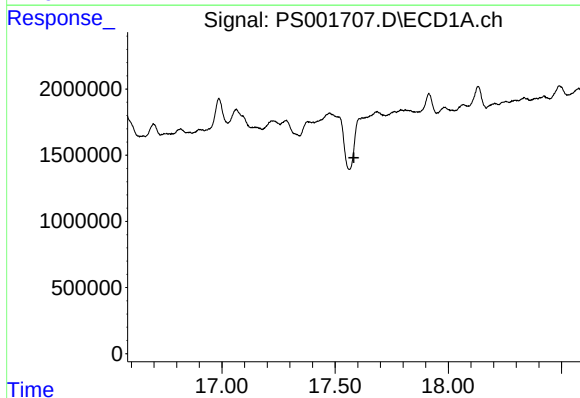

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

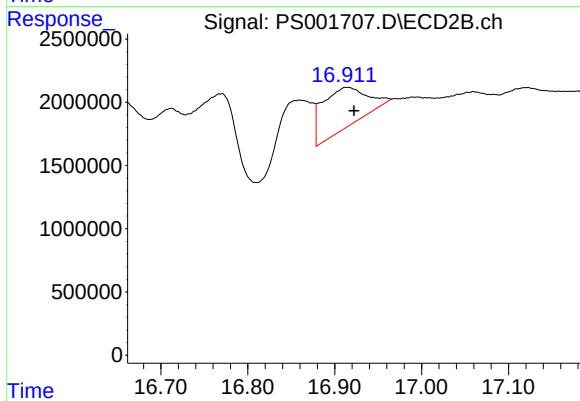

#16 DCPA

R.T.: 16.915 min
Delta R.T.: -0.008 min
Response: 11283183
Conc: 7.90 ng/ml