

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091120\
 Data File : PS012227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2020 17:26
 Operator : DD\AJ
 Sample : PB131536BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 18:56:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	548.6E6	317.2E6	502.918	593.083
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	54523616	N.D.	66.280
3) T	4-Nitroph...	7.114	6.554	10418412	28215936	17.687	77.387 #
5) T	DICAMBA	7.397	7.049	12225032	13059455	2.985	6.045 #
7) T	MCPA	7.763	7.375	41096710	36595111	9.035	13.355 #
8) T	DICHLORPROP	0.000	7.743	0	14137792	N.D.	25.039
9) T	2,4-D	8.394	7.952	121.8E6	27689349	107.877	37.690 #
10) T	Pentachlo...	8.639	8.432	8776930	9180318	<MDL	1.351 #
11) T	2,4,5-TP ...	0.000	8.766	0	20970859	N.D.	7.173
12) T	2,4,5-T	9.492	0.000	15678764	0	2.646	N.D. #
15) T	Picloram	11.046	11.027	54390890	64248429	6.959	14.175 #
16) T	DCPA	11.458	10.937	1691233	23071281	<MDL	6.275 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091120\
Data File : PS012227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2020 17:26
Operator : DD\AJ
Sample : PB131536BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 18:56:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

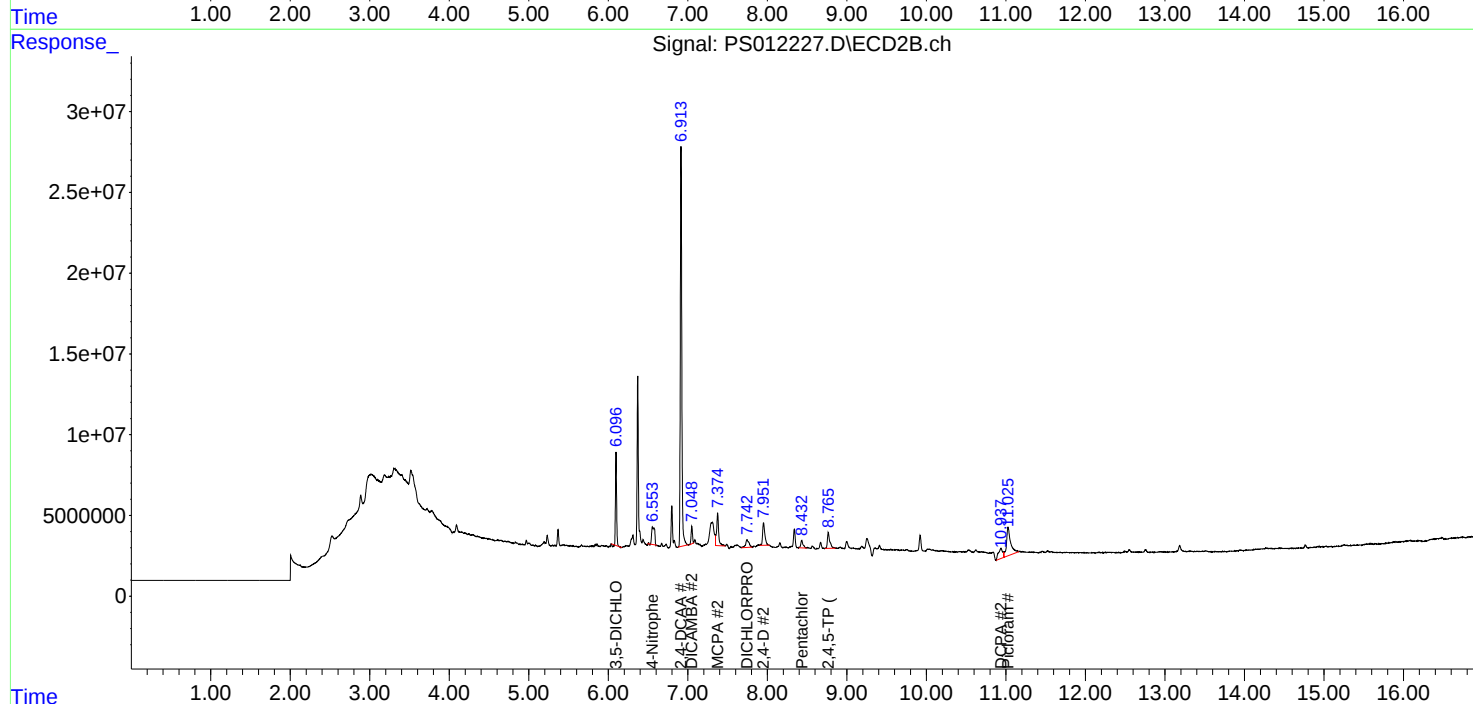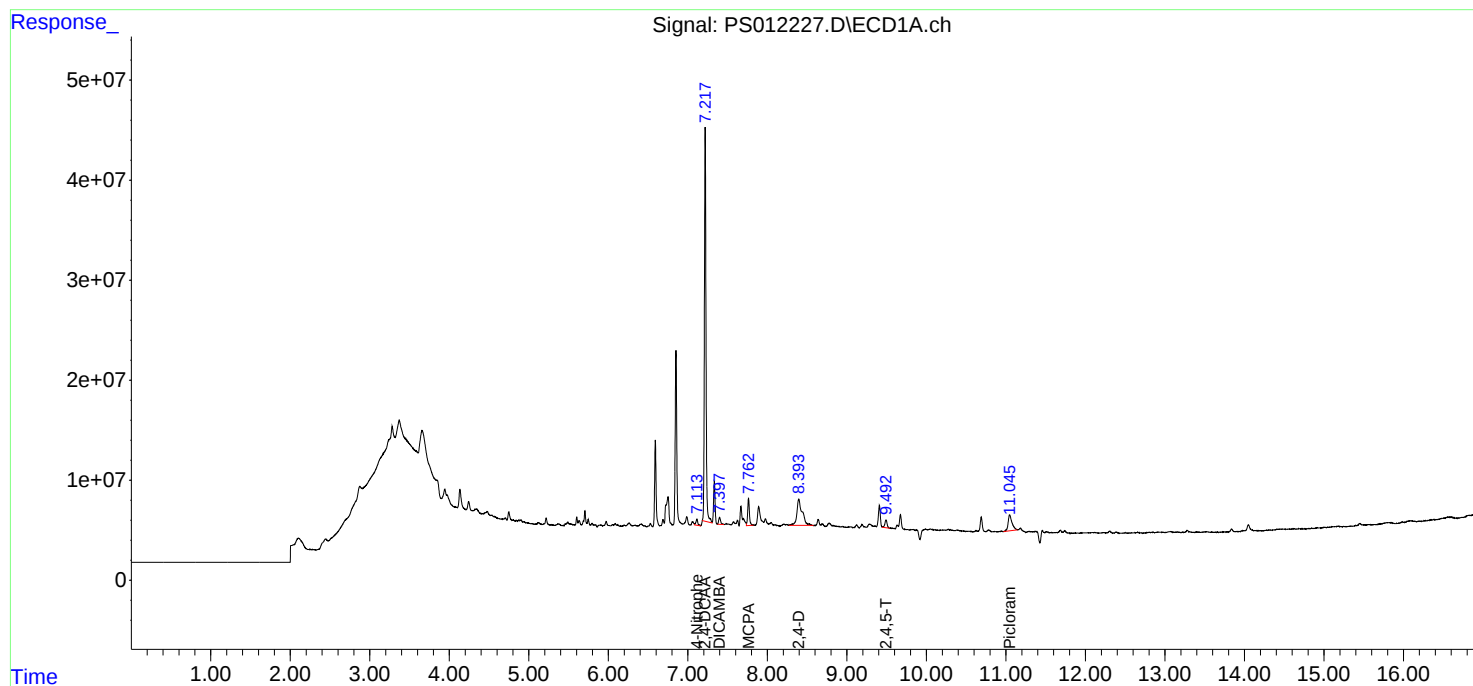


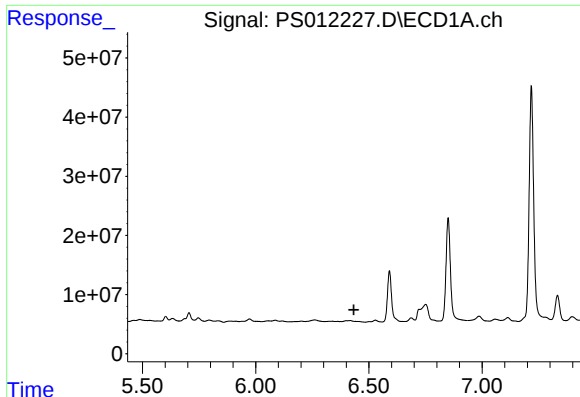

#2 3,5-DICHLORO BENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

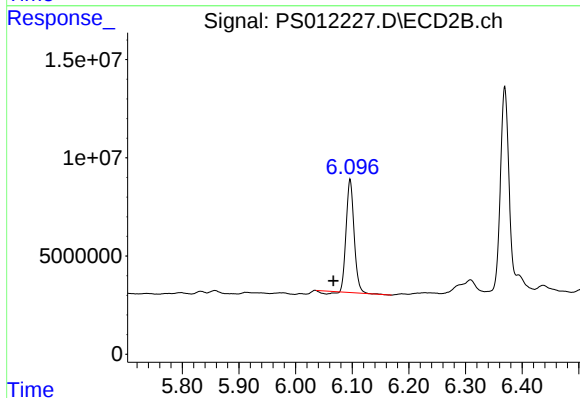


#2 3,5-DICHLORO BENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 54523616
Conc: 66.28 ng/ml

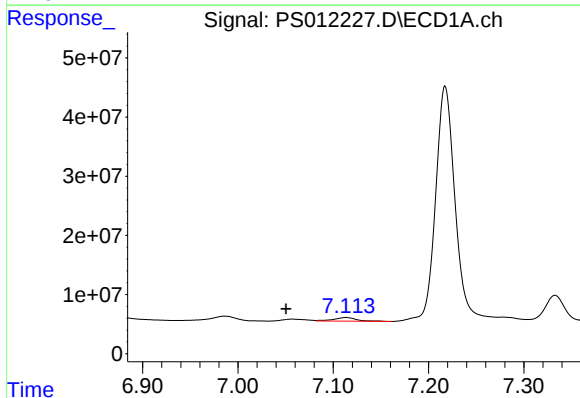


#3 4-Nitrophenol

R.T.: 7.114 min
Delta R.T.: 0.063 min
Response: 10418412
Conc: 17.69 ng/ml

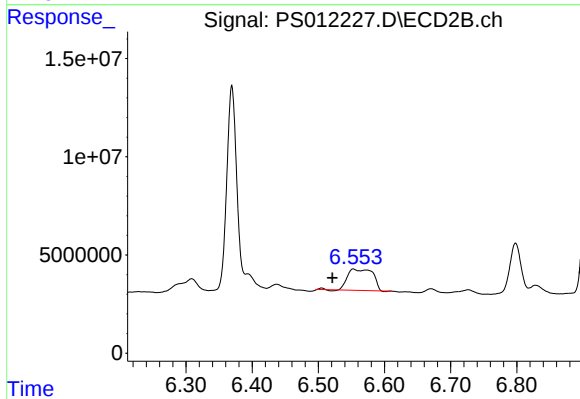

#3 4-Nitrophenol


R.T.: 6.554 min
Delta R.T.: 0.032 min
Response: 28215936
Conc: 77.39 ng/ml

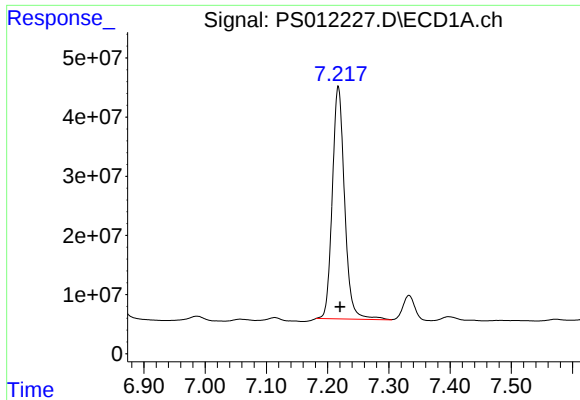

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.003 min
Response: 548567168
Conc: 502.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

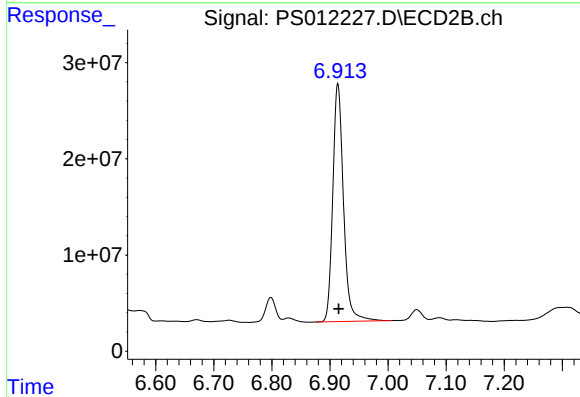


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 317172695
Conc: 593.08 ng/ml

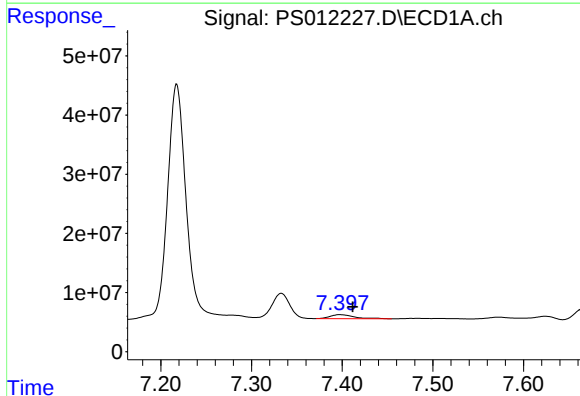


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.014 min
Response: 12225032
Conc: 2.98 ng/ml

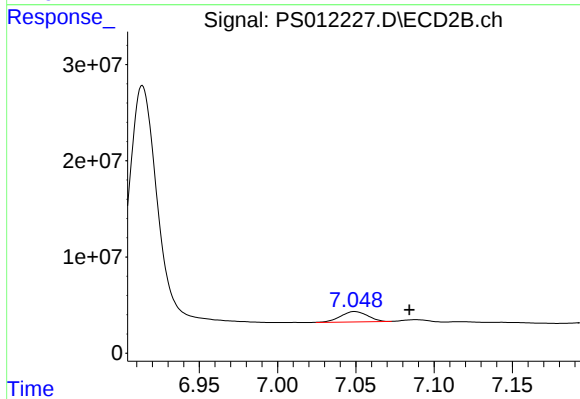

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 13059455
Conc: 6.04 ng/ml

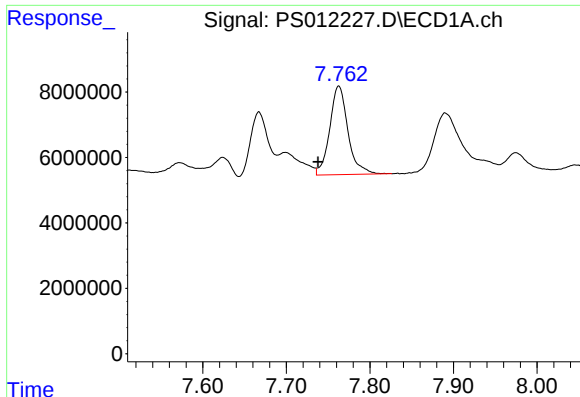

#7 MCPA


R.T.: 7.763 min
Delta R.T.: 0.025 min
Response: 41096710
Conc: 9.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

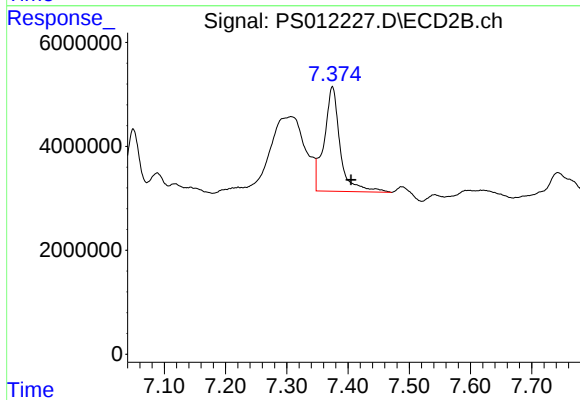


#7 MCPA

R.T.: 7.375 min
Delta R.T.: -0.030 min
Response: 36595111
Conc: 13.36 ug/ml

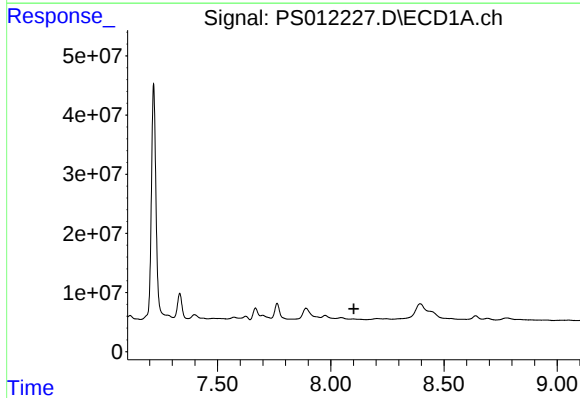


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

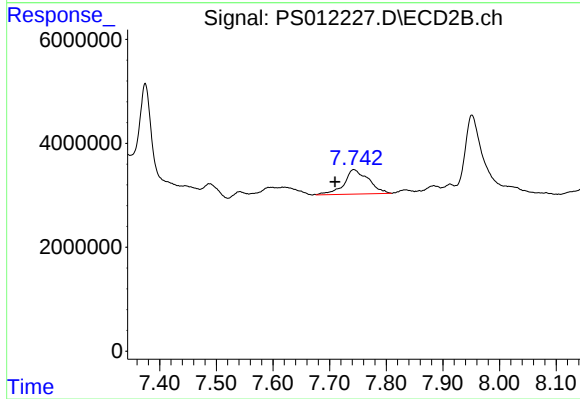

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.034 min
Response: 14137792
Conc: 25.04 ng/ml

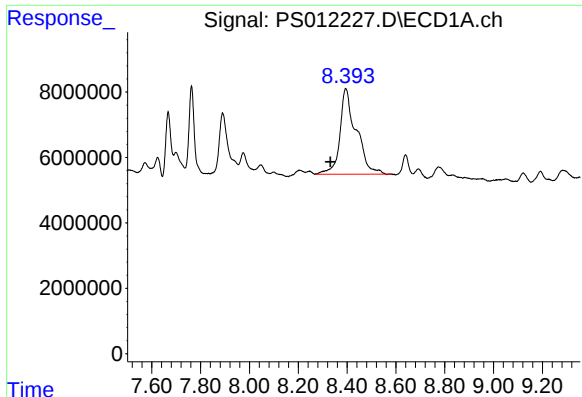

#9 2,4-D


R.T.: 8.394 min
Delta R.T.: 0.062 min
Response: 121803533
Conc: 107.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

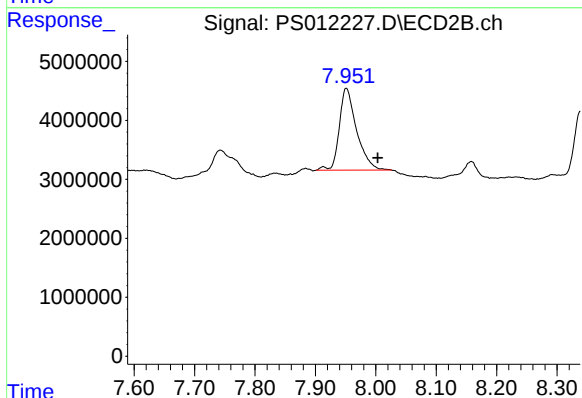


#9 2,4-D

R.T.: 7.952 min
Delta R.T.: -0.052 min
Response: 27689349
Conc: 37.69 ng/ml

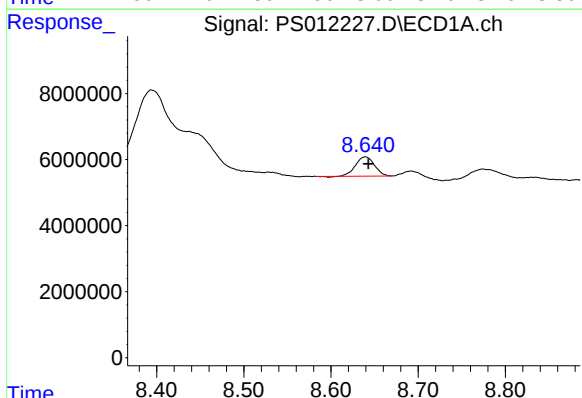


#10 Pentachlorophenol

R.T.: 8.639 min
Delta R.T.: -0.004 min
Response: 8776930
Conc: N.D.

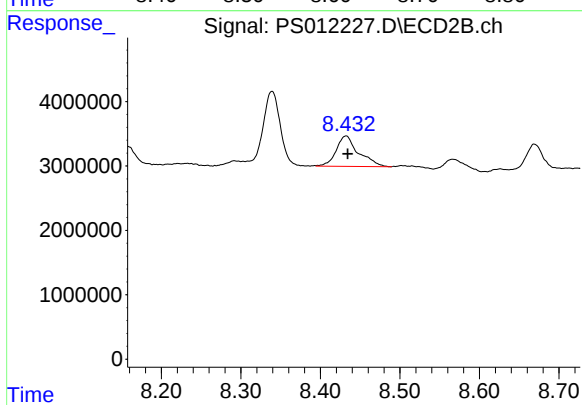

#10 Pentachlorophenol


R.T.: 8.432 min
Delta R.T.: -0.002 min
Response: 9180318
Conc: 1.35 ng/ml

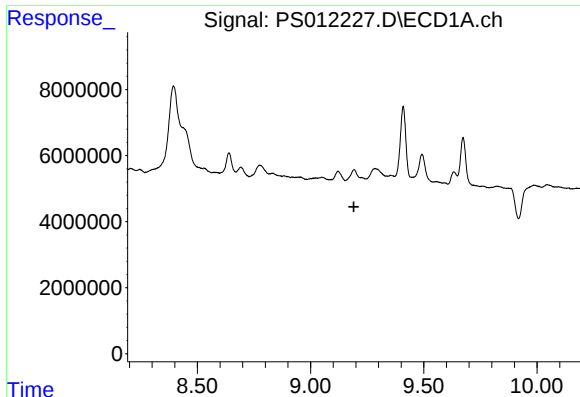

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

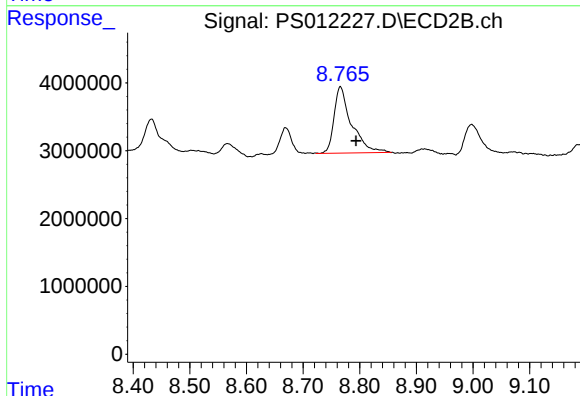


#11 2,4,5-TP (SILVEX)

R.T.: 8.766 min
Delta R.T.: -0.027 min
Response: 20970859
Conc: 7.17 ng/ml

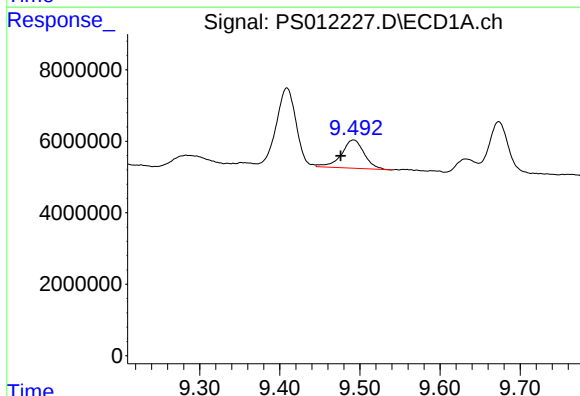


#12 2,4,5-T

R.T.: 9.492 min
Delta R.T.: 0.016 min
Response: 15678764
Conc: 2.65 ng/ml

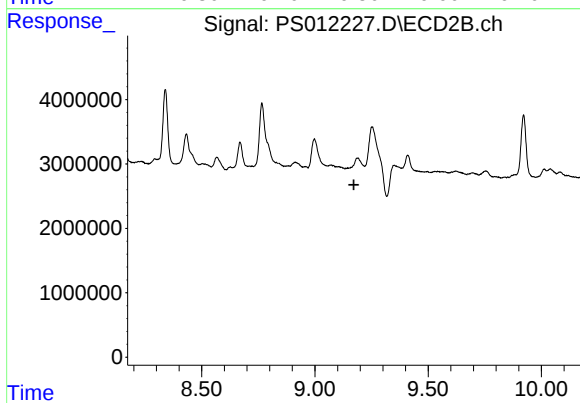

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

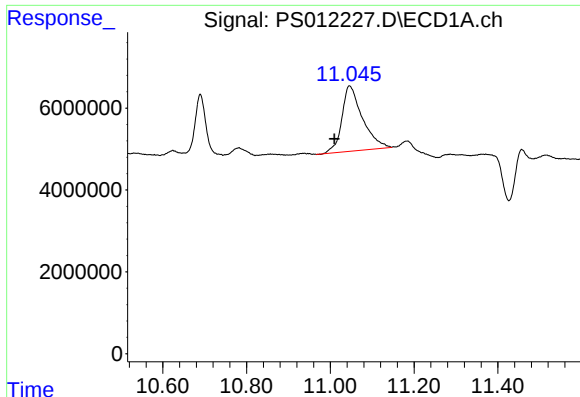

#15 Picloram


R.T.: 11.046 min
Delta R.T.: 0.036 min
Response: 54390890
Conc: 6.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

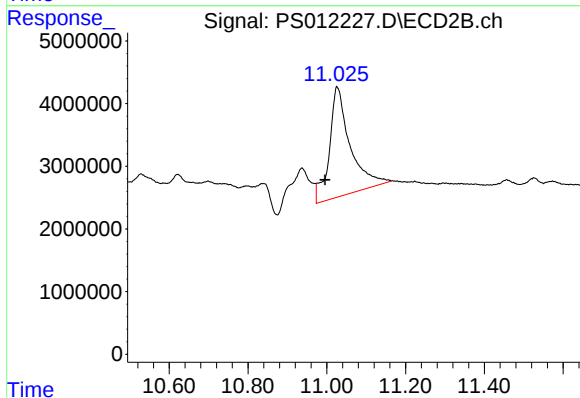


#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.031 min
Response: 64248429
Conc: 14.18 ng/ml

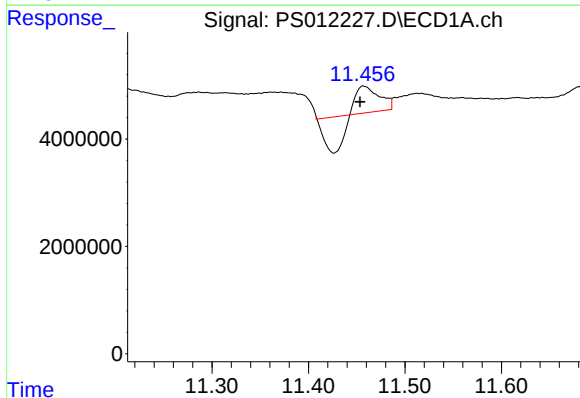

#16 DCPA

R.T.: 11.458 min
Delta R.T.: 0.004 min
Response: 1691233
Conc: N.D.

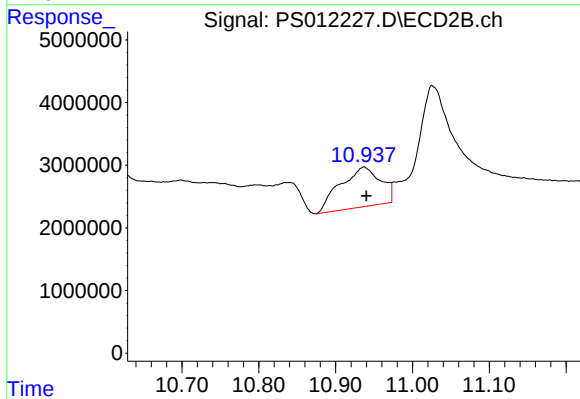

#16 DCPA

R.T.: 10.937 min
Delta R.T.: -0.003 min
Response: 23071281
Conc: 6.27 ng/ml