

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091125\
 Data File : PS031709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2025 19:43
 Operator : AR\AJ
 Sample : Q3032-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 02:37:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.744	1538.0E6	455.1E6	427.054	500.692
Target Compounds							
1) T	Dalapon	2.641f	2.678	1230.3E6	1660.1E6	212.829	589.173 #
2) T	3,5-DICHL...	6.446	6.733f	5836934	11960476	1.094	7.843 #
3) T	4-Nitroph...	7.065	0.000	2127786	0	1.929	N.D. #
6) T	MCP	7.630	8.007f	3837736	5776303	<MDL	3.067 #
8) T	DICHLORPROP	8.173	0.000	10515020	0	2.952	N.D. #
10) T	Pentachlo...	8.714	9.511	6844458	12572436	<MDL	<MDL #
11) T	2,4,5-TP ...	9.244f	9.885	333936	149.4E6	<MDL	9.927 #
12) T	2,4,5-T	0.000	10.344	0	38178932	N.D.	2.837
13) T	2,4-DB	10.191f	10.854f	123.8E6	46264044	53.074	43.236
14) T	DINOSEB	11.329f	11.291f	116.5E6	21830949	8.078	2.246 #
15) T	Picloram	11.164	0.000	54071831	0	3.002	N.D. #
16) T	DCPA	11.631	12.301	18066661	255.6E6	<MDL	10.606 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091125\
Data File : PS031709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2025 19:43
Operator : AR\AJ
Sample : Q3032-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 02:37:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

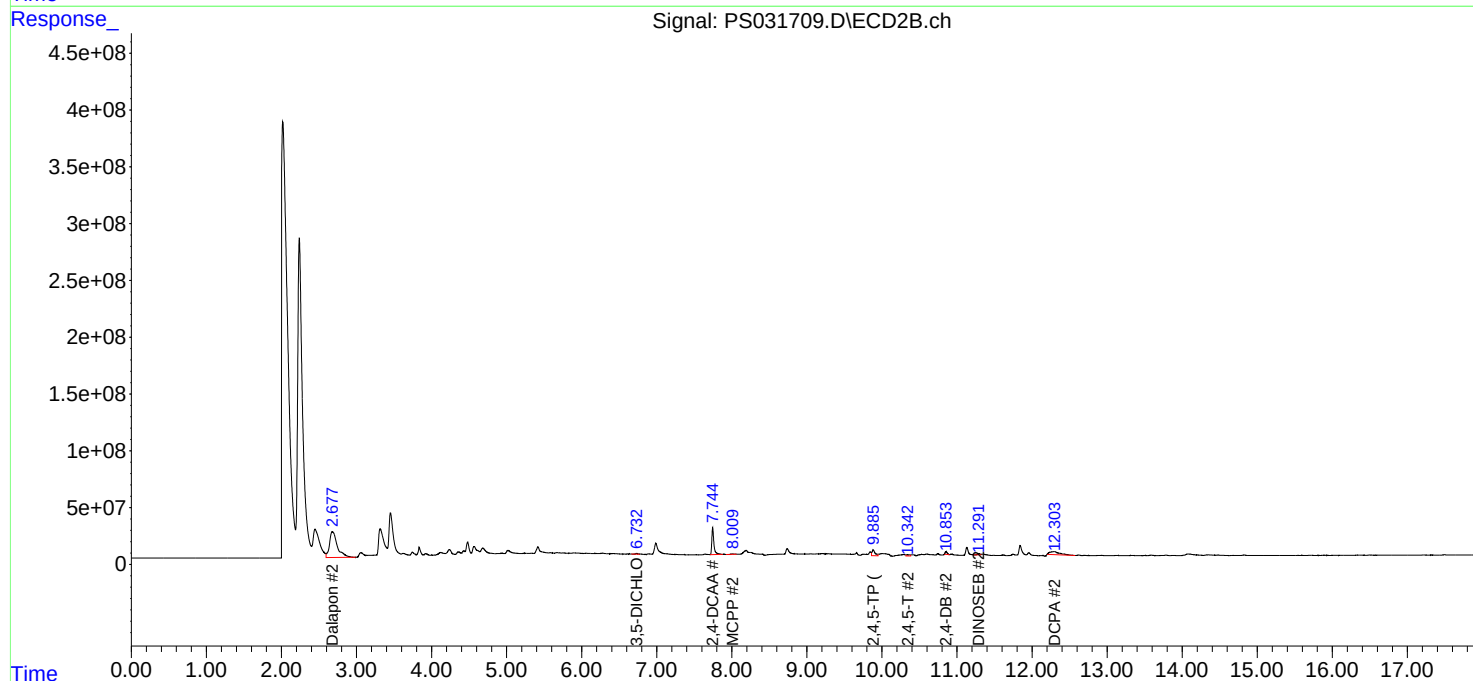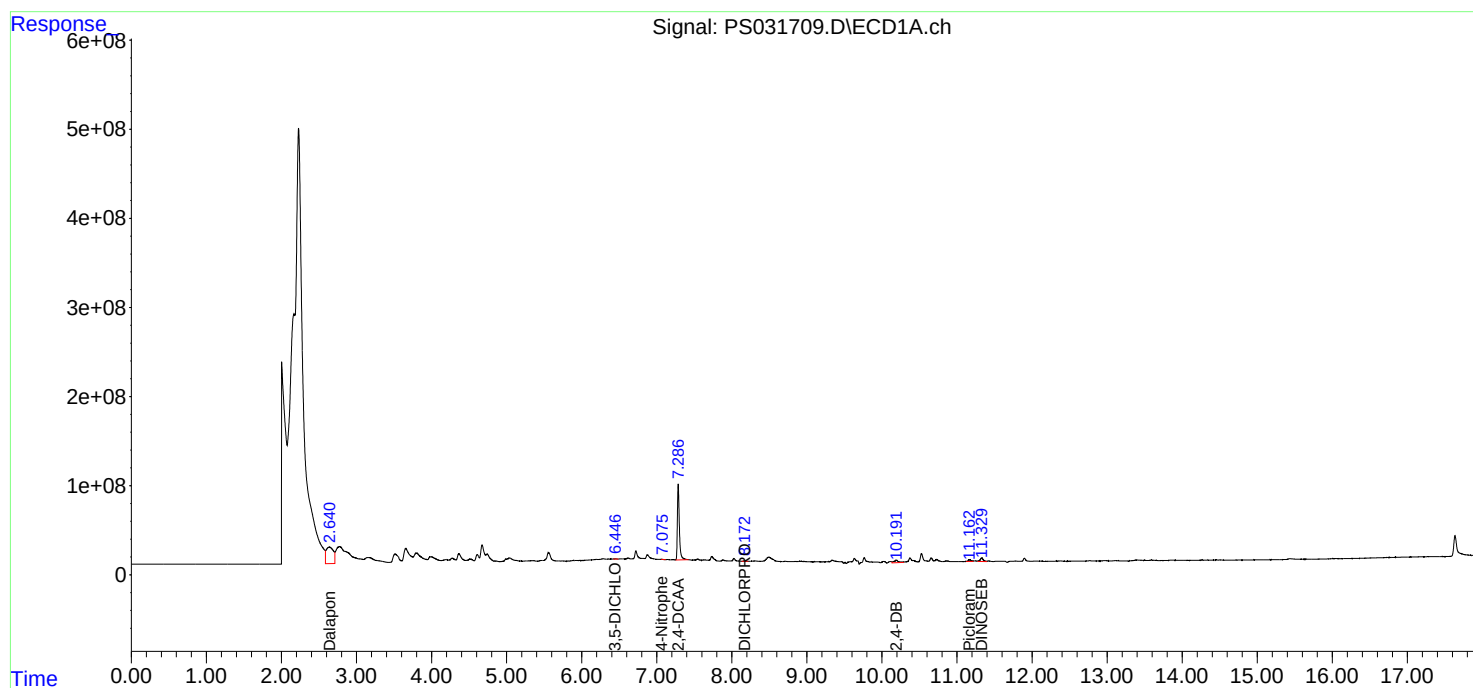


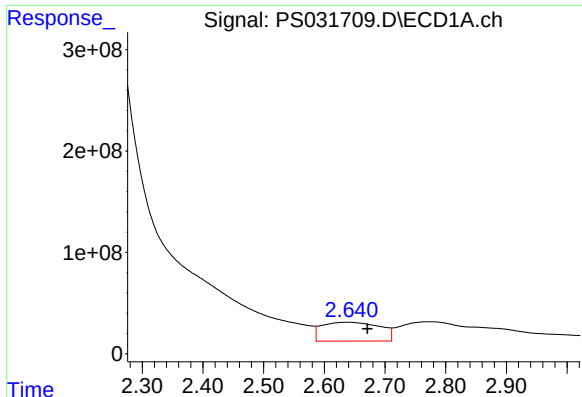

#1 Dalapon


R.T.: 2.641 min
Delta R.T.: -0.030 min
Response: 1230309862
Conc: 212.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

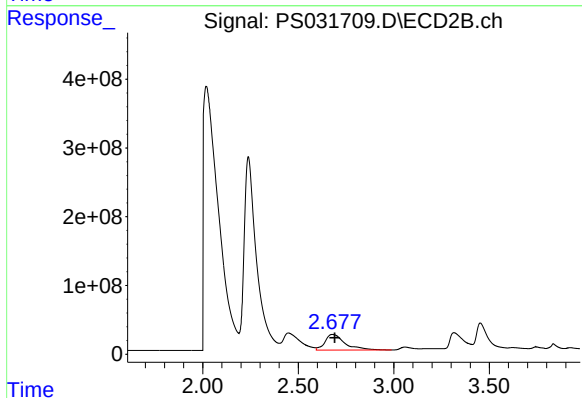


#1 Dalapon

R.T.: 2.678 min
Delta R.T.: -0.014 min
Response: 1660070096
Conc: 589.17 ng/ml

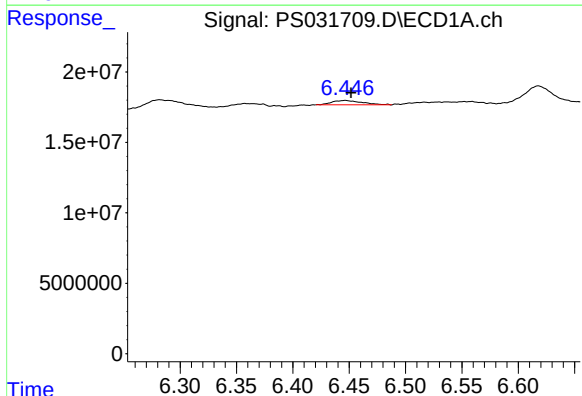


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.446 min
Delta R.T.: -0.005 min
Response: 5836934
Conc: 1.09 ng/ml

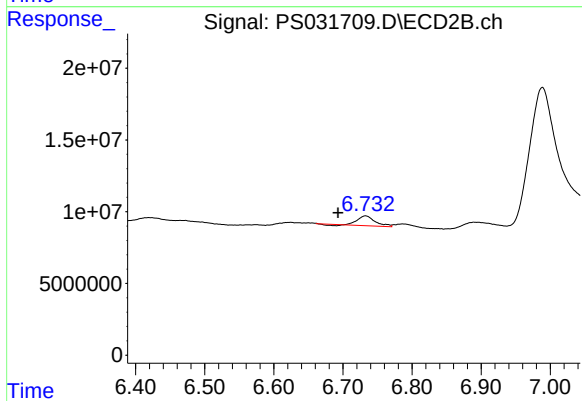

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.733 min
Delta R.T.: 0.040 min
Response: 11960476
Conc: 7.84 ng/ml

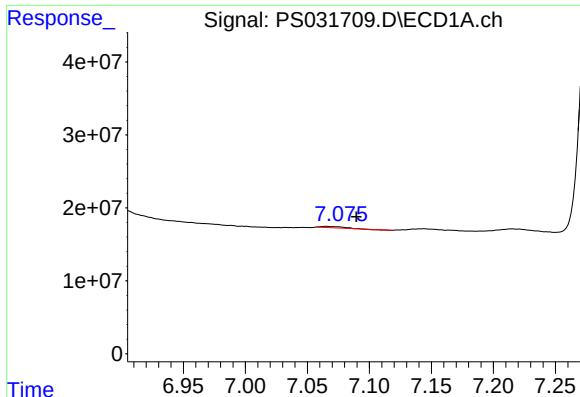

#3 4-Nitrophenol


R.T.: 7.065 min
Delta R.T.: -0.024 min
Response: 2127786
Conc: 1.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

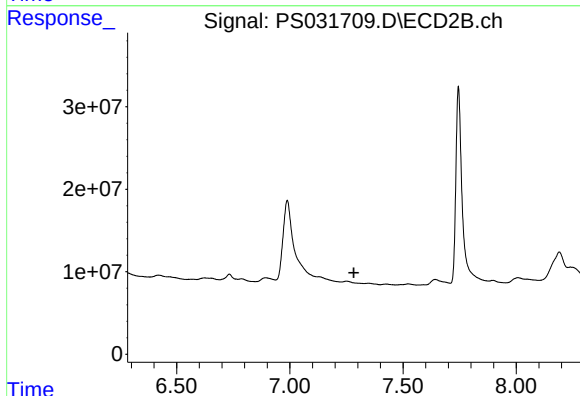


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

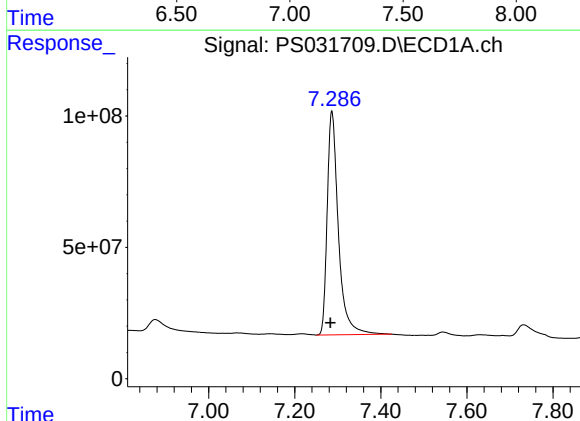


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.003 min
Response: 1538047256
Conc: 427.05 ng/ml

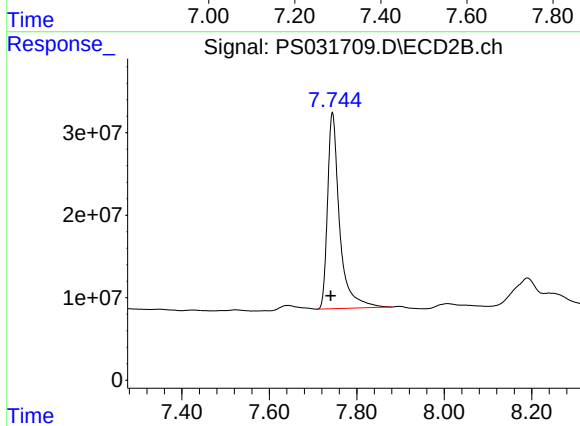

#4 2,4-DCAA


R.T.: 7.744 min
Delta R.T.: 0.004 min
Response: 455078339
Conc: 500.69 ng/ml

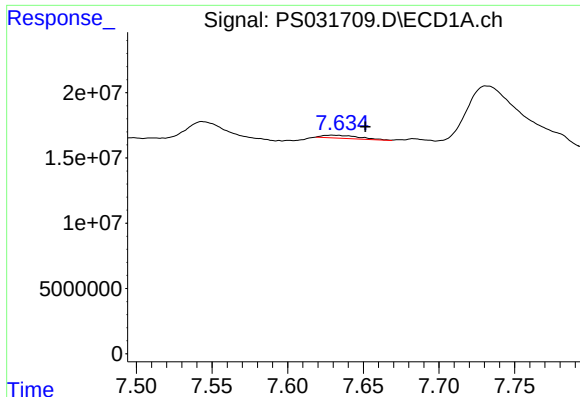

#6 MCP


R.T.: 7.630 min
Delta R.T.: -0.022 min
Response: 3837736
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

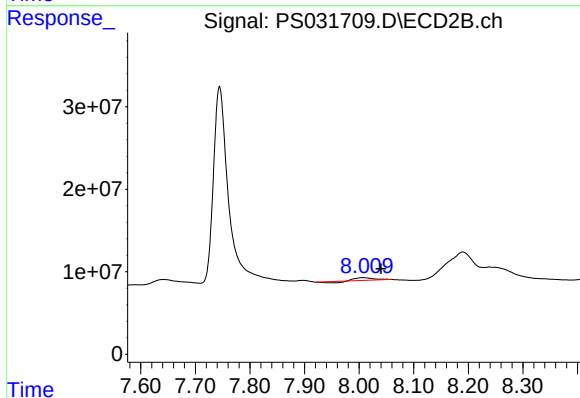


#6 MCP

R.T.: 8.007 min
Delta R.T.: -0.033 min
Response: 5776303
Conc: 3.07 ug/ml

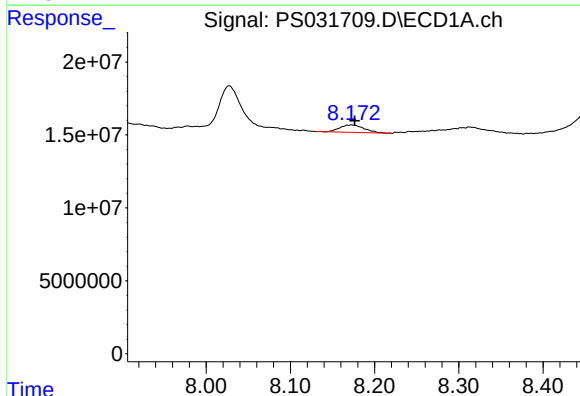


#8 DICHLORPROP

R.T.: 8.173 min
Delta R.T.: -0.004 min
Response: 10515020
Conc: 2.95 ng/ml

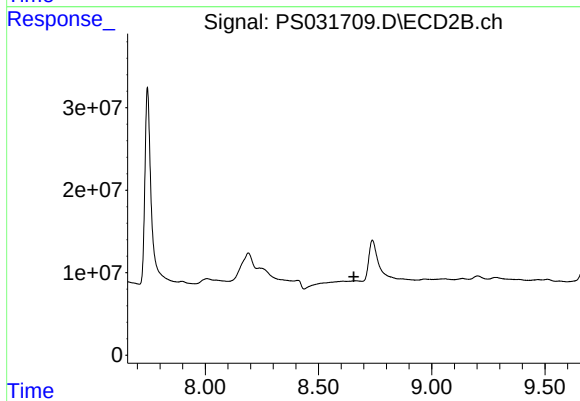

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.657 min
Response: 0
Conc: N.D.

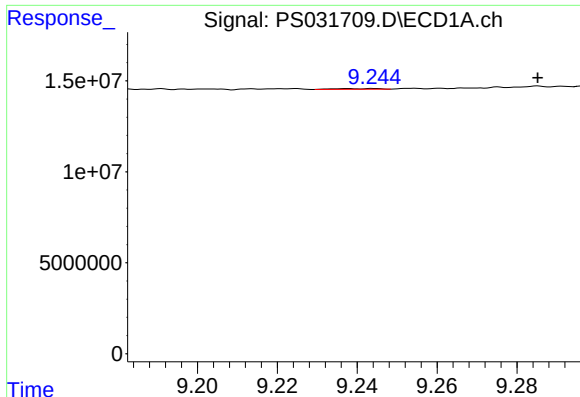

#11 2,4,5-TP (SILVEX)


R.T.: 9.244 min
Delta R.T.: -0.041 min
Response: 333936
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

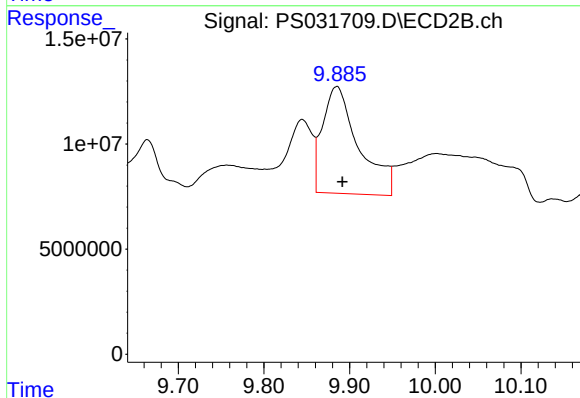


#11 2,4,5-TP (SILVEX)

R.T.: 9.885 min
Delta R.T.: -0.007 min
Response: 149449667
Conc: 9.93 ng/ml

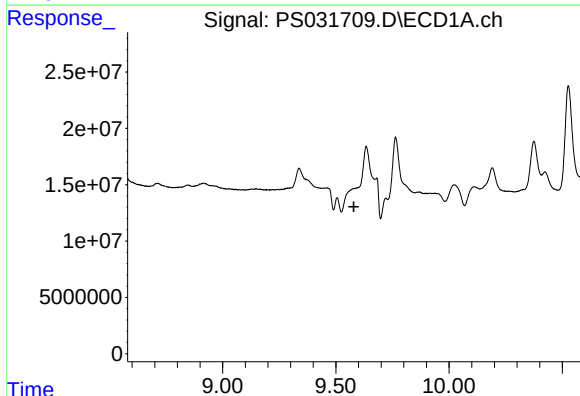


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.580 min
Response: 0
Conc: N.D.

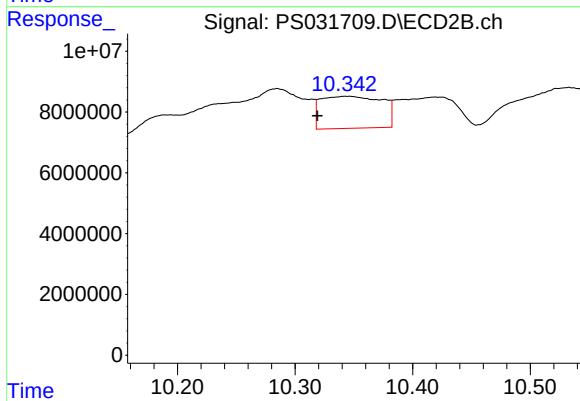

#12 2,4,5-T


R.T.: 10.344 min
Delta R.T.: 0.025 min
Response: 38178932
Conc: 2.84 ng/ml

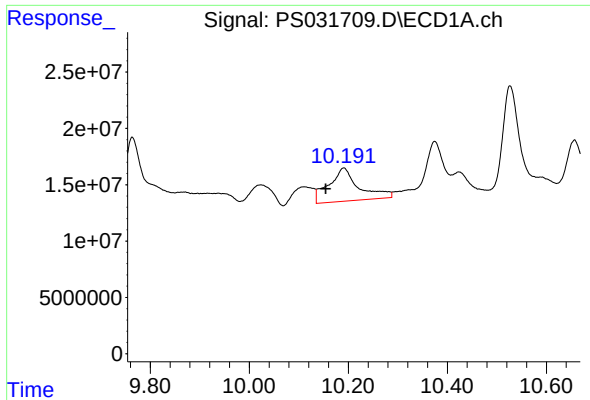

#13 2,4-DB


R.T.: 10.191 min
Delta R.T.: 0.037 min
Response: 123808075
Conc: 53.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

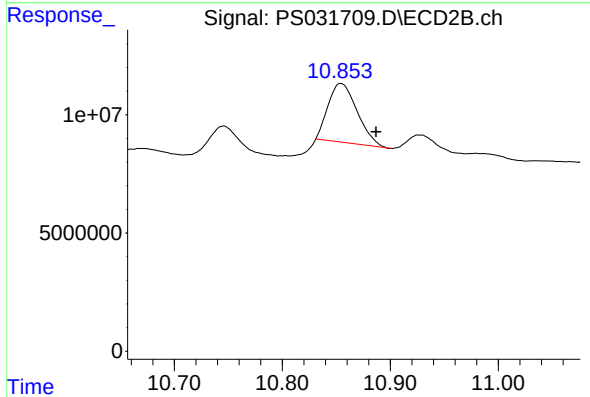


#13 2,4-DB

R.T.: 10.854 min
Delta R.T.: -0.032 min
Response: 46264044
Conc: 43.24 ng/ml

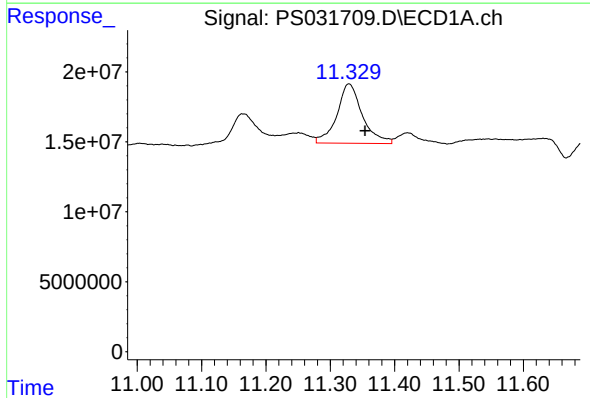


#14 DINOSEB

R.T.: 11.329 min
Delta R.T.: -0.025 min
Response: 116504769
Conc: 8.08 ng/ml

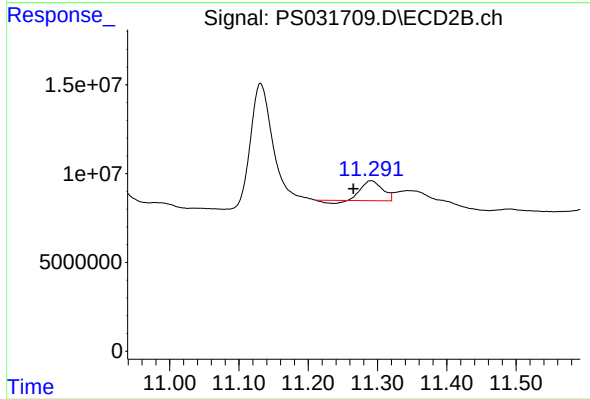

#14 DINOSEB


R.T.: 11.291 min
Delta R.T.: 0.025 min
Response: 21830949
Conc: 2.25 ng/ml

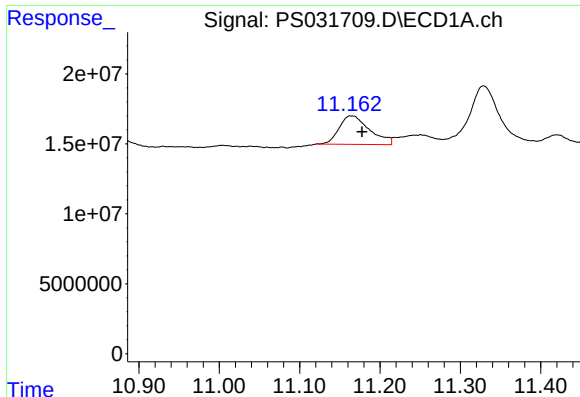

#15 Picloram


R.T.: 11.164 min
Delta R.T.: -0.014 min
Response: 54071831
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

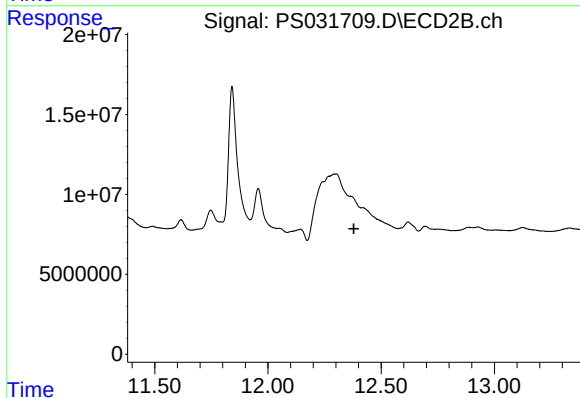


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.380 min
Response: 0
Conc: N.D.

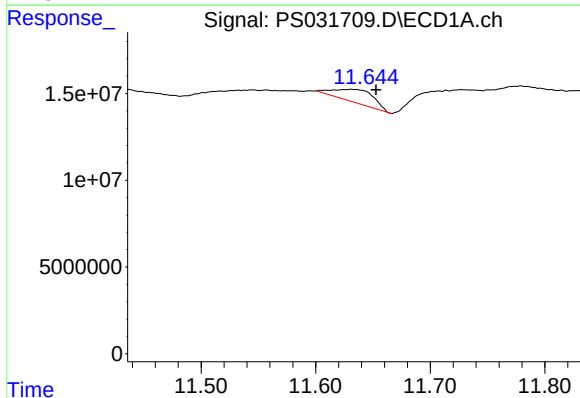

#16 DCPA

R.T.: 11.631 min
Delta R.T.: -0.022 min
Response: 18066661
Conc: N.D.

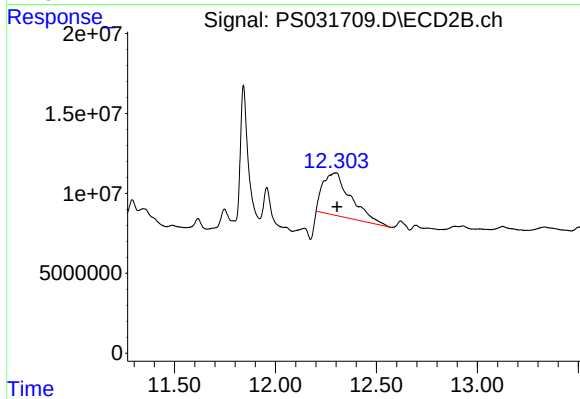

#16 DCPA

R.T.: 12.301 min
Delta R.T.: -0.005 min
Response: 255642717
Conc: 10.61 ng/ml