

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
 Data File : PS001713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2018 15:55
 Operator : EI\SJ
 Sample : J4838-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:15:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.491	10.986	11153041	10951459	60.417	54.073
Target Compounds							
3) T	4-Nitroph...	11.082	0.000	2511423	0	20.370	N.D. #
5) T	DICAMBA	0.000	11.231	0	1398470	N.D.	1.994 #
6) T	MCP	12.179	0.000	23306889	0	46.321	N.D. #
7) T	MCPA	12.458	11.926	3352892	11149053	4.016	15.297 #
9) T	2,4-D	0.000	12.836	0	3737850	N.D.	15.089 #
10) T	Pentachlo...	13.730	13.429	9831813	3364859	3.943	1.244 #
11) T	2,4,5-TP ...	0.000	14.062	0	1517408	N.D.	1.428 #
12) T	2,4,5-T	0.000	14.610	0	2632912	N.D.	3.048 #
13) T	2,4-DB	15.757	15.234	44988556	4027005	334.927	30.367 #
15) T	Picloram	17.002	16.868	5932999	13659369	4.236	10.475 #
16) T	DCPA	17.627	16.922	19369418	17230097	17.071	12.068 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
Data File : PS001713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2018 15:55
Operator : EI\SJ
Sample : J4838-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:15:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

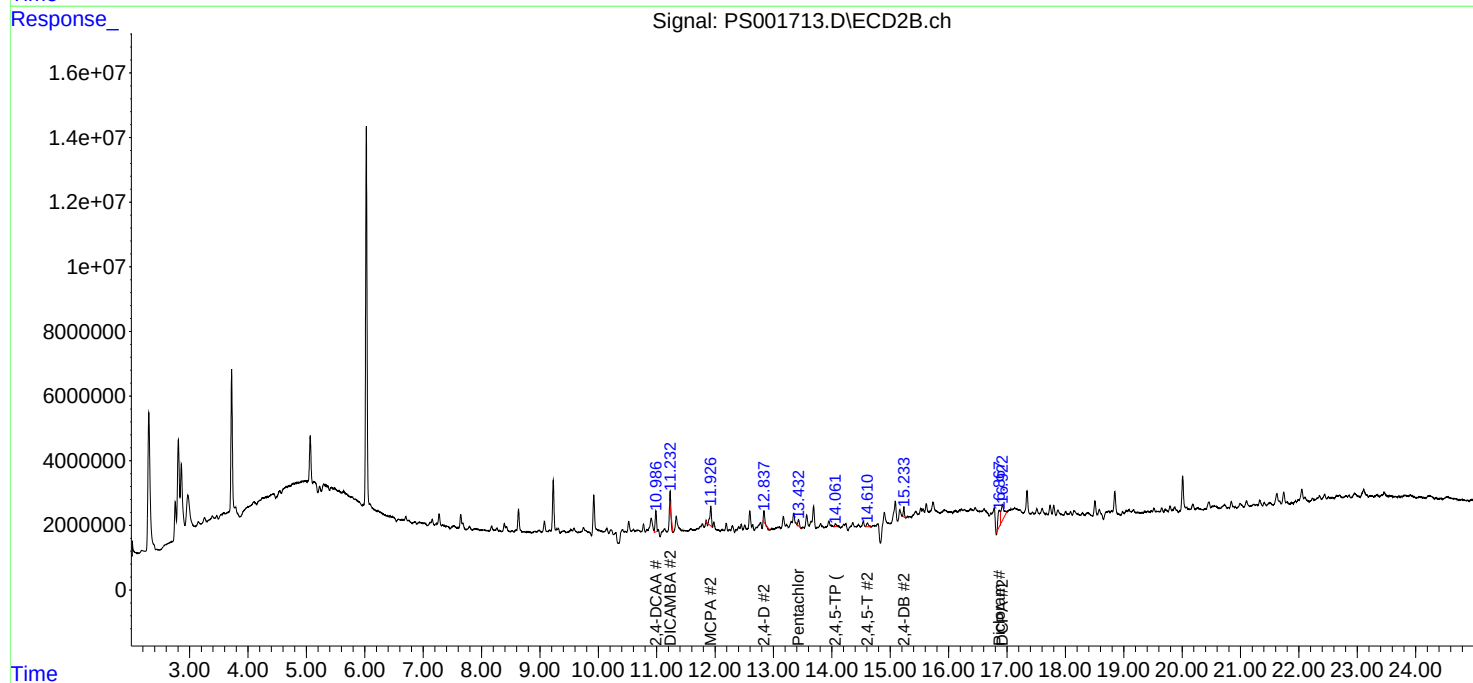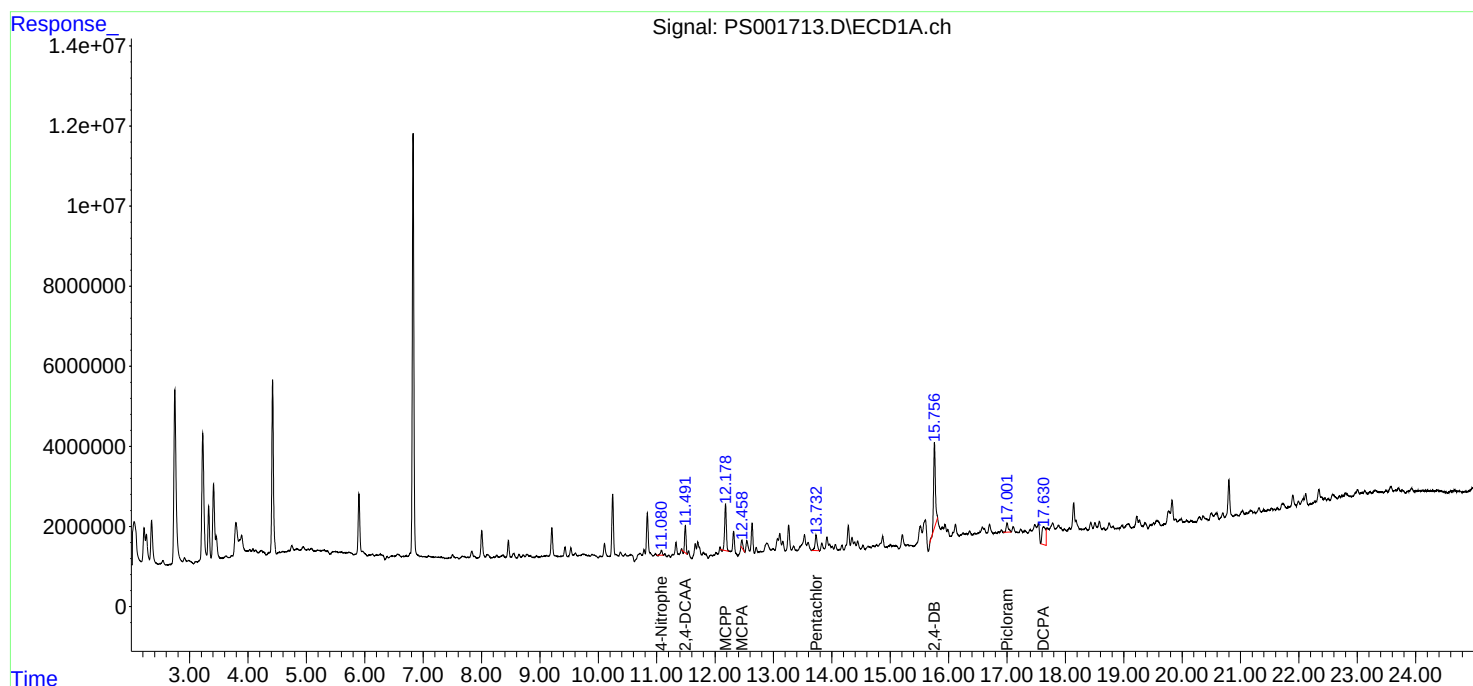


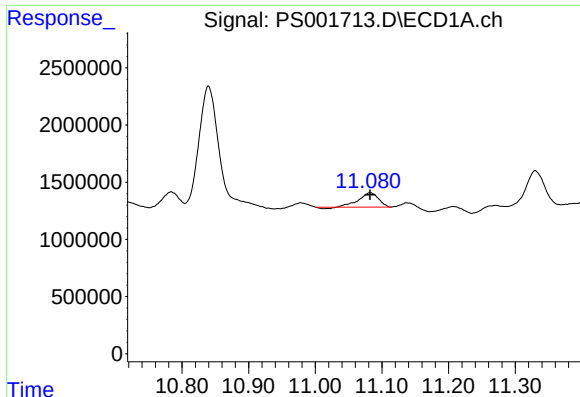

#3 4-Nitrophenol


R.T.: 11.082 min
Delta R.T.: 0.000 min
Response: 2511423
Conc: 20.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

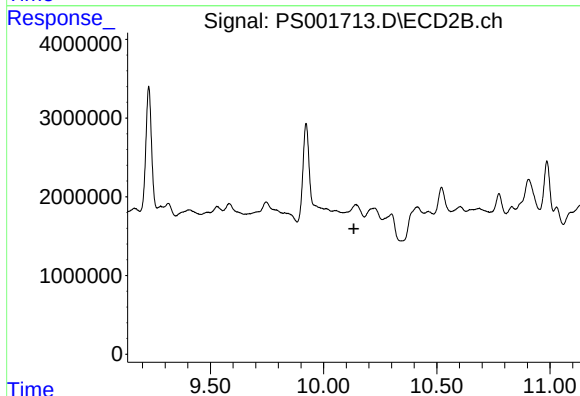


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.134 min
Response: 0
Conc: N.D.

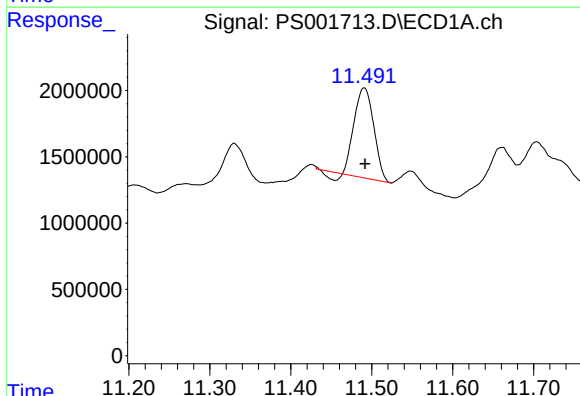


#4 2,4-DCAA

R.T.: 11.491 min
Delta R.T.: -0.001 min
Response: 11153041
Conc: 60.42 ng/ml

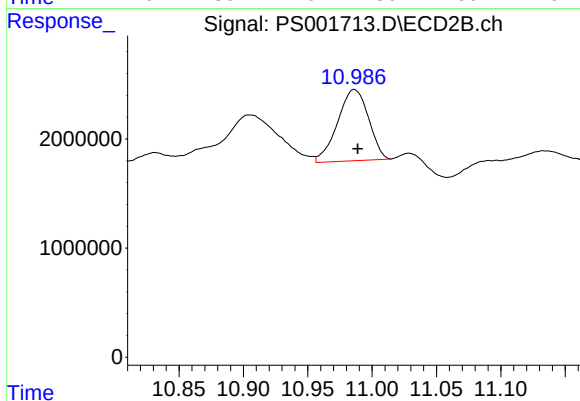

#4 2,4-DCAA


R.T.: 10.986 min
Delta R.T.: -0.003 min
Response: 10951459
Conc: 54.07 ng/ml

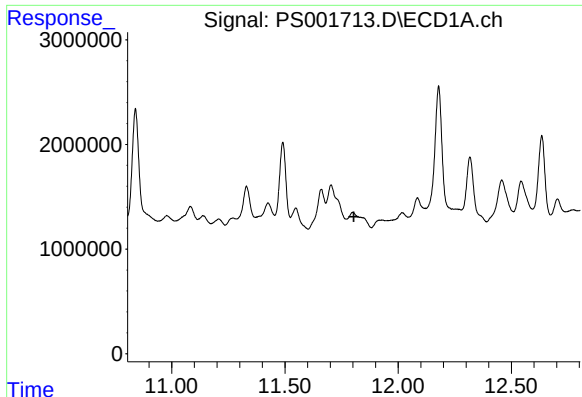

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

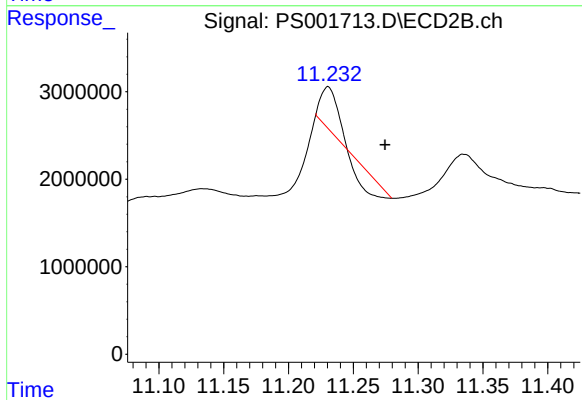


#5 DICAMBA

R.T.: 11.231 min
Delta R.T.: -0.044 min
Response: 1398470
Conc: 1.99 ng/ml

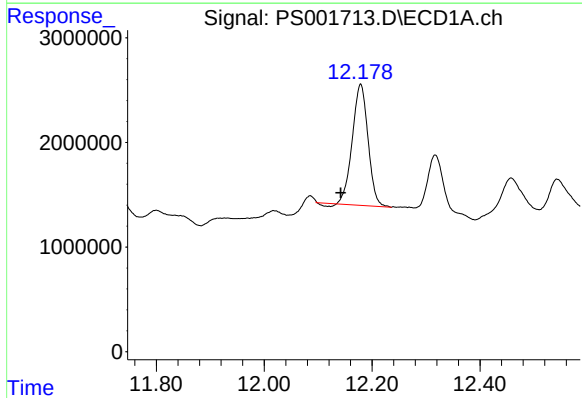


#6 MCP

R.T.: 12.179 min
Delta R.T.: 0.037 min
Response: 23306889
Conc: 46.32 ug/ml

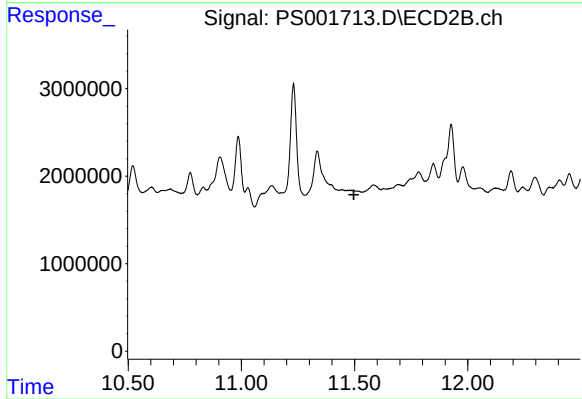

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

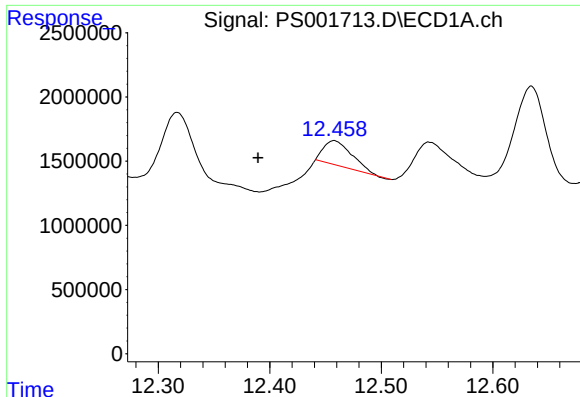

#7 MCPA


R.T.: 12.458 min
Delta R.T.: 0.068 min
Response: 3352892
Conc: 4.02 ug/ml

Instrument :
ECD_S
ClientSampleId :

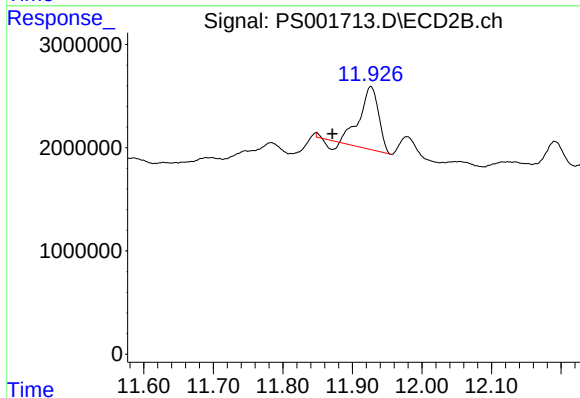


#7 MCPA

R.T.: 11.926 min
Delta R.T.: 0.055 min
Response: 11149053
Conc: 15.30 ug/ml

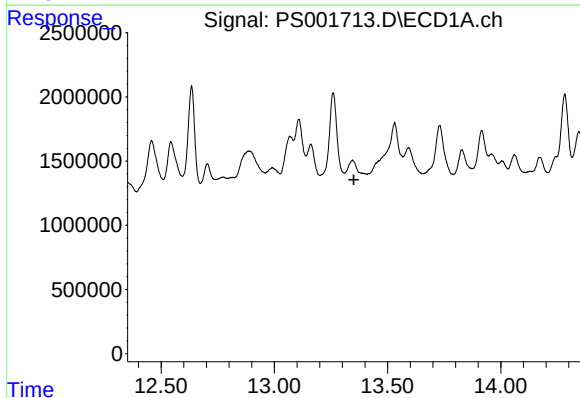


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.352 min
Response: 0
Conc: N.D.

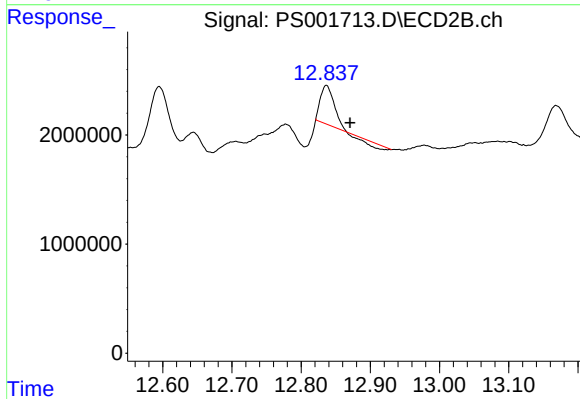

#9 2,4-D


R.T.: 12.836 min
Delta R.T.: -0.034 min
Response: 3737850
Conc: 15.09 ng/ml

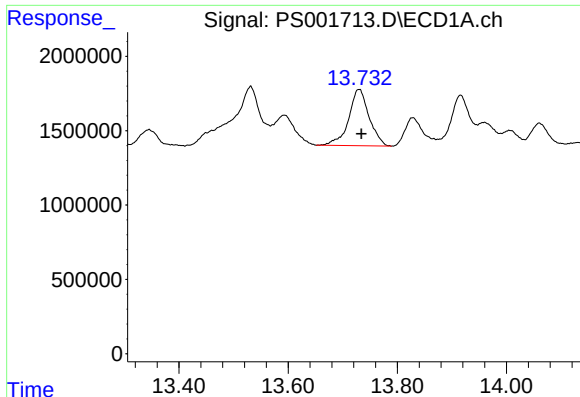

#10 Pentachlorophenol


R.T.: 13.730 min
Delta R.T.: -0.004 min
Response: 9831813
Conc: 3.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

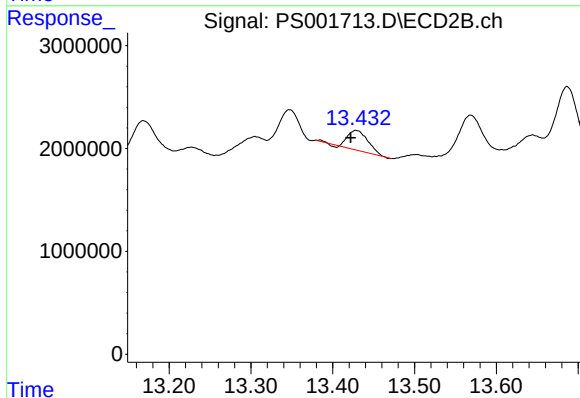


#10 Pentachlorophenol

R.T.: 13.429 min
Delta R.T.: 0.007 min
Response: 3364859
Conc: 1.24 ng/ml

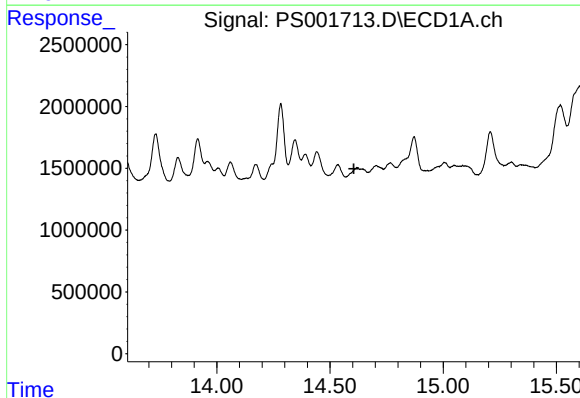


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.606 min
Response: 0
Conc: N.D.

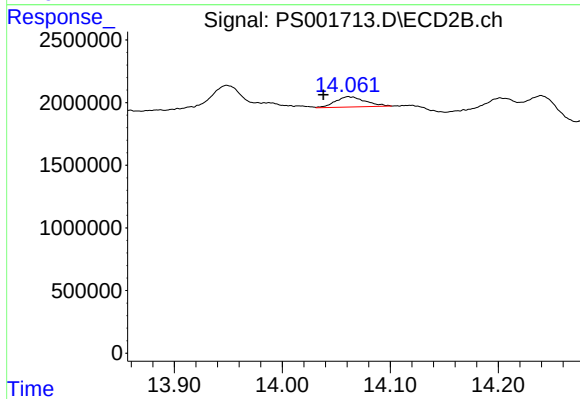

#11 2,4,5-TP (SILVEX)


R.T.: 14.062 min
Delta R.T.: 0.024 min
Response: 1517408
Conc: 1.43 ng/ml

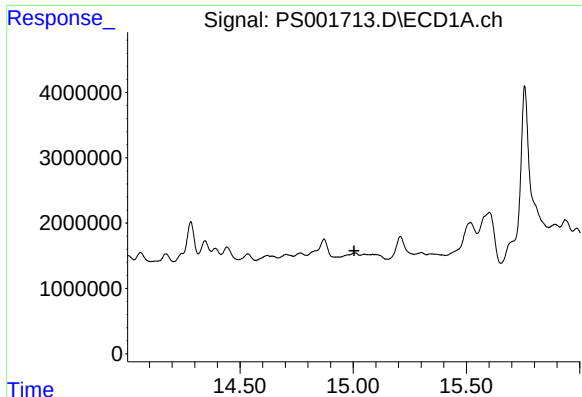

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

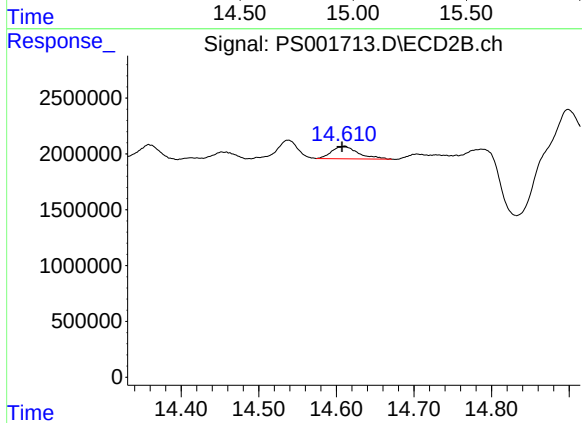


#12 2,4,5-T

R.T.: 14.610 min
Delta R.T.: 0.003 min
Response: 2632912
Conc: 3.05 ng/ml

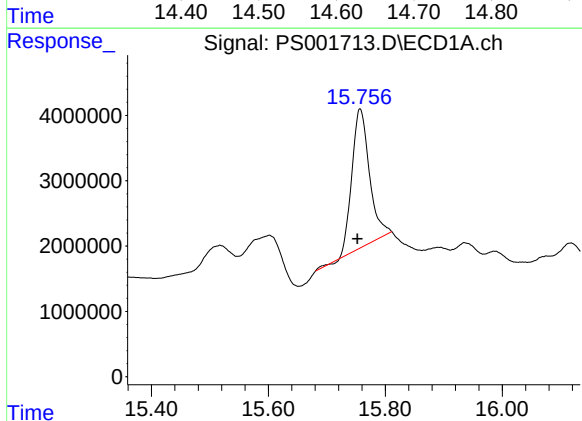


#13 2,4-DB

R.T.: 15.757 min
Delta R.T.: 0.005 min
Response: 44988556
Conc: 334.93 ng/ml

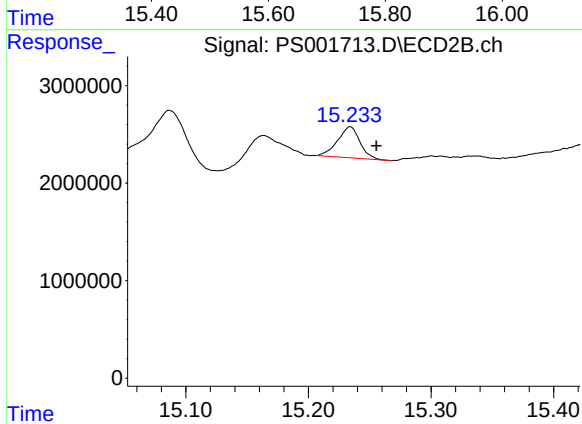

#13 2,4-DB


R.T.: 15.234 min
Delta R.T.: -0.021 min
Response: 4027005
Conc: 30.37 ng/ml

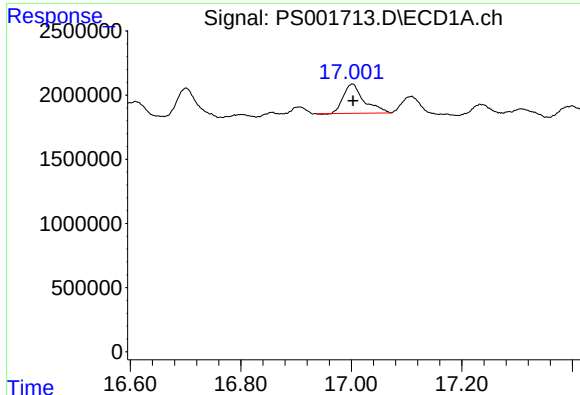

#15 Picloram


R.T.: 17.002 min
Delta R.T.: -0.001 min
Response: 5932999
Conc: 4.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

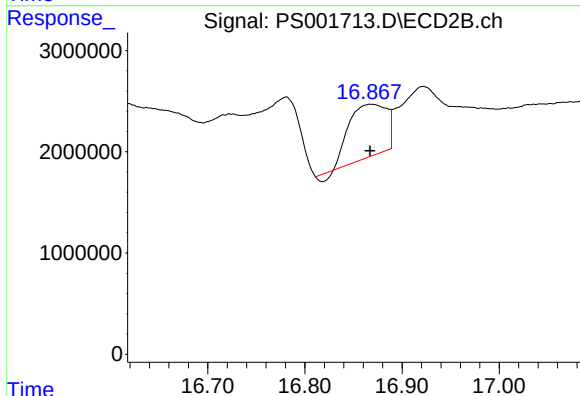


#15 Picloram

R.T.: 16.868 min
Delta R.T.: 0.001 min
Response: 13659369
Conc: 10.48 ng/ml

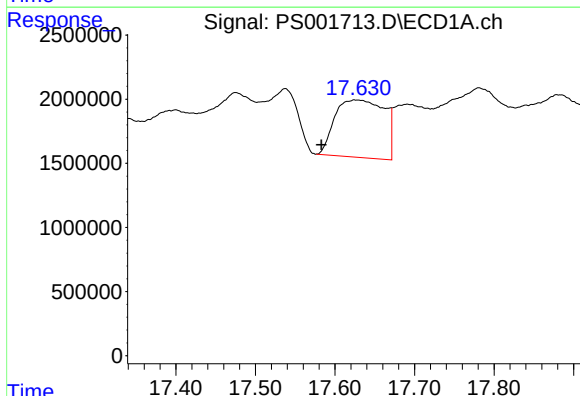

#16 DCPA

R.T.: 17.627 min
Delta R.T.: 0.044 min
Response: 19369418
Conc: 17.07 ng/ml

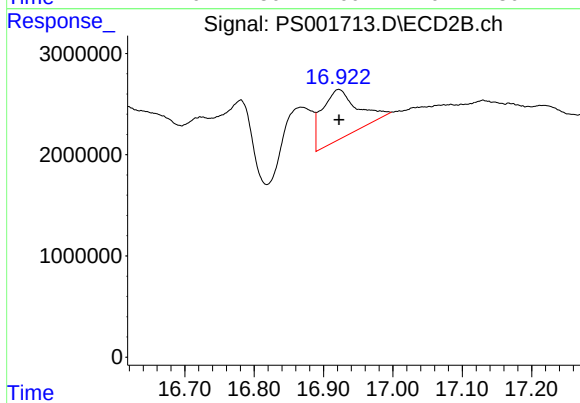

#16 DCPA

R.T.: 16.922 min
Delta R.T.: 0.000 min
Response: 17230097
Conc: 12.07 ng/ml