

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
 Data File : PS001716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2018 17:28
 Operator : EI\SJ
 Sample : PB112785BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:16:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.466	10.965	107.8E6	105.2E6	583.834	519.623
Target Compounds							
1) T	Dalapon	2.889	0.000	866368	0	3.447	N.D. #
2) T	3,5-DICHL...	0.000	9.205	0	29725508	N.D.	116.318 #
6) T	MCP	12.155	0.000	28005425	0	55.659	N.D. #
9) T	2,4-D	13.392	0.000	925694	0	3.904	N.D. #
12) T	2,4,5-T	0.000	14.627	0	2212165	N.D.	2.561 #
14) T	DINOSEB	0.000	15.717	0	4539052	N.D.	6.137 #
15) T	Picloram	16.972	16.899	7041927	20251377	5.028	15.531 #
16) T	DCPA	0.000	16.899	0	20251377	N.D.	14.184 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
Data File : PS001716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2018 17:28
Operator : EI\SJ
Sample : PB112785BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:16:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

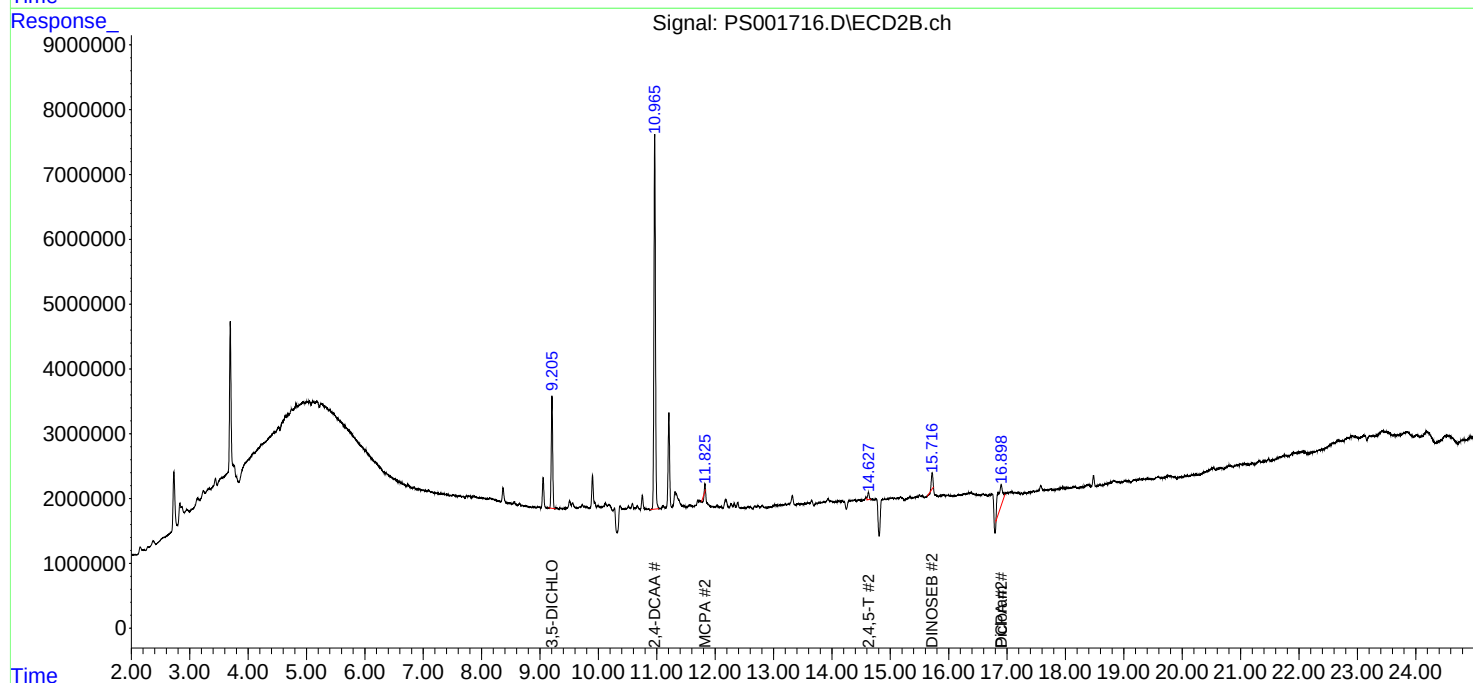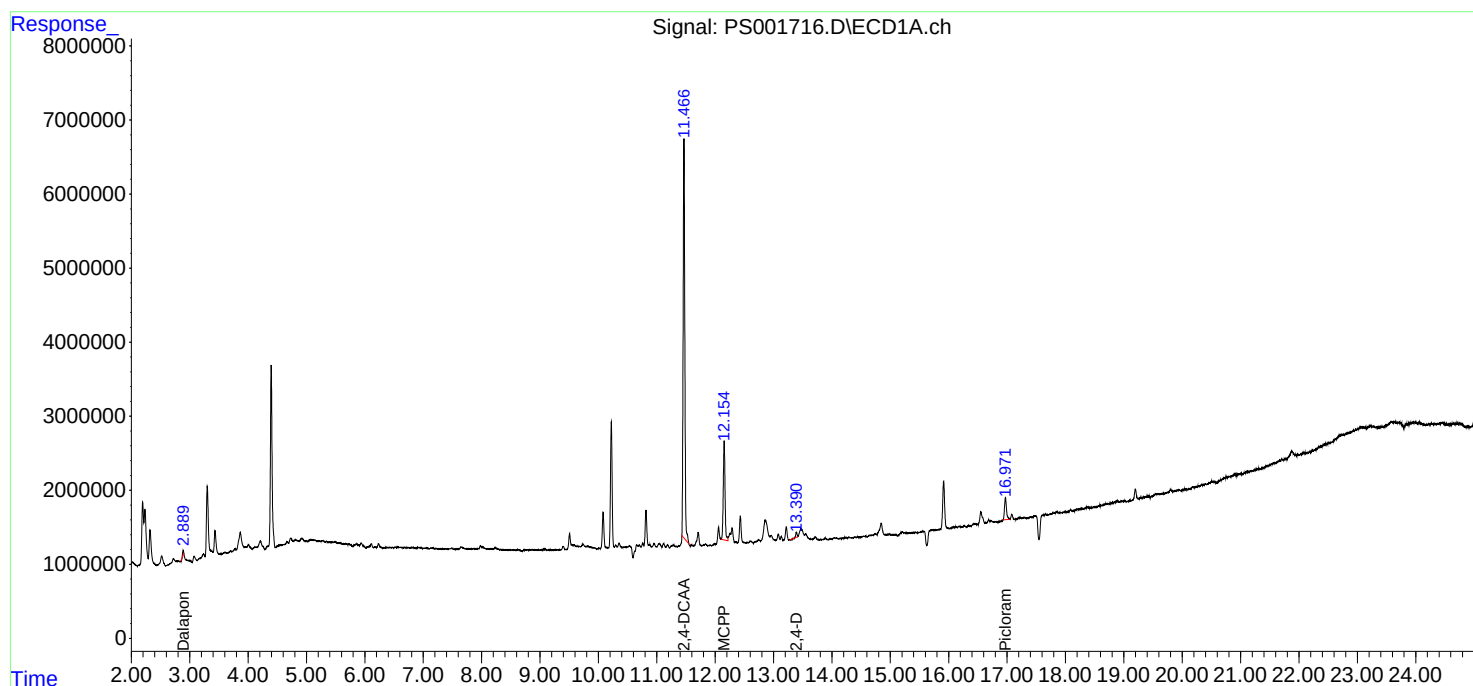


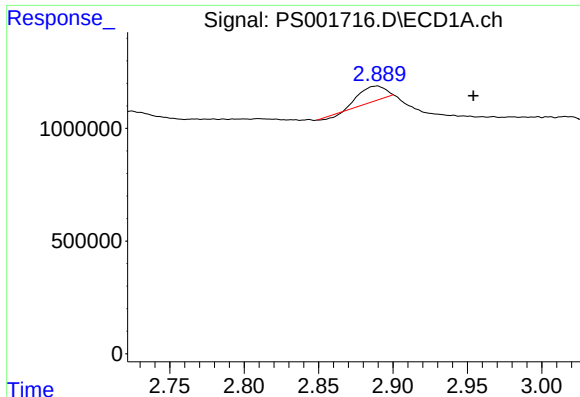

#1 Dalapon


R.T.: 2.889 min
Delta R.T.: -0.065 min
Response: 866368
Conc: 3.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

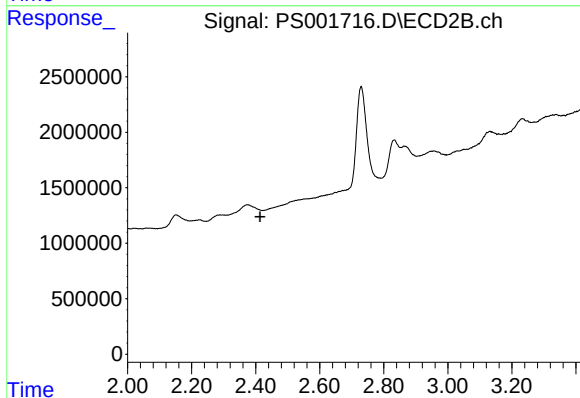


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.414 min
Response: 0
Conc: N.D.

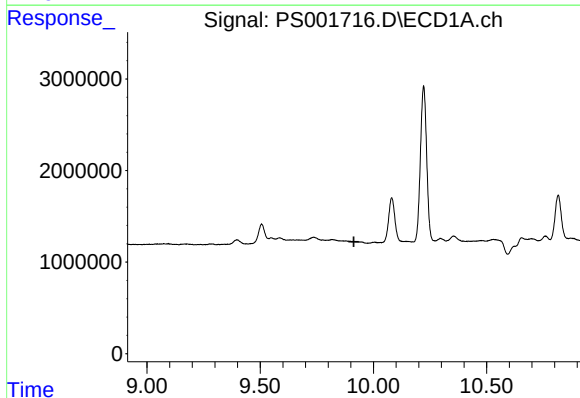


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

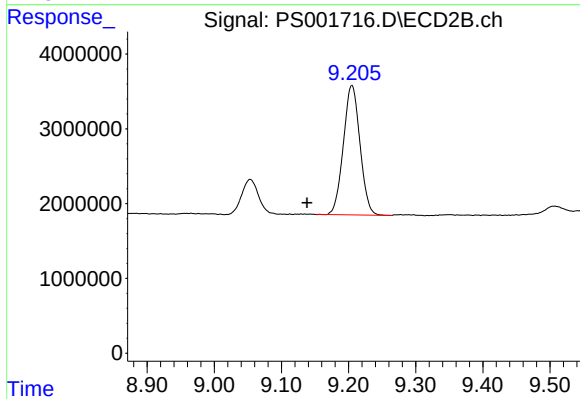

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.205 min
Delta R.T.: 0.067 min
Response: 29725508
Conc: 116.32 ng/ml

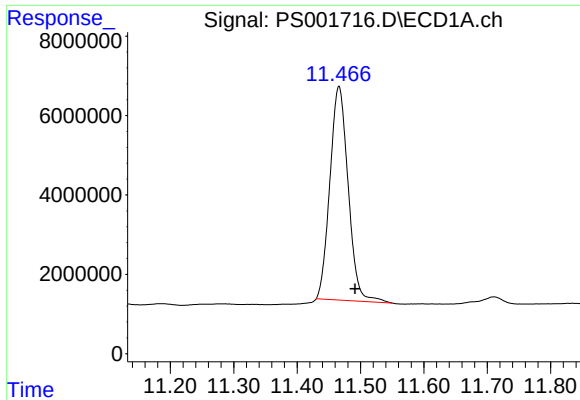

#4 2,4-DCAA


R.T.: 11.466 min
Delta R.T.: -0.026 min
Response: 107776023
Conc: 583.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

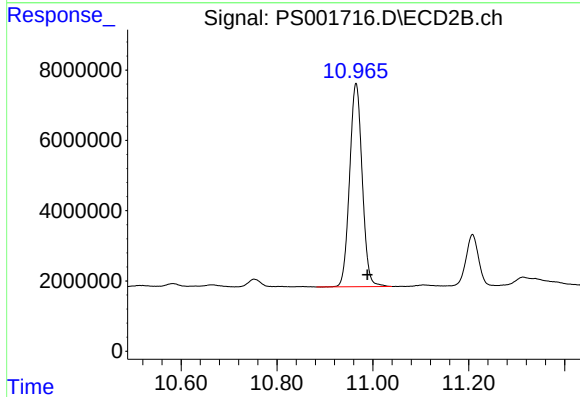


#4 2,4-DCAA

R.T.: 10.965 min
Delta R.T.: -0.024 min
Response: 105239307
Conc: 519.62 ng/ml

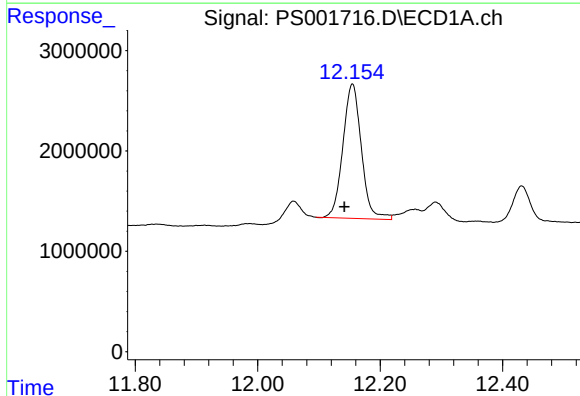


#6 MCP

R.T.: 12.155 min
Delta R.T.: 0.013 min
Response: 28005425
Conc: 55.66 ug/ml

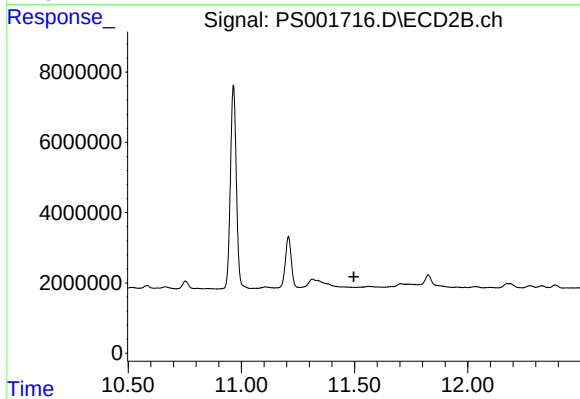

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

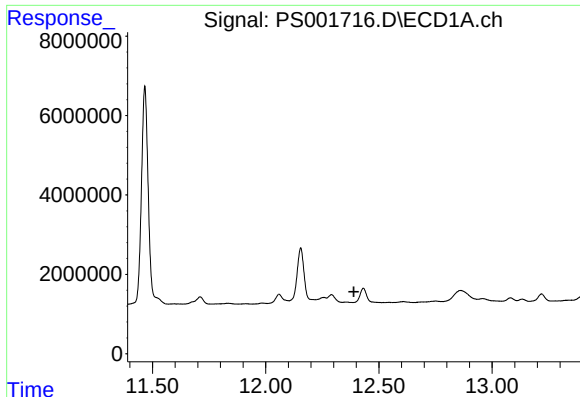

#7 MCPA


R.T.: 12.431 min
Delta R.T.: 0.041 min
Response: -951932
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

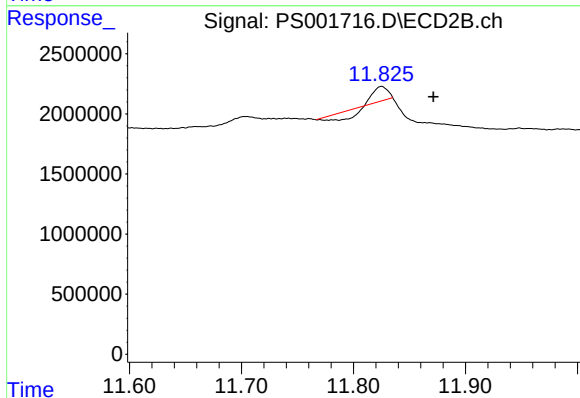


#7 MCPA

R.T.: 11.825 min
Delta R.T.: -0.046 min
Response: 228986
Conc: 0.31 ug/ml

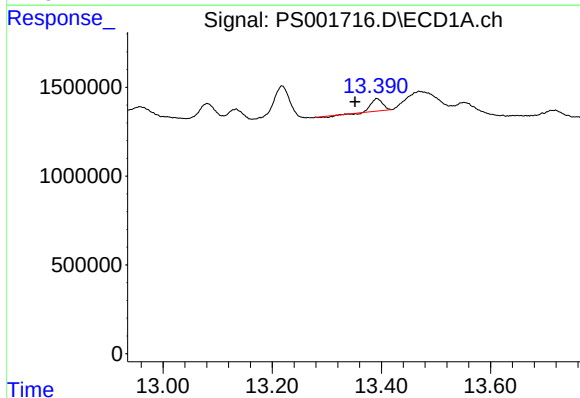


#9 2,4-D

R.T.: 13.392 min
Delta R.T.: 0.040 min
Response: 925694
Conc: 3.90 ng/ml

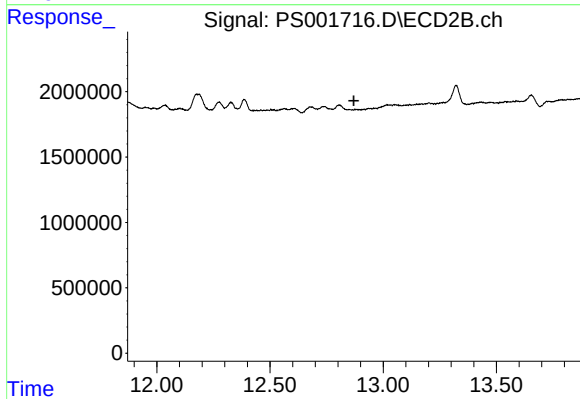

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.871 min
Response: 0
Conc: N.D.

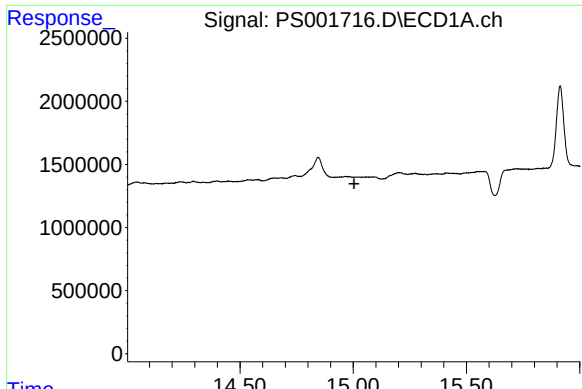

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

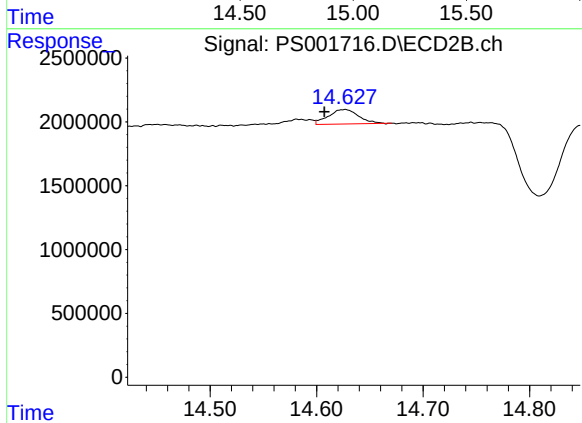


#12 2,4,5-T

R.T.: 14.627 min
Delta R.T.: 0.020 min
Response: 2212165
Conc: 2.56 ng/ml

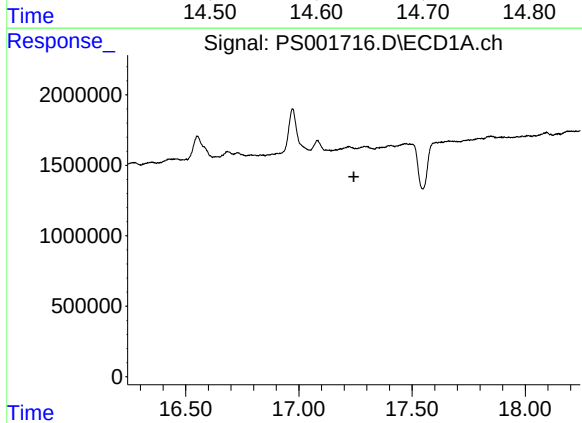


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.243 min
Response: 0
Conc: N.D.

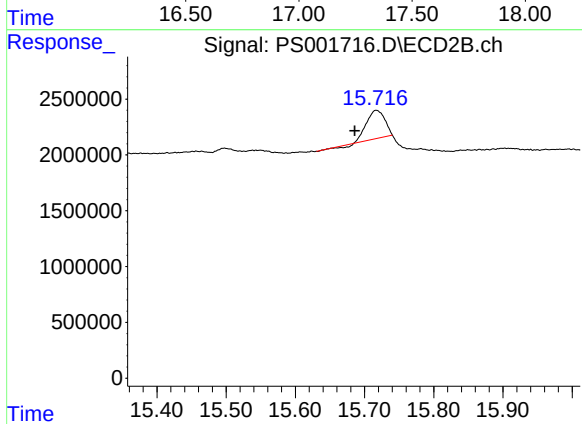

#14 DINOSEB


R.T.: 15.717 min
Delta R.T.: 0.031 min
Response: 4539052
Conc: 6.14 ng/ml

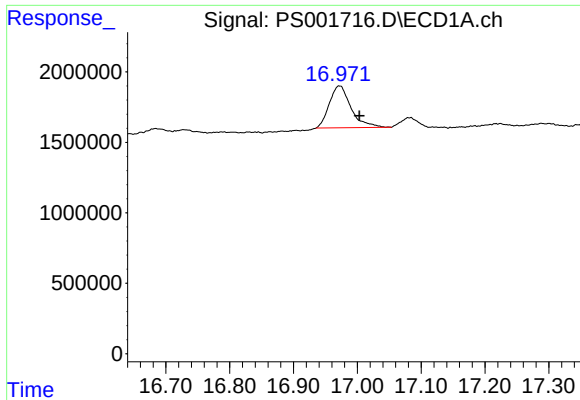

#15 Picloram


R.T.: 16.972 min
Delta R.T.: -0.031 min
Response: 7041927
Conc: 5.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

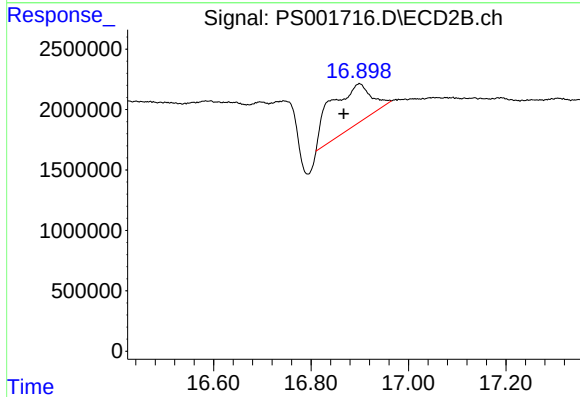


#15 Picloram

R.T.: 16.899 min
Delta R.T.: 0.032 min
Response: 20251377
Conc: 15.53 ng/ml

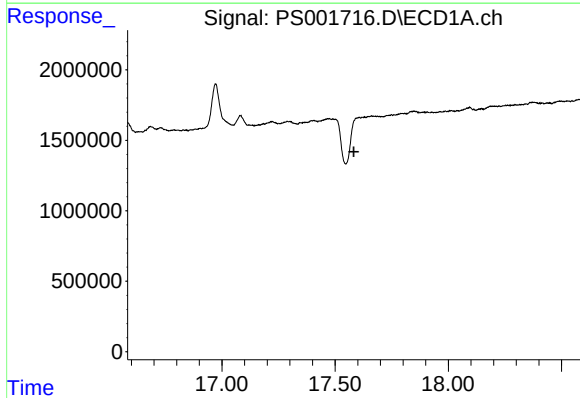

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

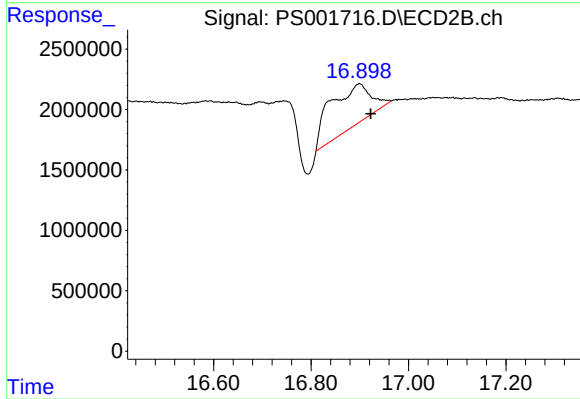

#16 DCPA

R.T.: 16.899 min
Delta R.T.: -0.023 min
Response: 20251377
Conc: 14.18 ng/ml