

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
 Data File : PS001718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2018 18:30
 Operator : EI\SJ
 Sample : PB112785TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:17:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.499	10.998	90863626	87573357	492.218	432.397
Target Compounds							
2) T	3,5-DICHL...	0.000	9.086	0	4676248	N.D.	18.298 #
5) T	DICAMBA	0.000	11.241	0	17470869	N.D.	24.910 #
6) T	MCP	12.187	0.000	29529610	0	58.688	N.D. #
11) T	2,4,5-TP ...	0.000	13.970	0	2475467	N.D.	2.329 #
15) T	Picloram	17.011	16.931	3479194	6654219	2.484	5.103 #
16) T	DCPA	0.000	16.931	0	6654219	N.D.	4.661 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
Data File : PS001718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2018 18:30
Operator : EI\SJ
Sample : PB112785TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:17:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

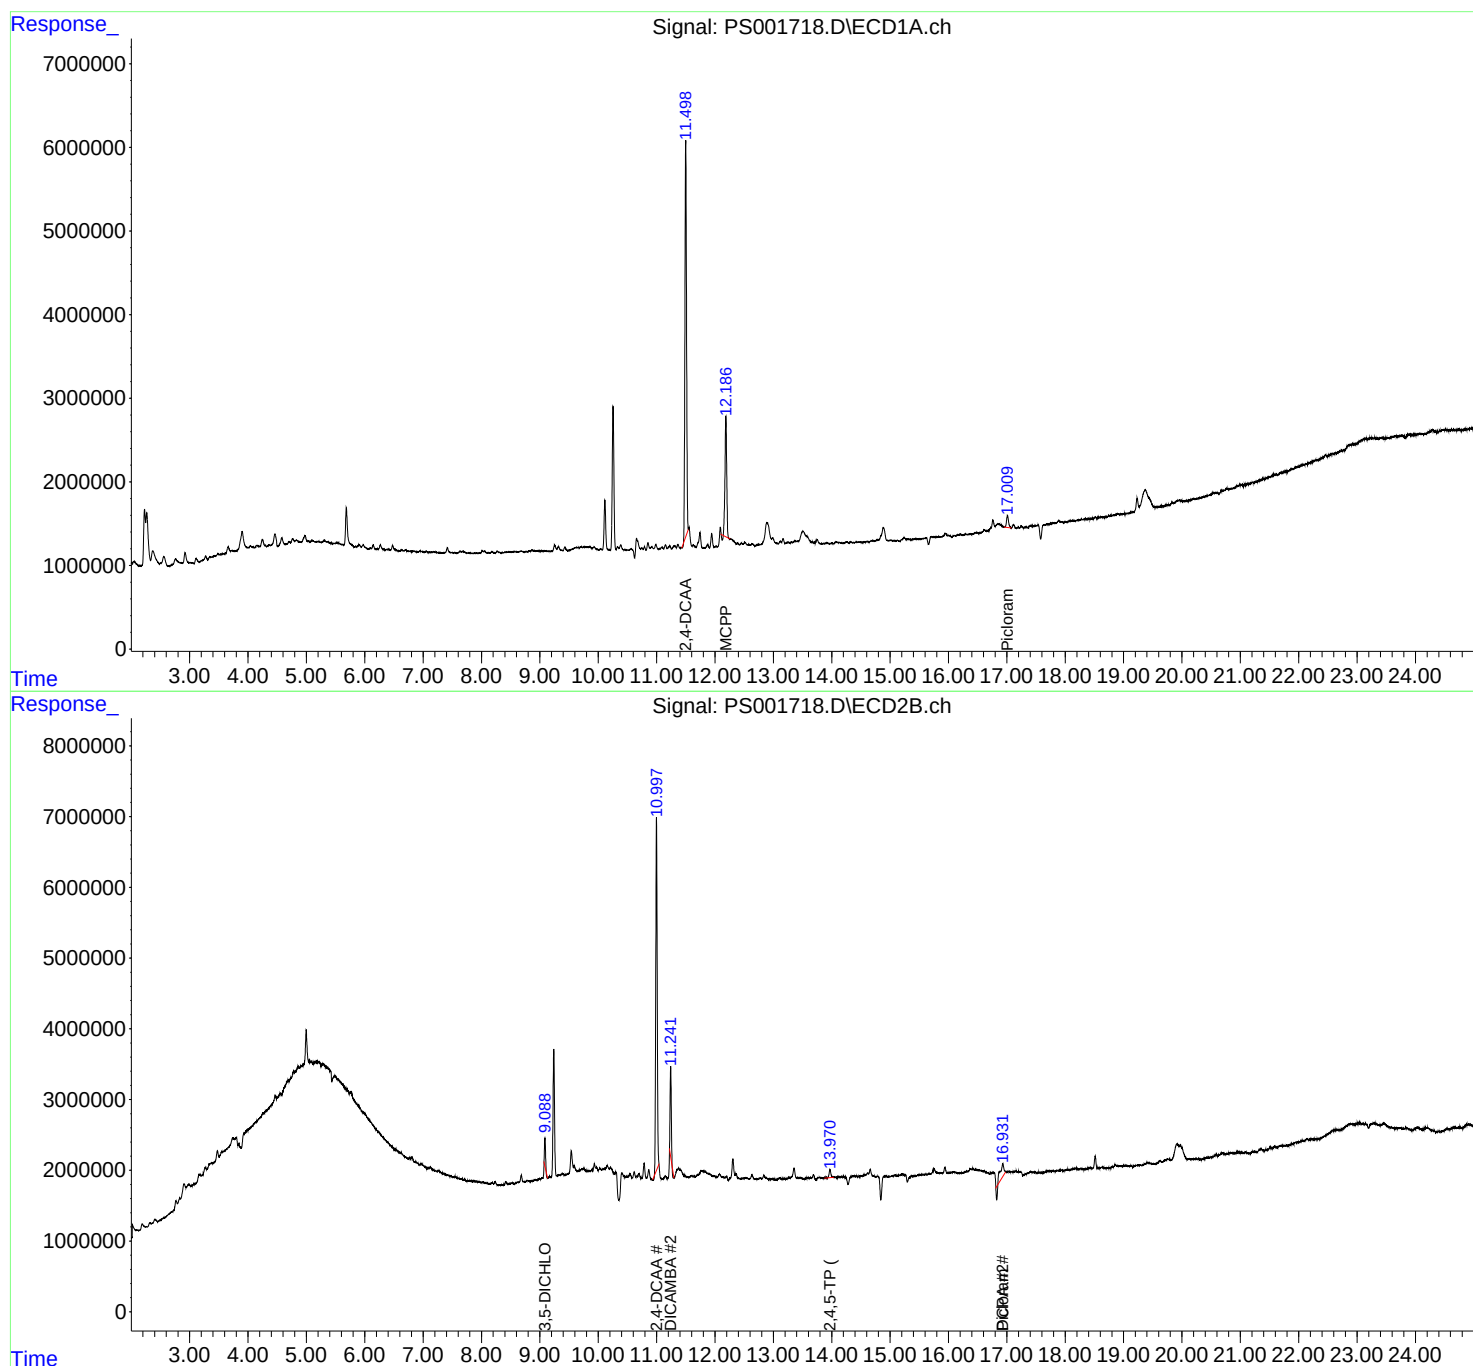


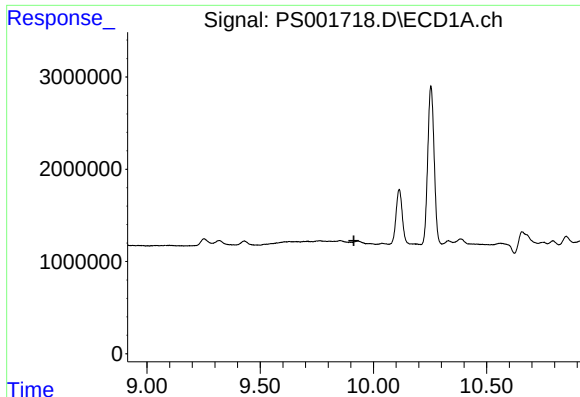

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

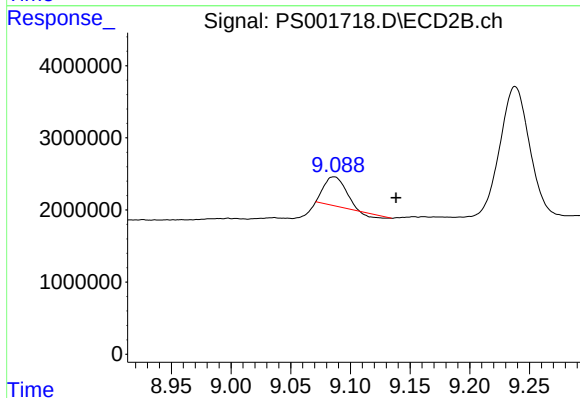


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.086 min
Delta R.T.: -0.052 min
Response: 4676248
Conc: 18.30 ng/ml

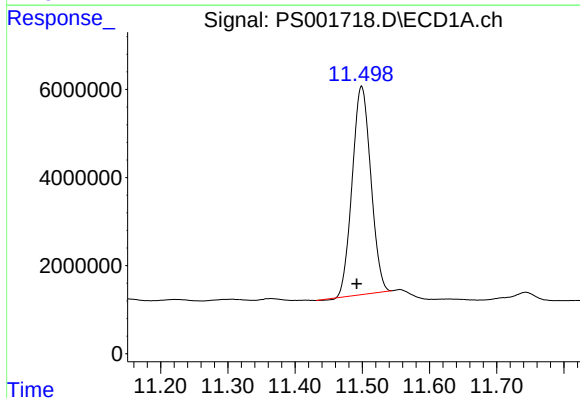


#4 2,4-DCAA

R.T.: 11.499 min
Delta R.T.: 0.007 min
Response: 90863626
Conc: 492.22 ng/ml

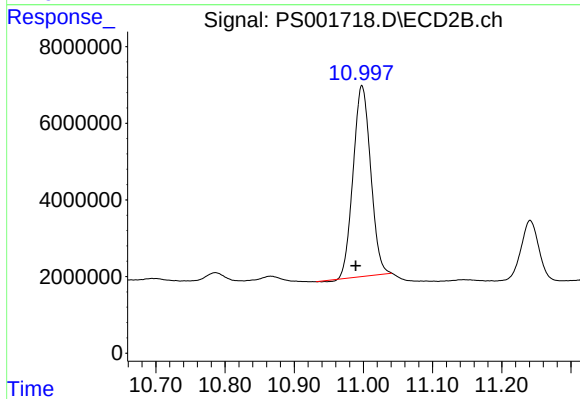

#4 2,4-DCAA


R.T.: 10.998 min
Delta R.T.: 0.009 min
Response: 87573357
Conc: 432.40 ng/ml

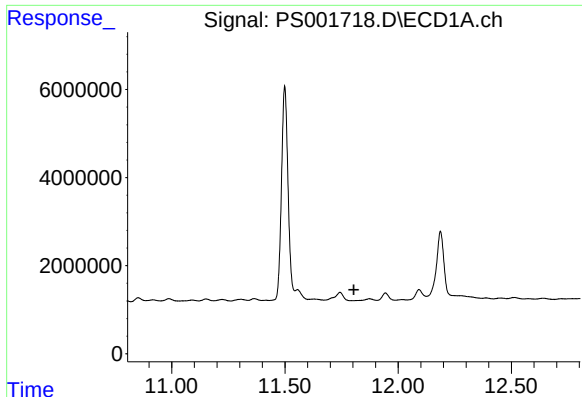

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

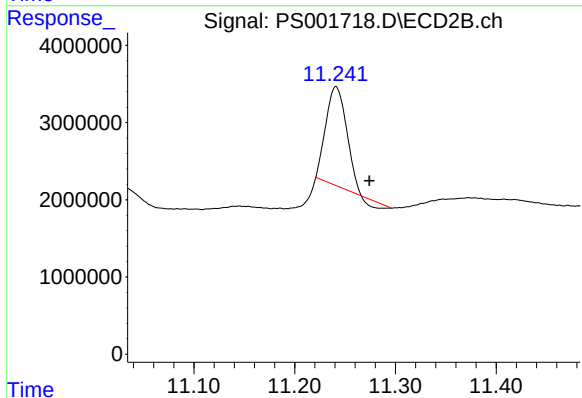


#5 DICAMBA

R.T.: 11.241 min
Delta R.T.: -0.033 min
Response: 17470869
Conc: 24.91 ng/ml

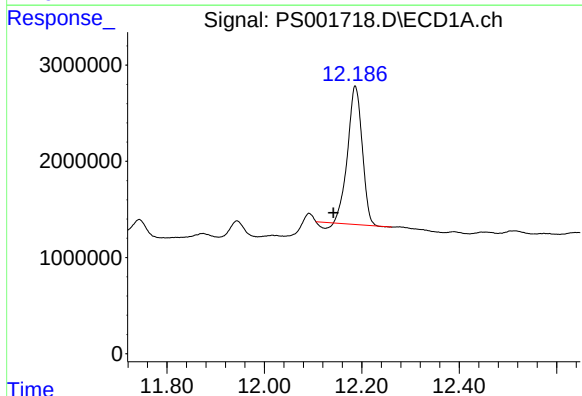


#6 MCP

R.T.: 12.187 min
Delta R.T.: 0.045 min
Response: 29529610
Conc: 58.69 ug/ml

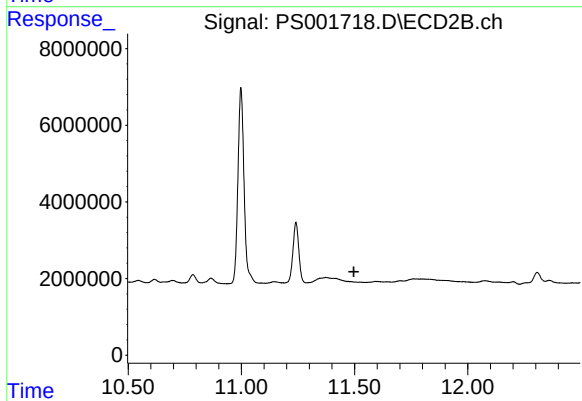

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

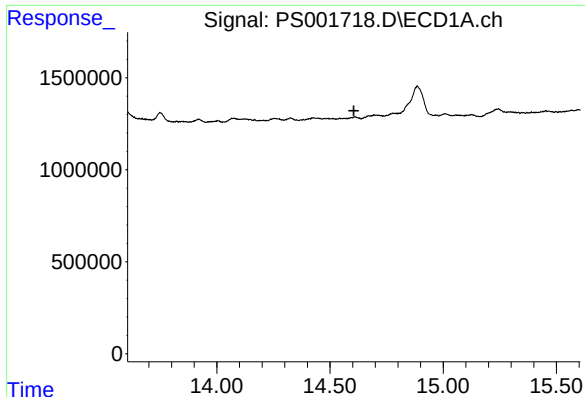

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

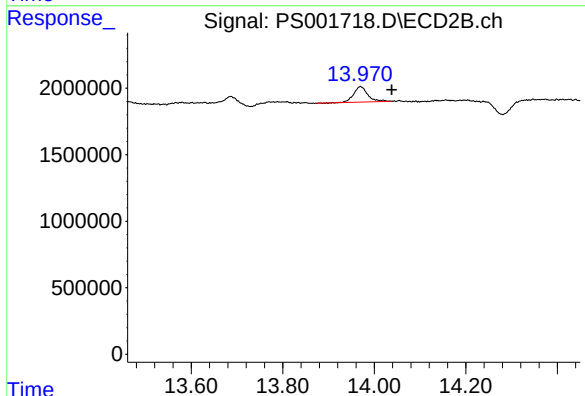


#11 2,4,5-TP (SILVEX)

R.T.: 13.970 min
Delta R.T.: -0.069 min
Response: 2475467
Conc: 2.33 ng/ml

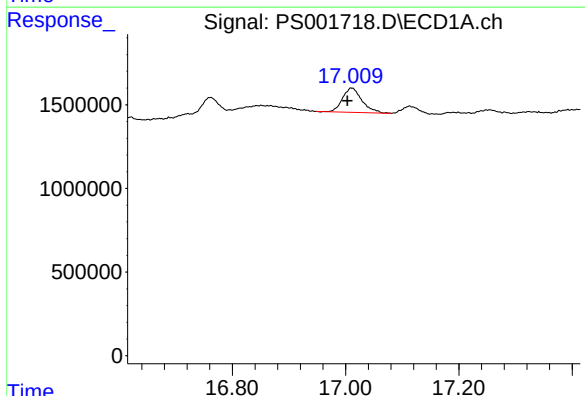


#15 Picloram

R.T.: 17.011 min
Delta R.T.: 0.008 min
Response: 3479194
Conc: 2.48 ng/ml

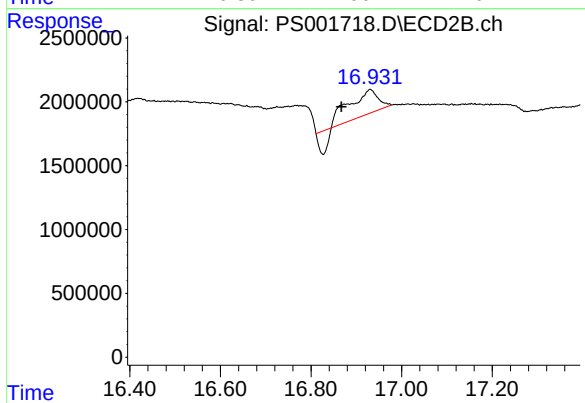

#15 Picloram


R.T.: 16.931 min
Delta R.T.: 0.063 min
Response: 6654219
Conc: 5.10 ng/ml

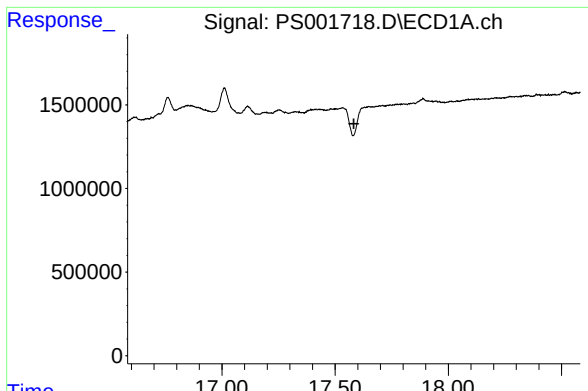

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

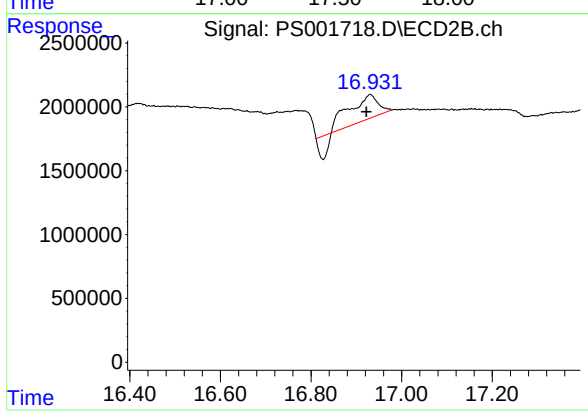

#16 DCPA

R.T.: 16.931 min
Delta R.T.: 0.008 min
Response: 6654219
Conc: 4.66 ng/ml