

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
 Data File : PS001722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2018 20:34
 Operator : EI\SJ
 Sample : J4842-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 01:18:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.504	11.003	102.5E6	96338468	555.142	475.675
Target Compounds							
1) T	Dalapon	2.927	0.000	3305066	0	13.148	N.D. #
2) T	3,5-DICHL...	0.000	9.092	0	10141785	N.D.	39.685 #
5) T	DICAMBA	0.000	11.246	0	22977946	N.D.	32.763 #
6) T	MCP	12.192	0.000	27213729	0	54.085	N.D. #
15) T	Picloram	17.010	16.882	8564013	-332397	6.114	N.D. #
16) T	DCPA	0.000	16.936	0	4540622	N.D.	3.180 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091218\
Data File : PS001722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2018 20:34
Operator : EI\SJ
Sample : J4842-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 01:18:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

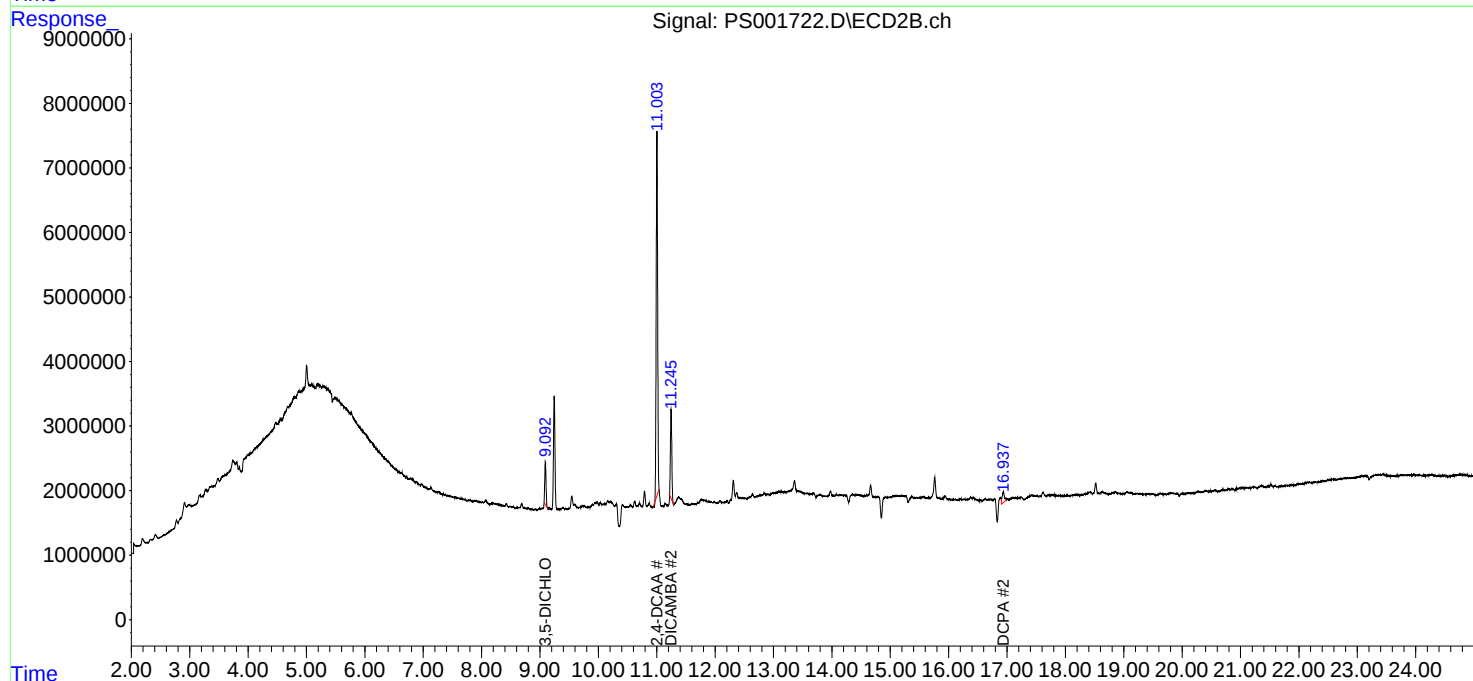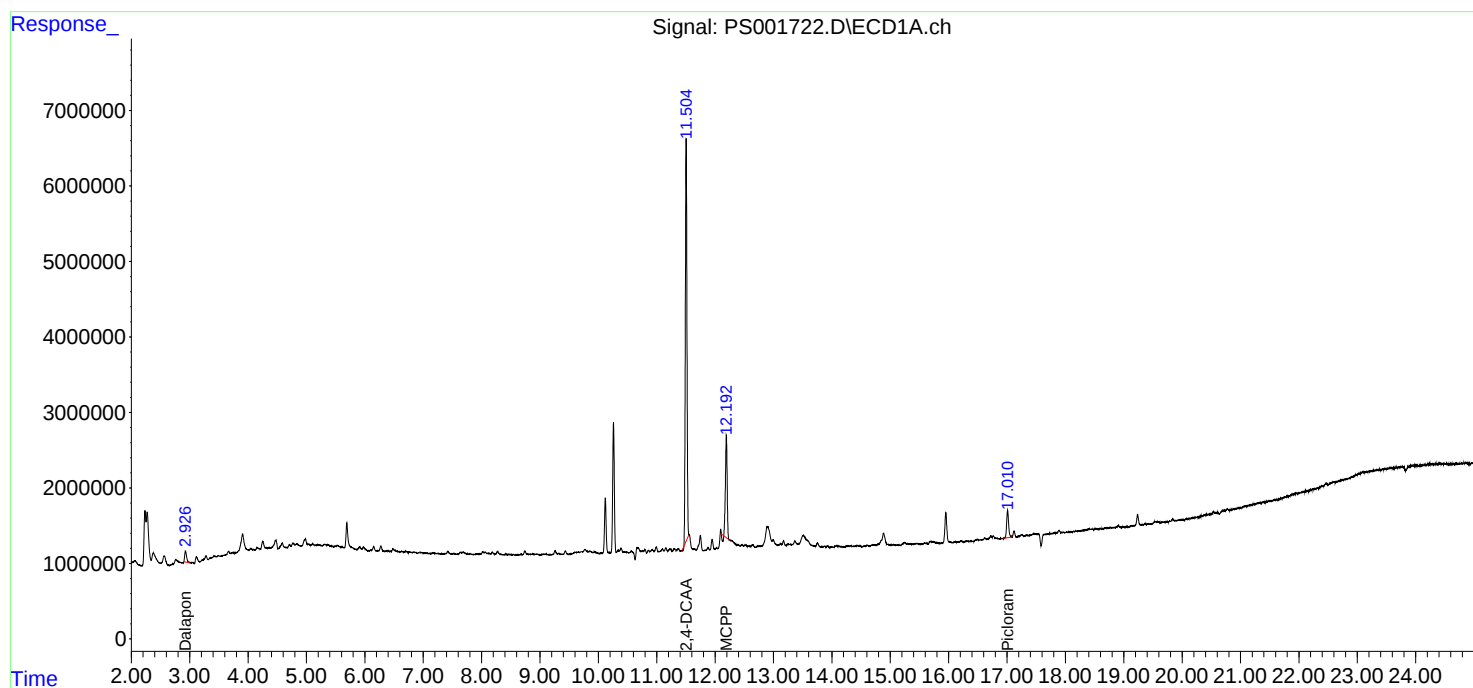


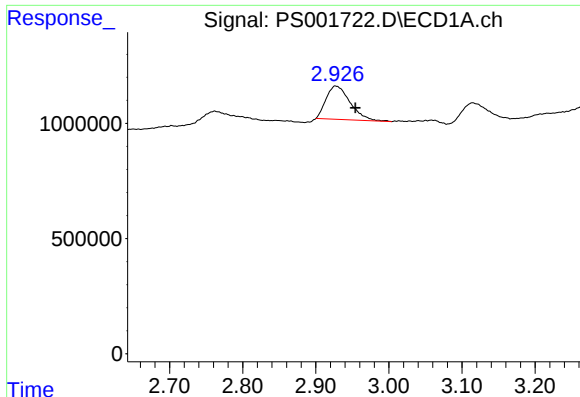

#1 Dalapon


R.T.: 2.927 min
Delta R.T.: -0.027 min
Response: 3305066
Conc: 13.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

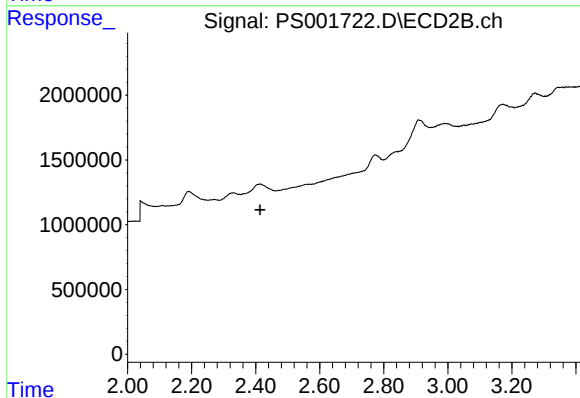


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.414 min
Response: 0
Conc: N.D.

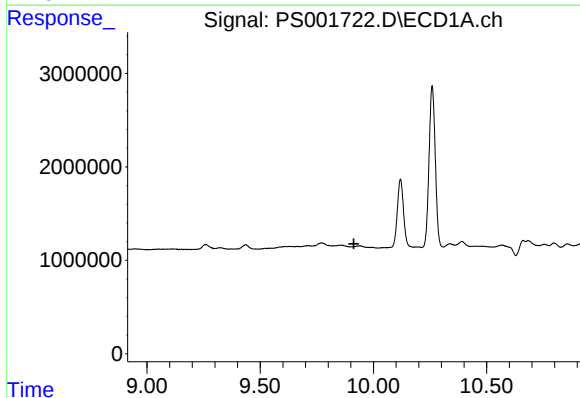


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

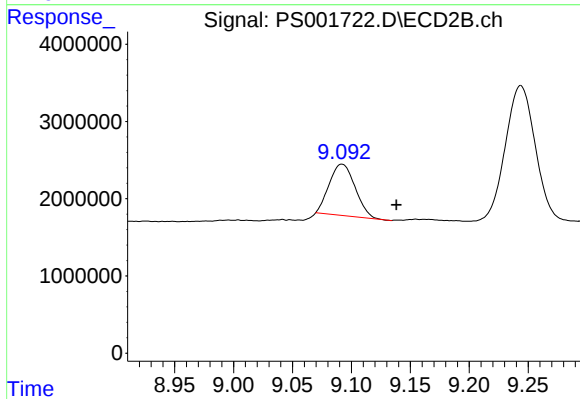

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.092 min
Delta R.T.: -0.046 min
Response: 10141785
Conc: 39.69 ng/ml

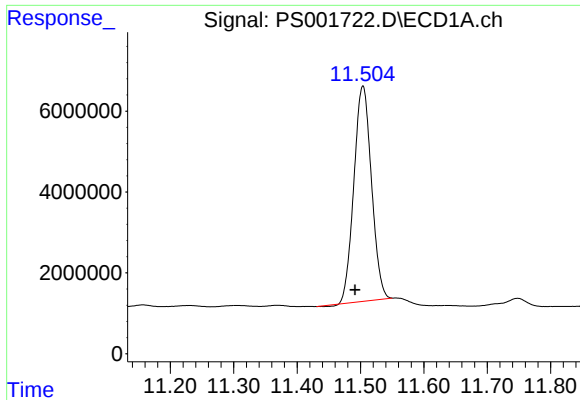

#4 2,4-DCAA


R.T.: 11.504 min
Delta R.T.: 0.012 min
Response: 102479450
Conc: 555.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

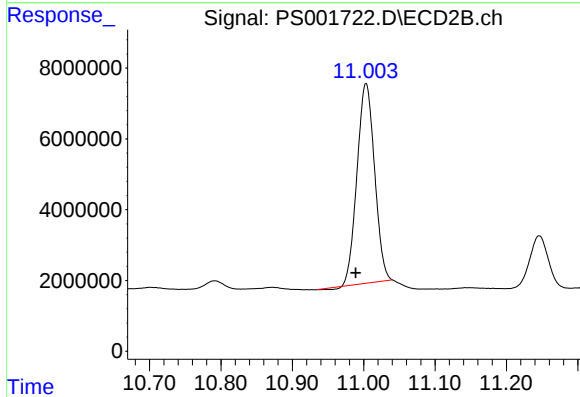


#4 2,4-DCAA

R.T.: 11.003 min
Delta R.T.: 0.014 min
Response: 96338468
Conc: 475.68 ng/ml

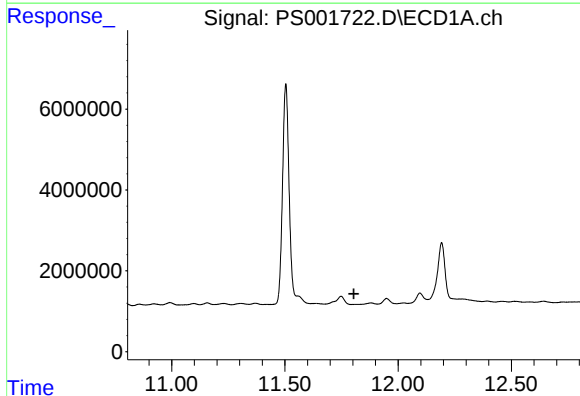


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

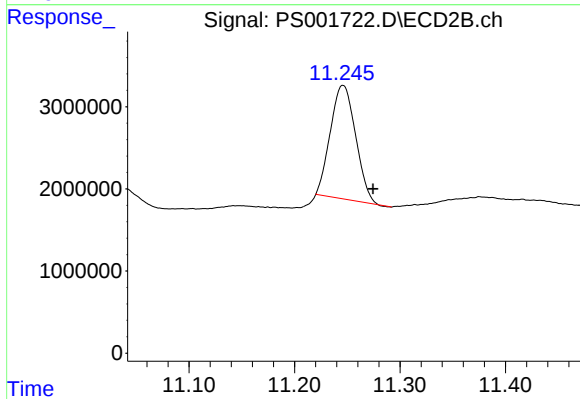

#5 DICAMBA


R.T.: 11.246 min
Delta R.T.: -0.028 min
Response: 22977946
Conc: 32.76 ng/ml

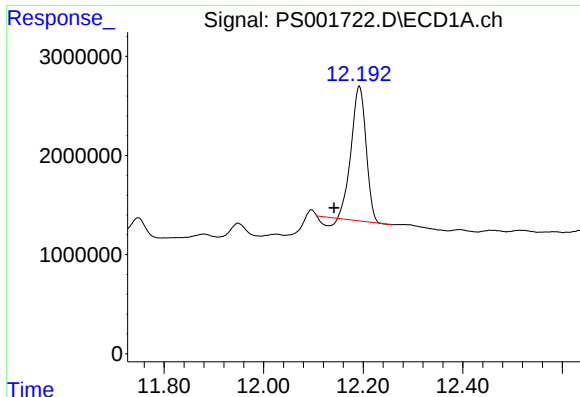

#6 MCP


R.T.: 12.192 min
Delta R.T.: 0.050 min
Response: 27213729
Conc: 54.09 ug/ml

Instrument :
ECD_S
ClientSampleId :

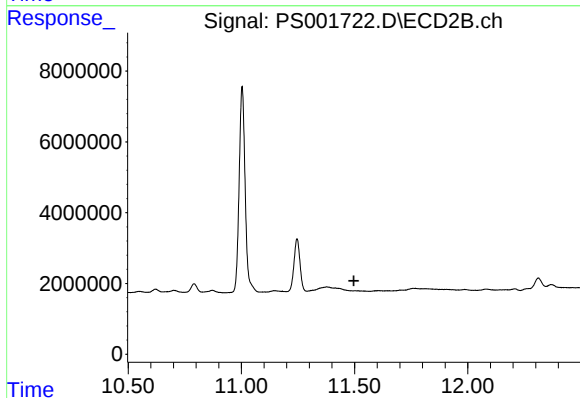


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

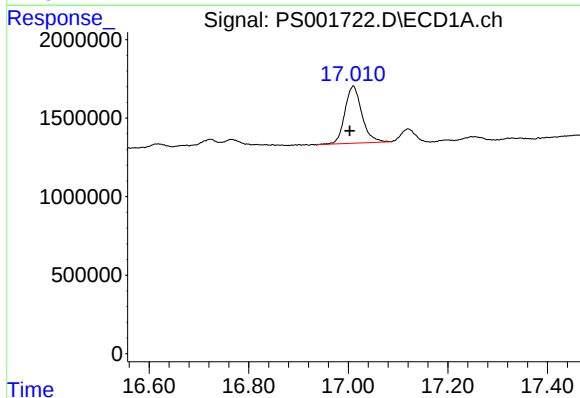


#15 Picloram

R.T.: 17.010 min
Delta R.T.: 0.007 min
Response: 8564013
Conc: 6.11 ng/ml

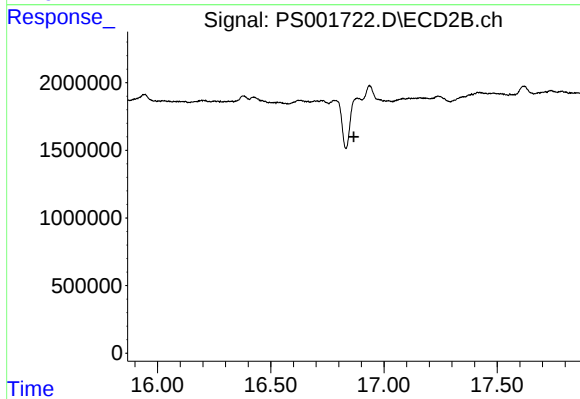

#15 Picloram


R.T.: 16.882 min
Delta R.T.: 0.014 min
Response: -332397
Conc: N.D.

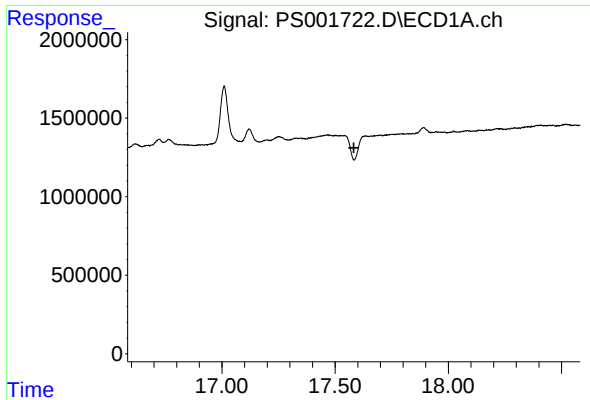

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

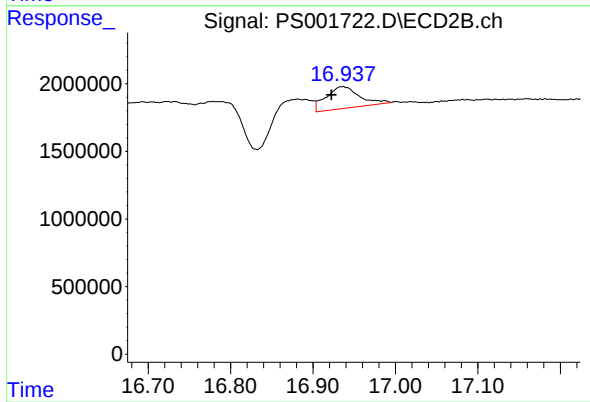

#16 DCPA

R.T.: 16.936 min
Delta R.T.: 0.013 min
Response: 4540622
Conc: 3.18 ng/ml