

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091219\
 Data File : PS006671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2019 13:26
 Operator : SM\AJ
 Sample : K4764-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ROLL-OFF-COMPOSITE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 04:49:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.496	5.226	206.1E6	110.5E6	265.254	258.751
Target Compounds							
1) T	Dalapon	2.040	1.754	129.2E6	155.0E6	132.146	303.267 #
2) T	3,5-DICHL...	0.000	4.554	0	53005535	N.D.	97.931
3) T	4-Nitroph...	5.350	0.000	15863071	0	44.701	N.D. #
5) T	DICAMBA	5.709	0.000	6489713	0	2.251	N.D. #
7) T	MCPA	5.972	5.602	15097542	28987978	5.342	16.527 #
9) T	2,4-D	6.560	0.000	132.8E6	0	171.882	N.D. #
13) T	2,4-DB	8.100	0.000	31373636	0	51.554	N.D. #
16) T	DCPA	9.452	0.000	80958596	0	14.331	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091219\
Data File : PS006671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2019 13:26
Operator : SM\AJ
Sample : K4764-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 04:49:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

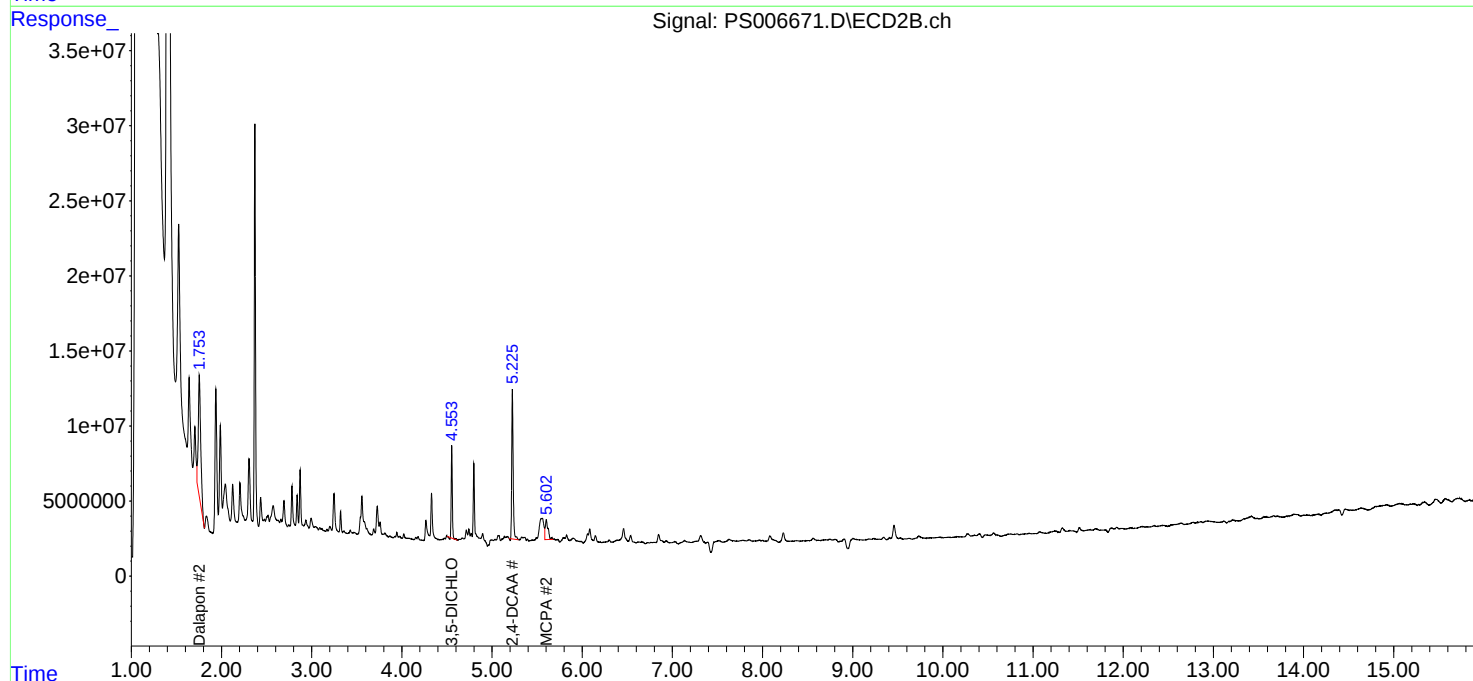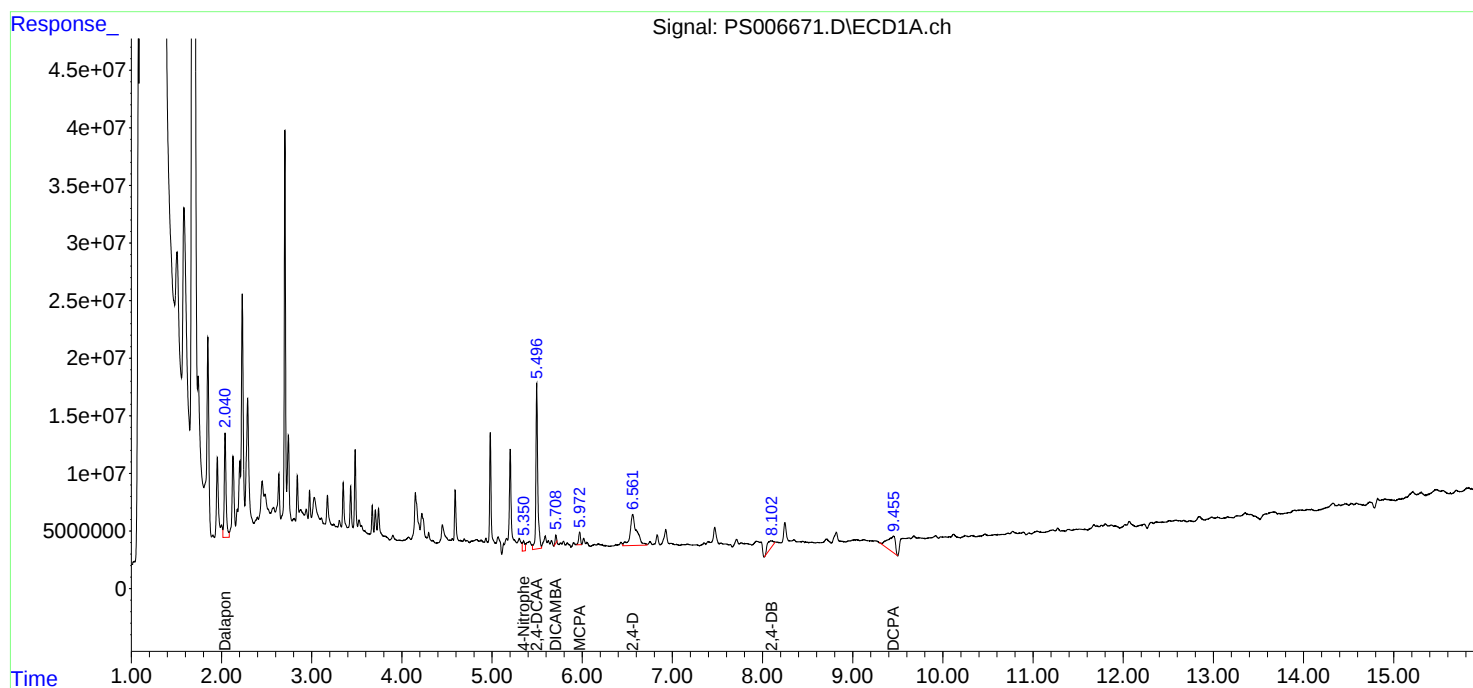


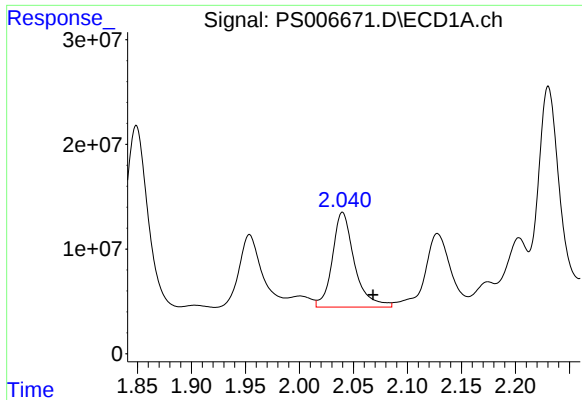

#1 Dalapon


R.T.: 2.040 min
Delta R.T.: -0.028 min
Response: 129159598
Conc: 132.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-1

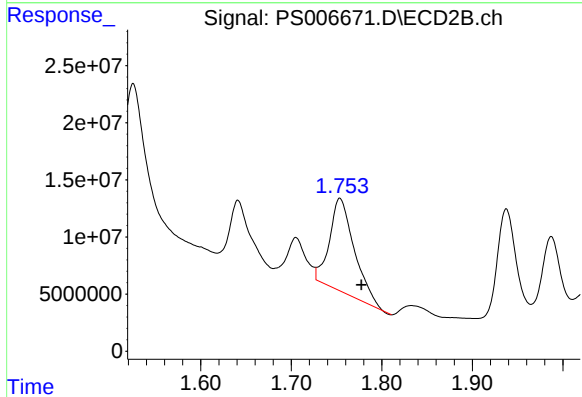


#1 Dalapon

R.T.: 1.754 min
Delta R.T.: -0.024 min
Response: 154983985
Conc: 303.27 ng/ml

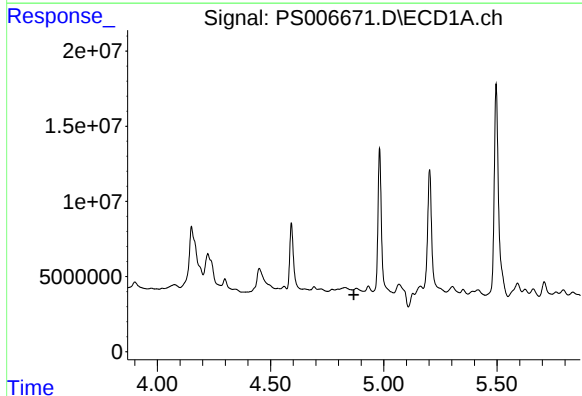


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

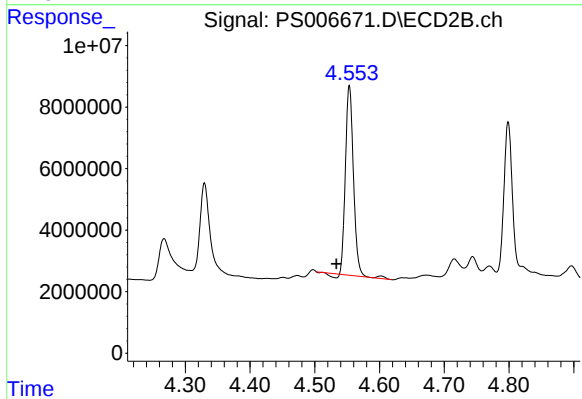

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.554 min
Delta R.T.: 0.020 min
Response: 53005535
Conc: 97.93 ng/ml

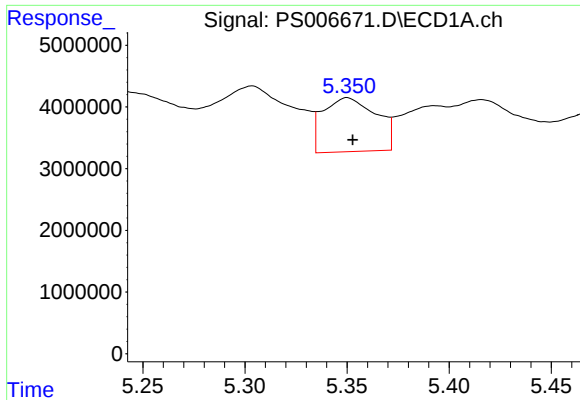

#3 4-Nitrophenol


R.T.: 5.350 min
Delta R.T.: -0.003 min
Response: 15863071
Conc: 44.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-1

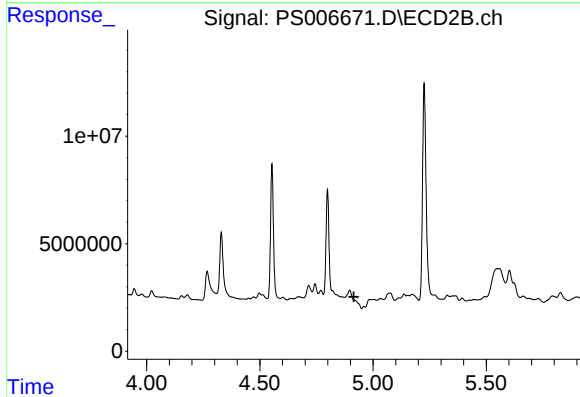


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

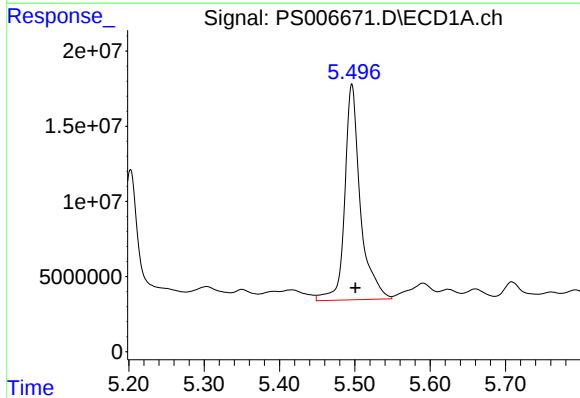


#4 2,4-DCAA

R.T.: 5.496 min
Delta R.T.: -0.005 min
Response: 206072283
Conc: 265.25 ng/ml

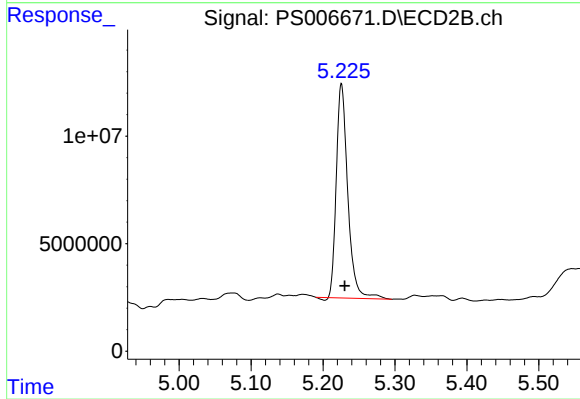

#4 2,4-DCAA


R.T.: 5.226 min
Delta R.T.: -0.004 min
Response: 110487454
Conc: 258.75 ng/ml

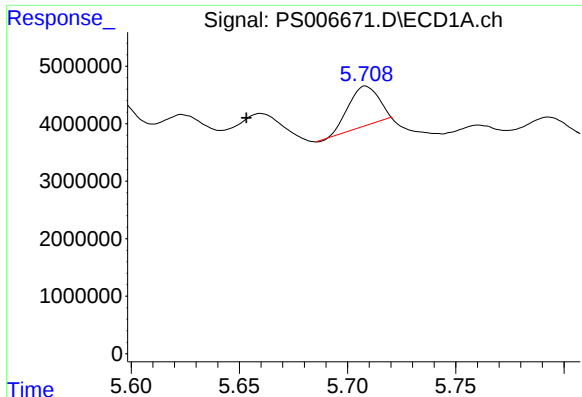

#5 DICAMBA


R.T.: 5.709 min
Delta R.T.: 0.055 min
Response: 6489713
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-1

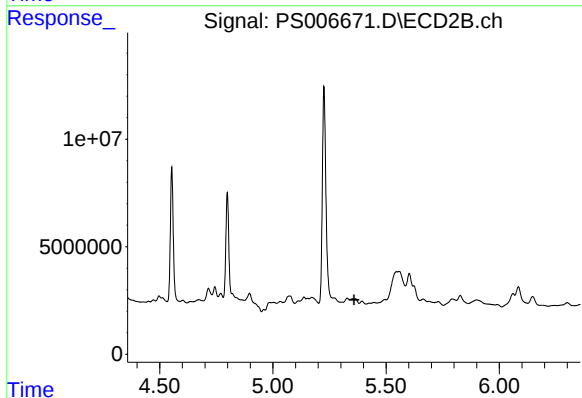


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

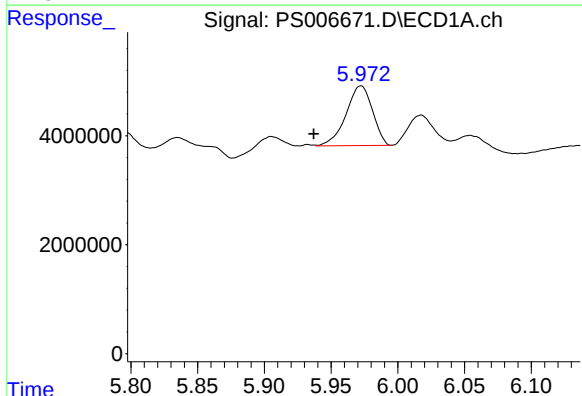


#7 MCPA

R.T.: 5.972 min
Delta R.T.: 0.035 min
Response: 15097542
Conc: 5.34 ug/ml

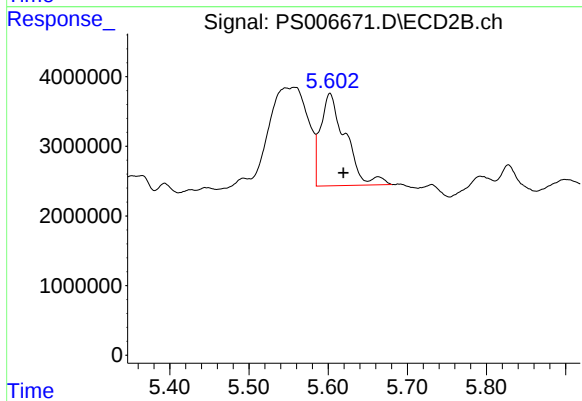

#7 MCPA


R.T.: 5.602 min
Delta R.T.: -0.017 min
Response: 28987978
Conc: 16.53 ug/ml

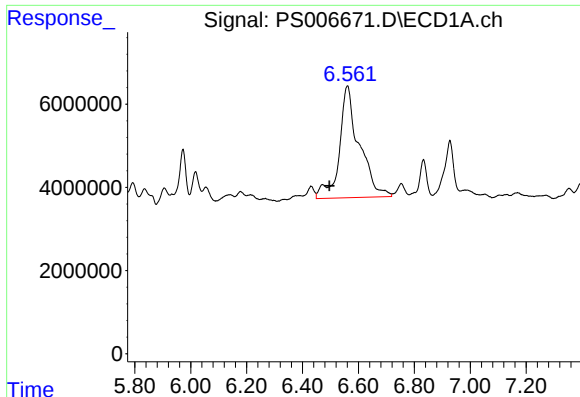

#9 2,4-D


R.T.: 6.560 min
Delta R.T.: 0.064 min
Response: 132799969
Conc: 171.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-1

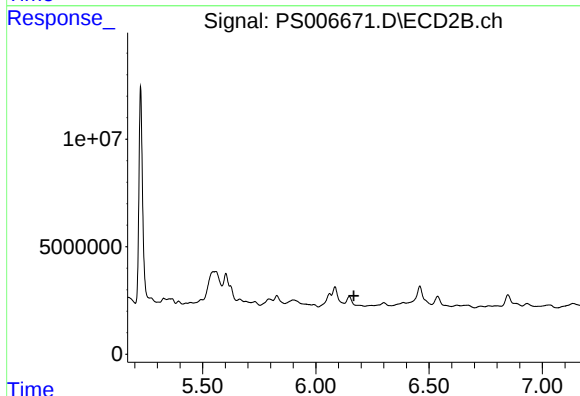


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

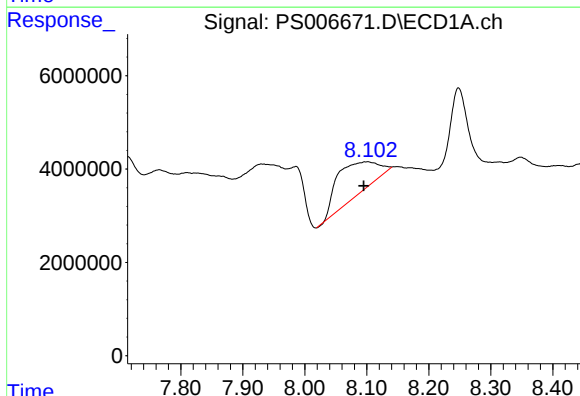


#13 2,4-DB

R.T.: 8.100 min
Delta R.T.: 0.005 min
Response: 31373636
Conc: 51.55 ng/ml

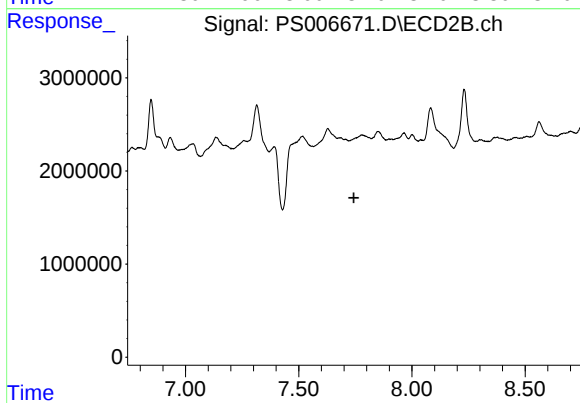

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

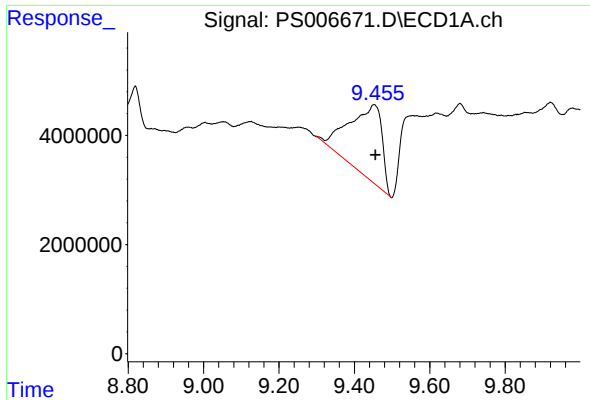

#16 DCPA

R.T.: 9.452 min
Delta R.T.: -0.004 min
Response: 80958596
Conc: 14.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-1

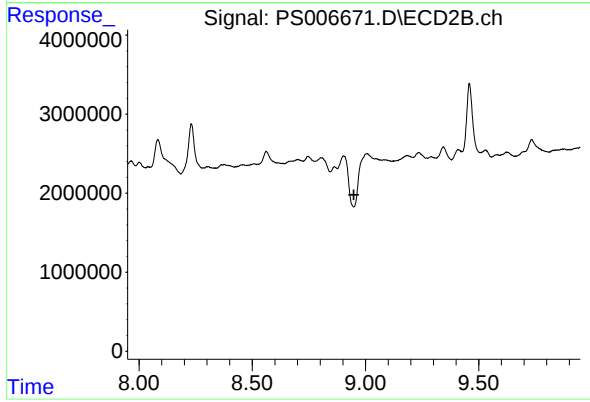

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.949 min
Response: 0
Conc: N.D.