

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091219\
 Data File : PS006672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2019 13:48
 Operator : SM\AJ
 Sample : K4764-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ROLL-OFF-COMPOSITE-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 04:49:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.215	231.6E6	119.7E6	298.087	280.338
Target Compounds							
1) T	Dalapon	2.029	1.742	90793385	56219334	92.893	110.008
2) T	3,5-DICHL...	4.920	4.543	7407696	42120553	7.483	77.821 #
3) T	4-Nitroph...	5.338	0.000	13976126	0	39.384	N.D. #
5) T	DICAMBA	5.650	0.000	11960969	0	4.149	N.D. #
7) T	MCPA	5.961	5.591	12124585	27206870	4.290	15.511 #
9) T	2,4-D	6.550	0.000	115.0E6	0	148.887	N.D. #
10) T	Pentachlo...	6.821	0.000	11139476	0	<MDL	N.D. #
13) T	2,4-DB	8.088	0.000	67002922	0	110.102	N.D. #
16) T	DCPA	9.442	0.000	84519675	0	14.961	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091219\
Data File : PS006672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2019 13:48
Operator : SM\AJ
Sample : K4764-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 04:49:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

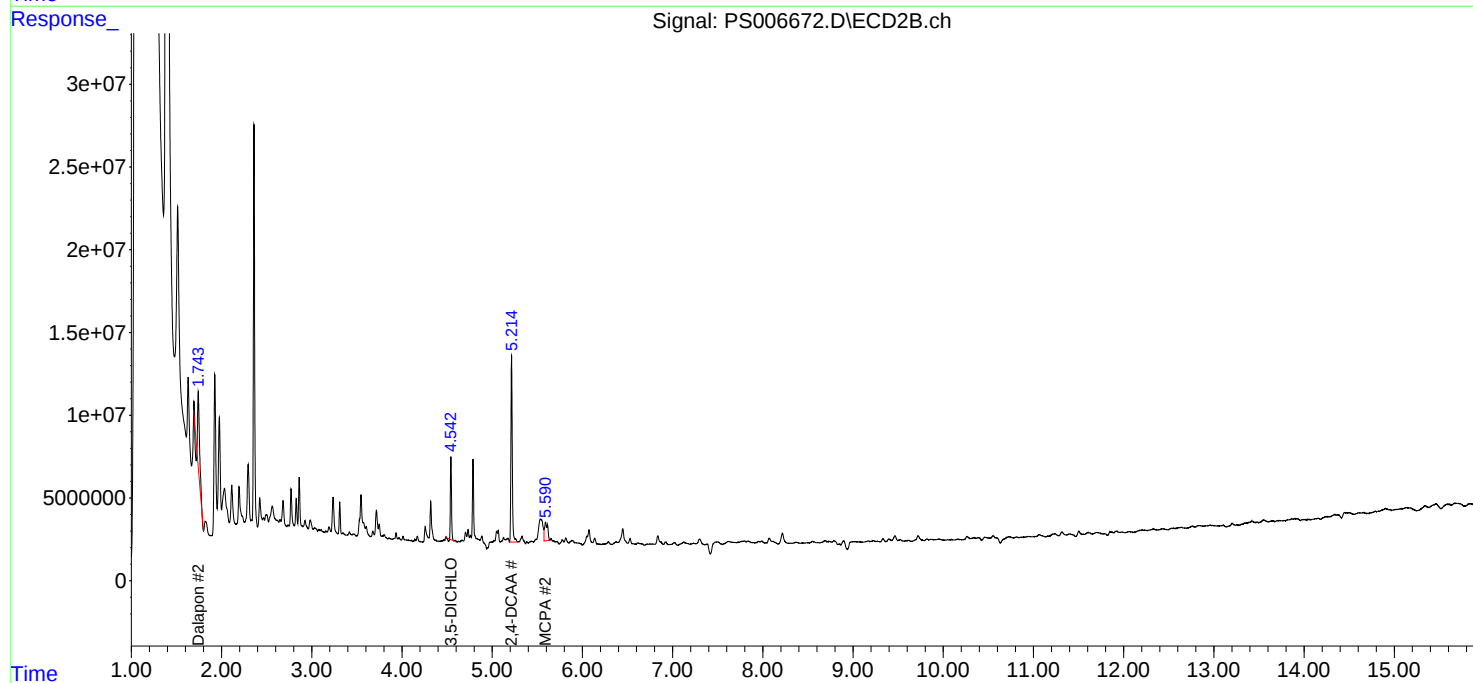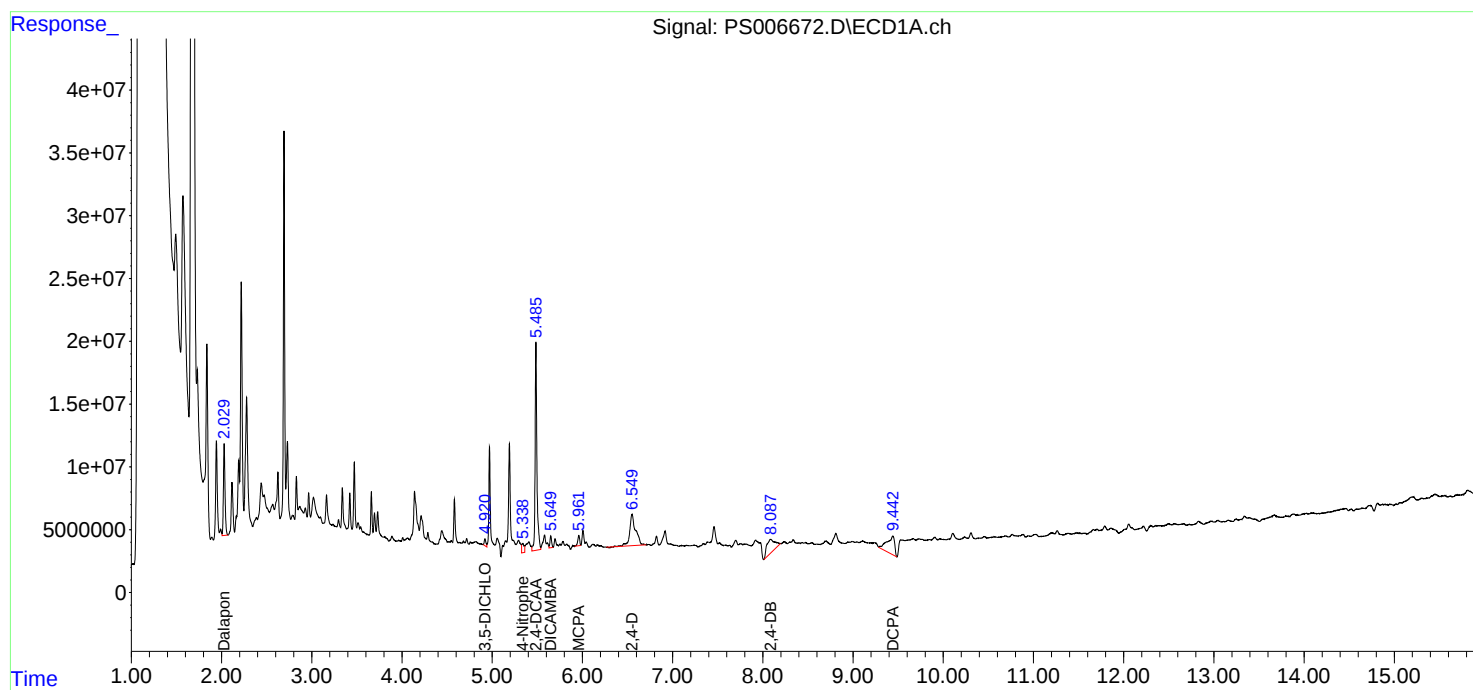


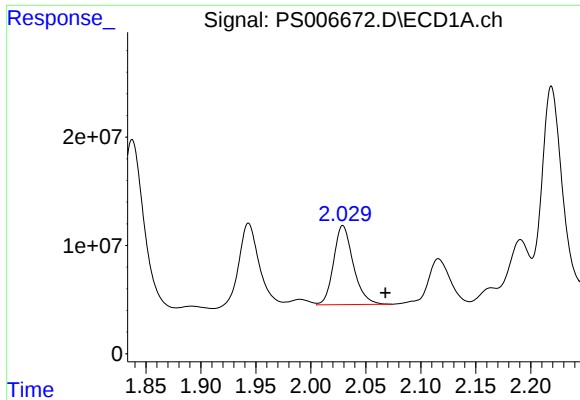

#1 Dalapon


R.T.: 2.029 min
Delta R.T.: -0.039 min
Response: 90793385
Conc: 92.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-2

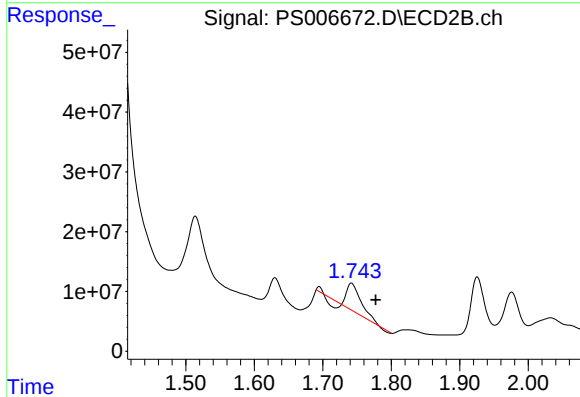


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.035 min
Response: 56219334
Conc: 110.01 ng/ml

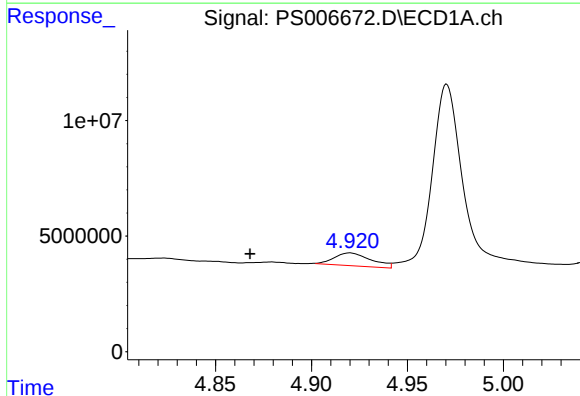


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.920 min
Delta R.T.: 0.052 min
Response: 7407696
Conc: 7.48 ng/ml

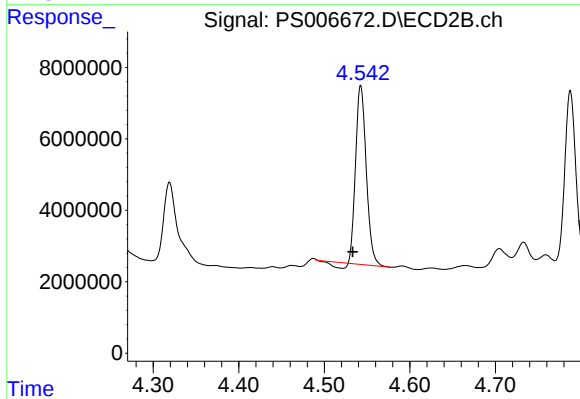

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.543 min
Delta R.T.: 0.009 min
Response: 42120553
Conc: 77.82 ng/ml

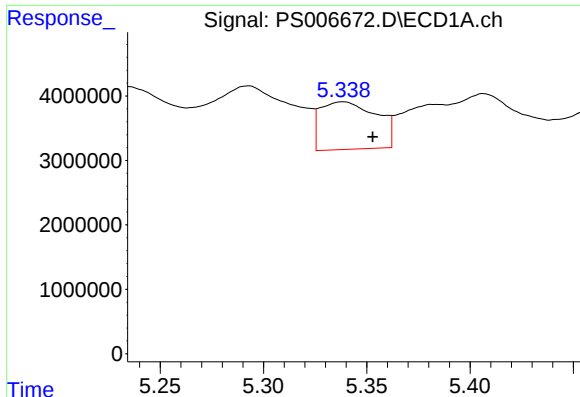

#3 4-Nitrophenol


R.T.: 5.338 min
Delta R.T.: -0.015 min
Response: 13976126
Conc: 39.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-2

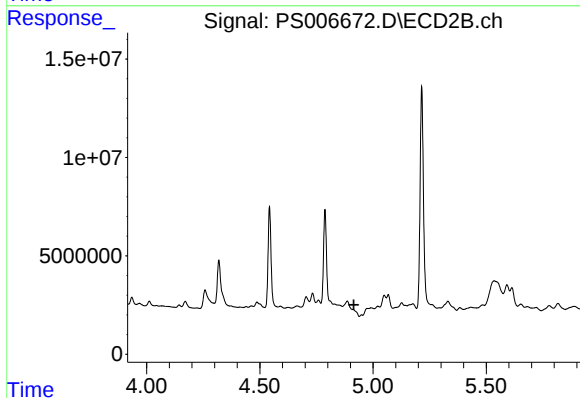


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

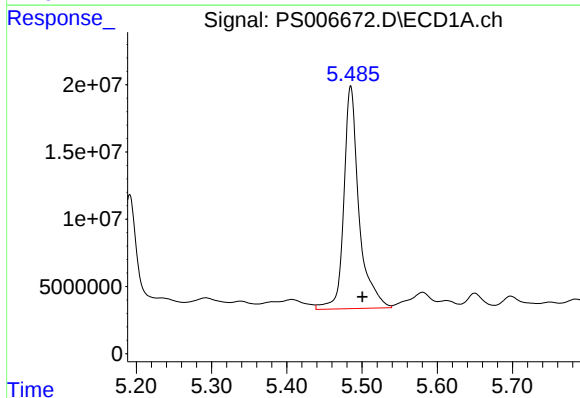


#4 2,4-DCAA

R.T.: 5.485 min
Delta R.T.: -0.016 min
Response: 231579340
Conc: 298.09 ng/ml

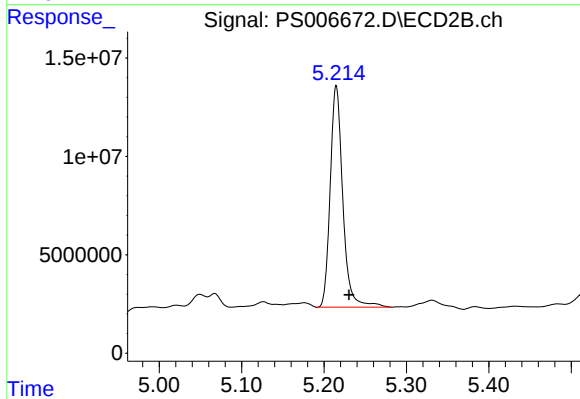

#4 2,4-DCAA


R.T.: 5.215 min
Delta R.T.: -0.015 min
Response: 119705228
Conc: 280.34 ng/ml

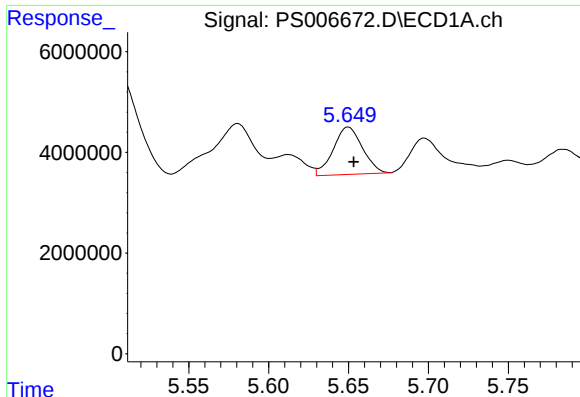

#5 DICAMBA


R.T.: 5.650 min
Delta R.T.: -0.003 min
Response: 11960969
Conc: 4.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-2

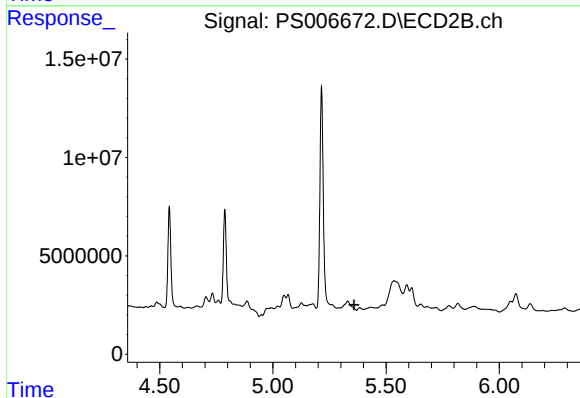


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

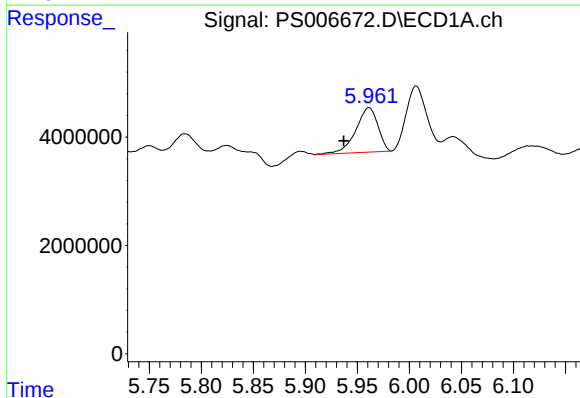


#7 MCPA

R.T.: 5.961 min
Delta R.T.: 0.024 min
Response: 12124585
Conc: 4.29 ug/ml

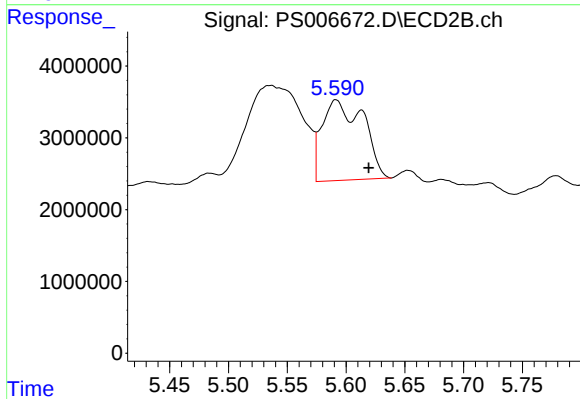

#7 MCPA


R.T.: 5.591 min
Delta R.T.: -0.028 min
Response: 27206870
Conc: 15.51 ug/ml

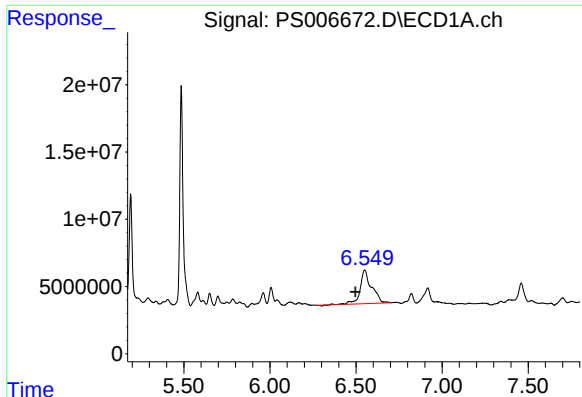

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.053 min
Response: 115033861
Conc: 148.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-2

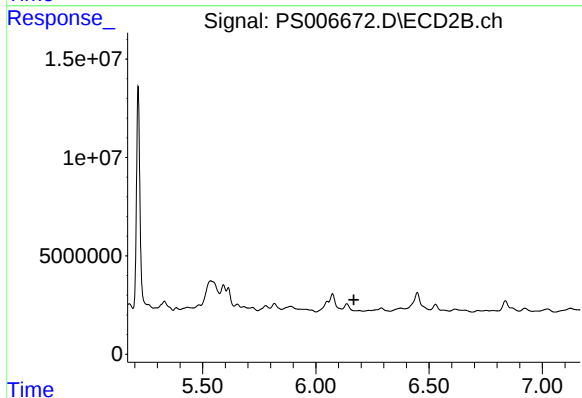


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

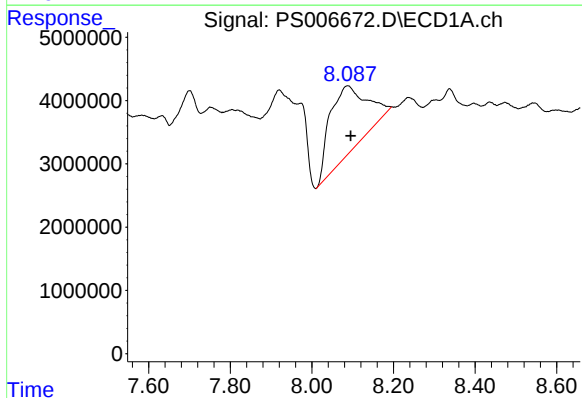


#13 2,4-DB

R.T.: 8.088 min
Delta R.T.: -0.007 min
Response: 67002922
Conc: 110.10 ng/ml

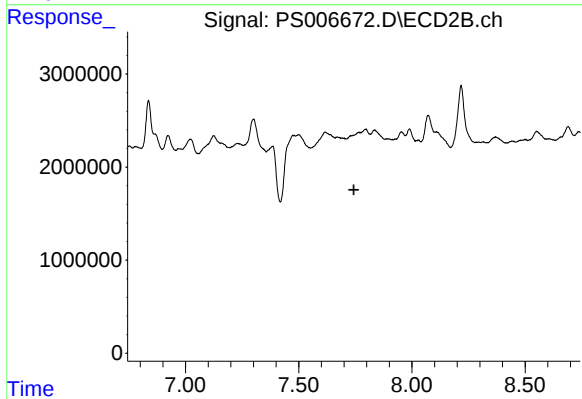

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

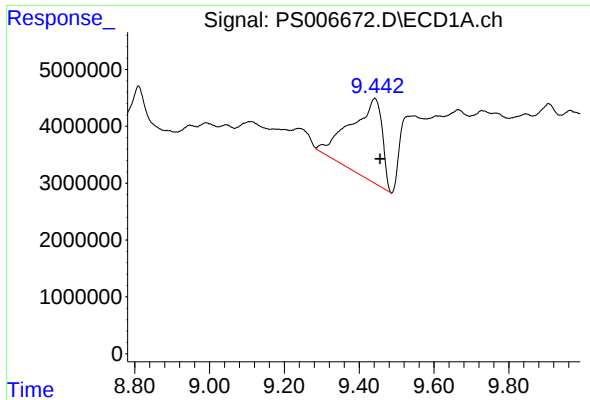

#16 DCPA

R.T.: 9.442 min
Delta R.T.: -0.014 min
Response: 84519675
Conc: 14.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-2

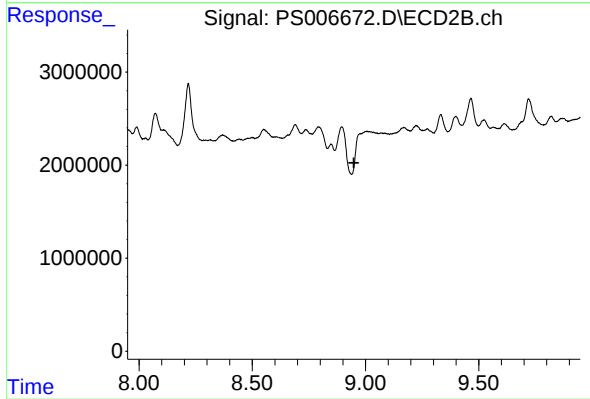

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.949 min
Response: 0
Conc: N.D.