

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091219\
 Data File : PS006673.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2019 14:10
 Operator : SM\AJ
 Sample : K4764-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ROLL-OFF-COMPOSITE-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 04:49:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.484	5.214	271.5E6	143.8E6	349.449	336.705
Target Compounds							
1) T	Dalapon	2.029	1.742	98695998	27823165	100.978	54.443 #
2) T	3,5-DICHL...	4.921	4.542	9863972	38848672	9.964	71.776 #
3) T	4-Nitroph...	5.338	0.000	16375791	0	46.146	N.D. #
5) T	DICAMBA	5.697	0.000	8436024	0	2.926	N.D. #
7) T	MCPA	5.959	5.612	7153158	12197548	2.531	6.954 #
9) T	2,4-D	6.549	0.000	89325385	0	115.613	N.D. #
10) T	Pentachlo...	6.787	0.000	8133735	0	<MDL	N.D. #
13) T	2,4-DB	8.087	0.000	65687859	0	107.941	N.D. #
16) T	DCPA	9.442	0.000	98632926	0	17.460	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091219\
Data File : PS006673.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2019 14:10
Operator : SM\AJ
Sample : K4764-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 04:49:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

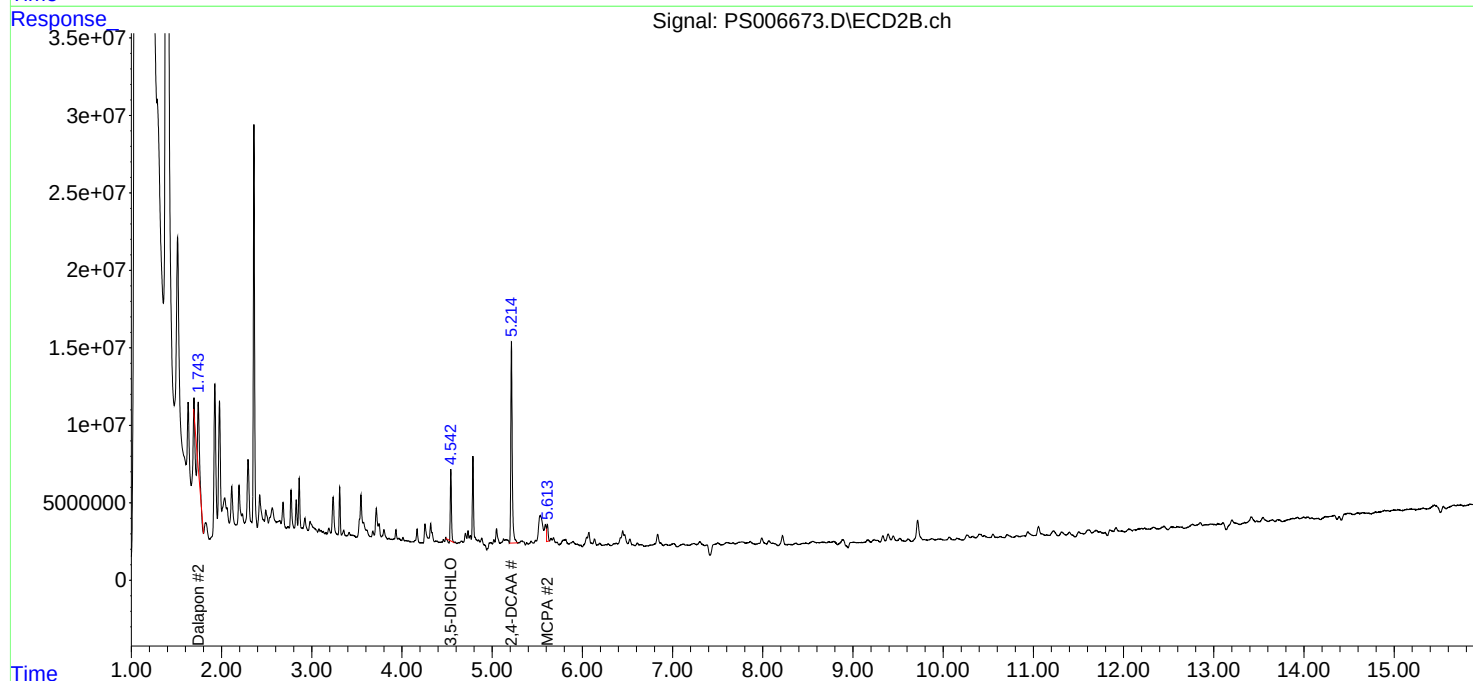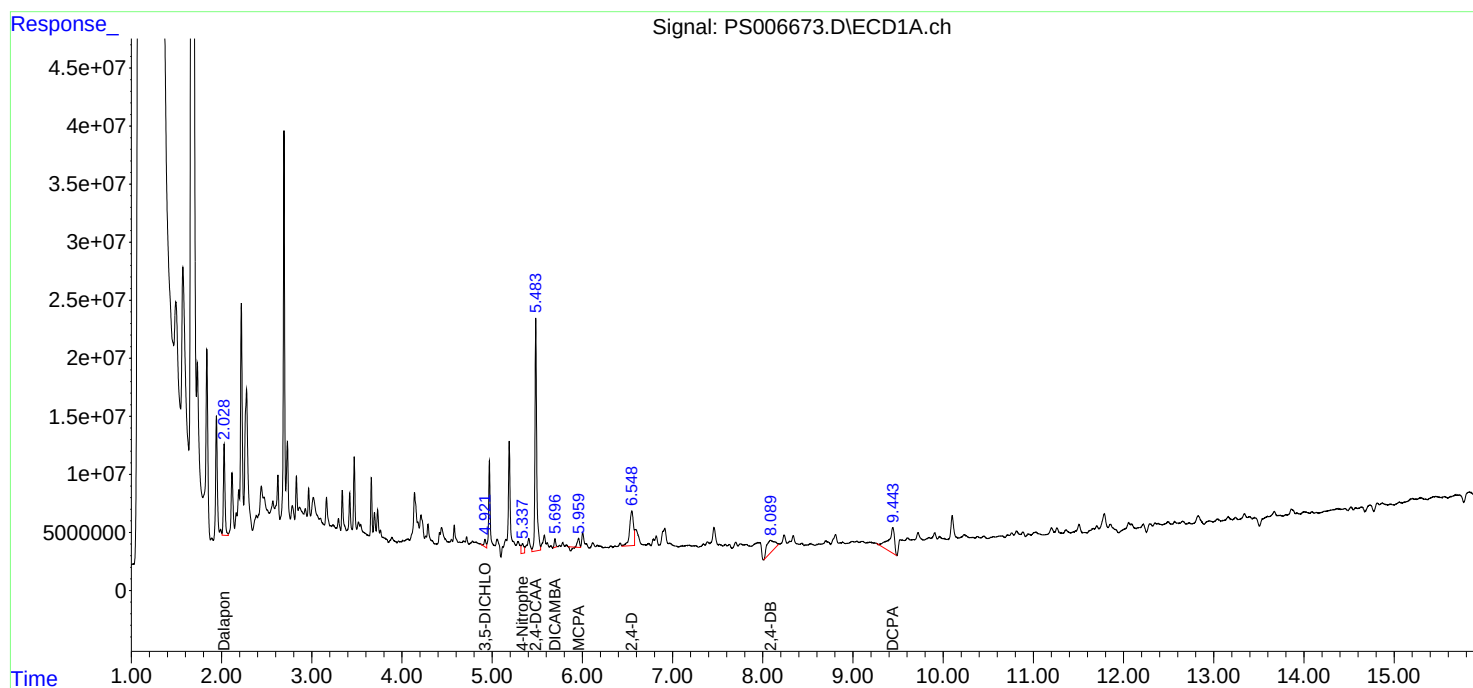


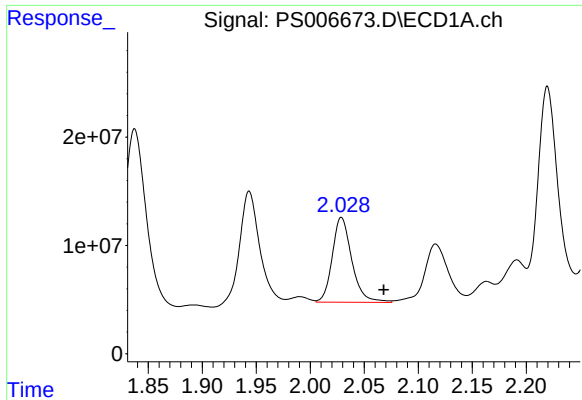

#1 Dalapon


R.T.: 2.029 min
Delta R.T.: -0.039 min
Response: 98695998
Conc: 100.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-3

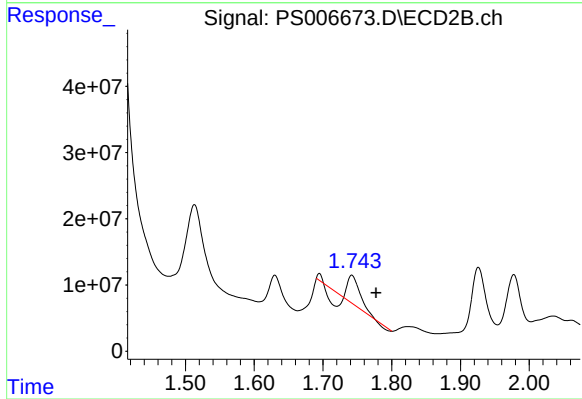


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.035 min
Response: 27823165
Conc: 54.44 ng/ml

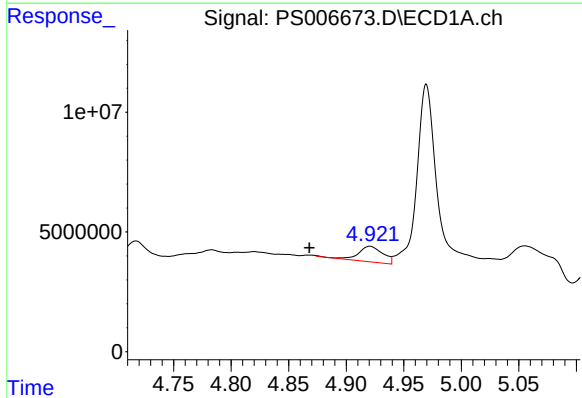


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.921 min
Delta R.T.: 0.053 min
Response: 9863972
Conc: 9.96 ng/ml

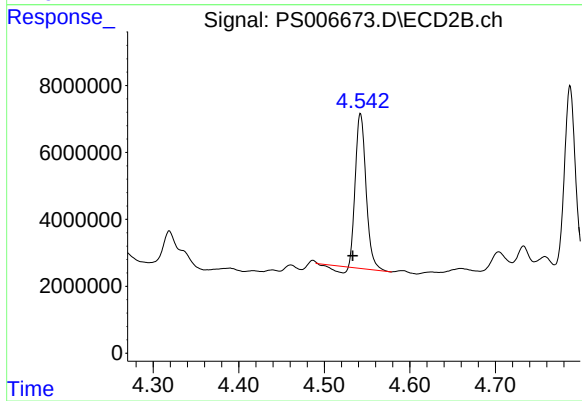

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.542 min
Delta R.T.: 0.009 min
Response: 38848672
Conc: 71.78 ng/ml

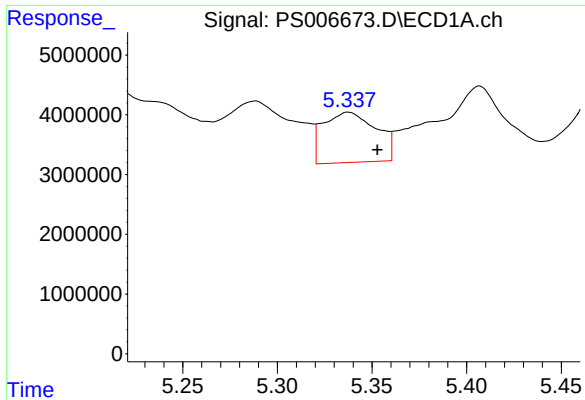

#3 4-Nitrophenol


R.T.: 5.338 min
Delta R.T.: -0.015 min
Response: 16375791
Conc: 46.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-3

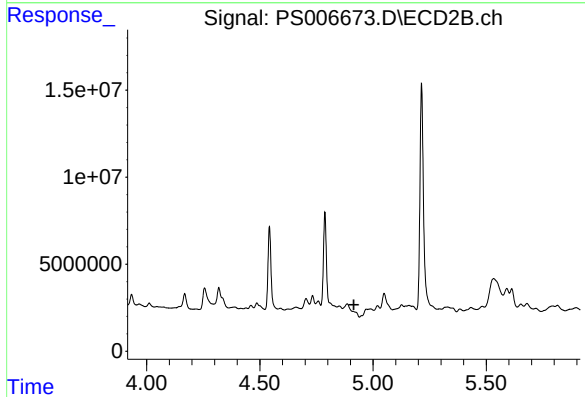


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

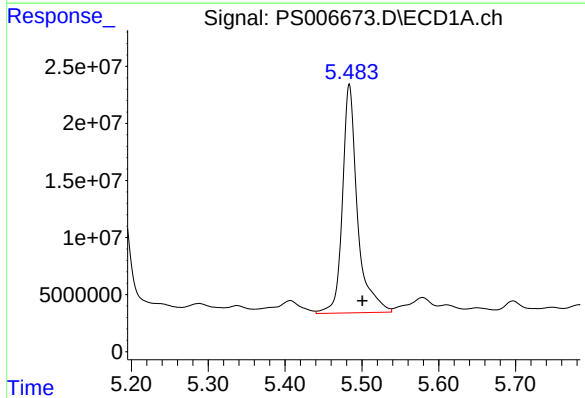


#4 2,4-DCAA

R.T.: 5.484 min
Delta R.T.: -0.017 min
Response: 271482167
Conc: 349.45 ng/ml

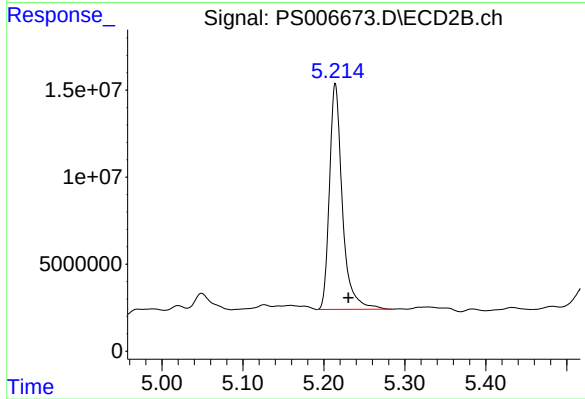

#4 2,4-DCAA


R.T.: 5.214 min
Delta R.T.: -0.016 min
Response: 143773983
Conc: 336.71 ng/ml

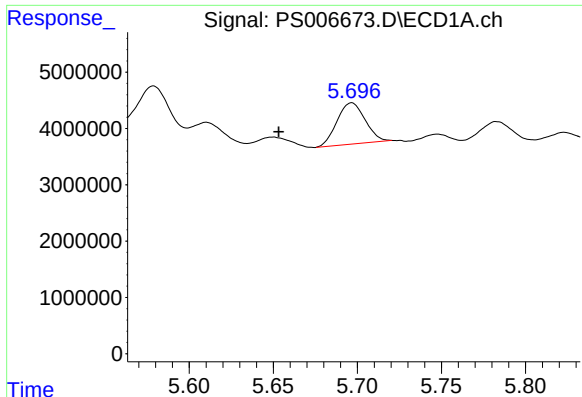

#5 DICAMBA


R.T.: 5.697 min
Delta R.T.: 0.043 min
Response: 8436024
Conc: 2.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-3

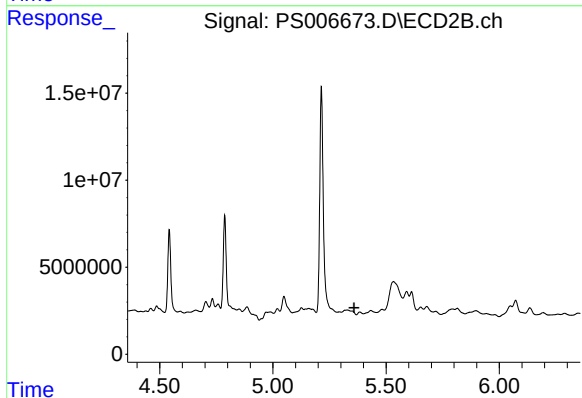


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

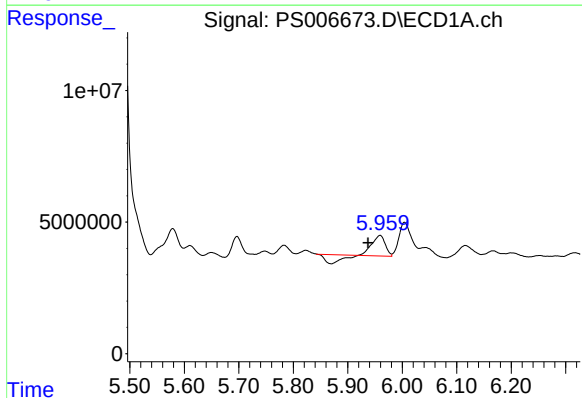


#7 MCPA

R.T.: 5.959 min
Delta R.T.: 0.022 min
Response: 7153158
Conc: 2.53 ug/ml

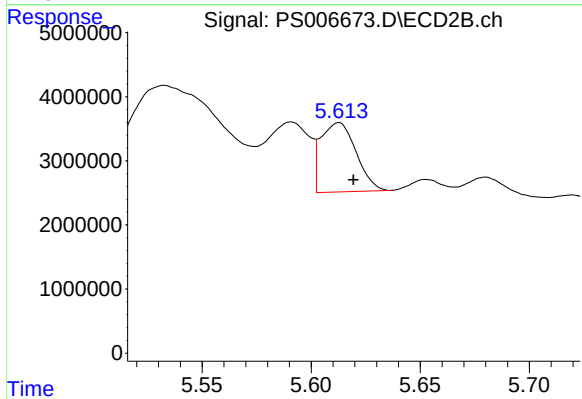

#7 MCPA


R.T.: 5.612 min
Delta R.T.: -0.007 min
Response: 12197548
Conc: 6.95 ug/ml

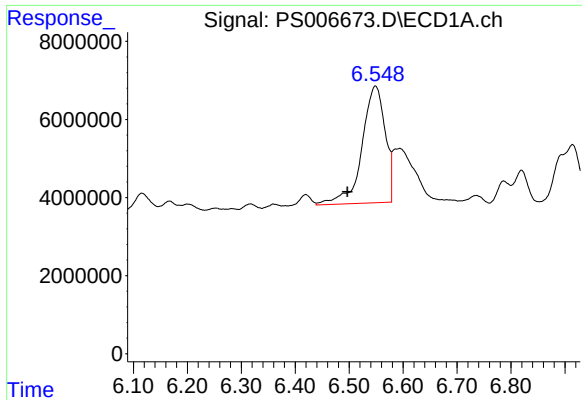

#9 2,4-D


R.T.: 6.549 min
Delta R.T.: 0.052 min
Response: 89325385
Conc: 115.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-3

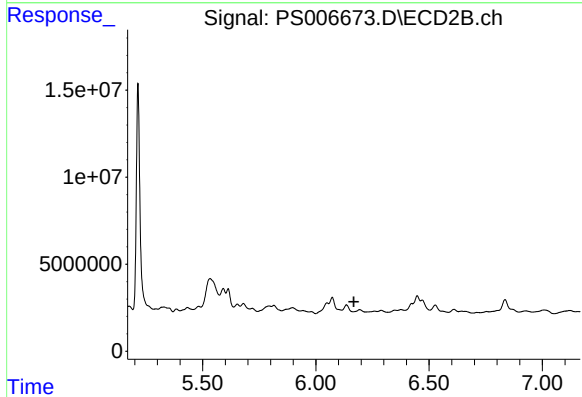


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

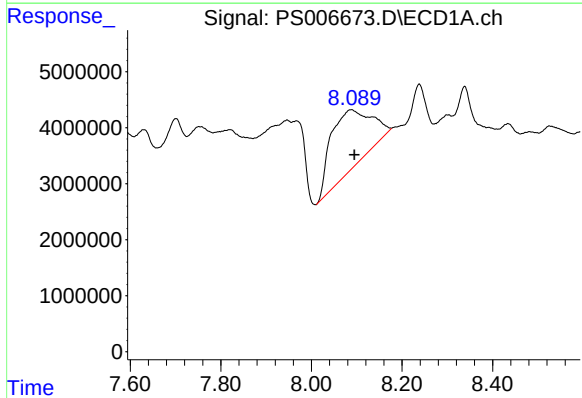


#13 2,4-DB

R.T.: 8.087 min
Delta R.T.: -0.008 min
Response: 65687859
Conc: 107.94 ng/ml

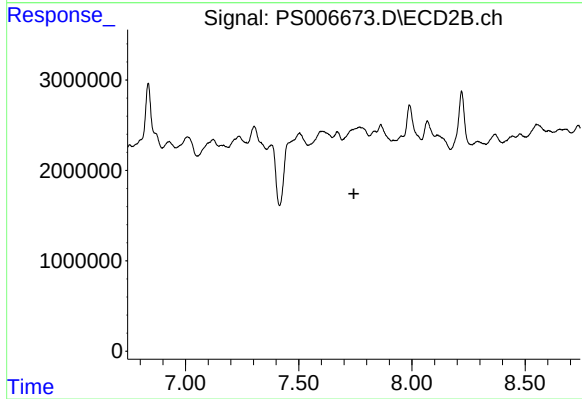

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

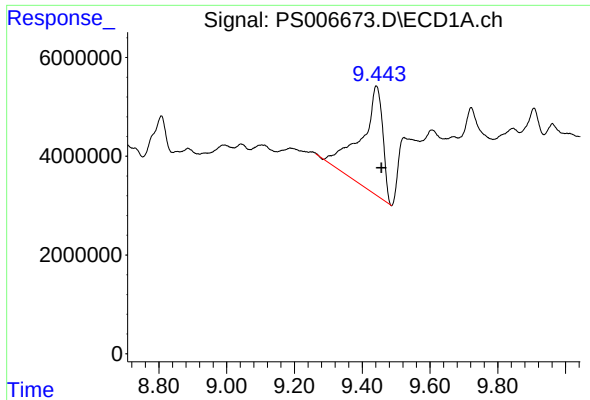

#16 DCPA

R.T.: 9.442 min
Delta R.T.: -0.014 min
Response: 98632926
Conc: 17.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLL-OFF-COMPOSITE-3

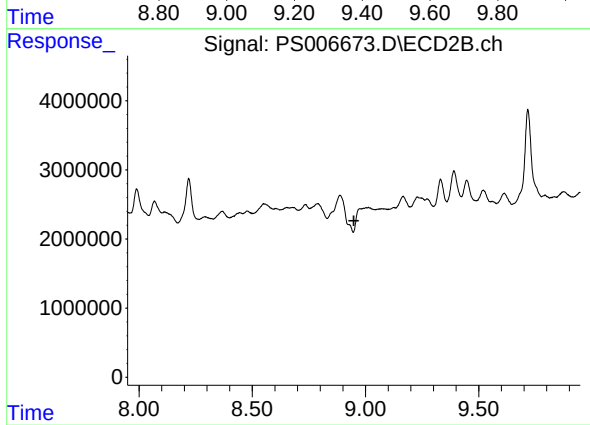

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.949 min
Response: 0
Conc: N.D.