

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091318\
 Data File : PS001731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2018 12:27
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 04:15:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.506	11.003	96339237	92685490	521.880	457.638
Target Compounds							
6) T	MCP	12.183	0.000	1717779	0	3.414	N.D. #
7) T	MCPA	0.000	11.806	0	3308108	N.D.	4.539 #
16) T	DCPA	0.000	16.939	0	2173822	N.D.	1.523 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091318\
Data File : PS001731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2018 12:27
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 04:15:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

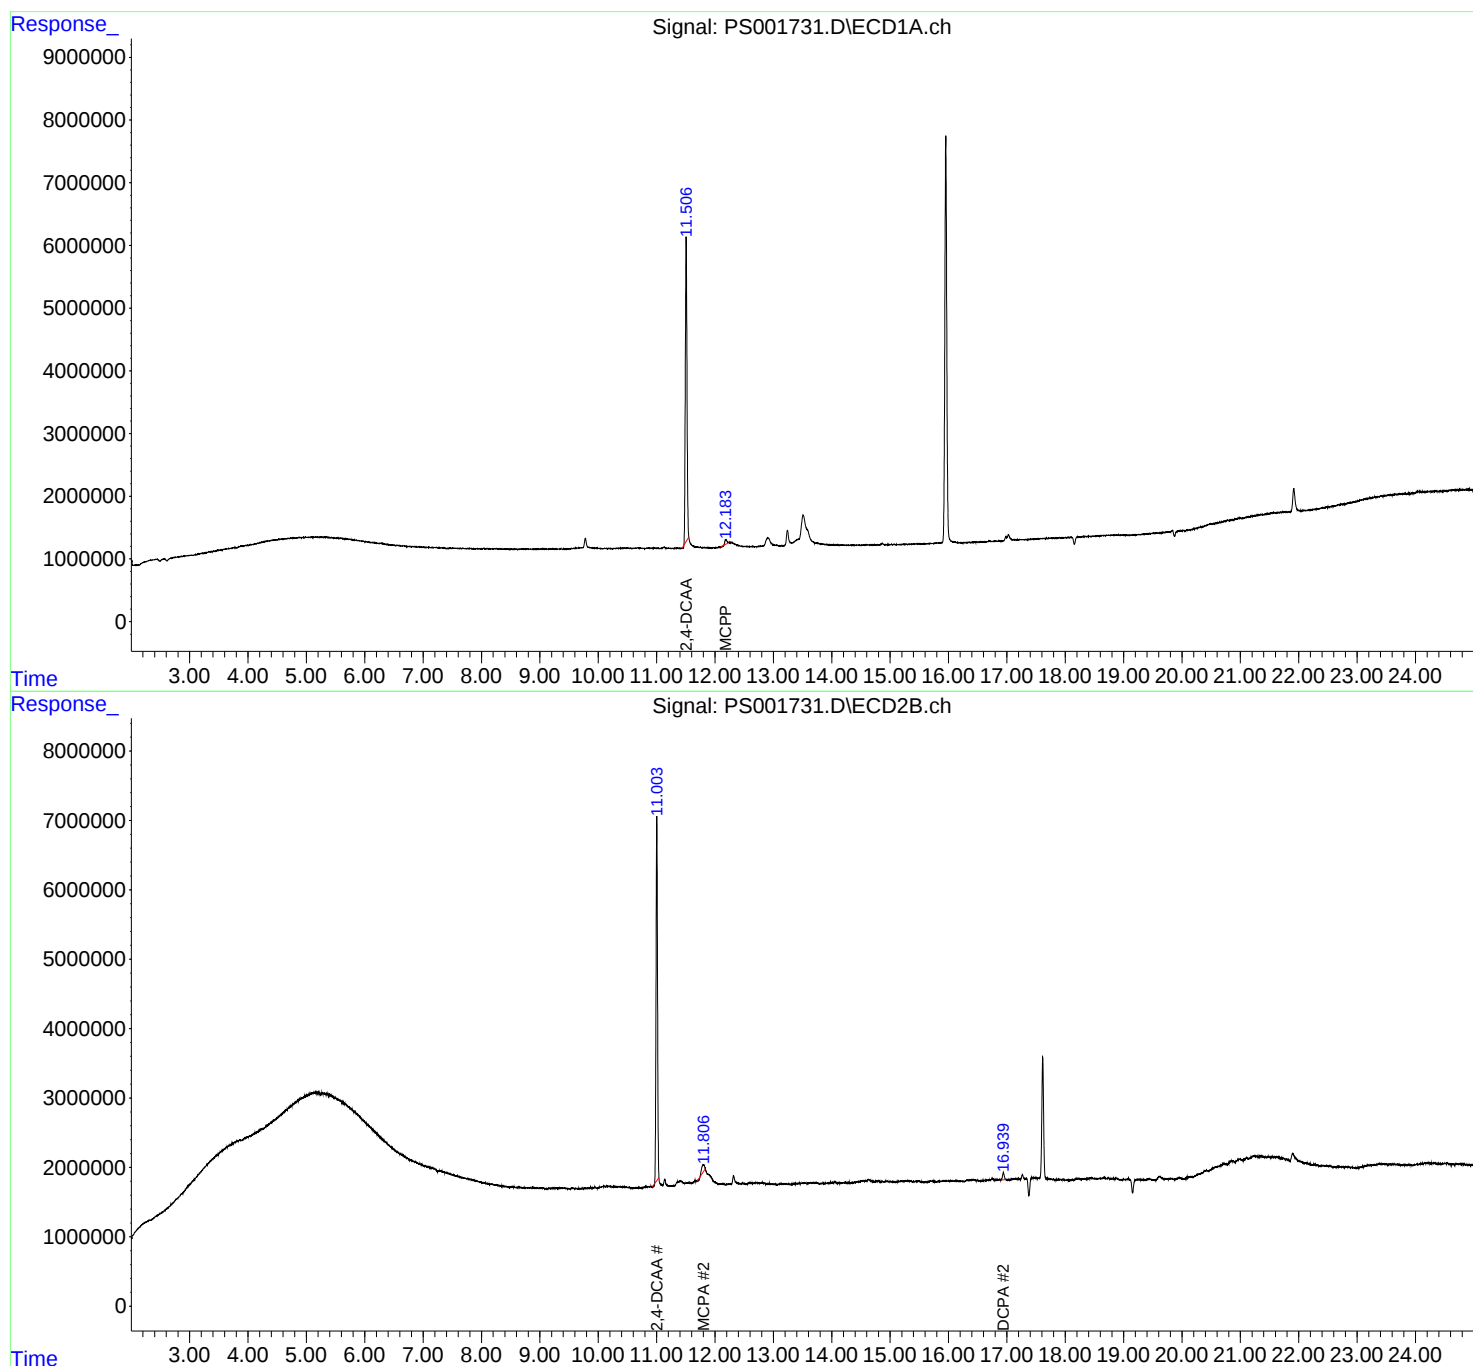


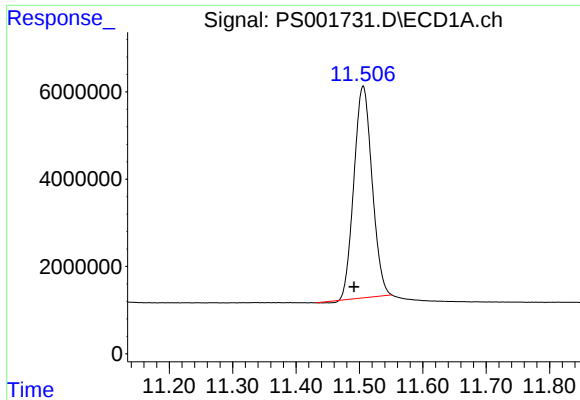

#4 2,4-DCAA


R.T.: 11.506 min
Delta R.T.: 0.014 min
Response: 96339237
Conc: 521.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

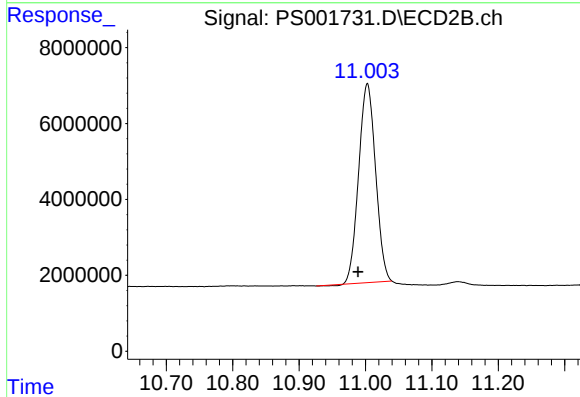


#4 2,4-DCAA

R.T.: 11.003 min
Delta R.T.: 0.014 min
Response: 92685490
Conc: 457.64 ng/ml

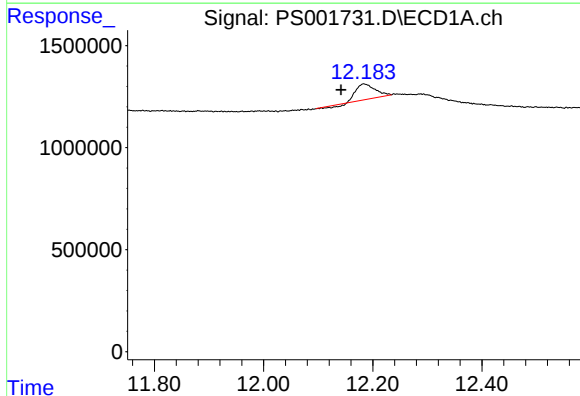


#6 MCP

R.T.: 12.183 min
Delta R.T.: 0.042 min
Response: 1717779
Conc: 3.41 ug/ml

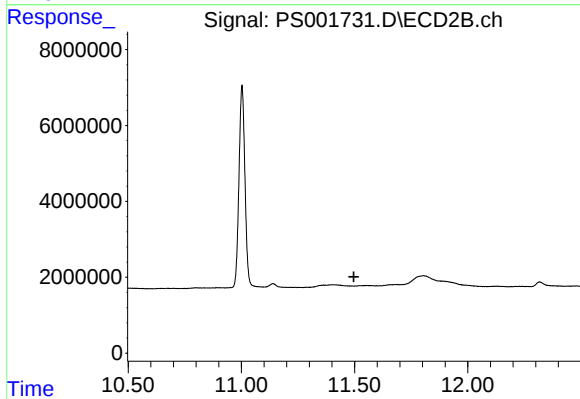

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

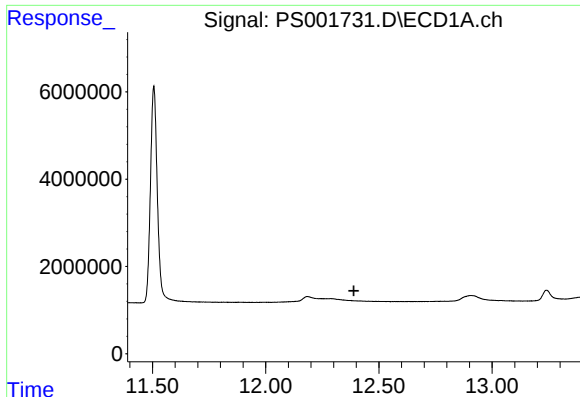

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

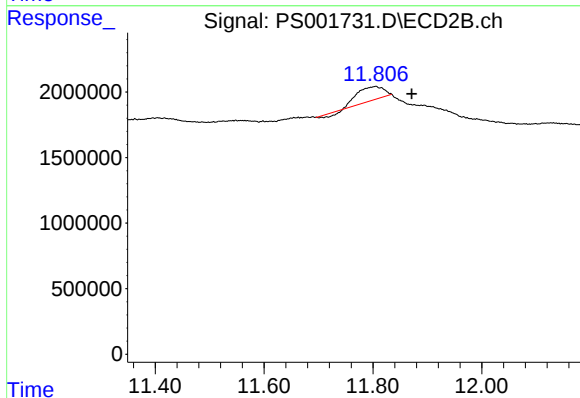


#7 MCPA

R.T.: 11.806 min
Delta R.T.: -0.066 min
Response: 3308108
Conc: 4.54 ug/ml

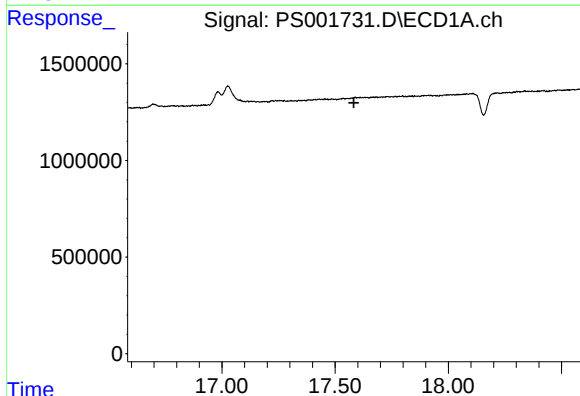

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

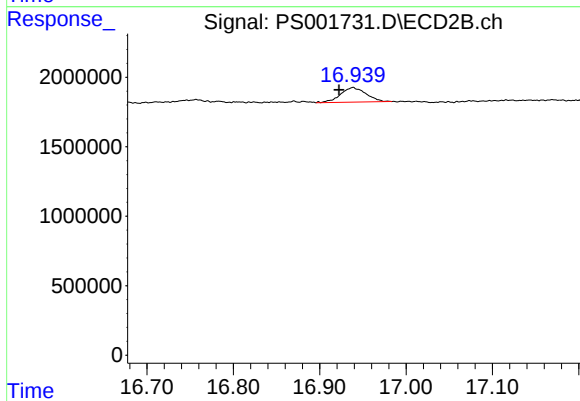

#16 DCPA

R.T.: 16.939 min
Delta R.T.: 0.016 min
Response: 2173822
Conc: 1.52 ng/ml