

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091319\
 Data File : PS006700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2019 10:32
 Operator : SM\AJ
 Sample : PB123030BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB123030BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 13:24:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.499	5.223	582.7E6	320.9E6	750.059	751.563
Target Compounds							
1) T	Dalapon	2.041	1.751	153.5E6	67329342	157.022	131.747
2) T	3,5-DICHL...	0.000	4.551	0	31985765	N.D.	59.096
3) T	4-Nitroph...	5.352	0.000	4193632	0	11.817	N.D. #
5) T	DICAMBA	5.592	0.000	17161793	0	5.953	N.D. #
7) T	MCPA	5.915	0.000	2704520	0	<MDL	N.D. #
8) T	DICHLORPROP	6.310	0.000	31547598	0	44.360	N.D. #
9) T	2,4-D	6.438	0.000	20990160	0	27.167	N.D. #
15) T	Picloram	9.055	9.004	59488063	34075871	8.819	9.208
16) T	DCPA	0.000	9.004	0	34075871	N.D.	10.817



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091319\
Data File : PS006700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2019 10:32
Operator : SM\AJ
Sample : PB123030BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB123030BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 13:24:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

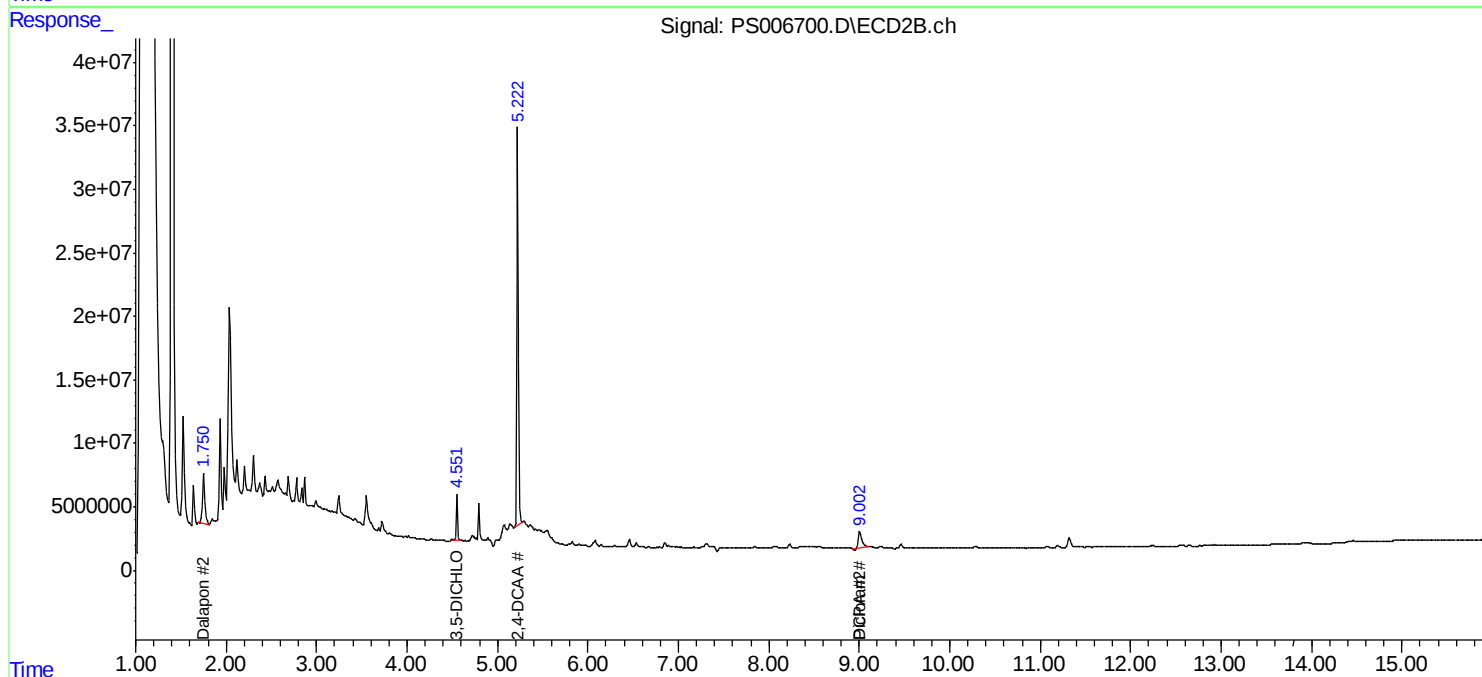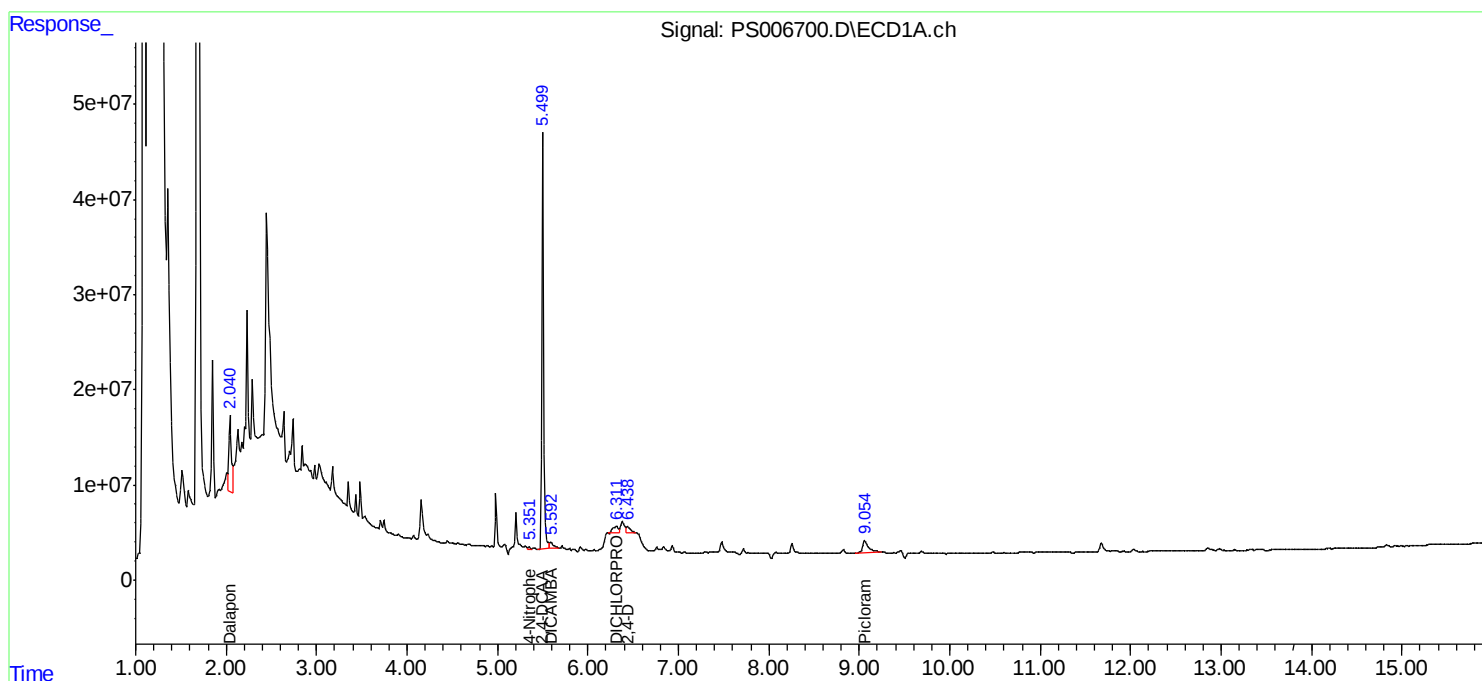


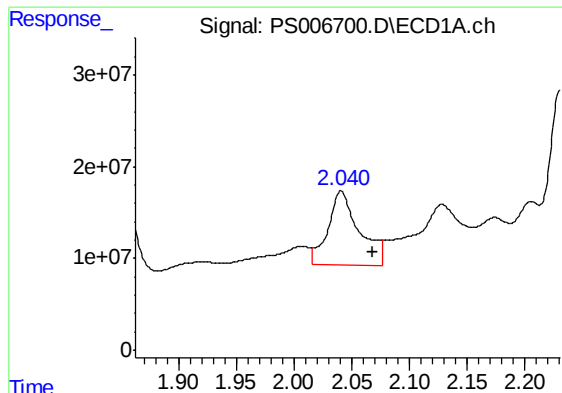

#1 Dalapon


R.T.: 2.041 min
Delta R.T.: -0.027 min
Response: 153473597
Conc: 157.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123030BL

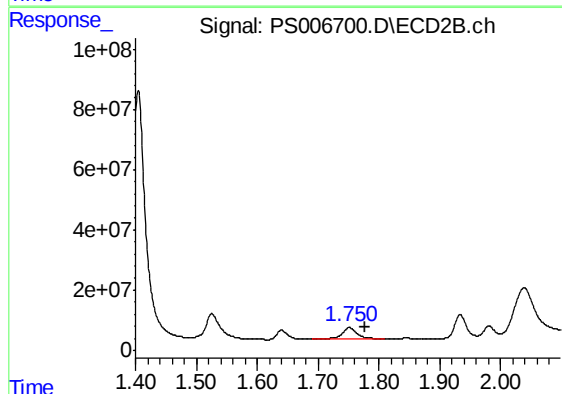


#1 Dalapon

R.T.: 1.751 min
Delta R.T.: -0.027 min
Response: 67329342
Conc: 131.75 ng/ml

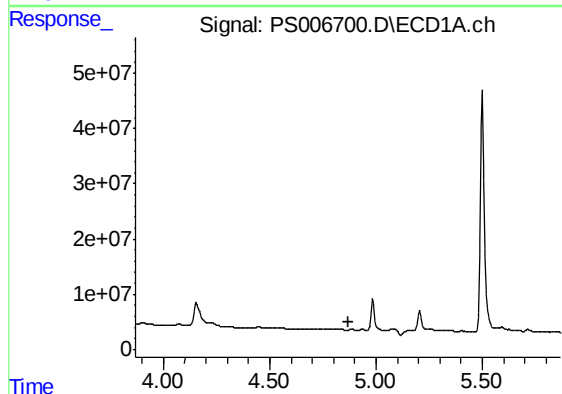


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

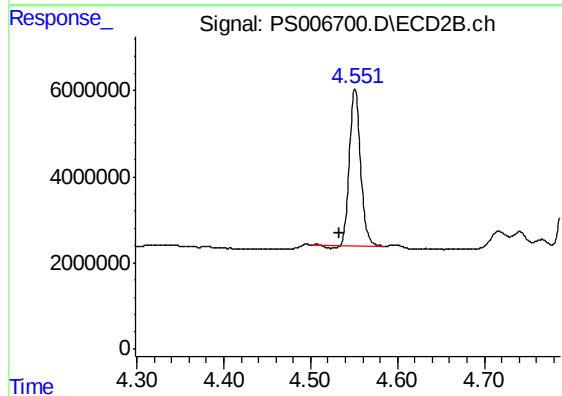

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.551 min
Delta R.T.: 0.018 min
Response: 31985765
Conc: 59.10 ng/ml

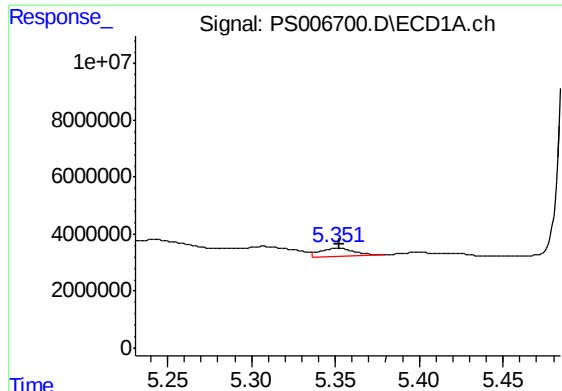

#3 4-Nitrophenol


R.T.: 5.352 min
Delta R.T.: -0.001 min
Response: 4193632
Conc: 11.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123030BL

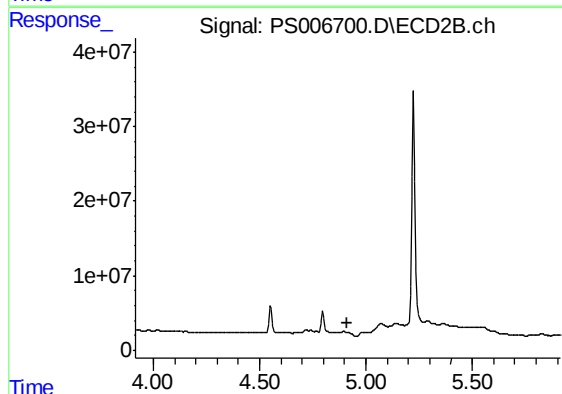


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

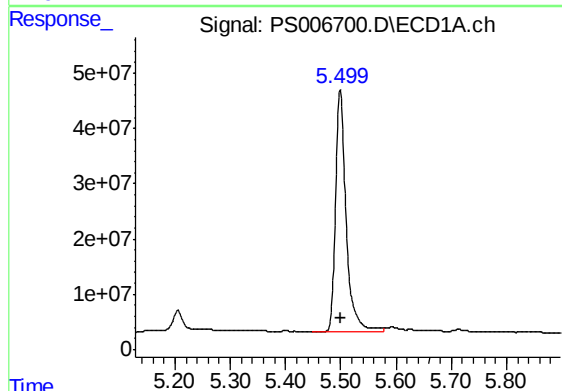


#4 2,4-DCAA

R.T.: 5.499 min
Delta R.T.: -0.002 min
Response: 582709784
Conc: 750.06 ng/ml

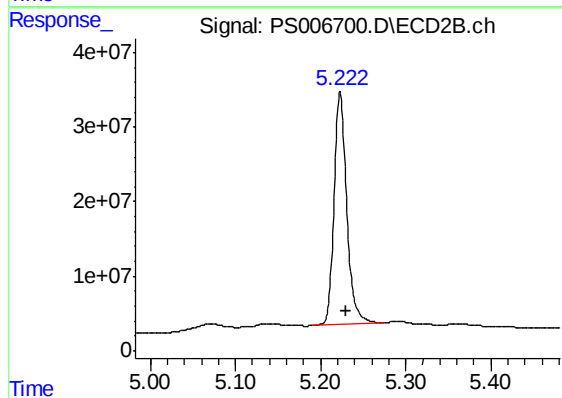

#4 2,4-DCAA


R.T.: 5.223 min
Delta R.T.: -0.007 min
Response: 320919450
Conc: 751.56 ng/ml

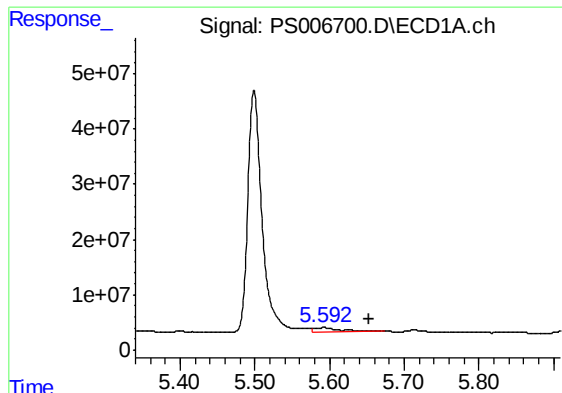

#5 DICAMBA


R.T.: 5.592 min
Delta R.T.: -0.061 min
Response: 17161793
Conc: 5.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123030BL

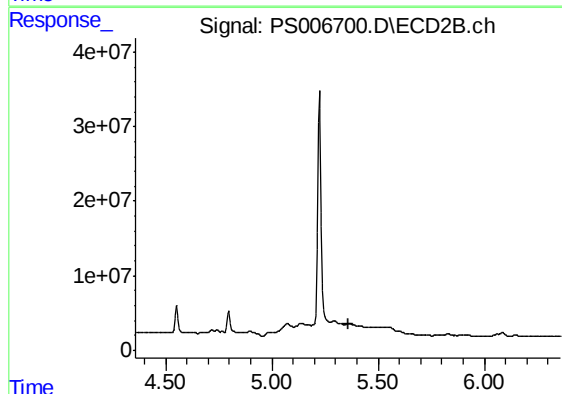


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

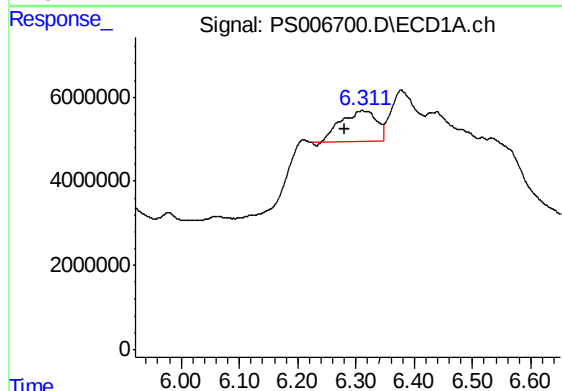


#8 DICHLORPROP

R.T.: 6.310 min
Delta R.T.: 0.028 min
Response: 31547598
Conc: 44.36 ng/ml

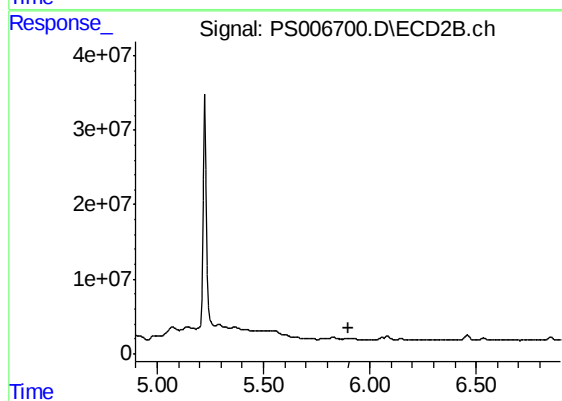

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 5.897 min
Response: 0
Conc: N.D.

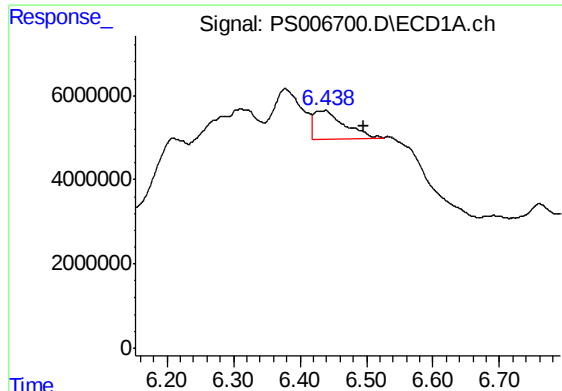

#9 2,4-D


R.T.: 6.438 min
Delta R.T.: -0.059 min
Response: 20990160
Conc: 27.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123030BL

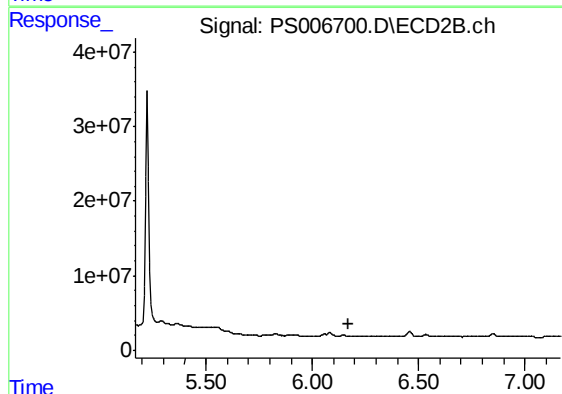


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

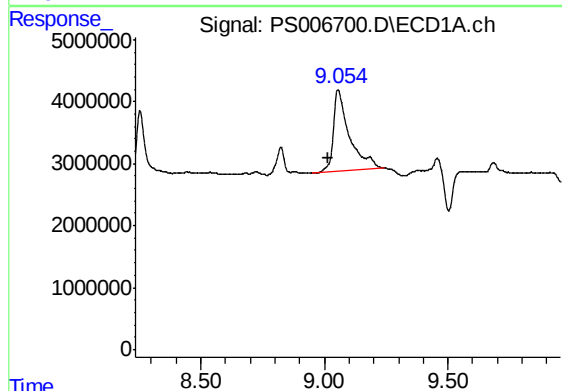


#15 Picloram

R.T.: 9.055 min
Delta R.T.: 0.038 min
Response: 59488063
Conc: 8.82 ng/ml

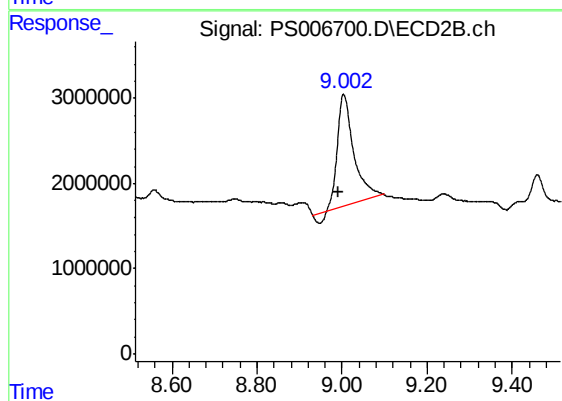

#15 Picloram


R.T.: 9.004 min
Delta R.T.: 0.013 min
Response: 34075871
Conc: 9.21 ng/ml

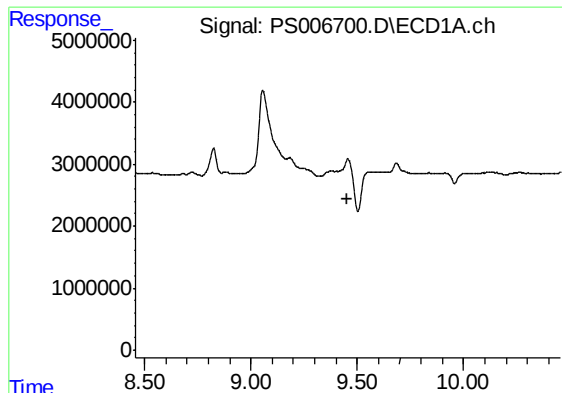

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB123030BL

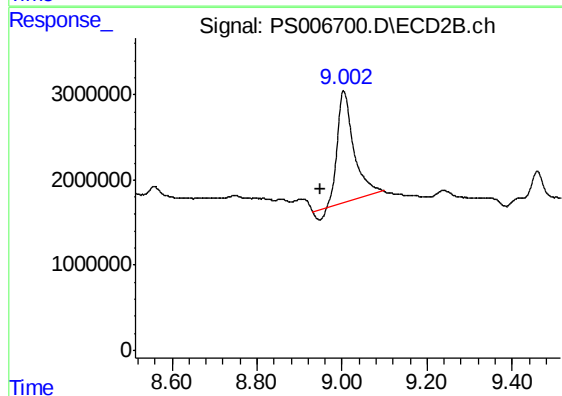

#16 DCPA

R.T.: 9.004 min
Delta R.T.: 0.055 min
Response: 34075871
Conc: 10.82 ng/ml