

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091319\
 Data File : PS006711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2019 18:41
 Operator : SM\AJ
 Sample : K4852-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 23:46:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	5.476	0.000	58882594	0	75.793	N.D.	#
Target Compounds								
3) T	4-Nitroph...	5.296	0.000	70641272	0	199.062	N.D.	#
5) T	DICAMBA	5.665	5.320	5527995	788351	1.917	<MDL	#
7) T	MCPA	0.000	5.670	0	19944952	N.D.	11.371	
9) T	2,4-D	6.498	0.000	8894752	0	11.512	N.D.	#
11) T	2,4,5-TP ...	7.337	0.000	6063882	0	1.409	N.D.	#
12) T	2,4,5-T	7.574	0.000	39826110	0	8.547	N.D.	#
13) T	2,4-DB	8.081	0.000	81944299	0	134.654	N.D.	#
16) T	DCPA	9.468	0.000	19393256	0	3.433	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091319\
Data File : PS006711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2019 18:41
Operator : SM\AJ
Sample : K4852-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 23:46:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

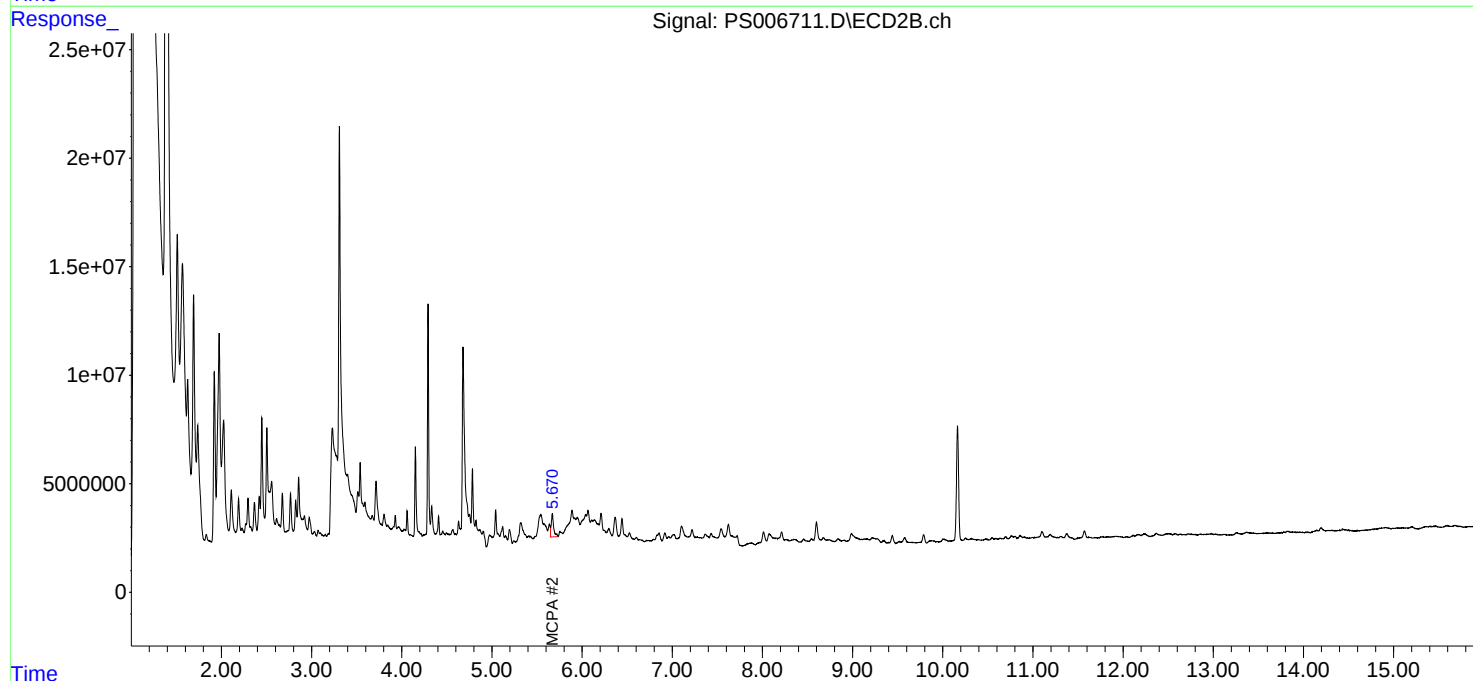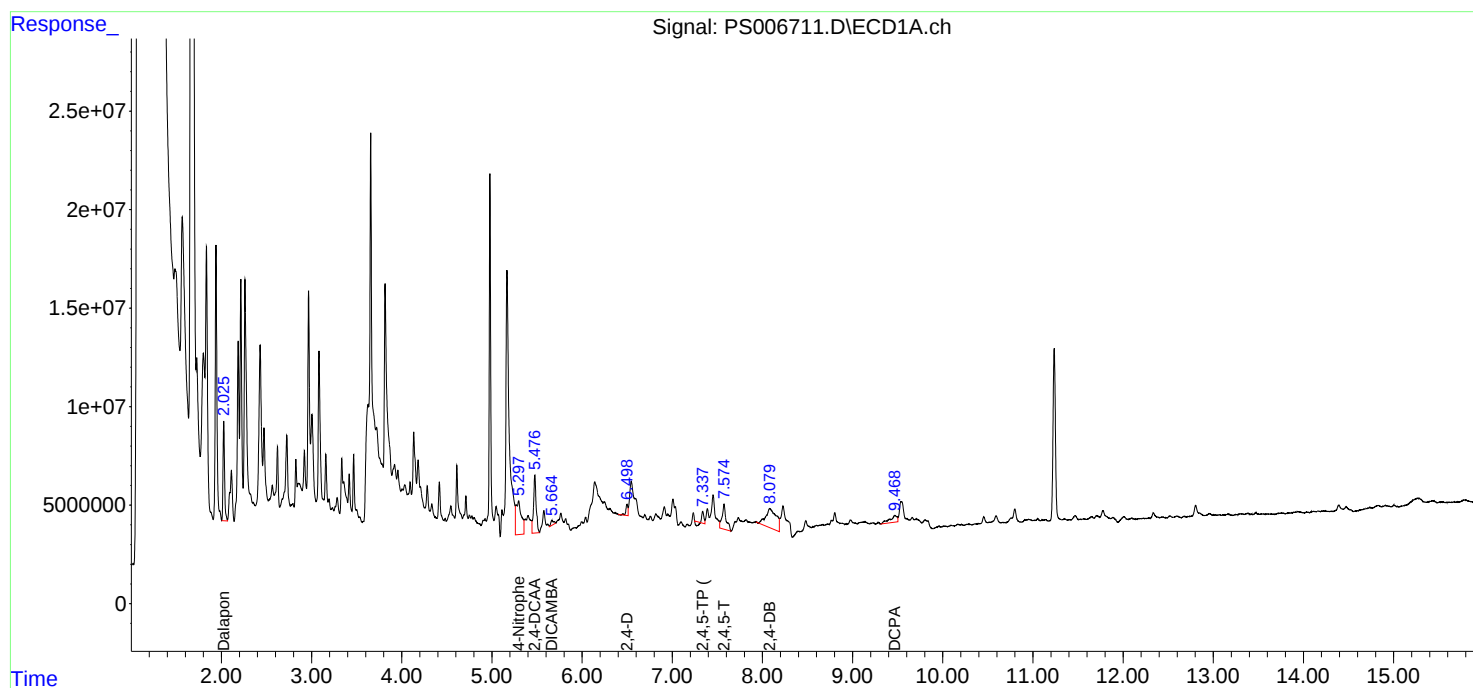


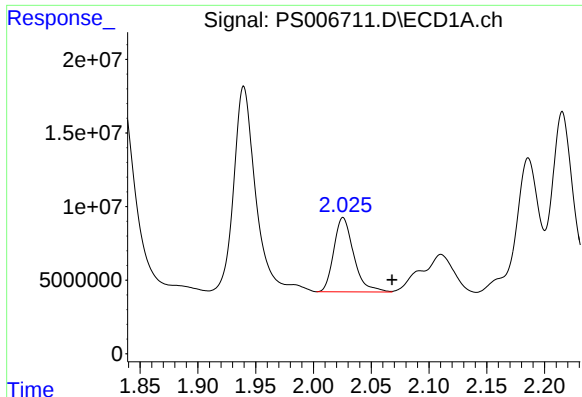

#1 Dalapon


R.T.: 2.026 min
Delta R.T.: -0.042 min
Response: 60379865
Conc: 61.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

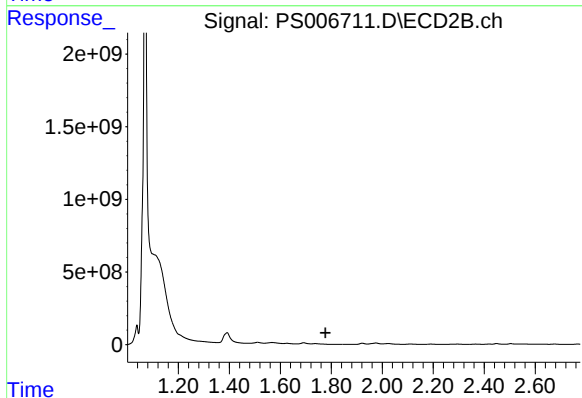


#1 Dalapon

R.T.: 1.737 min
Delta R.T.: -0.040 min
Response: -137381751
Conc: N.D.

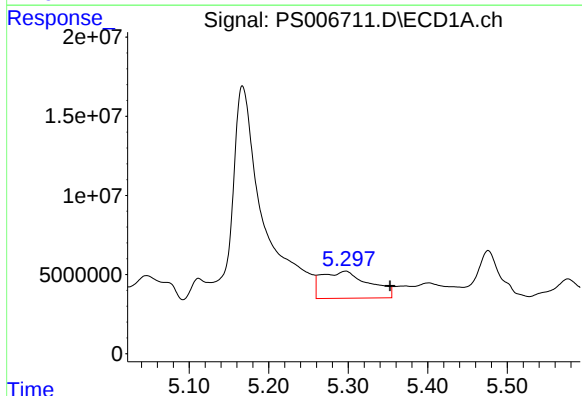


#3 4-Nitrophenol

R.T.: 5.296 min
Delta R.T.: -0.056 min
Response: 70641272
Conc: 199.06 ng/ml

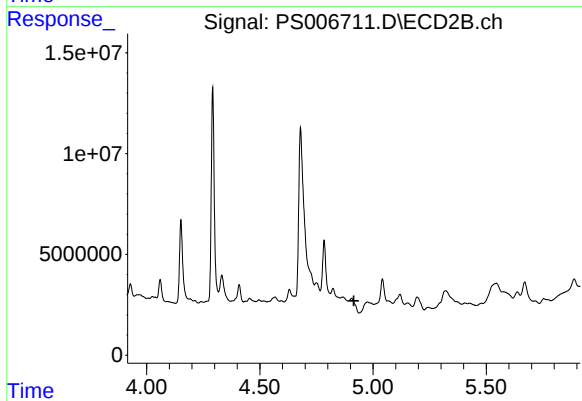

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

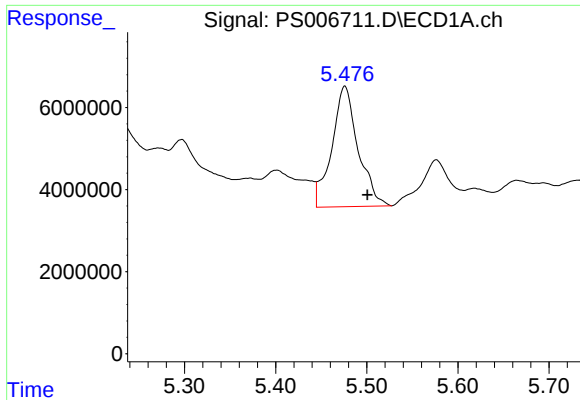

#4 2,4-DCAA


R.T.: 5.476 min
Delta R.T.: -0.025 min
Response: 58882594
Conc: 75.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

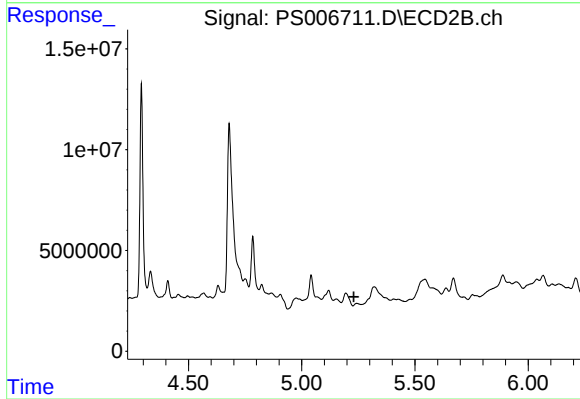


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.230 min
Response: 0
Conc: N.D.

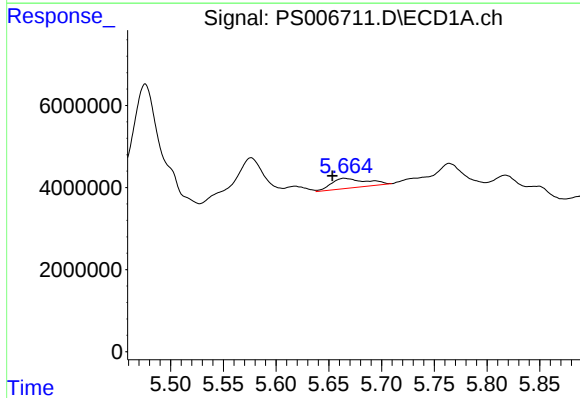


#5 DICAMBA

R.T.: 5.665 min
Delta R.T.: 0.012 min
Response: 5527995
Conc: 1.92 ng/ml

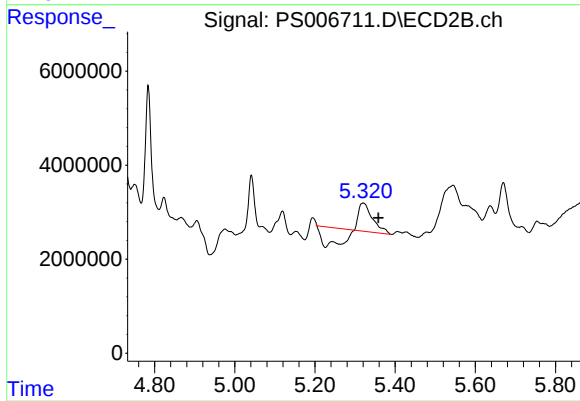

#5 DICAMBA


R.T.: 5.320 min
Delta R.T.: -0.038 min
Response: 788351
Conc: N.D.

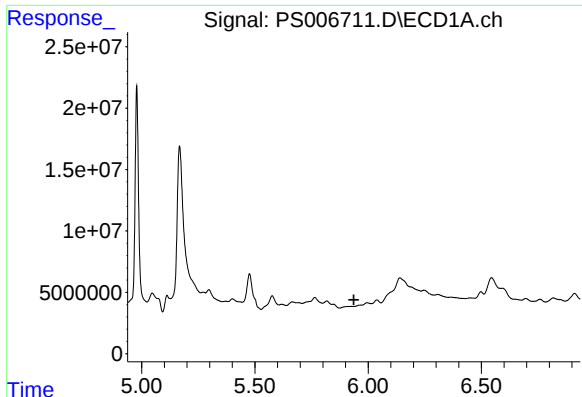

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

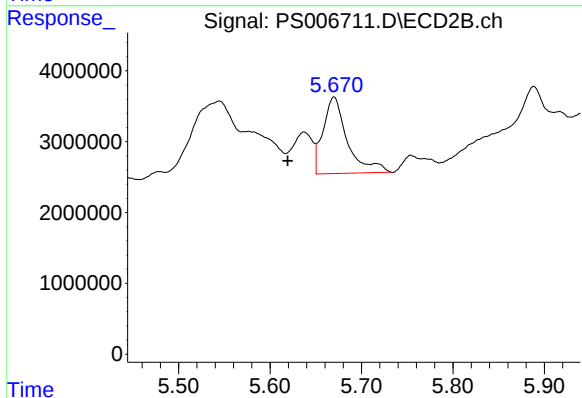


#7 MCPA

R.T.: 5.670 min
Delta R.T.: 0.051 min
Response: 19944952
Conc: 11.37 ug/ml

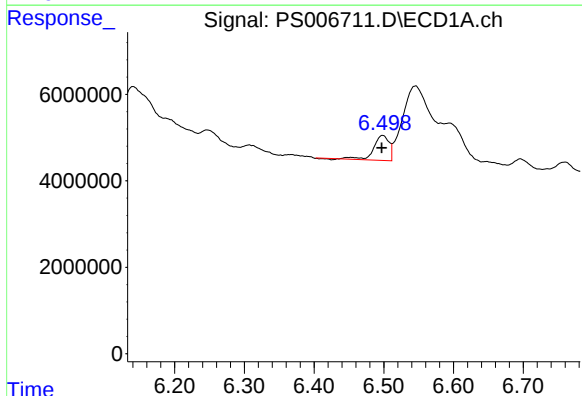


#9 2,4-D

R.T.: 6.498 min
Delta R.T.: 0.001 min
Response: 8894752
Conc: 11.51 ng/ml

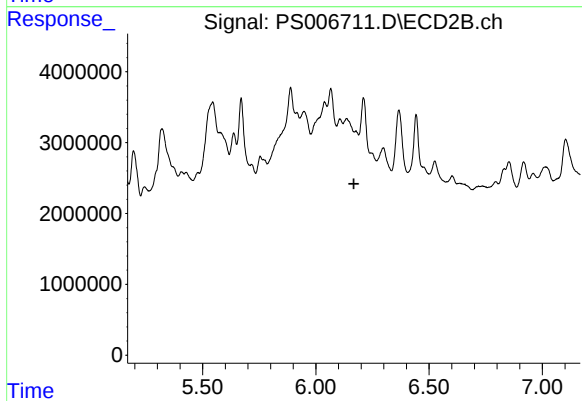

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.168 min
Response: 0
Conc: N.D.

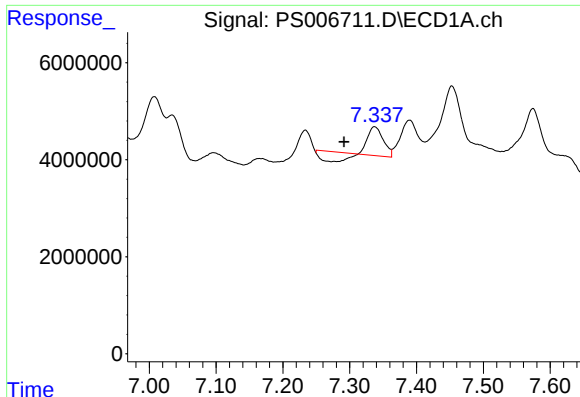

#11 2,4,5-TP (SILVEX)


R.T.: 7.337 min
Delta R.T.: 0.046 min
Response: 6063882
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

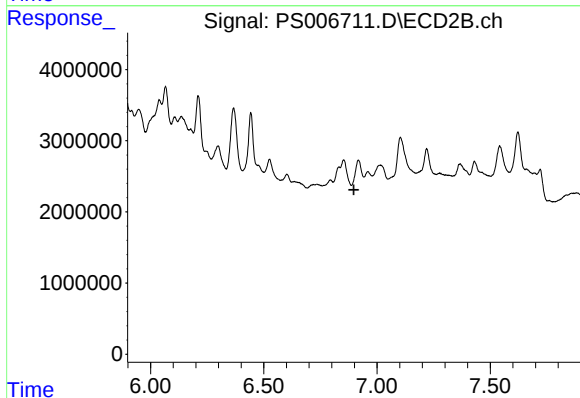


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 6.898 min
Response: 0
Conc: N.D.

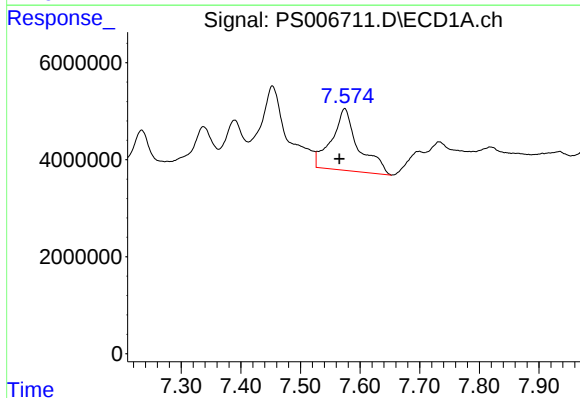


#12 2,4,5-T

R.T.: 7.574 min
Delta R.T.: 0.009 min
Response: 39826110
Conc: 8.55 ng/ml

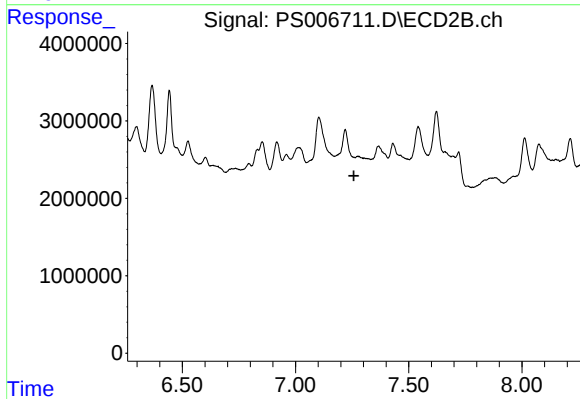

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 7.258 min
Response: 0
Conc: N.D.

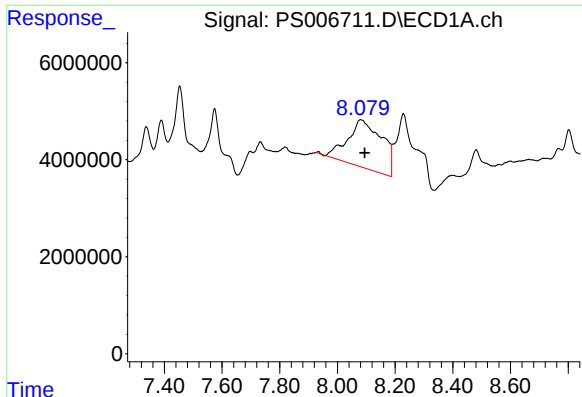

#13 2,4-DB


R.T.: 8.081 min
Delta R.T.: -0.014 min
Response: 81944299
Conc: 134.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

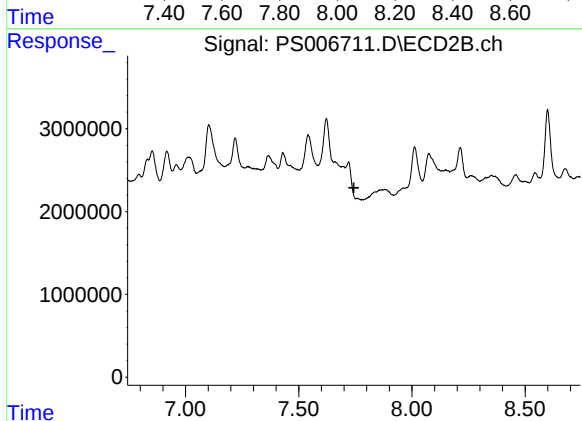


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

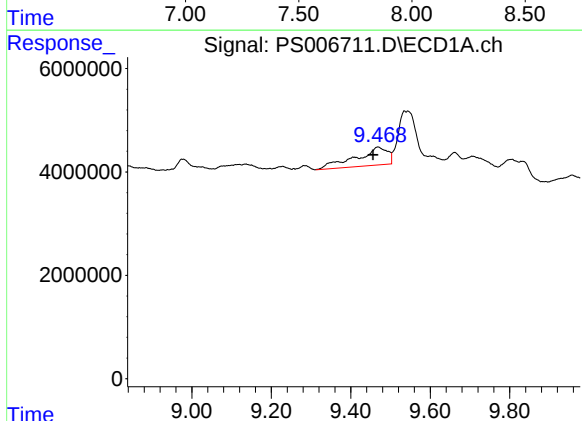

#16 DCPA

R.T.: 9.468 min
Delta R.T.: 0.012 min
Response: 19393256
Conc: 3.43 ng/ml

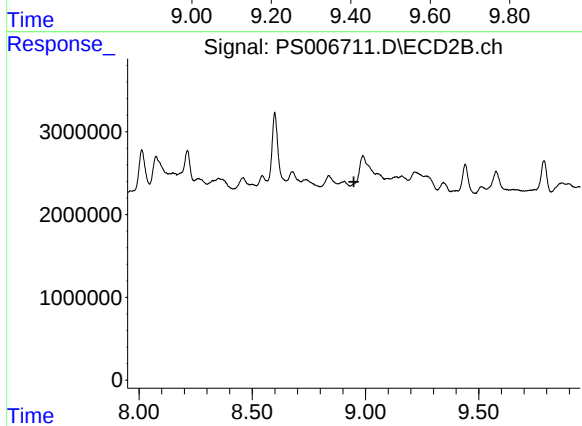

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.949 min
Response: 0
Conc: N.D.