

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091319\
 Data File : PS006712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2019 19:03
 Operator : SM\AJ
 Sample : K4852-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 GIS-4(0-4)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 23:46:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	5.463	0.000	111.1E6	0	142.976	N.D.	#
Target Compounds								
1) T	Dalapon	2.098	1.724	159.7E6	-30345554	163.405	N.D.	#
2) T	3,5-DICHL...	4.906	0.000	9031821	0	9.123	N.D.	#
3) T	4-Nitroph...	5.346	4.976	15475322	9769727	43.608	44.137	
5) T	DICAMBA	5.616	0.000	8512502	0	2.953	N.D.	#
7) T	MCPA	5.883	0.000	618988	0	<MDL	N.D.	#
9) T	2,4-D	6.532	0.000	79718225	0	103.179	N.D.	#
10) T	Pentachlo...	6.803	0.000	16056358	0	1.441	N.D.	#
13) T	2,4-DB	8.095	0.000	14396783	0	23.657	N.D.	#
15) T	Picloram	8.962	0.000	6046227	0	<MDL	N.D.	#
16) T	DCPA	9.432	0.000	14399130	0	2.549	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091319\
Data File : PS006712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2019 19:03
Operator : SM\AJ
Sample : K4852-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
GIS-4(0-4)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 23:46:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

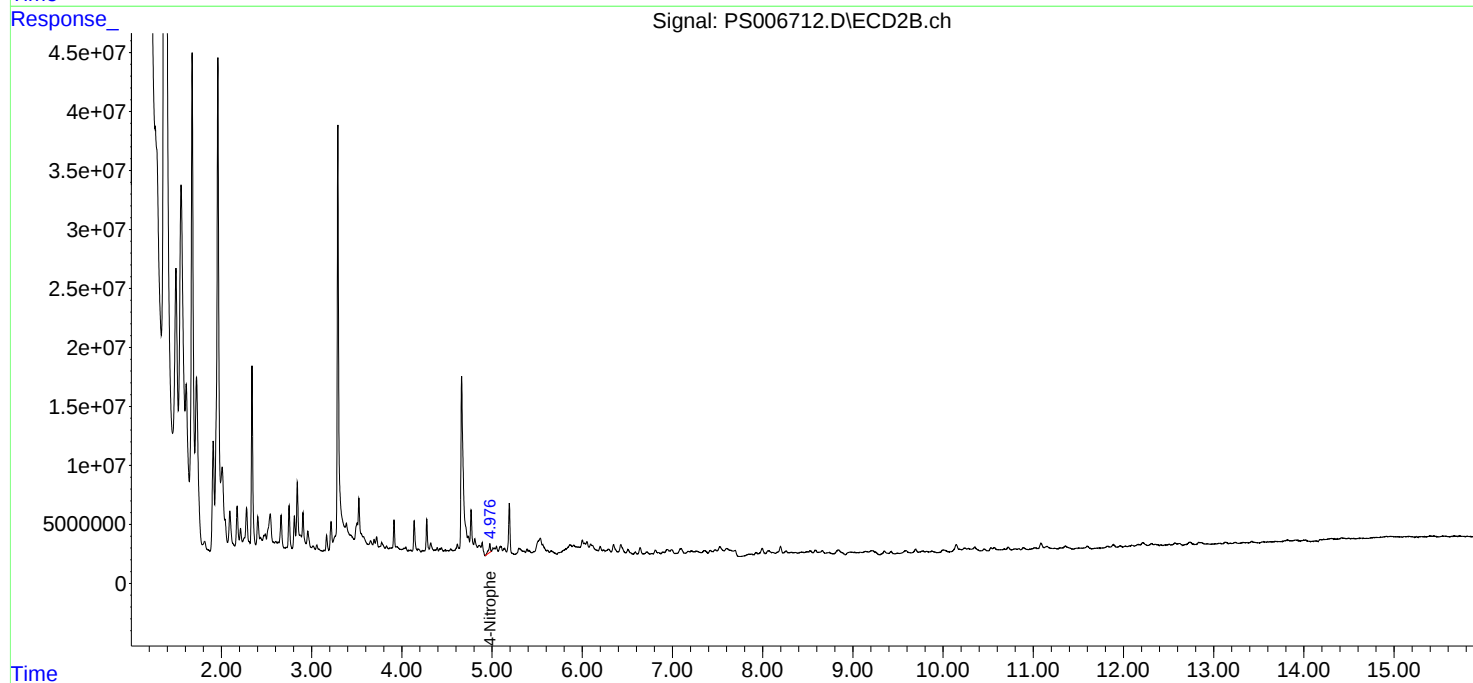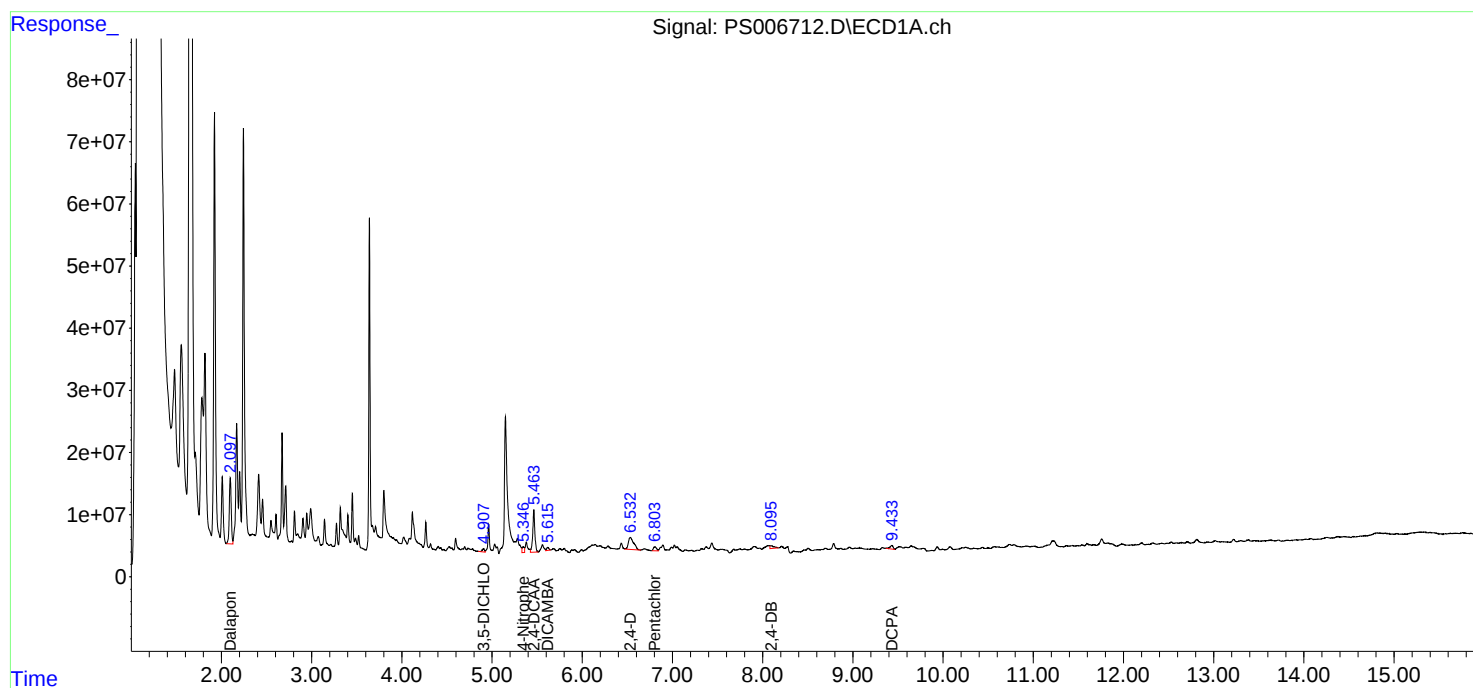


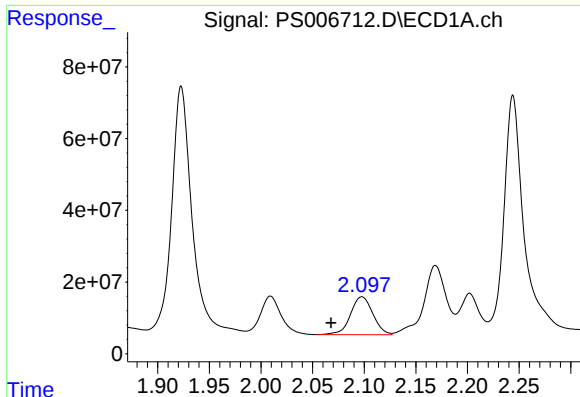

#1 Dalapon


R.T.: 2.098 min
Delta R.T.: 0.030 min
Response: 159712183
Conc: 163.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
GIS-4(0-4)

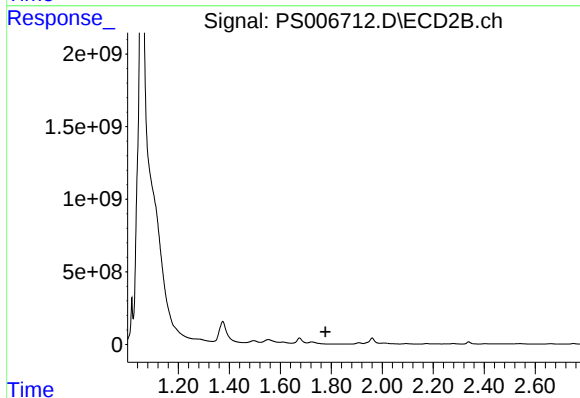


#1 Dalapon

R.T.: 1.724 min
Delta R.T.: -0.054 min
Response: -30345554
Conc: N.D.

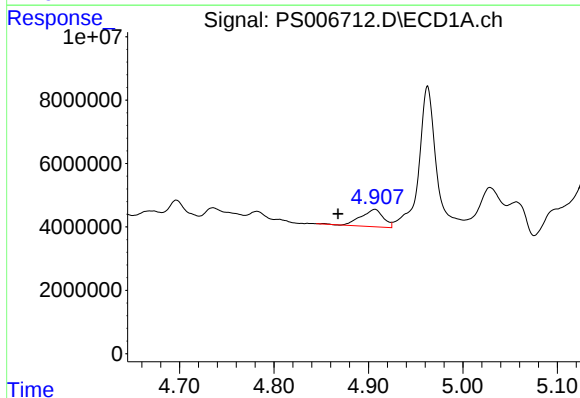


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.906 min
Delta R.T.: 0.038 min
Response: 9031821
Conc: 9.12 ng/ml

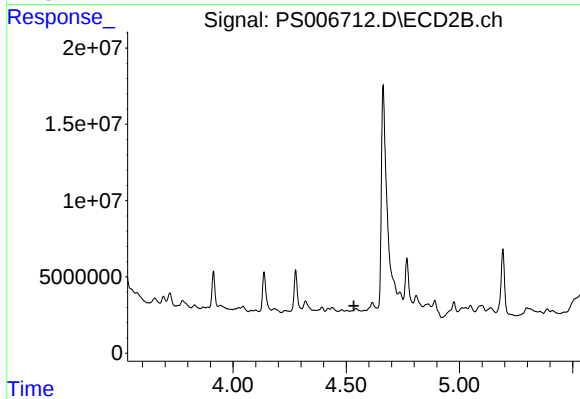

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.533 min
Response: 0
Conc: N.D.

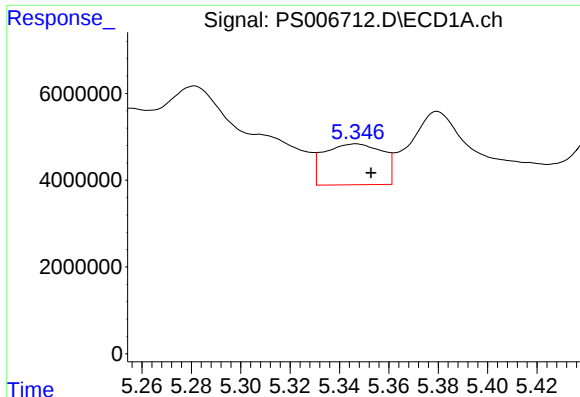

#3 4-Nitrophenol


R.T.: 5.346 min
Delta R.T.: -0.006 min
Response: 15475322
Conc: 43.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
GIS-4(0-4)

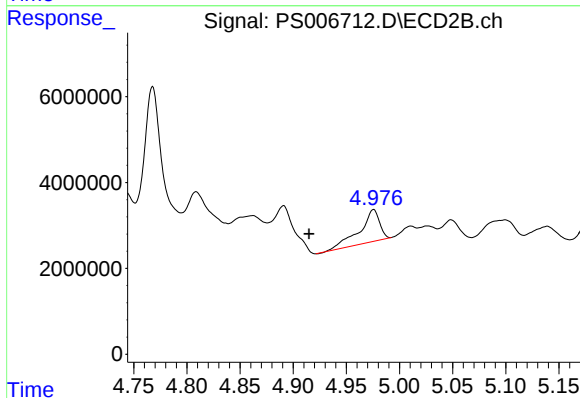


#3 4-Nitrophenol

R.T.: 4.976 min
Delta R.T.: 0.060 min
Response: 9769727
Conc: 44.14 ng/ml

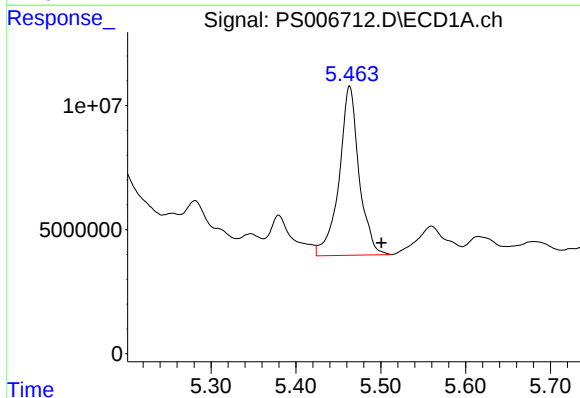


#4 2,4-DCAA

R.T.: 5.463 min
Delta R.T.: -0.037 min
Response: 111075636
Conc: 142.98 ng/ml

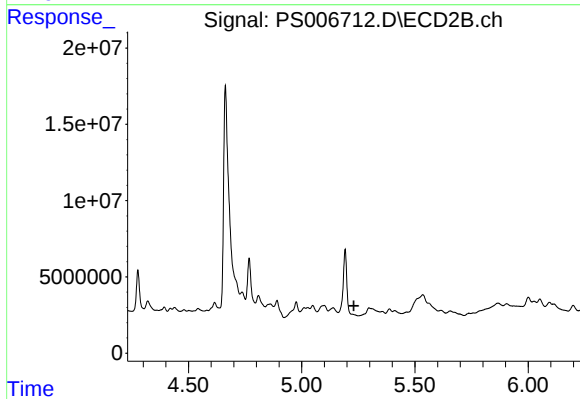

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.230 min
Response: 0
Conc: N.D.

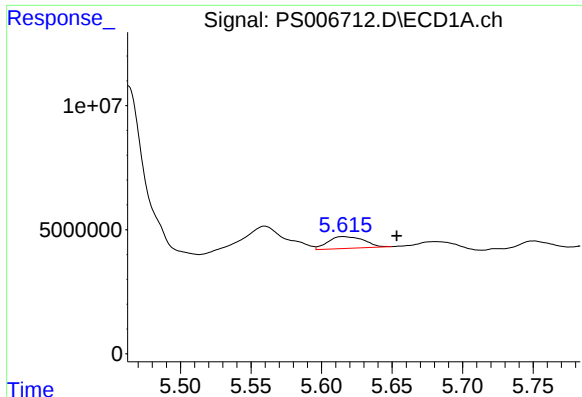

#5 DICAMBA


R.T.: 5.616 min
Delta R.T.: -0.038 min
Response: 8512502
Conc: 2.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
GIS-4(0-4)

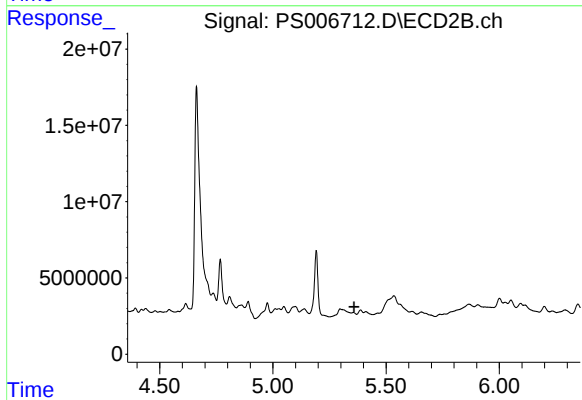


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

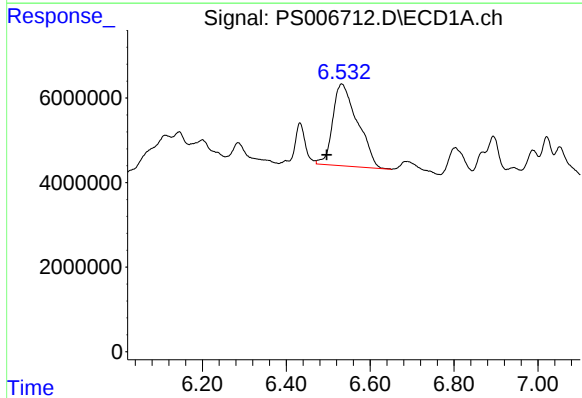


#9 2,4-D

R.T.: 6.532 min
Delta R.T.: 0.036 min
Response: 79718225
Conc: 103.18 ng/ml

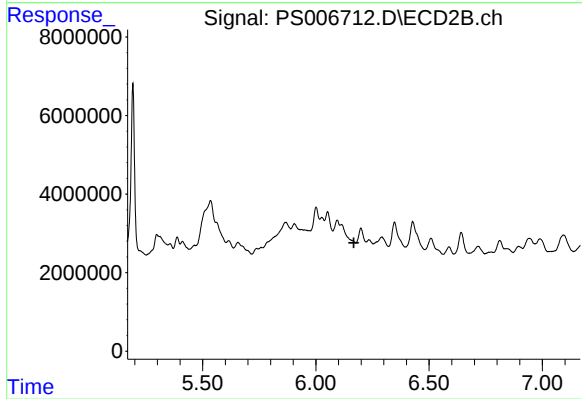

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

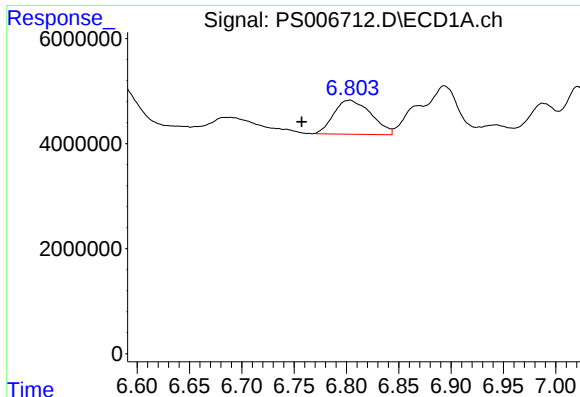

#10 Pentachlorophenol


R.T.: 6.803 min
Delta R.T.: 0.045 min
Response: 16056358
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
GIS-4(0-4)

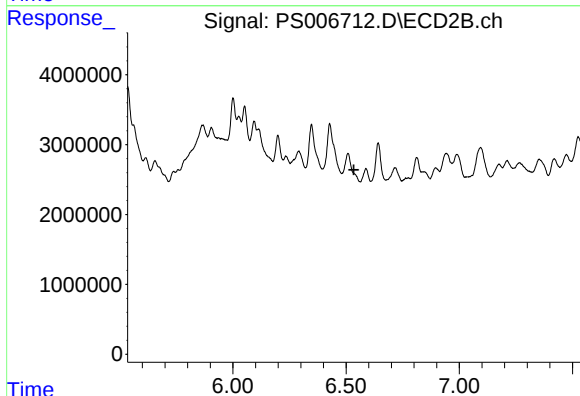


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.535 min
Response: 0
Conc: N.D.

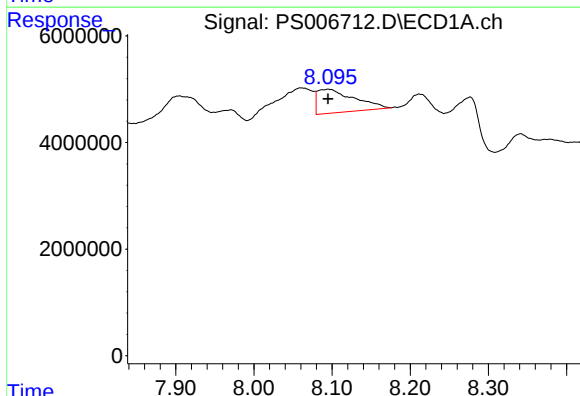


#13 2,4-DB

R.T.: 8.095 min
Delta R.T.: 0.000 min
Response: 14396783
Conc: 23.66 ng/ml

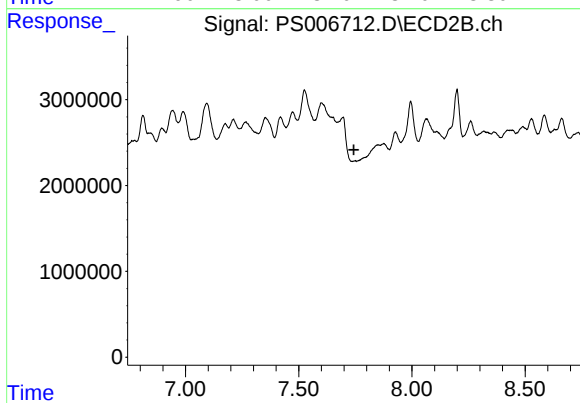

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

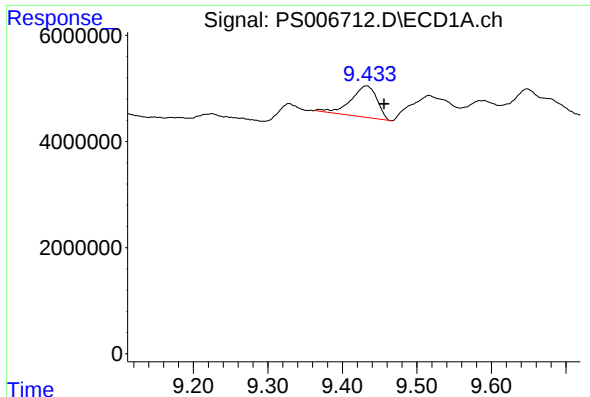

#16 DCPA

R.T.: 9.432 min
Delta R.T.: -0.024 min
Response: 14399130
Conc: 2.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
GIS-4(0-4)

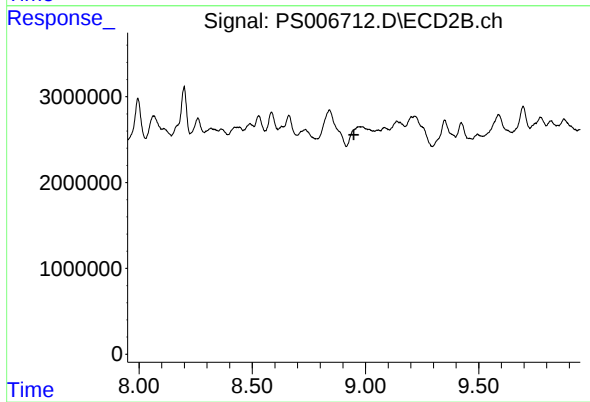

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.949 min
Response: 0
Conc: N.D.