

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091321\
 Data File : PS016795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2021 16:46
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 13 18:28:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS083121.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 01 10:13:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.762	657.6E6	296.3E6	437.841	571.545 #
Target Compounds							
9) T	2,4-D	8.364f	0.000	206.3E6	0	136.208	N.D. #
12) T	2,4,5-T	9.409	0.000	6906088	0	<MDL	N.D. #
15) T	Picloram	11.031f	10.849	90620906	32814295	10.170	8.955



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091321\
Data File : PS016795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2021 16:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 13 18:28:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS083121.M
Quant Title : 8080.M
QLast Update : Wed Sep 01 10:13:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

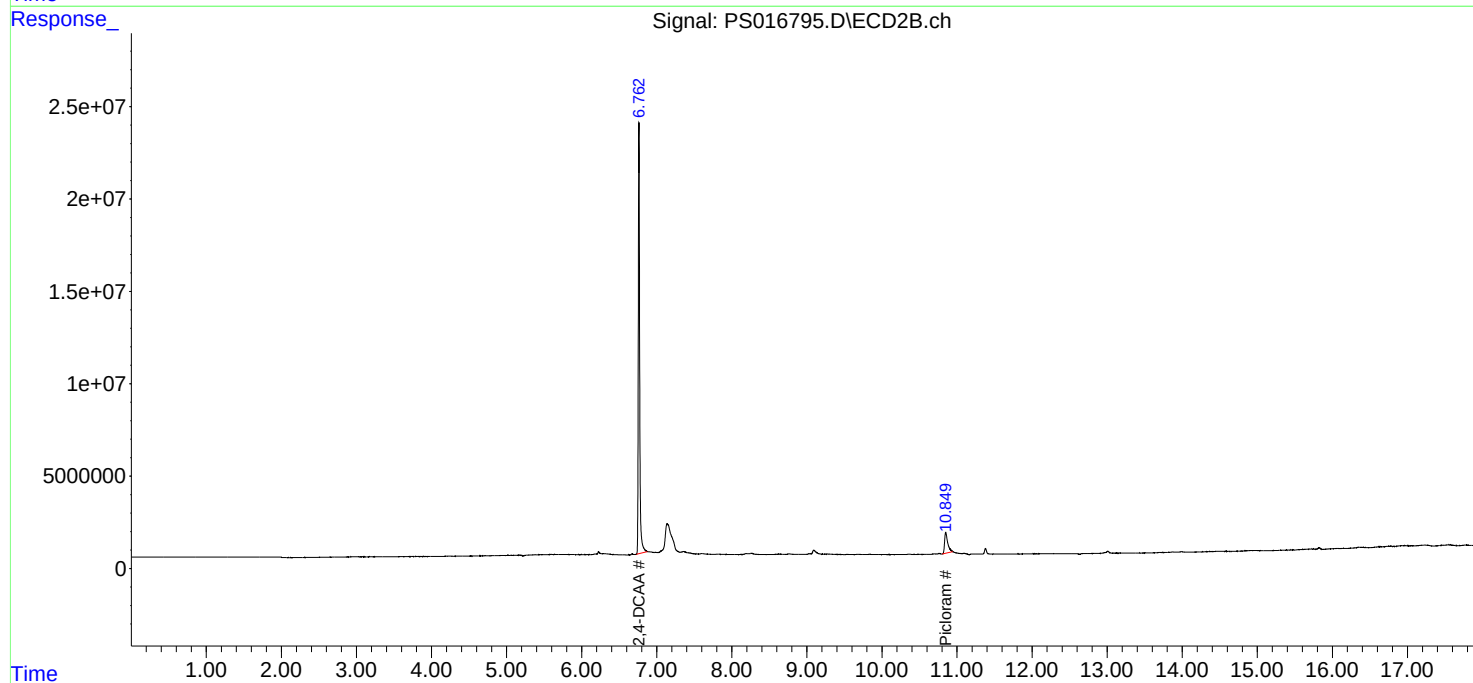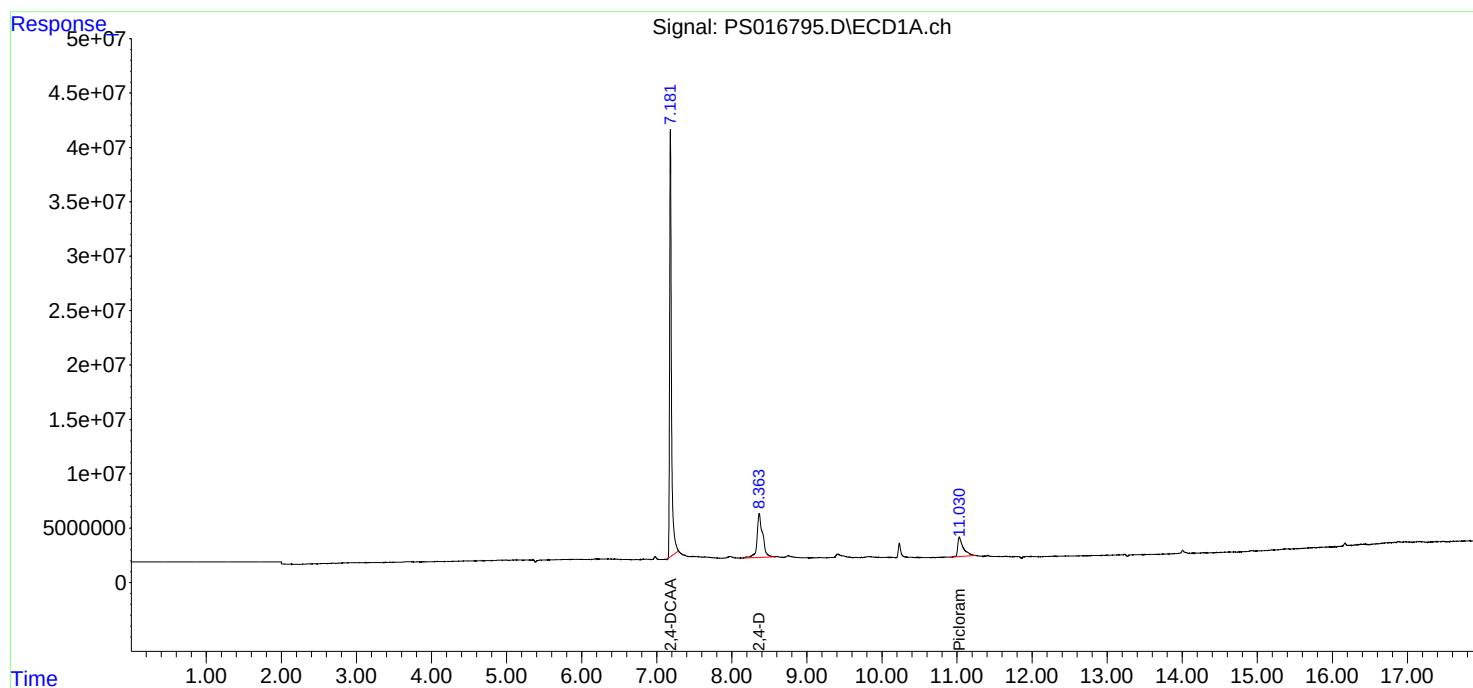


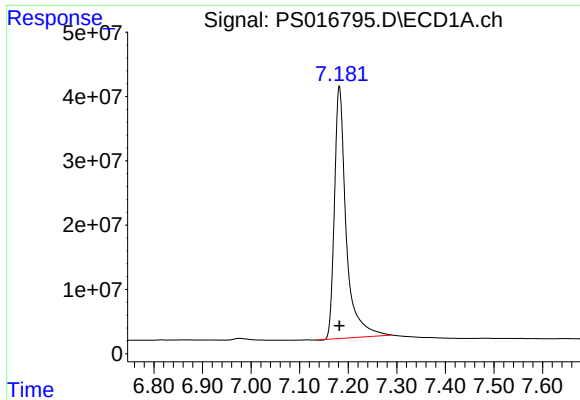

#4 2,4-DCAA


R.T.: 7.182 min
Delta R.T.: 0.000 min
Response: 657577330
Conc: 437.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

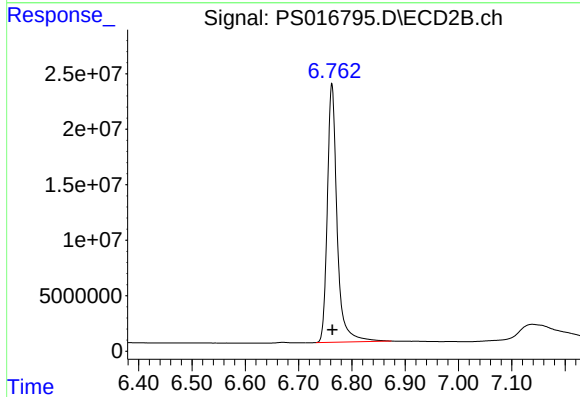


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: 0.000 min
Response: 296252555
Conc: 571.55 ng/ml

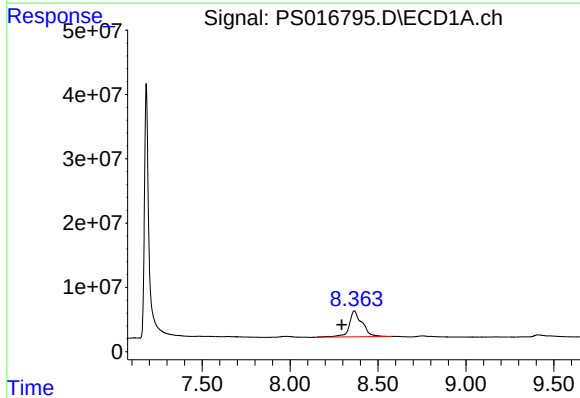


#9 2,4-D

R.T.: 8.364 min
Delta R.T.: 0.069 min
Response: 206322789
Conc: 136.21 ng/ml

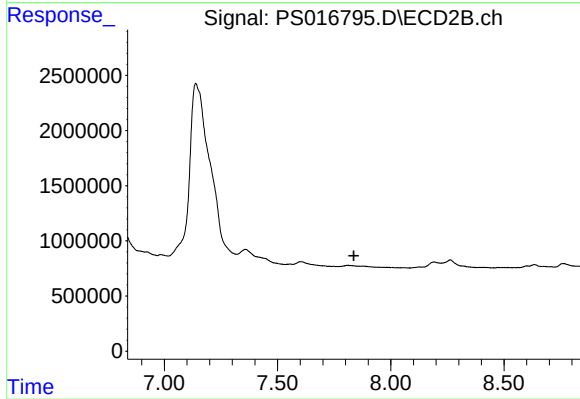

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.837 min
Response: 0
Conc: N.D.

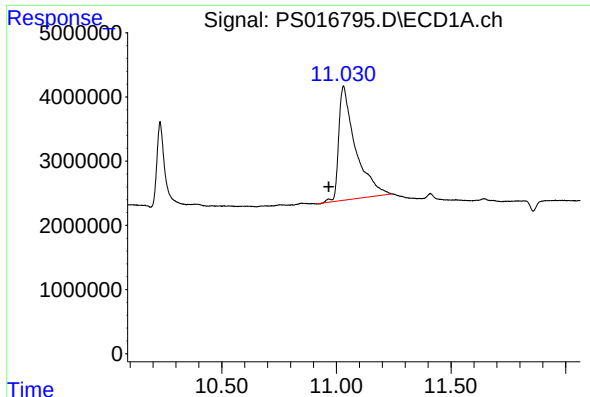

#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.064 min
Response: 90620906
Conc: 10.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

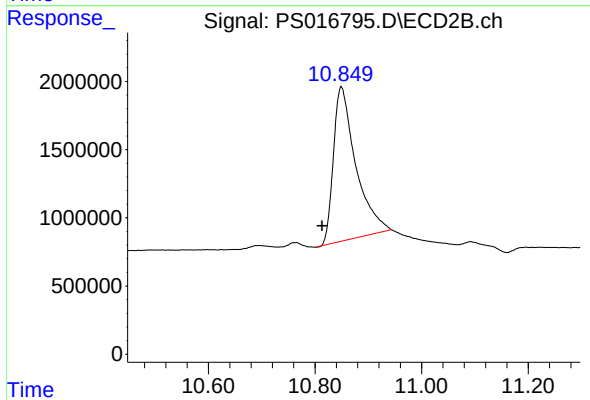

#15 Picloram

R.T.: 10.849 min
Delta R.T.: 0.036 min
Response: 32814295
Conc: 8.96 ng/ml