

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
 Data File : PS020500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2022 11:11
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 02:54:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	2.993	0.000	2261286	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.432	0.000	6989.1E6	0	1401.584	N.D. #
3) T	4-Nitroph...	6.966f	0.000	9440126	0	132.011	N.D. #
5) T	DICAMBA	7.382	6.973f	278062	1508.2E6	<MDL	391.778 #
6) T	MCP	0.000	6.973	0	1508.2E6	N.D.	522.251
8) T	DICHLORPROP	7.989f	7.603f	2708039	7408636	<MDL	7.343 #
9) T	2,4-D	8.355f	7.891f	5641.6E6	-401825	1213.742	N.D. #
10) T	Pentachlo...	8.620	0.000	24377323	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.157	0.000	8315570	0	<MDL	N.D. #
12) T	2,4,5-T	9.460	0.000	4562302	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.509	0	3272604	N.D.	4.575
14) T	DINOSEB	11.176f	0.000	56965641	0	3.102	N.D. #
15) T	Picloram	10.929	10.835	1787.7E6	27352261	59.404	3.397 #
16) T	DCPA	11.406	10.763	13578357	3784954	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
Data File : PS020500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2022 11:11
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 02:54:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

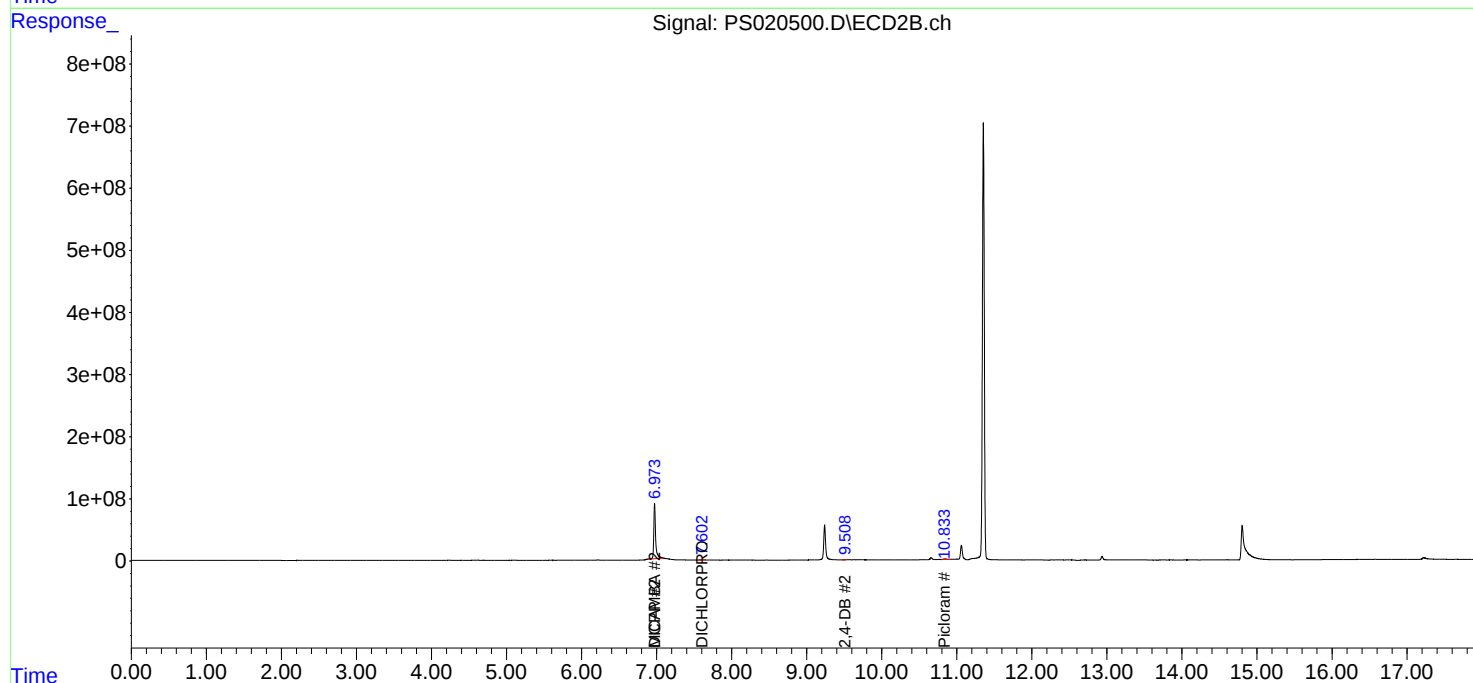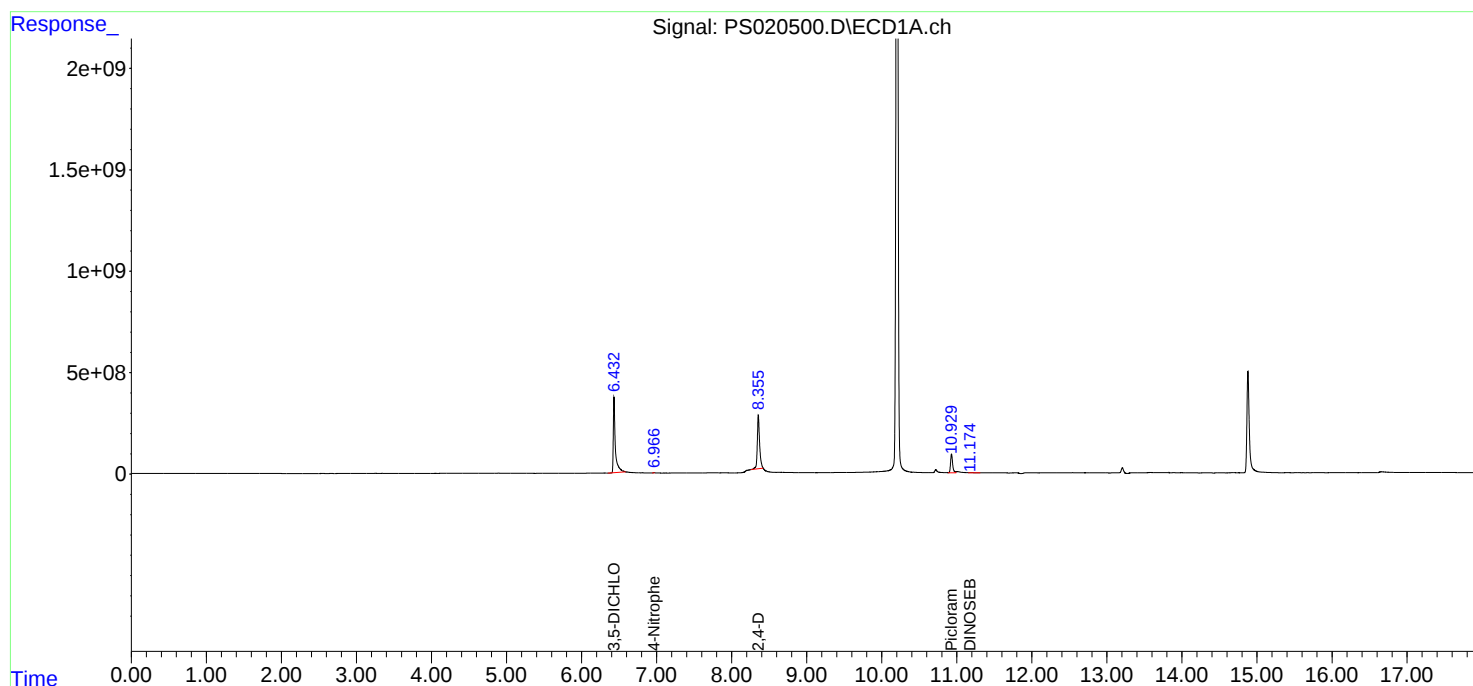


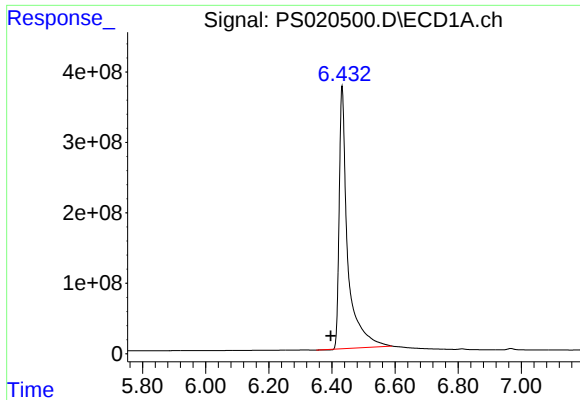

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.432 min
Delta R.T.: 0.036 min
Response: 6989102575
Conc: 1401.58 ng/m

Instrument :
ECD_S
ClientSampleId :

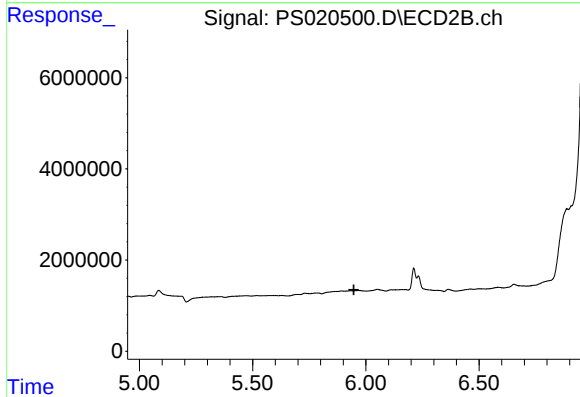


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

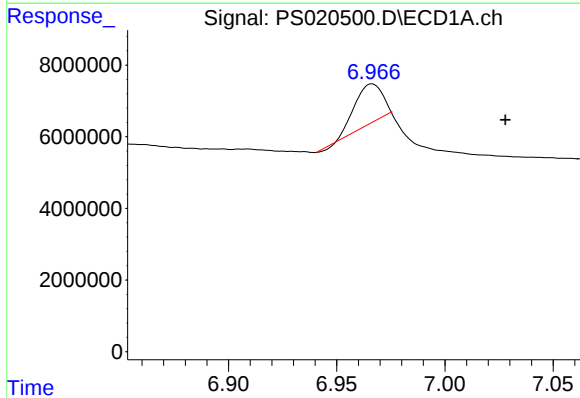


#3 4-Nitrophenol

R.T.: 6.966 min
Delta R.T.: -0.062 min
Response: 9440126
Conc: 132.01 ng/ml

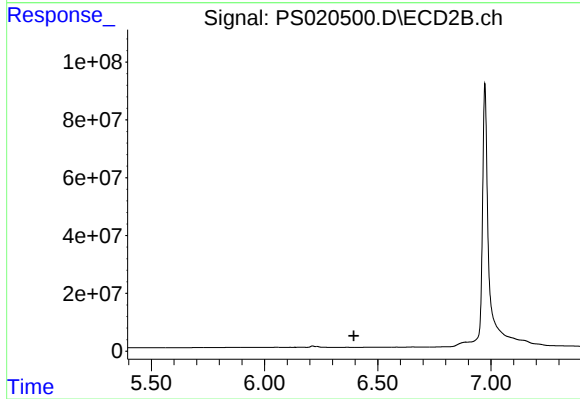

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

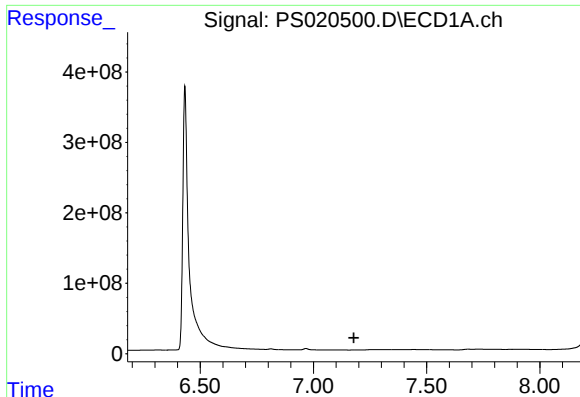

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: 0.021 min
Response: -1068206
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

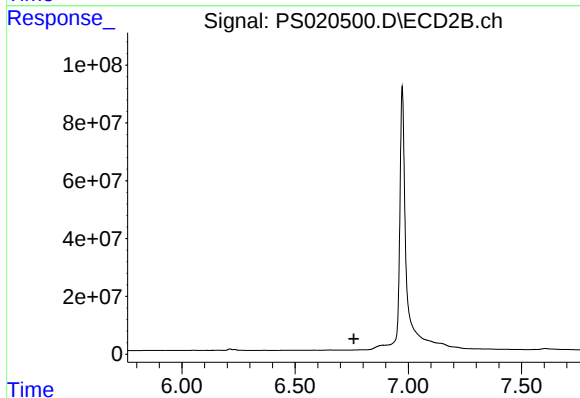


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.760 min
Response: 0
Conc: N.D.

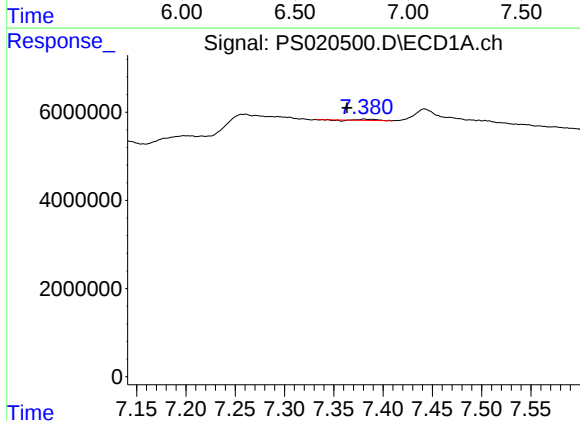


#5 DICAMBA

R.T.: 7.382 min
Delta R.T.: 0.018 min
Response: 278062
Conc: N.D.

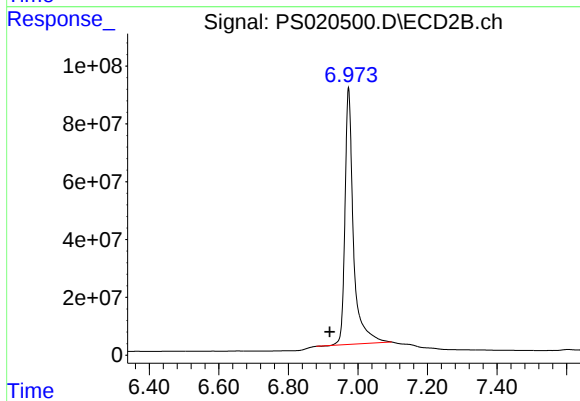

#5 DICAMBA


R.T.: 6.973 min
Delta R.T.: 0.054 min
Response: 1508203387
Conc: 391.78 ng/ml

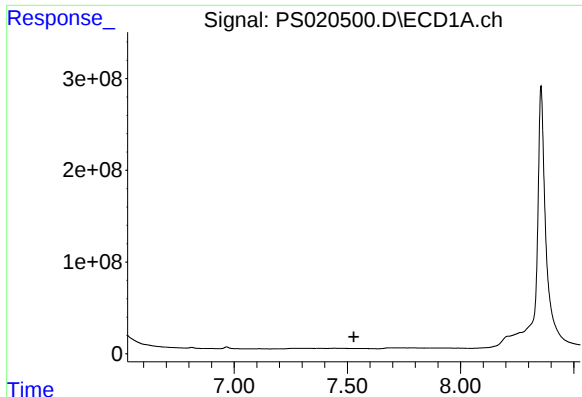

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

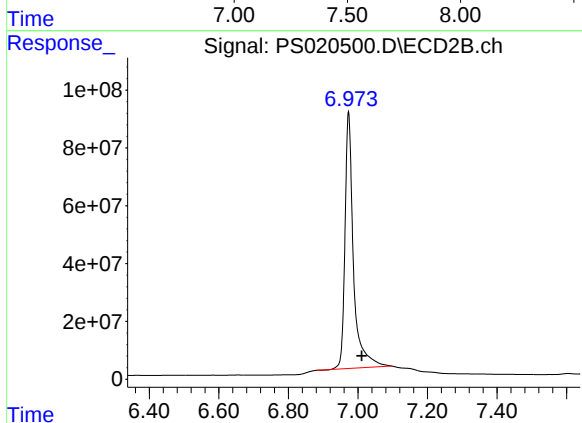


#6 MCP

R.T.: 6.973 min
Delta R.T.: -0.038 min
Response: 1508203387
Conc: 522.25 ug/ml

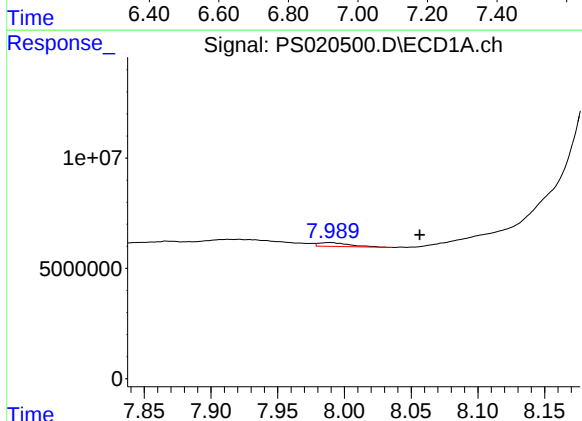


#8 DICHLORPROP

R.T.: 7.989 min
Delta R.T.: -0.068 min
Response: 2708039
Conc: N.D.

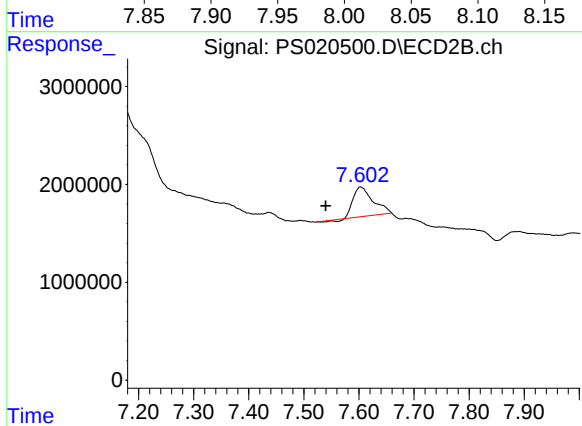

#8 DICHLORPROP


R.T.: 7.603 min
Delta R.T.: 0.063 min
Response: 7408636
Conc: 7.34 ng/ml

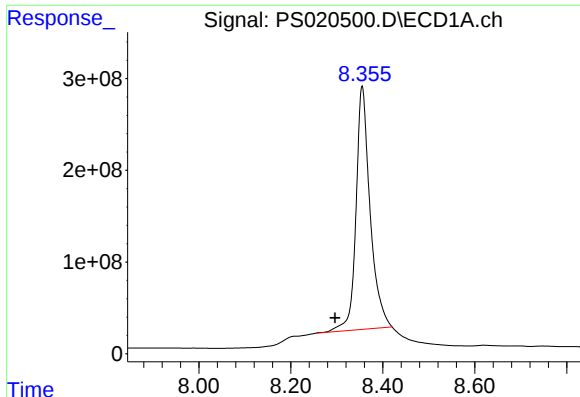

#9 2,4-D


R.T.: 8.355 min
Delta R.T.: 0.059 min
Response: 5641562174
Conc: 1213.74 ng/m

Instrument :
ECD_S
ClientSampleId :

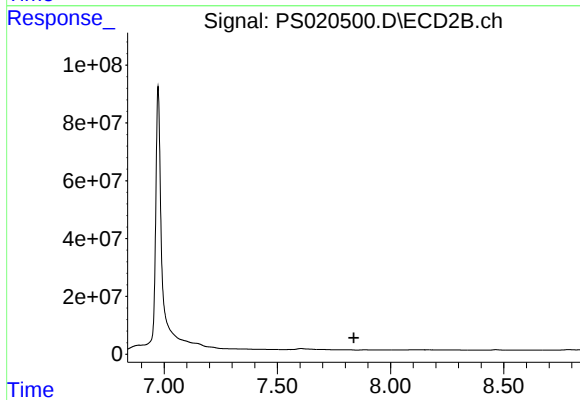


#9 2,4-D

R.T.: 7.891 min
Delta R.T.: 0.053 min
Response: -401825
Conc: N.D.

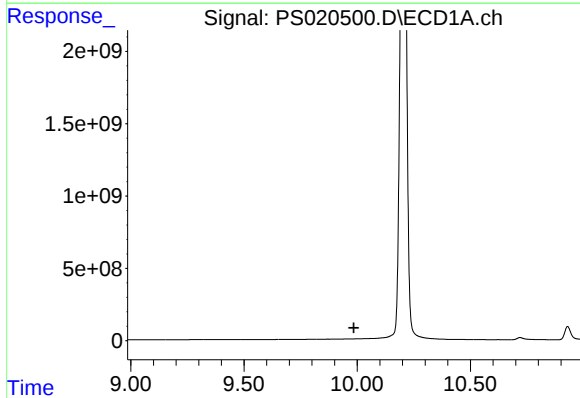


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.985 min
Response: 0
Conc: N.D.

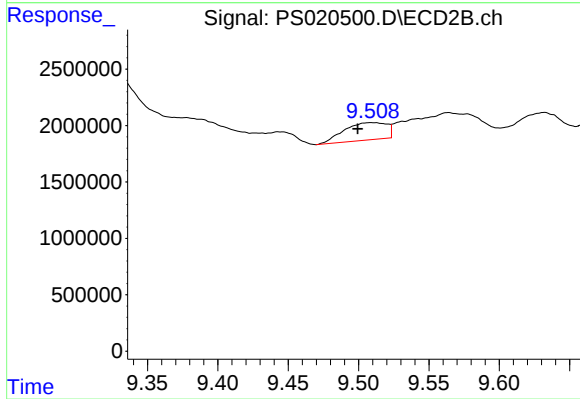

#13 2,4-DB


R.T.: 9.509 min
Delta R.T.: 0.009 min
Response: 3272604
Conc: 4.57 ng/ml

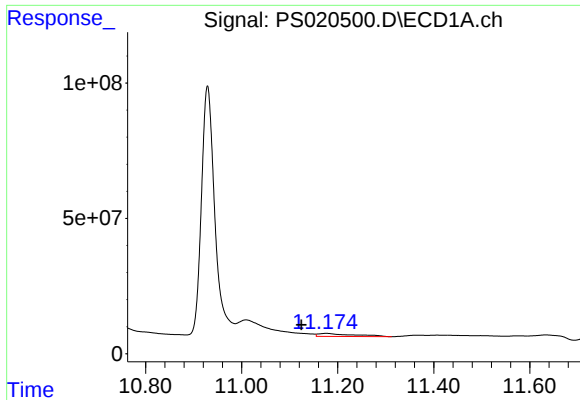

#14 DINOSEB


R.T.: 11.176 min
Delta R.T.: 0.051 min
Response: 56965641
Conc: 3.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

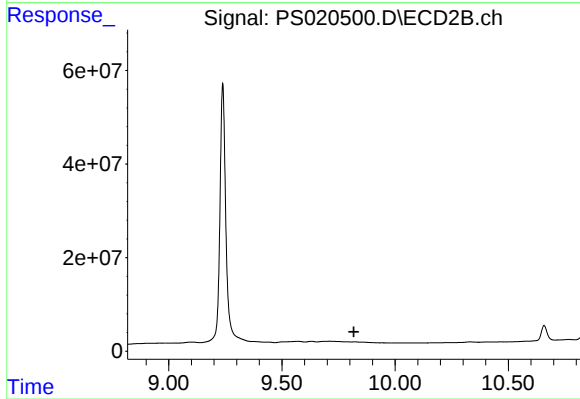


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

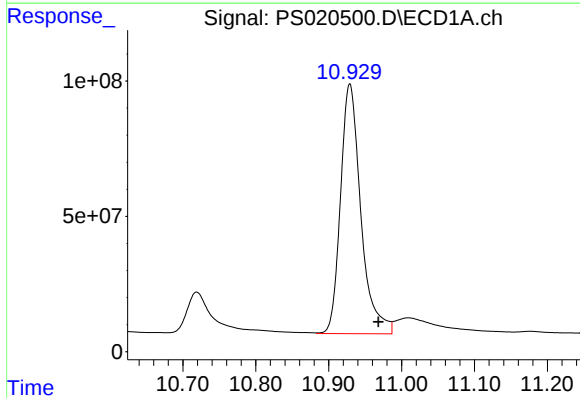

#15 Picloram

R.T.: 10.929 min
Delta R.T.: -0.039 min
Response: 1787656503
Conc: 59.40 ng/ml

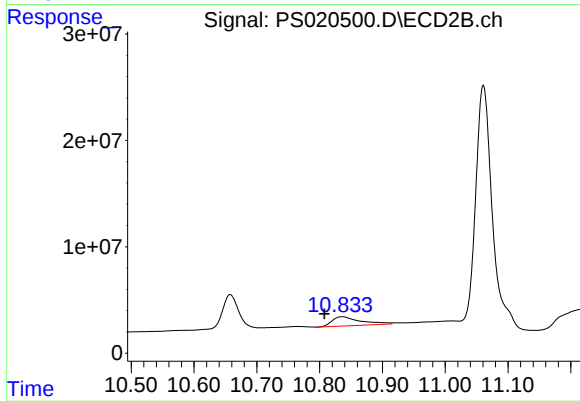

#15 Picloram

R.T.: 10.835 min
Delta R.T.: 0.027 min
Response: 27352261
Conc: 3.40 ng/ml