

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
 Data File : PS020520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 02:28
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 02:59:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.177	6.758	1568.7E6	453.7E6	455.829	532.711
Target Compounds							
1) T	Dalapon	2.972	0.000	211527	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.453f	0.000	3420863	0	<MDL	N.D. #
9) T	2,4-D	8.359f	0.000	150.1E6	0	32.291	N.D. #
10) T	Pentachlo...	8.590	0.000	1001832	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.156	0.000	1941838	0	<MDL	N.D. #
12) T	2,4,5-T	9.405	0.000	13786957	0	<MDL	N.D. #
13) T	2,4-DB	10.007	0.000	17544363	0	4.831	N.D. #
14) T	DINOSEB	11.122	9.828	10146371	685287	<MDL	<MDL #
15) T	Picloram	10.952	10.853f	-52053	12034481	N.D.	1.494
16) T	DCPA	11.395	10.746	7721016	715071	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
Data File : PS020520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 02:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 02:59:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

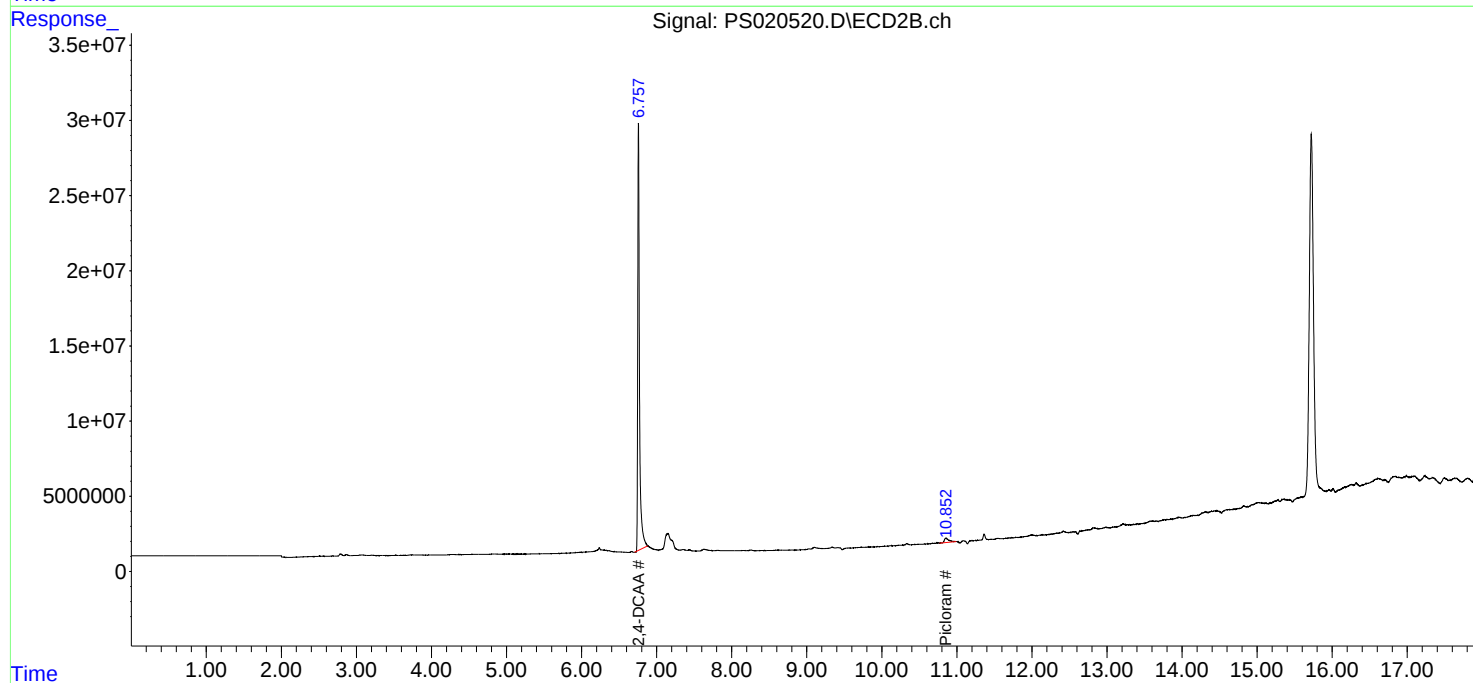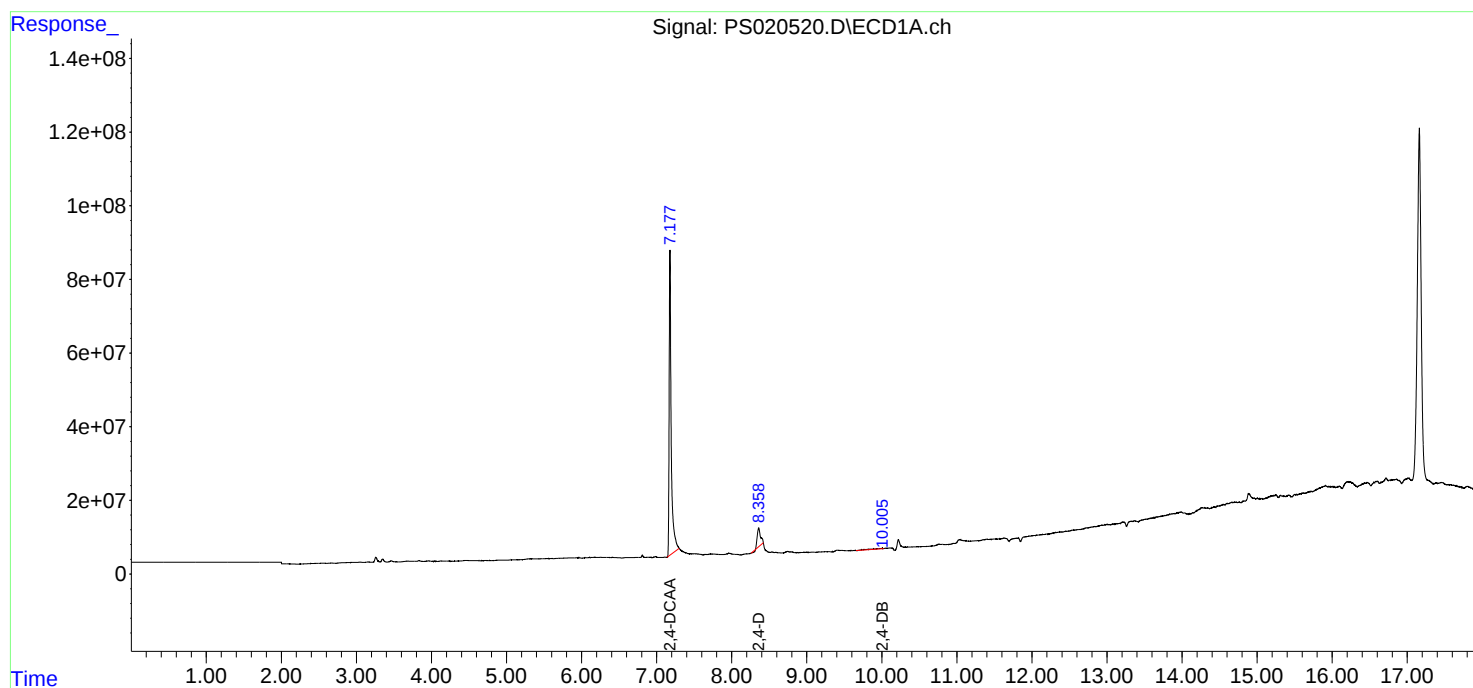


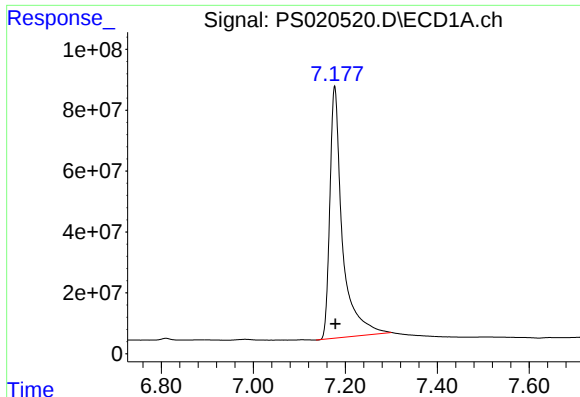

#4 2,4-DCAA


R.T.: 7.177 min
Delta R.T.: -0.002 min
Response: 1568728780
Conc: 455.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

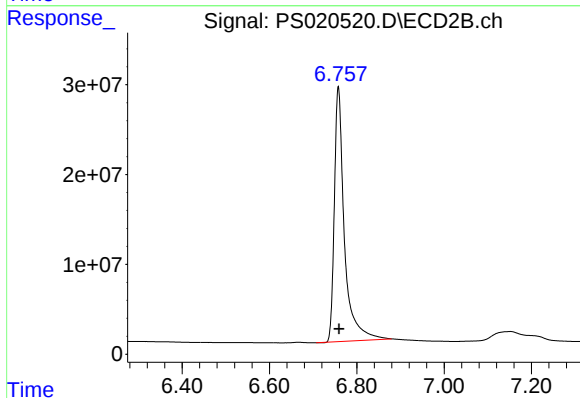


#4 2,4-DCAA

R.T.: 6.758 min
Delta R.T.: -0.002 min
Response: 453707597
Conc: 532.71 ng/ml

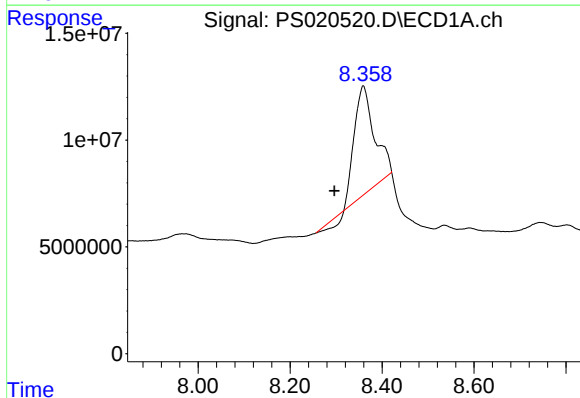


#9 2,4-D

R.T.: 8.359 min
Delta R.T.: 0.063 min
Response: 150090930
Conc: 32.29 ng/ml

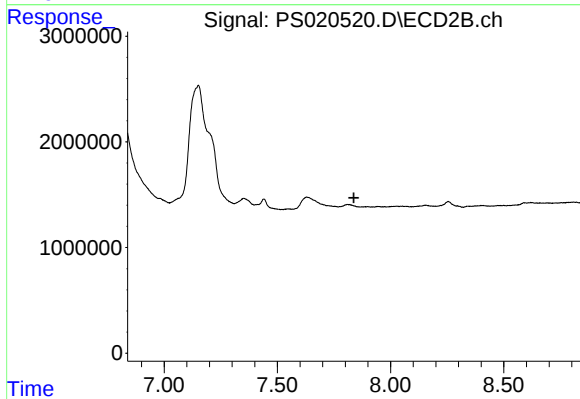

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

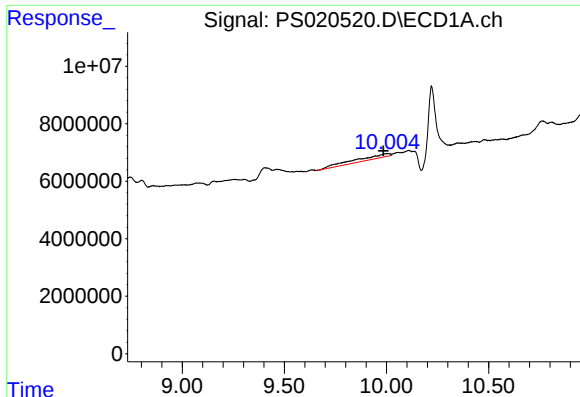

#13 2,4-DB


R.T.: 10.007 min
Delta R.T.: 0.022 min
Response: 17544363
Conc: 4.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

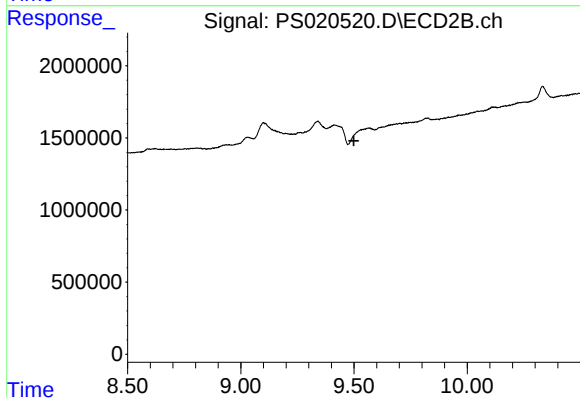


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.499 min
Response: 0
Conc: N.D.

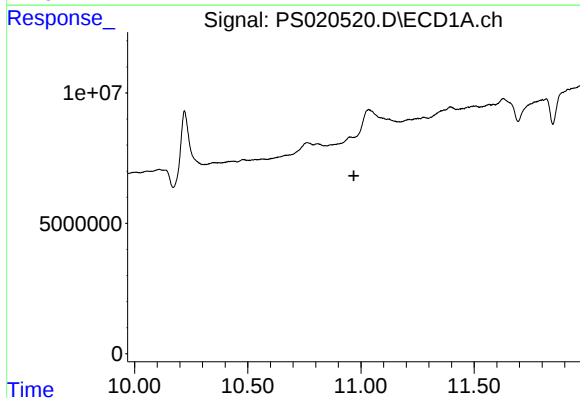

#15 Picloram

R.T.: 10.952 min
Delta R.T.: -0.016 min
Response: -52053
Conc: N.D.

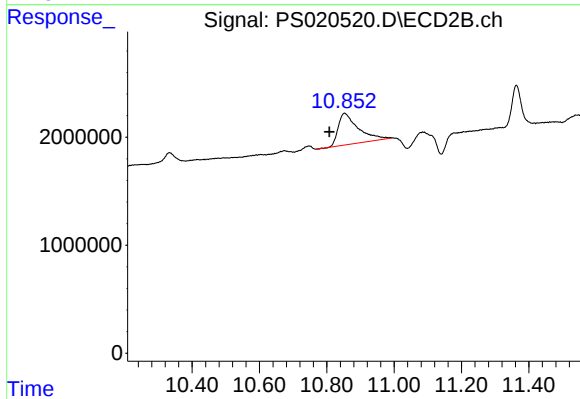

#15 Picloram

R.T.: 10.853 min
Delta R.T.: 0.045 min
Response: 12034481
Conc: 1.49 ng/ml