

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
 Data File : PS020529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 07:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 08:09:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.178	6.759	1636.6E6	464.4E6	475.562	545.245
Target Compounds							
1) T	Dalapon	2.987	0.000	432118	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.455f	0.000	8373940	0	1.679	N.D. #
9) T	2,4-D	8.354f	0.000	166.6E6	0	35.835	N.D. #
10) T	Pentachlo...	8.593	0.000	1378795	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.155	0.000	3270110	0	<MDL	N.D. #
12) T	2,4,5-T	9.412	9.034	21266752	437082	<MDL	<MDL #
13) T	2,4-DB	10.005	0.000	1718870	0	<MDL	N.D. #
15) T	Picloram	10.953	10.862f	29158510	16918568	<MDL	2.101 #
16) T	DCPA	11.396	10.747	6370788	1053892	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
Data File : PS020529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 07:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 08:09:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

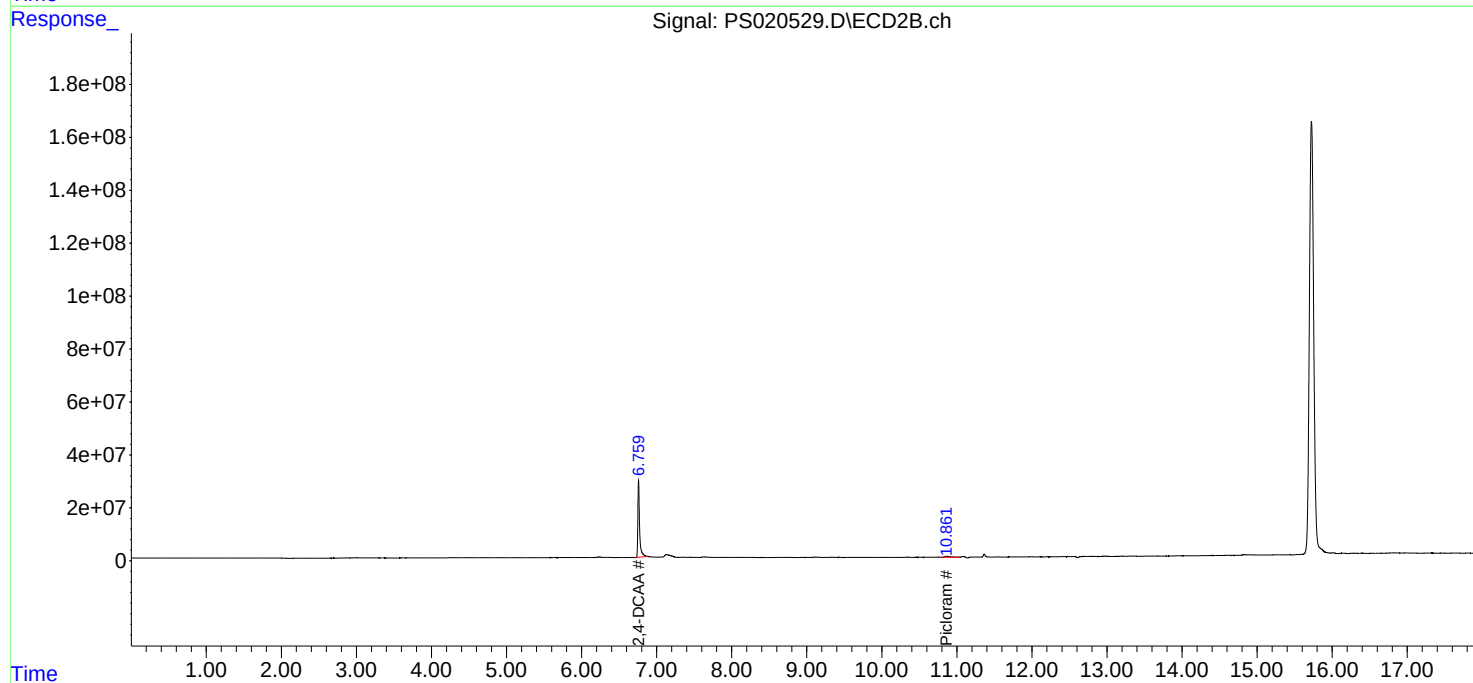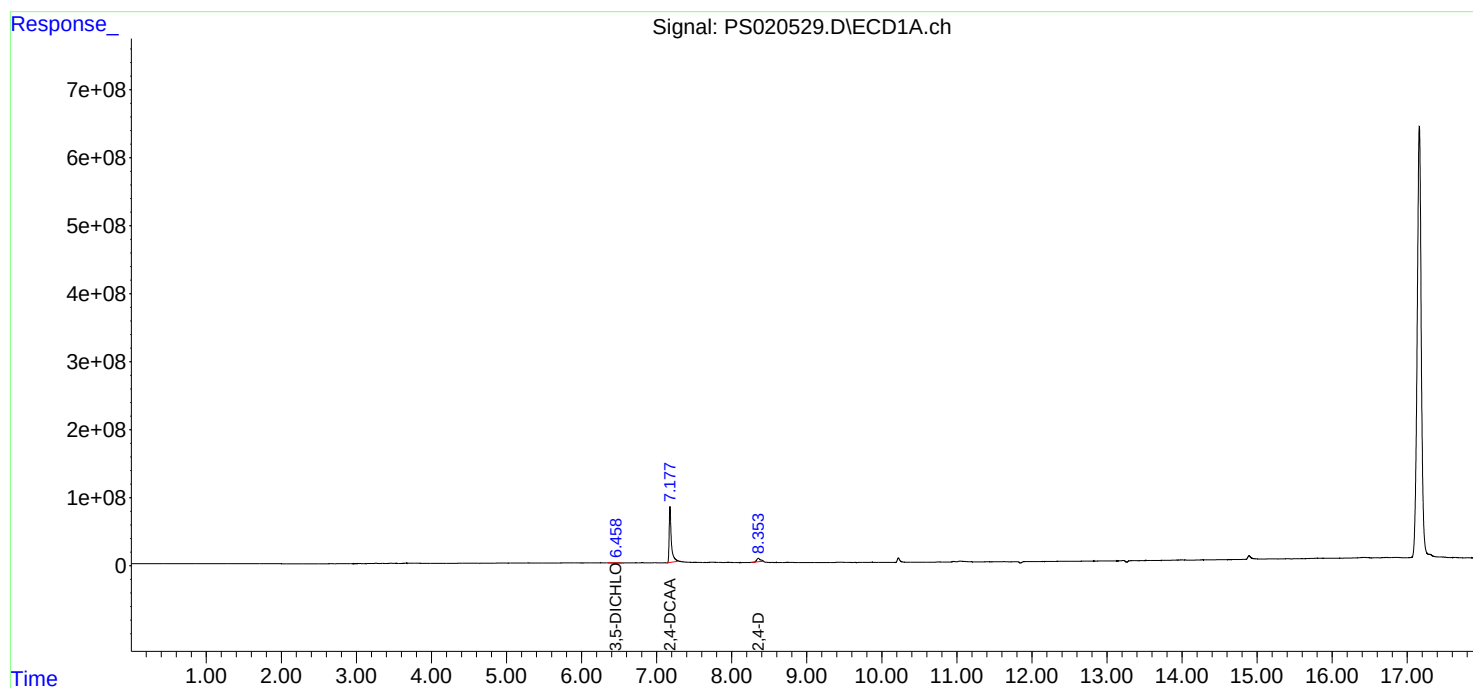


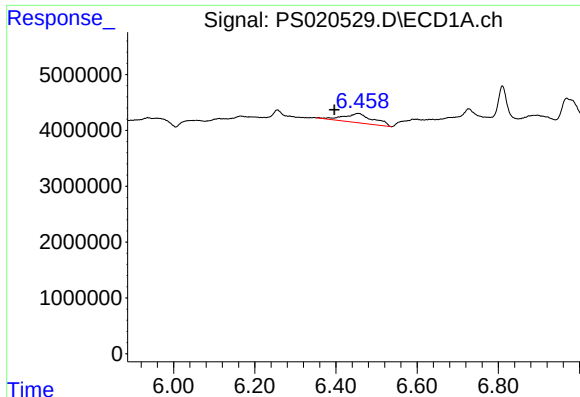

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.455 min
Delta R.T.: 0.058 min
Response: 8373940
Conc: 1.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

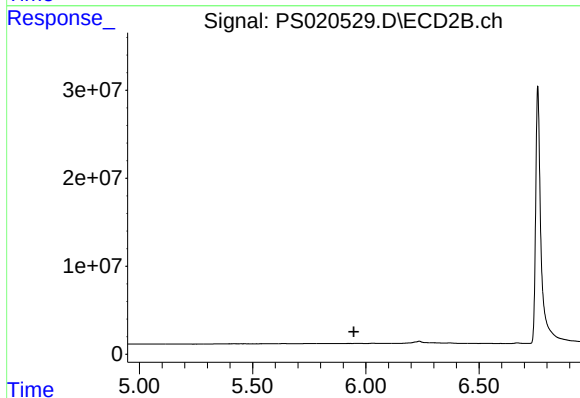


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

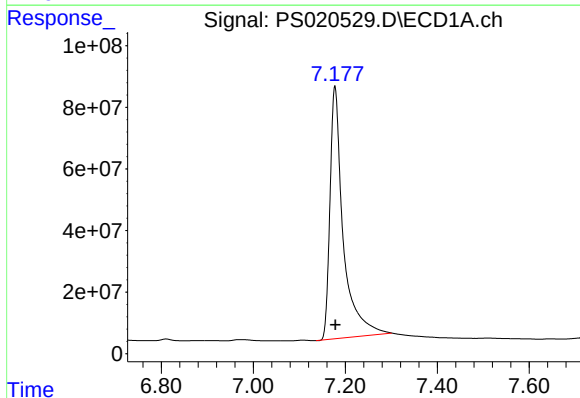


#4 2,4-DCAA

R.T.: 7.178 min
Delta R.T.: -0.001 min
Response: 1636639241
Conc: 475.56 ng/ml

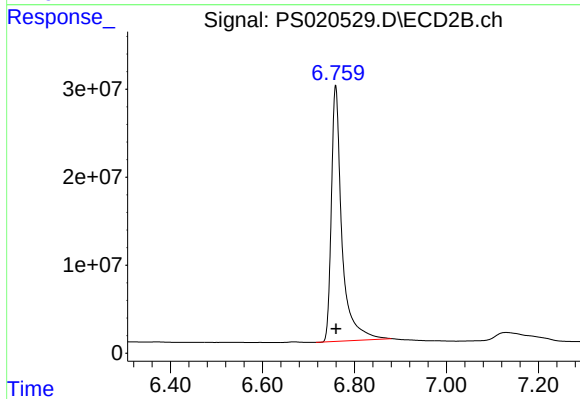

#4 2,4-DCAA


R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 464382508
Conc: 545.24 ng/ml

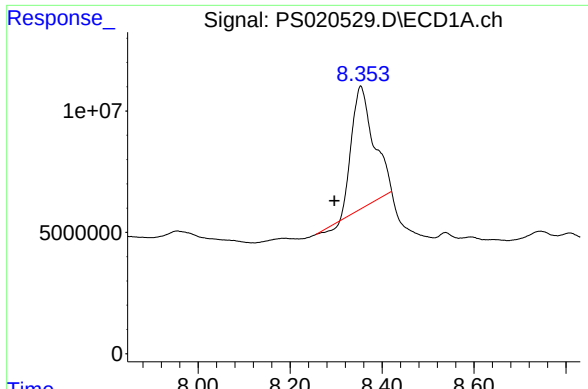

#9 2,4-D


R.T.: 8.354 min
Delta R.T.: 0.057 min
Response: 166564628
Conc: 35.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

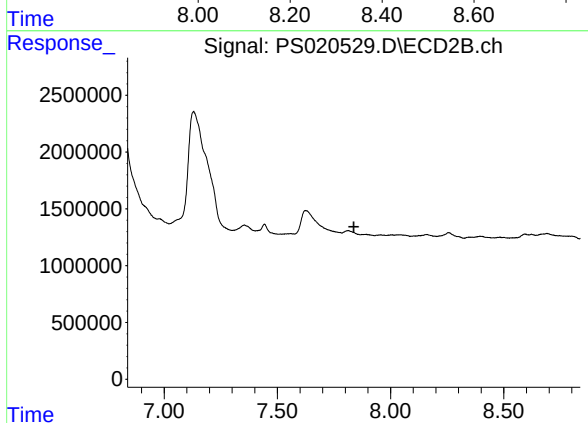


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

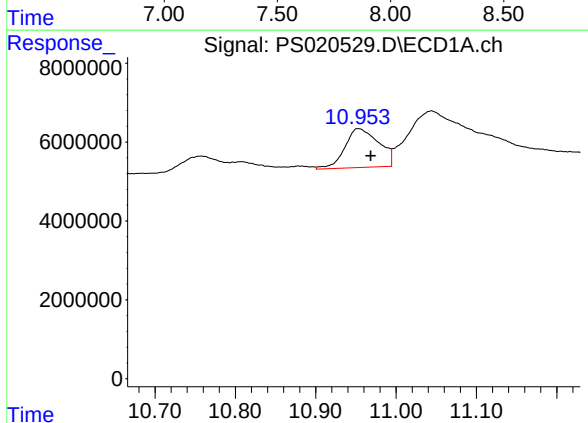

#15 Picloram

R.T.: 10.953 min
Delta R.T.: -0.015 min
Response: 29158510
Conc: N.D.

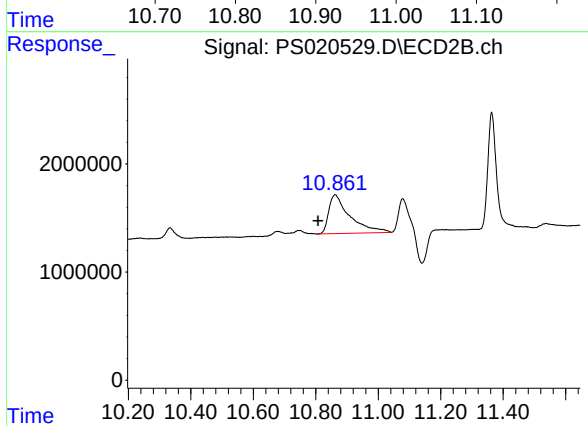

#15 Picloram

R.T.: 10.862 min
Delta R.T.: 0.054 min
Response: 16918568
Conc: 2.10 ng/ml