

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
 Data File : PS020506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Sep 2022 20:47
 Operator : AJ\MA
 Sample : HSTDICC1500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC1500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 02:42:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:40:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.175	6.756	5001.7E6	1286.2E6	1502.324	1524.243
Target Compounds							
1) T	Dalapon	3.001	2.518	6575.1E6	1647.4E6	1352.375	1377.451
2) T	3,5-DICHL...	6.392	5.943	6487.6E6	1867.3E6	1372.548	1393.805
3) T	4-Nitroph...	7.008	6.379	2432.3E6	703.6E6	1492.492	1412.970
5) T	DICAMBA	7.363	6.919	18081.0E6	5253.1E6	1385.464	1393.831
6) T	MCP	7.536	7.020	1597.5E6	429.8E6	147.637	145.216
7) T	MCPA	7.686	7.234	2161.5E6	608.0E6	144.039	142.278
8) T	DICHLORPROP	8.054	7.538	4812.4E6	1390.4E6	1406.151	1413.132
9) T	2,4-D	8.285	7.830	5816.2E6	1761.7E6	1342.423	1407.009
10) T	Pentachlo...	8.590	8.252	46949.7E6	17213.8E6	1183.975	1324.880
11) T	2,4,5-TP ...	9.138	8.613	26421.2E6	7842.0E6	1386.962	1384.003
12) T	2,4,5-T	9.424	8.990	28276.3E6	7564.3E6	1378.976	1405.498
13) T	2,4-DB	9.976	9.495	5717.9E6	1058.6E6	1493.656	1462.433
14) T	DINOSEB	11.123	9.817	22604.9E6	5787.6E6	1365.744	1388.515
15) T	Picloram	10.953	10.798	44122.7E6	11394.2E6	1438.410	1416.075
16) T	DCPA	11.393	10.744	32896.9E6	9591.0E6	1392.535	1381.149



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
Data File : PS020506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Sep 2022 20:47
Operator : AJ\MA
Sample : HSTDICC1500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 02:42:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:40:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

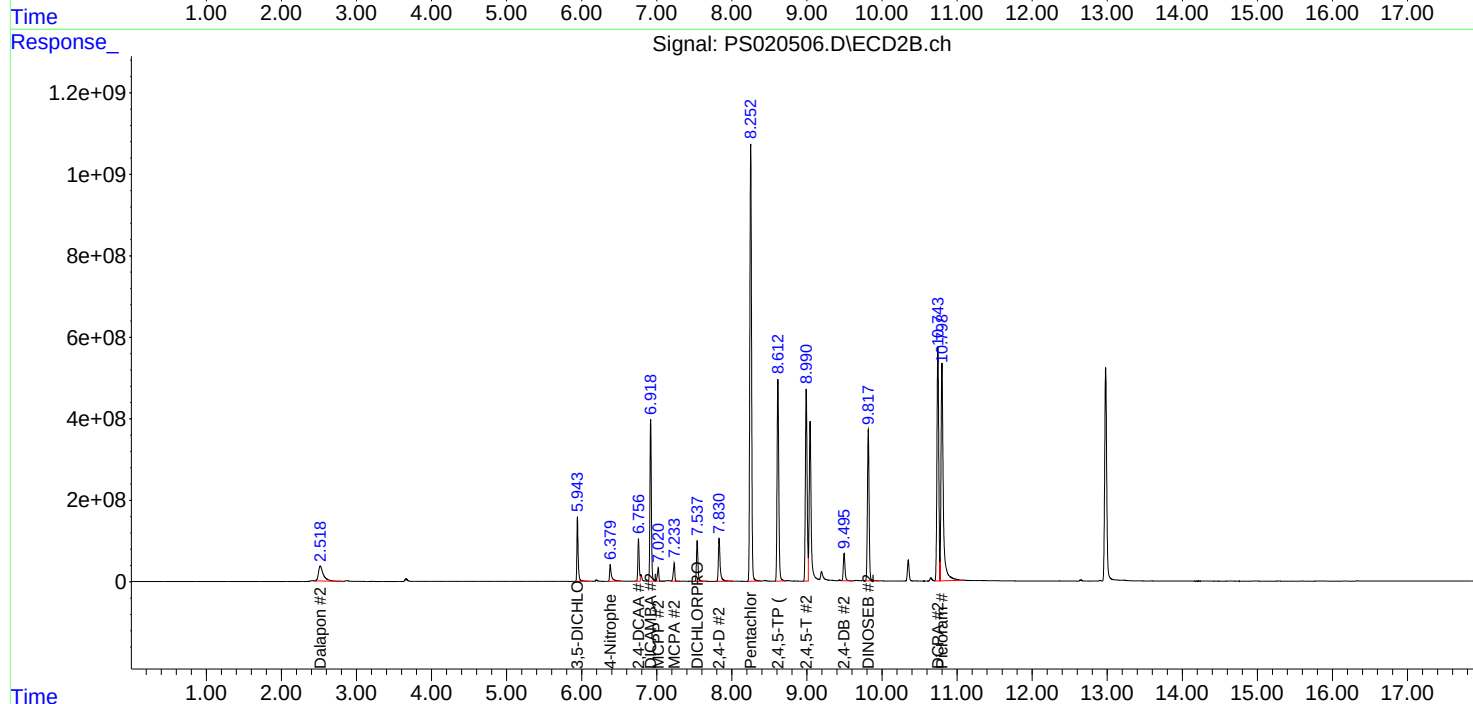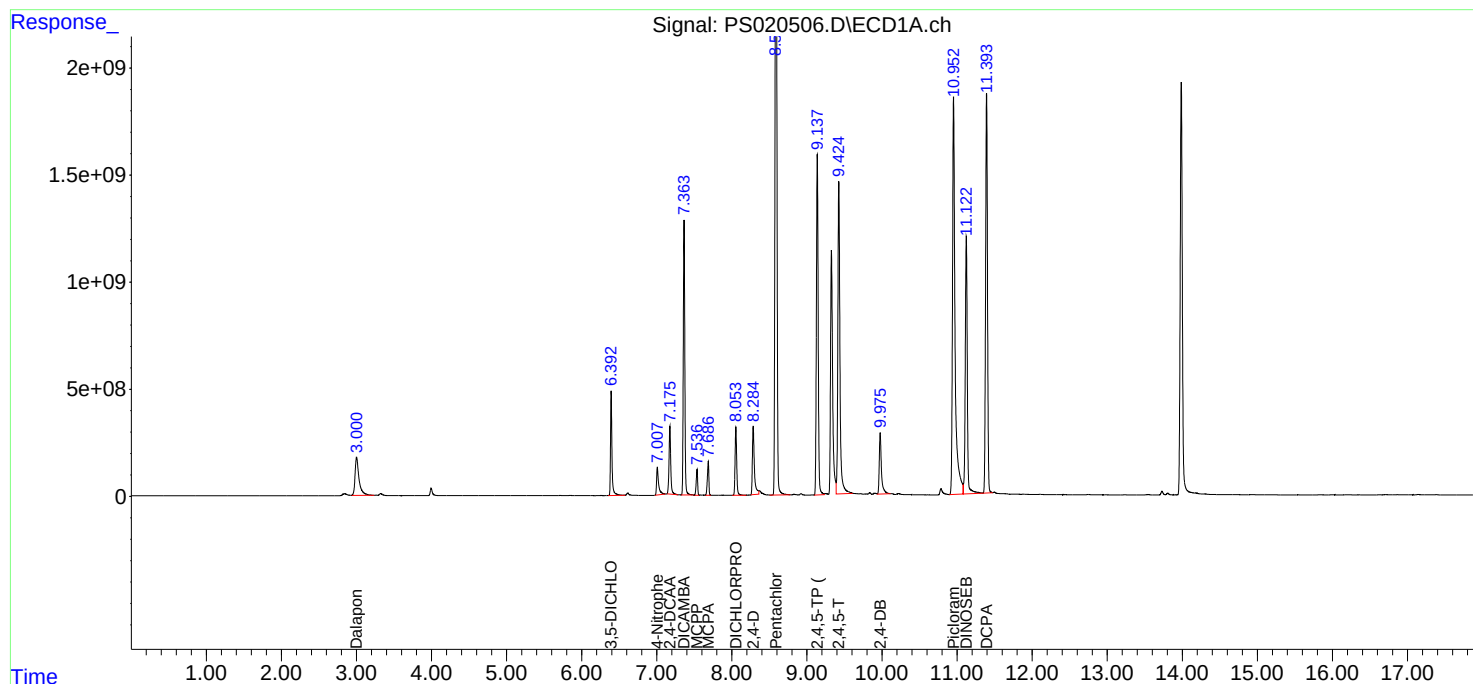


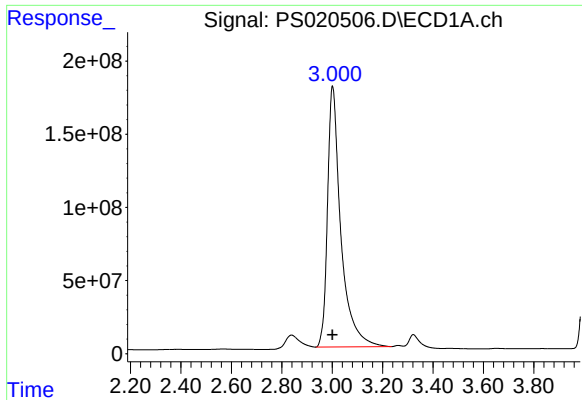

#1 Dalapon


R.T.: 3.001 min
Delta R.T.: 0.000 min
Response: 6575072483
Conc: 1352.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

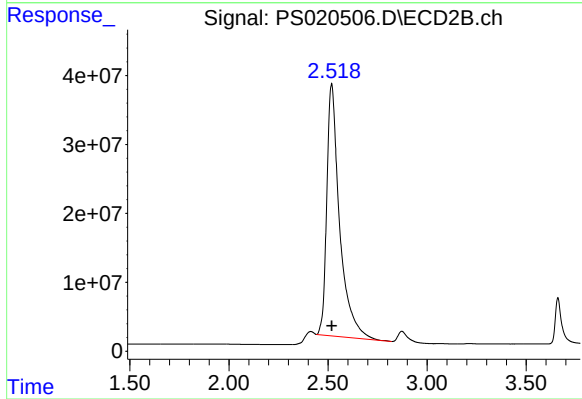


#1 Dalapon

R.T.: 2.518 min
Delta R.T.: 0.000 min
Response: 1647381367
Conc: 1377.45 ng/ml

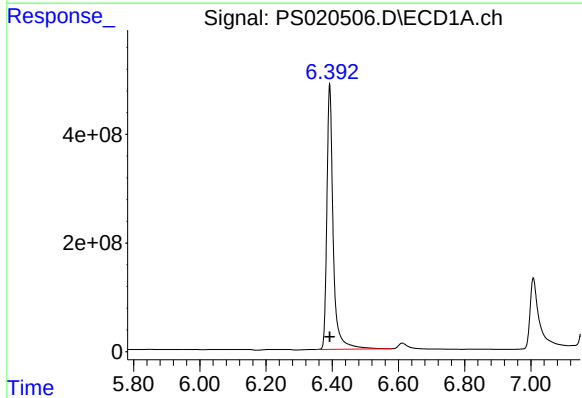


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 6487649603
Conc: 1372.55 ng/ml

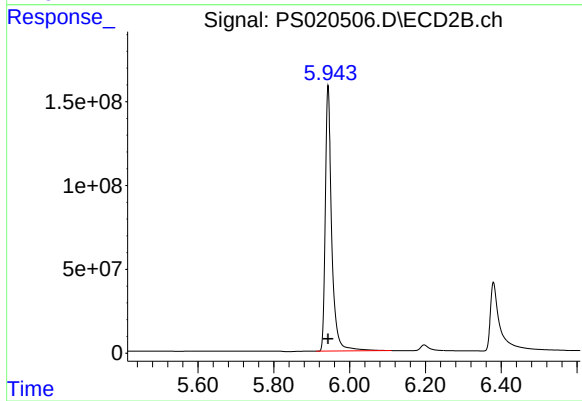

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 1867276977
Conc: 1393.81 ng/ml

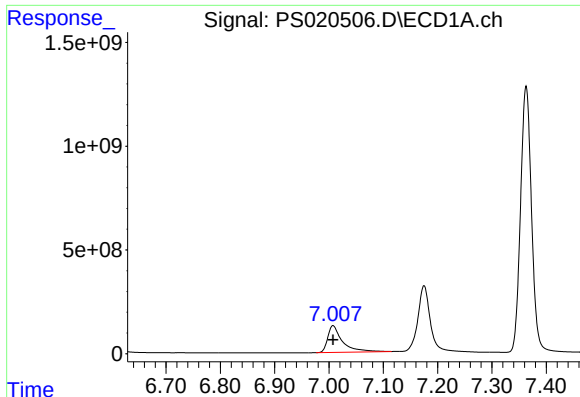

#3 4-Nitrophenol


R.T.: 7.008 min
Delta R.T.: 0.000 min
Response: 2432287303
Conc: 1492.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

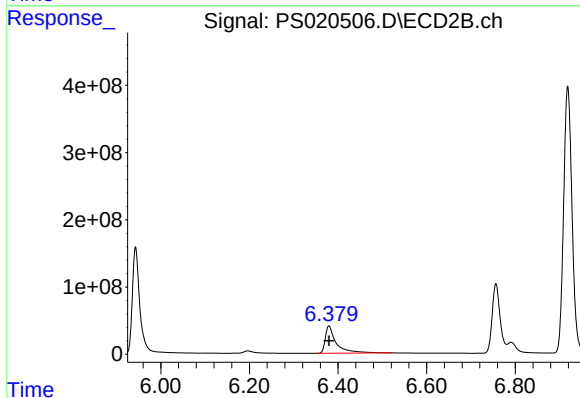


#3 4-Nitrophenol

R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 703572974
Conc: 1412.97 ng/ml

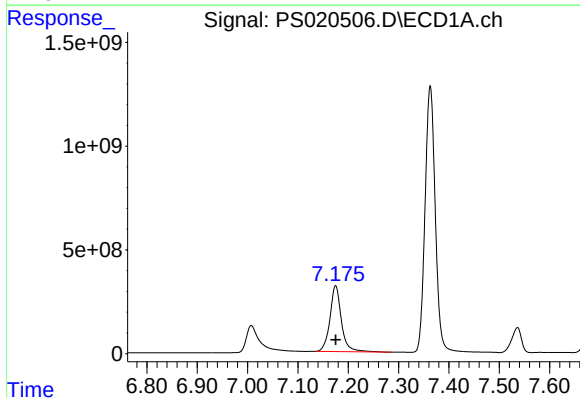


#4 2,4-DCAA

R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 5001655107
Conc: 1502.32 ng/ml

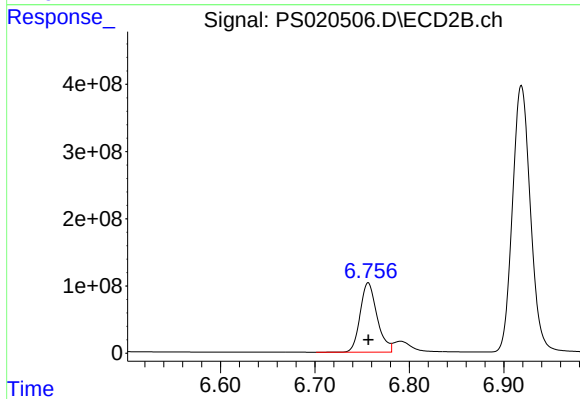

#4 2,4-DCAA


R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 1286207191
Conc: 1524.24 ng/ml

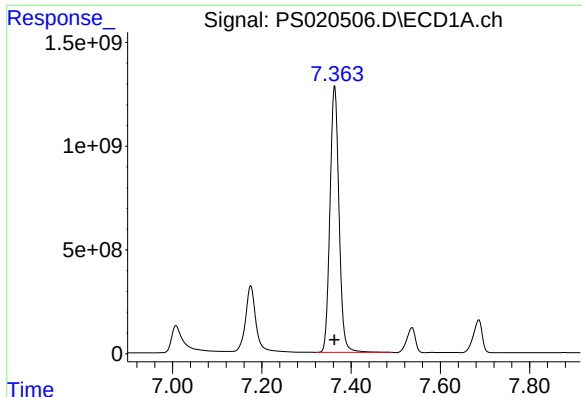

#5 DICAMBA


R.T.: 7.363 min
Delta R.T.: 0.000 min
Response: 18080957391
Conc: 1385.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

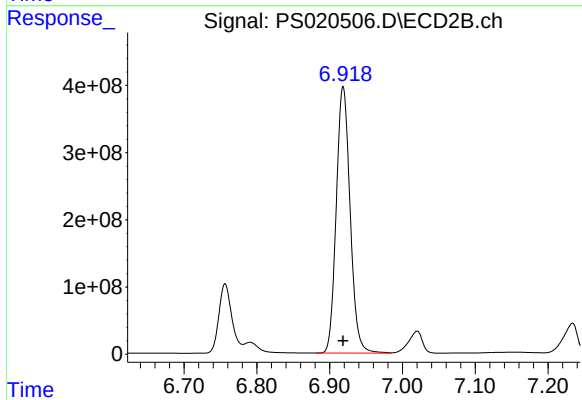


#5 DICAMBA

R.T.: 6.919 min
Delta R.T.: 0.000 min
Response: 5253122581
Conc: 1393.83 ng/ml

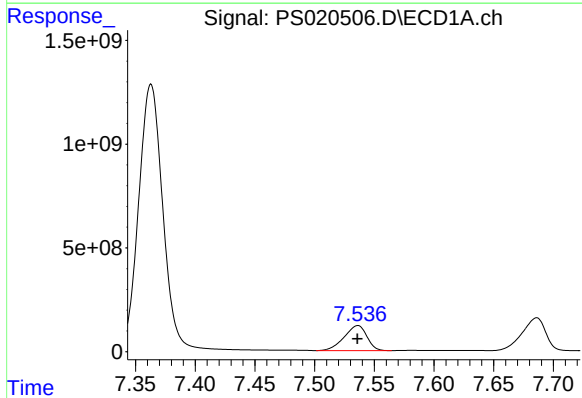


#6 MCP

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 1597534831
Conc: 147.64 ug/ml

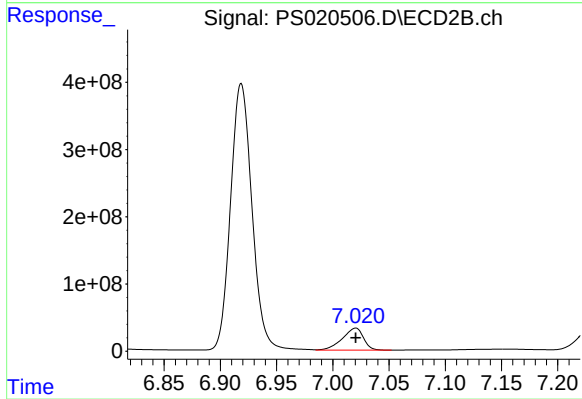

#6 MCP


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 429790492
Conc: 145.22 ug/ml

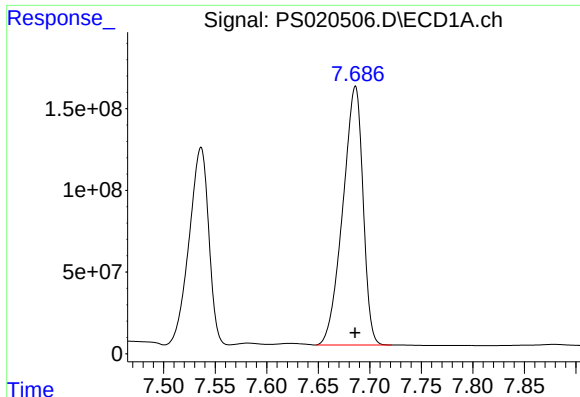

#7 MCPA


R.T.: 7.686 min
Delta R.T.: 0.000 min
Response: 2161494342
Conc: 144.04 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

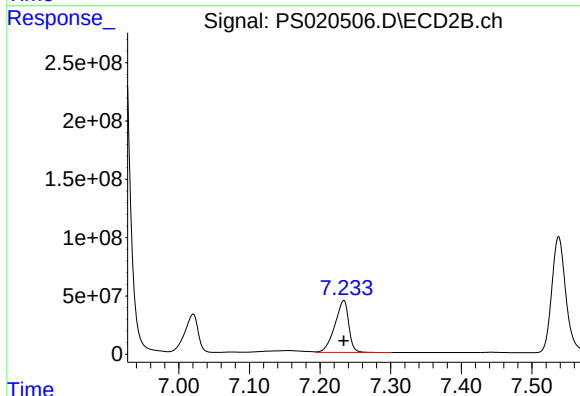


#7 MCPA

R.T.: 7.234 min
Delta R.T.: 0.000 min
Response: 608040820
Conc: 142.28 ug/ml

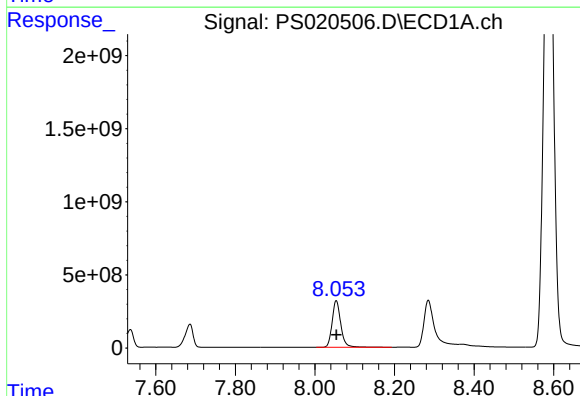


#8 DICHLORPROP

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 4812406050
Conc: 1406.15 ng/ml

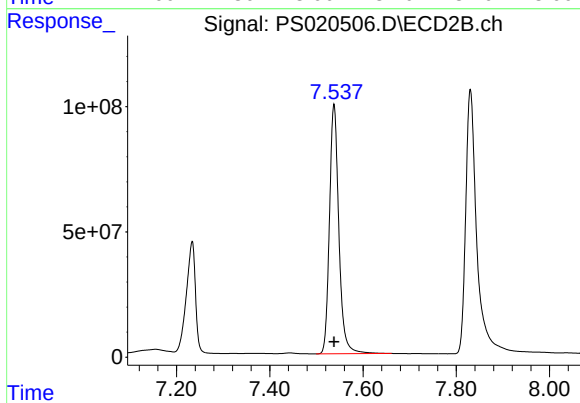

#8 DICHLORPROP


R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 1390437519
Conc: 1413.13 ng/ml

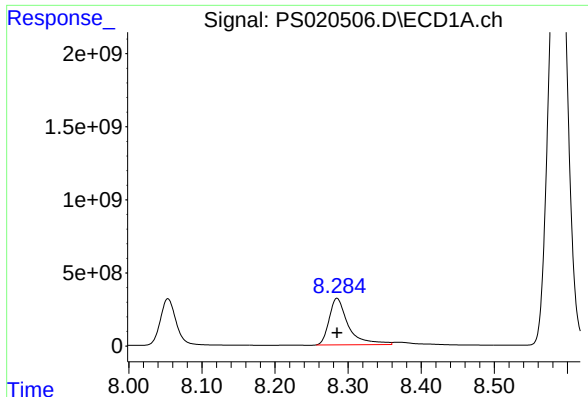

#9 2,4-D


R.T.: 8.285 min
Delta R.T.: 0.000 min
Response: 5816156430
Conc: 1342.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

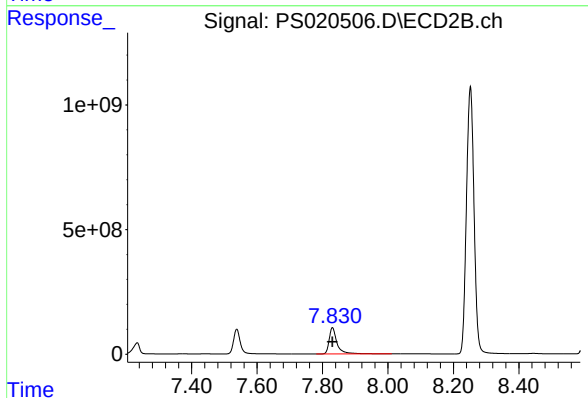


#9 2,4-D

R.T.: 7.830 min
Delta R.T.: 0.000 min
Response: 1761661904
Conc: 1407.01 ng/ml

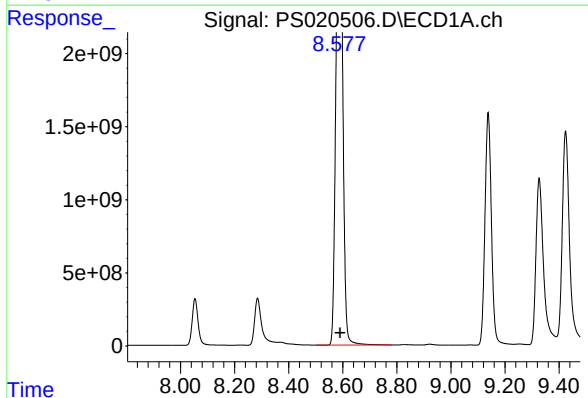


#10 Pentachlorophenol

R.T.: 8.590 min
Delta R.T.: 0.000 min
Response: 46949665232
Conc: 1183.97 ng/ml

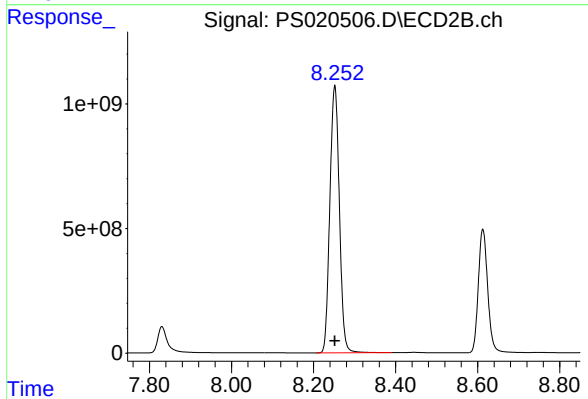

#10 Pentachlorophenol


R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 17213841950
Conc: 1324.88 ng/ml

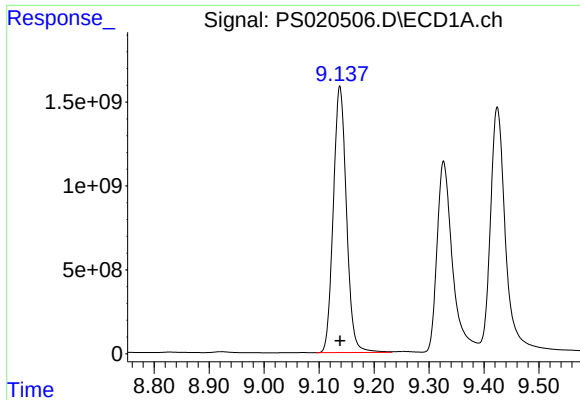

#11 2,4,5-TP (SILVEX)


R.T.: 9.138 min
Delta R.T.: 0.000 min
Response: 26421180313
Conc: 1386.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

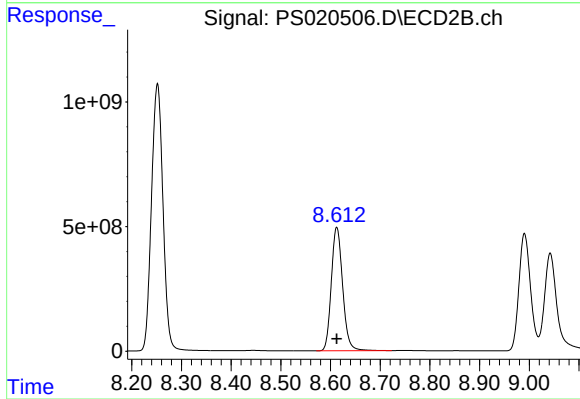


#11 2,4,5-TP (SILVEX)

R.T.: 8.613 min
Delta R.T.: 0.000 min
Response: 7841956345
Conc: 1384.00 ng/ml

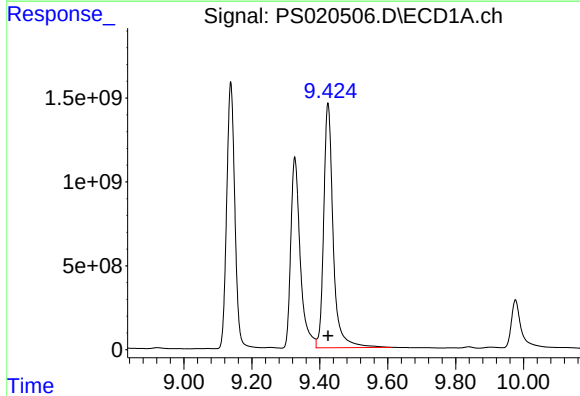


#12 2,4,5-T

R.T.: 9.424 min
Delta R.T.: 0.000 min
Response: 28276288942
Conc: 1378.98 ng/ml

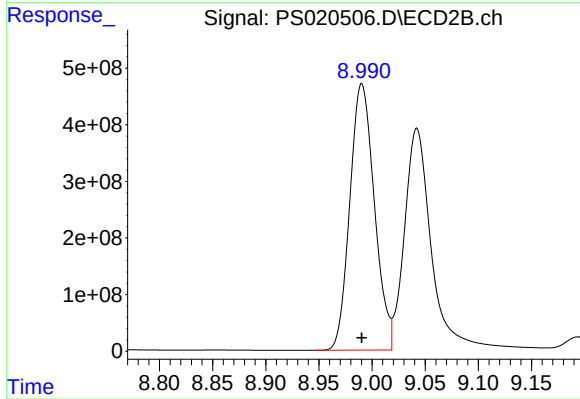

#12 2,4,5-T


R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 7564294390
Conc: 1405.50 ng/ml

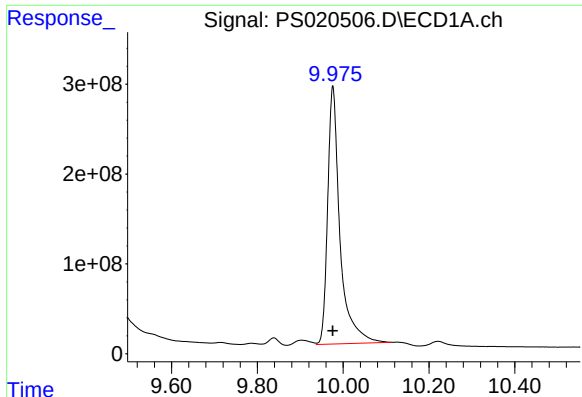

#13 2,4-DB


R.T.: 9.976 min
Delta R.T.: 0.000 min
Response: 5717945864
Conc: 1493.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

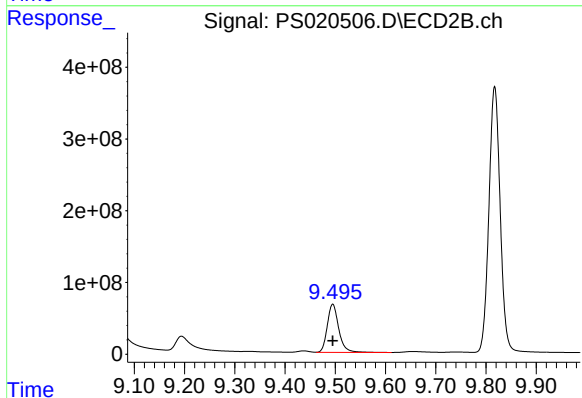


#13 2,4-DB

R.T.: 9.495 min
Delta R.T.: 0.000 min
Response: 1058622689
Conc: 1462.43 ng/ml

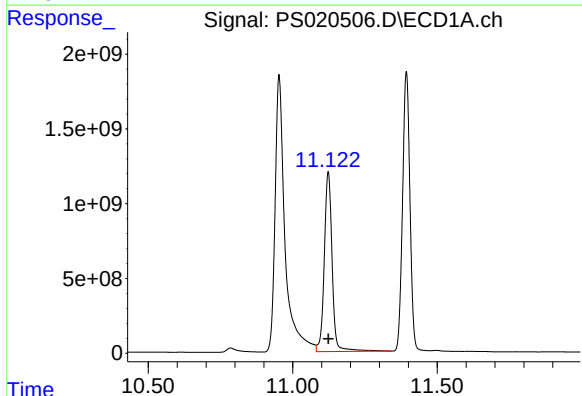


#14 DINOSEB

R.T.: 11.123 min
Delta R.T.: 0.000 min
Response: 22604863528
Conc: 1365.74 ng/ml

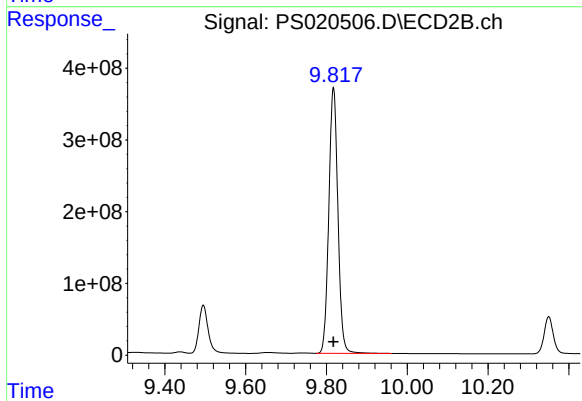

#14 DINOSEB


R.T.: 9.817 min
Delta R.T.: 0.000 min
Response: 5787590287
Conc: 1388.52 ng/ml

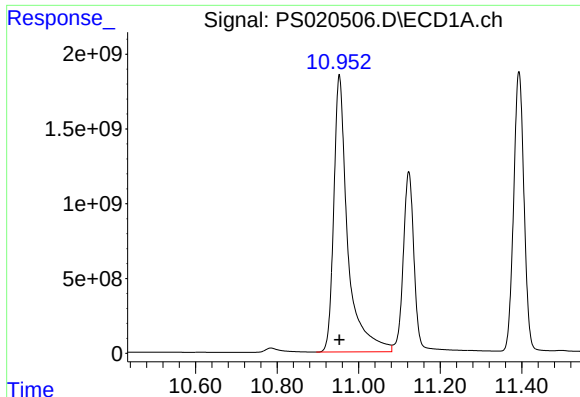

#15 Picloram


R.T.: 10.953 min
Delta R.T.: 0.000 min
Response: 44122665688
Conc: 1438.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

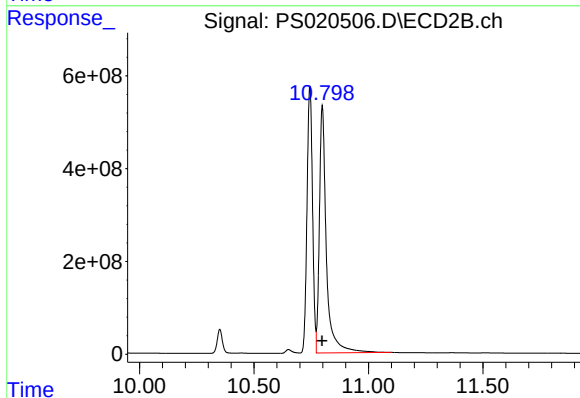


#15 Picloram

R.T.: 10.798 min
Delta R.T.: 0.000 min
Response: 11394215490
Conc: 1416.07 ng/ml

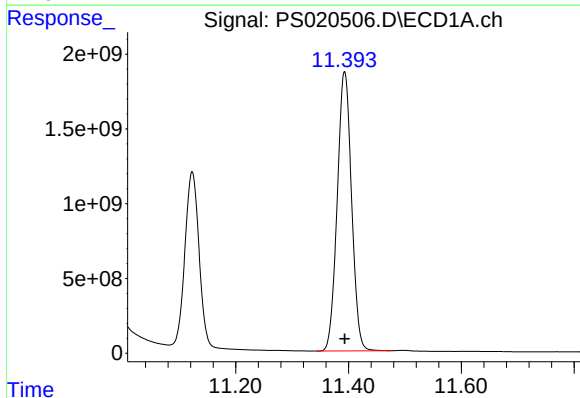

#16 DCPA

R.T.: 11.393 min
Delta R.T.: 0.000 min
Response: 32896851830
Conc: 1392.53 ng/ml

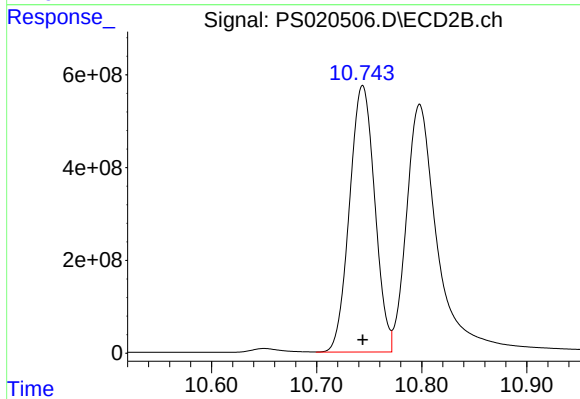

#16 DCPA

R.T.: 10.744 min
Delta R.T.: 0.000 min
Response: 9590987870
Conc: 1381.15 ng/ml