

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
 Data File : PS020515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 00:26
 Operator : AJ\MA
 Sample : N4572-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PSC-124035

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/14/2022
 Supervised By : Ankita Jodhani 09/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 02:57:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 7.169 6.762 1230.4E6 961.5E6 357.534m 1128.975 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091322\
Data File : PS020515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 00:26
Operator : AJ\MA
Sample : N4572-07
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PSC-124035


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/14/2022
Supervised By : Ankita Jodhani 09/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 02:57:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

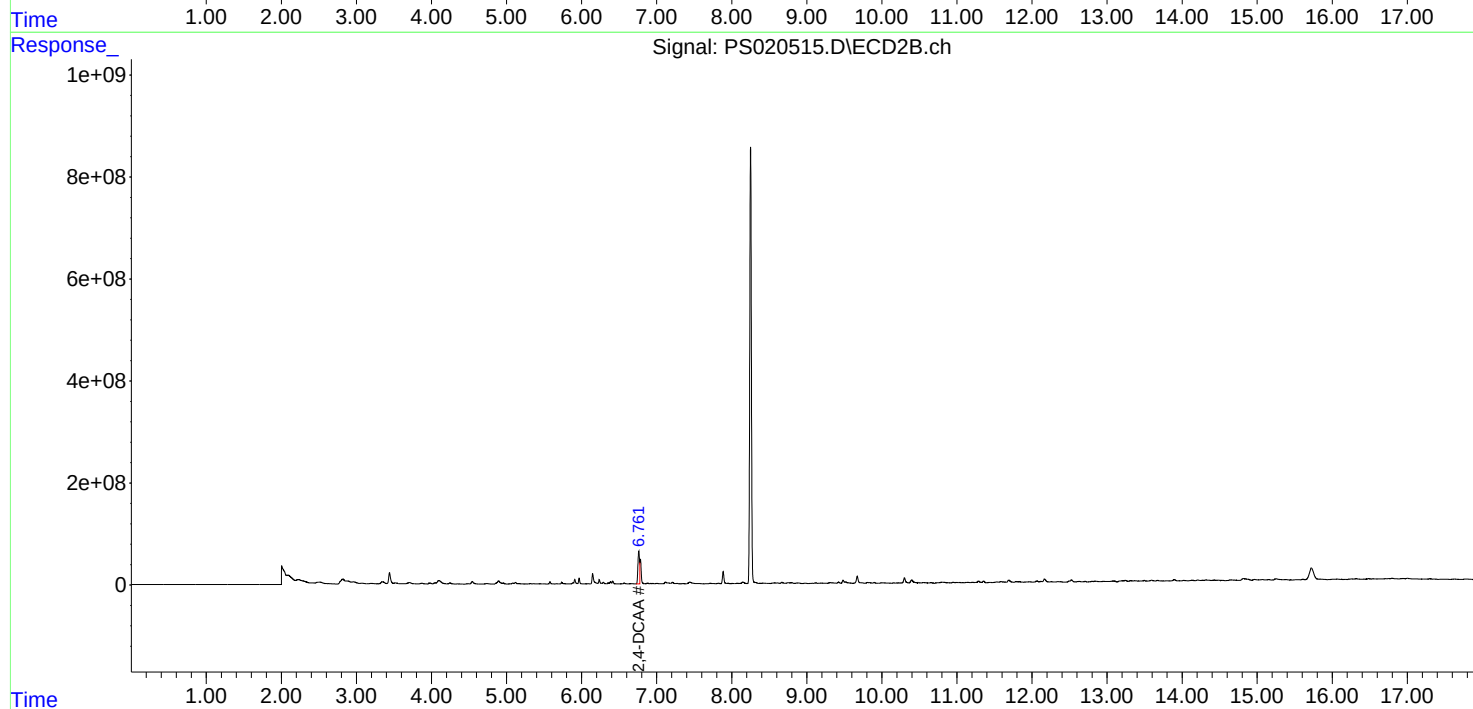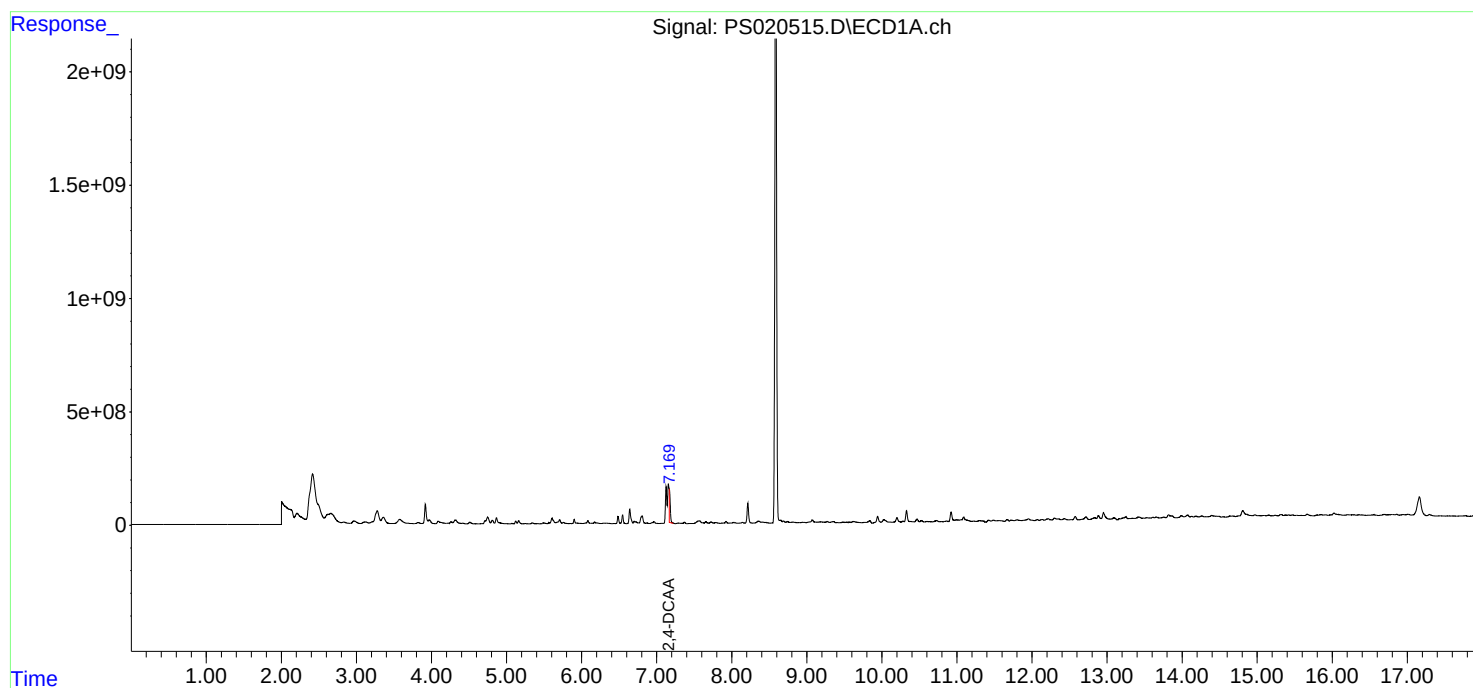

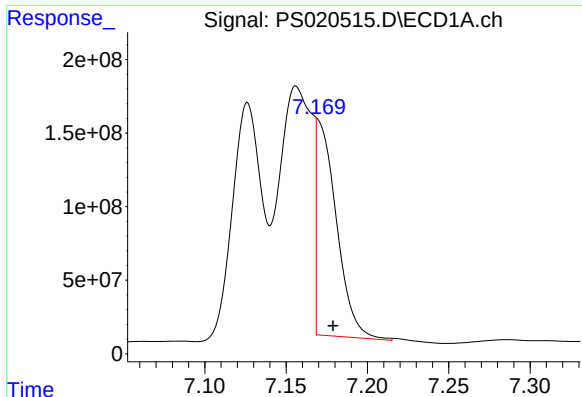

#4 2,4-DCAA

R.T.: 7.169 min
Delta R.T.: -0.010 min
Response: 1230447543
Conc: 357.53 ng/ml

Instrument :

ECD_S

ClientSampleId :


PSC-124035

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 09/14/2022

Supervised By :Ankita Jodhani 09/14/2022

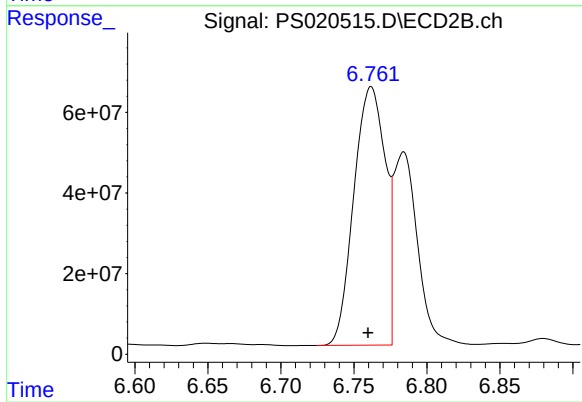

#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: 0.002 min
Response: 961542908
Conc: 1128.98 ng/ml