

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS091418\  
 Data File : PS001737.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Sep 2018 13:19  
 Operator : EI\SJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 14 23:02:42 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS082218.M  
 Quant Title : 8080.M  
 QLast Update : Thu Aug 23 02:55:24 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

##### Target Compounds

|       |             |        |        |         |         |        |         |
|-------|-------------|--------|--------|---------|---------|--------|---------|
| 1) T  | Dalapon     | 3.019  | 2.459  | 1971202 | 1193844 | 7.842  | 4.988 # |
| 6) T  | MCPP        | 0.000  | 11.440 | 0       | 801707  | N.D.   | 1.741 # |
| 8) T  | DICHLORPROP | 12.971 | 0.000  | 4562716 | 0       | 24.161 | N.D. #  |
| 15) T | Picloram    | 16.973 | 0.000  | 2334001 | 0       | 1.666  | N.D. #  |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS091418\  
Data File : PS001737.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Sep 2018 13:19  
Operator : EI\SJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 14 23:02:42 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS082218.M  
Quant Title : 8080.M  
QLast Update : Thu Aug 23 02:55:24 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

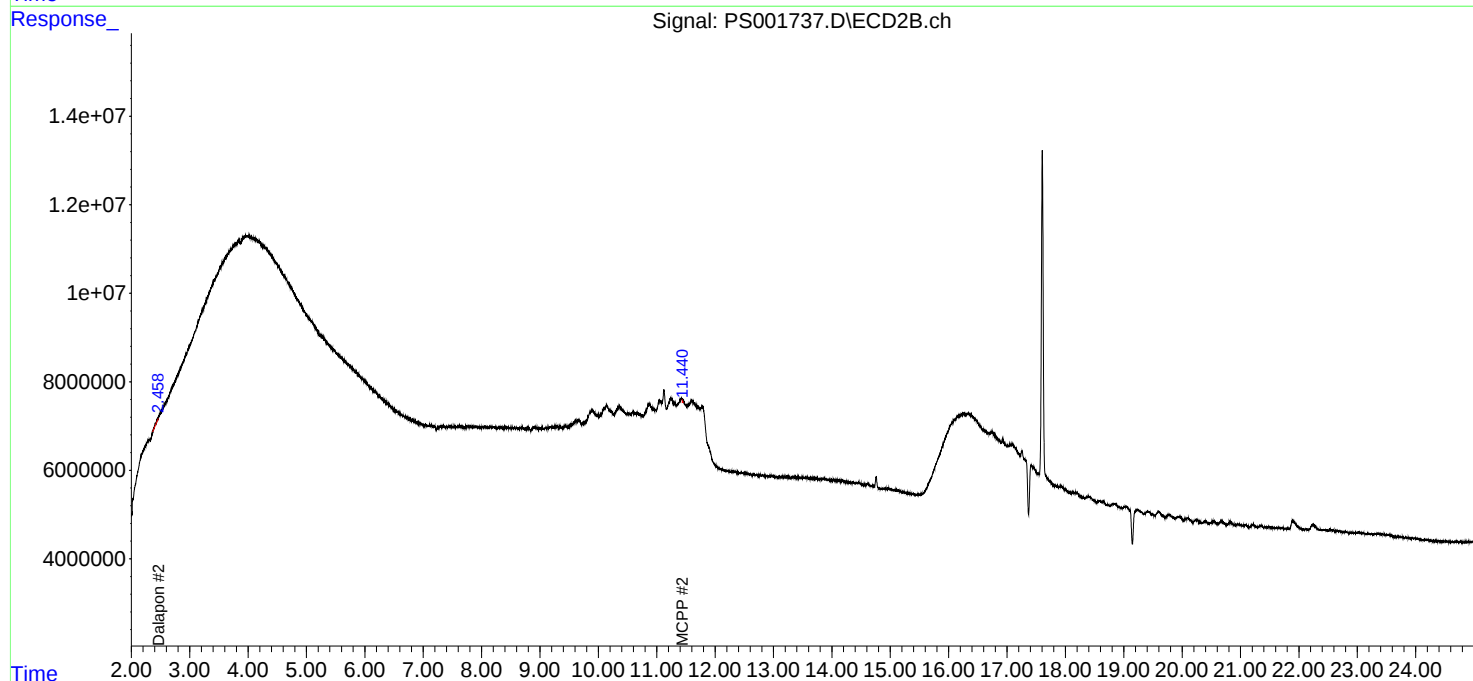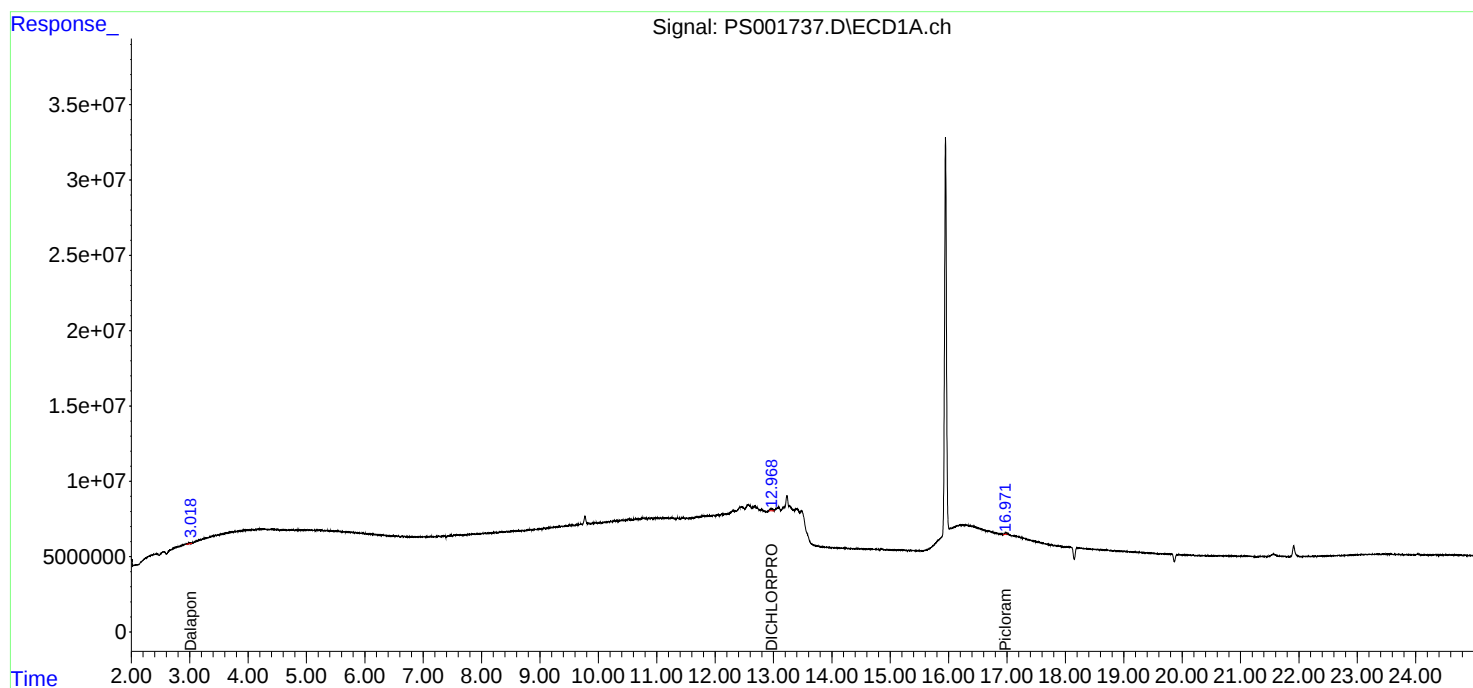


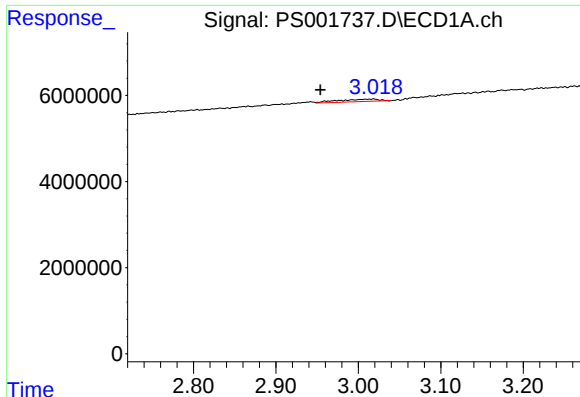

#1 Dalapon


R.T.: 3.019 min  
Delta R.T.: 0.065 min  
Response: 1971202  
Conc: 7.84 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

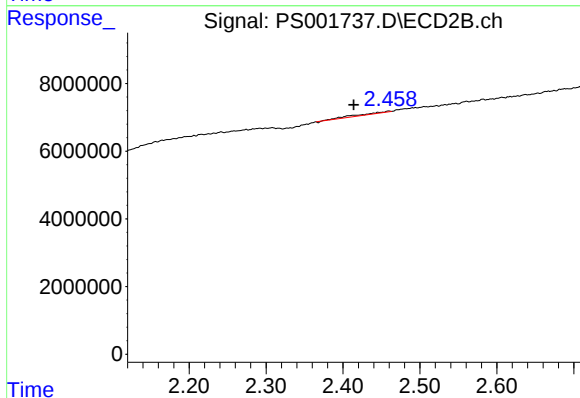


#1 Dalapon

R.T.: 2.459 min  
Delta R.T.: 0.045 min  
Response: 1193844  
Conc: 4.99 ng/ml

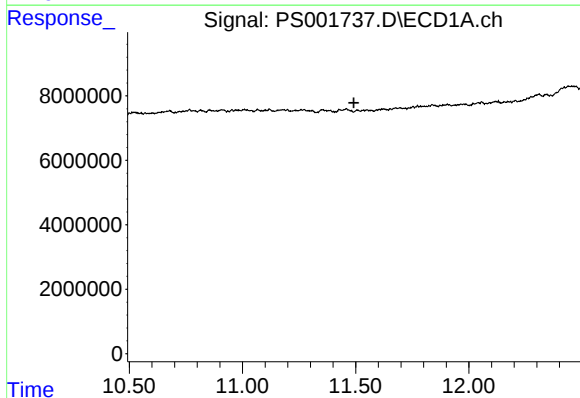


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 11.492 min  
Response: 0  
Conc: N.D.

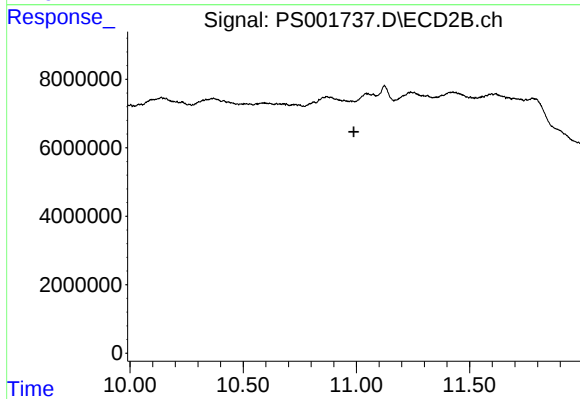

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T. : 10.989 min  
Response: 0  
Conc: N.D.

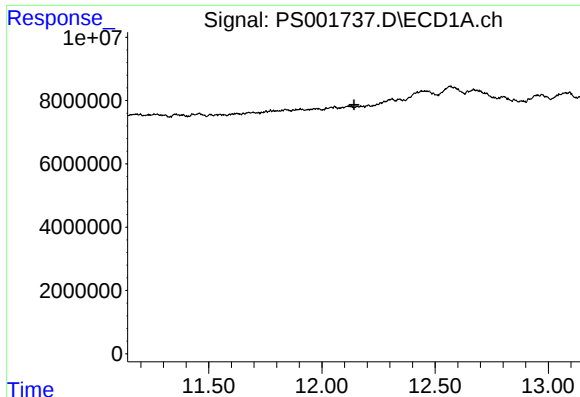

#6 MCP


R.T.: 0.000 min  
Exp R.T.: 12.142 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

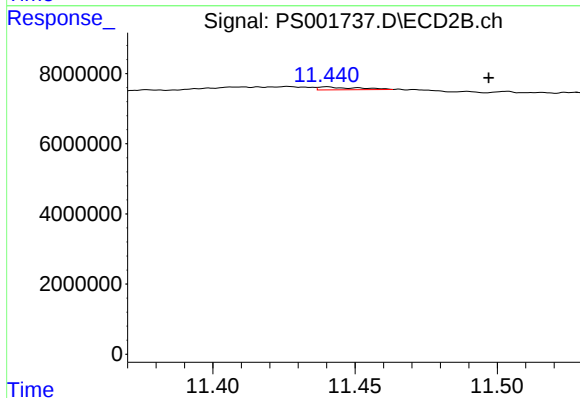


#6 MCP

R.T.: 11.440 min  
Delta R.T.: -0.057 min  
Response: 801707  
Conc: 1.74 ug/ml

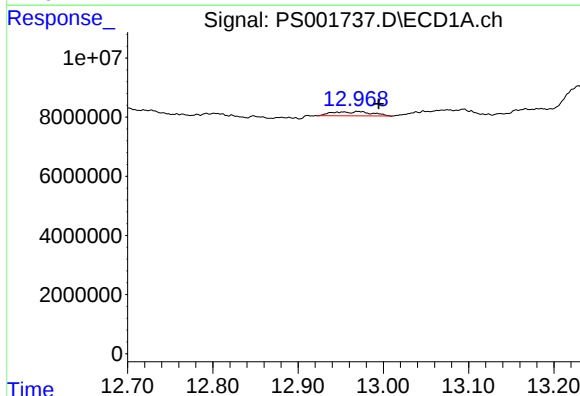


#8 DICHLORPROP

R.T.: 12.971 min  
Delta R.T.: -0.023 min  
Response: 4562716  
Conc: 24.16 ng/ml

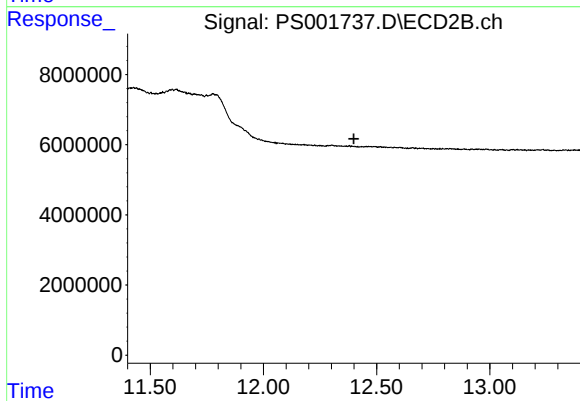

#8 DICHLORPROP


R.T.: 0.000 min  
Exp R.T.: 12.399 min  
Response: 0  
Conc: N.D.

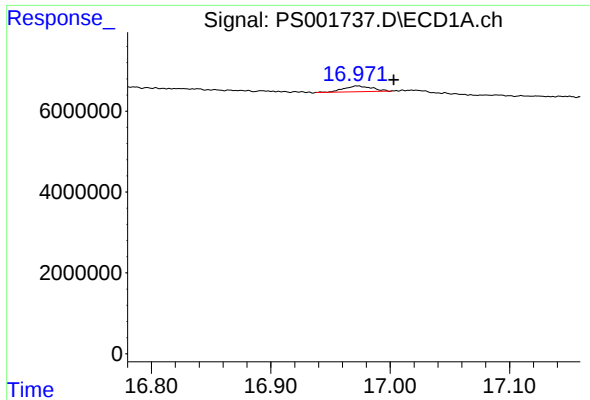

#15 Picloram

R.T.: 16.973 min  
Delta R.T.: -0.030 min  
Response: 2334001  
Conc: 1.67 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

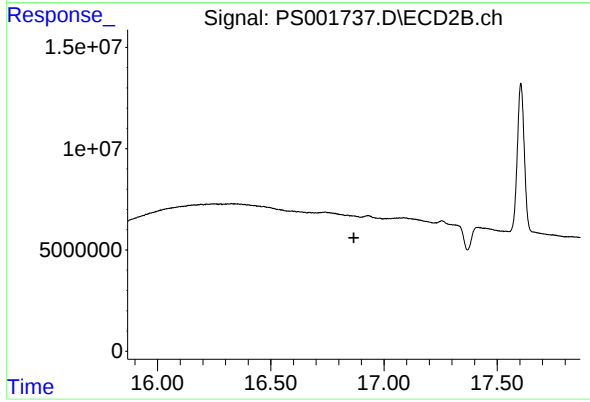

#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 16.867 min  
Response: 0  
Conc: N.D.