

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001740.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 16:31
 Operator : EI\SJ
 Sample : PB112847BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:03:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.480	10.969	97988091	85420228	530.812	421.766
Target Compounds							
2) T	3,5-DICHL...	0.000	9.205	0	32823119	N.D.	128.439 #
3) T	4-Nitroph...	0.000	10.138	0	1038624	N.D.	9.854 #
5) T	DICAMBA	0.000	11.212	0	980395	N.D.	1.398 #
6) T	MCP	12.168	0.000	16372111	0	32.538	N.D. #
9) T	2,4-D	13.386	0.000	9408458	0	39.678	N.D. #
12) T	2,4,5-T	0.000	14.591	0	2489234	N.D.	2.882 #
14) T	DINOSEB	0.000	15.665	0	2914766	N.D.	3.941 #
15) T	Picloram	17.000	16.857	13136846	27543936	9.379	21.123 #
16) T	DCPA	0.000	16.911	0	50267237	N.D.	35.207 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001740.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 16:31
Operator : EI\SJ
Sample : PB112847BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:03:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

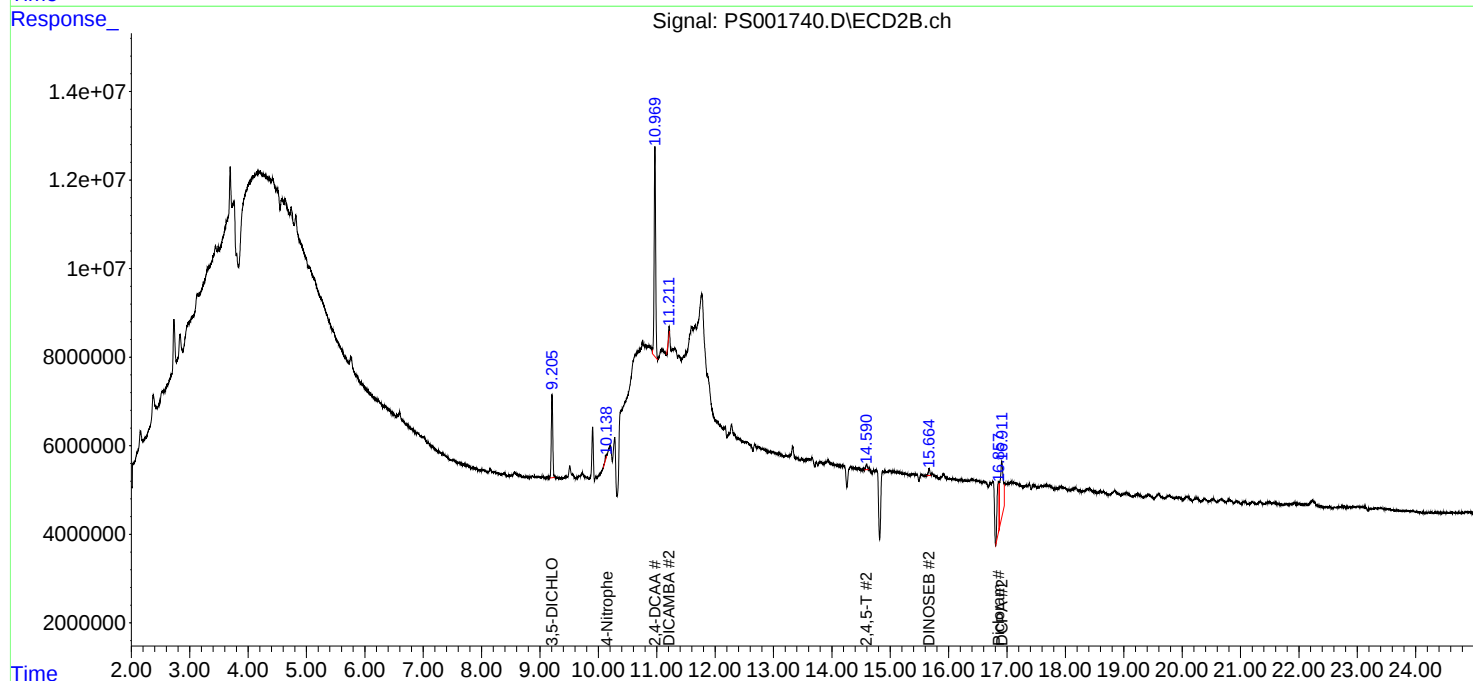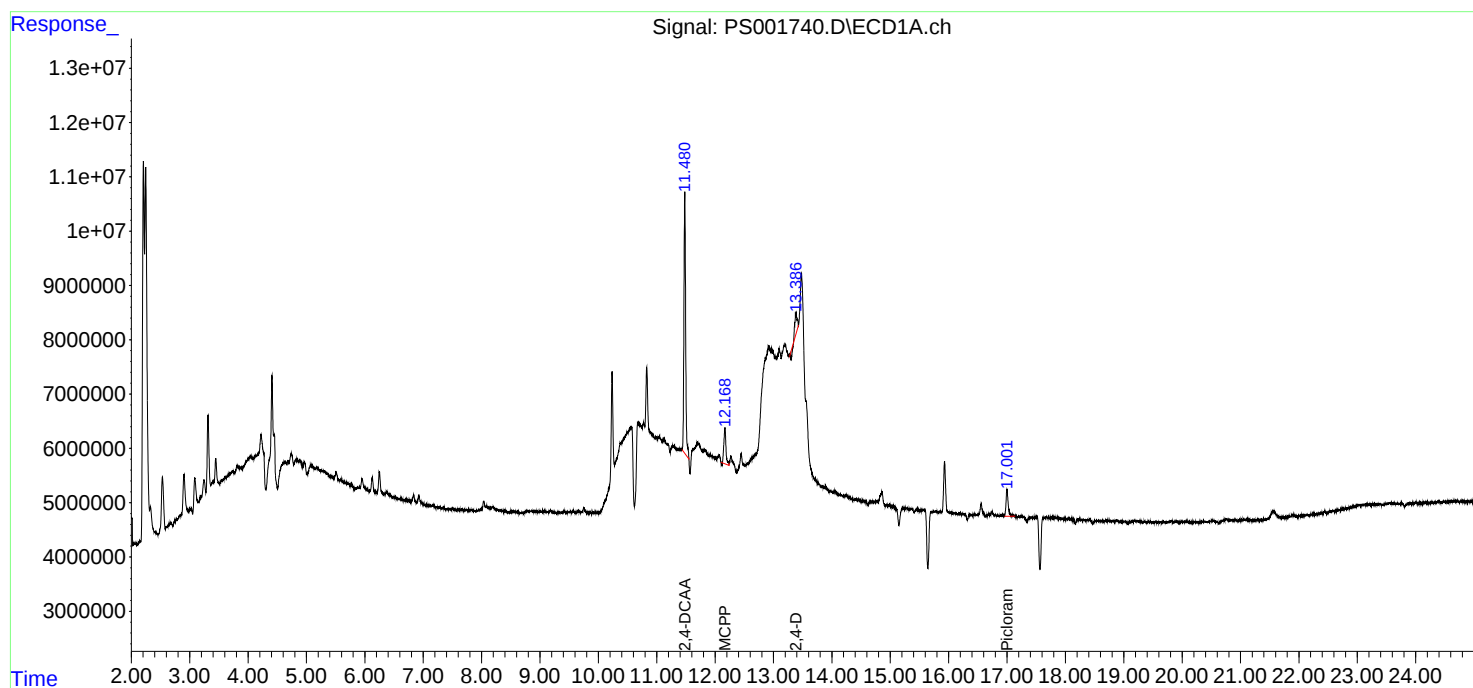


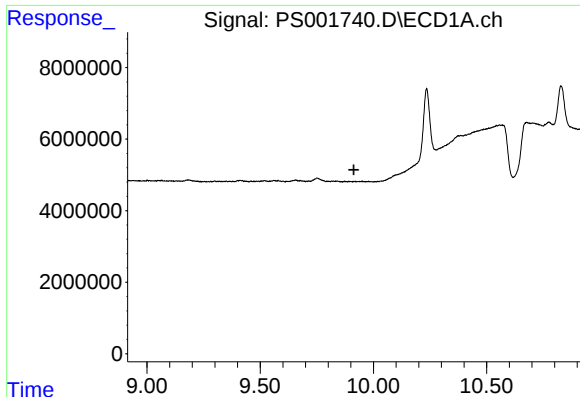

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

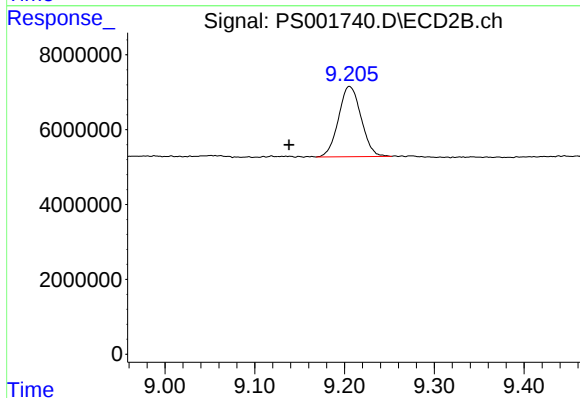


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.205 min
Delta R.T.: 0.067 min
Response: 32823119
Conc: 128.44 ng/ml

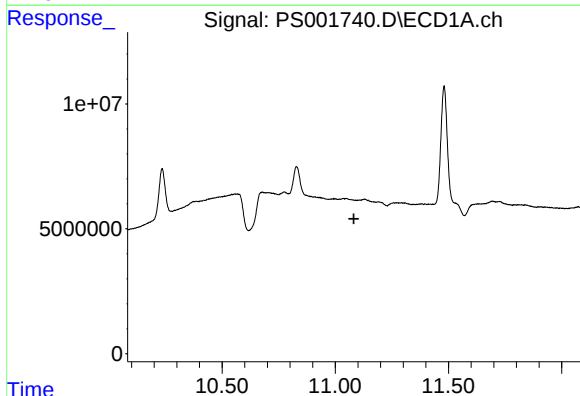


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.082 min
Response: 0
Conc: N.D.

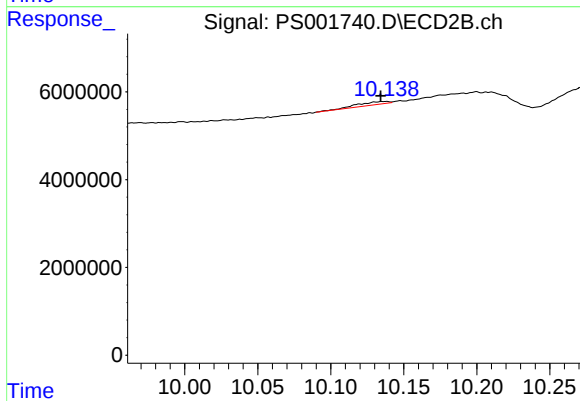

#3 4-Nitrophenol


R.T.: 10.138 min
Delta R.T.: 0.004 min
Response: 1038624
Conc: 9.85 ng/ml

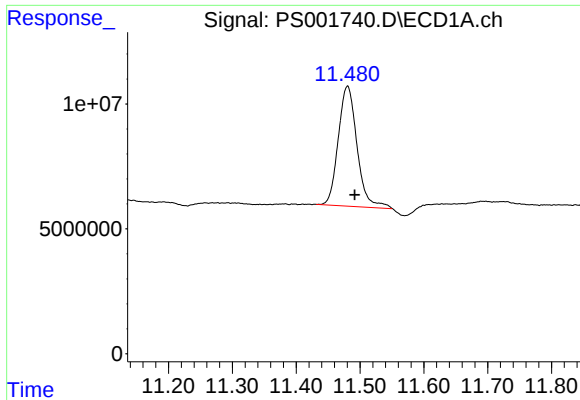

#4 2,4-DCAA


R.T.: 11.480 min
Delta R.T.: -0.011 min
Response: 97988091
Conc: 530.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

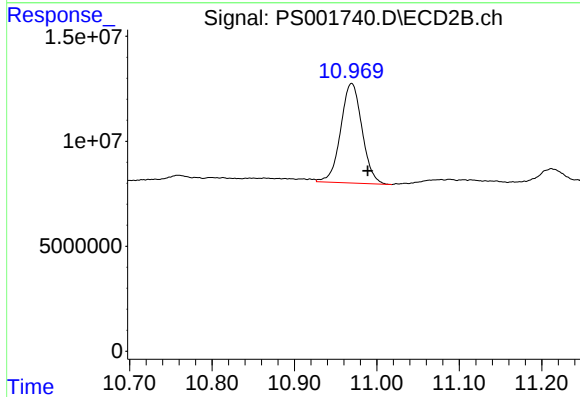


#4 2,4-DCAA

R.T.: 10.969 min
Delta R.T.: -0.019 min
Response: 85420228
Conc: 421.77 ng/ml

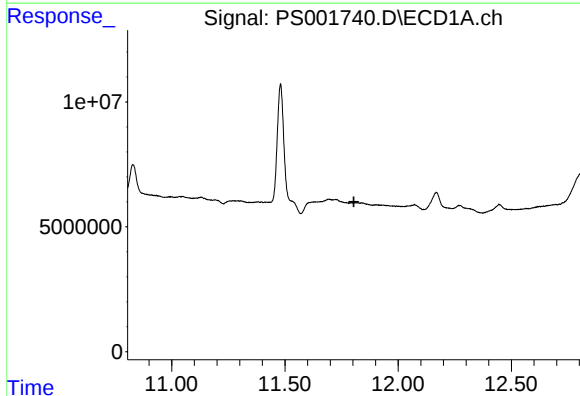


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

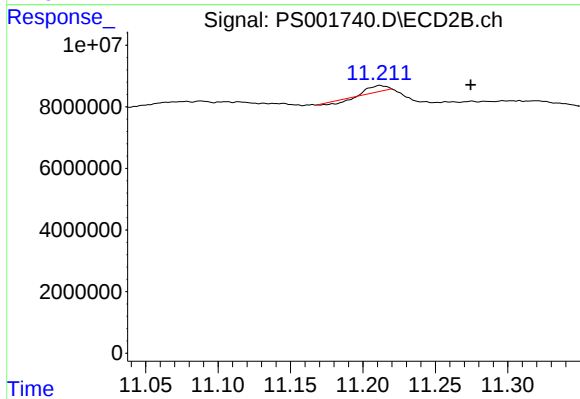

#5 DICAMBA


R.T.: 11.212 min
Delta R.T.: -0.063 min
Response: 980395
Conc: 1.40 ng/ml

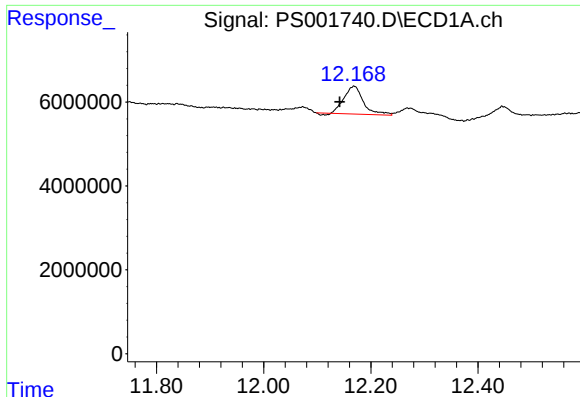

#6 MCPP


R.T.: 12.168 min
Delta R.T.: 0.027 min
Response: 16372111
Conc: 32.54 ug/ml

Instrument :
ECD_S
ClientSampleId :

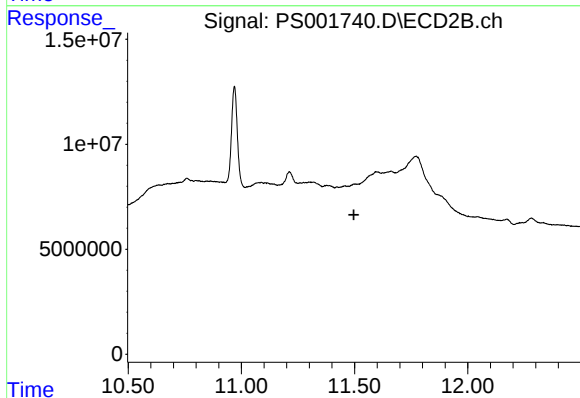


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

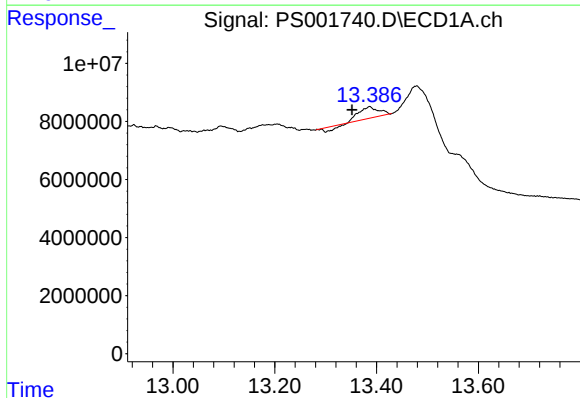


#9 2,4-D

R.T.: 13.386 min
Delta R.T.: 0.035 min
Response: 9408458
Conc: 39.68 ng/ml

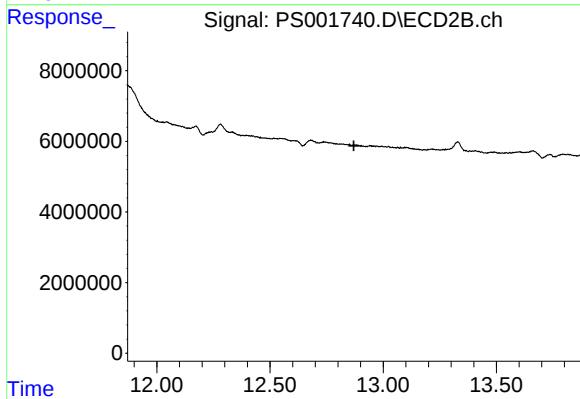

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 12.871 min
Response: 0
Conc: N.D.

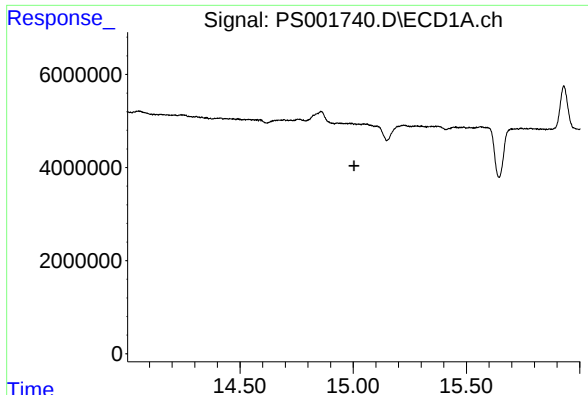

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

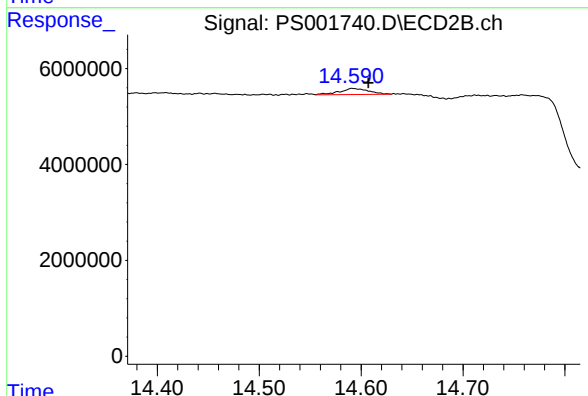


#12 2,4,5-T

R.T.: 14.591 min
Delta R.T.: -0.016 min
Response: 2489234
Conc: 2.88 ng/ml

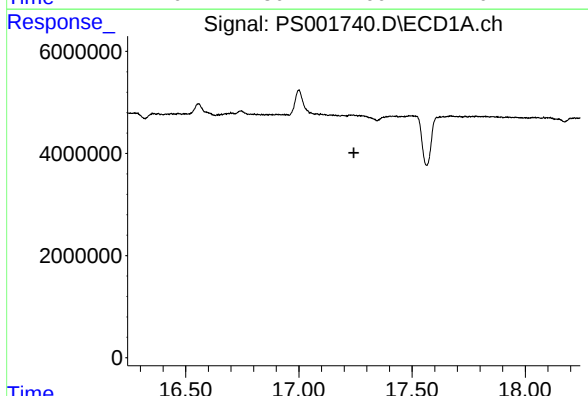


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.243 min
Response: 0
Conc: N.D.

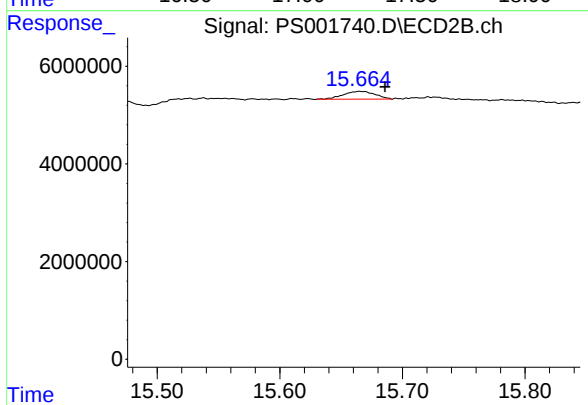

#14 DINOSEB


R.T.: 15.665 min
Delta R.T.: -0.021 min
Response: 2914766
Conc: 3.94 ng/ml

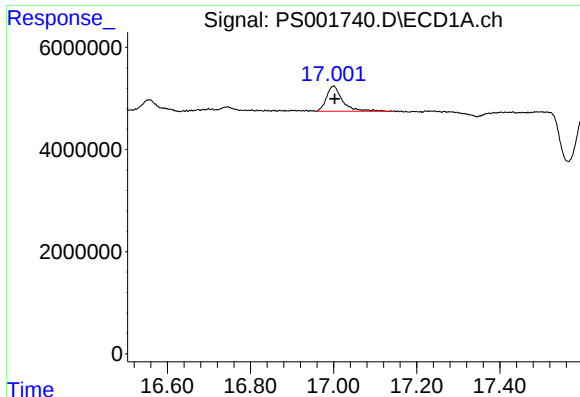

#15 Picloram


R.T.: 17.000 min
Delta R.T.: -0.003 min
Response: 13136846
Conc: 9.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

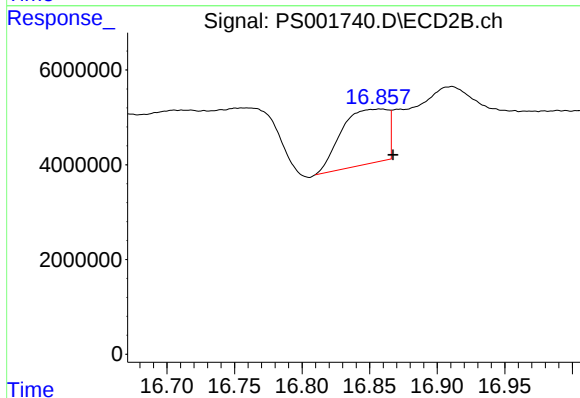


#15 Picloram

R.T.: 16.857 min
Delta R.T.: -0.010 min
Response: 27543936
Conc: 21.12 ng/ml

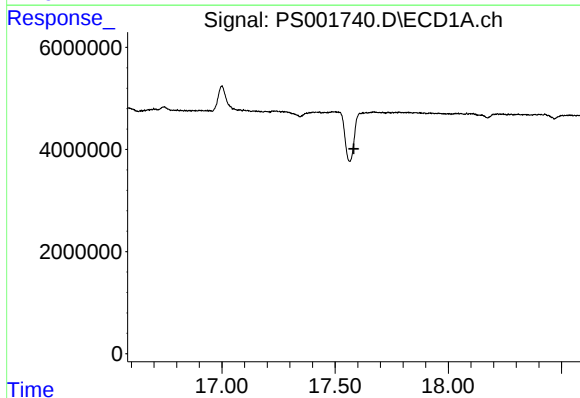

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

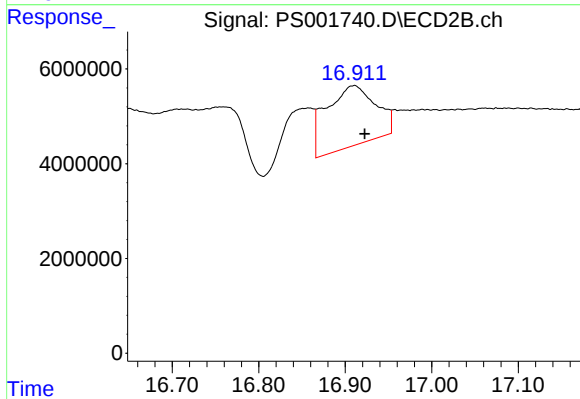

#16 DCPA

R.T.: 16.911 min
Delta R.T.: -0.011 min
Response: 50267237
Conc: 35.21 ng/ml