

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 17:34
 Operator : EI\SJ
 Sample : PB112847TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:03:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.500	10.998	75919176	70589963	411.262	348.541
Target Compounds							
1) T	Dalapon	2.924	2.407	11489599	17391324	45.707	72.667 #
3) T	4-Nitroph...	11.151	10.086	6587979	6724098	53.434	63.794
5) T	DICAMBA	0.000	11.241	0	7158912	N.D.	10.207 #
6) T	MCP	12.186	0.000	13391872	0	26.615	N.D. #
11) T	2,4,5-TP ...	0.000	13.972	0	10324921	N.D.	9.714 #
15) T	Picloram	17.014	16.870	3514747	-263342	2.509	N.D. #
16) T	DCPA	0.000	16.932	0	8089317	N.D.	5.666 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 17:34
Operator : EI\SJ
Sample : PB112847TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:03:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

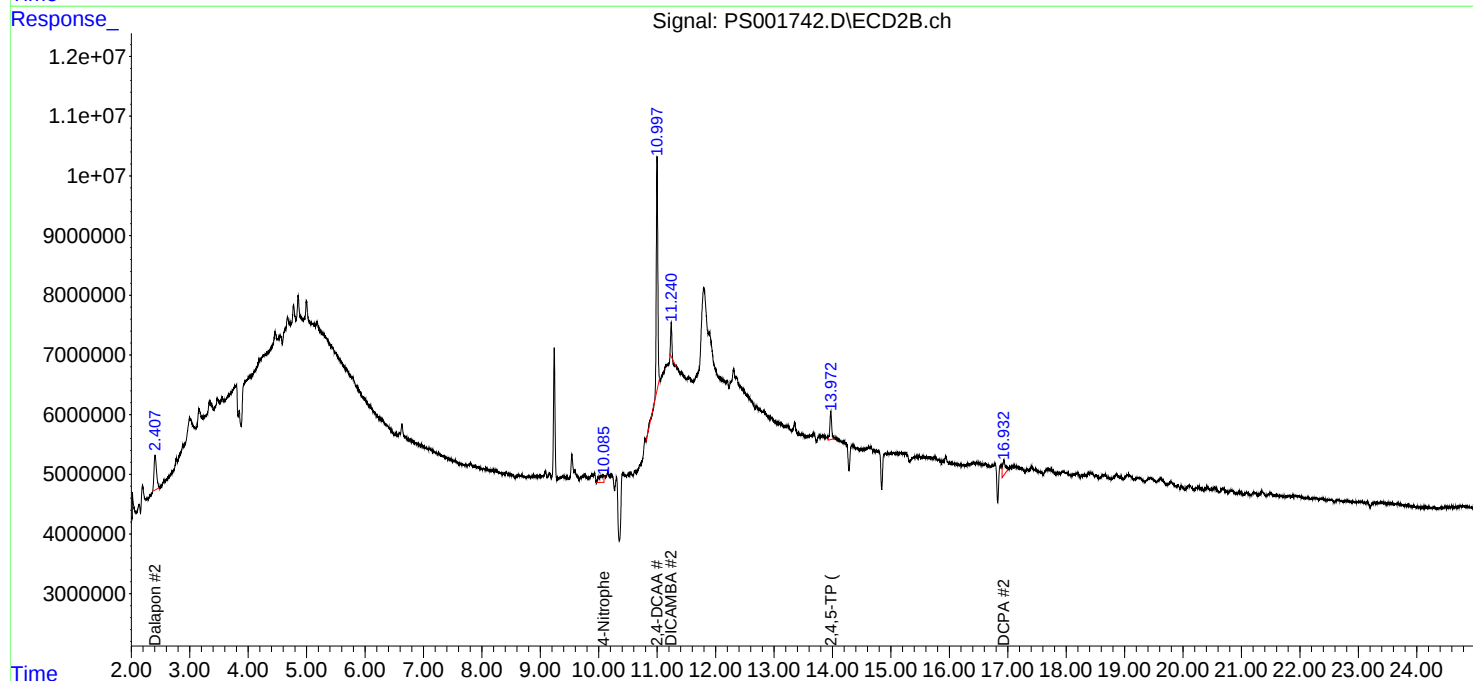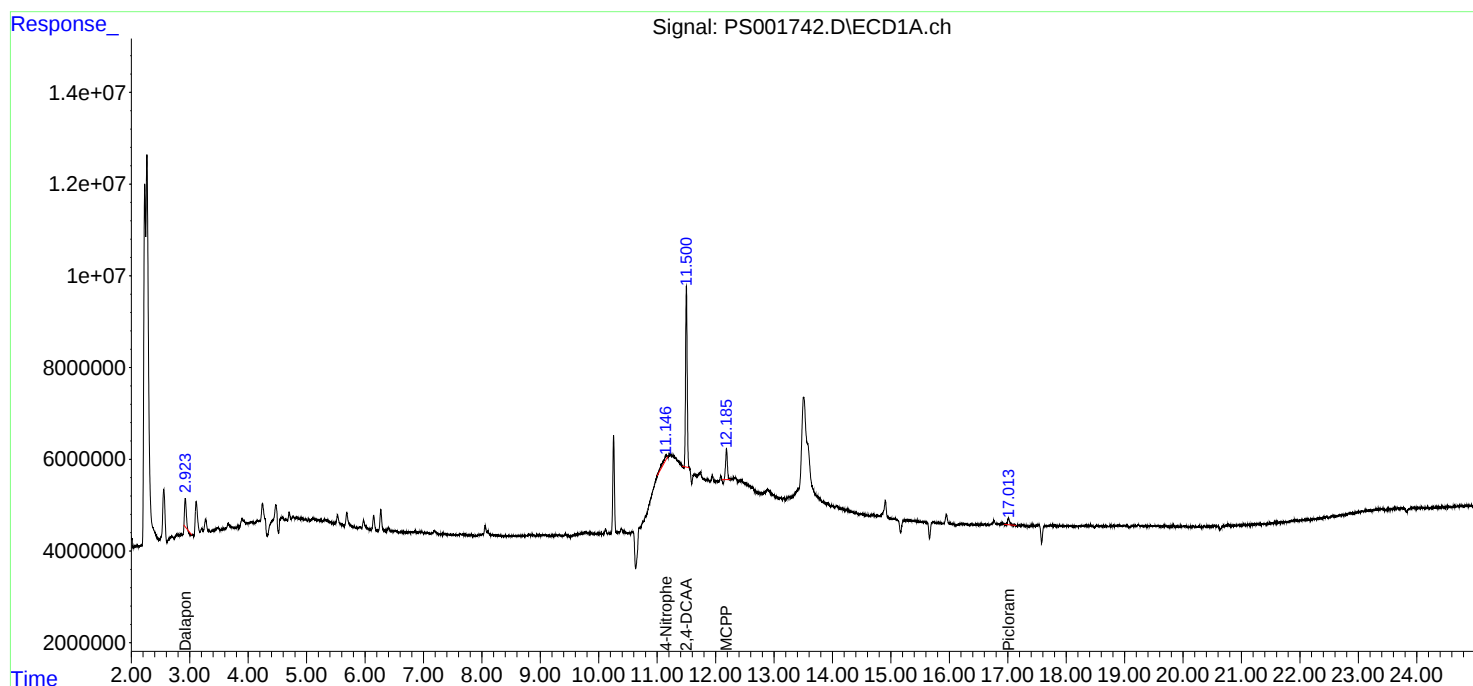


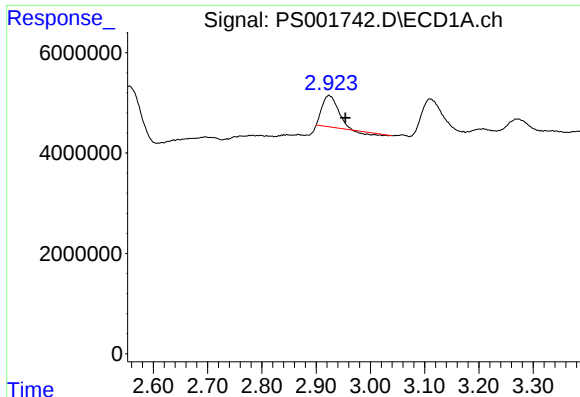

#1 Dalapon


R.T.: 2.924 min
Delta R.T.: -0.030 min
Response: 11489599
Conc: 45.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

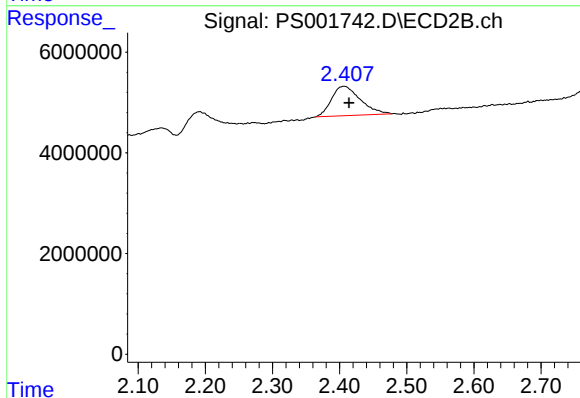


#1 Dalapon

R.T.: 2.407 min
Delta R.T.: -0.007 min
Response: 17391324
Conc: 72.67 ng/ml

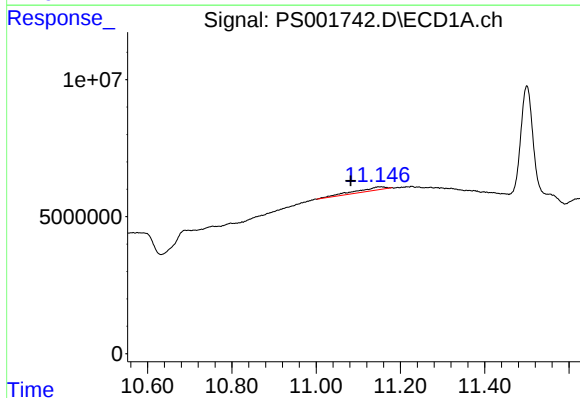


#3 4-Nitrophenol

R.T.: 11.151 min
Delta R.T.: 0.069 min
Response: 6587979
Conc: 53.43 ng/ml

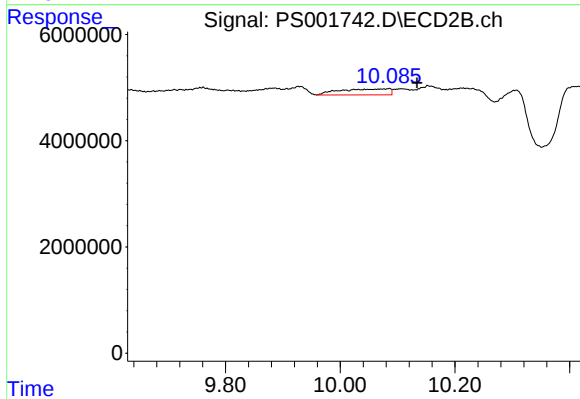

#3 4-Nitrophenol


R.T.: 10.086 min
Delta R.T.: -0.048 min
Response: 6724098
Conc: 63.79 ng/ml

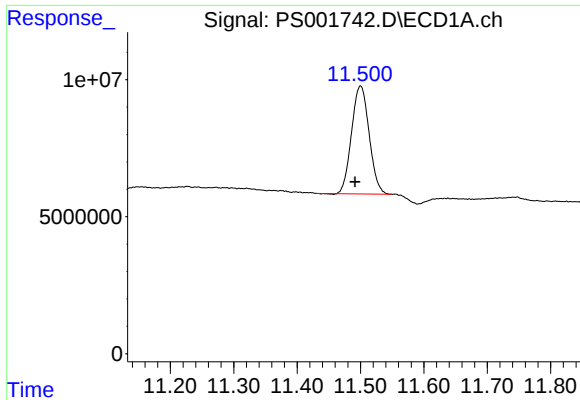

#4 2,4-DCAA


R.T.: 11.500 min
Delta R.T.: 0.008 min
Response: 75919176
Conc: 411.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

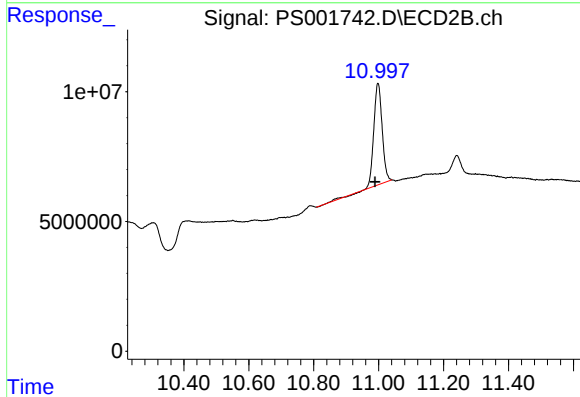


#4 2,4-DCAA

R.T.: 10.998 min
Delta R.T.: 0.009 min
Response: 70589963
Conc: 348.54 ng/ml

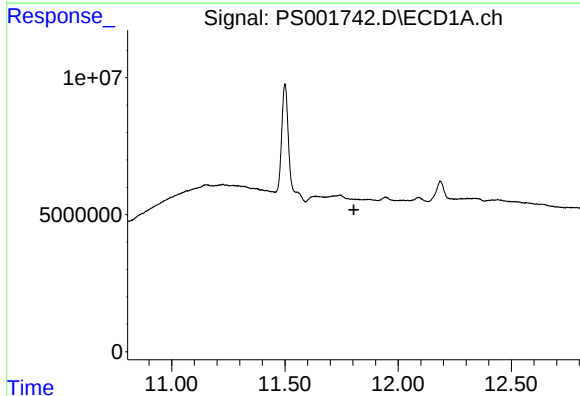


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

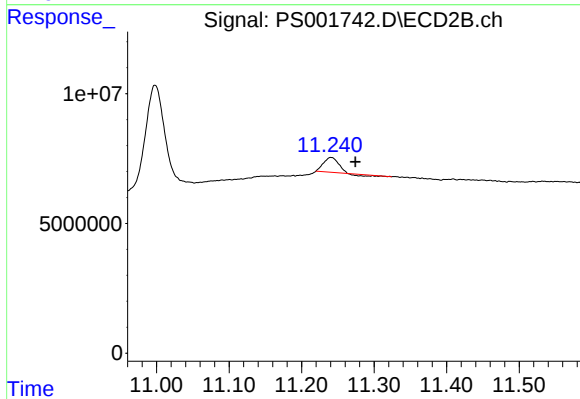

#5 DICAMBA


R.T.: 11.241 min
Delta R.T.: -0.034 min
Response: 7158912
Conc: 10.21 ng/ml

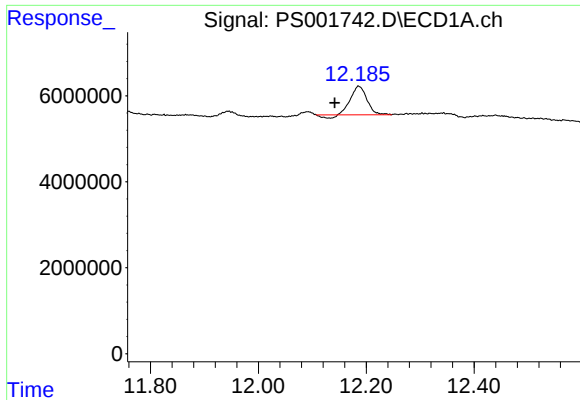

#6 MCP


R.T.: 12.186 min
Delta R.T.: 0.044 min
Response: 13391872
Conc: 26.62 ug/ml

Instrument :
ECD_S
ClientSampleId :

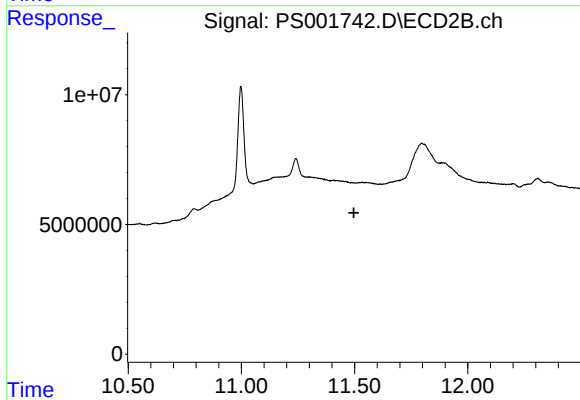


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

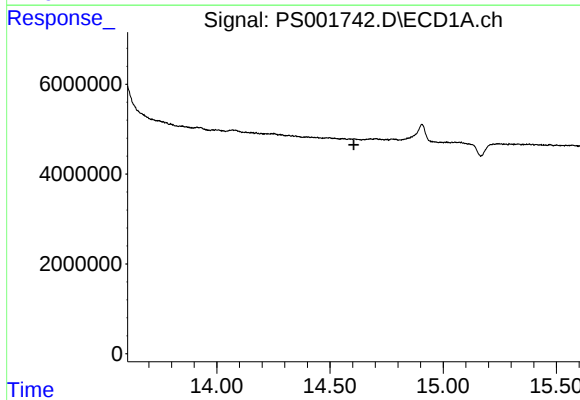


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.606 min
Response: 0
Conc: N.D.

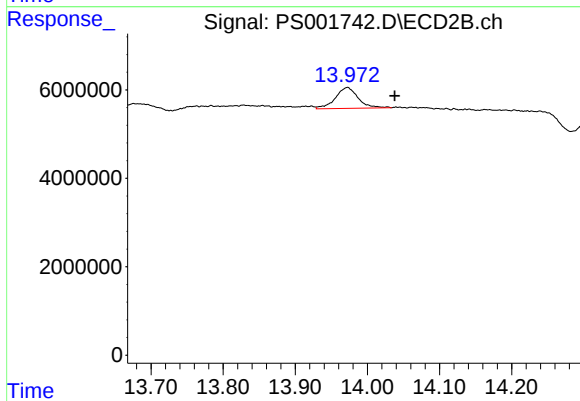

#11 2,4,5-TP (SILVEX)


R.T.: 13.972 min
Delta R.T.: -0.066 min
Response: 10324921
Conc: 9.71 ng/ml

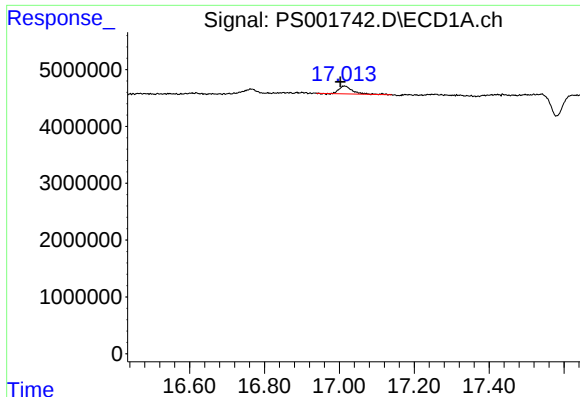

#15 Picloram


R.T.: 17.014 min
Delta R.T.: 0.011 min
Response: 3514747
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

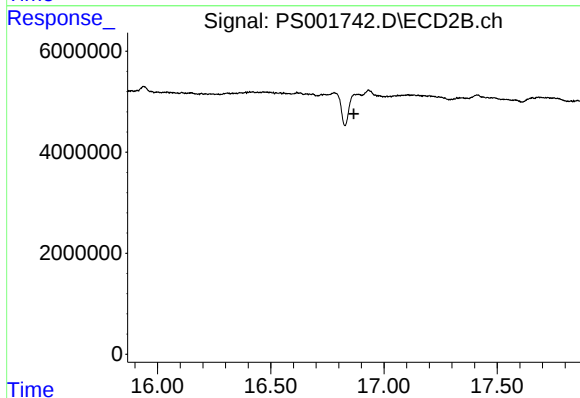


#15 Picloram

R.T.: 16.870 min
Delta R.T.: 0.002 min
Response: -263342
Conc: N.D.

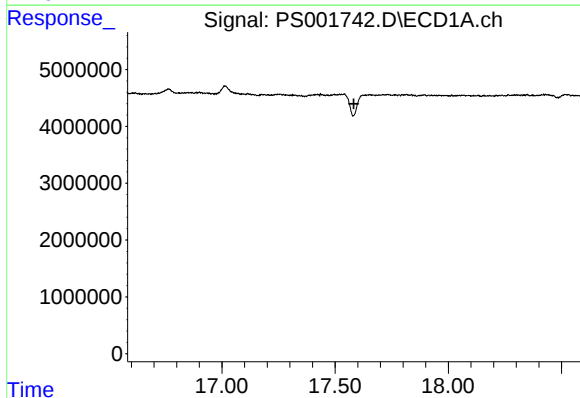

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

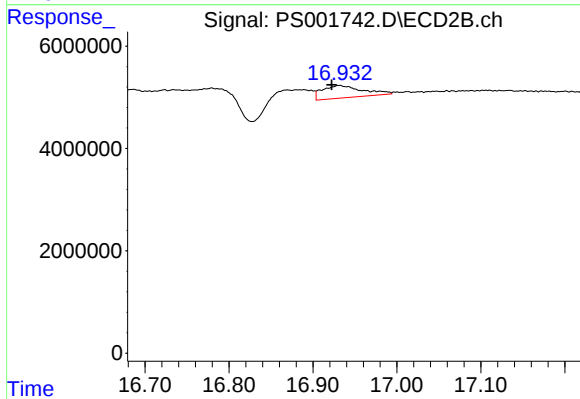

#16 DCPA

R.T.: 16.932 min
Delta R.T.: 0.009 min
Response: 8089317
Conc: 5.67 ng/ml