

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 18:05
 Operator : EI\SJ
 Sample : J4771-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:03:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.462	10.962	77303125	81570276	418.759	402.757
Target Compounds							
2) T	3,5-DICHL...	0.000	9.114	0	2532680	N.D.	9.911 #
5) T	DICAMBA	11.836	11.288	3025211	63997	4.331	0.091 #
6) T	MCP	12.150	0.000	33387041	0	66.354	N.D. #
7) T	MCPA	0.000	11.861	0	665192	N.D.	0.913 #
12) T	2,4,5-T	0.000	14.618	0	29175	N.D.	0.034 #
14) T	DINOSEB	0.000	15.686	0	1892600	N.D.	2.559 #
15) T	Picloram	16.970	16.851	3381036	260378	2.414	0.200 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 18:05
Operator : EI\SJ
Sample : J4771-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:03:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

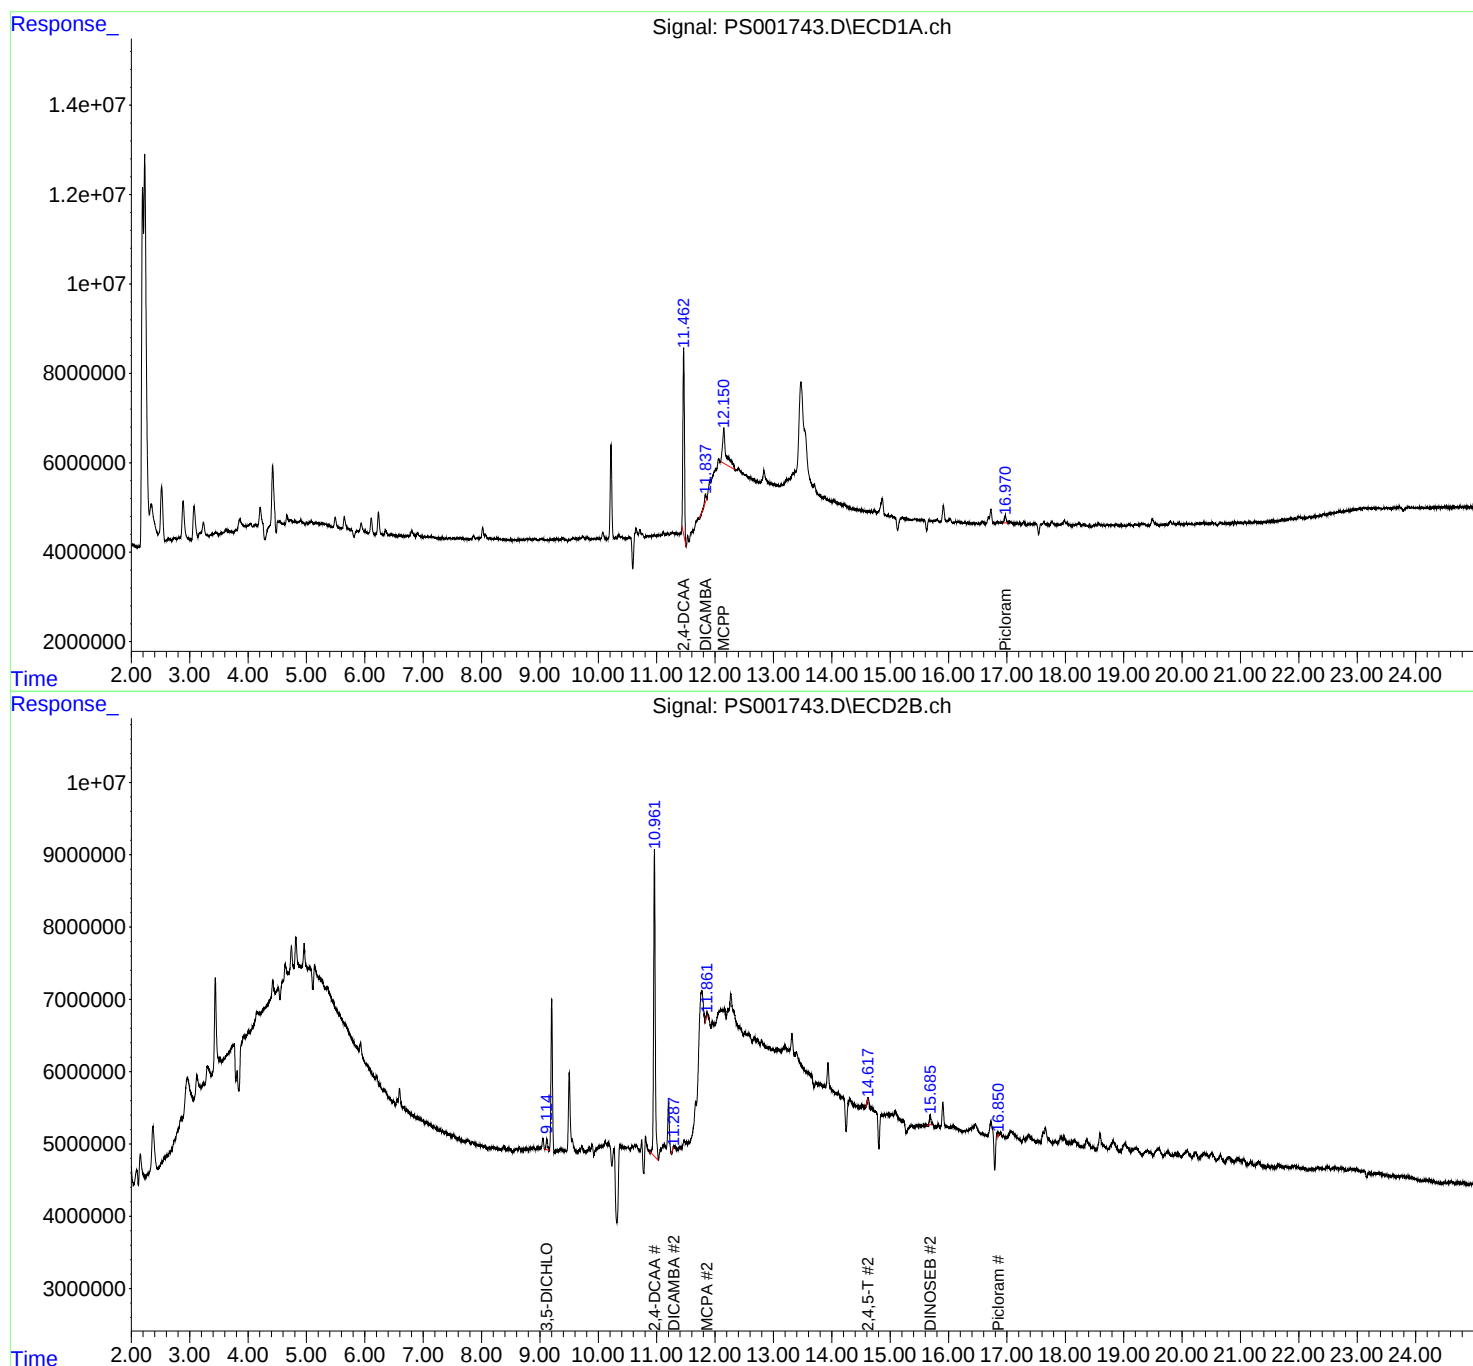


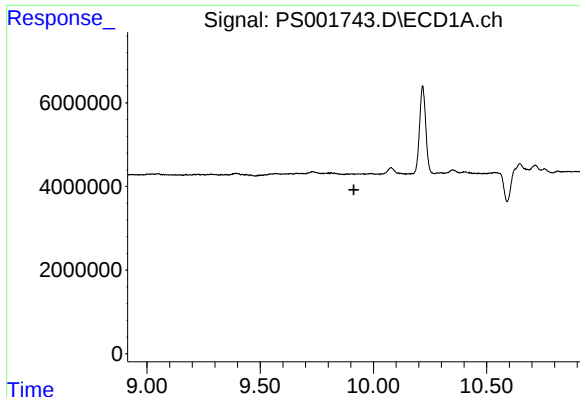

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

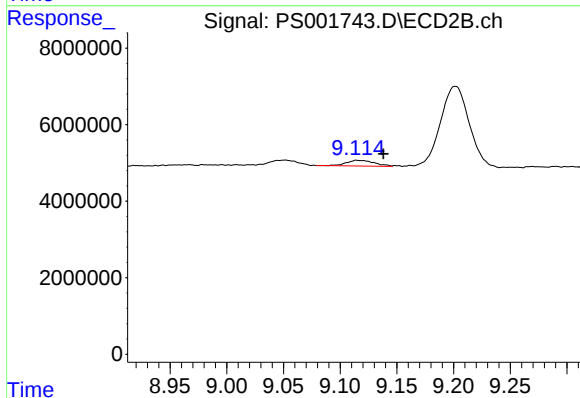


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.114 min
Delta R.T.: -0.024 min
Response: 2532680
Conc: 9.91 ng/ml

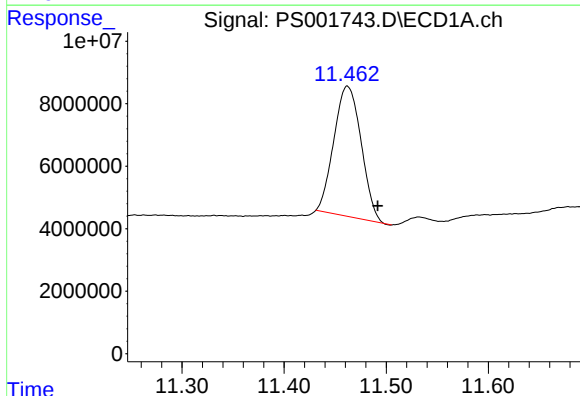


#4 2,4-DCAA

R.T.: 11.462 min
Delta R.T.: -0.030 min
Response: 77303125
Conc: 418.76 ng/ml

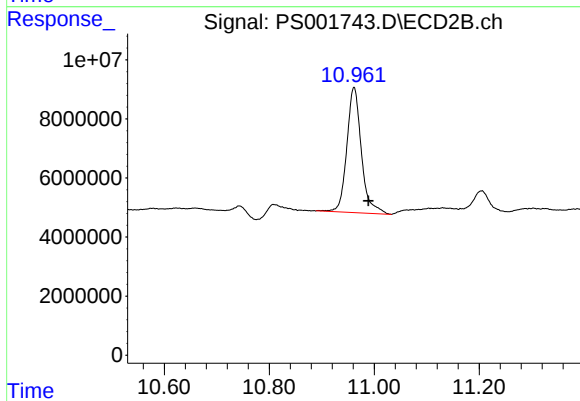

#4 2,4-DCAA


R.T.: 10.962 min
Delta R.T.: -0.027 min
Response: 81570276
Conc: 402.76 ng/ml

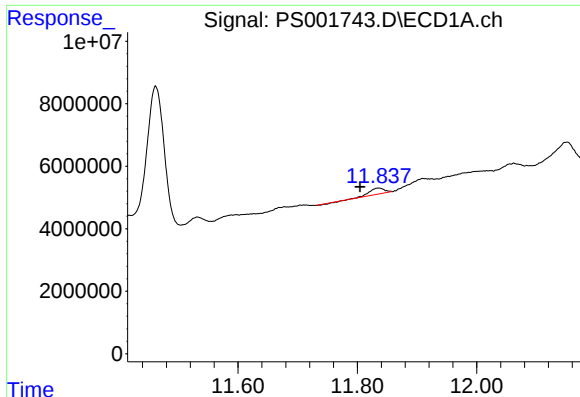

#5 DICAMBA


R.T.: 11.836 min
Delta R.T.: 0.031 min
Response: 3025211
Conc: 4.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

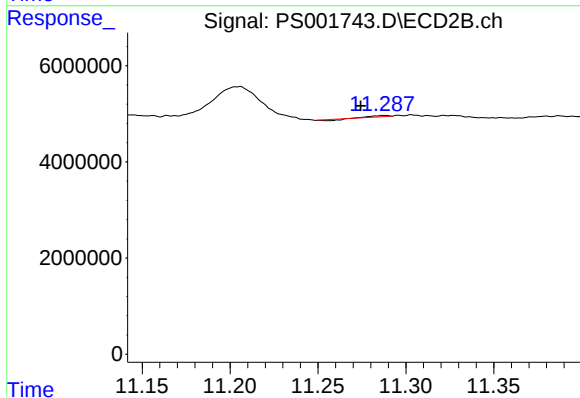


#5 DICAMBA

R.T.: 11.288 min
Delta R.T.: 0.014 min
Response: 63997
Conc: 0.09 ng/ml

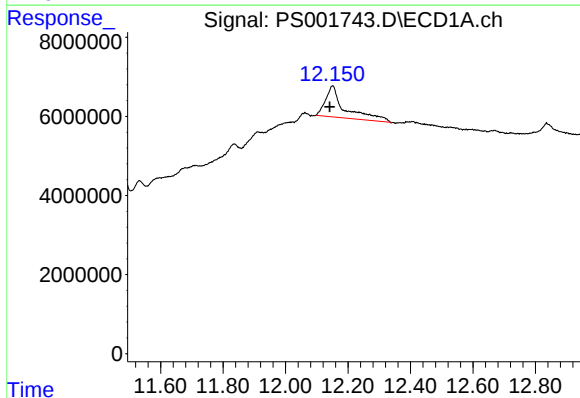


#6 MCP

R.T.: 12.150 min
Delta R.T.: 0.009 min
Response: 33387041
Conc: 66.35 ug/ml

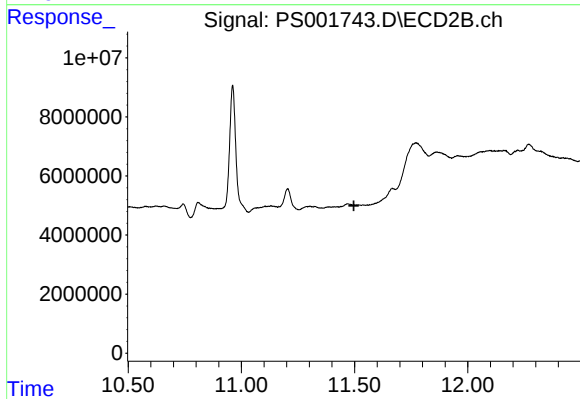

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

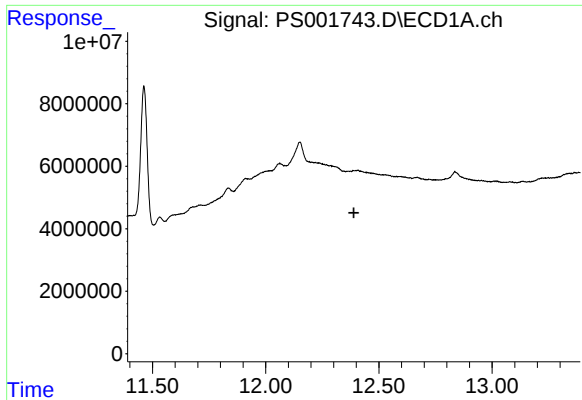

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

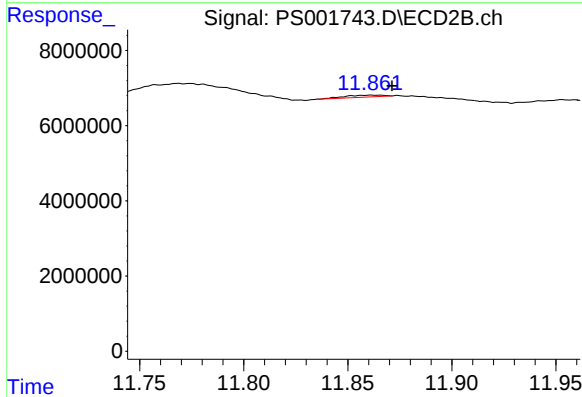


#7 MCPA

R.T.: 11.861 min
Delta R.T.: -0.010 min
Response: 665192
Conc: 0.91 ug/ml

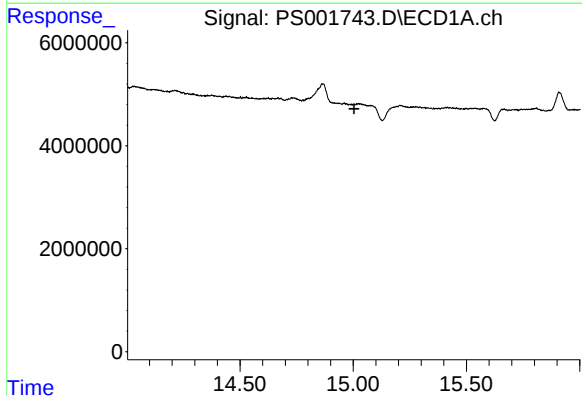


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

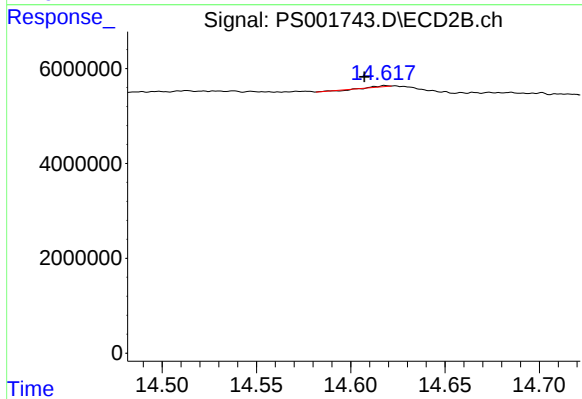

#12 2,4,5-T


R.T.: 14.618 min
Delta R.T.: 0.011 min
Response: 29175
Conc: 0.03 ng/ml

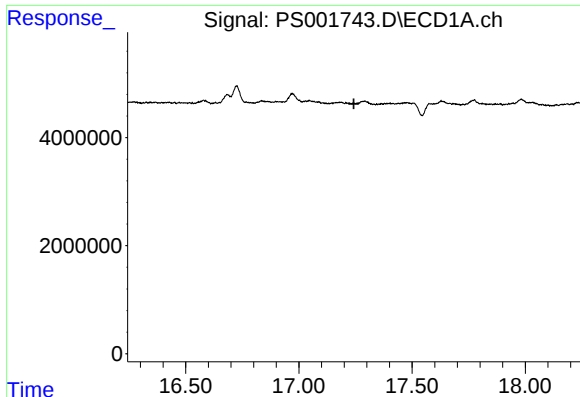

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

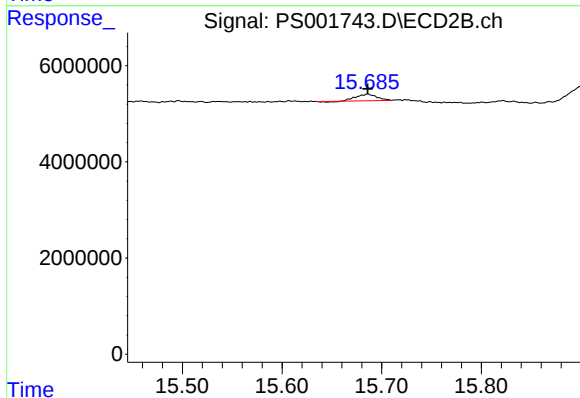


#14 DINOSEB

R.T.: 15.686 min
Delta R.T.: 0.000 min
Response: 1892600
Conc: 2.56 ng/ml

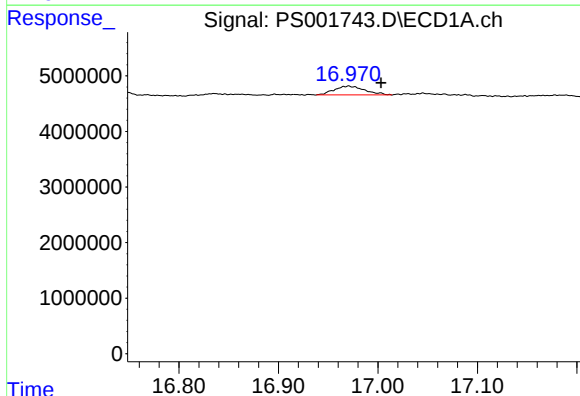

#15 Picloram

R.T.: 16.970 min
Delta R.T.: -0.033 min
Response: 3381036
Conc: 2.41 ng/ml

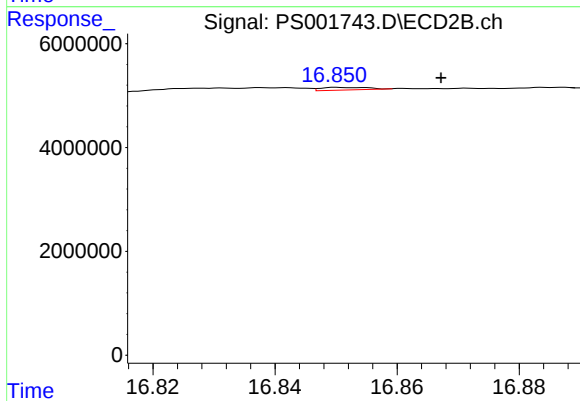

#15 Picloram

R.T.: 16.851 min
Delta R.T.: -0.016 min
Response: 260378
Conc: 0.20 ng/ml