

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 19:38
 Operator : EI\SJ
 Sample : J4873-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:04:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.515	11.015	66497465	55531467	360.224	274.189
Target Compounds							
1) T	Dalapon	2.941	2.421	19601195	14625270	77.976	61.110
2) T	3,5-DICHL...	0.000	9.105	0	3541067	N.D.	13.856 #
5) T	DICAMBA	11.829	11.256	3582150	10550031	5.128	15.043 #
6) T	MCP	12.203	11.453	13752725	343638	27.333	0.746 #
7) T	MCPA	0.000	11.819	0	14294633	N.D.	19.613 #
9) T	2,4-D	13.376	12.896	24686221	22806626	104.108	92.067
10) T	Pentachlo...	0.000	13.369	0	3851618	N.D.	1.424 #
11) T	2,4,5-TP ...	0.000	13.990	0	7495588	N.D.	7.052 #
12) T	2,4,5-T	0.000	14.607	0	362105	N.D.	0.419 #
13) T	2,4-DB	15.723	0.000	10712380	0	79.751	N.D. #
15) T	Picloram	17.030	16.885	4303219	10578351	3.072	8.113 #
16) T	DCPA	0.000	16.913	0	1227291	N.D.	0.860 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 19:38
Operator : EI\SJ
Sample : J4873-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:04:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

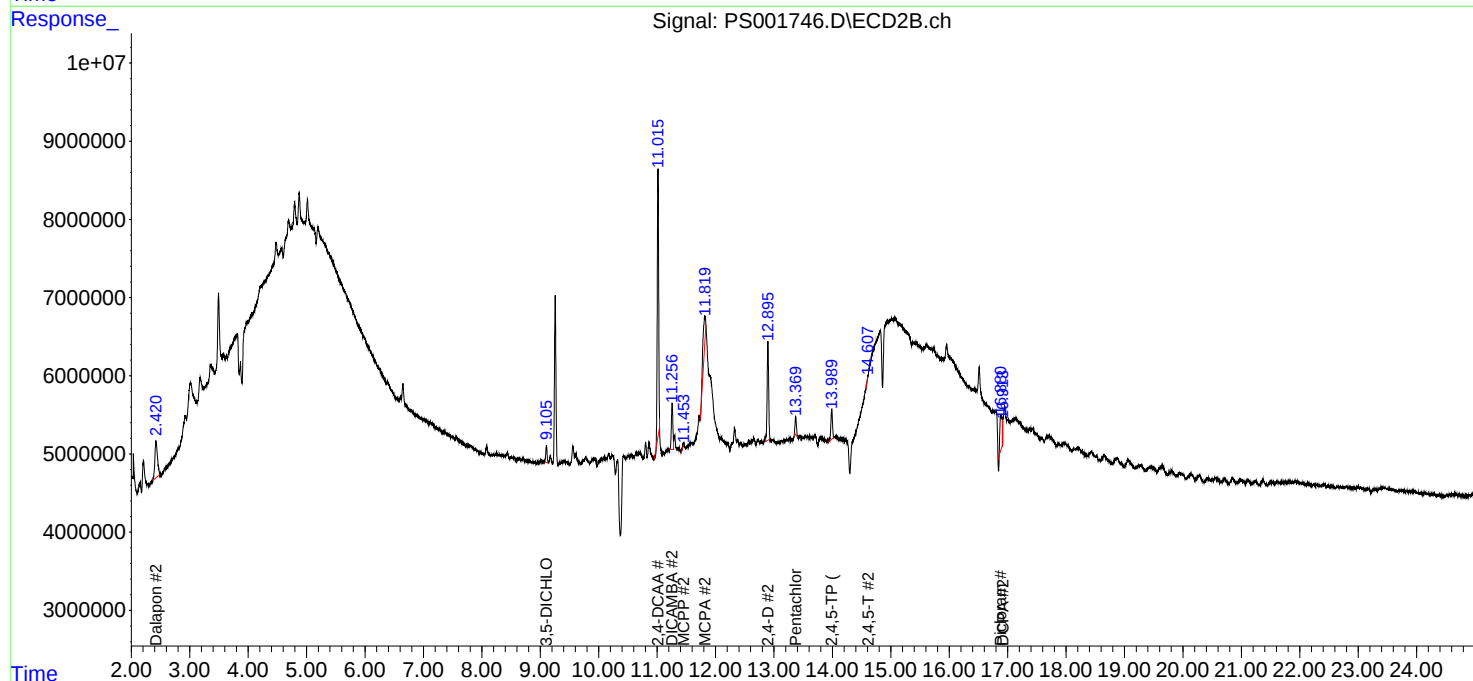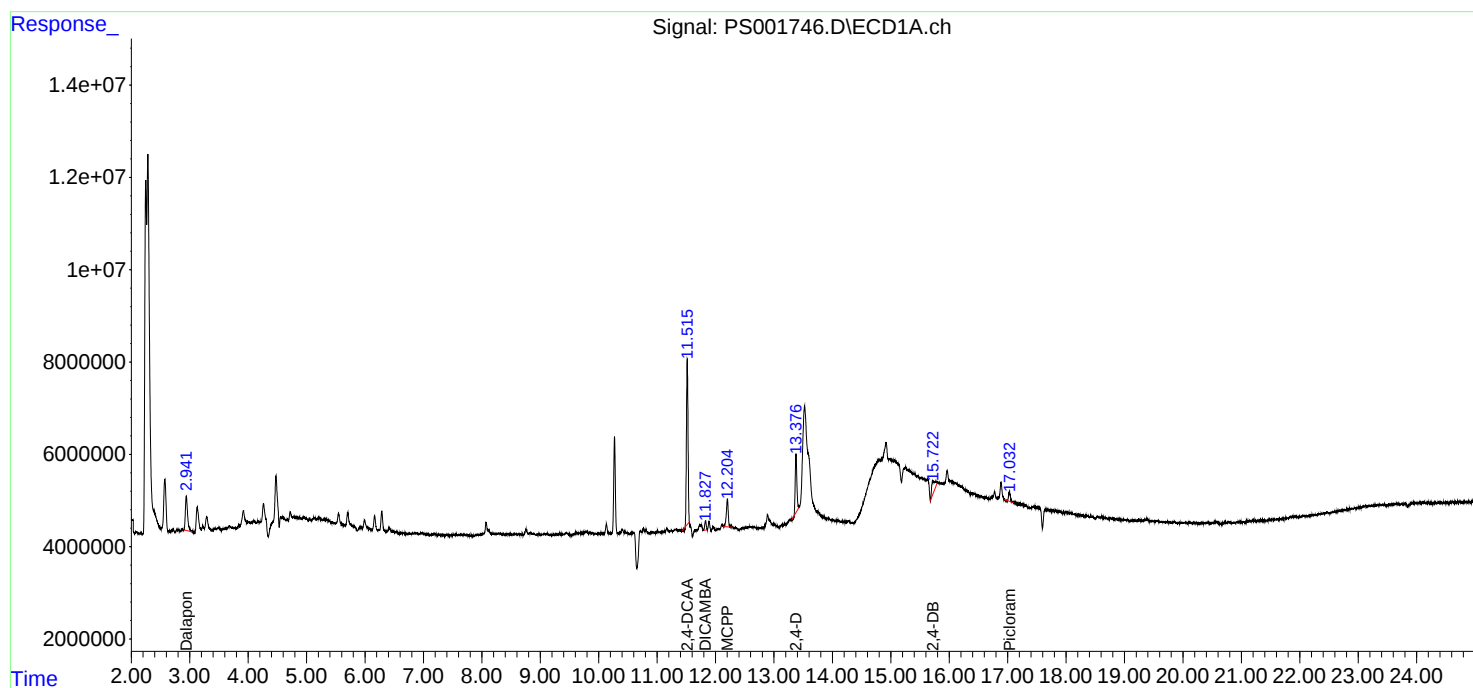


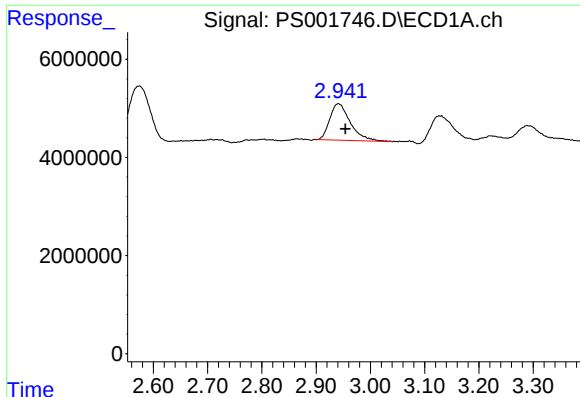

#1 Dalapon


R.T.: 2.941 min
Delta R.T.: -0.013 min
Response: 19601195
Conc: 77.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

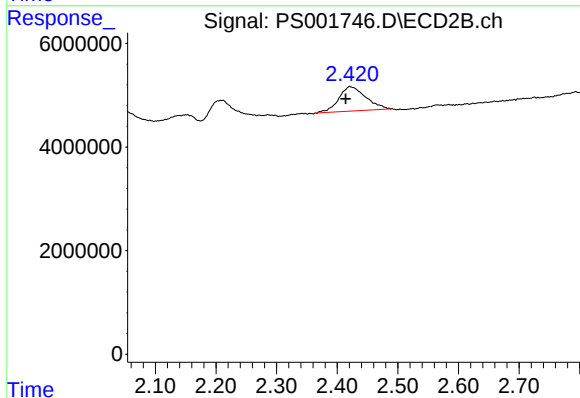


#1 Dalapon

R.T.: 2.421 min
Delta R.T.: 0.007 min
Response: 14625270
Conc: 61.11 ng/ml

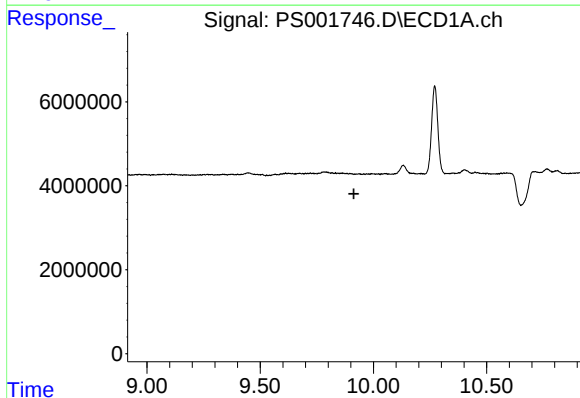


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

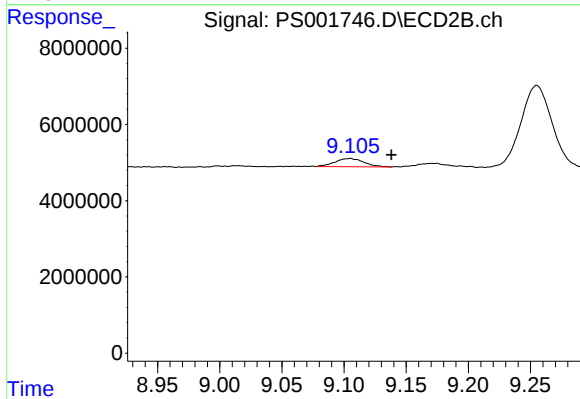

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.105 min
Delta R.T.: -0.033 min
Response: 3541067
Conc: 13.86 ng/ml

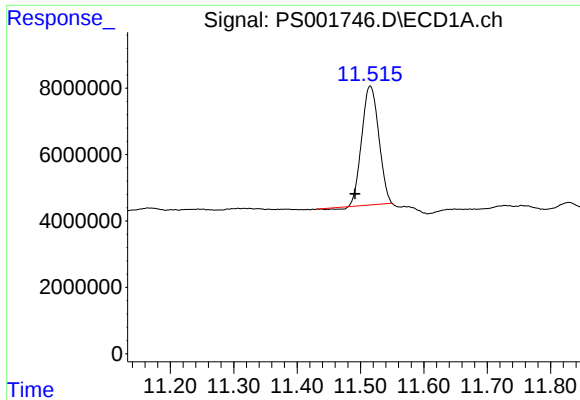

#4 2,4-DCAA


R.T.: 11.515 min
Delta R.T.: 0.024 min
Response: 66497465
Conc: 360.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

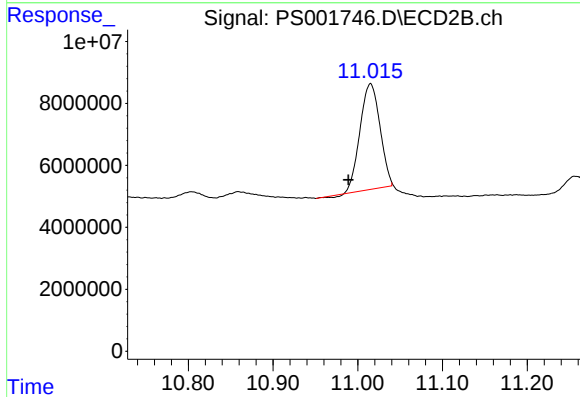


#4 2,4-DCAA

R.T.: 11.015 min
Delta R.T.: 0.026 min
Response: 55531467
Conc: 274.19 ng/ml

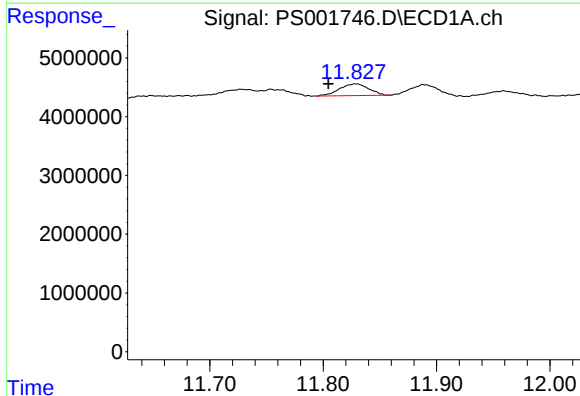


#5 DICAMBA

R.T.: 11.829 min
Delta R.T.: 0.024 min
Response: 3582150
Conc: 5.13 ng/ml

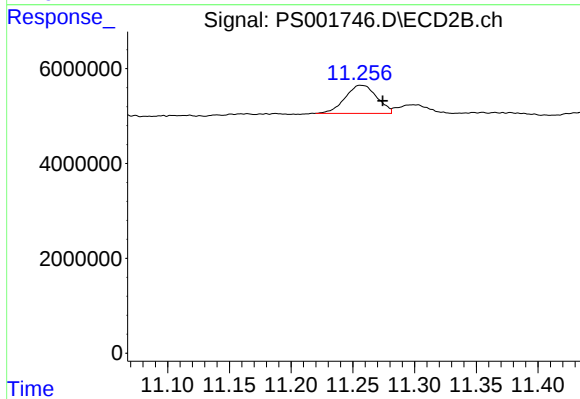

#5 DICAMBA


R.T.: 11.256 min
Delta R.T.: -0.018 min
Response: 10550031
Conc: 15.04 ng/ml

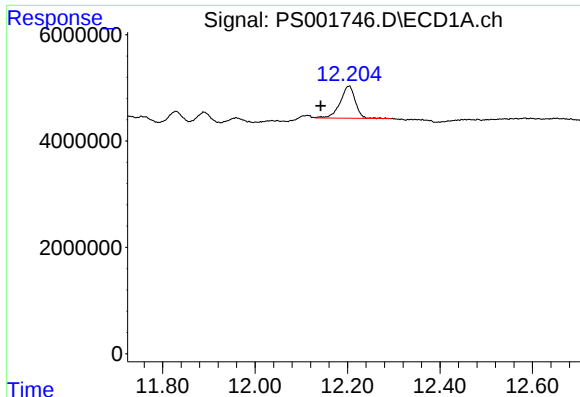

#6 MCPP


R.T.: 12.203 min
Delta R.T.: 0.061 min
Response: 13752725
Conc: 27.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

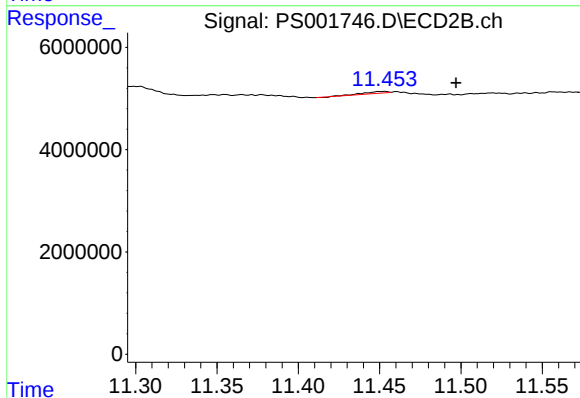


#6 MCPP

R.T.: 11.453 min
Delta R.T.: -0.044 min
Response: 343638
Conc: 0.75 ug/ml

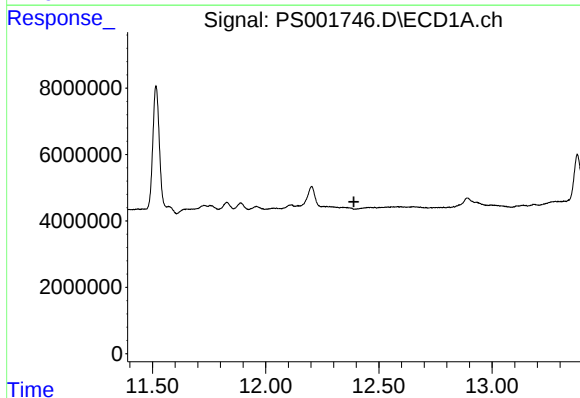


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.390 min
Response: 0
Conc: N.D.

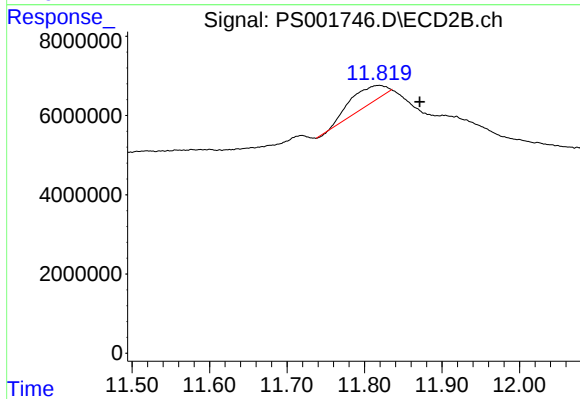

#7 MCPA


R.T.: 11.819 min
Delta R.T.: -0.052 min
Response: 14294633
Conc: 19.61 ug/ml

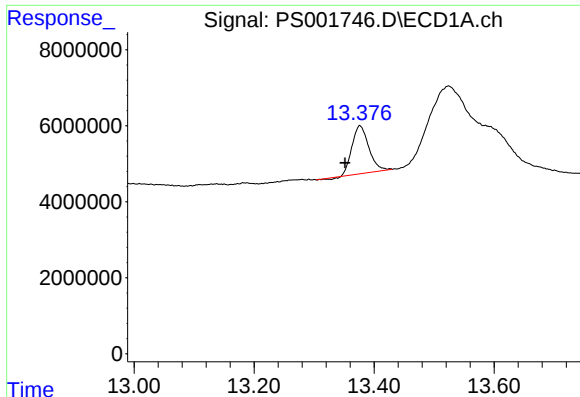

#9 2,4-D


R.T.: 13.376 min
Delta R.T.: 0.025 min
Response: 24686221
Conc: 104.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

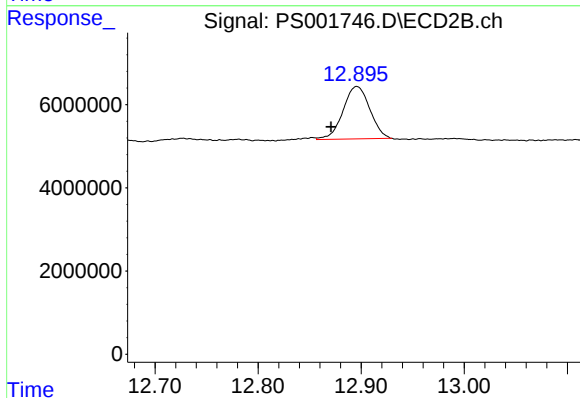


#9 2,4-D

R.T.: 12.896 min
Delta R.T.: 0.025 min
Response: 22806626
Conc: 92.07 ng/ml

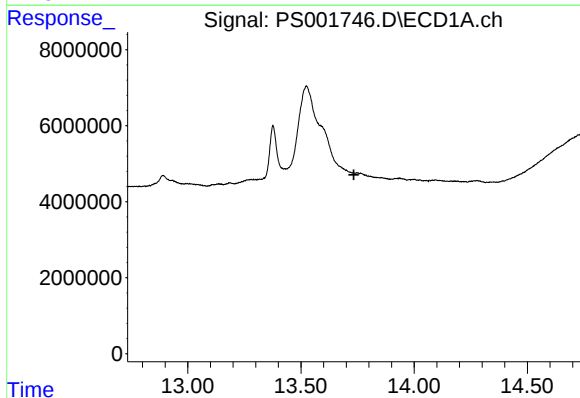


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.734 min
Response: 0
Conc: N.D.

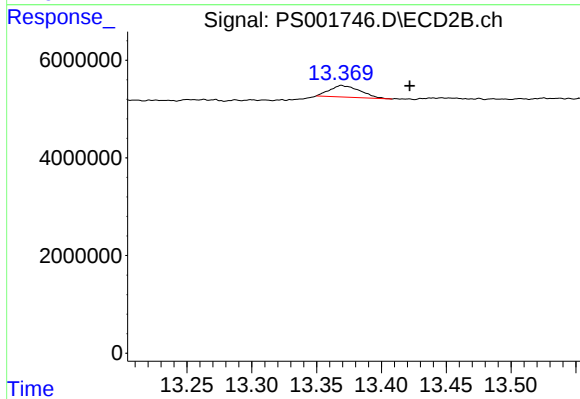

#10 Pentachlorophenol


R.T.: 13.369 min
Delta R.T.: -0.053 min
Response: 3851618
Conc: 1.42 ng/ml

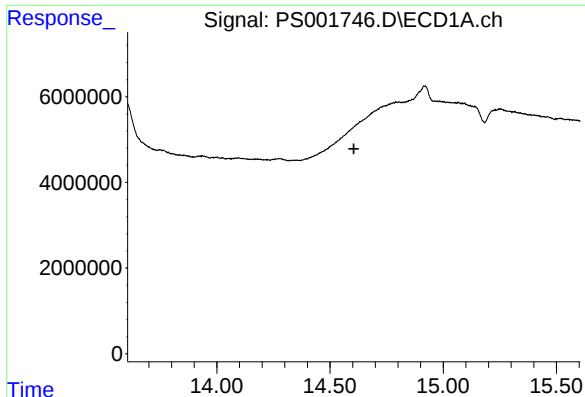

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

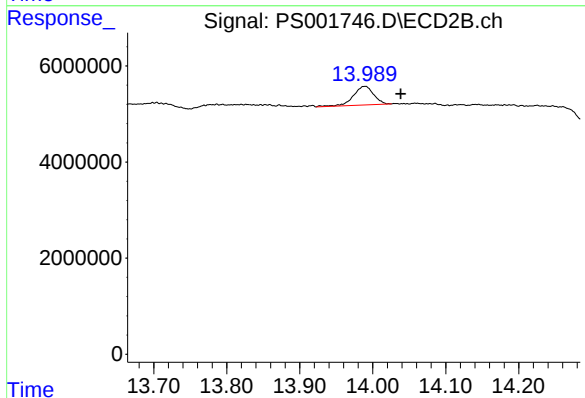


#11 2,4,5-TP (SILVEX)

R.T.: 13.990 min
Delta R.T.: -0.048 min
Response: 7495588
Conc: 7.05 ng/ml

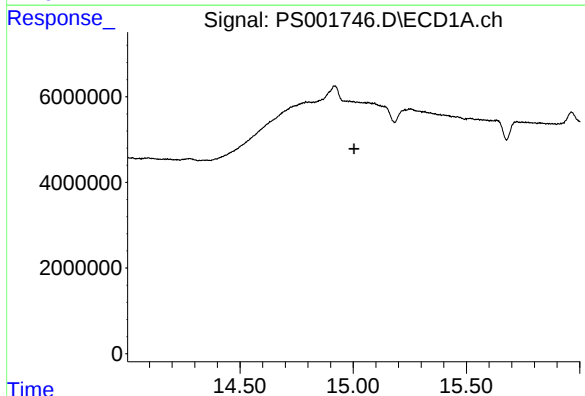


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

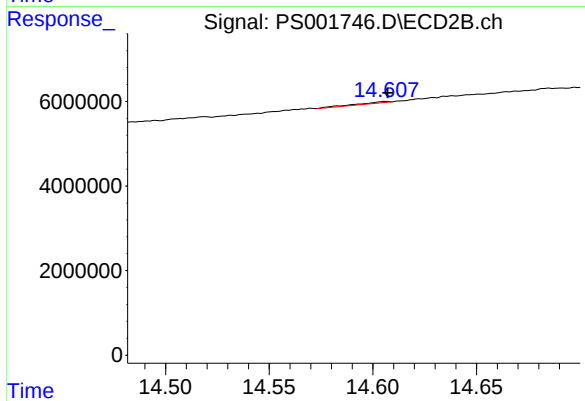

#12 2,4,5-T


R.T.: 14.607 min
Delta R.T.: 0.000 min
Response: 362105
Conc: 0.42 ng/ml

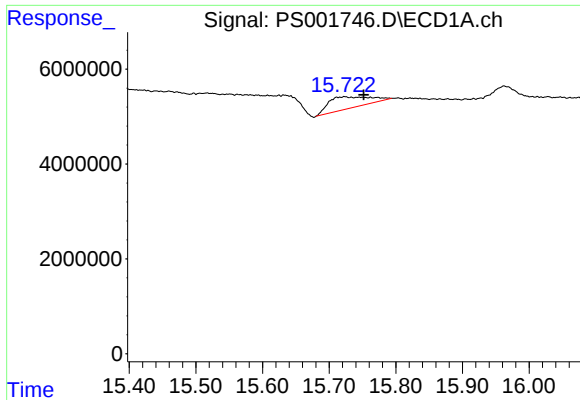

#13 2,4-DB


R.T.: 15.723 min
Delta R.T.: -0.029 min
Response: 10712380
Conc: 79.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

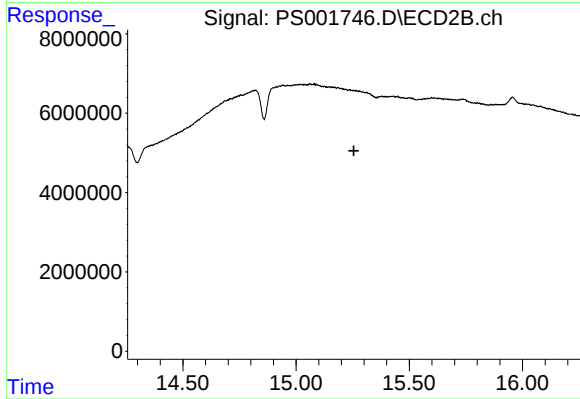


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.255 min
Response: 0
Conc: N.D.

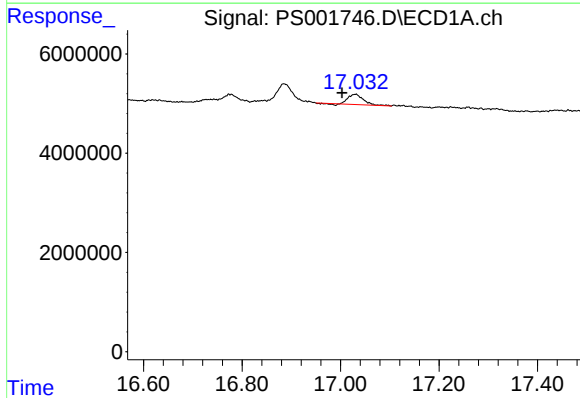


#15 Picloram

R.T.: 17.030 min
Delta R.T.: 0.027 min
Response: 4303219
Conc: 3.07 ng/ml

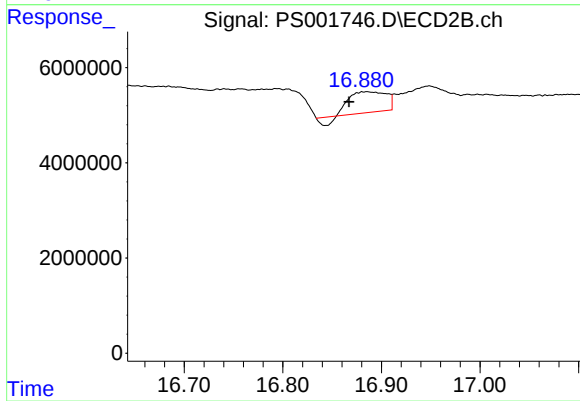

#15 Picloram


R.T.: 16.885 min
Delta R.T.: 0.018 min
Response: 10578351
Conc: 8.11 ng/ml

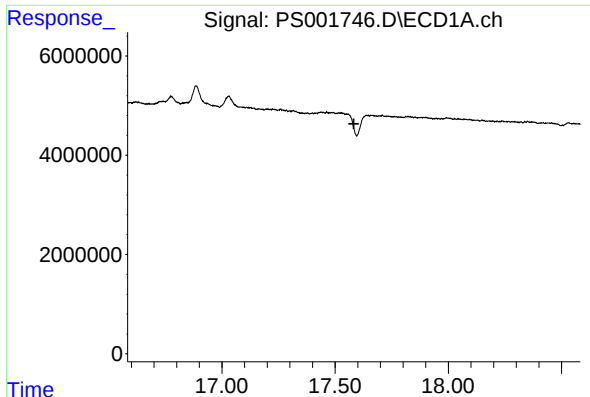

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

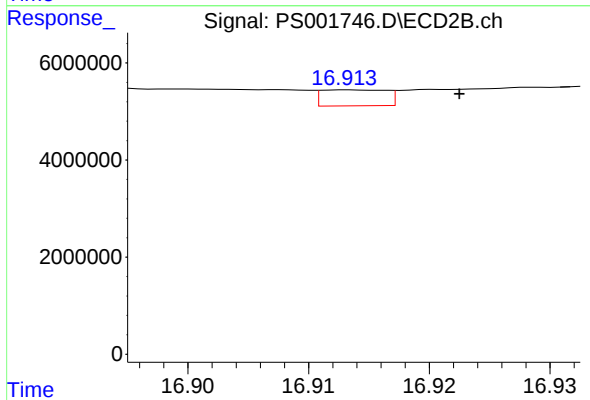

#16 DCPA

R.T.: 16.913 min
Delta R.T.: -0.009 min
Response: 1227291
Conc: 0.86 ng/ml