

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 22:45
 Operator : EI\SJ
 Sample : J4898-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 14 23:37:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.476	10.974	65390266	56128472	354.226	277.137
Target Compounds							
1) T	Dalapon	0.000	2.383	0	8183380	N.D.	34.193 #
2) T	3,5-DICHL...	0.000	9.164	0	3199518	N.D.	12.520 #
6) T	MCP	12.164	11.489	30240407	4348916	60.101	9.444 #
8) T	DICHLORPROP	0.000	12.373	0	4817586	N.D.	25.864 #
11) T	2,4,5-TP ...	0.000	14.049	0	5199916	N.D.	4.892 #
12) T	2,4,5-T	15.073	14.628	9426218	7490758	9.961	8.671
13) T	2,4-DB	15.759	15.230	6030005	6357600	44.892	47.942
14) T	DINOSEB	0.000	15.716	0	406926	N.D.	0.550 #
15) T	Picloram	16.983	16.906	10728589	34878593	7.660	26.748 #
16) T	DCPA	17.603	16.906	-6749353	34878593	N.D.	24.429



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 22:45
Operator : EI\SJ
Sample : J4898-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 14 23:37:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

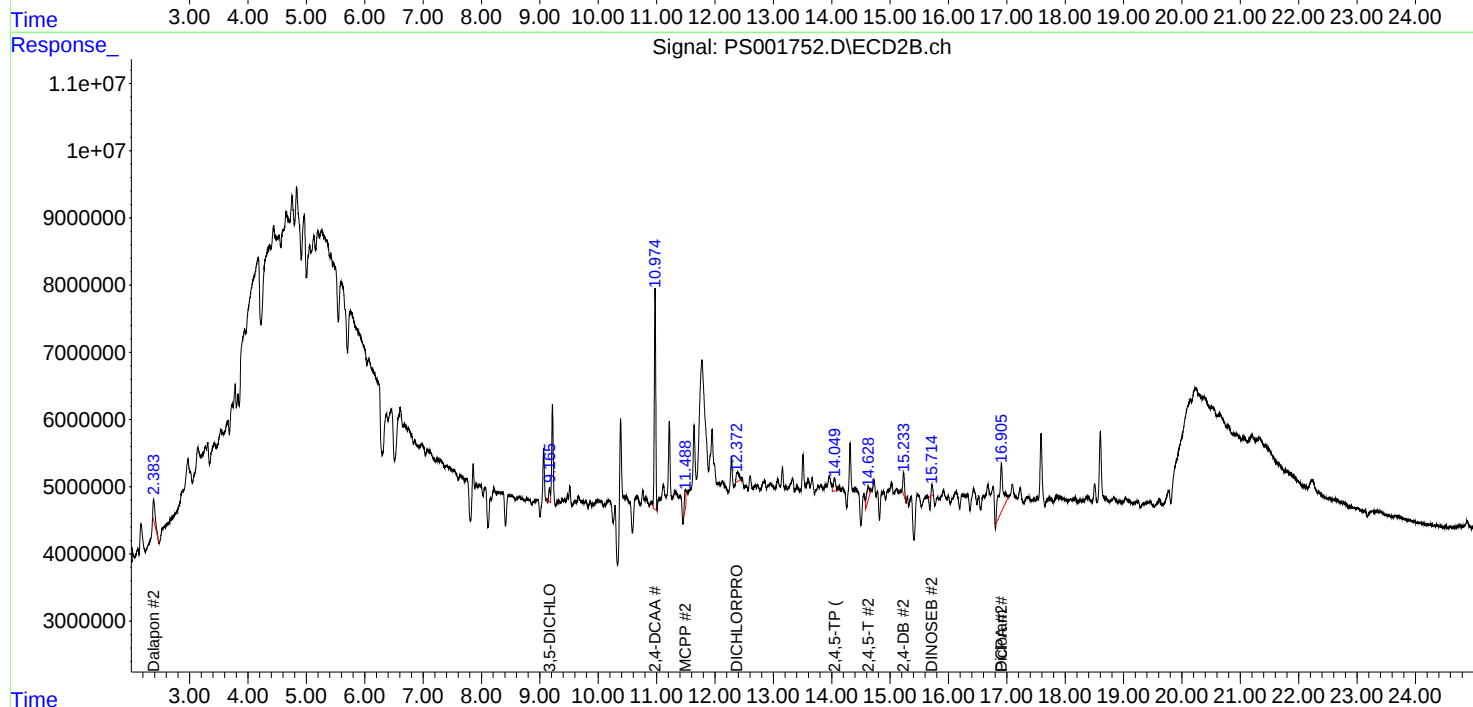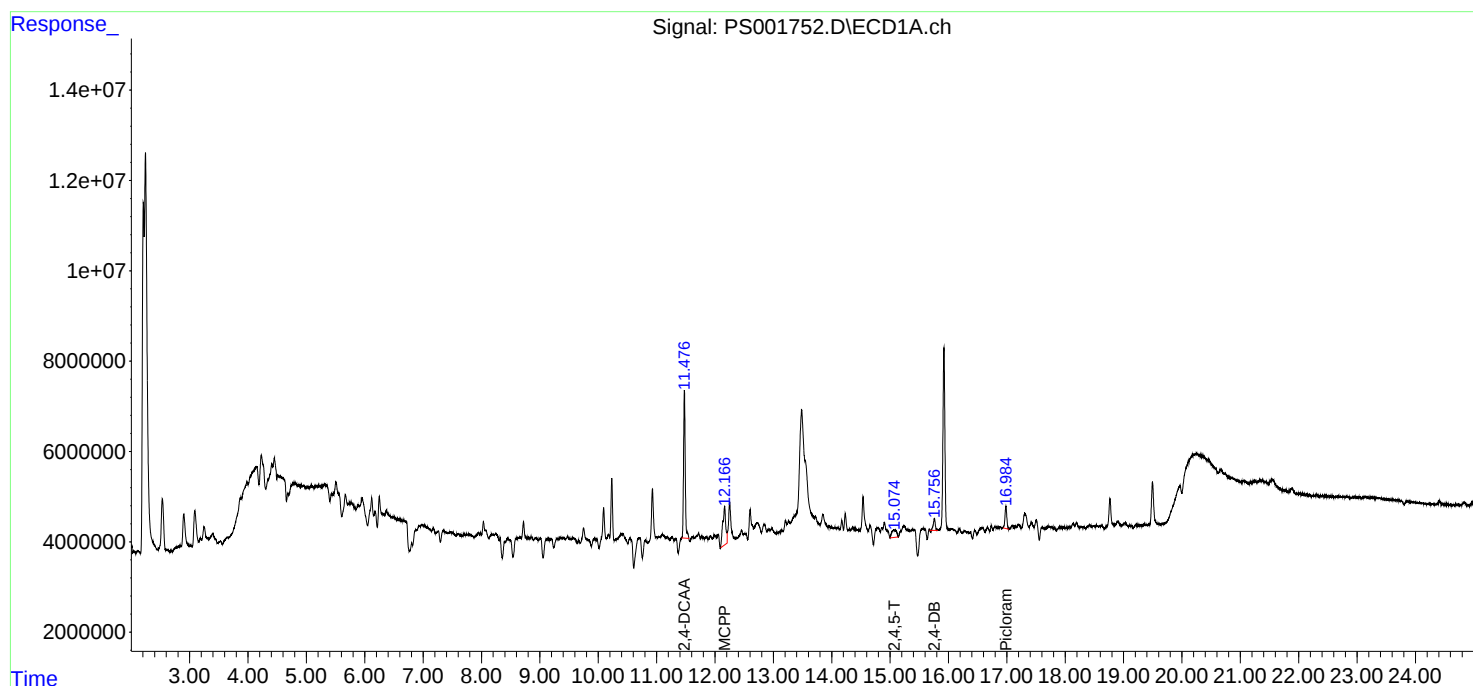


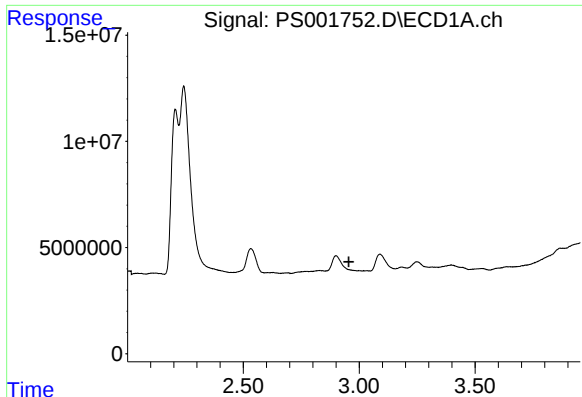

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

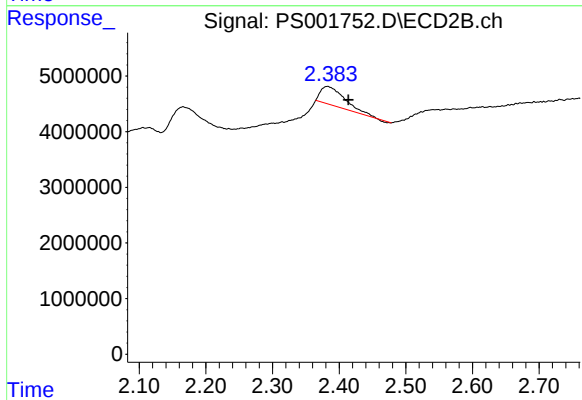


#1 Dalapon

R.T.: 2.383 min
Delta R.T.: -0.031 min
Response: 8183380
Conc: 34.19 ng/ml

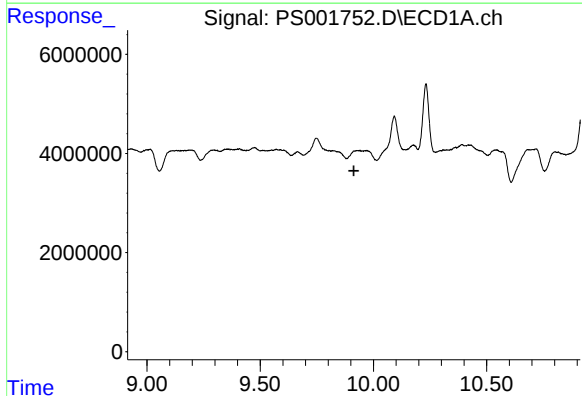


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

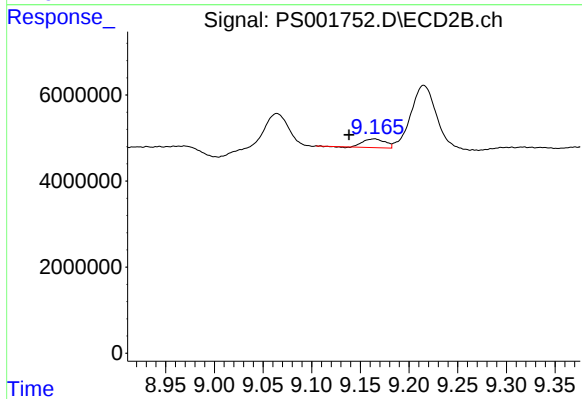

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.164 min
Delta R.T.: 0.026 min
Response: 3199518
Conc: 12.52 ng/ml

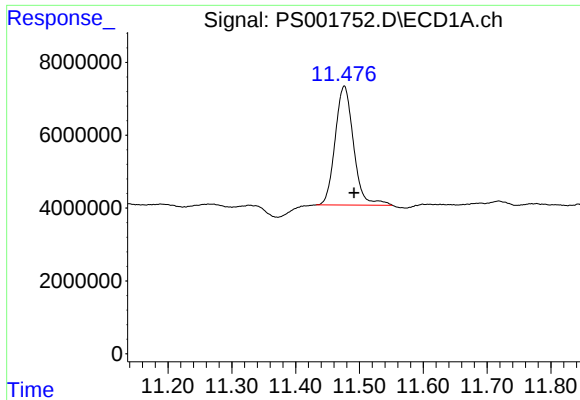

#4 2,4-DCAA


R.T.: 11.476 min
Delta R.T.: -0.016 min
Response: 65390266
Conc: 354.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

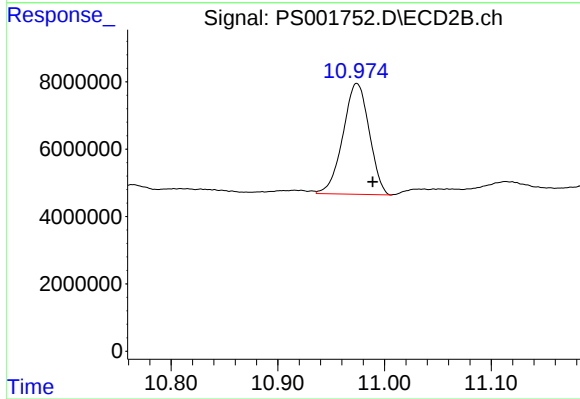


#4 2,4-DCAA

R.T.: 10.974 min
Delta R.T.: -0.015 min
Response: 56128472
Conc: 277.14 ng/ml

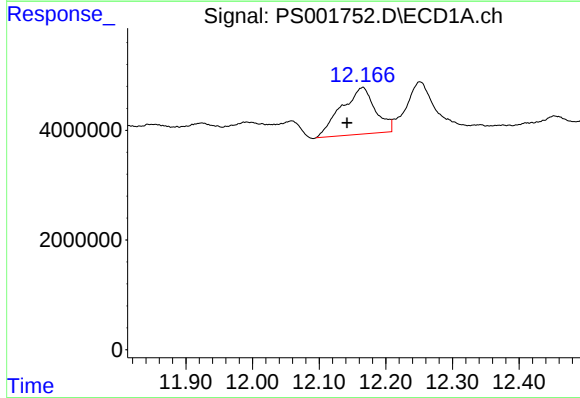


#6 MCP

R.T.: 12.164 min
Delta R.T.: 0.023 min
Response: 30240407
Conc: 60.10 ug/ml

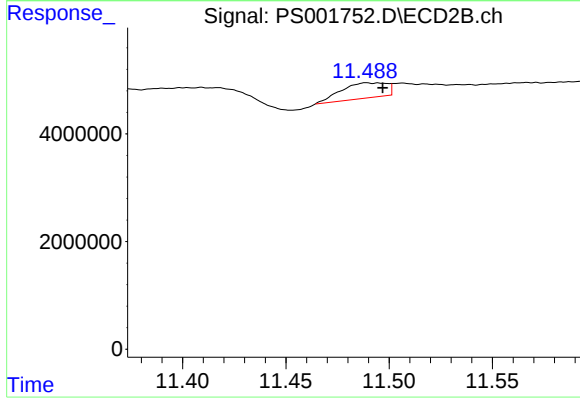

#6 MCP


R.T.: 11.489 min
Delta R.T.: -0.008 min
Response: 4348916
Conc: 9.44 ug/ml

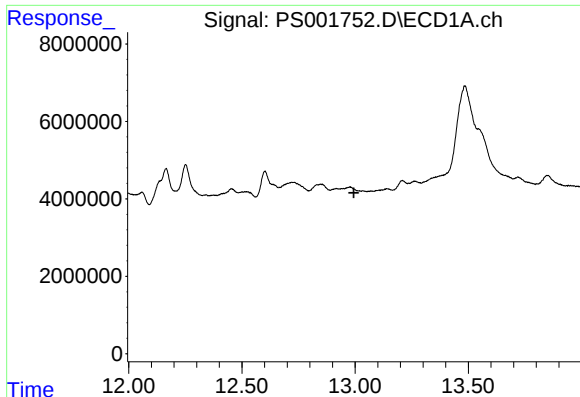

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.995 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

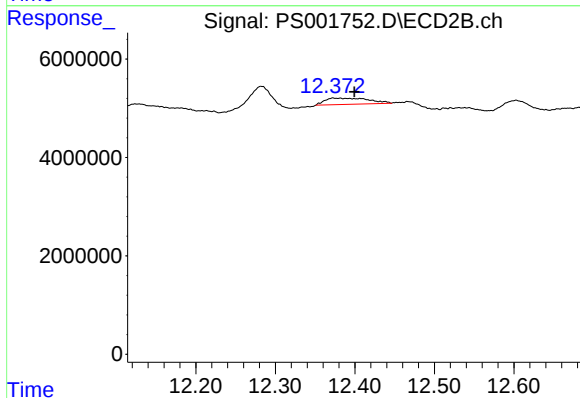


#8 DICHLORPROP

R.T.: 12.373 min
Delta R.T.: -0.027 min
Response: 4817586
Conc: 25.86 ng/ml

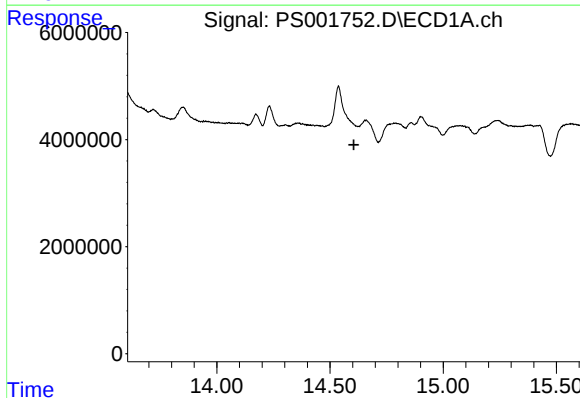


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.606 min
Response: 0
Conc: N.D.

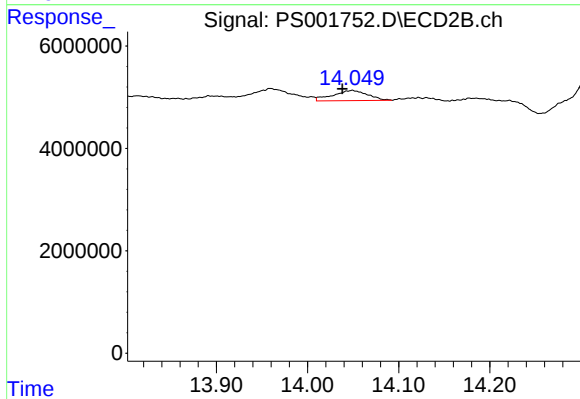

#11 2,4,5-TP (SILVEX)


R.T.: 14.049 min
Delta R.T.: 0.011 min
Response: 5199916
Conc: 4.89 ng/ml

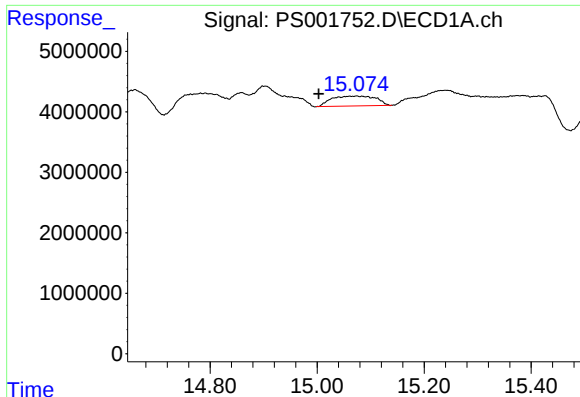

#12 2,4,5-T


R.T.: 15.073 min
Delta R.T.: 0.069 min
Response: 9426218
Conc: 9.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

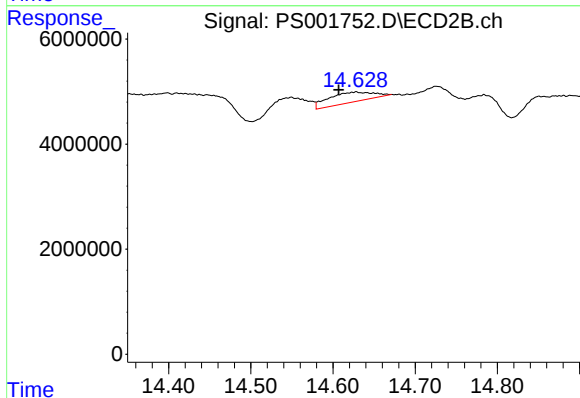


#12 2,4,5-T

R.T.: 14.628 min
Delta R.T.: 0.021 min
Response: 7490758
Conc: 8.67 ng/ml

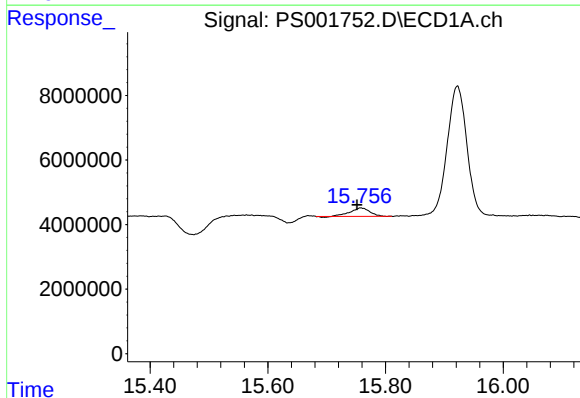


#13 2,4-DB

R.T.: 15.759 min
Delta R.T.: 0.007 min
Response: 6030005
Conc: 44.89 ng/ml

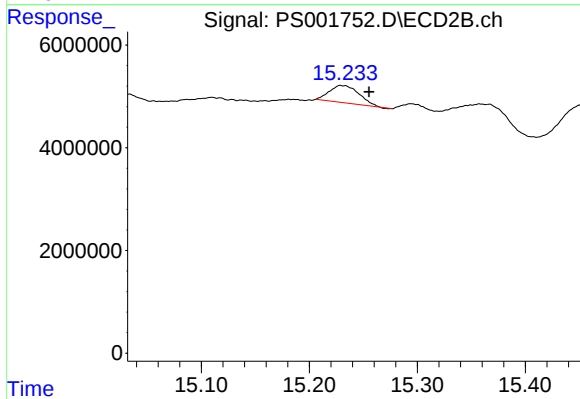

#13 2,4-DB


R.T.: 15.230 min
Delta R.T.: -0.025 min
Response: 6357600
Conc: 47.94 ng/ml

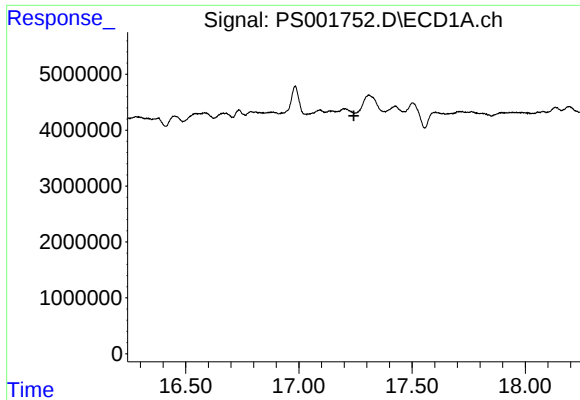

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

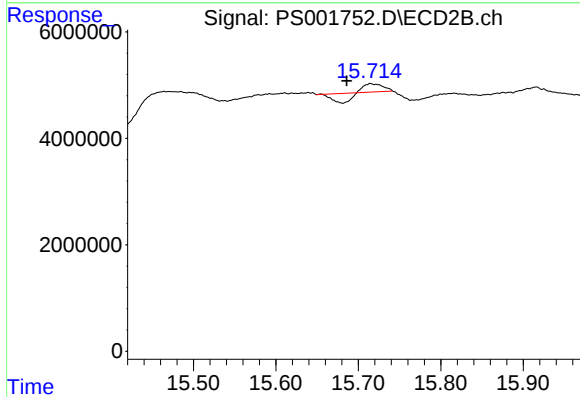


#14 DINOSEB

R.T.: 15.716 min
Delta R.T.: 0.030 min
Response: 406926
Conc: 0.55 ng/ml

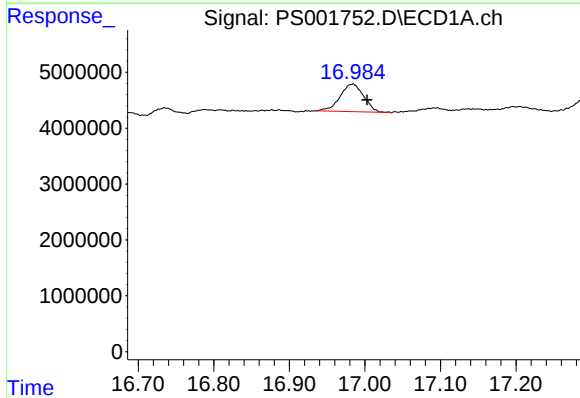


#15 Picloram

R.T.: 16.983 min
Delta R.T.: -0.020 min
Response: 10728589
Conc: 7.66 ng/ml

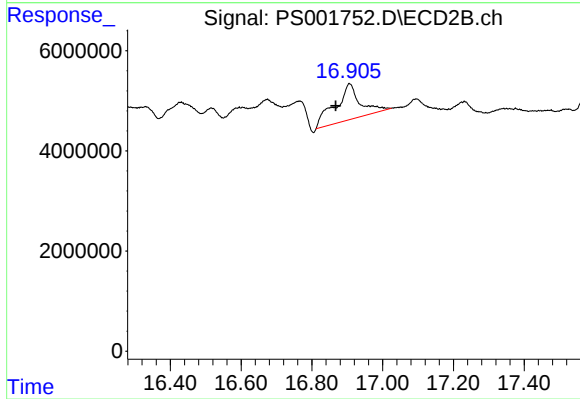

#15 Picloram


R.T.: 16.906 min
Delta R.T.: 0.039 min
Response: 34878593
Conc: 26.75 ng/ml

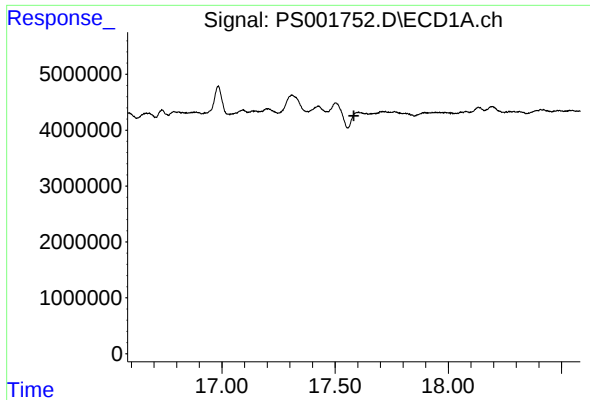

#16 DCPA

R.T.: 17.603 min
Delta R.T.: 0.020 min
Response: -6749353
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

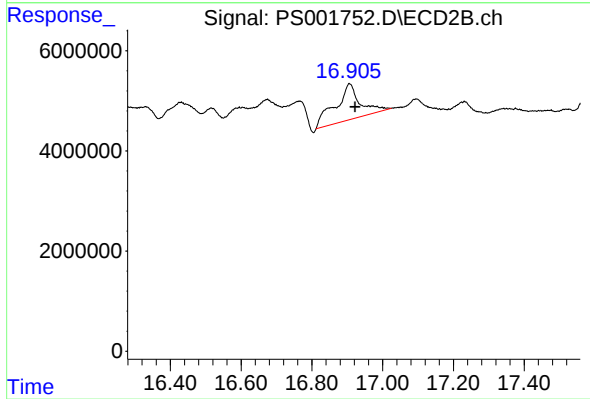

#16 DCPA

R.T.: 16.906 min
Delta R.T.: -0.016 min
Response: 34878593
Conc: 24.43 ng/ml