

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 23:16
 Operator : EI\SJ
 Sample : J4898-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:46:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.462	10.960	63313076	56727446	342.974	280.094
Target Compounds							
2) T	3,5-DICHL...	0.000	9.201	0	28475383	N.D.	111.426 #
6) T	MCPD	12.151	11.495	23823142	1862039	47.347	4.044 #
7) T	MCPA	0.000	11.900	0	1751191	N.D.	2.403 #
10) T	Pentachlo...	0.000	13.492	0	6223335	N.D.	2.301 #
12) T	2,4,5-T	0.000	14.620	0	6021789	N.D.	6.971 #
14) T	DINOSEB	0.000	15.708	0	1368474	N.D.	1.850 #
15) T	Picloram	16.970	16.858	3112148	509001	2.222	0.390 #
16) T	DCPA	17.583	16.893	-846566	4137252	N.D.	2.898



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 23:16
Operator : EI\SJ
Sample : J4898-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:46:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

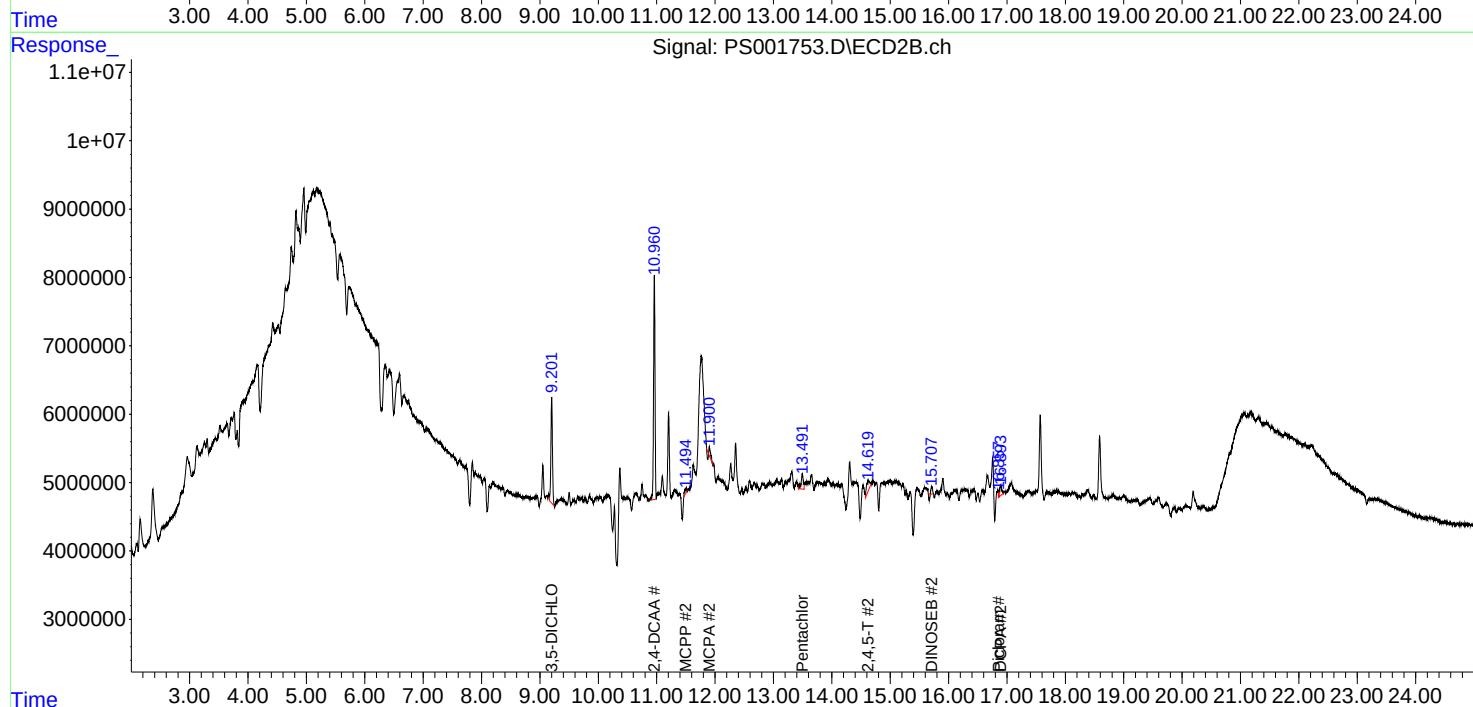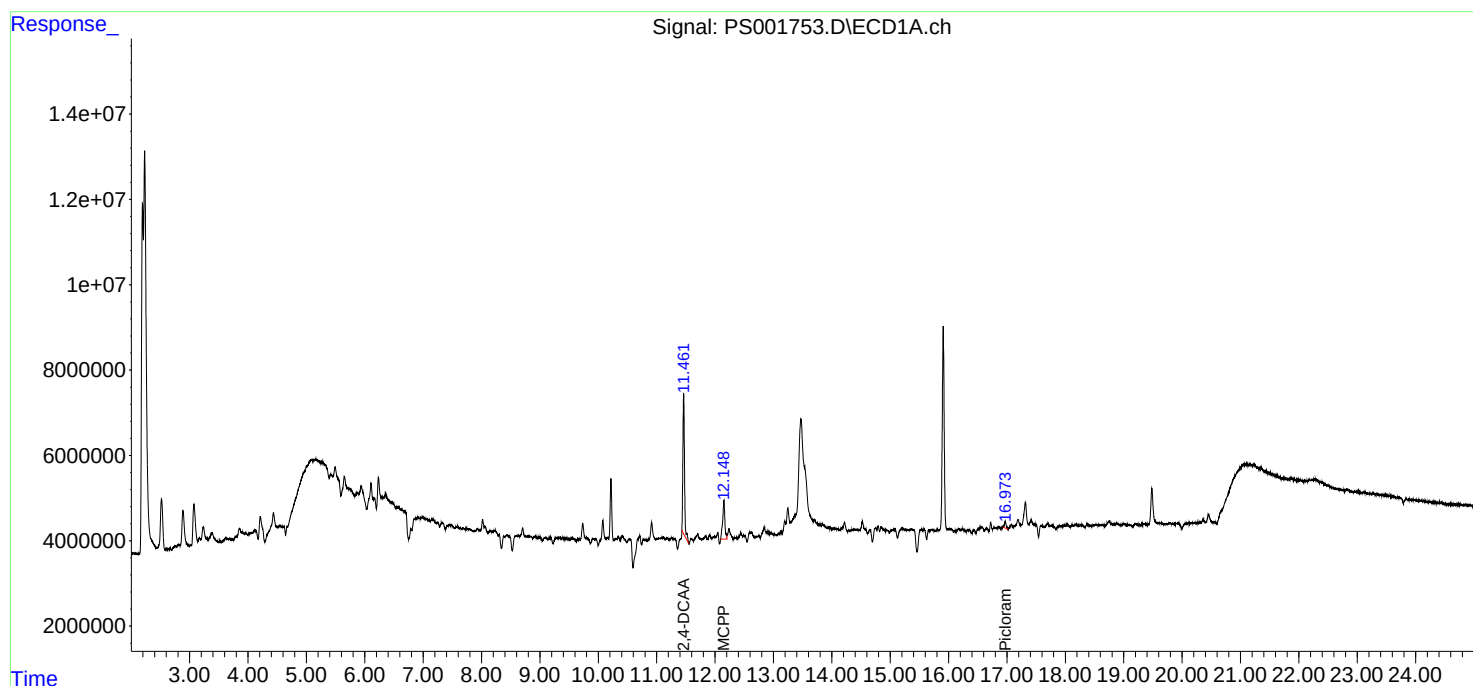


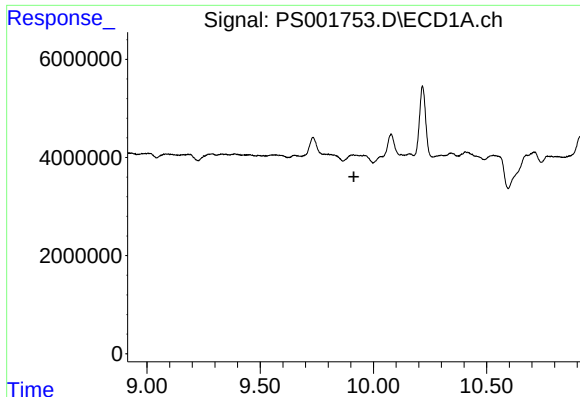

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

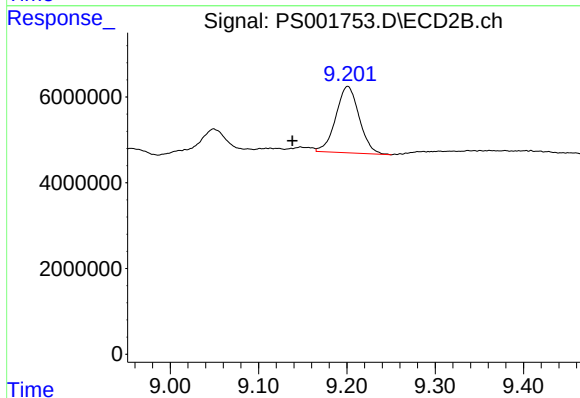


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.201 min
Delta R.T.: 0.063 min
Response: 28475383
Conc: 111.43 ng/ml

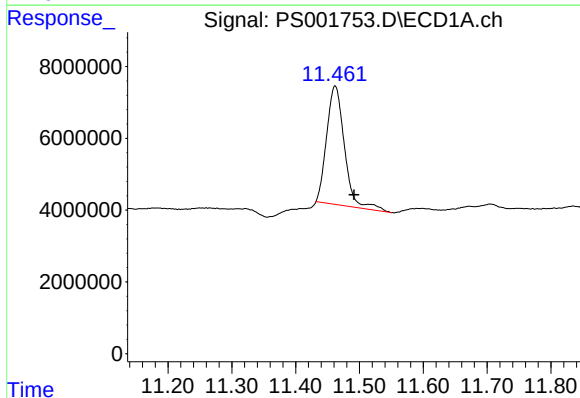


#4 2,4-DCAA

R.T.: 11.462 min
Delta R.T.: -0.030 min
Response: 63313076
Conc: 342.97 ng/ml

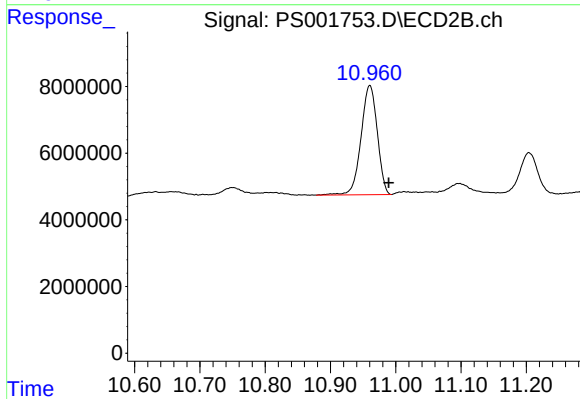

#4 2,4-DCAA


R.T.: 10.960 min
Delta R.T.: -0.029 min
Response: 56727446
Conc: 280.09 ng/ml

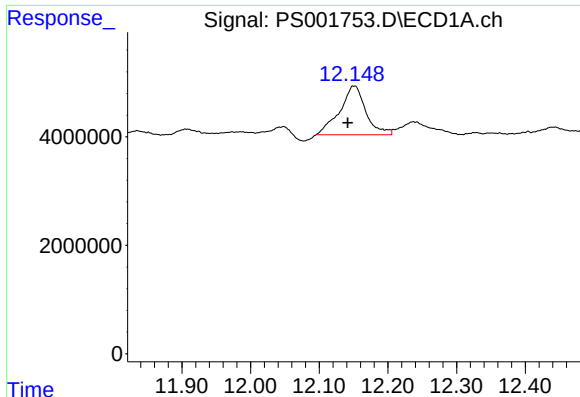

#6 MCPP


R.T.: 12.151 min
Delta R.T.: 0.009 min
Response: 23823142
Conc: 47.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

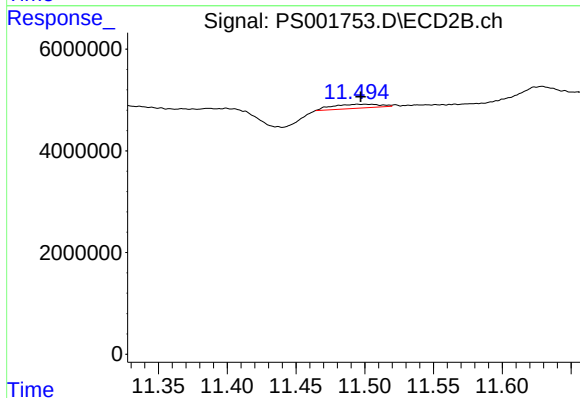


#6 MCPP

R.T.: 11.495 min
Delta R.T.: -0.002 min
Response: 1862039
Conc: 4.04 ug/ml

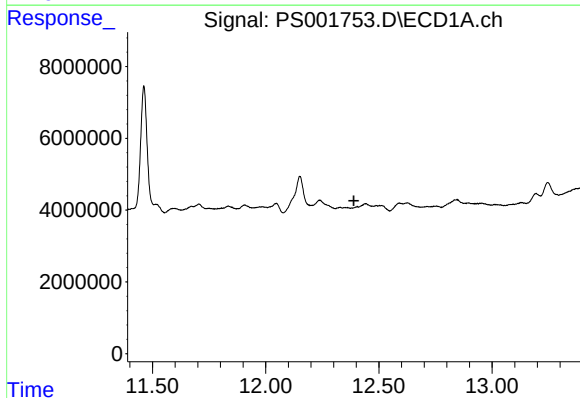


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.390 min
Response: 0
Conc: N.D.

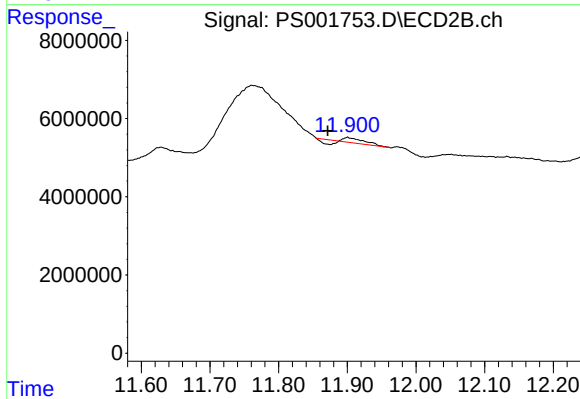

#7 MCPA


R.T.: 11.900 min
Delta R.T.: 0.029 min
Response: 1751191
Conc: 2.40 ug/ml

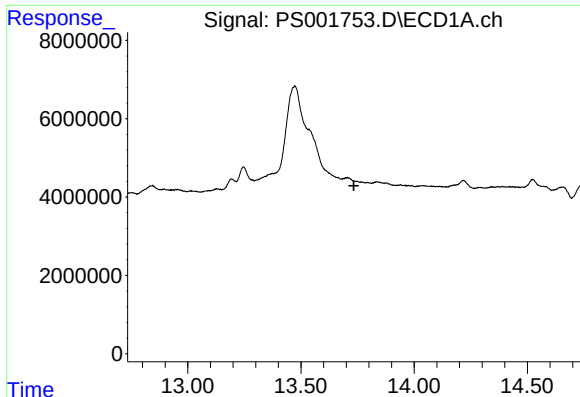

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

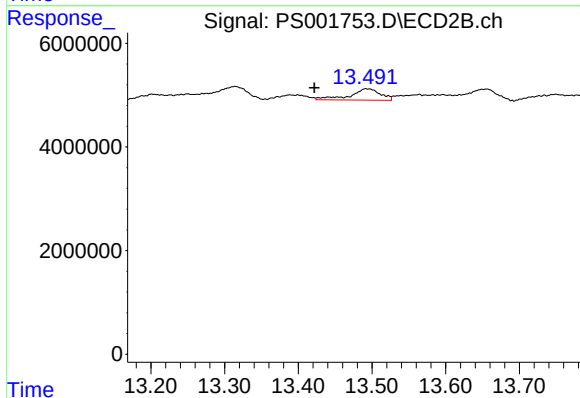


#10 Pentachlorophenol

R.T.: 13.492 min
Delta R.T.: 0.070 min
Response: 6223335
Conc: 2.30 ng/ml

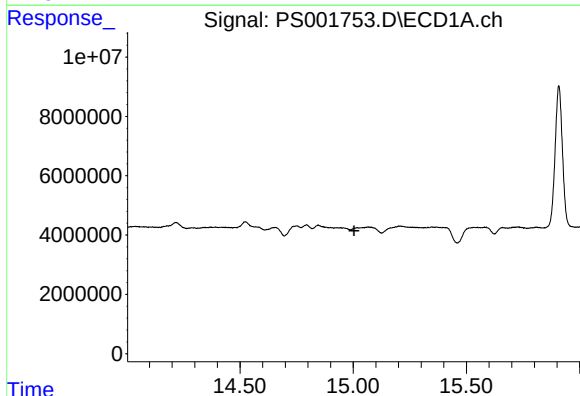


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

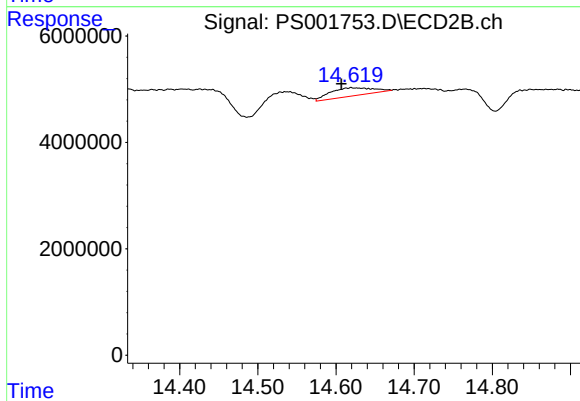

#12 2,4,5-T


R.T.: 14.620 min
Delta R.T.: 0.012 min
Response: 6021789
Conc: 6.97 ng/ml

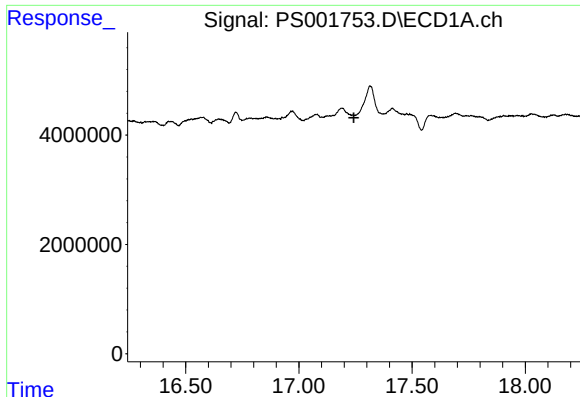

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

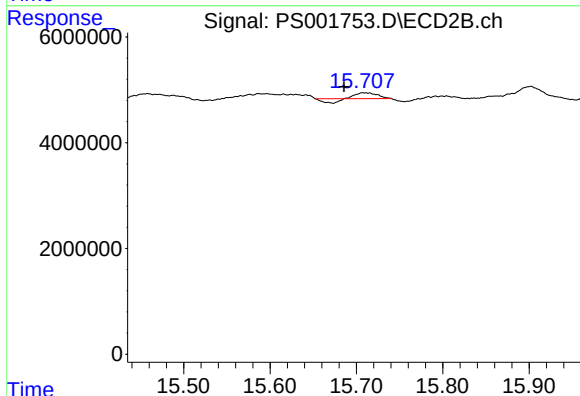


#14 DINOSEB

R.T.: 15.708 min
Delta R.T.: 0.022 min
Response: 1368474
Conc: 1.85 ng/ml

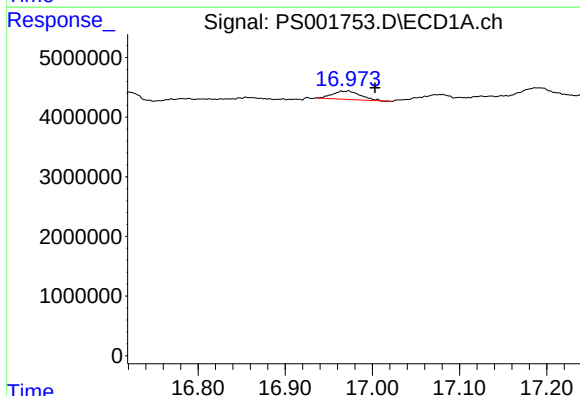


#15 Picloram

R.T.: 16.970 min
Delta R.T.: -0.033 min
Response: 3112148
Conc: 2.22 ng/ml

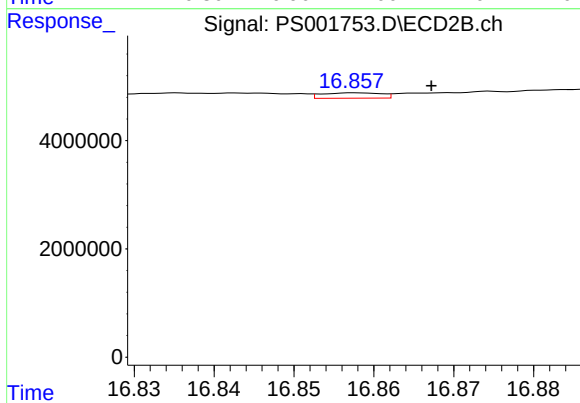

#15 Picloram


R.T.: 16.858 min
Delta R.T.: -0.009 min
Response: 509001
Conc: 0.39 ng/ml

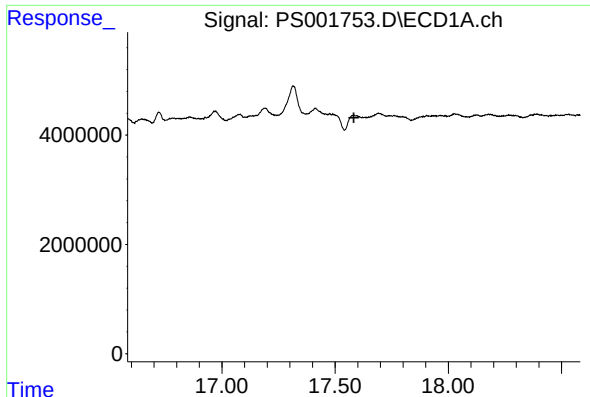

#16 DCPA

R.T.: 17.583 min
Delta R.T.: 0.000 min
Response: -846566
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

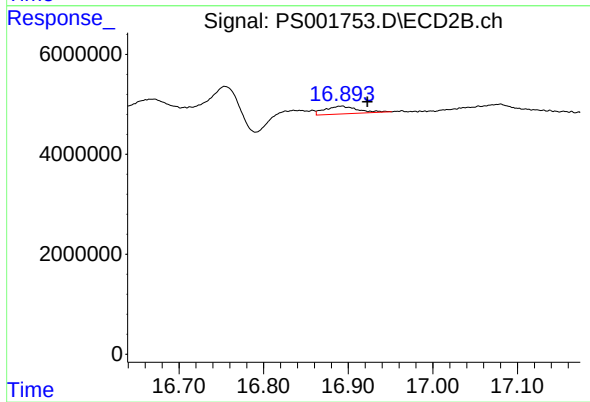

#16 DCPA

R.T.: 16.893 min
Delta R.T.: -0.030 min
Response: 4137252
Conc: 2.90 ng/ml