

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2018 23:47
 Operator : EI\SJ
 Sample : J4906-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:46:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.465	10.964	52162863	51043647	282.572	252.030
Target Compounds							
1) T	Dalapon	2.890	0.000	4318496	0	17.179	N.D. #
2) T	3,5-DICHL...	0.000	9.204	0	23042078	N.D.	90.165 #
5) T	DICAMBA	0.000	11.206	0	7677857	N.D.	10.947 #
6) T	MCP	12.152	0.000	23633115	0	46.969	N.D. #
15) T	Picloram	0.000	16.896	0	7211209	N.D.	5.530 #
16) T	DCPA	17.592	16.896	-3399100	7211209	N.D.	5.051



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2018 23:47
Operator : EI\SJ
Sample : J4906-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:46:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

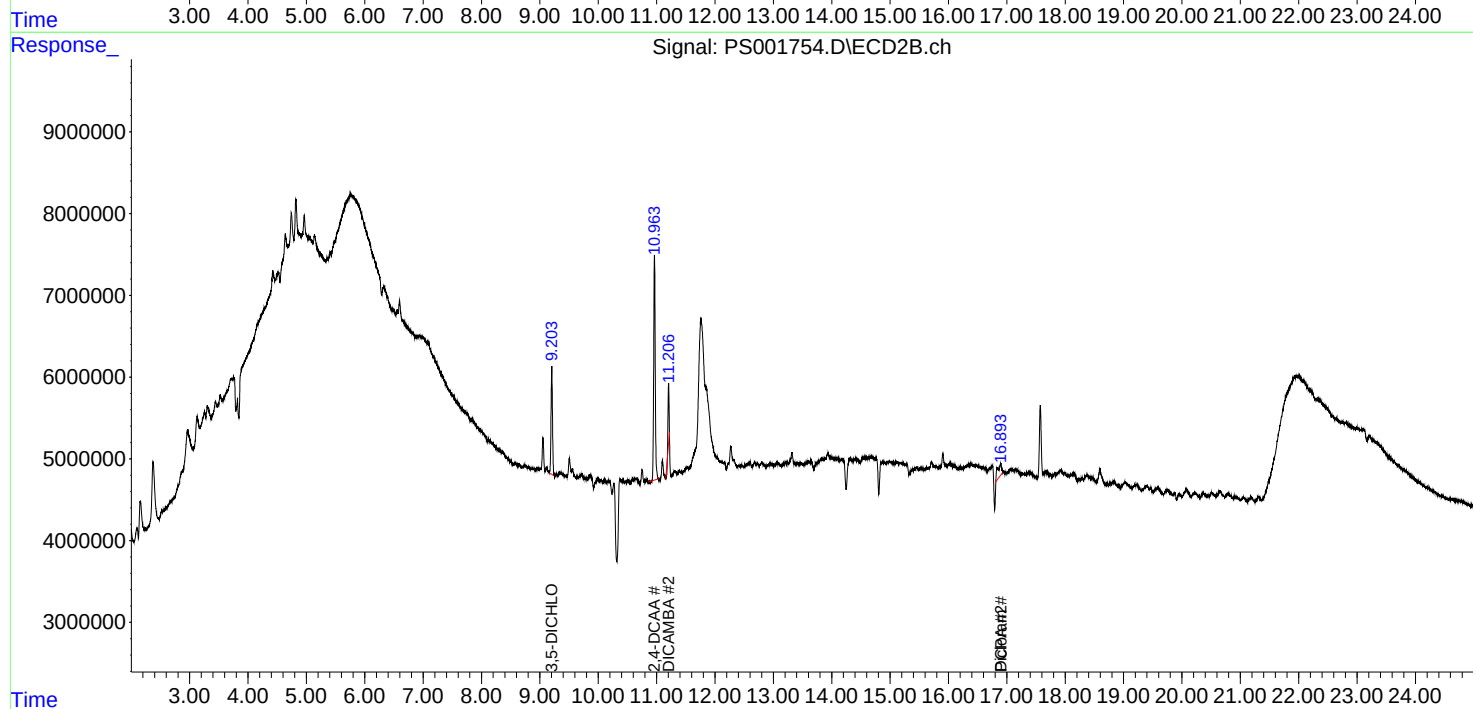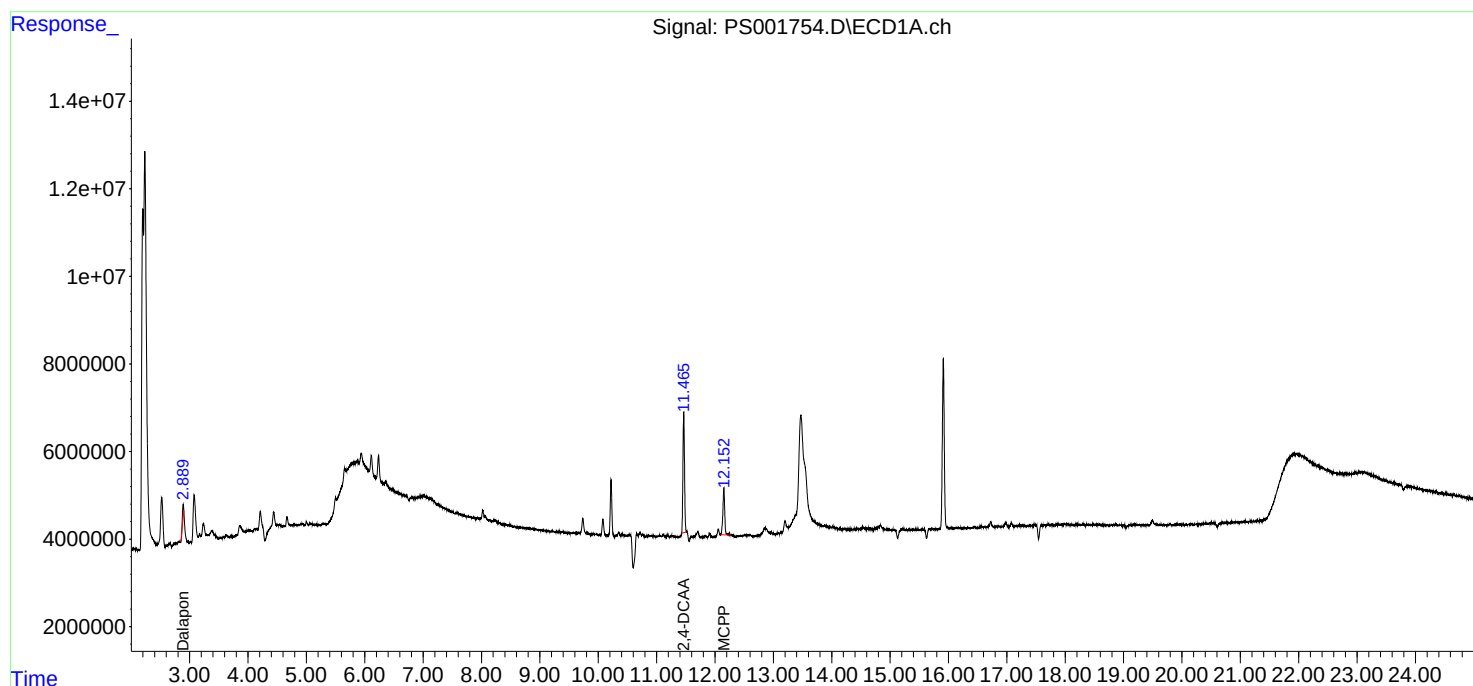


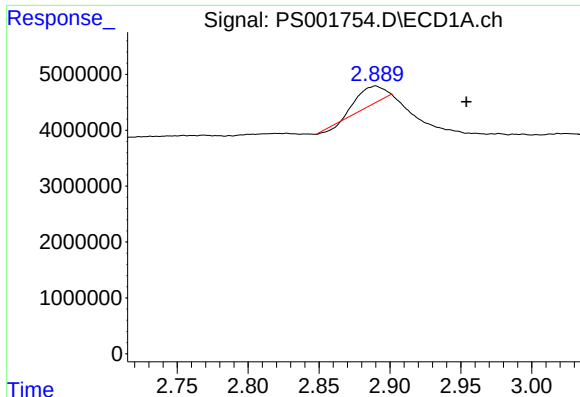

#1 Dalapon


R.T.: 2.890 min
Delta R.T.: -0.064 min
Response: 4318496
Conc: 17.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

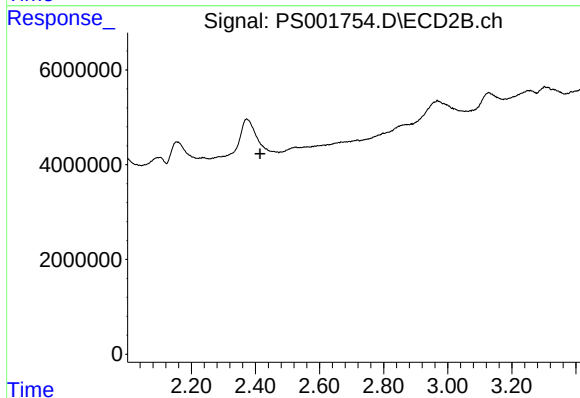


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.414 min
Response: 0
Conc: N.D.

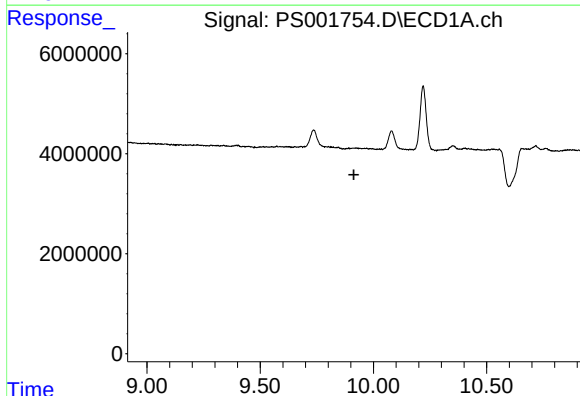


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

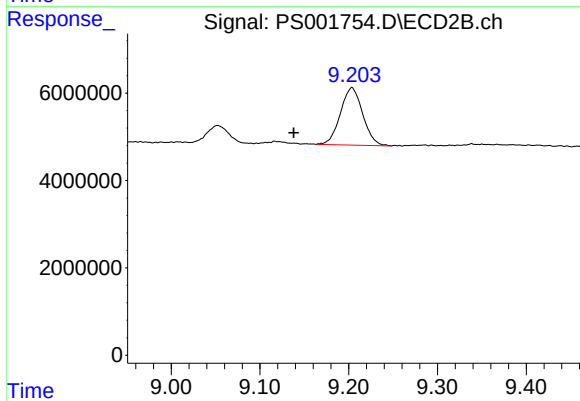

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.204 min
Delta R.T.: 0.066 min
Response: 23042078
Conc: 90.16 ng/ml

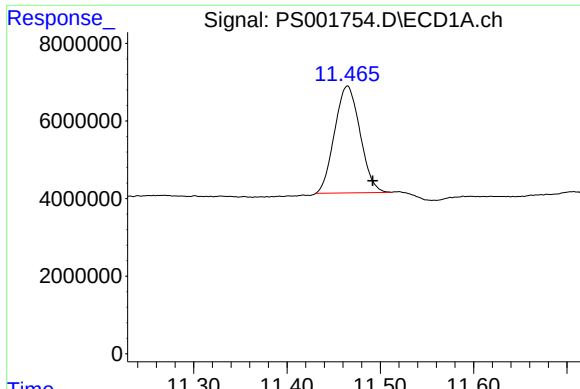

#4 2,4-DCAA


R.T.: 11.465 min
Delta R.T.: -0.027 min
Response: 52162863
Conc: 282.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

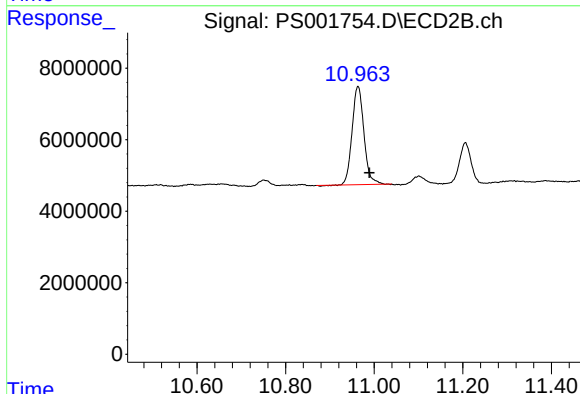


#4 2,4-DCAA

R.T.: 10.964 min
Delta R.T.: -0.025 min
Response: 51043647
Conc: 252.03 ng/ml

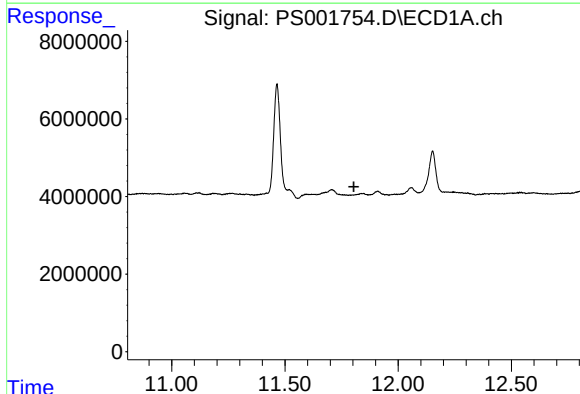


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

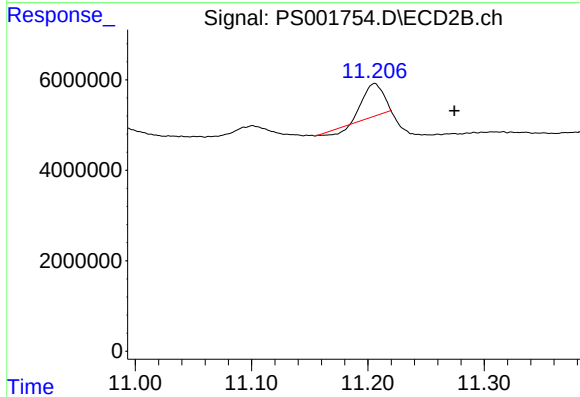

#5 DICAMBA


R.T.: 11.206 min
Delta R.T.: -0.069 min
Response: 7677857
Conc: 10.95 ng/ml

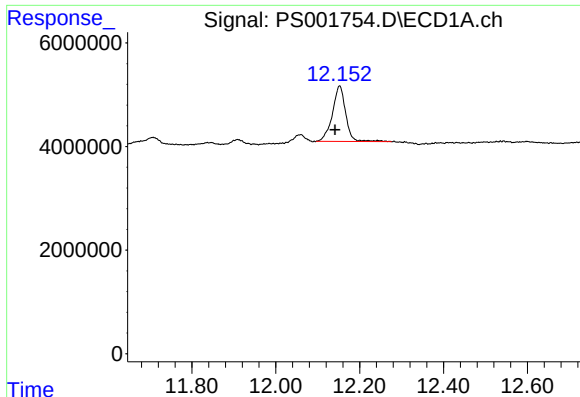

#6 MCP


R.T.: 12.152 min
Delta R.T.: 0.011 min
Response: 23633115
Conc: 46.97 ug/ml

Instrument :
ECD_S
ClientSampleId :

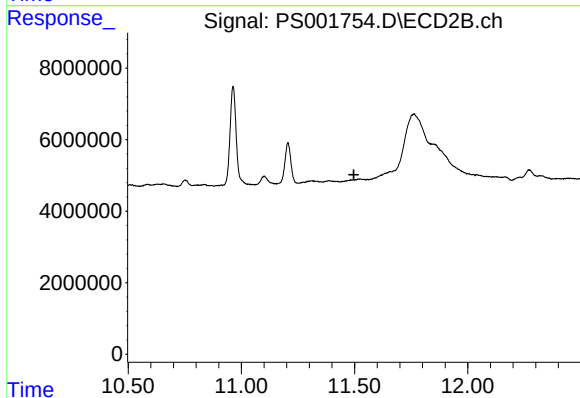


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

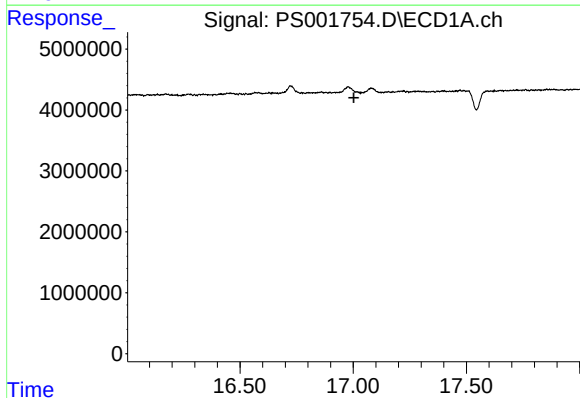


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.003 min
Response: 0
Conc: N.D.

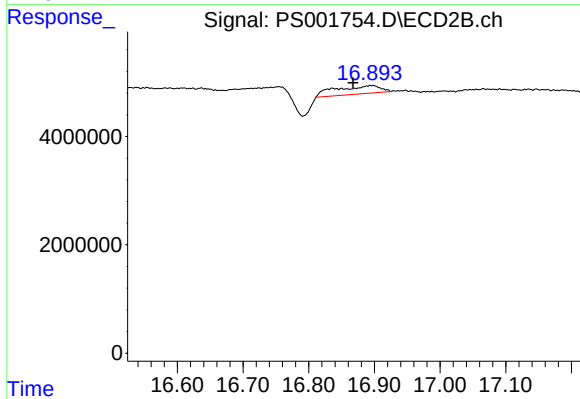

#15 Picloram


R.T.: 16.896 min
Delta R.T.: 0.029 min
Response: 7211209
Conc: 5.53 ng/ml

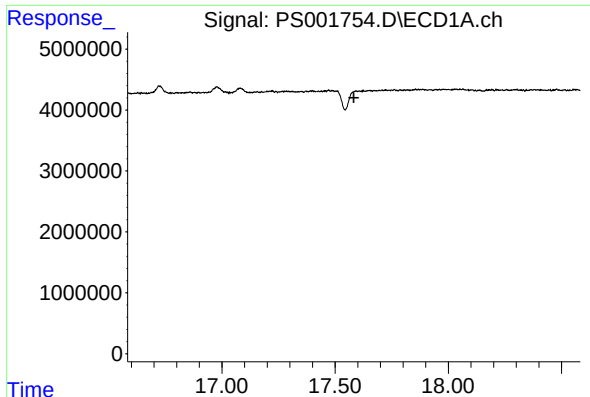

#16 DCPA

R.T.: 17.592 min
Delta R.T.: 0.009 min
Response: -3399100
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

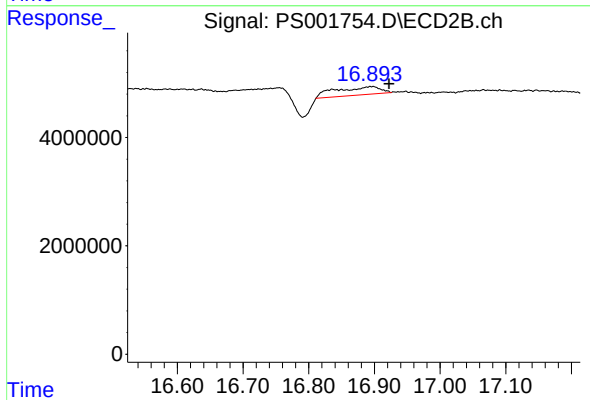

#16 DCPA

R.T.: 16.896 min
Delta R.T.: -0.026 min
Response: 7211209
Conc: 5.05 ng/ml