

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 00:49
 Operator : EI\SJ
 Sample : J4906-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:41:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.509	11.009	76880429	68164916	416.469	336.567
Target Compounds							
1) T	Dalapon	2.936	2.418	25823901	30249006	102.731	126.391
2) T	3,5-DICHL...	0.000	9.097	0	8491977	N.D.	33.230 #
5) T	DICAMBA	0.000	11.252	0	21780200	N.D.	31.055 #
6) T	MCP	12.197	0.000	22928112	0	45.568	N.D. #
7) T	MCPA	0.000	11.814	0	9855650	N.D.	13.523 #
11) T	2,4,5-TP ...	0.000	13.976	0	10736321	N.D.	10.101 #
13) T	2,4-DB	15.771	0.000	6138338	0	45.698	N.D. #
16) T	DCPA	0.000	16.942	0	2181090	N.D.	1.528 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 00:49
Operator : EI\SJ
Sample : J4906-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:41:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

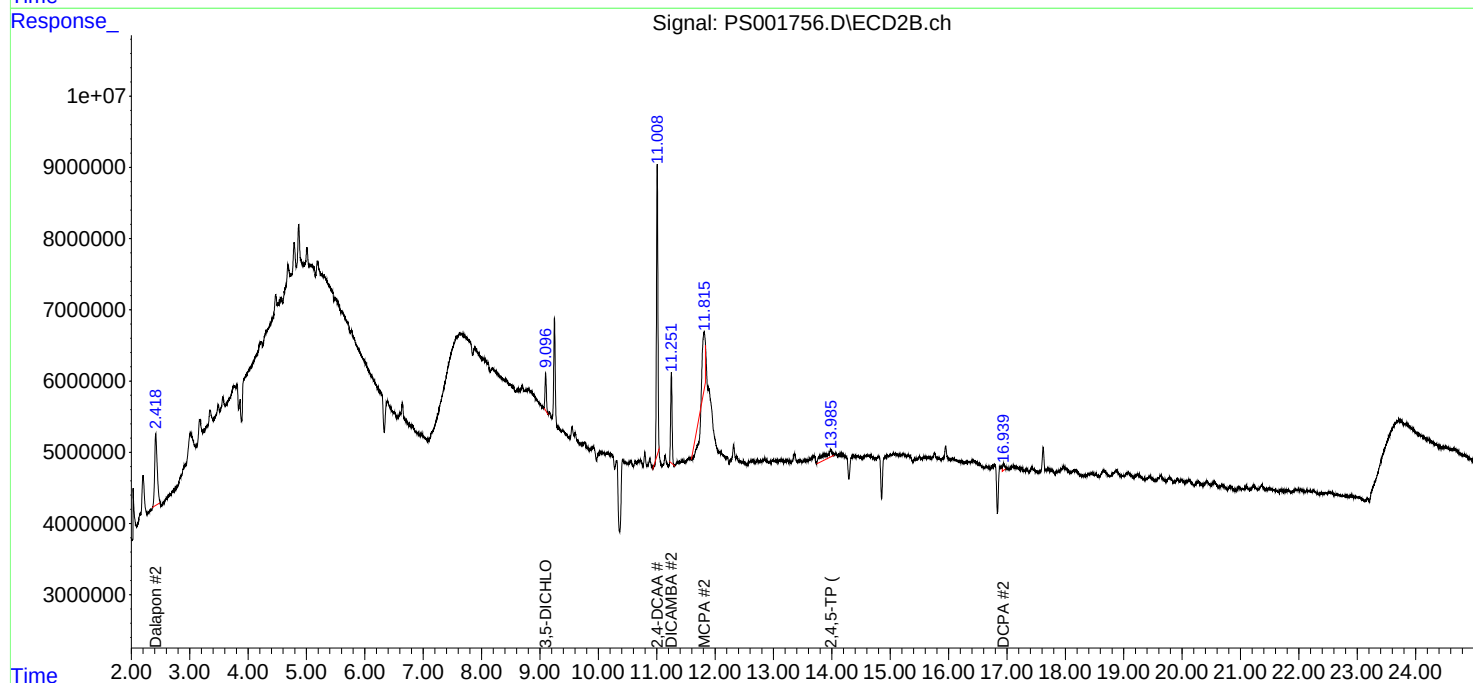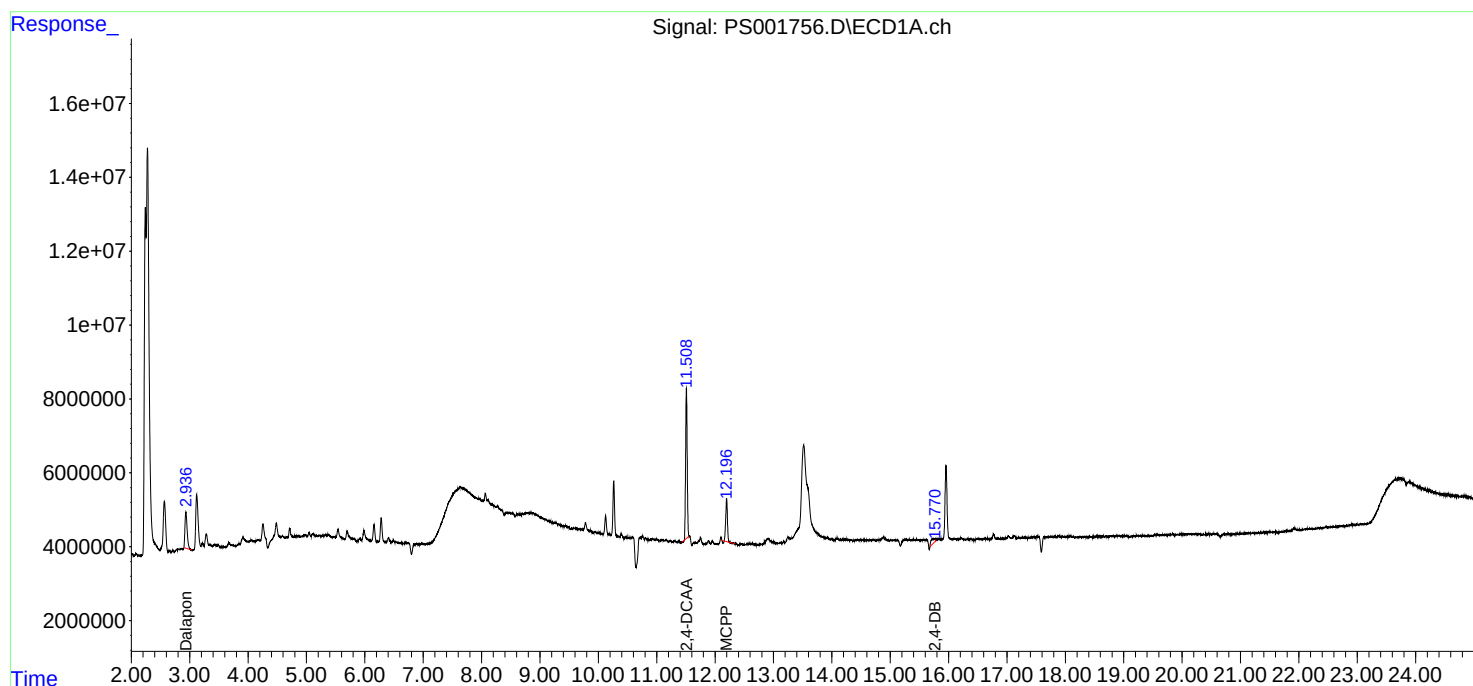


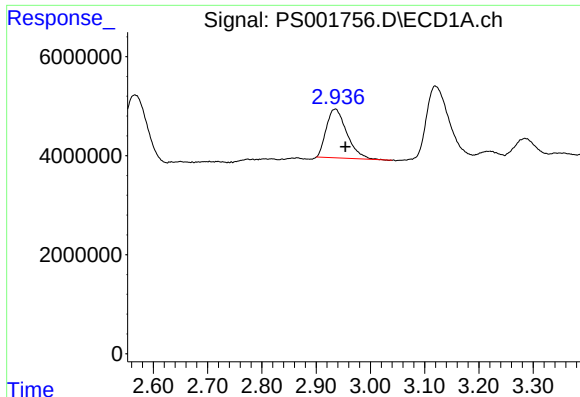

#1 Dalapon


R.T.: 2.936 min
Delta R.T.: -0.018 min
Response: 25823901
Conc: 102.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

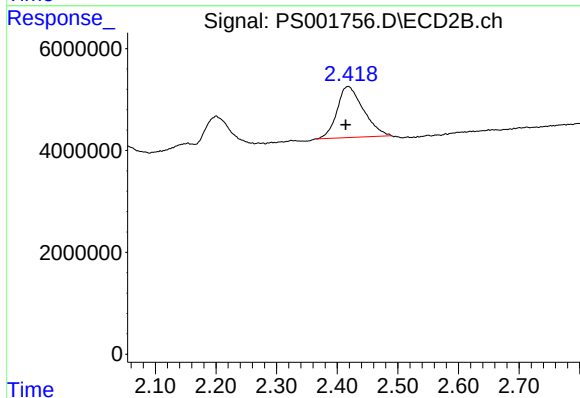


#1 Dalapon

R.T.: 2.418 min
Delta R.T.: 0.004 min
Response: 30249006
Conc: 126.39 ng/ml

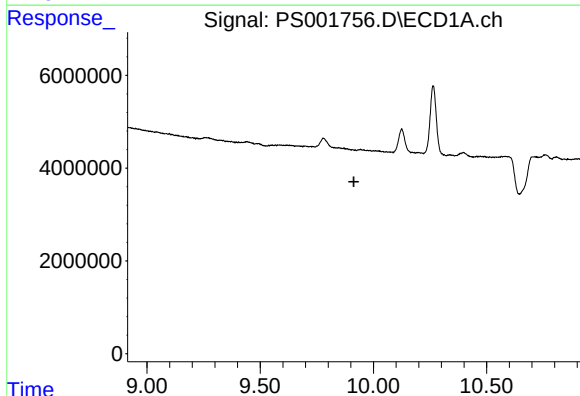


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

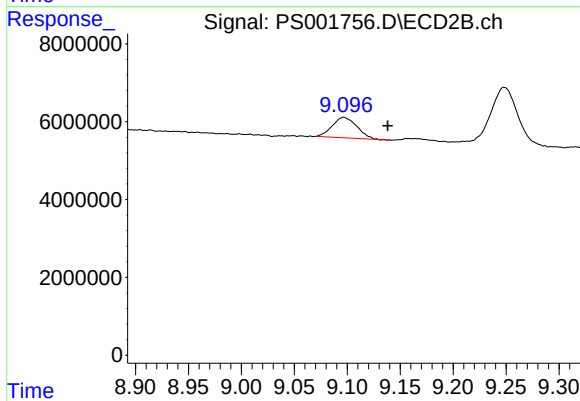

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.097 min
Delta R.T.: -0.041 min
Response: 8491977
Conc: 33.23 ng/ml

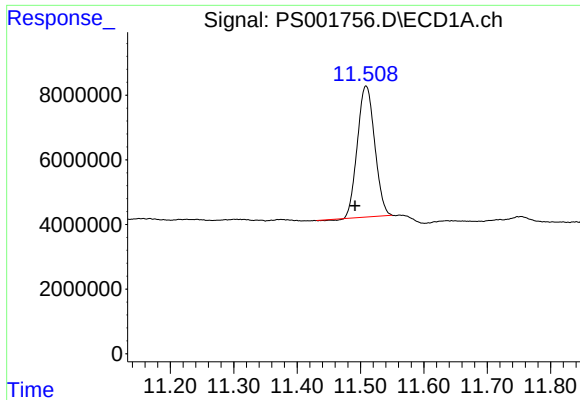

#4 2,4-DCAA


R.T.: 11.509 min
Delta R.T.: 0.017 min
Response: 76880429
Conc: 416.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

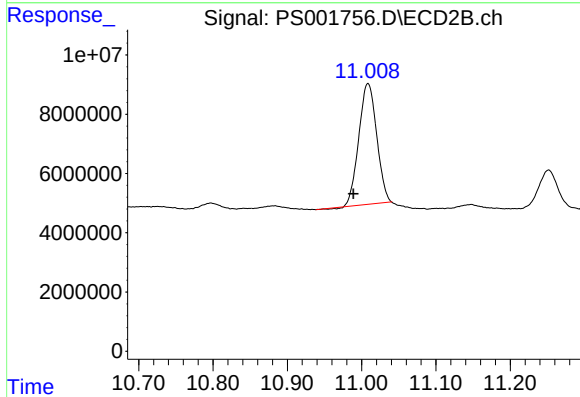


#4 2,4-DCAA

R.T.: 11.009 min
Delta R.T.: 0.020 min
Response: 68164916
Conc: 336.57 ng/ml

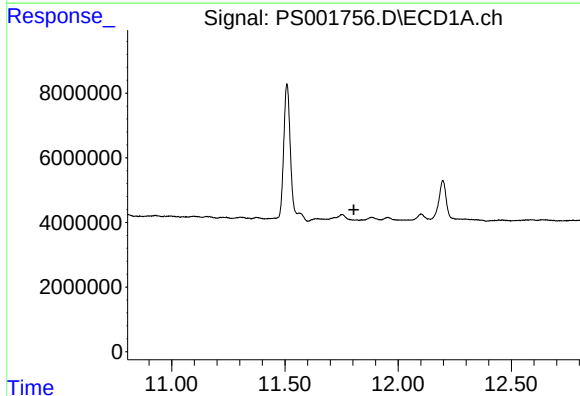


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

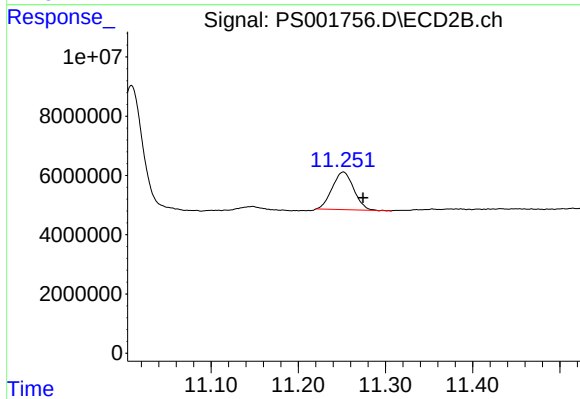

#5 DICAMBA


R.T.: 11.252 min
Delta R.T.: -0.023 min
Response: 21780200
Conc: 31.05 ng/ml

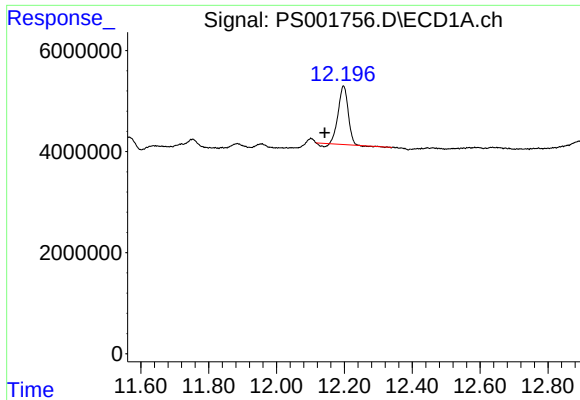

#6 MCPP


R.T.: 12.197 min
Delta R.T.: 0.056 min
Response: 22928112
Conc: 45.57 ug/ml

Instrument :
ECD_S
ClientSampleId :

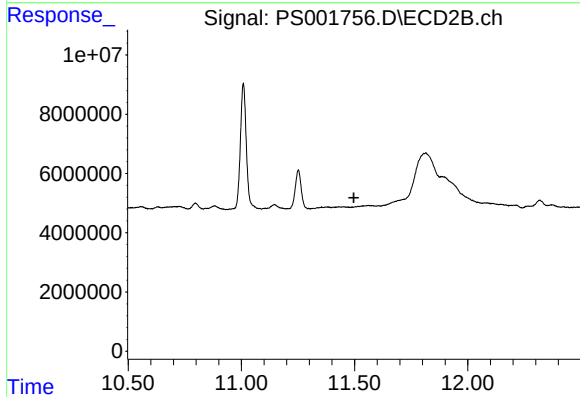


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

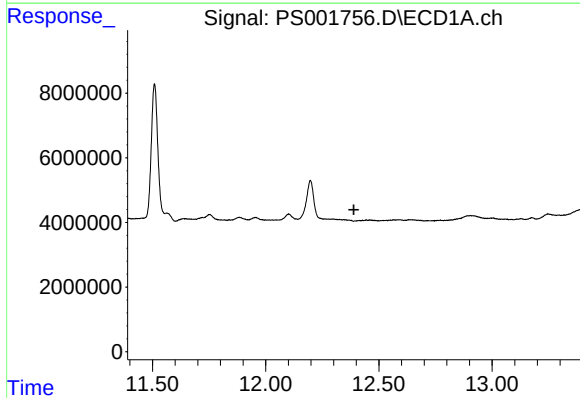


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.390 min
Response: 0
Conc: N.D.

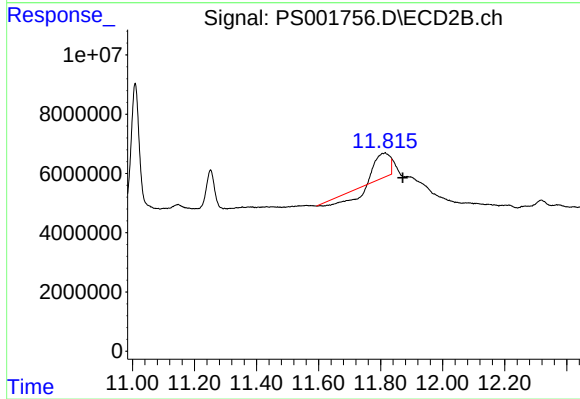

#7 MCPA


R.T.: 11.814 min
Delta R.T.: -0.057 min
Response: 9855650
Conc: 13.52 ug/ml

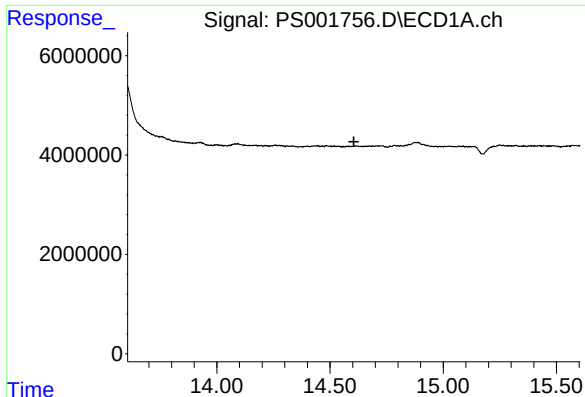

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

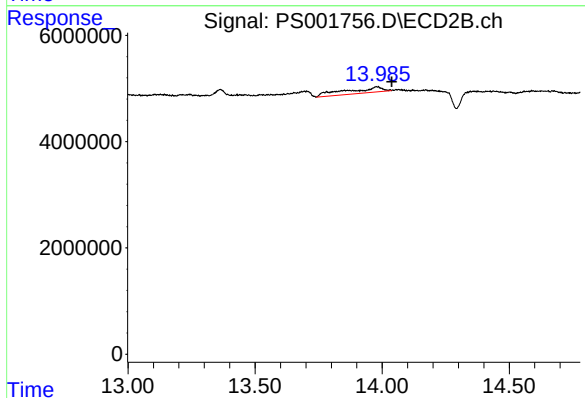


#11 2,4,5-TP (SILVEX)

R.T.: 13.976 min
Delta R.T.: -0.062 min
Response: 10736321
Conc: 10.10 ng/ml

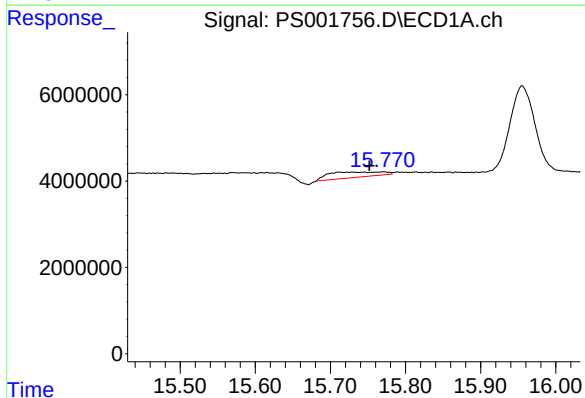


#13 2,4-DB

R.T.: 15.771 min
Delta R.T.: 0.019 min
Response: 6138338
Conc: 45.70 ng/ml

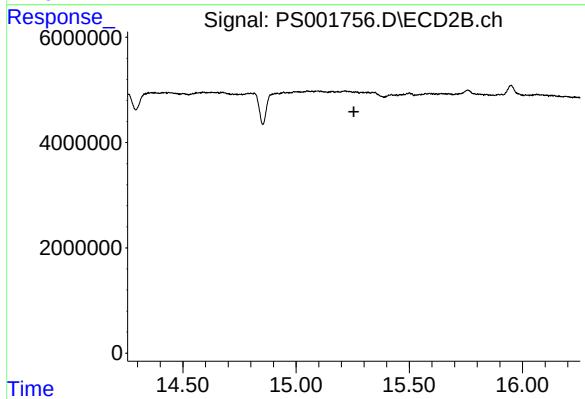

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.255 min
Response: 0
Conc: N.D.

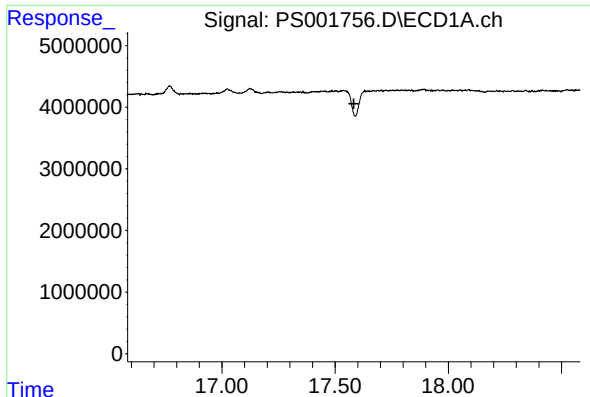

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

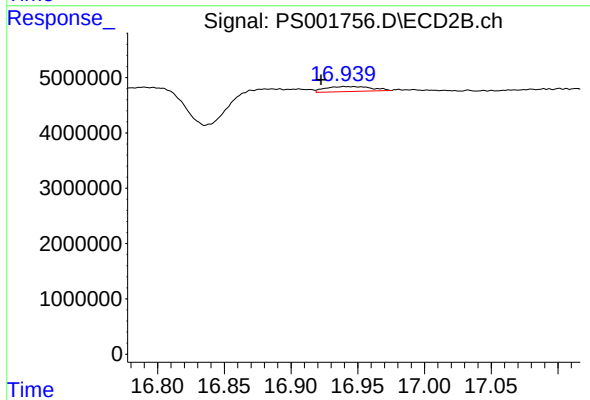

#16 DCPA

R.T.: 16.942 min
Delta R.T.: 0.020 min
Response: 2181090
Conc: 1.53 ng/ml