

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 01:51
 Operator : EI\SJ
 Sample : J4906-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:41:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.493	10.992	81830222	78898633	443.283	389.565
Target Compounds							
1) T	Dalapon	2.918	2.401	1298610	21923390	5.166	91.604 #
2) T	3,5-DICHL...	0.000	9.082	0	3483998	N.D.	13.633 #
5) T	DICAMBA	0.000	11.235	0	9896146	N.D.	14.110 #
6) T	MCP	12.181	0.000	20495426	0	40.733	N.D. #
15) T	Picloram	0.000	16.924	0	22822644	N.D.	17.503 #
16) T	DCPA	0.000	16.924	0	22822644	N.D.	15.985 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 01:51
Operator : EI\SJ
Sample : J4906-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:41:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

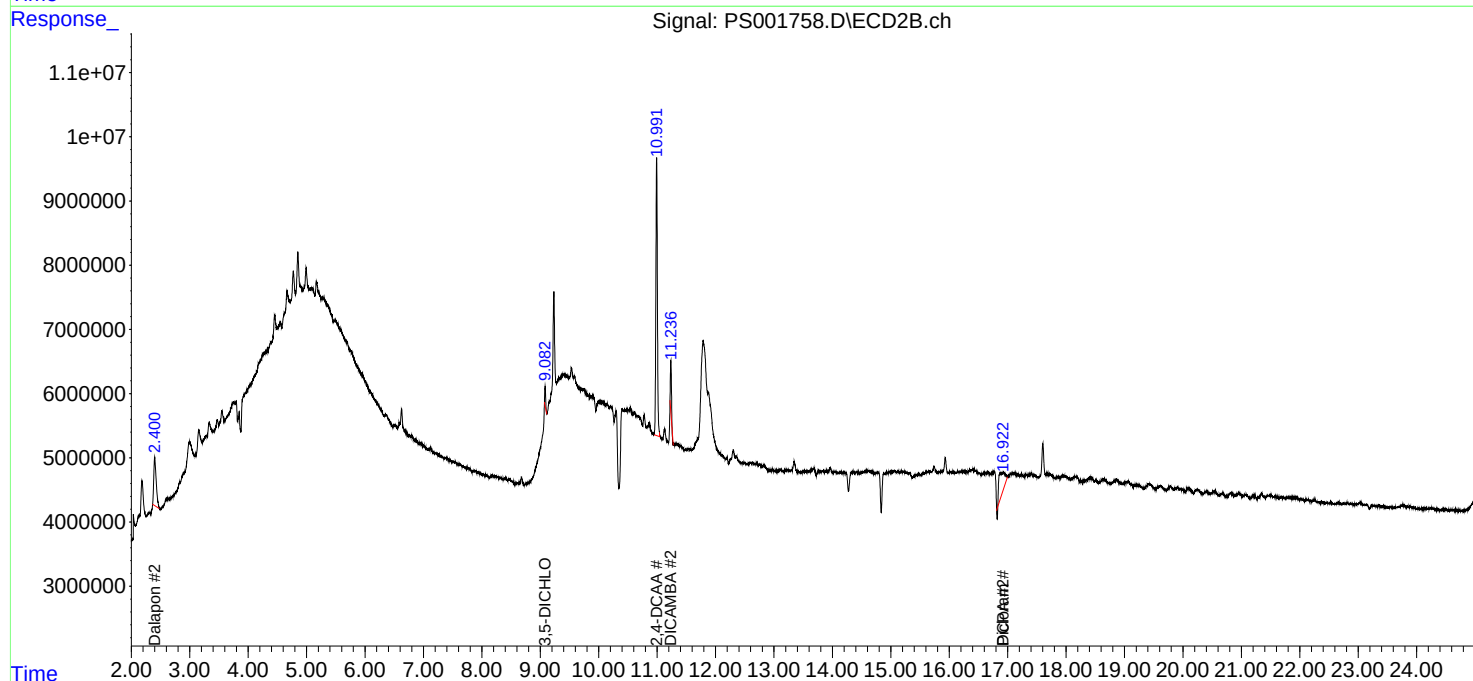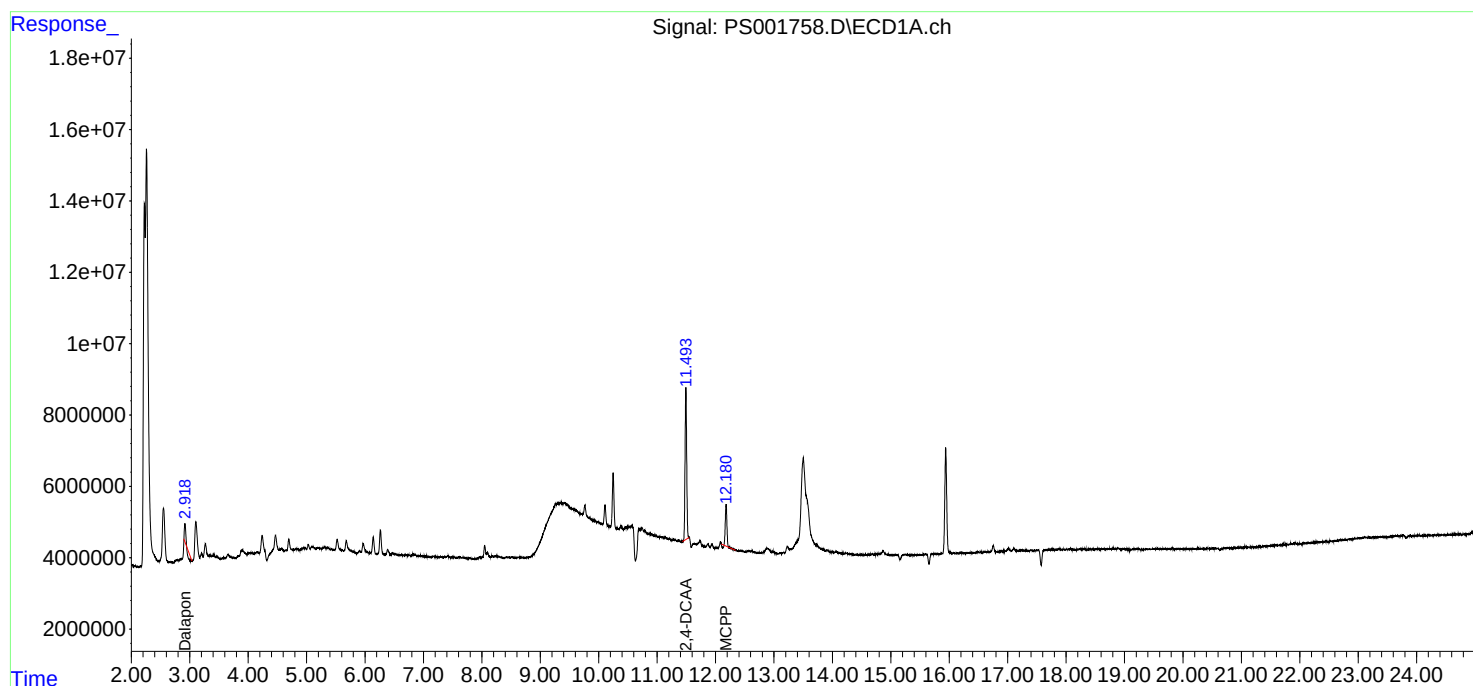


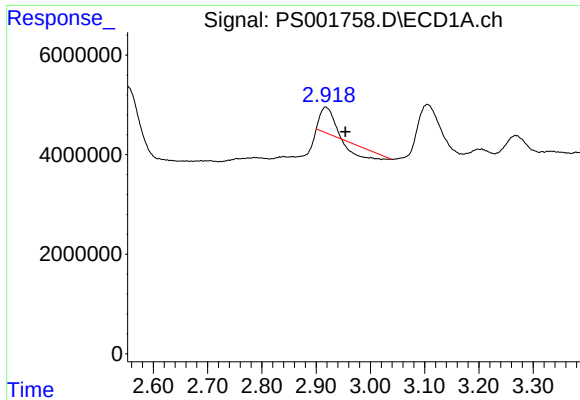

#1 Dalapon


R.T.: 2.918 min
Delta R.T.: -0.036 min
Response: 1298610
Conc: 5.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

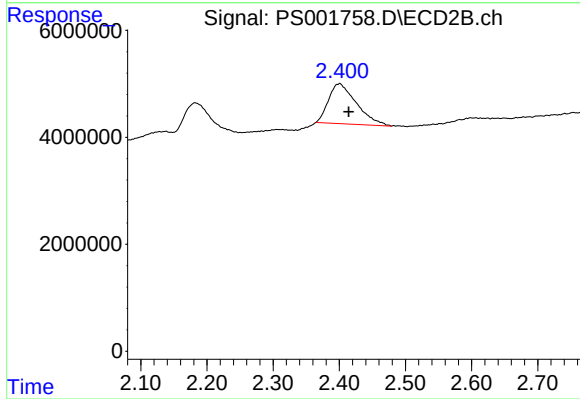


#1 Dalapon

R.T.: 2.401 min
Delta R.T.: -0.013 min
Response: 21923390
Conc: 91.60 ng/ml

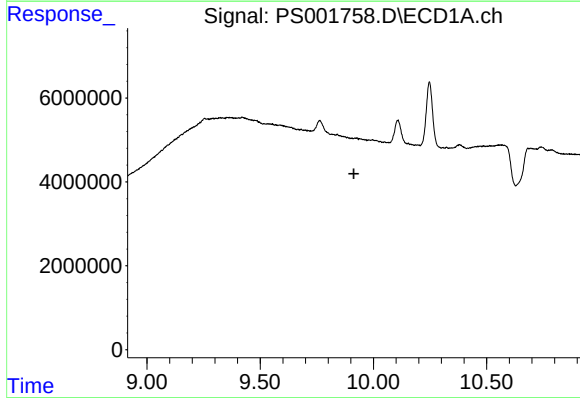


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

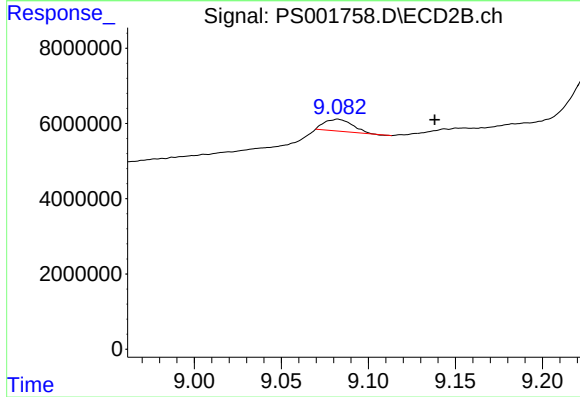

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.082 min
Delta R.T.: -0.056 min
Response: 3483998
Conc: 13.63 ng/ml

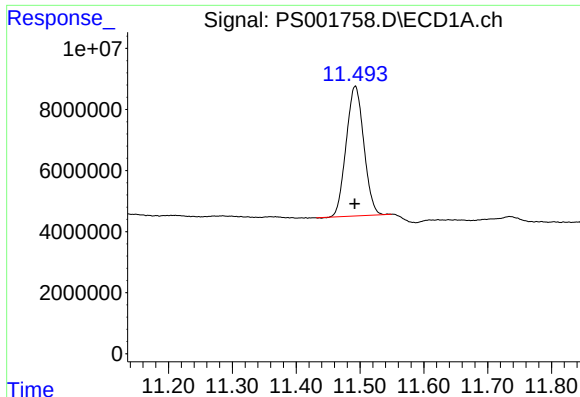

#4 2,4-DCAA


R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 81830222
Conc: 443.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

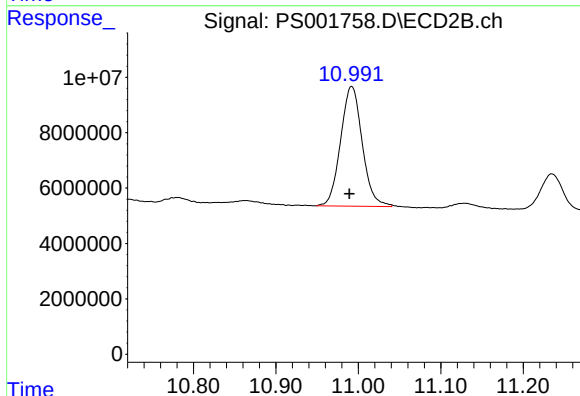


#4 2,4-DCAA

R.T.: 10.992 min
Delta R.T.: 0.003 min
Response: 78898633
Conc: 389.57 ng/ml

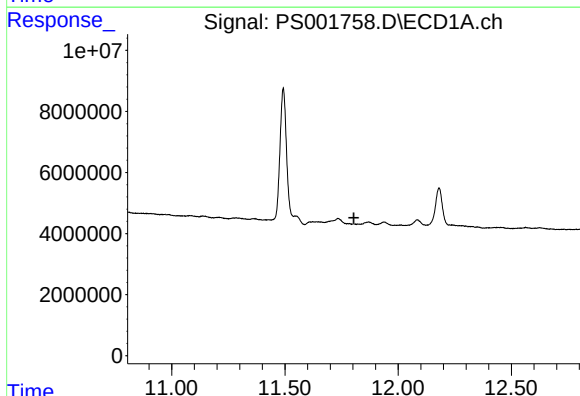


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

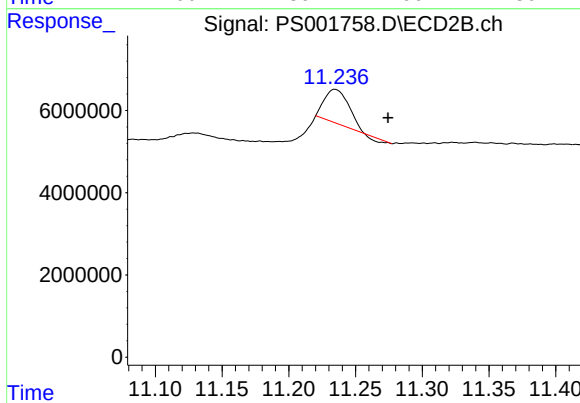

#5 DICAMBA


R.T.: 11.235 min
Delta R.T.: -0.040 min
Response: 9896146
Conc: 14.11 ng/ml

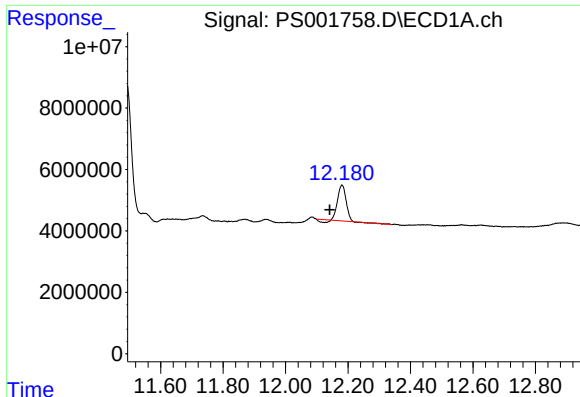

#6 MCP


R.T.: 12.181 min
Delta R.T.: 0.039 min
Response: 20495426
Conc: 40.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

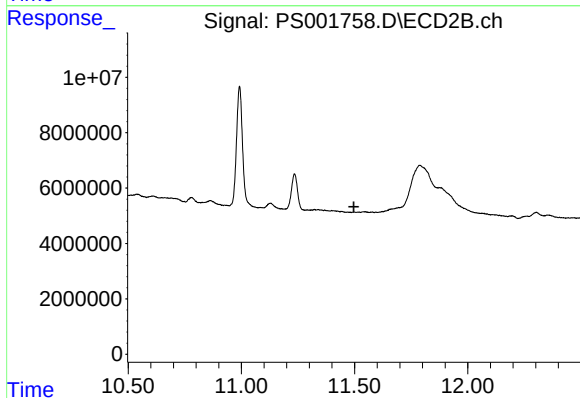


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

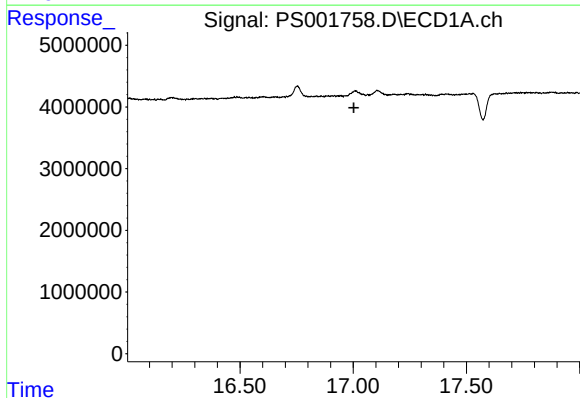


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.003 min
Response: 0
Conc: N.D.

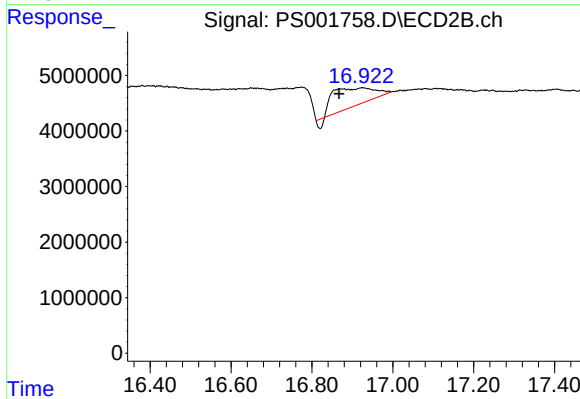

#15 Picloram


R.T.: 16.924 min
Delta R.T.: 0.057 min
Response: 22822644
Conc: 17.50 ng/ml

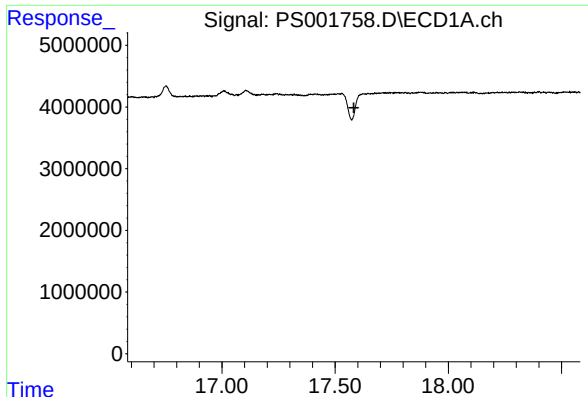

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

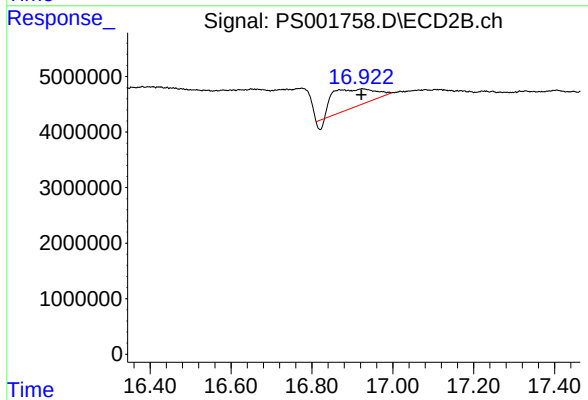

#16 DCPA

R.T.: 16.924 min
Delta R.T.: 0.002 min
Response: 22822644
Conc: 15.99 ng/ml