

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
 Data File : PS001759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2018 02:22
 Operator : EI\SJ
 Sample : J4906-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 03:41:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.458	10.957	86124329	86493949	466.544	427.067
Target Compounds							
2) T	3,5-DICHL...	0.000	9.198	0	28608037	N.D.	111.945 #
6) T	MCP	12.147	0.000	28822621	0	57.283	N.D. #
15) T	Picloram	0.000	16.892	0	3989974	N.D.	3.060 #
16) T	DCPA	17.629	16.892	1115880	3989974	0.983	2.795 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091418\
Data File : PS001759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2018 02:22
Operator : EI\SJ
Sample : J4906-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 03:41:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

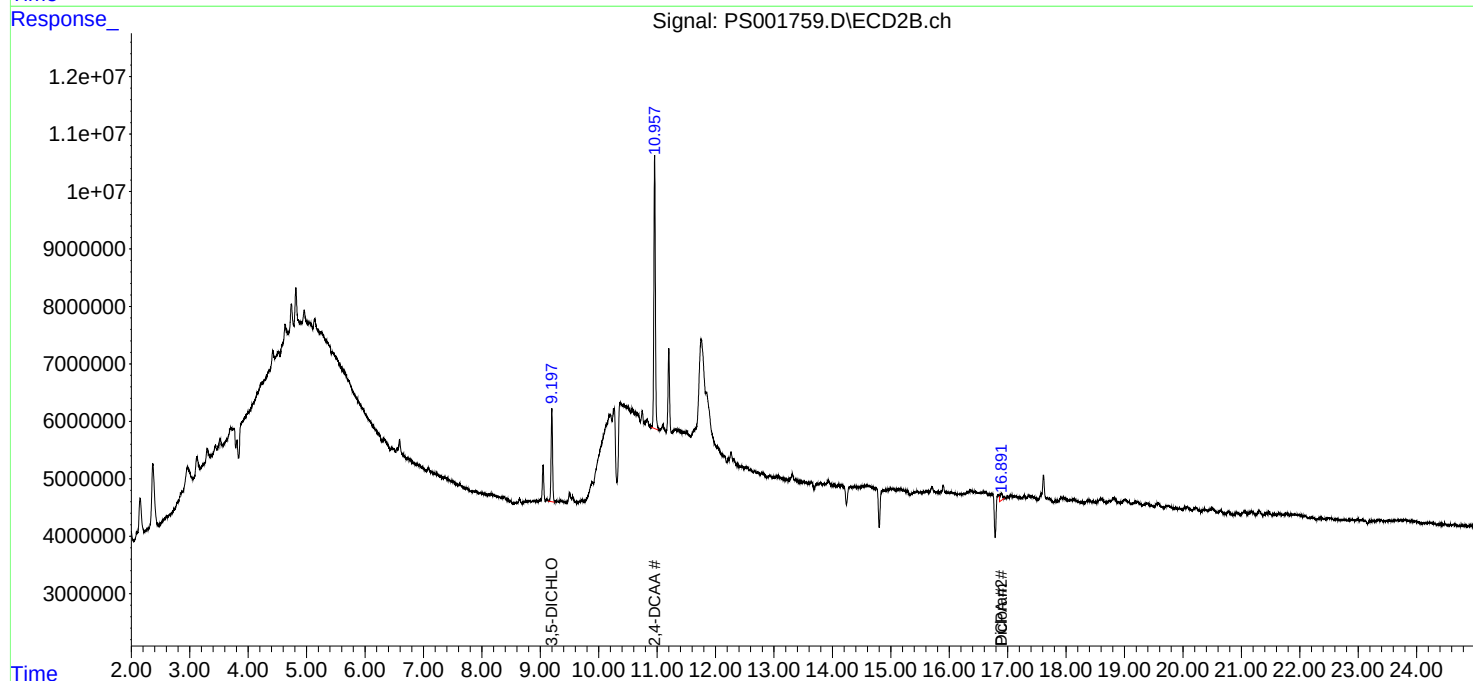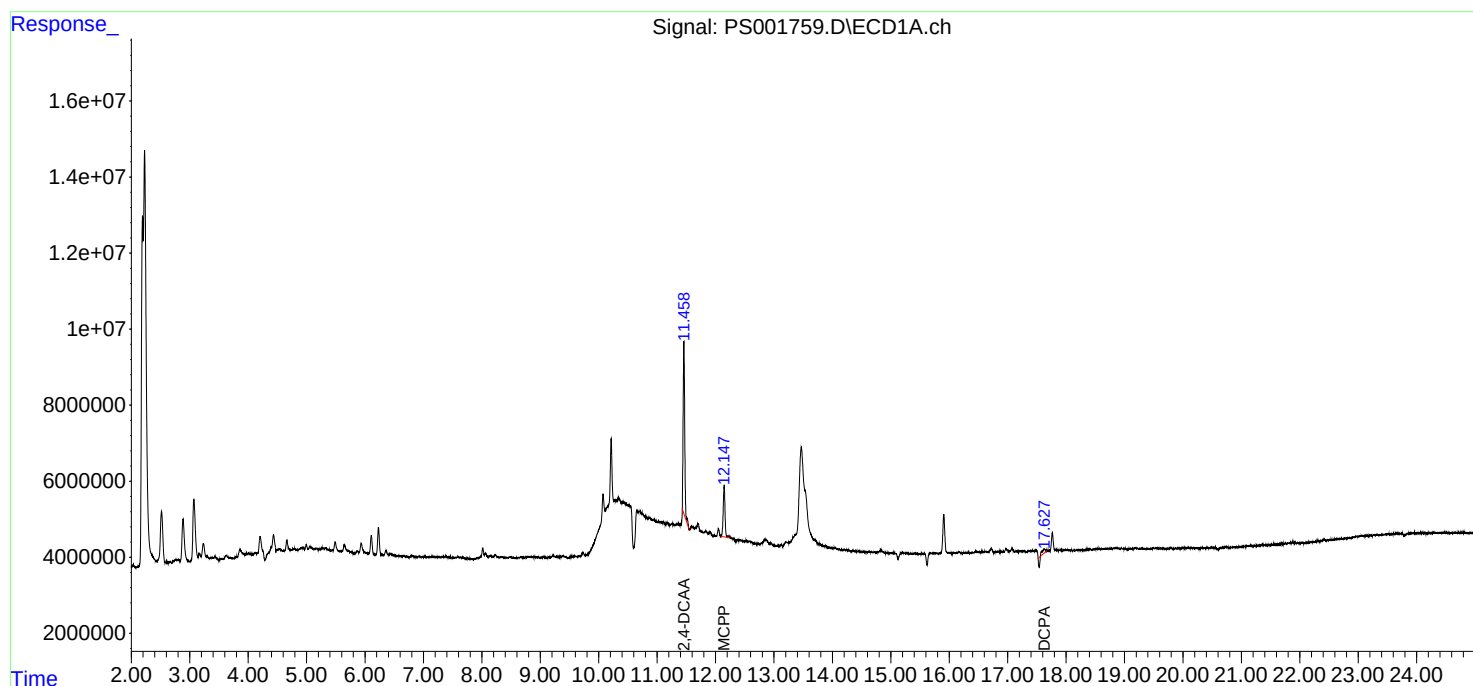


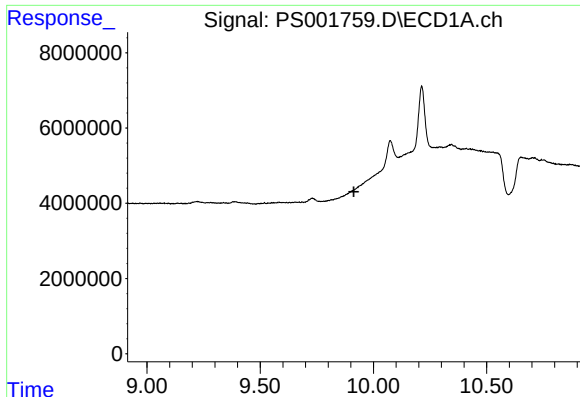

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

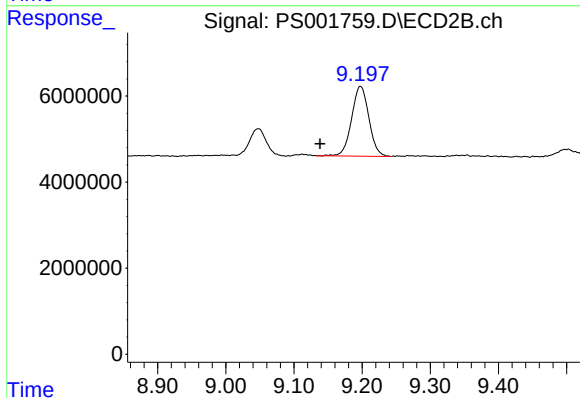


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.198 min
Delta R.T.: 0.059 min
Response: 28608037
Conc: 111.94 ng/ml

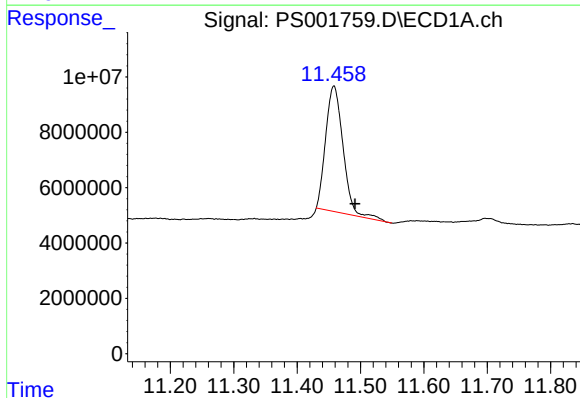


#4 2,4-DCAA

R.T.: 11.458 min
Delta R.T.: -0.034 min
Response: 86124329
Conc: 466.54 ng/ml

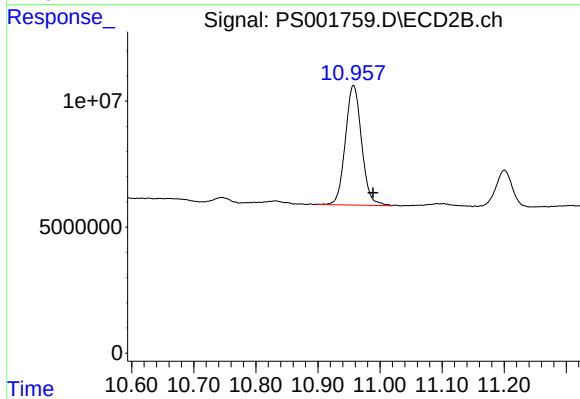

#4 2,4-DCAA


R.T.: 10.957 min
Delta R.T.: -0.032 min
Response: 86493949
Conc: 427.07 ng/ml

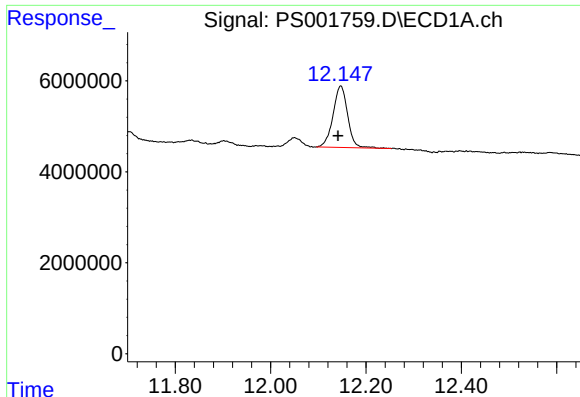

#6 MCP


R.T.: 12.147 min
Delta R.T.: 0.005 min
Response: 28822621
Conc: 57.28 ug/ml

Instrument :
ECD_S
ClientSampleId :

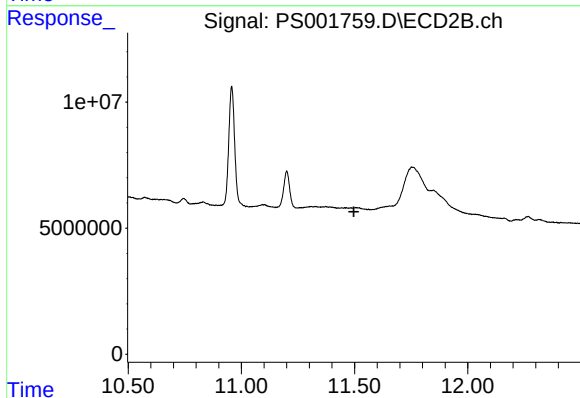


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

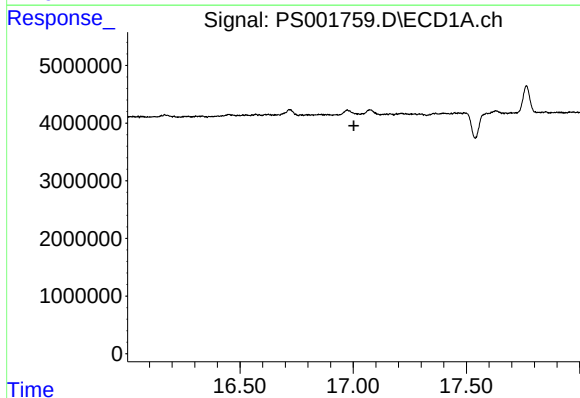


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.003 min
Response: 0
Conc: N.D.

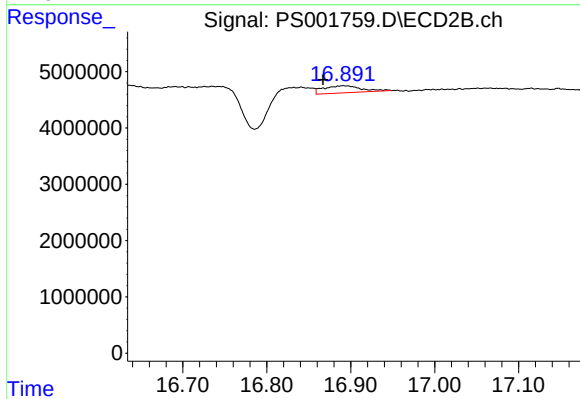

#15 Picloram


R.T.: 16.892 min
Delta R.T.: 0.025 min
Response: 3989974
Conc: 3.06 ng/ml

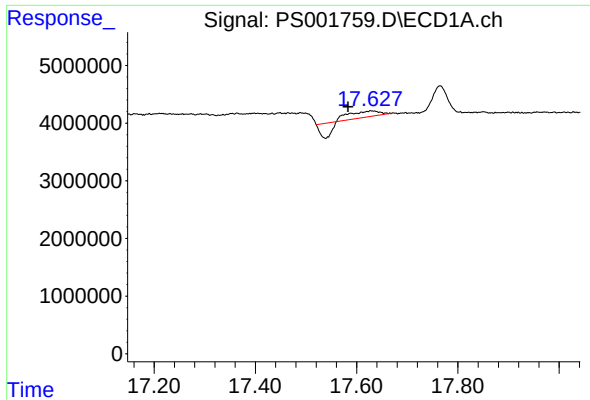

#16 DCPA

R.T.: 17.629 min
Delta R.T.: 0.047 min
Response: 1115880
Conc: 0.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

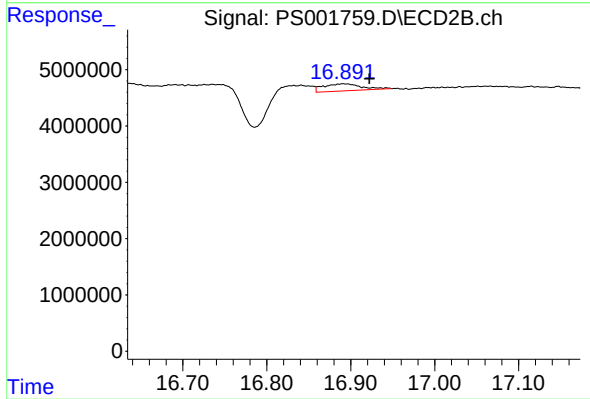

#16 DCPA

R.T.: 16.892 min
Delta R.T.: -0.031 min
Response: 3989974
Conc: 2.79 ng/ml