

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091420\
 Data File : PS012241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2020 17:59
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 05:54:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 05:52:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	800.7E6	391.0E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.032	2.622	836.0E6	457.6E6	682.500	682.500
2) T	3,5-DICHL...	6.431	6.065	1009.7E6	557.9E6	697.500	697.500
3) T	4-Nitroph...	7.048	6.522	360.3E6	218.7E6	682.500	682.500
5) T	DICAMBA	7.407	7.080	2950.4E6	1511.0E6	705.000	705.000
6) T	MCPD	7.576	7.177	229.2E6	121.0E6	70.500	70.500
7) T	MCPA	7.726	7.392	325.8E6	191.5E6	69.750	69.750
8) T	DICHLORPROP	8.099	7.706	709.7E6	391.0E6	705.000	705.000
9) T	2,4-D	8.329	8.001	793.3E6	505.0E6	705.000	705.000
10) T	Pentachlo...	8.638	8.429	10377.7E6	4735.7E6	712.500	712.500
11) T	2,4,5-TP ...	9.187	8.789	4160.8E6	2042.6E6	712.500	712.500
12) T	2,4,5-T	9.473	9.170	4308.9E6	2048.4E6	712.500	712.500
13) T	2,4-DB	10.026	9.677	544.1E6	286.1E6	712.500	712.500
14) T	DINOSEB	11.183	10.007	3278.3E6	1454.5E6	705.000	705.000
15) T	Picloram	11.009	10.996	5281.4E6	3082.0E6	712.500	712.500
16) T	DCPA	11.448	10.935	5278.9E6	2587.9E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091420\
Data File : PS012241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2020 17:59
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 05:54:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 05:52:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

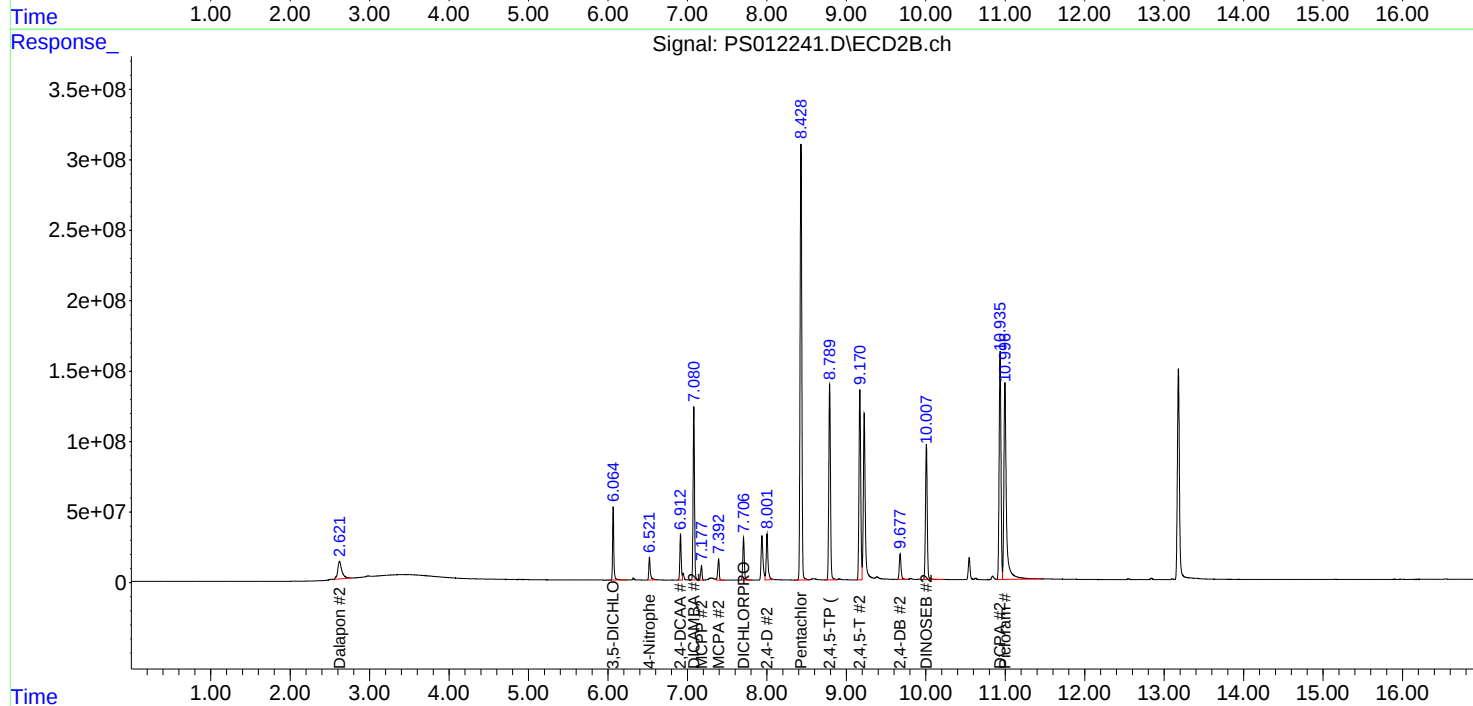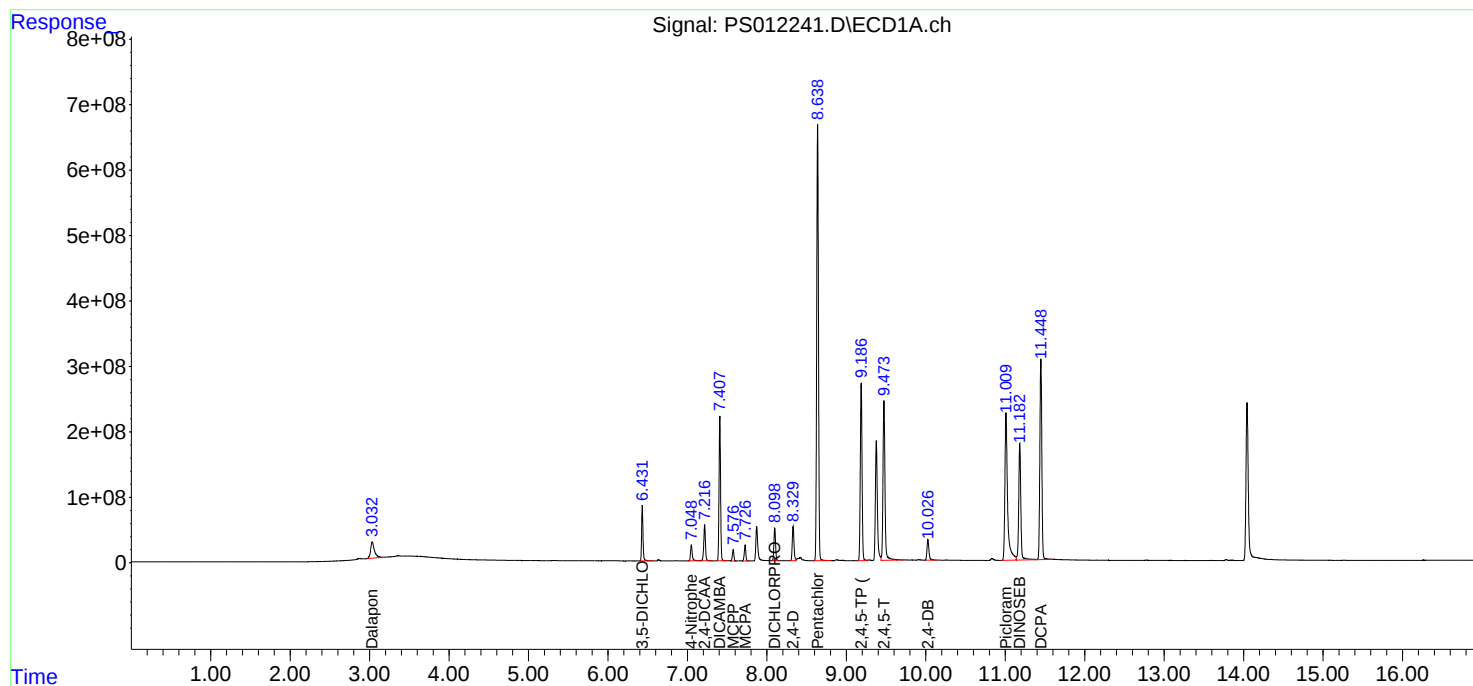


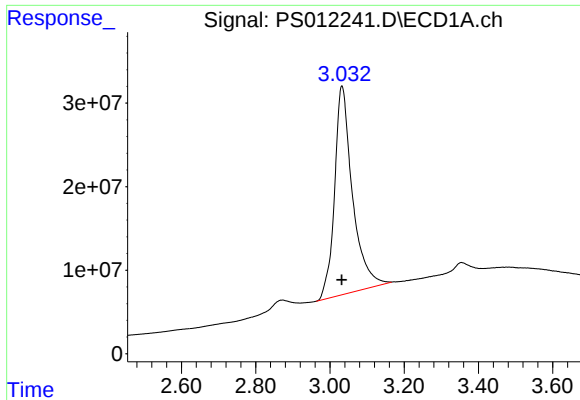

#1 Dalapon


R.T.: 3.032 min
Delta R.T.: 0.000 min
Response: 835983530
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

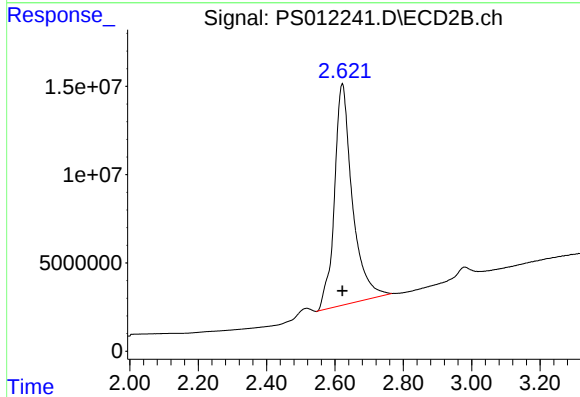


#1 Dalapon

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 457579466
Conc: 682.50 ng/ml

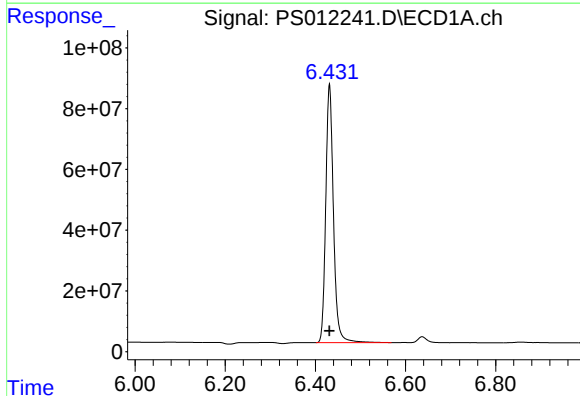


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.431 min
Delta R.T.: 0.000 min
Response: 1009700516
Conc: 697.50 ng/ml

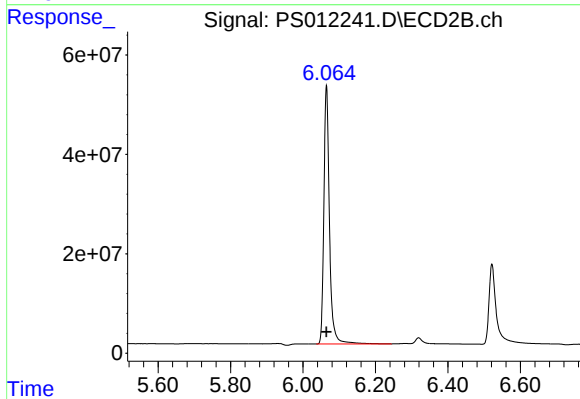

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 557885642
Conc: 697.50 ng/ml

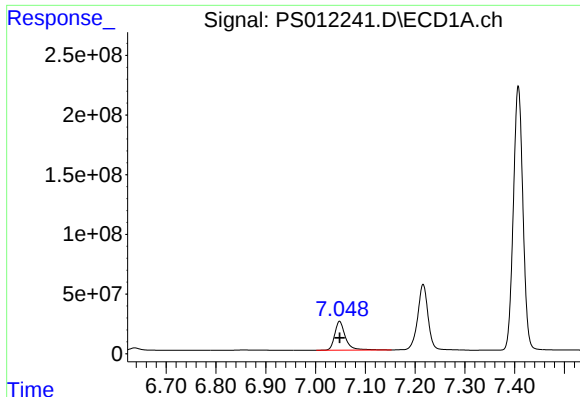

#3 4-Nitrophenol


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 360284482
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

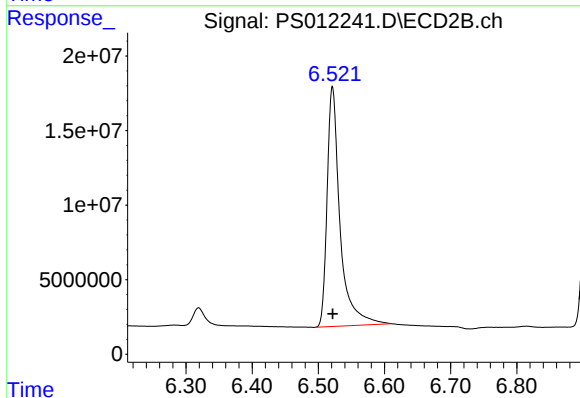


#3 4-Nitrophenol

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 218737306
Conc: 682.50 ng/ml

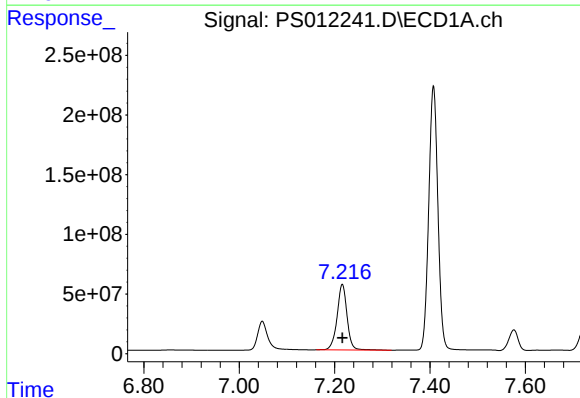


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 800700651
Conc: 750.00 ng/ml

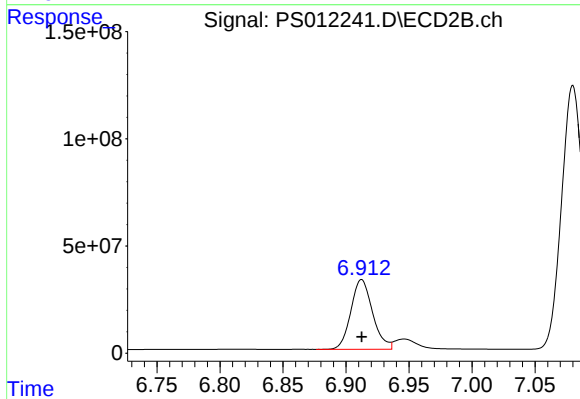

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 390990585
Conc: 750.00 ng/ml

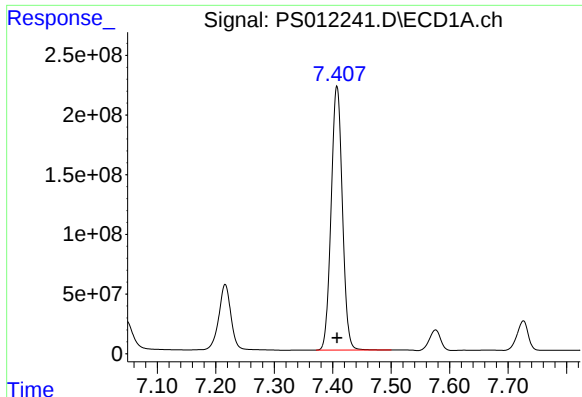

#5 DICAMBA


R.T.: 7.407 min
Delta R.T.: 0.000 min
Response: 2950397358
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

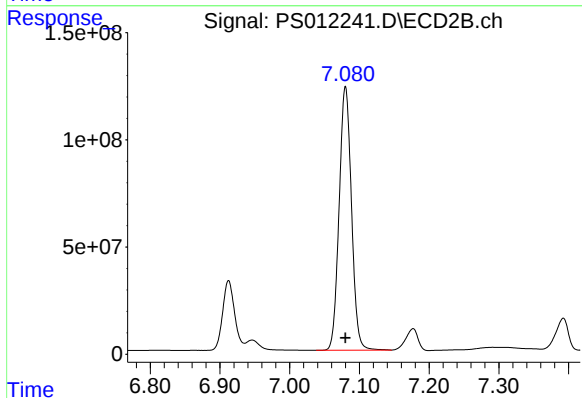


#5 DICAMBA

R.T.: 7.080 min
Delta R.T.: 0.000 min
Response: 1510969243
Conc: 705.00 ng/ml

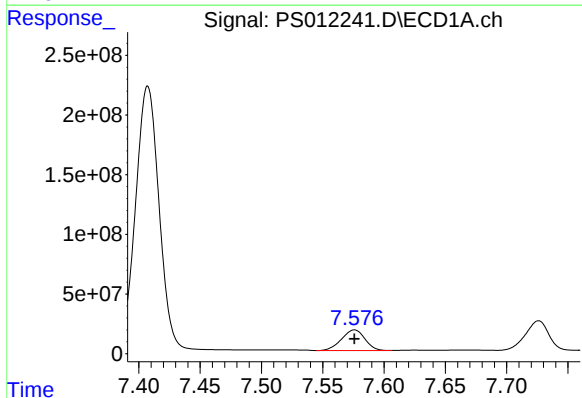


#6 MCP

R.T.: 7.576 min
Delta R.T.: 0.000 min
Response: 229176371
Conc: 70.50 ug/ml

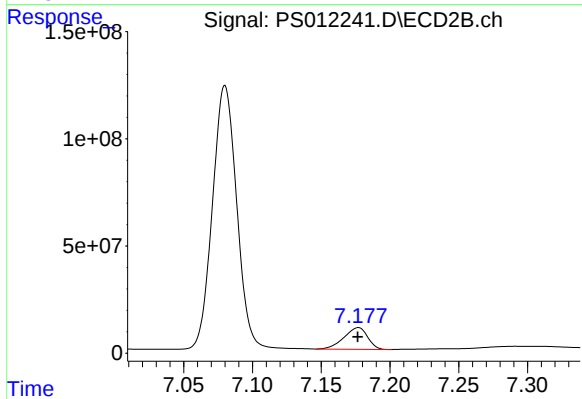

#6 MCP


R.T.: 7.177 min
Delta R.T.: 0.000 min
Response: 120989476
Conc: 70.50 ug/ml

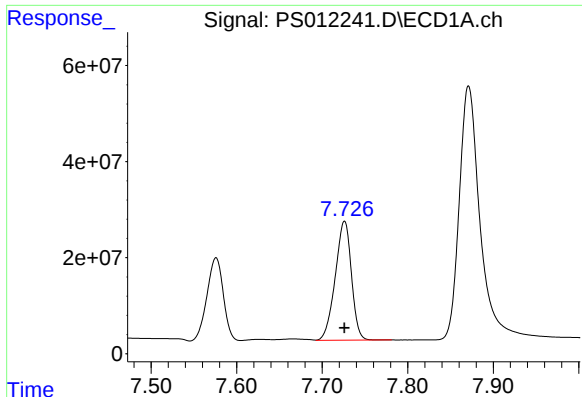

#7 MCPA


R.T.: 7.726 min
Delta R.T.: 0.000 min
Response: 325777750
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

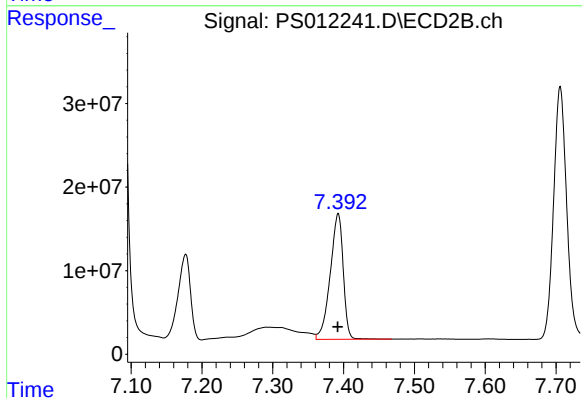


#7 MCPA

R.T.: 7.392 min
Delta R.T.: 0.000 min
Response: 191511241
Conc: 69.75 ug/ml

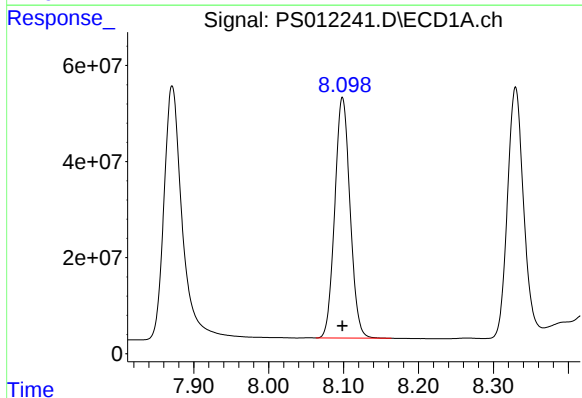


#8 DICHLORPROP

R.T.: 8.099 min
Delta R.T.: 0.000 min
Response: 709684888
Conc: 705.00 ng/ml

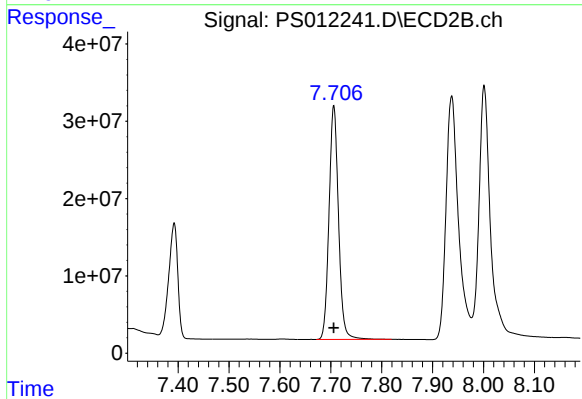

#8 DICHLORPROP


R.T.: 7.706 min
Delta R.T.: 0.000 min
Response: 390956154
Conc: 705.00 ng/ml

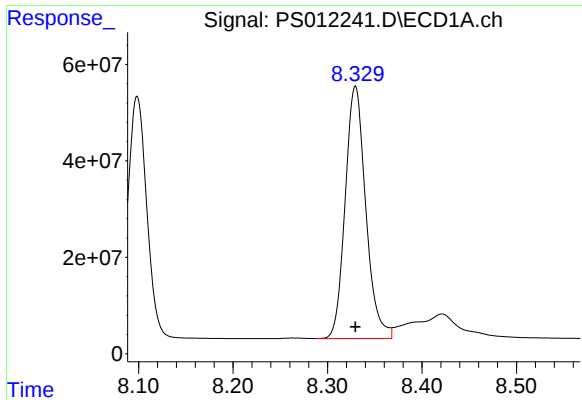

#9 2,4-D


R.T.: 8.329 min
Delta R.T.: 0.000 min
Response: 793320466
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

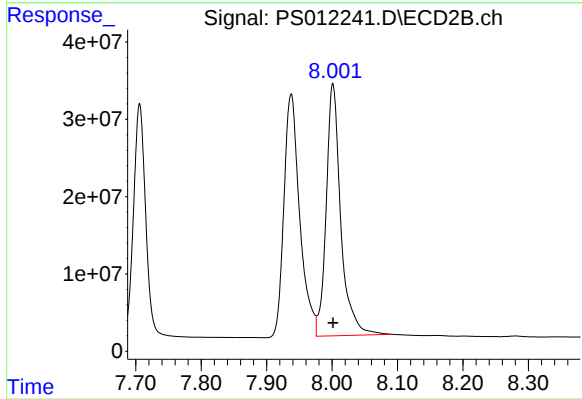


#9 2,4-D

R.T.: 8.001 min
Delta R.T.: 0.000 min
Response: 505027340
Conc: 705.00 ng/ml

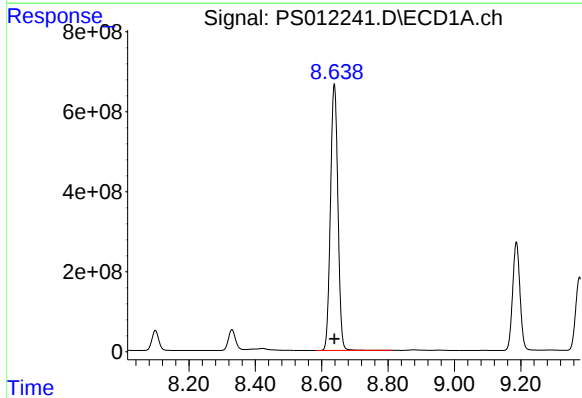


#10 Pentachlorophenol

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 10377713289
Conc: 712.50 ng/ml

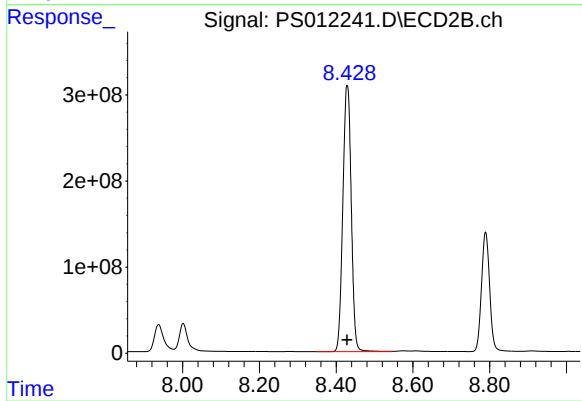

#10 Pentachlorophenol


R.T.: 8.429 min
Delta R.T.: 0.000 min
Response: 4735672755
Conc: 712.50 ng/ml

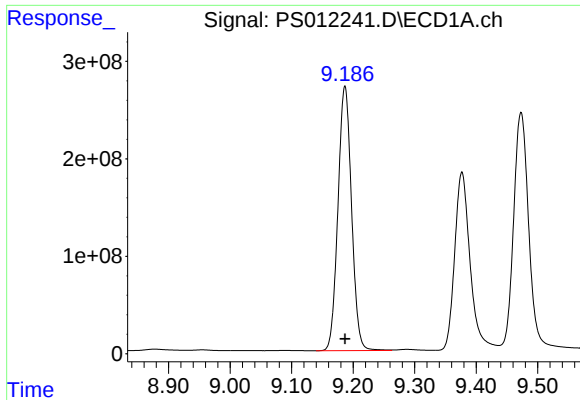

#11 2,4,5-TP (SILVEX)


R.T.: 9.187 min
Delta R.T.: 0.000 min
Response: 4160791170
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

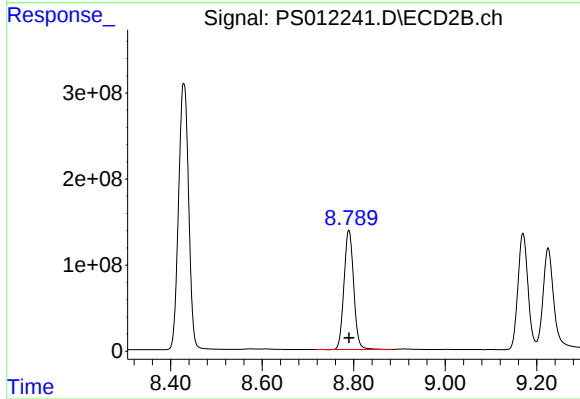


#11 2,4,5-TP (SILVEX)

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 2042614435
Conc: 712.50 ng/ml

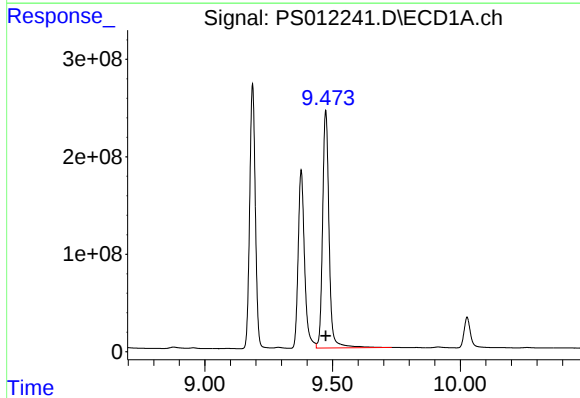


#12 2,4,5-T

R.T.: 9.473 min
Delta R.T.: 0.000 min
Response: 4308860645
Conc: 712.50 ng/ml

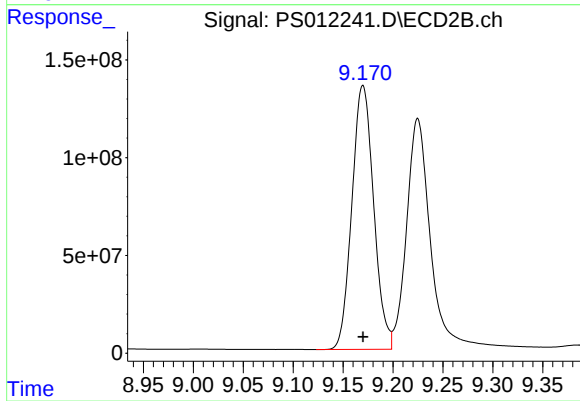

#12 2,4,5-T


R.T.: 9.170 min
Delta R.T.: 0.000 min
Response: 2048419683
Conc: 712.50 ng/ml

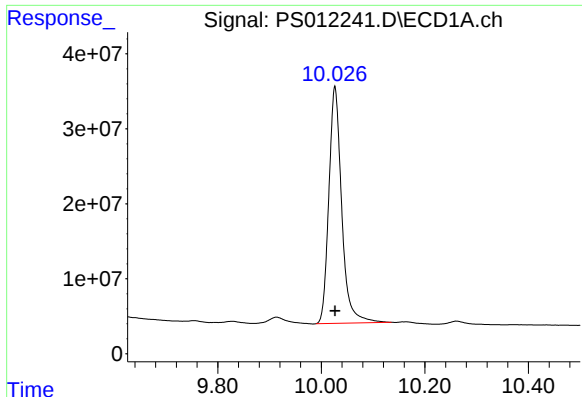

#13 2,4-DB


R.T.: 10.026 min
Delta R.T.: 0.000 min
Response: 544127288
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

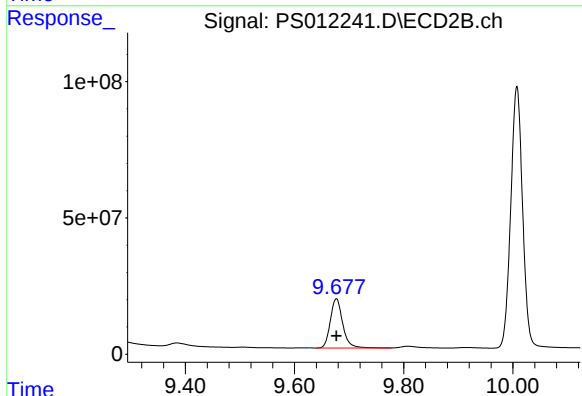


#13 2,4-DB

R.T.: 9.677 min
Delta R.T.: 0.000 min
Response: 286095658
Conc: 712.50 ng/ml

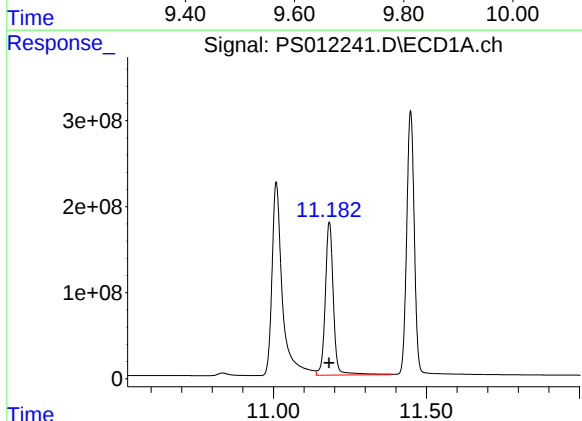


#14 DINOSEB

R.T.: 11.183 min
Delta R.T.: 0.000 min
Response: 3278261504
Conc: 705.00 ng/ml

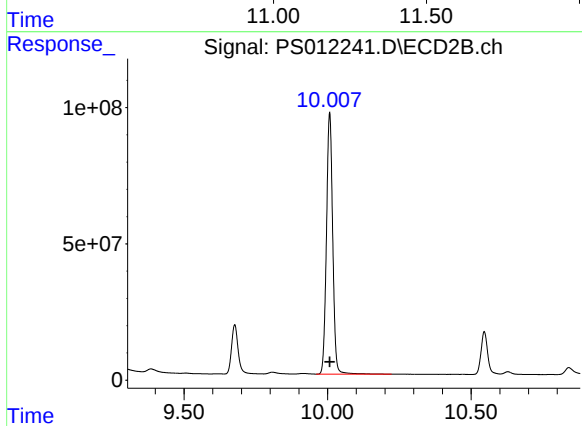

#14 DINOSEB


R.T.: 10.007 min
Delta R.T.: 0.000 min
Response: 1454536409
Conc: 705.00 ng/ml

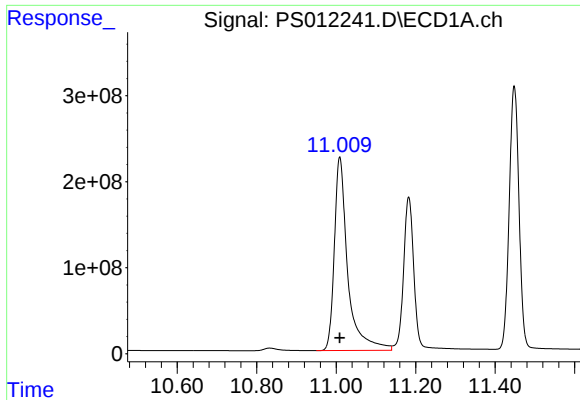

#15 Picloram


R.T.: 11.009 min
Delta R.T.: 0.000 min
Response: 5281375451
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

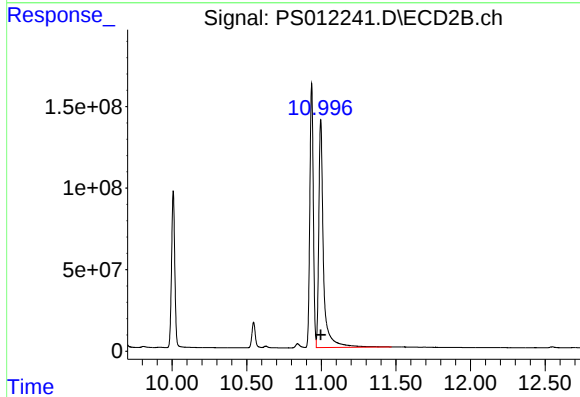


#15 Picloram

R.T.: 10.996 min
Delta R.T.: 0.000 min
Response: 3082039714
Conc: 712.50 ng/ml

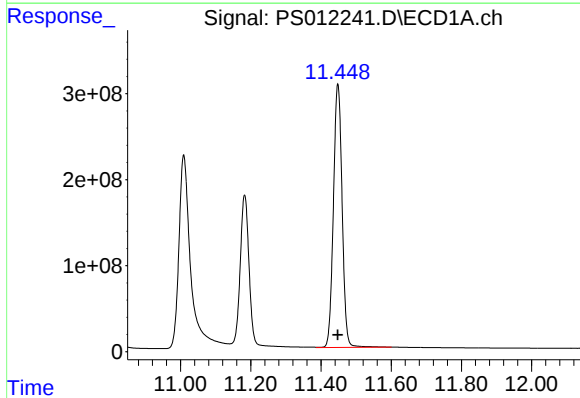

#16 DCPA

R.T.: 11.448 min
Delta R.T.: 0.000 min
Response: 5278936118
Conc: 720.00 ng/ml

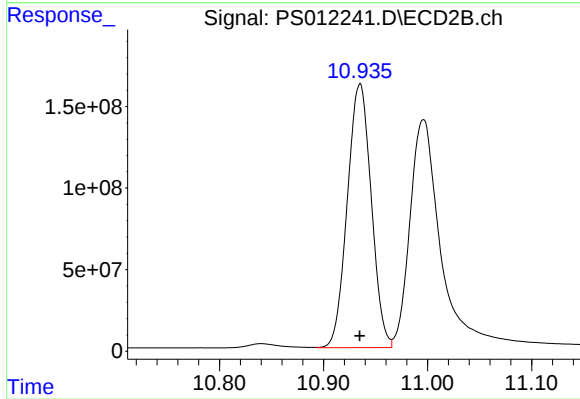

#16 DCPA

R.T.: 10.935 min
Delta R.T.: 0.000 min
Response: 2587862729
Conc: 720.00 ng/ml