

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091422\
 Data File : PS020531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 10:12
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:10:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	3.047f	0.000	1618848	0	<MDL	N.D.	#
2) T	3,5-DICHL...	6.460f	0.000	1551448	0	<MDL	N.D.	#
5) T	DICAMBA	7.380	6.942	2746715	24425768	<MDL	6.345	#
6) T	MCP	7.463f	6.976	856097	19847264	<MDL	6.873	#
7) T	MCPA	7.660	0.000	349880	0	<MDL	N.D.	#
9) T	2,4-D	8.304	0.000	150.4E6	0	32.351	N.D.	#
10) T	Pentachlo...	8.604	8.257	4594199	1055128	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.167	0.000	7664186	0	<MDL	N.D.	#
12) T	2,4,5-T	9.438	0.000	51688931	0	2.334	N.D.	#
14) T	DINOSEB	11.061f	0.000	293.4E6	0	15.976	N.D.	#
15) T	Picloram	0.000	10.872f	0	55420328	N.D.	6.882	#
16) T	DCPA	11.400	10.744	13534202	5959741	<MDL	<MDL	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091422\
Data File : PS020531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 10:12
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:10:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

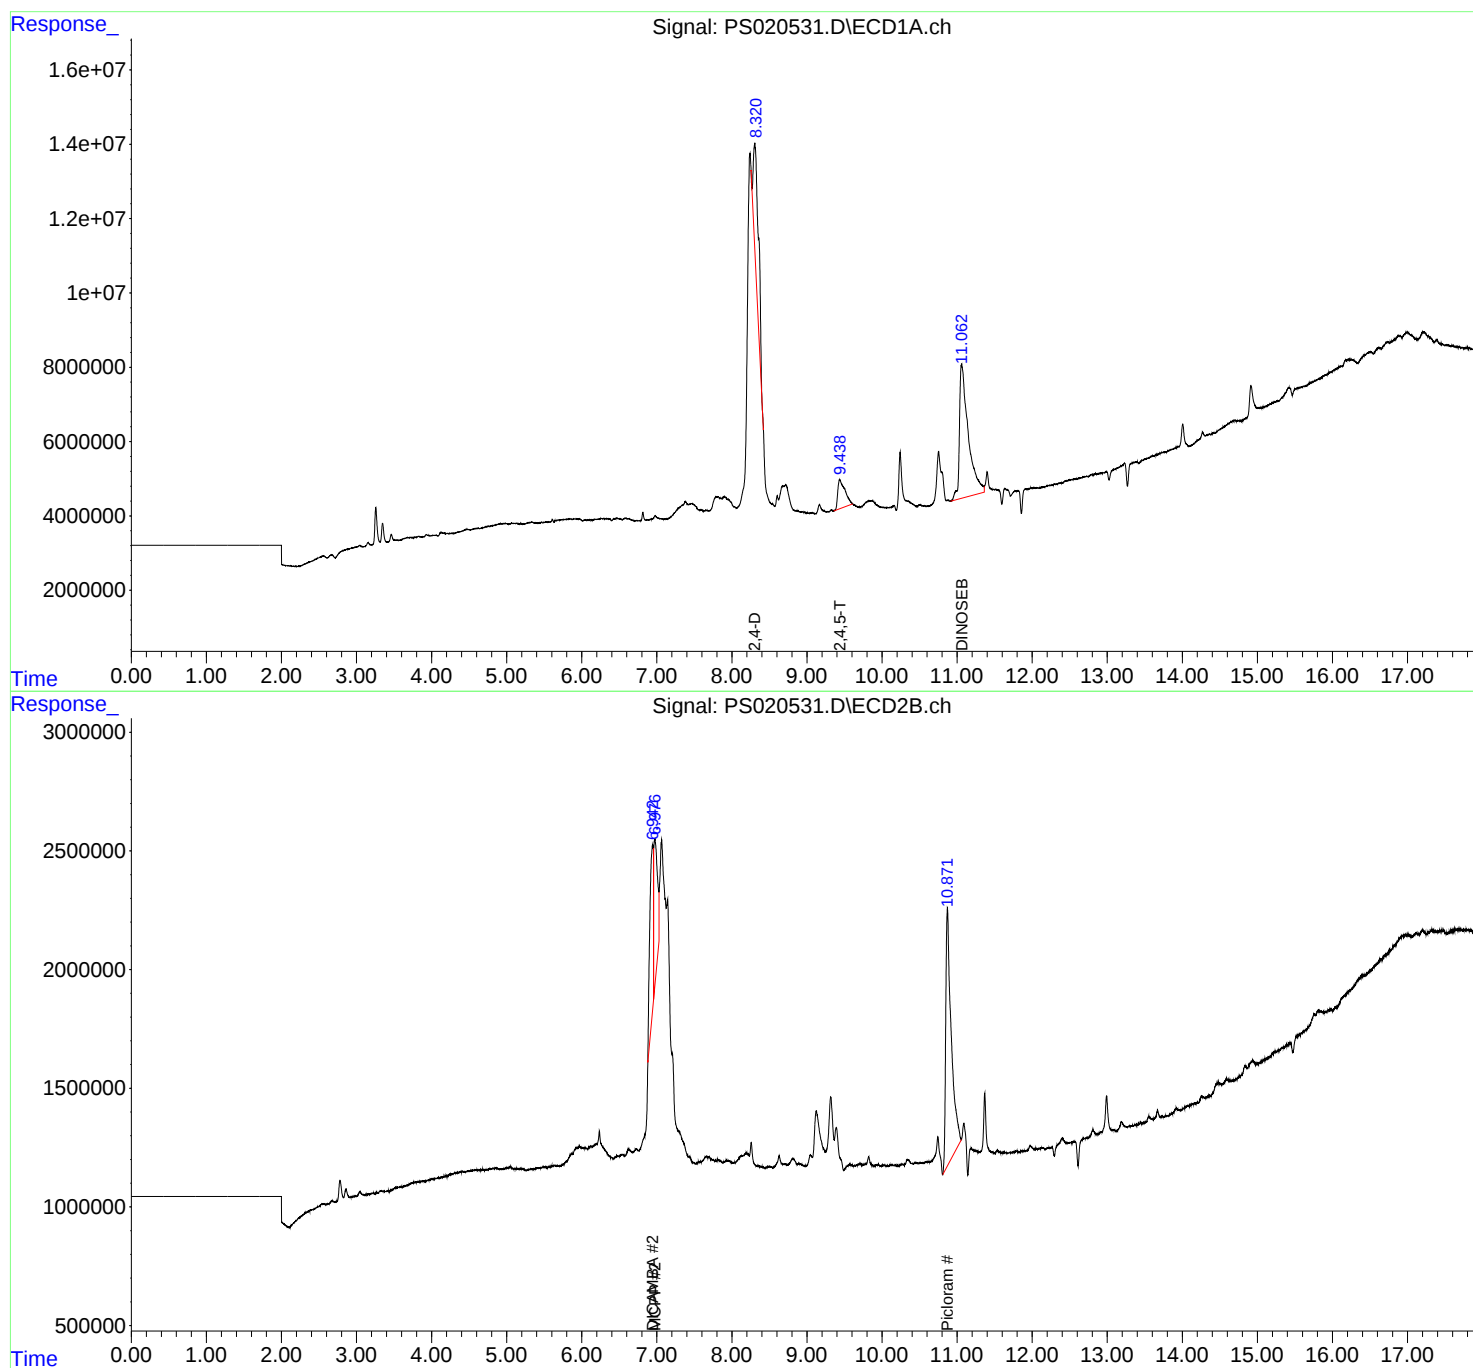


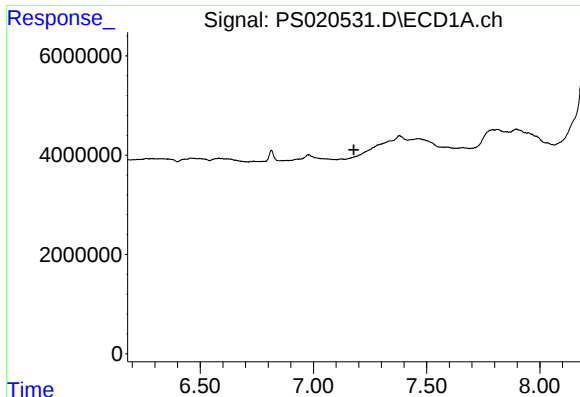

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

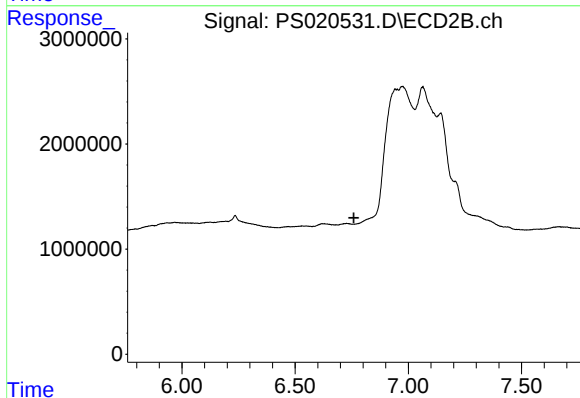


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.760 min
Response: 0
Conc: N.D.

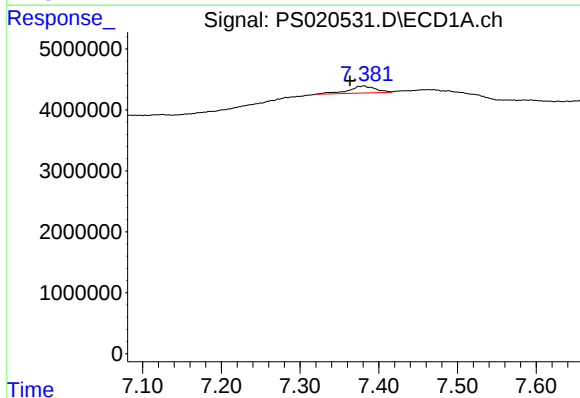


#5 DICAMBA

R.T.: 7.380 min
Delta R.T.: 0.016 min
Response: 2746715
Conc: N.D.

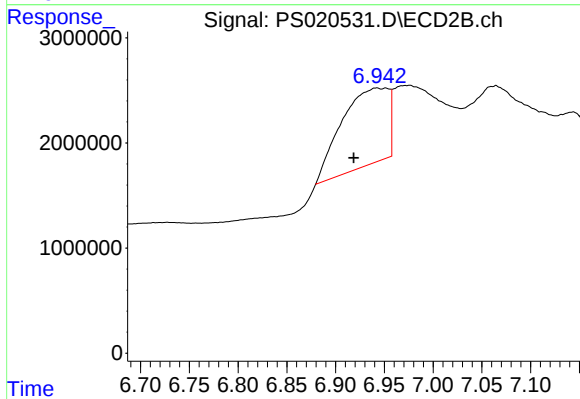

#5 DICAMBA


R.T.: 6.942 min
Delta R.T.: 0.023 min
Response: 24425768
Conc: 6.34 ng/ml

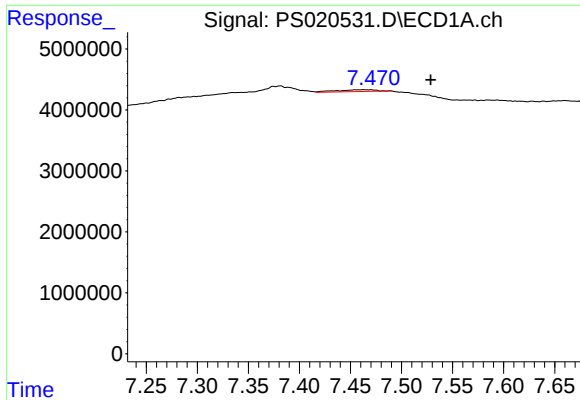

#6 MCPP


R.T.: 7.463 min
Delta R.T.: -0.066 min
Response: 856097
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

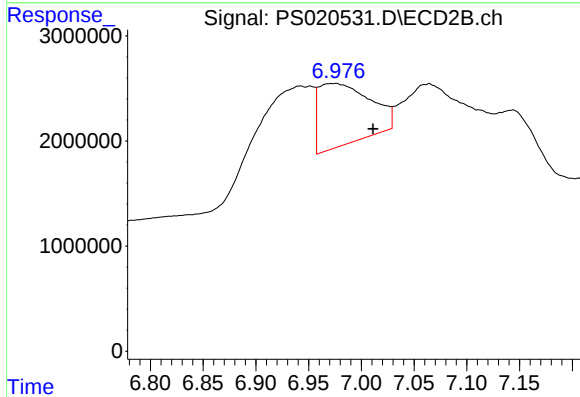


#6 MCPP

R.T.: 6.976 min
Delta R.T.: -0.035 min
Response: 19847264
Conc: 6.87 ug/ml

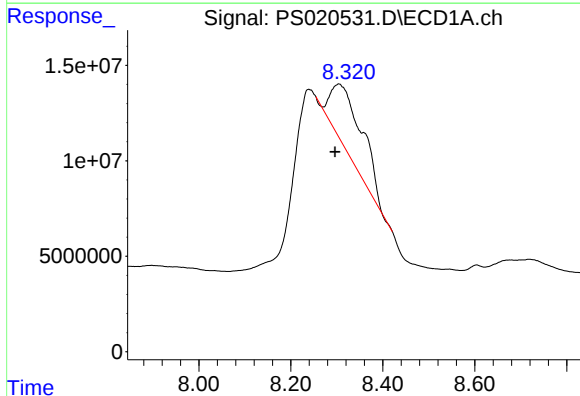


#9 2,4-D

R.T.: 8.304 min
Delta R.T.: 0.008 min
Response: 150372099
Conc: 32.35 ng/ml

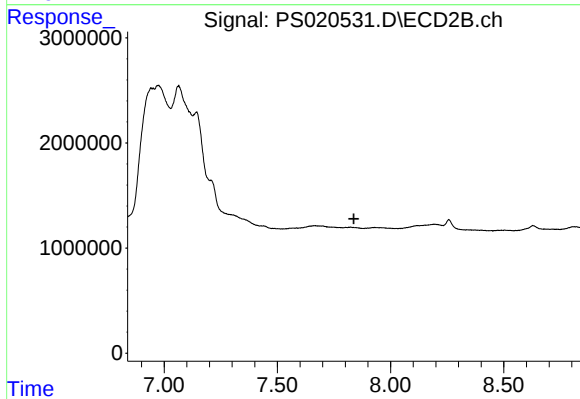

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

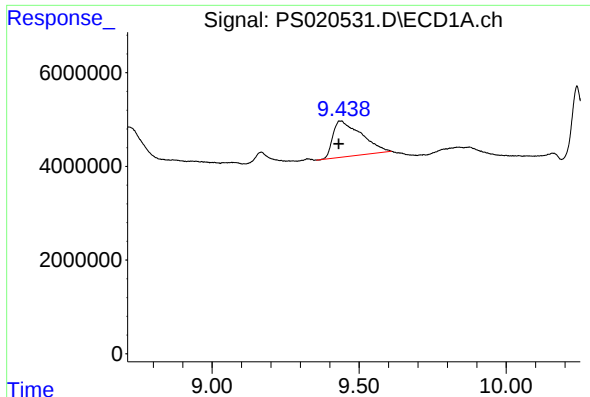

#12 2,4,5-T


R.T.: 9.438 min
Delta R.T.: 0.008 min
Response: 51688931
Conc: 2.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

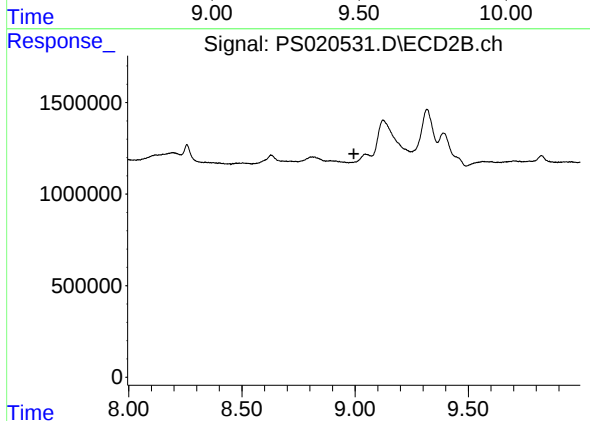


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.995 min
Response: 0
Conc: N.D.

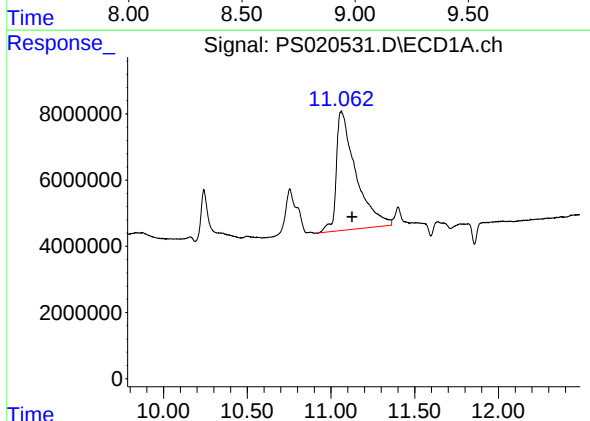


#14 DINOSEB

R.T.: 11.061 min
Delta R.T.: -0.064 min
Response: 293399017
Conc: 15.98 ng/ml

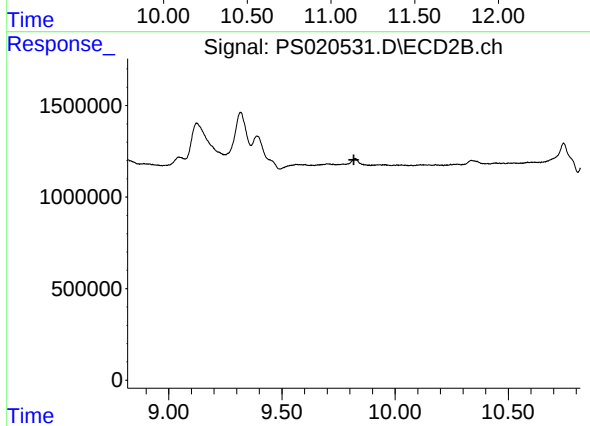

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

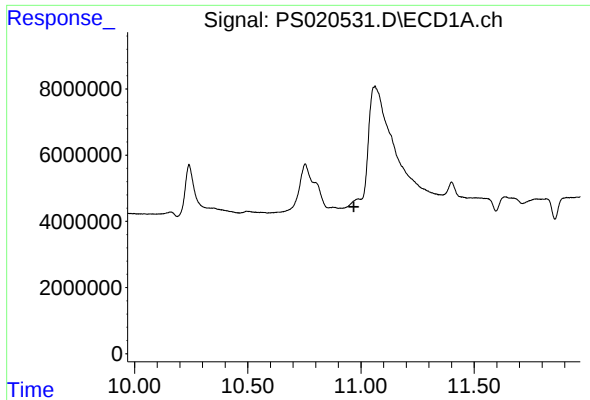

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.968 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

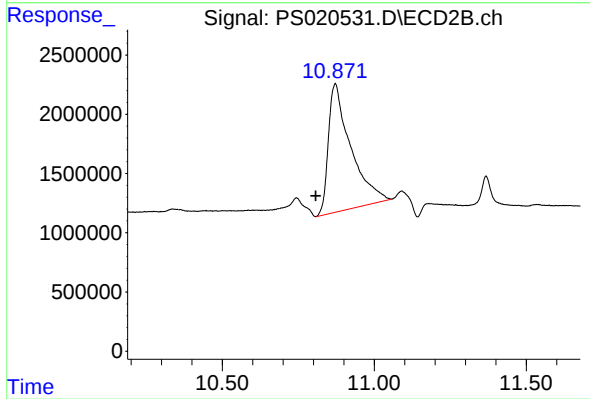

#15 Picloram

R.T.: 10.872 min
Delta R.T.: 0.064 min
Response: 55420328
Conc: 6.88 ng/ml