

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091422\
 Data File : PS020532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2022 10:36
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 04:11:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.761	1580.1E6	443.5E6	459.135	520.675
Target Compounds							
1) T	Dalapon	3.049f	0.000	1583809	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.457f	0.000	7268746	0	1.458	N.D. #
3) T	4-Nitroph...	6.991	0.000	-460822	0	126.863	N.D. #
7) T	MCPA	7.655	7.196	1833197	11355055	<MDL	2.630 #
9) T	2,4-D	8.358f	0.000	93162916	0	20.043	N.D. #
10) T	Pentachlo...	8.601	0.000	1528835	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.173	0.000	5595337	0	<MDL	N.D. #
12) T	2,4,5-T	9.459	0.000	28294069	0	1.278	N.D. #
13) T	2,4-DB	9.947	0.000	583191	0	<MDL	N.D. #
14) T	DINOSEB	11.076f	0.000	189.8E6	0	10.335	N.D. #
15) T	Picloram	10.968	10.746f	61654291	2016211	2.049	<MDL #
16) T	DCPA	11.398	10.746	10646021	2016211	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091422\
Data File : PS020532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2022 10:36
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 04:11:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

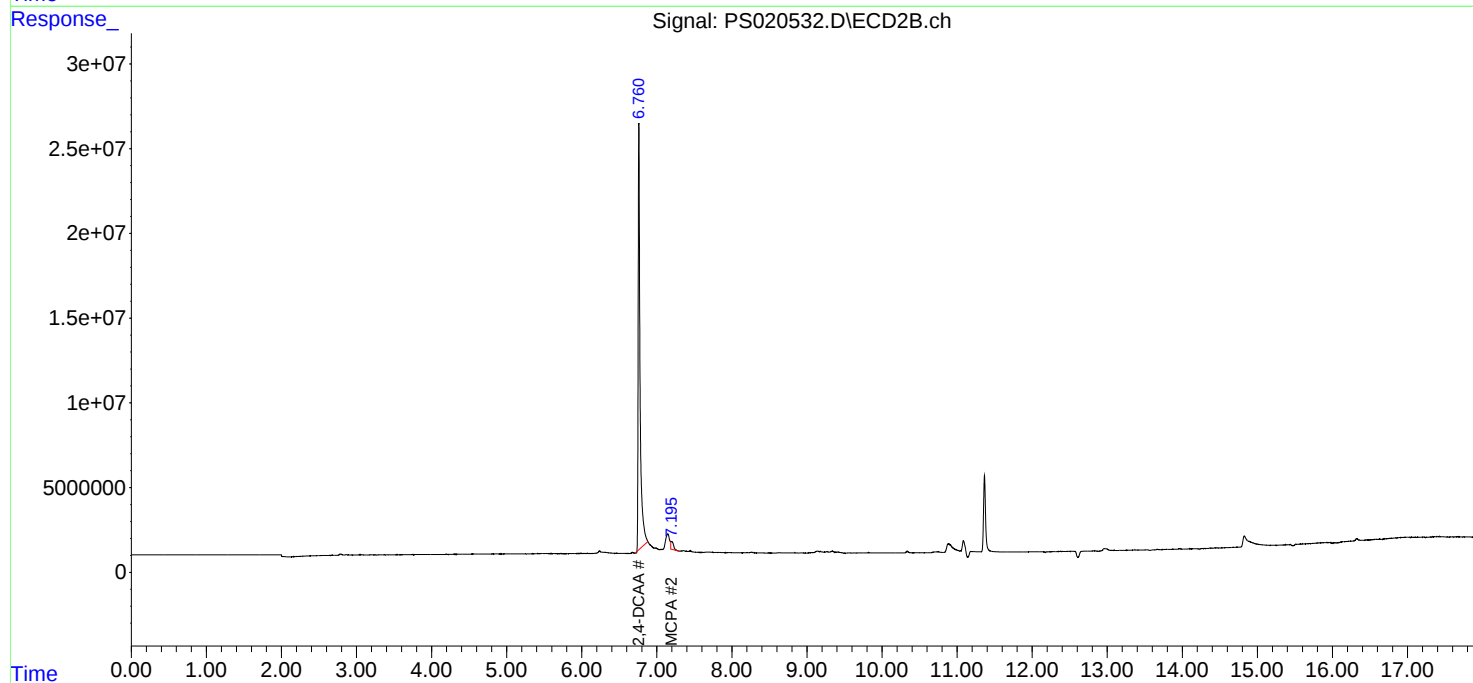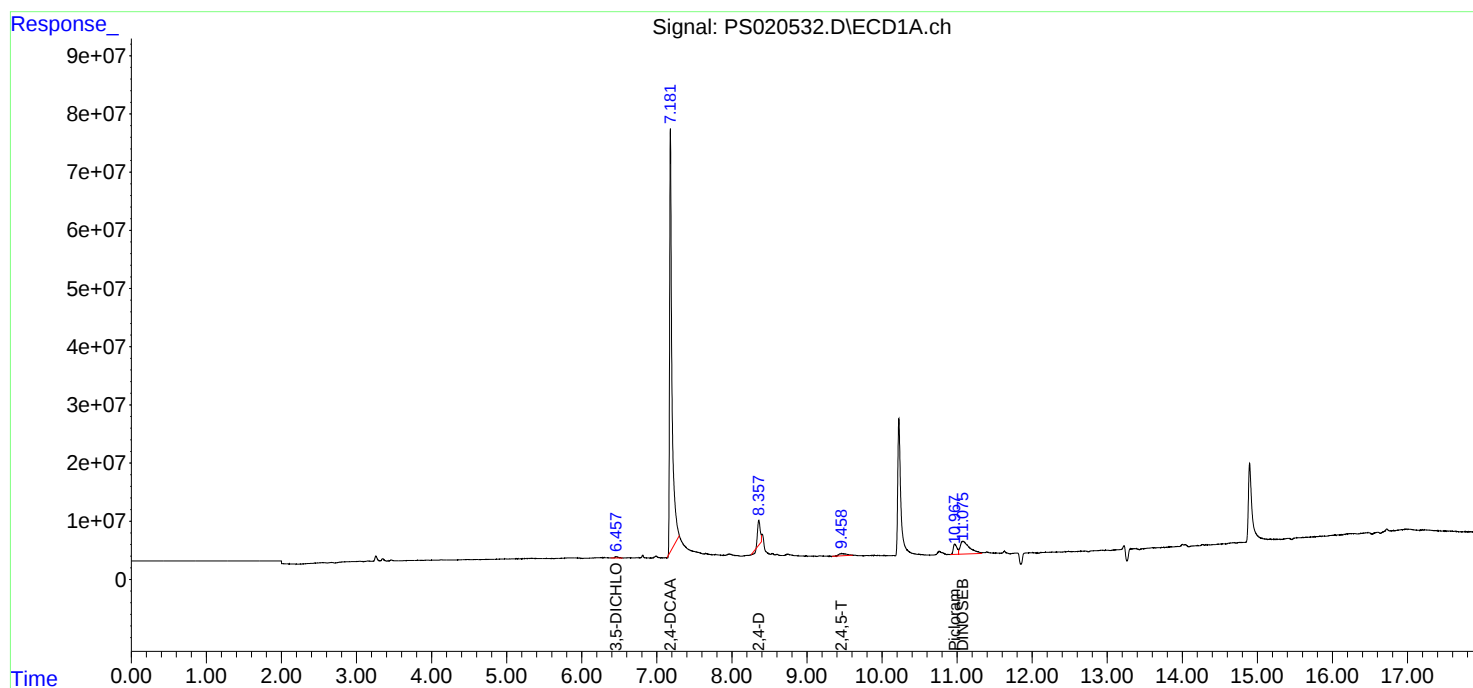


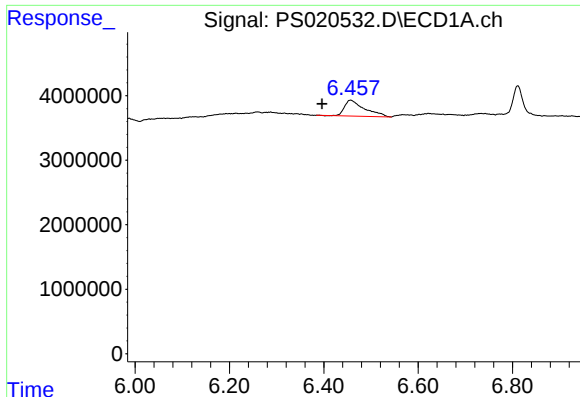

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.457 min
Delta R.T.: 0.061 min
Response: 7268746
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

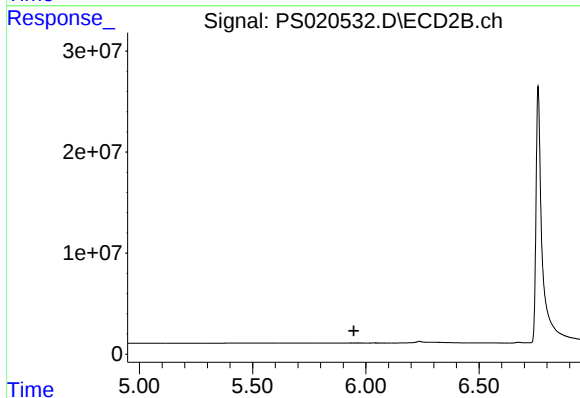


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

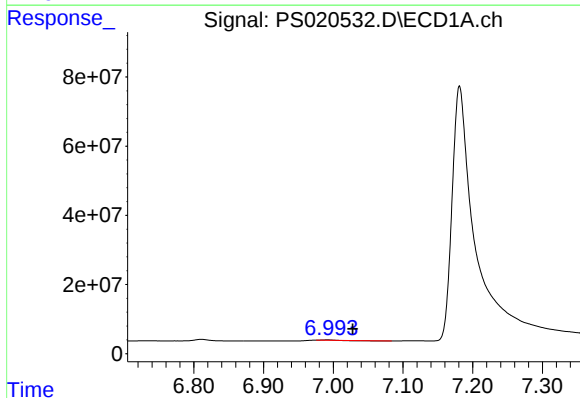


#3 4-Nitrophenol

R.T.: 6.991 min
Delta R.T.: -0.037 min
Response: -460822
Conc: 126.86 ng/ml

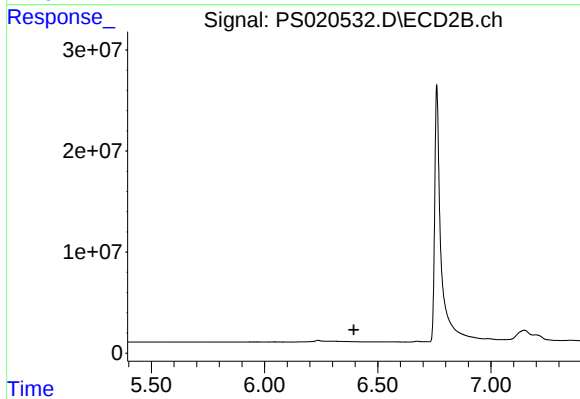

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

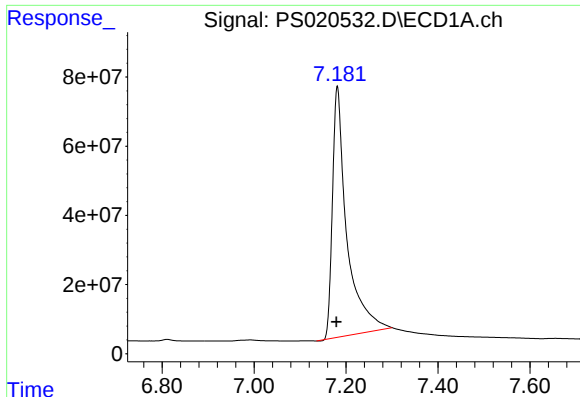

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: 0.002 min
Response: 1580108076
Conc: 459.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

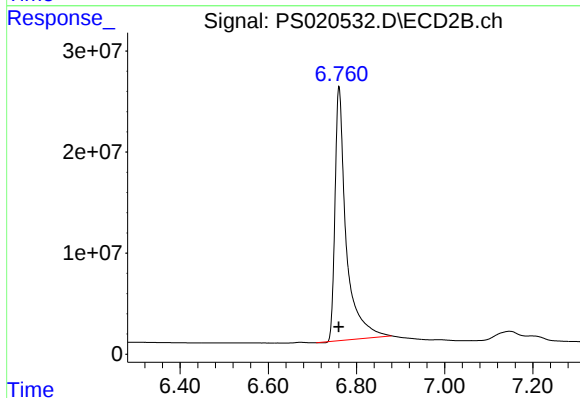


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 443456316
Conc: 520.67 ng/ml

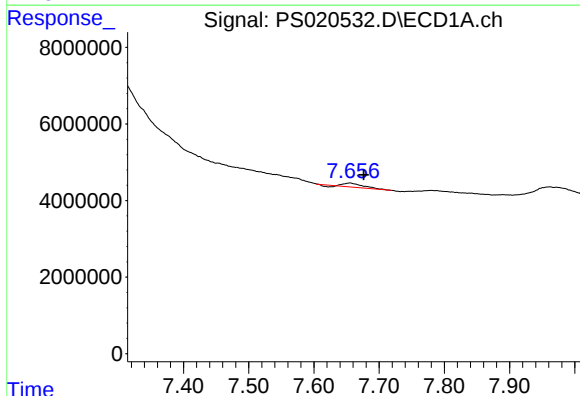


#7 MCPA

R.T.: 7.655 min
Delta R.T.: -0.021 min
Response: 1833197
Conc: N.D.

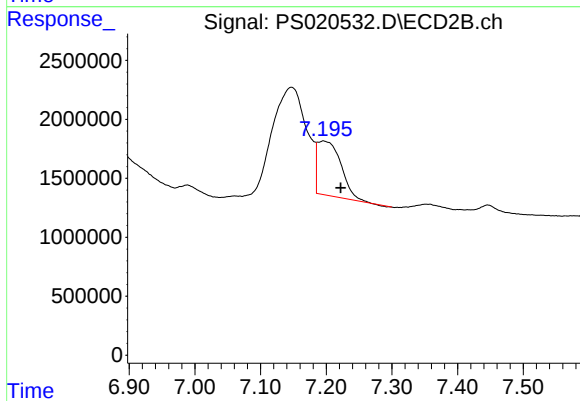

#7 MCPA


R.T.: 7.196 min
Delta R.T.: -0.026 min
Response: 11355055
Conc: 2.63 ug/ml

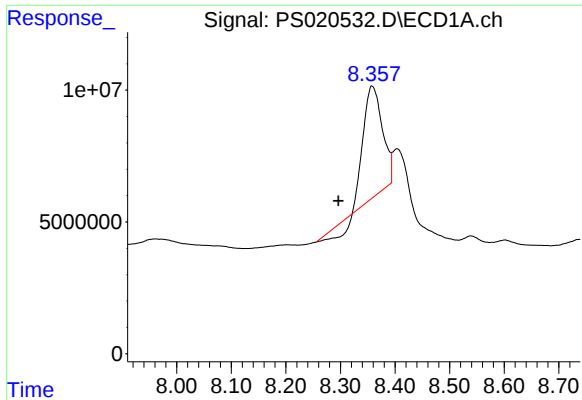

#9 2,4-D


R.T.: 8.358 min
Delta R.T.: 0.062 min
Response: 93162916
Conc: 20.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

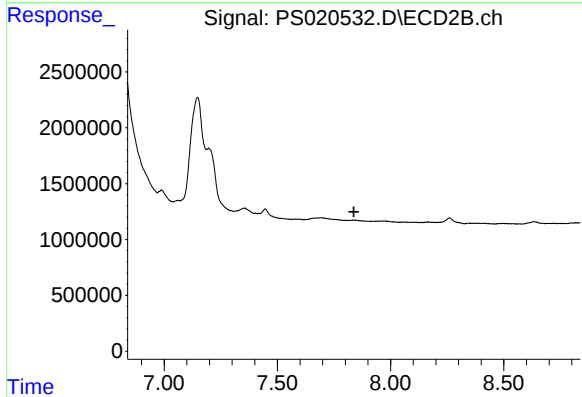


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

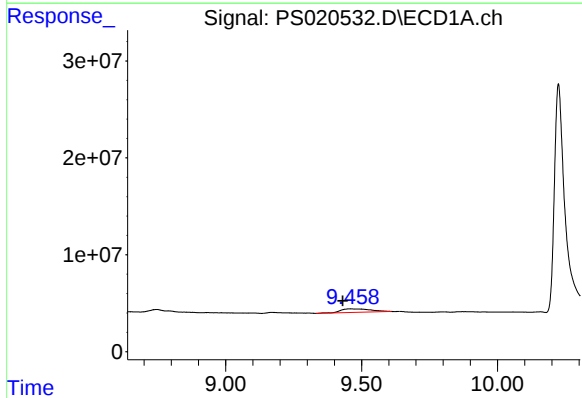


#12 2,4,5-T

R.T.: 9.459 min
Delta R.T.: 0.028 min
Response: 28294069
Conc: 1.28 ng/ml

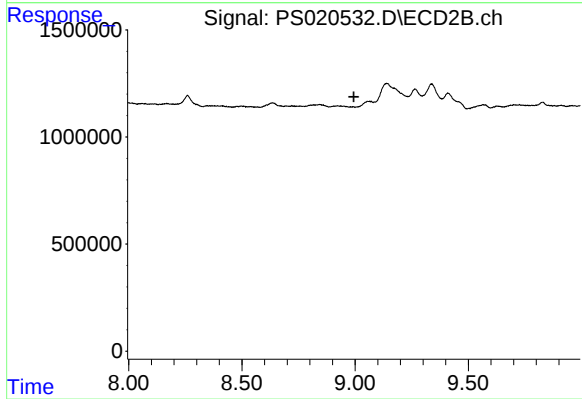

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.995 min
Response: 0
Conc: N.D.

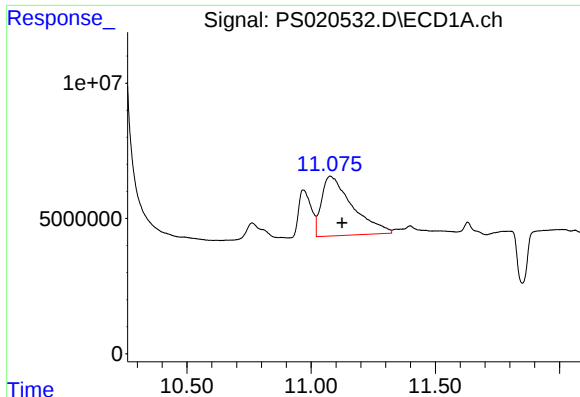

#14 DINOSEB


R.T.: 11.076 min
Delta R.T.: -0.049 min
Response: 189801399
Conc: 10.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

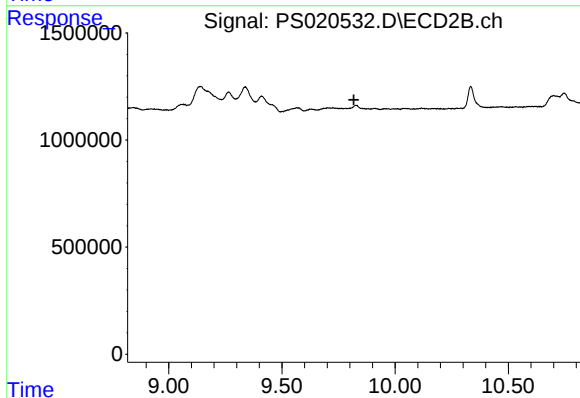


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

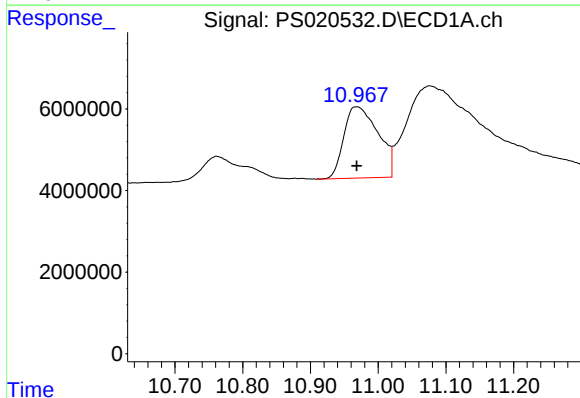

#15 Picloram

R.T.: 10.968 min
Delta R.T.: 0.000 min
Response: 61654291
Conc: 2.05 ng/ml

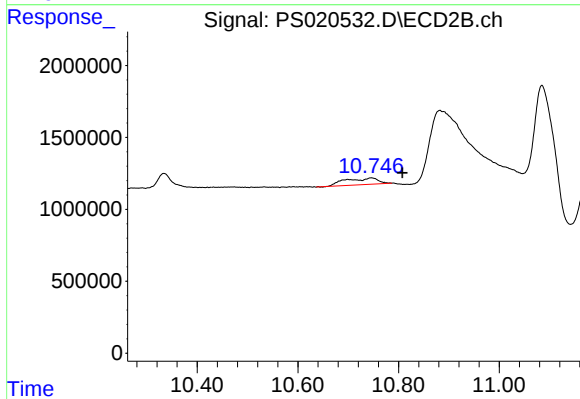

#15 Picloram

R.T.: 10.746 min
Delta R.T.: -0.062 min
Response: 2016211
Conc: N.D.