

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091423\
 Data File : PS024301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2023 09:06
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 01:59:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.353	0.000	2605449	0	1.308	N.D. #
Target Compounds							
1) T	Dalapon	2.517	2.573	6557686	4600137	3.017	4.362 #
3) T	4-Nitroph...	6.198	0.000	7300294	0	5.876	N.D. #
5) T	DICAMBA	6.493	6.995	766353	32867813	<MDL	11.412 #
6) T	MCP	6.683	6.995f	4017443	32867813	<MDL	17.157 #
7) T	MCPA	6.849f	0.000	1294725	0	<MDL	N.D. #
8) T	DICHLORPROP	7.082	7.578	93298	2420603	<MDL	3.332 #
9) T	2,4-D	7.253	7.795f	333.1E6	802156	125.228	<MDL #
10) T	Pentachlo...	7.555	0.000	694508	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.053	8.631	709896	1102768	<MDL	<MDL #
12) T	2,4,5-T	8.300	9.049	822237	1326146	<MDL	<MDL #
13) T	2,4-DB	8.746f	9.498	1655636	720035	<MDL	1.567 #
14) T	DINOSEB	9.848	0.000	370309	0	<MDL	N.D. #
15) T	Picloram	9.658	10.793	134.9E6	20339582	8.258	3.425 #
16) T	DCPA	10.175f	10.793	-4206834	20339582	N.D.	3.965



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091423\
Data File : PS024301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2023 09:06
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 01:59:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

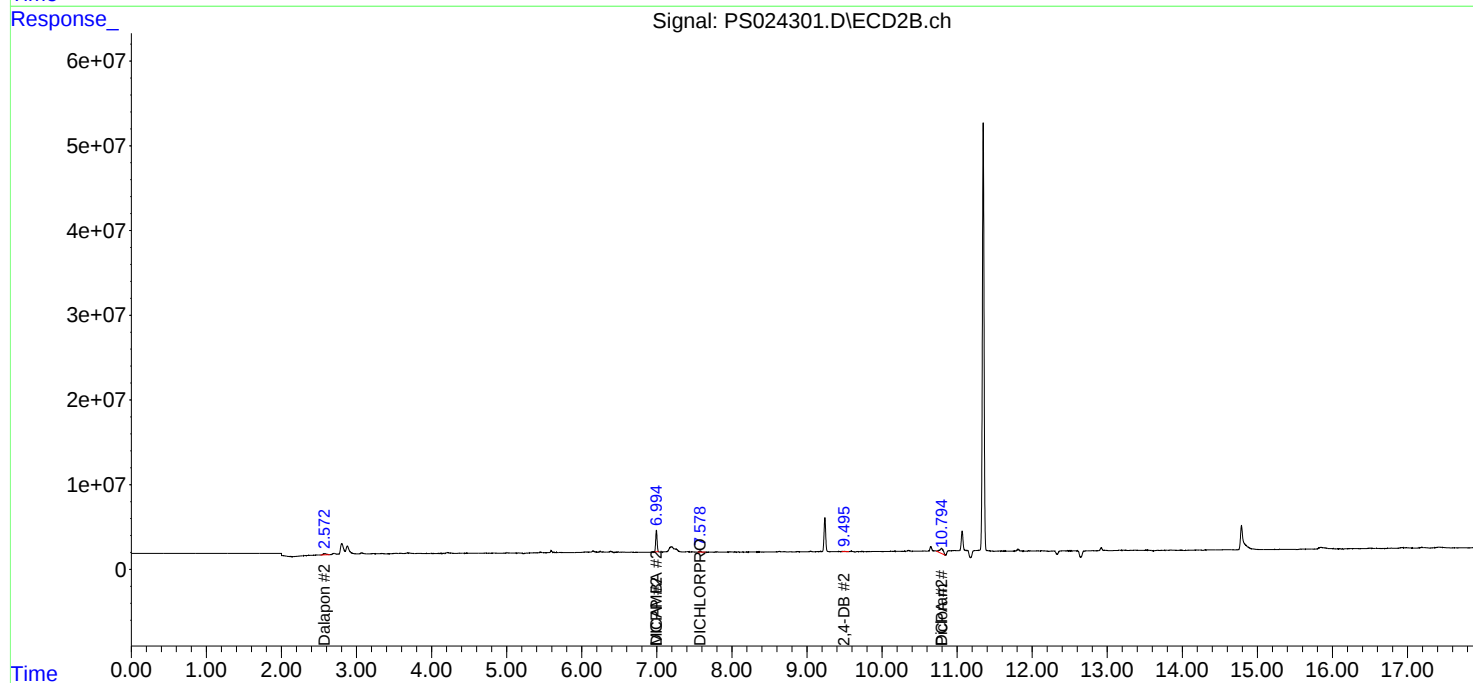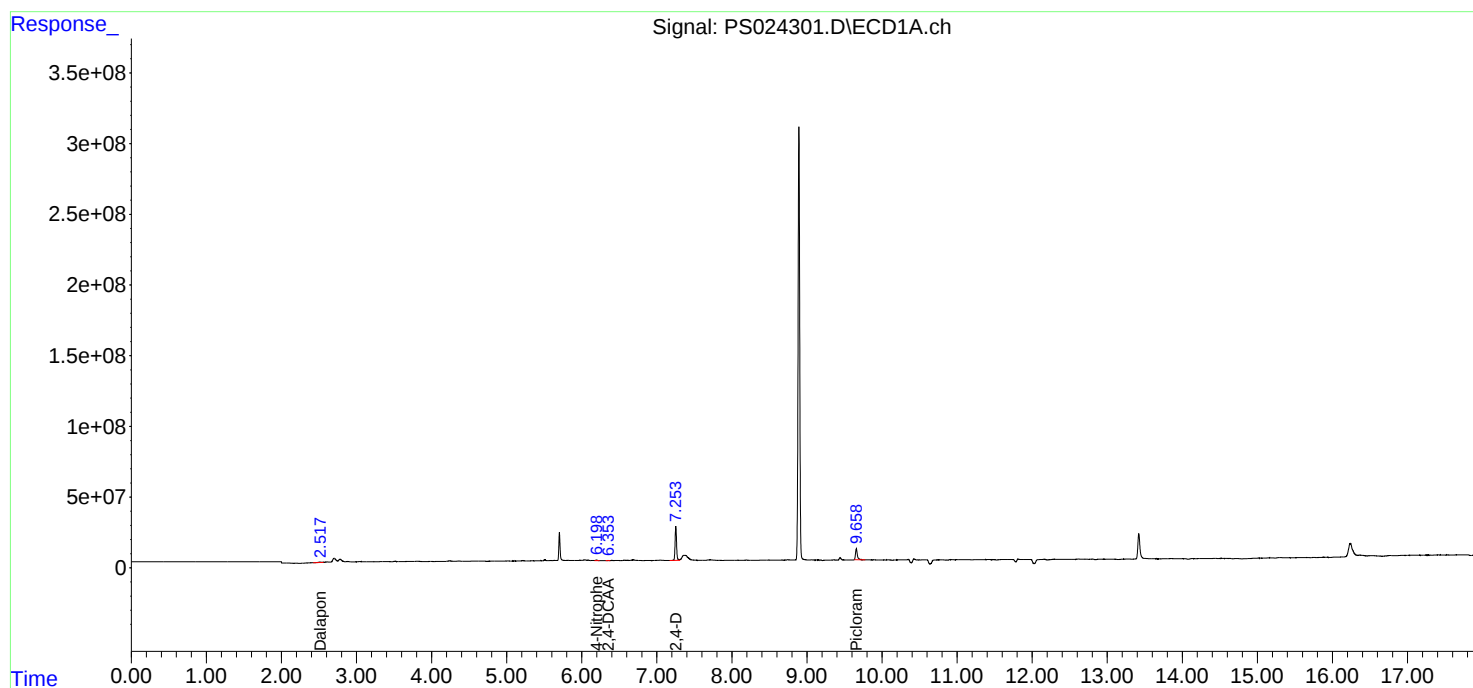


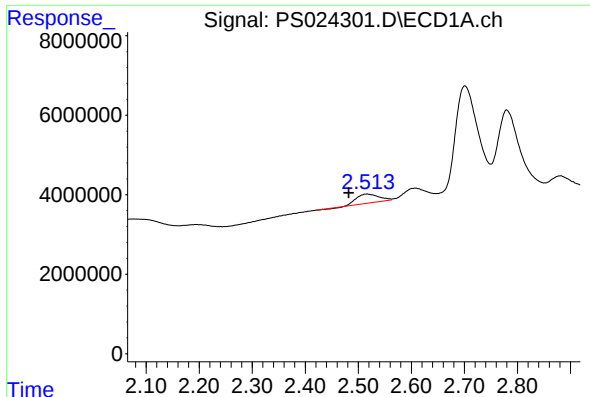

#1 Dalapon


R.T.: 2.517 min
Delta R.T.: 0.035 min
Response: 6557686
Conc: 3.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

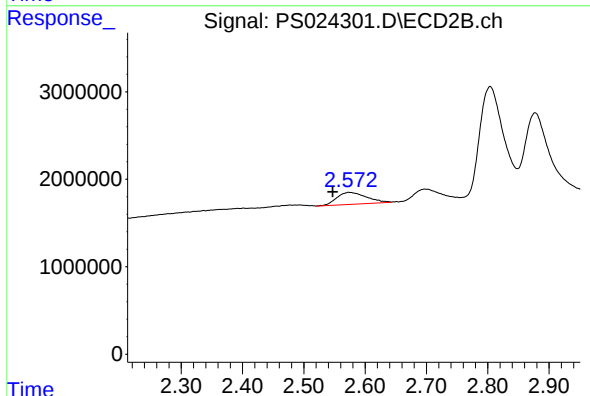


#1 Dalapon

R.T.: 2.573 min
Delta R.T.: 0.026 min
Response: 4600137
Conc: 4.36 ng/ml

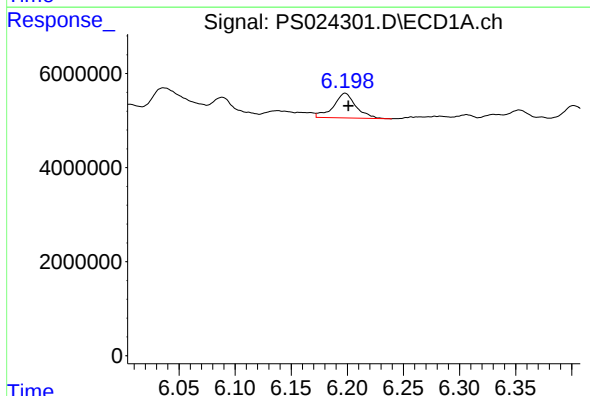


#3 4-Nitrophenol

R.T.: 6.198 min
Delta R.T.: -0.003 min
Response: 7300294
Conc: 5.88 ng/ml

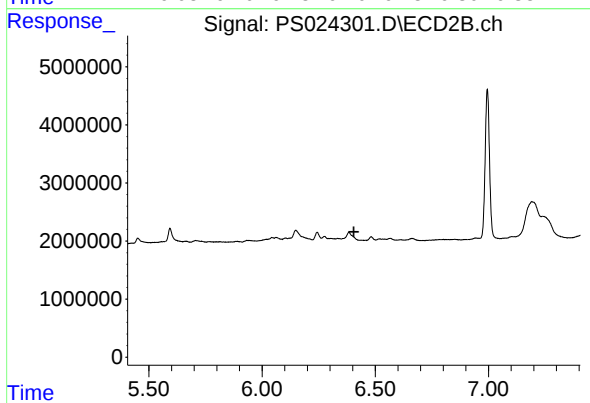

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.405 min
Response: 0
Conc: N.D.

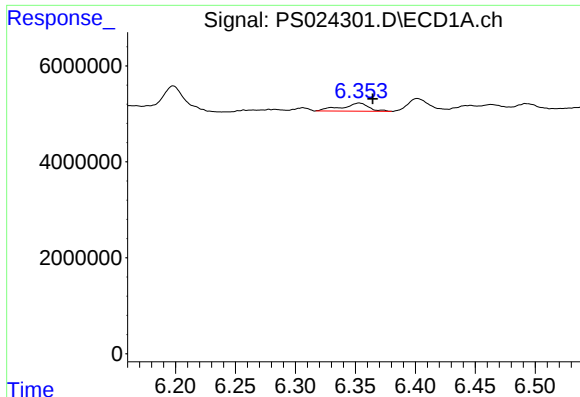

#4 2,4-DCAA


R.T.: 6.353 min
Delta R.T.: -0.011 min
Response: 2605449
Conc: 1.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

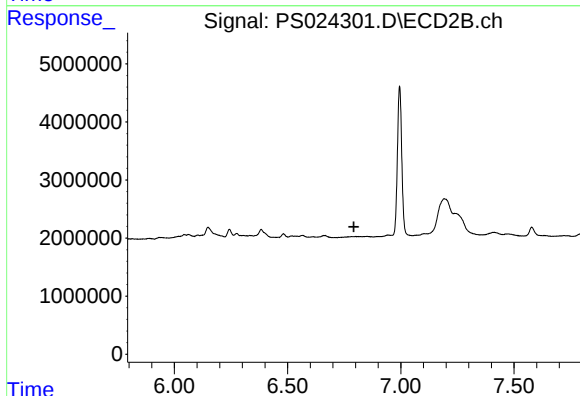


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.793 min
Response: 0
Conc: N.D.

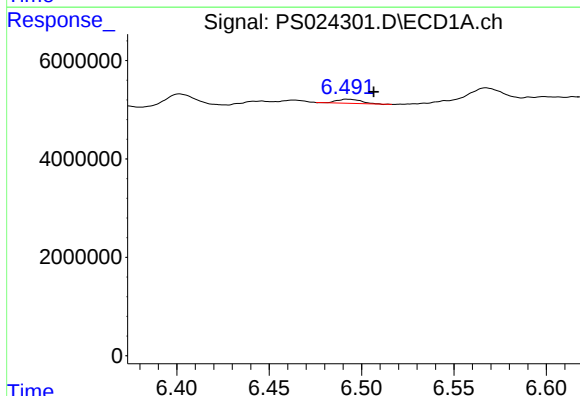


#5 DICAMBA

R.T.: 6.493 min
Delta R.T.: -0.014 min
Response: 766353
Conc: N.D.

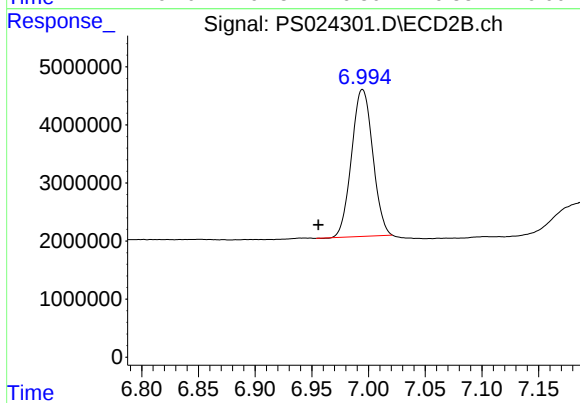

#5 DICAMBA


R.T.: 6.995 min
Delta R.T.: 0.039 min
Response: 32867813
Conc: 11.41 ng/ml

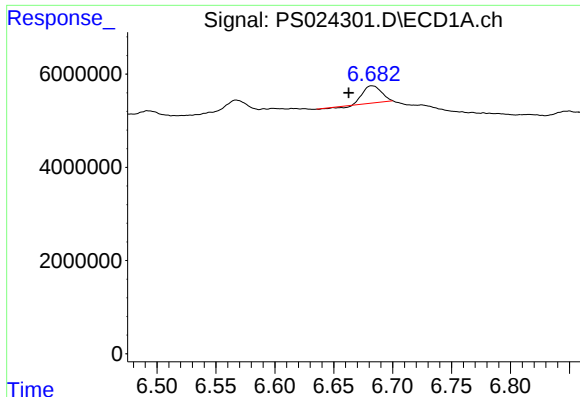

#6 MCP


R.T.: 6.683 min
Delta R.T.: 0.020 min
Response: 4017443
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

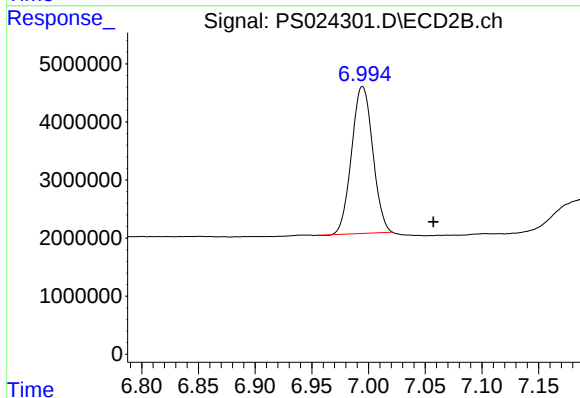


#6 MCP

R.T.: 6.995 min
Delta R.T.: -0.063 min
Response: 32867813
Conc: 17.16 ug/ml

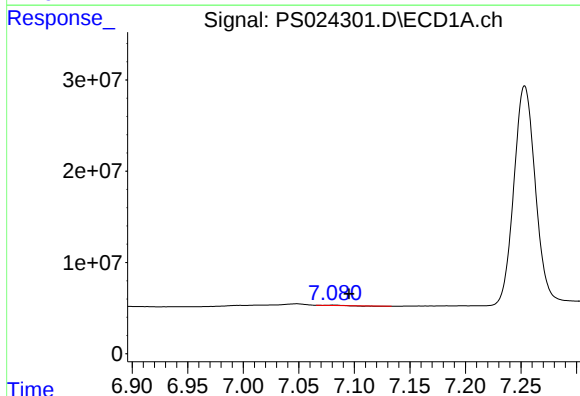


#8 DICHLORPROP

R.T.: 7.082 min
Delta R.T.: -0.014 min
Response: 93298
Conc: N.D.

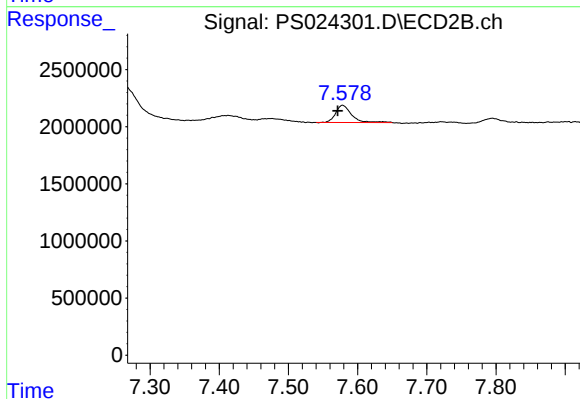

#8 DICHLORPROP


R.T.: 7.578 min
Delta R.T.: 0.007 min
Response: 2420603
Conc: 3.33 ng/ml

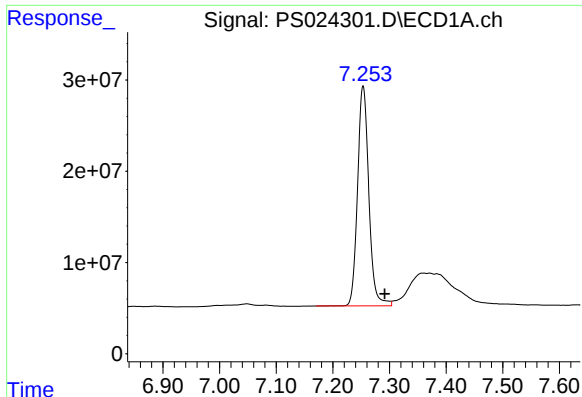

#9 2,4-D


R.T.: 7.253 min
Delta R.T.: -0.038 min
Response: 333091551
Conc: 125.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

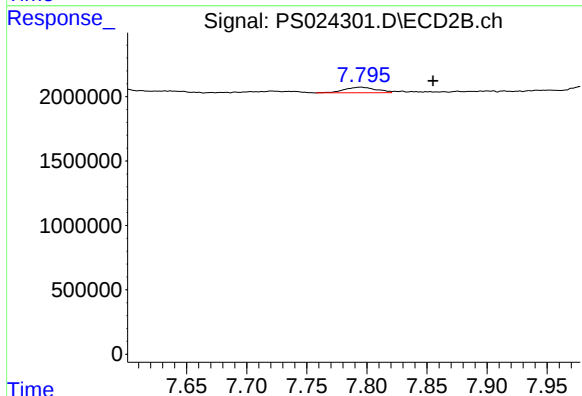


#9 2,4-D

R.T.: 7.795 min
Delta R.T.: -0.060 min
Response: 802156
Conc: N.D.

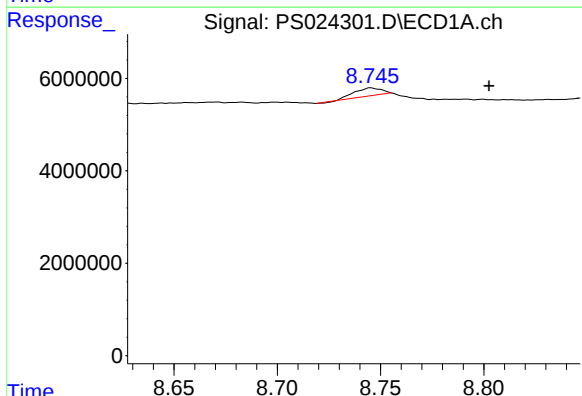


#13 2,4-DB

R.T.: 8.746 min
Delta R.T.: -0.057 min
Response: 1655636
Conc: N.D.

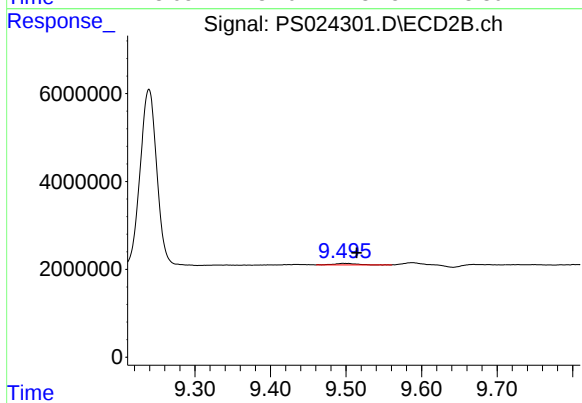

#13 2,4-DB


R.T.: 9.498 min
Delta R.T.: -0.016 min
Response: 720035
Conc: 1.57 ng/ml

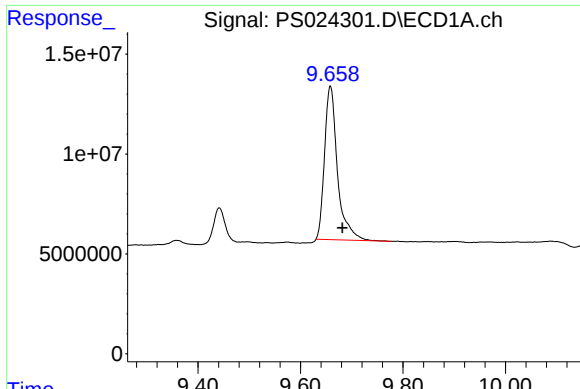

#15 Picloram


R.T.: 9.658 min
Delta R.T.: -0.023 min
Response: 134855068
Conc: 8.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

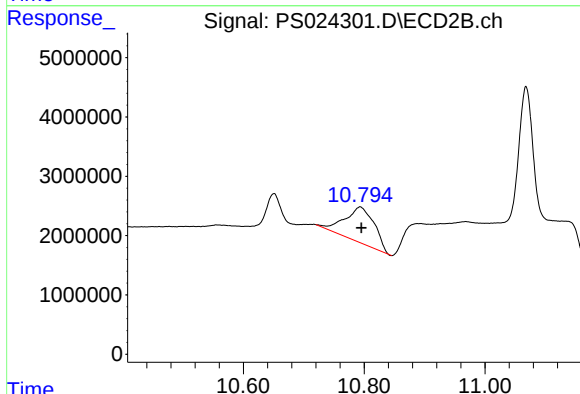


#15 Picloram

R.T.: 10.793 min
Delta R.T.: -0.003 min
Response: 20339582
Conc: 3.42 ng/ml

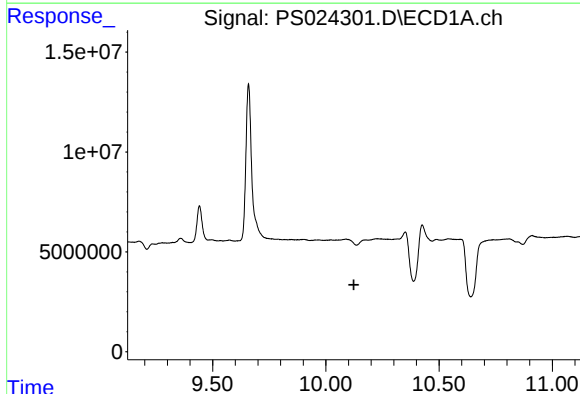

#16 DCPA

R.T.: 10.175 min
Delta R.T.: 0.051 min
Response: -4206834
Conc: N.D.

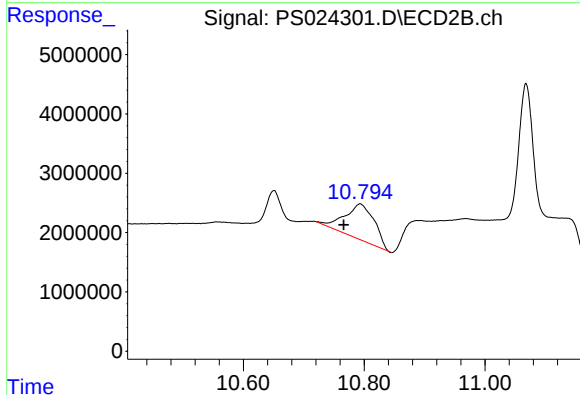

#16 DCPA

R.T.: 10.793 min
Delta R.T.: 0.027 min
Response: 20339582
Conc: 3.96 ng/ml