

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091423\
 Data File : PS024316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2023 00:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 02:12:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 28 16:48:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.362	6.789	1041.1E6	353.6E6	522.569	526.504
Target Compounds							
1) T	Dalapon	2.515	2.578	4635024	2959623	2.133	2.807 #
3) T	4-Nitroph...	6.200	0.000	15239881	0	12.267	N.D. #
5) T	DICAMBA	6.492	6.995	930451	23038846	<MDL	7.999 #
6) T	MCP	6.683	7.104f	13789948	243590	2.214	<MDL #
7) T	MCPA	6.814	0.000	82373	0	<MDL	N.D. #
8) T	DICHLORPROP	7.081	7.578	269927	10332907	<MDL	14.221 #
9) T	2,4-D	7.253	7.794f	207.2E6	2071331	77.914	2.325 #
10) T	Pentachlo...	7.529	8.269	3404997	806508	<MDL	<MDL #
11) T	2,4,5-TP ...	8.083	8.630	4696100	1242917	<MDL	<MDL #
12) T	2,4,5-T	8.300	9.046	1275520	1075036	<MDL	<MDL #
13) T	2,4-DB	8.746f	9.498	1977353	1218520	<MDL	2.651 #
14) T	DINOSEB	9.858	0.000	806612	0	<MDL	N.D. #
15) T	Picloram	9.657	10.792	193.2E6	21148835	11.830	3.561 #
16) T	DCPA	10.166f	10.792	-1886054	21148835	N.D.	4.123



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091423\
Data File : PS024316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 00:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 02:12:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082823.M
Quant Title : 8080.M
QLast Update : Mon Aug 28 16:48:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

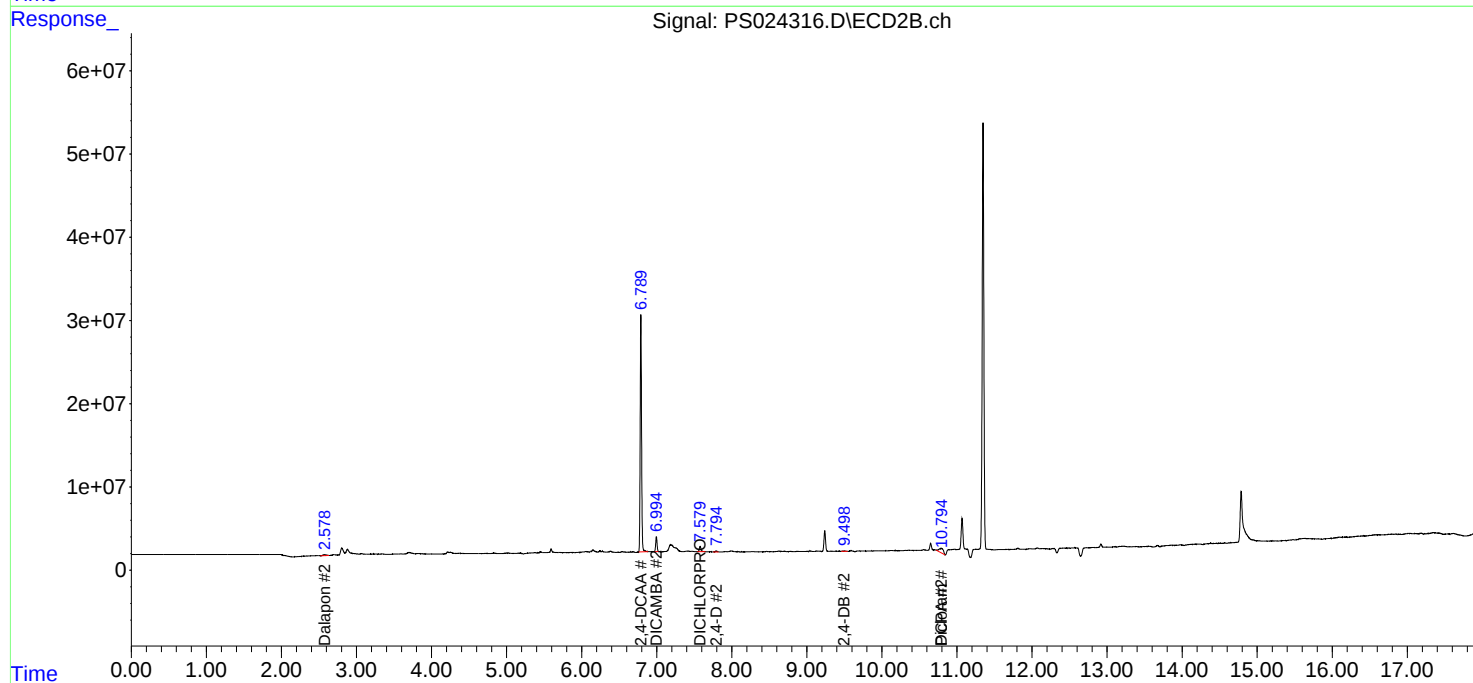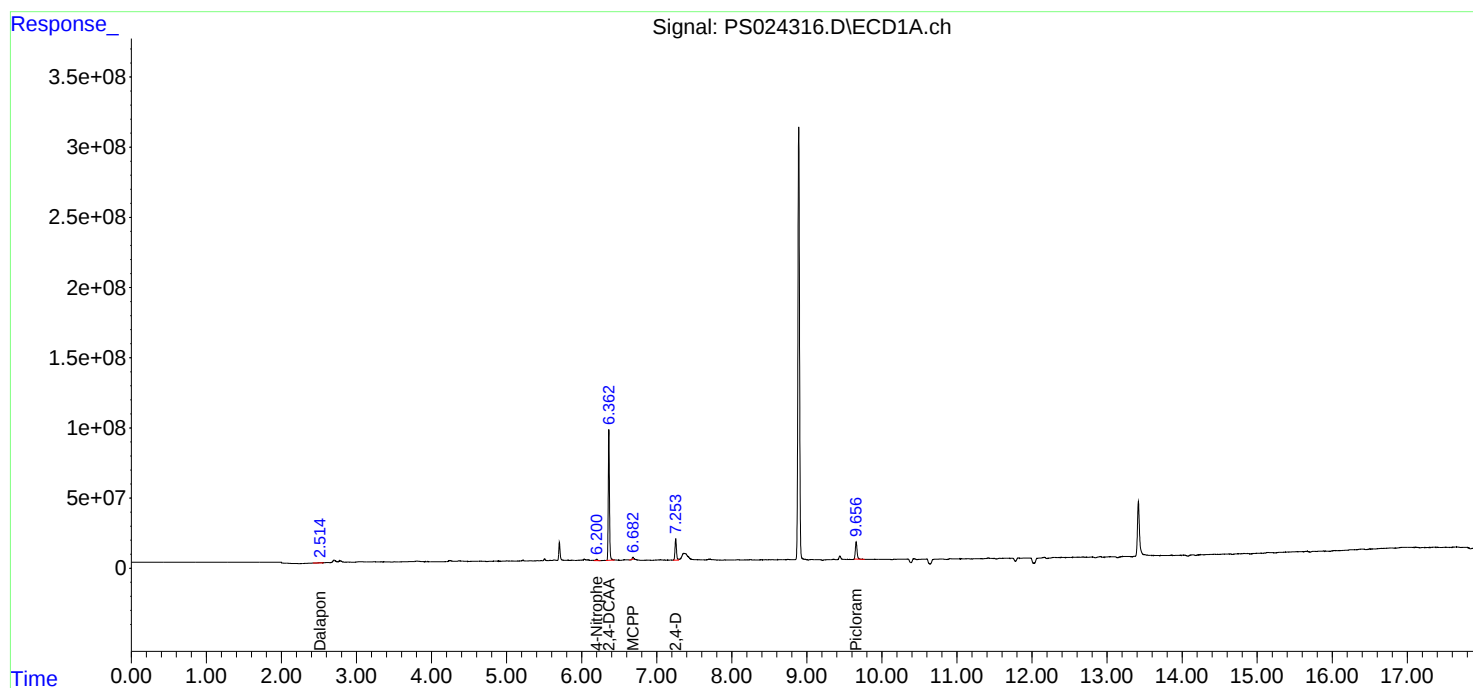


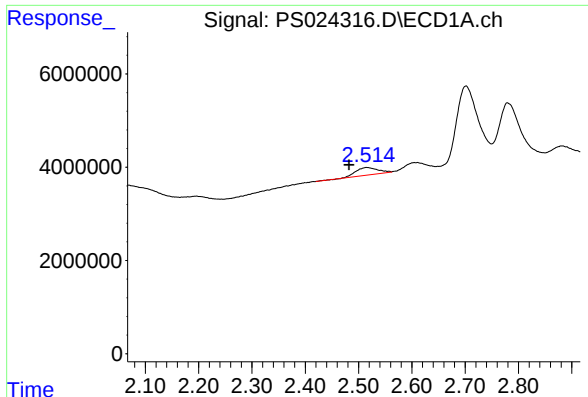

#1 Dalapon


R.T.: 2.515 min
Delta R.T.: 0.033 min
Response: 4635024
Conc: 2.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

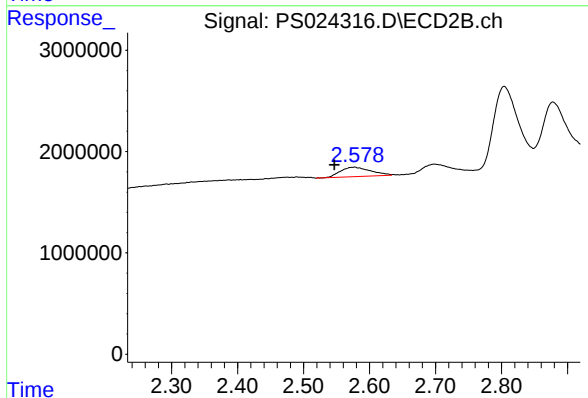


#1 Dalapon

R.T.: 2.578 min
Delta R.T.: 0.031 min
Response: 2959623
Conc: 2.81 ng/ml

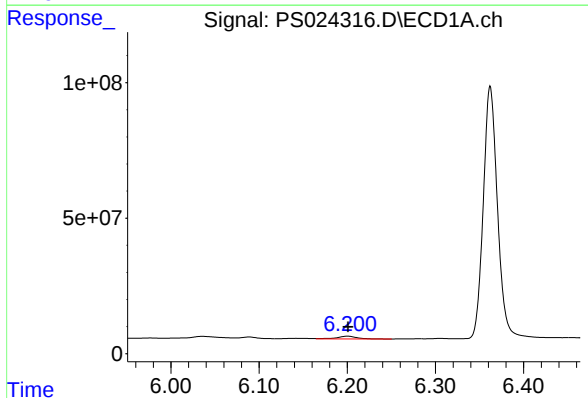


#3 4-Nitrophenol

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 15239881
Conc: 12.27 ng/ml

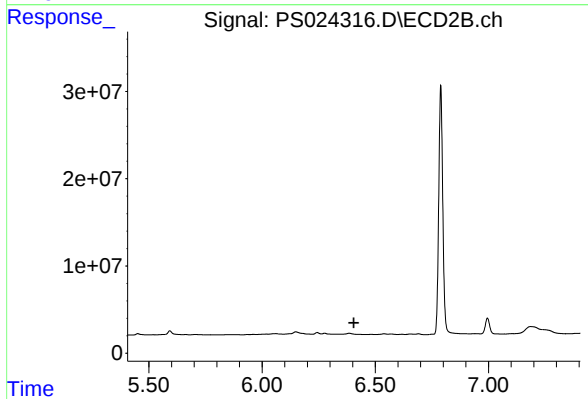

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.405 min
Response: 0
Conc: N.D.

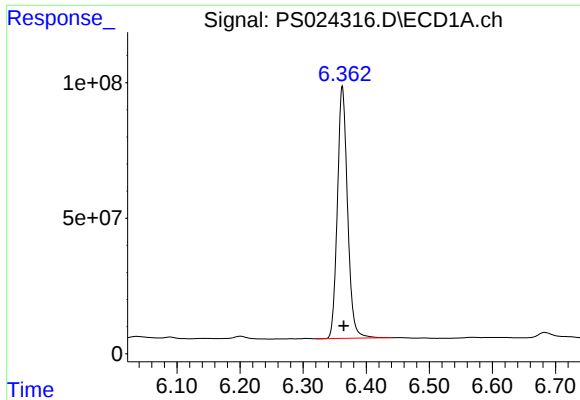

#4 2,4-DCAA


R.T.: 6.362 min
Delta R.T.: -0.002 min
Response: 1041125878
Conc: 522.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

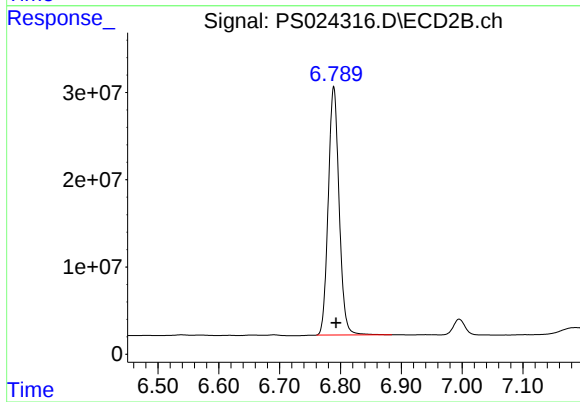


#4 2,4-DCAA

R.T.: 6.789 min
Delta R.T.: -0.004 min
Response: 353596040
Conc: 526.50 ng/ml

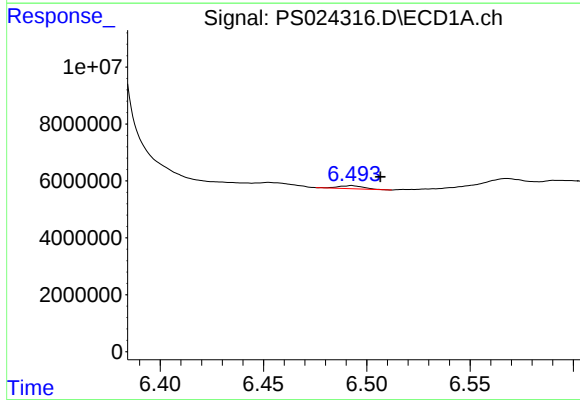


#5 DICAMBA

R.T.: 6.492 min
Delta R.T.: -0.014 min
Response: 930451
Conc: N.D.

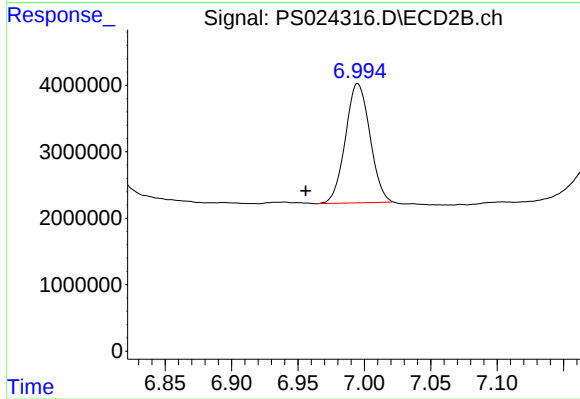

#5 DICAMBA


R.T.: 6.995 min
Delta R.T.: 0.039 min
Response: 23038846
Conc: 8.00 ng/ml

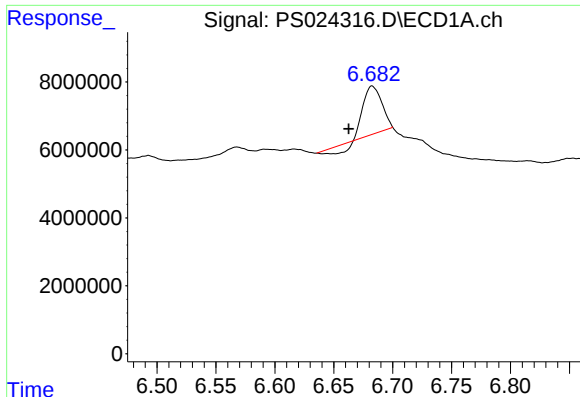

#6 MCP


R.T.: 6.683 min
Delta R.T.: 0.020 min
Response: 13789948
Conc: 2.21 ug/ml

Instrument :
ECD_S
ClientSampleId :

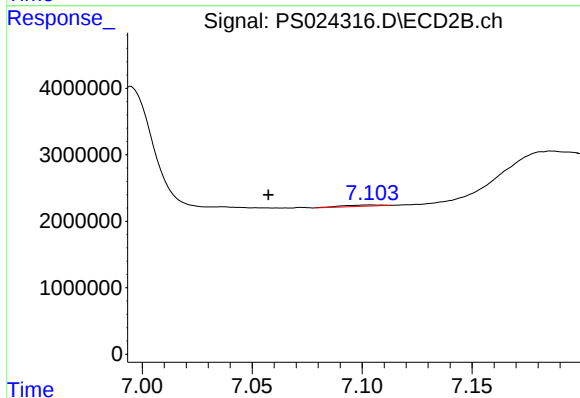


#6 MCP

R.T.: 7.104 min
Delta R.T.: 0.047 min
Response: 243590
Conc: N.D.

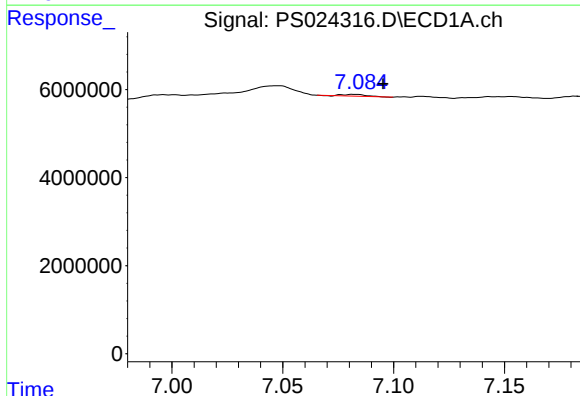


#8 DICHLORPROP

R.T.: 7.081 min
Delta R.T.: -0.014 min
Response: 269927
Conc: N.D.

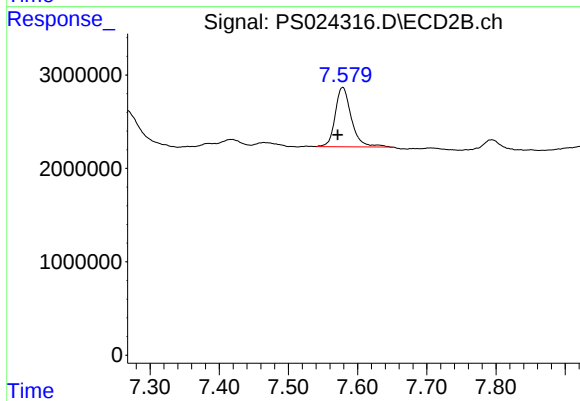

#8 DICHLORPROP


R.T.: 7.578 min
Delta R.T.: 0.007 min
Response: 10332907
Conc: 14.22 ng/ml

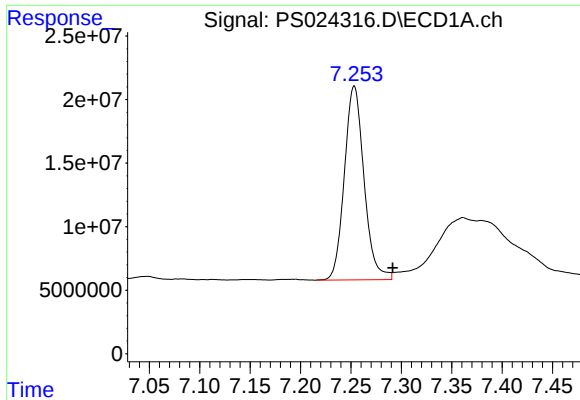

#9 2,4-D


R.T.: 7.253 min
Delta R.T.: -0.038 min
Response: 207240816
Conc: 77.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

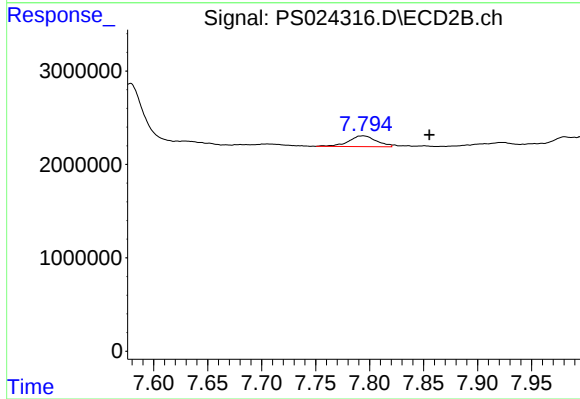


#9 2,4-D

R.T.: 7.794 min
Delta R.T.: -0.061 min
Response: 2071331
Conc: 2.33 ng/ml

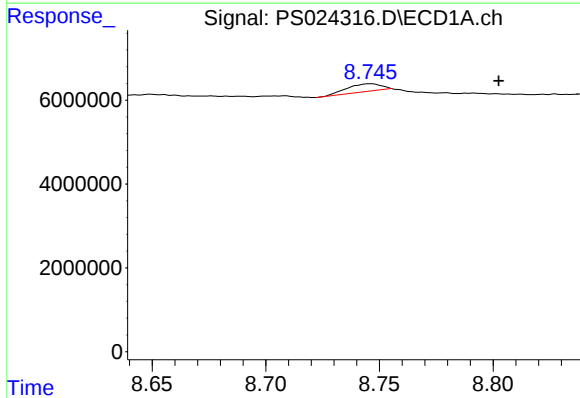


#13 2,4-DB

R.T.: 8.746 min
Delta R.T.: -0.057 min
Response: 1977353
Conc: N.D.

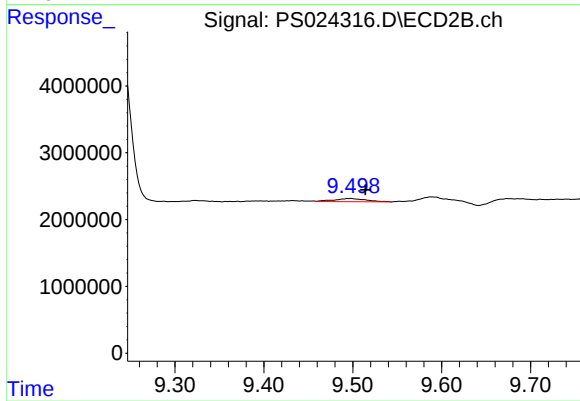

#13 2,4-DB


R.T.: 9.498 min
Delta R.T.: -0.016 min
Response: 1218520
Conc: 2.65 ng/ml

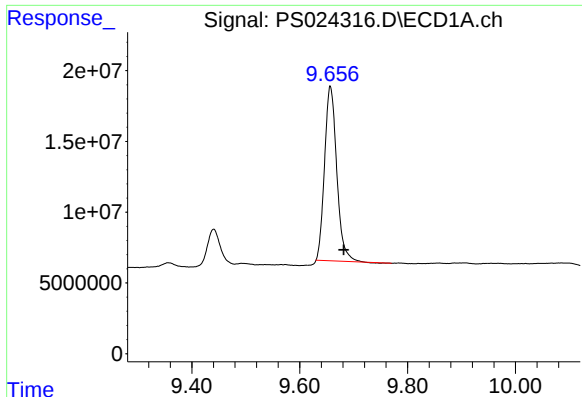

#15 Picloram


R.T.: 9.657 min
Delta R.T.: -0.025 min
Response: 193195166
Conc: 11.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

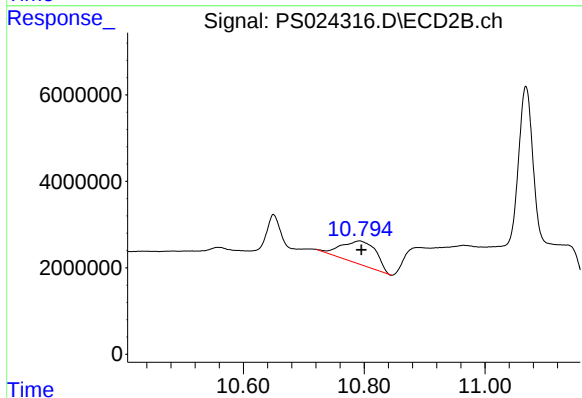


#15 Picloram

R.T.: 10.792 min
Delta R.T.: -0.003 min
Response: 21148835
Conc: 3.56 ng/ml

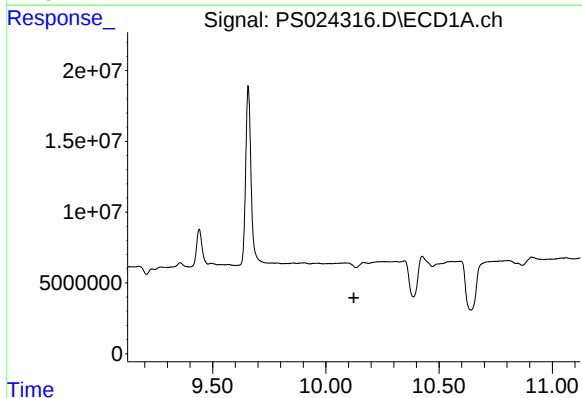

#16 DCPA

R.T.: 10.166 min
Delta R.T.: 0.043 min
Response: -1886054
Conc: N.D.

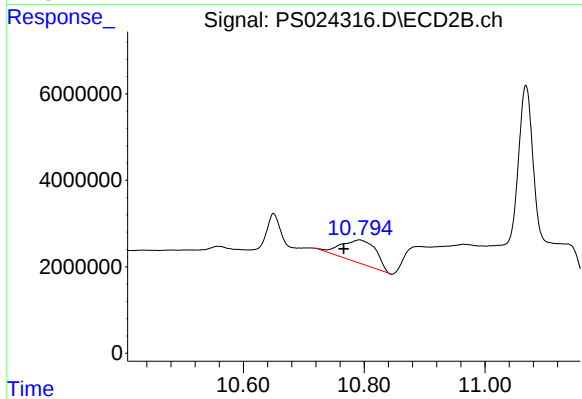

#16 DCPA

R.T.: 10.792 min
Delta R.T.: 0.026 min
Response: 21148835
Conc: 4.12 ng/ml