

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 12:18
 Operator : DD\AJ
 Sample : L3660-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 13:18:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	289.5E6	166.0E6	267.076	314.697
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	54280003	N.D.	67.095
3) T	4-Nitroph...	7.108	0.000	8691784	0	16.321	N.D. #
5) T	DICAMBA	7.393	7.045	6498487	11397683	1.544	5.285 #
6) T	MCP	7.570	0.000	5331819	0	1.655	N.D. #
7) T	MCPA	7.685	7.462	325.4E6	186.7E6	69.641	66.443
8) T	DICHLORPROP	0.000	7.737	0	14014805	N.D.	24.769
9) T	2,4-D	8.395	7.955	100.6E6	11367272	88.368	15.627 #
11) T	2,4,5-TP ...	0.000	8.759	0	10821564	N.D.	3.739
12) T	2,4,5-T	9.409	0.000	17762657	0	2.896	N.D. #
14) T	DINOSEB	0.000	10.070	0	7663827	N.D.	3.690
15) T	Picloram	10.999	0.000	11909774	0	1.618	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 12:18
Operator : DD\AJ
Sample : L3660-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 13:18:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

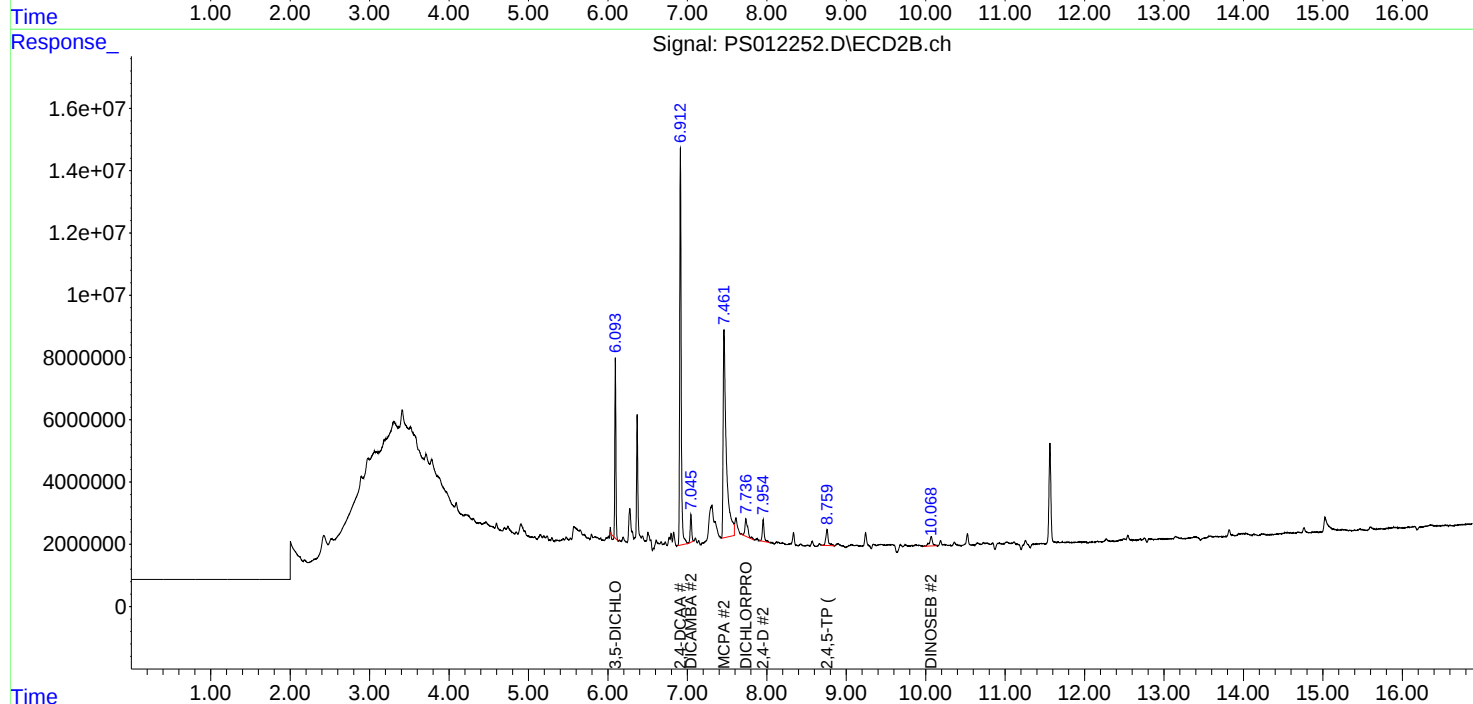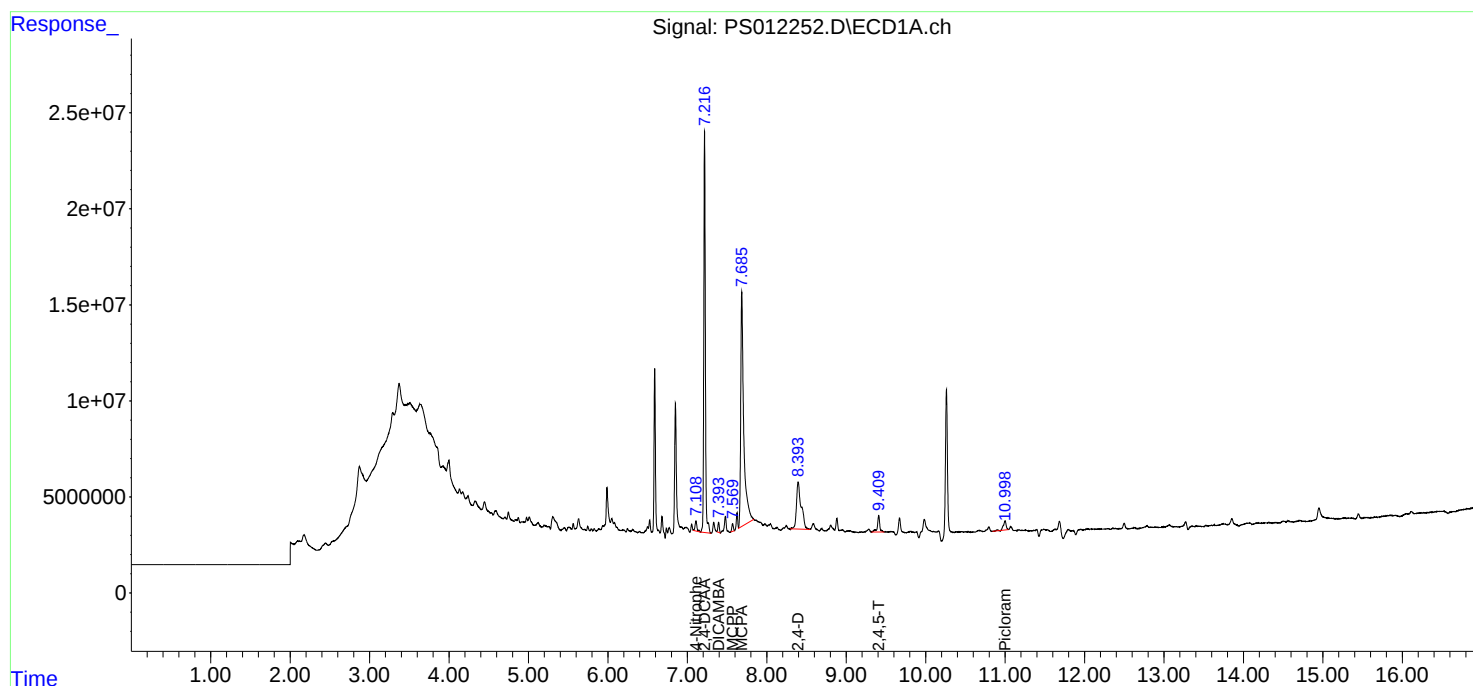


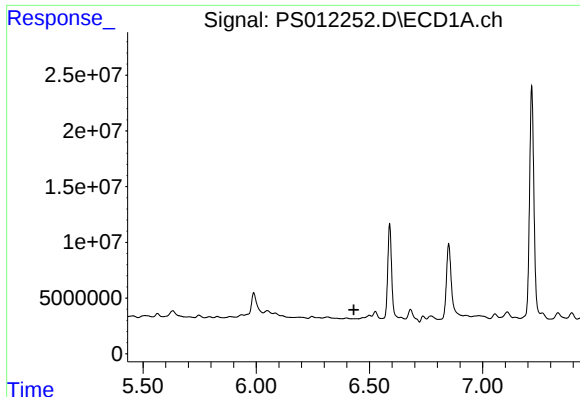

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

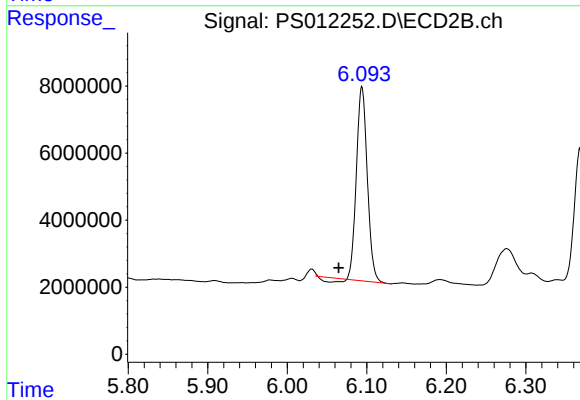


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 54280003
Conc: 67.10 ng/ml

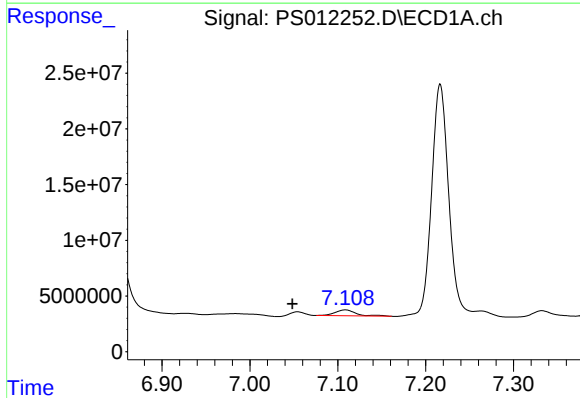


#3 4-Nitrophenol

R.T.: 7.108 min
Delta R.T.: 0.060 min
Response: 8691784
Conc: 16.32 ng/ml

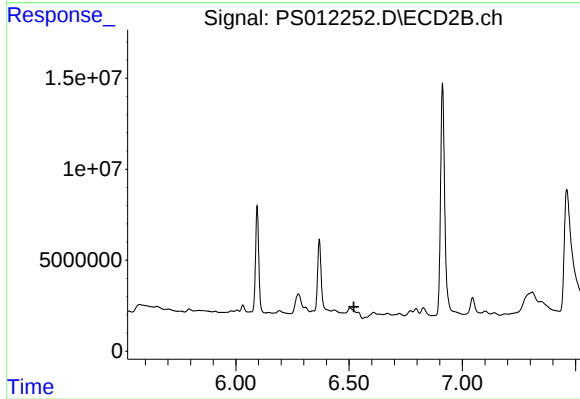

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

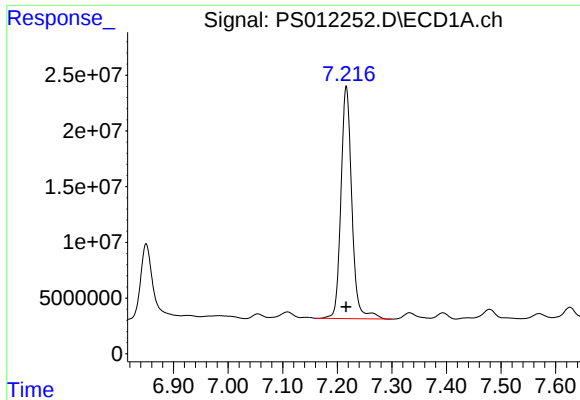

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 289482507
Conc: 267.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

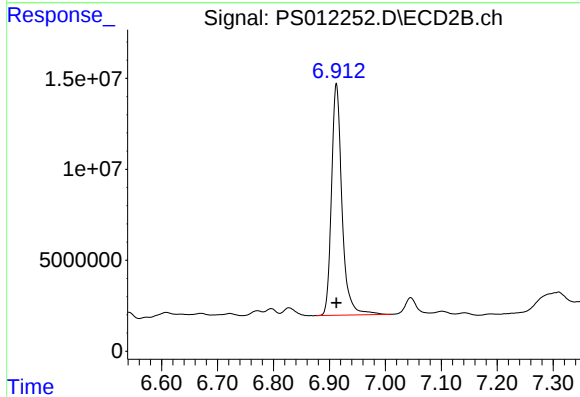


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 166035632
Conc: 314.70 ng/ml

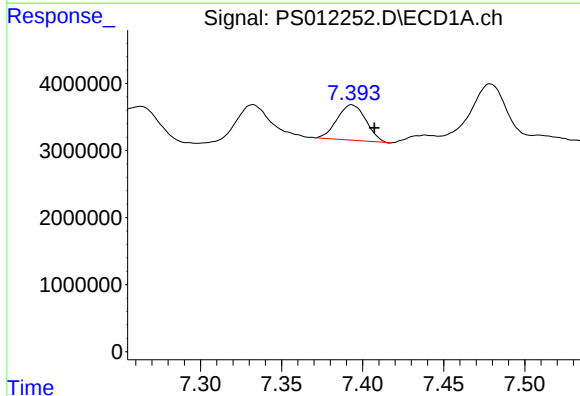


#5 DICAMBA

R.T.: 7.393 min
Delta R.T.: -0.014 min
Response: 6498487
Conc: 1.54 ng/ml

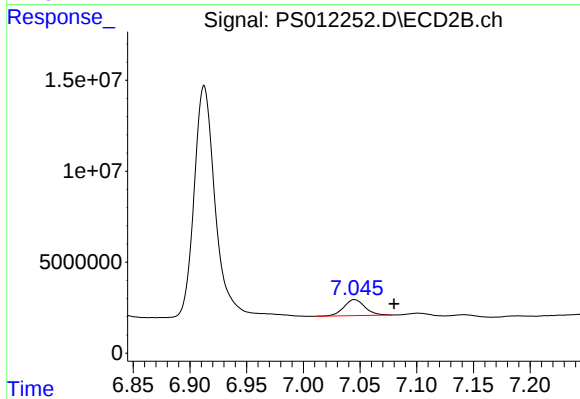

#5 DICAMBA


R.T.: 7.045 min
Delta R.T.: -0.035 min
Response: 11397683
Conc: 5.28 ng/ml

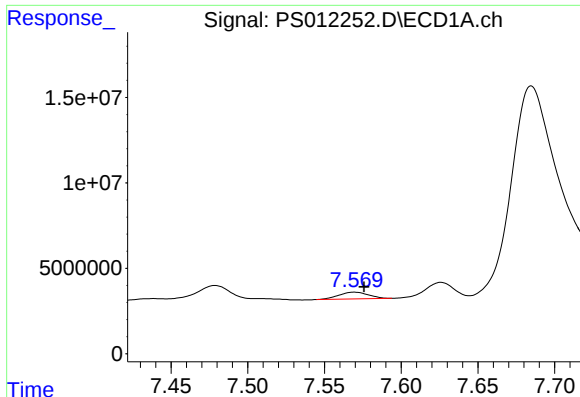

#6 MCPP


R.T.: 7.570 min
Delta R.T.: -0.006 min
Response: 5331819
Conc: 1.65 ug/ml

Instrument :
ECD_S
ClientSampleId :

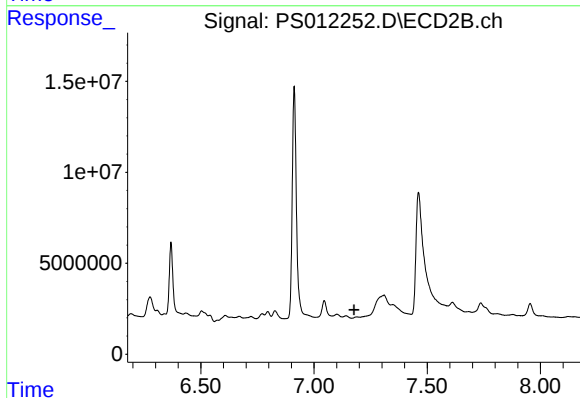


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

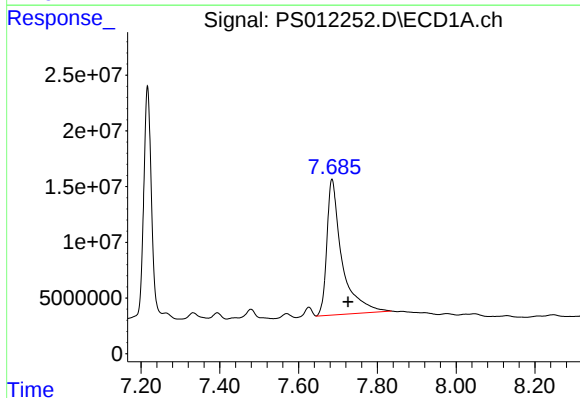


#7 MCPA

R.T.: 7.685 min
Delta R.T.: -0.041 min
Response: 325391756
Conc: 69.64 ug/ml

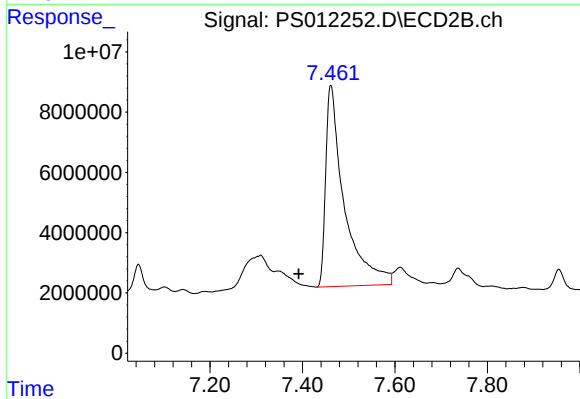

#7 MCPA


R.T.: 7.462 min
Delta R.T.: 0.070 min
Response: 186722273
Conc: 66.44 ug/ml

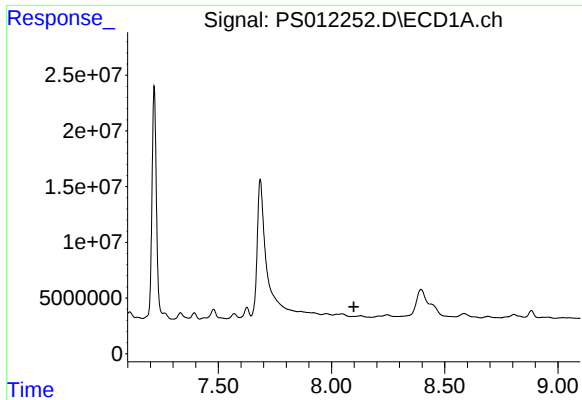

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

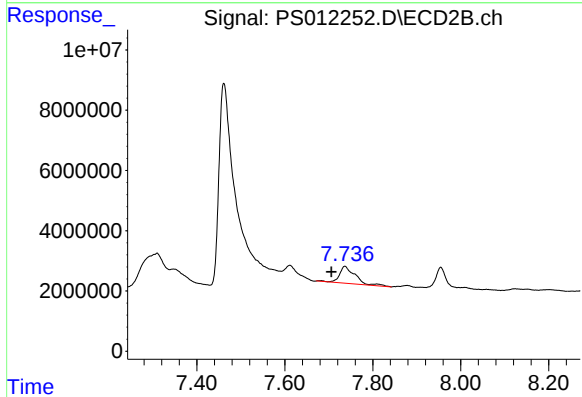


#8 DICHLORPROP

R.T.: 7.737 min
Delta R.T.: 0.031 min
Response: 14014805
Conc: 24.77 ng/ml

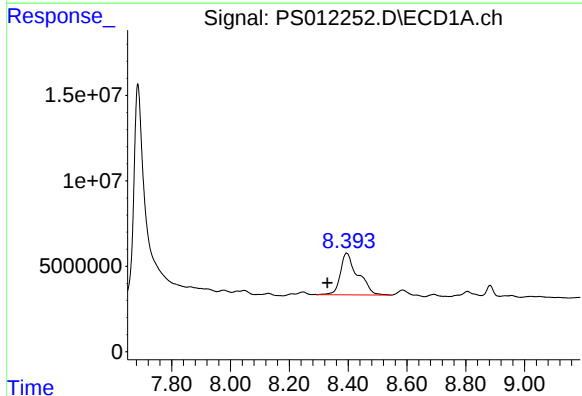


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.065 min
Response: 100647355
Conc: 88.37 ng/ml

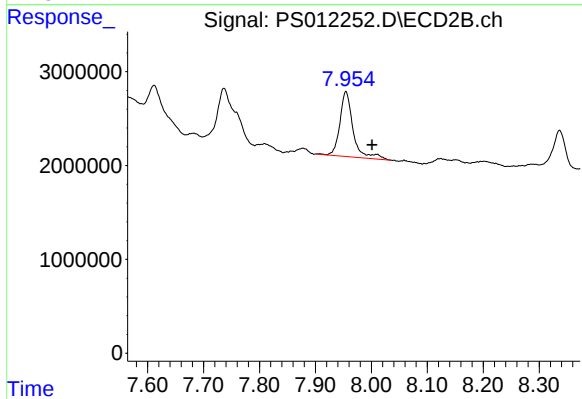

#9 2,4-D


R.T.: 7.955 min
Delta R.T.: -0.047 min
Response: 11367272
Conc: 15.63 ng/ml

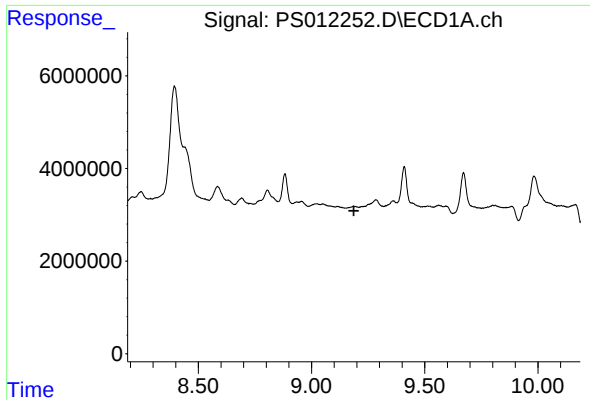

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

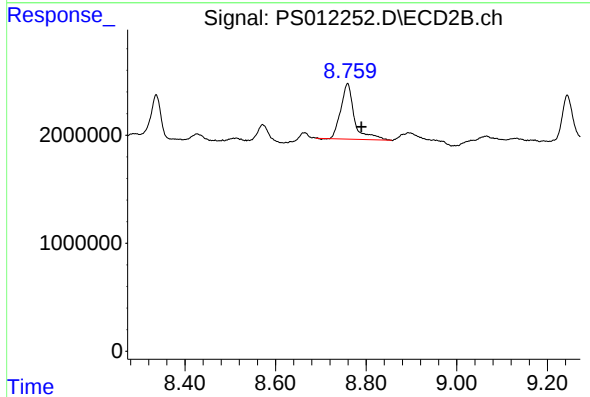


#11 2,4,5-TP (SILVEX)

R.T.: 8.759 min
Delta R.T.: -0.031 min
Response: 10821564
Conc: 3.74 ng/ml

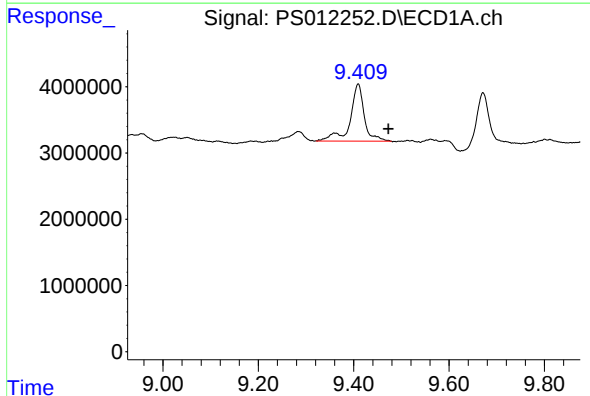


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.064 min
Response: 17762657
Conc: 2.90 ng/ml

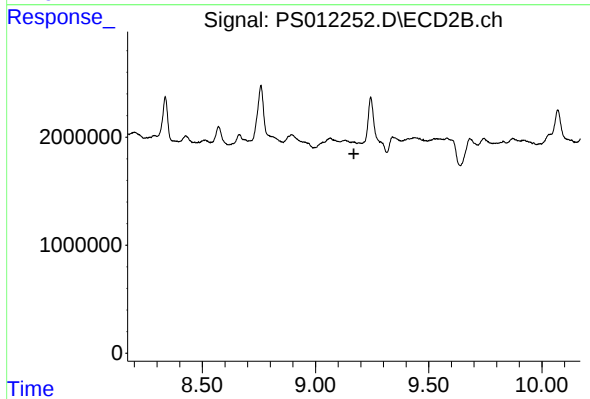

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

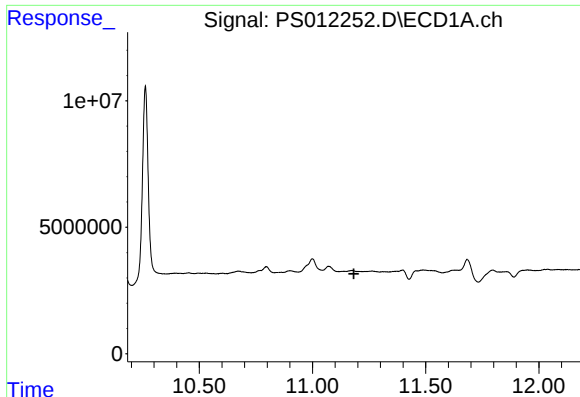

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

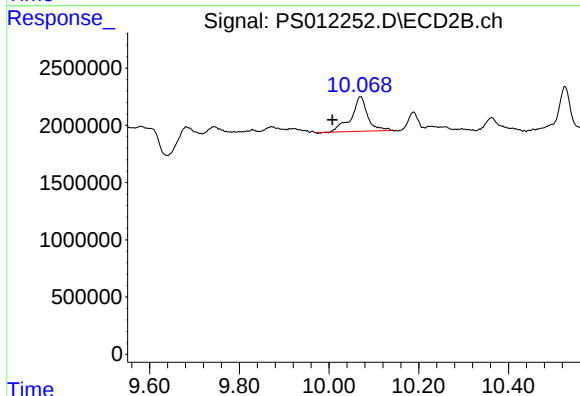


#14 DINOSEB

R.T.: 10.070 min
Delta R.T.: 0.063 min
Response: 7663827
Conc: 3.69 ng/ml

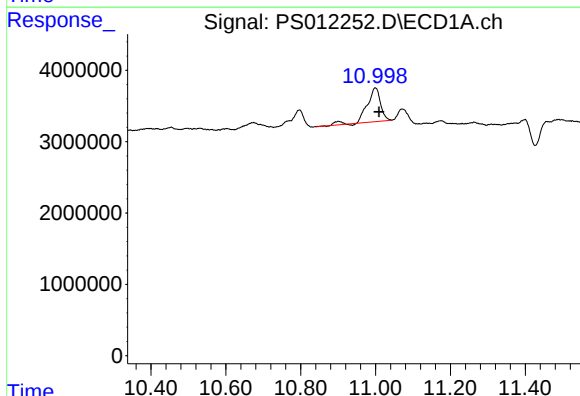

#15 Picloram

R.T.: 10.999 min
Delta R.T.: -0.010 min
Response: 11909774
Conc: 1.62 ng/ml

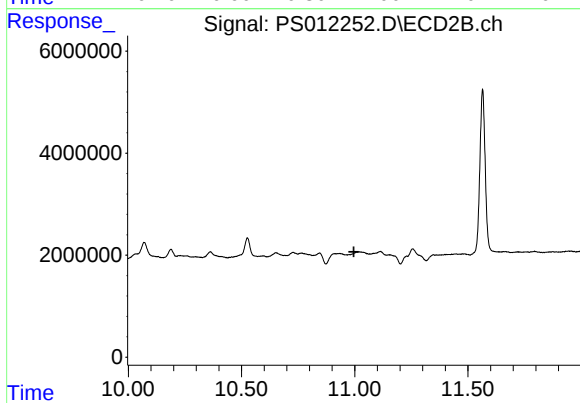

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.996 min
Response: 0
Conc: N.D.