

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 12:41
 Operator : DD\AJ
 Sample : L3660-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 13:18:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	349.0E6	192.0E6	321.944	364.003
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	59139703	N.D.	73.102
3) T	4-Nitroph...	7.113	6.542	20848204	7916990	39.149	24.751 #
5) T	DICAMBA	7.393	7.046	6288239	11670323	1.494	5.411 #
6) T	MCP	7.627	0.000	11316015	0	3.512	N.D. #
7) T	MCPA	7.685	0.000	320.7E6	0	68.631	N.D. #
8) T	DICHLORPROP	8.045	7.736	8727356	9427915	8.534	16.663 #
9) T	2,4-D	8.395	0.000	97177320	0	85.321	N.D. #
11) T	2,4,5-TP ...	0.000	8.759	0	9849271	N.D.	3.403
12) T	2,4,5-T	9.410	0.000	22034246	0	3.593	N.D. #
13) T	2,4-DB	0.000	9.684	0	2517133	N.D.	6.187



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 12:41
Operator : DD\AJ
Sample : L3660-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 13:18:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

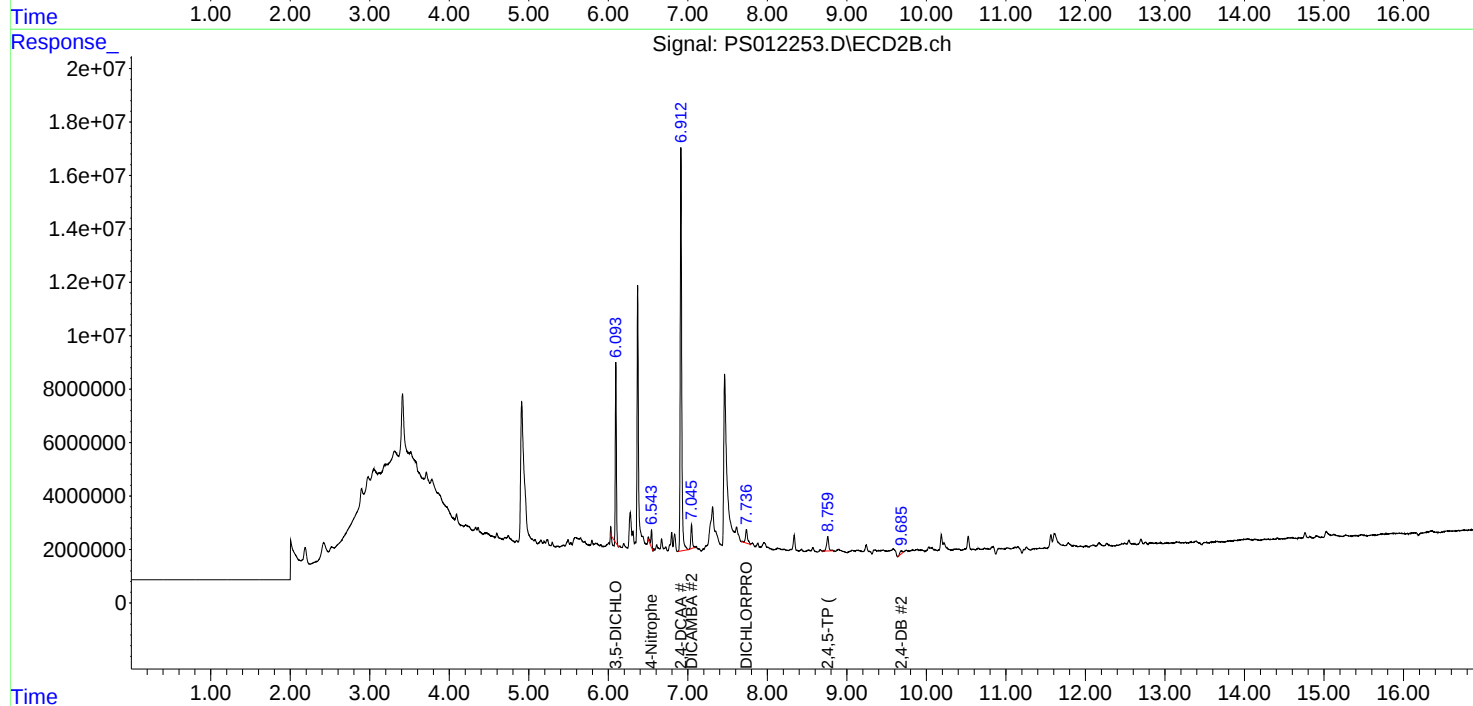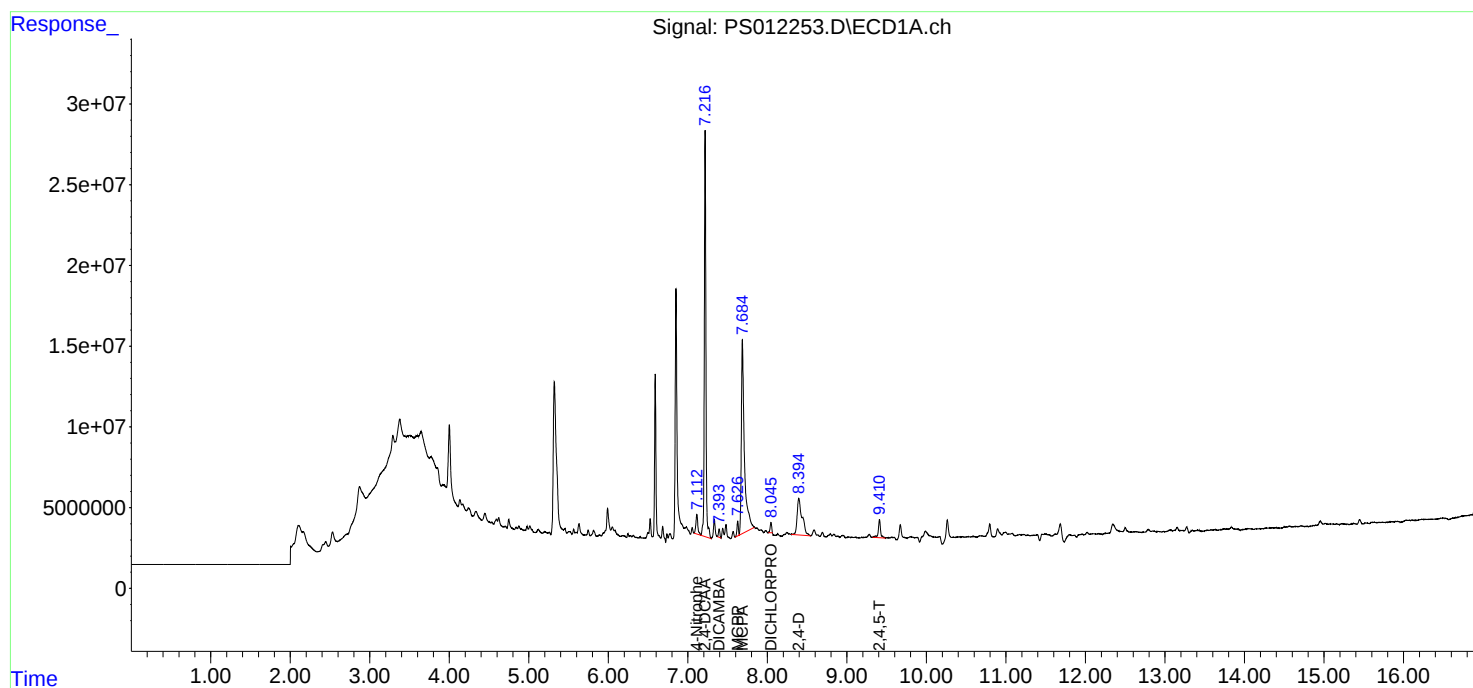


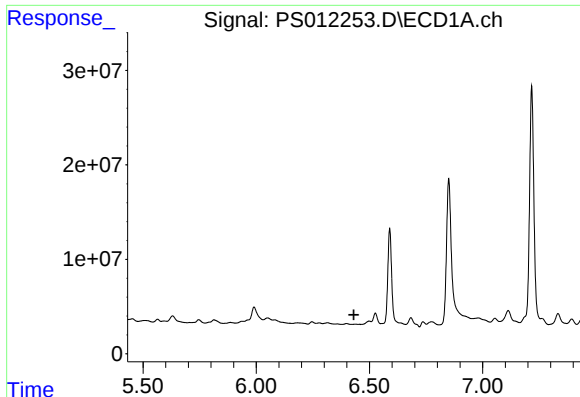

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

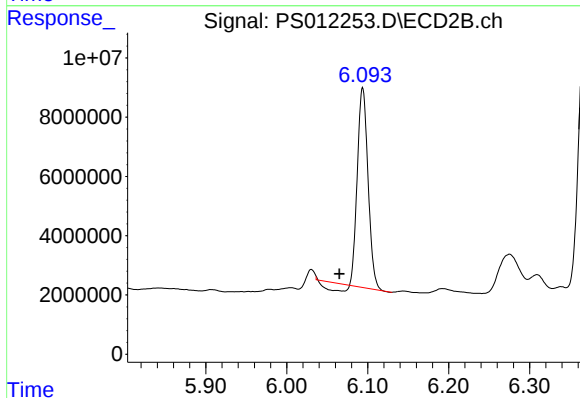


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 59139703
Conc: 73.10 ng/ml

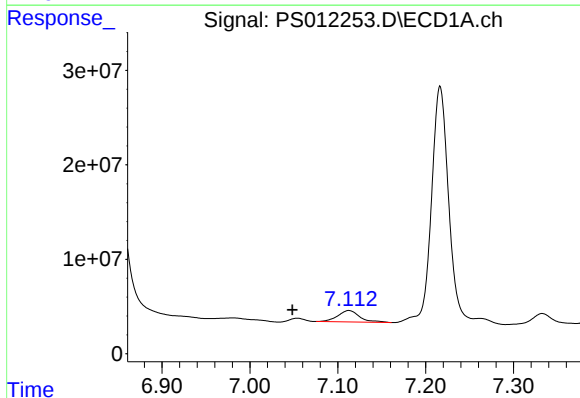


#3 4-Nitrophenol

R.T.: 7.113 min
Delta R.T.: 0.064 min
Response: 20848204
Conc: 39.15 ng/ml

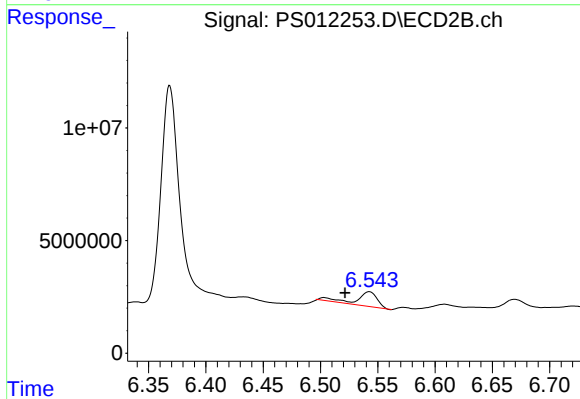

#3 4-Nitrophenol


R.T.: 6.542 min
Delta R.T.: 0.021 min
Response: 7916990
Conc: 24.75 ng/ml

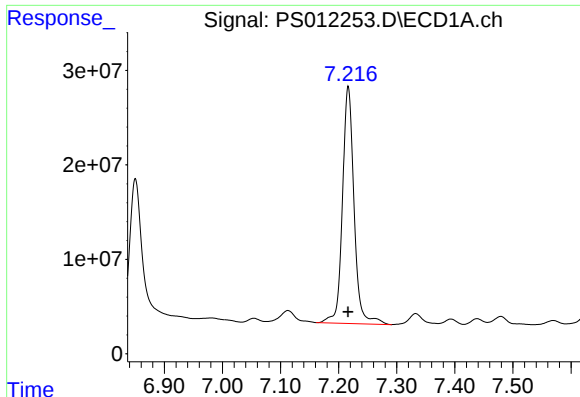

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 348954163
Conc: 321.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

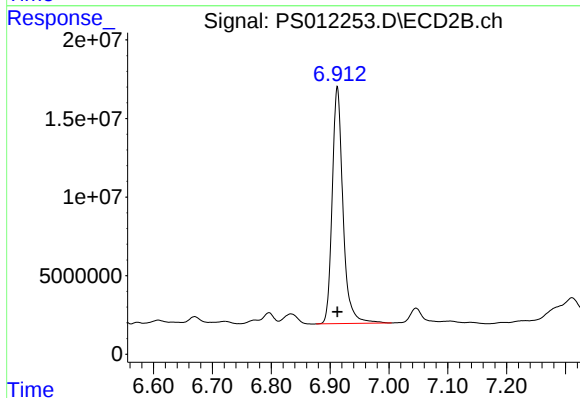


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 192049693
Conc: 364.00 ng/ml

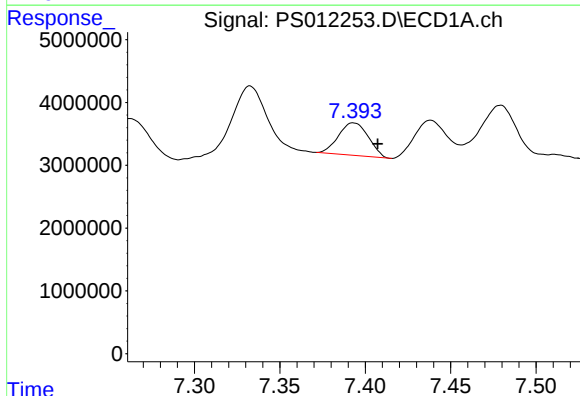


#5 DICAMBA

R.T.: 7.393 min
Delta R.T.: -0.014 min
Response: 6288239
Conc: 1.49 ng/ml

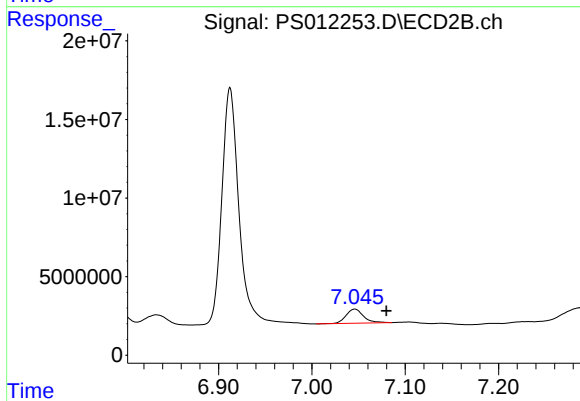

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 11670323
Conc: 5.41 ng/ml

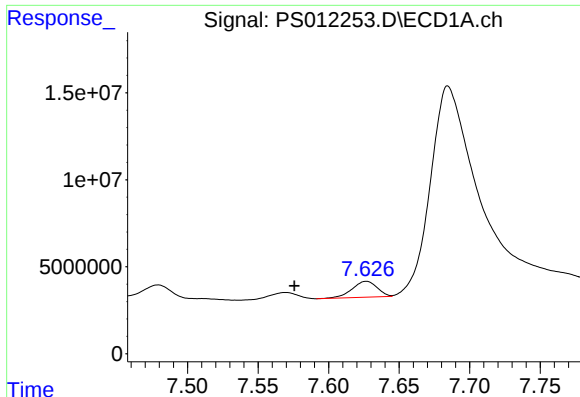

#6 MCPP


R.T.: 7.627 min
Delta R.T.: 0.051 min
Response: 11316015
Conc: 3.51 ug/ml

Instrument :
ECD_S
ClientSampleId :

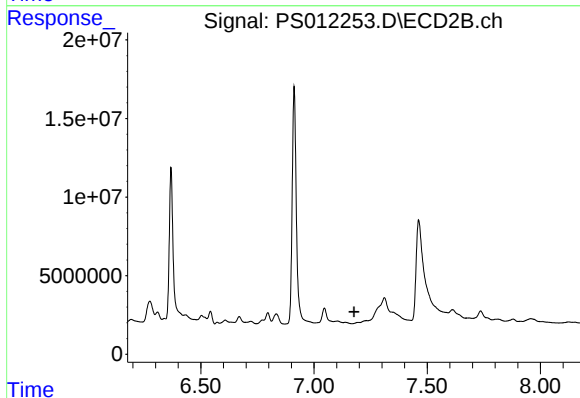


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

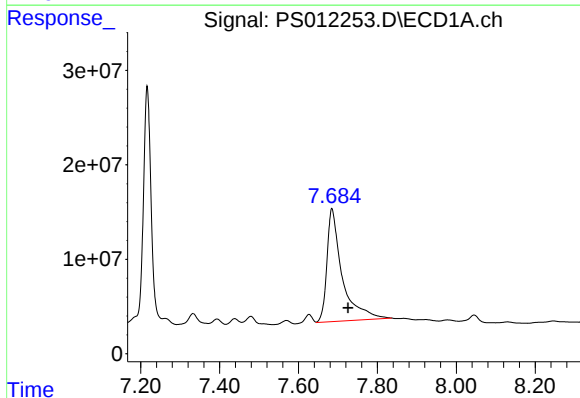


#7 MCPA

R.T.: 7.685 min
Delta R.T.: -0.041 min
Response: 320673619
Conc: 68.63 ug/ml

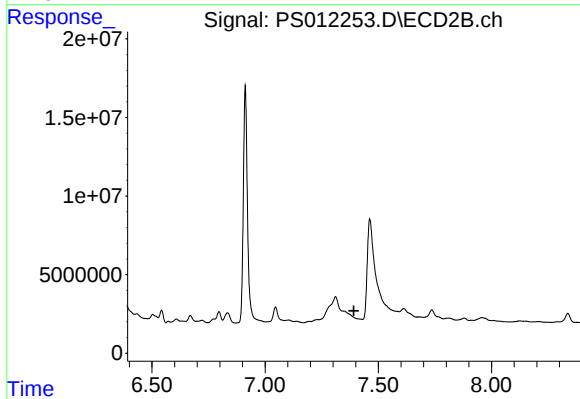

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

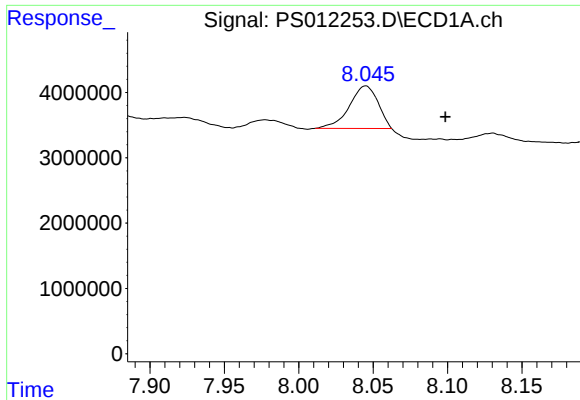

#8 DICHLORPROP


R.T.: 8.045 min
Delta R.T.: -0.054 min
Response: 8727356
Conc: 8.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

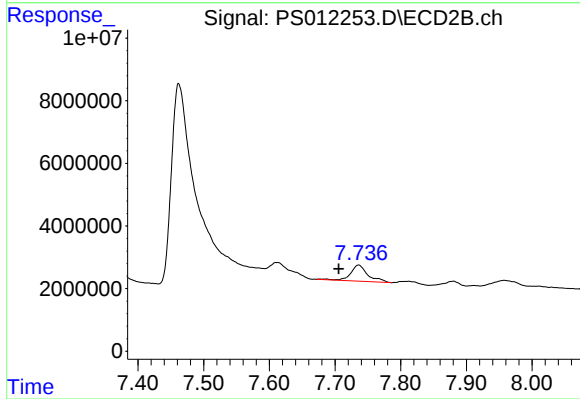


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.030 min
Response: 9427915
Conc: 16.66 ng/ml

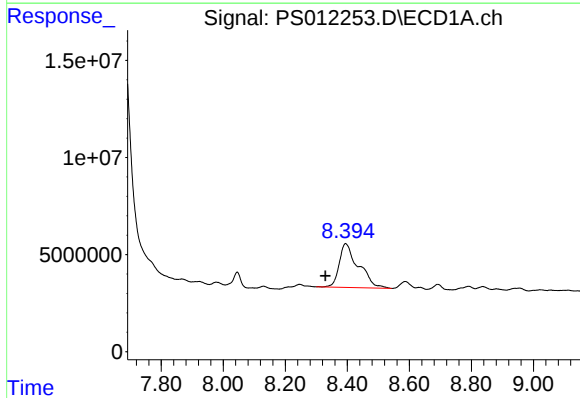


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.065 min
Response: 97177320
Conc: 85.32 ng/ml

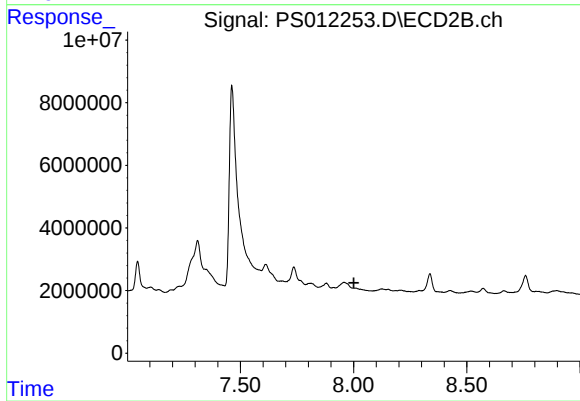

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

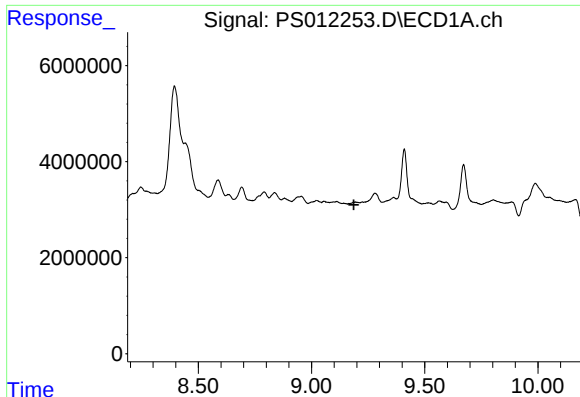

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

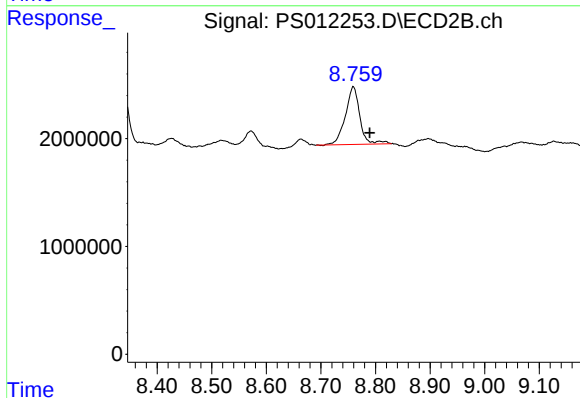


#11 2,4,5-TP (SILVEX)

R.T.: 8.759 min
Delta R.T.: -0.030 min
Response: 9849271
Conc: 3.40 ng/ml

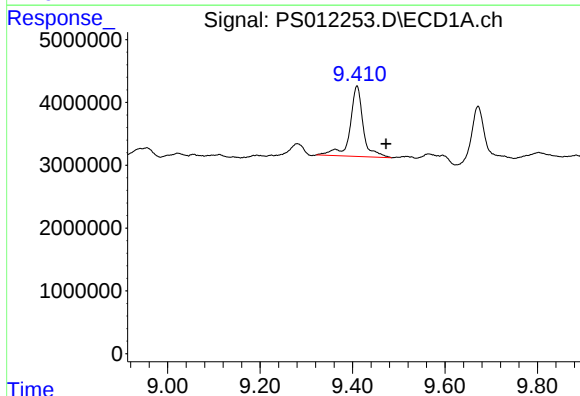


#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.063 min
Response: 22034246
Conc: 3.59 ng/ml

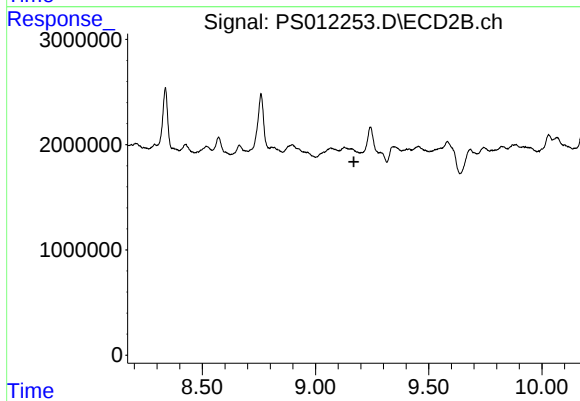

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

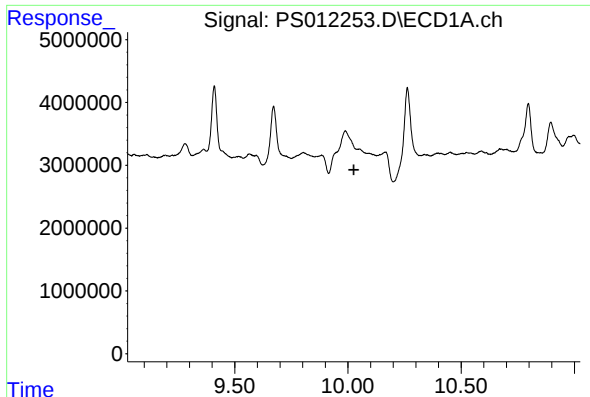

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

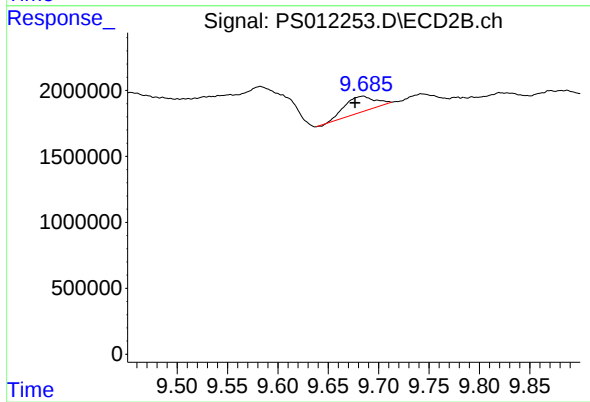

#13 2,4-DB

R.T.: 9.684 min
Delta R.T.: 0.007 min
Response: 2517133
Conc: 6.19 ng/ml