

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012254.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 13:04
 Operator : DD\AJ
 Sample : PB131595BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 13:35:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	618.3E6	341.1E6	570.428	646.580
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	68383153	N.D.	84.528
3) T	4-Nitroph...	7.053	0.000	4202889	0	7.892	N.D. #
5) T	DICAMBA	7.394	7.047	10292105	12681339	2.446	5.880 #
6) T	MCP	7.626	0.000	15050961	0	4.671	N.D. #
7) T	MCPA	7.762	7.373	19958902	25366713	4.272	9.026 #
8) T	DICHLORPROP	0.000	7.745	0	8412943	N.D.	14.869
9) T	2,4-D	8.395	0.000	93333837	0	81.947	N.D. #
11) T	2,4,5-TP ...	0.000	8.765	0	12017429	N.D.	4.152
12) T	2,4,5-T	9.410	0.000	15339881	0	2.501	N.D. #
14) T	DINOSEB	0.000	10.041	0	1436418	N.D.	<MDL
15) T	Picloram	11.009	11.006	11169286	22705685	1.517	5.356 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012254.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 13:04
Operator : DD\AJ
Sample : PB131595BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 13:35:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

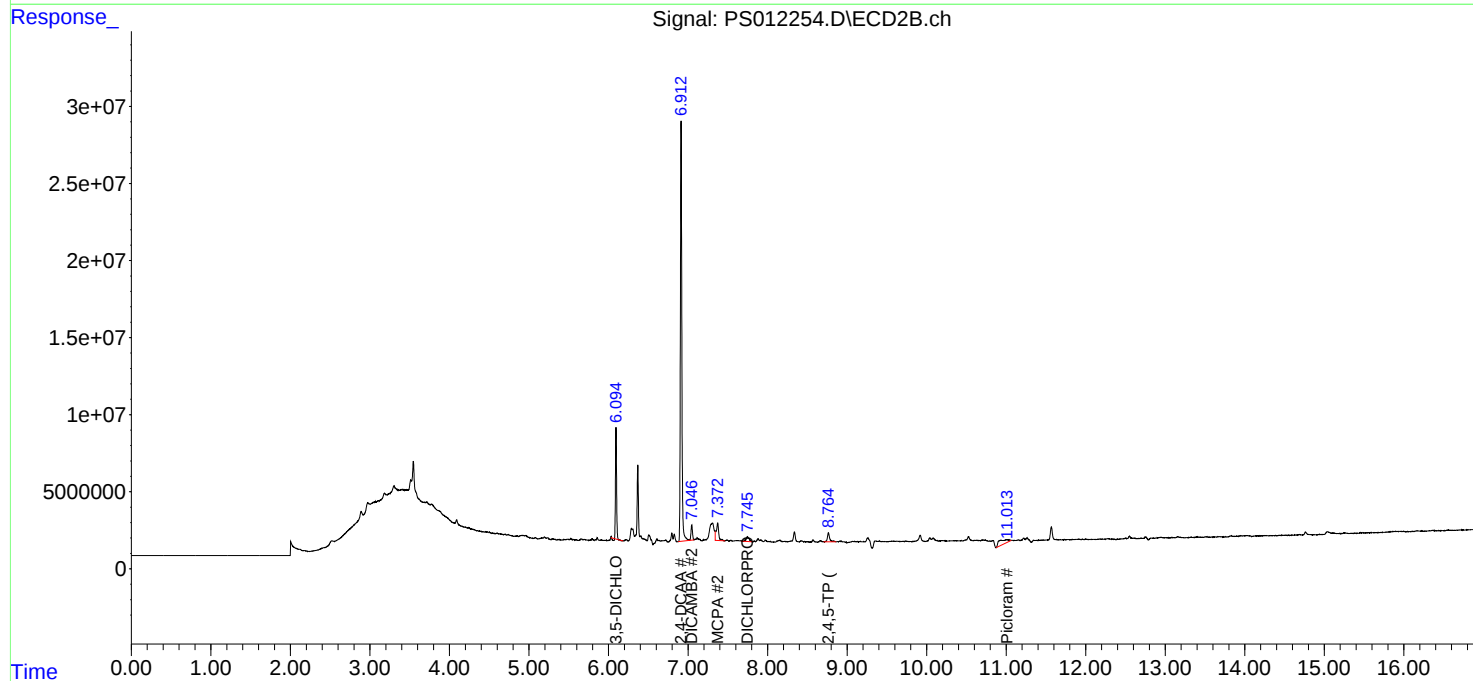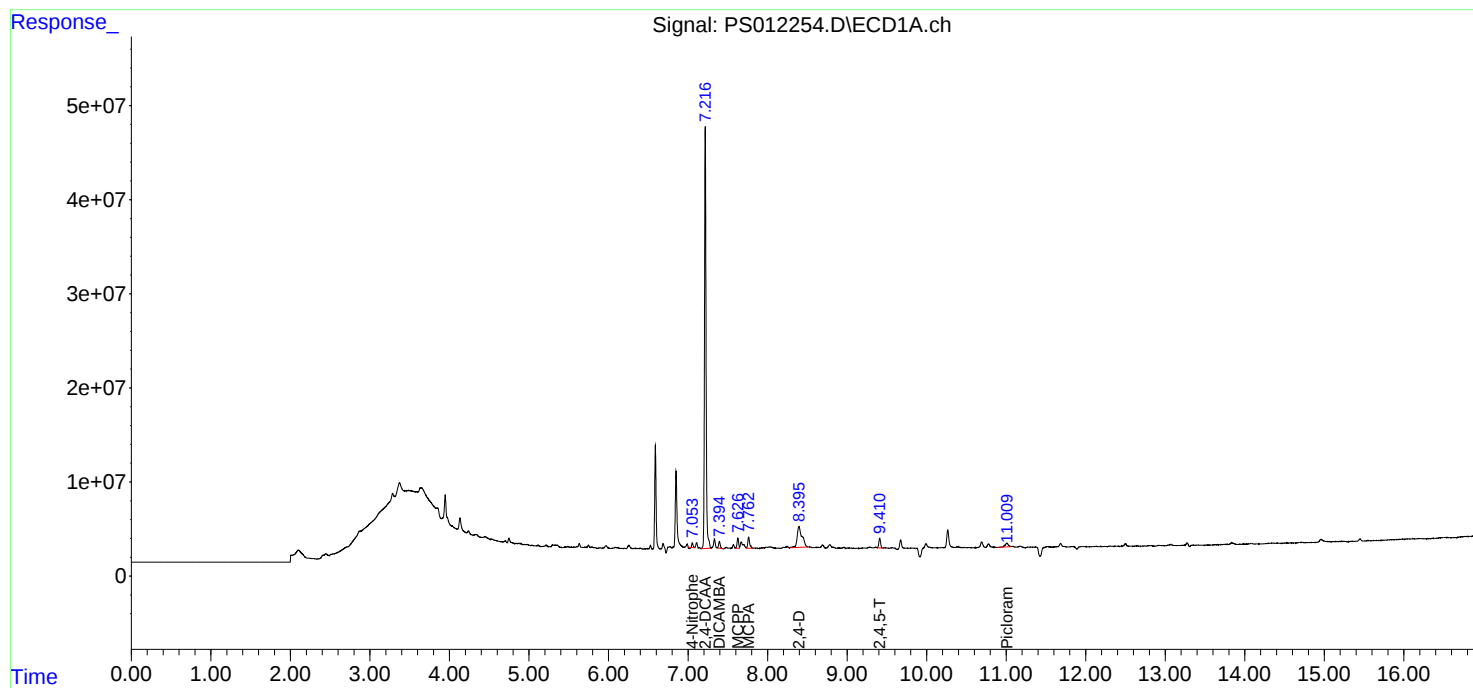


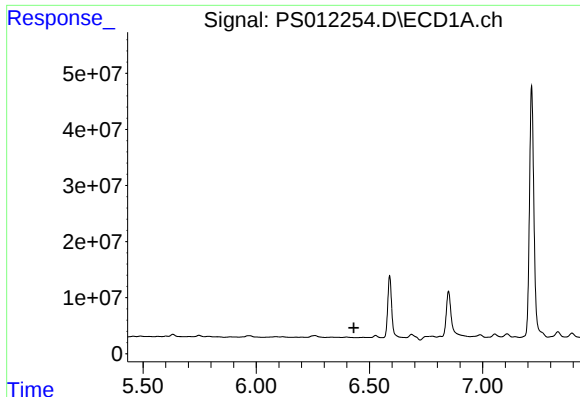

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

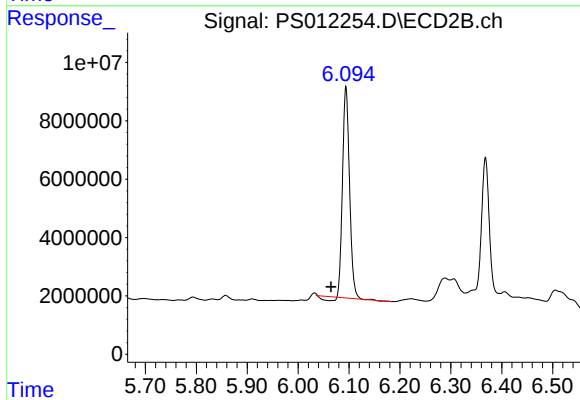


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 68383153
Conc: 84.53 ng/ml

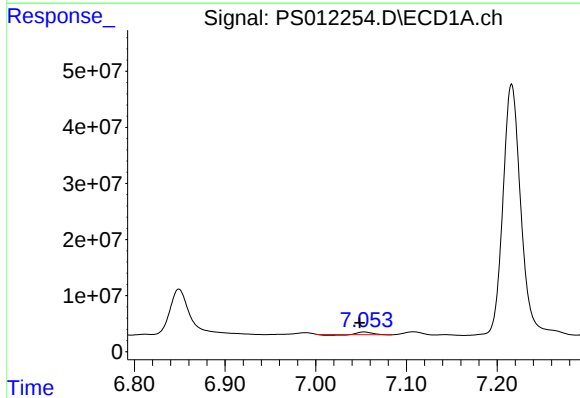


#3 4-Nitrophenol

R.T.: 7.053 min
Delta R.T.: 0.005 min
Response: 4202889
Conc: 7.89 ng/ml

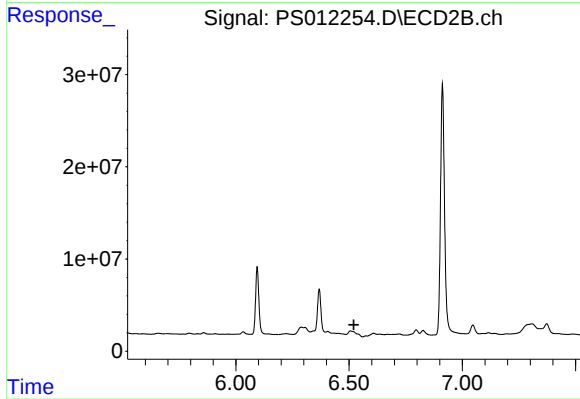

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

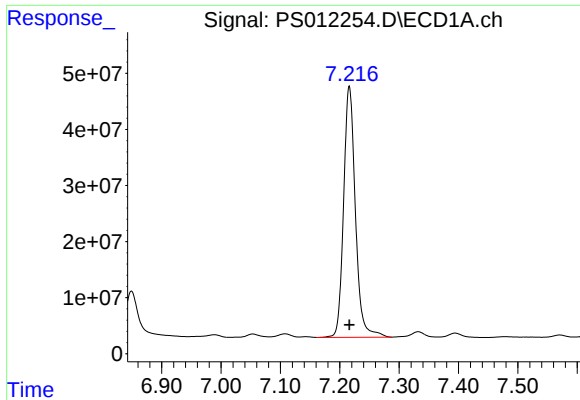

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 618284909
Conc: 570.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

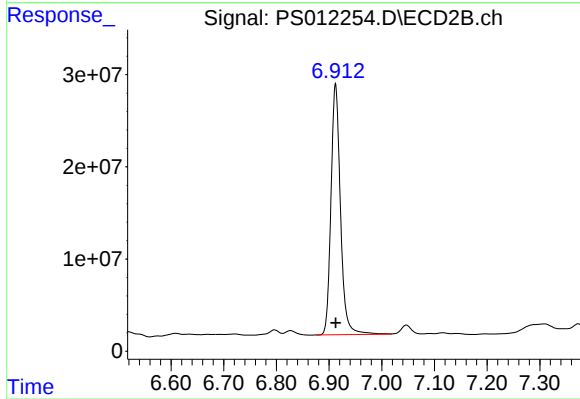


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 341138998
Conc: 646.58 ng/ml

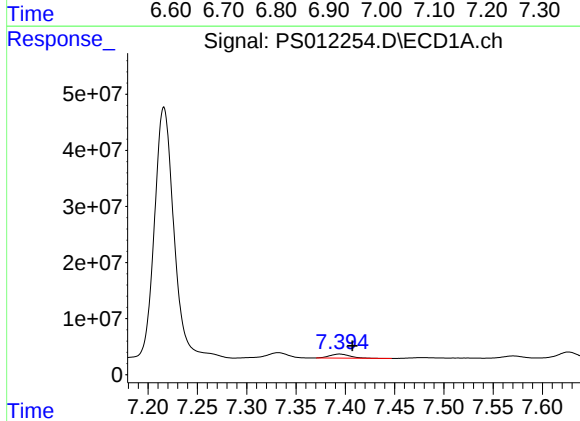


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.013 min
Response: 10292105
Conc: 2.45 ng/ml

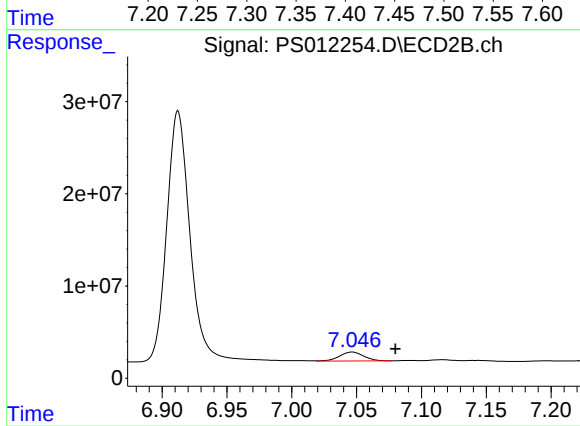

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.034 min
Response: 12681339
Conc: 5.88 ng/ml

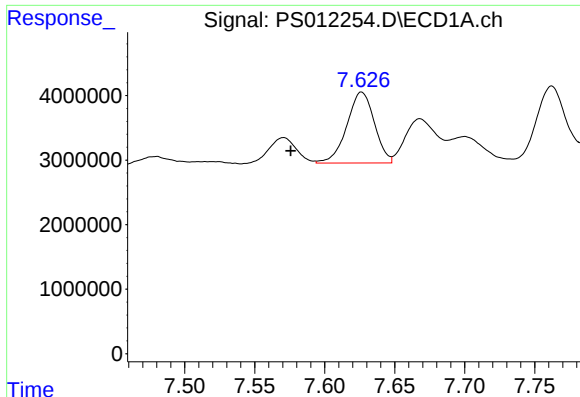

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.051 min
Response: 15050961
Conc: 4.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

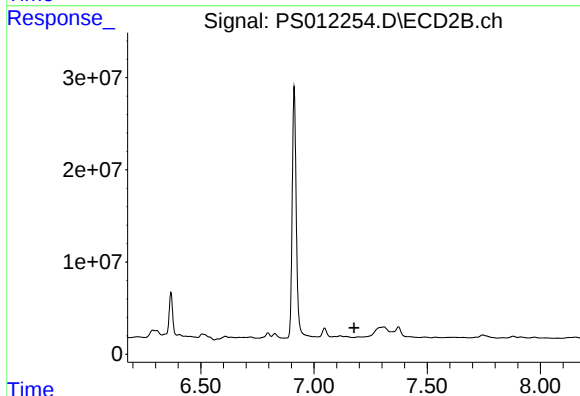


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

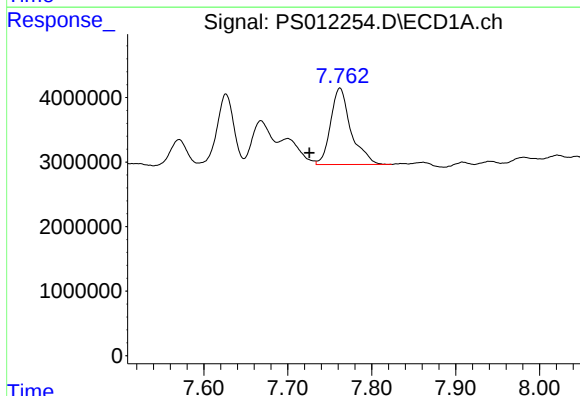


#7 MCPA

R.T.: 7.762 min
Delta R.T.: 0.036 min
Response: 19958902
Conc: 4.27 ug/ml

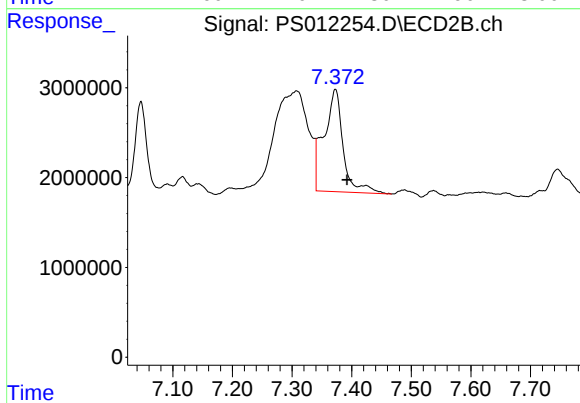

#7 MCPA


R.T.: 7.373 min
Delta R.T.: -0.019 min
Response: 25366713
Conc: 9.03 ug/ml

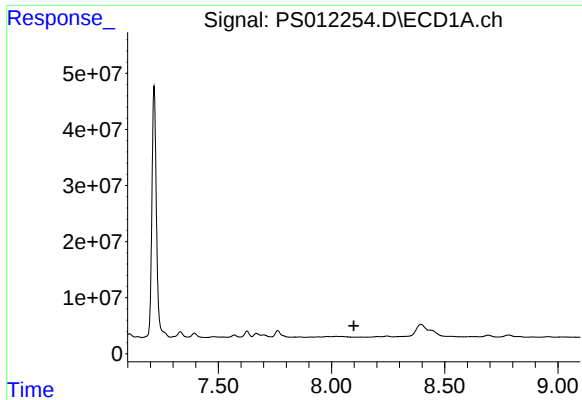

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

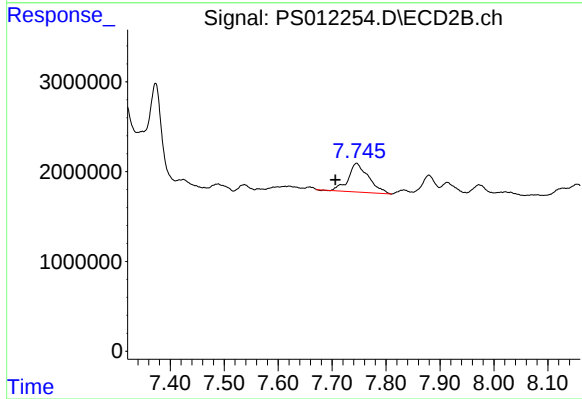


#8 DICHLORPROP

R.T.: 7.745 min
Delta R.T.: 0.039 min
Response: 8412943
Conc: 14.87 ng/ml

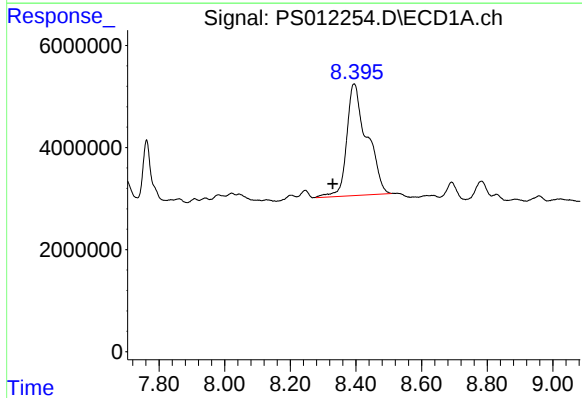


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.065 min
Response: 93333837
Conc: 81.95 ng/ml

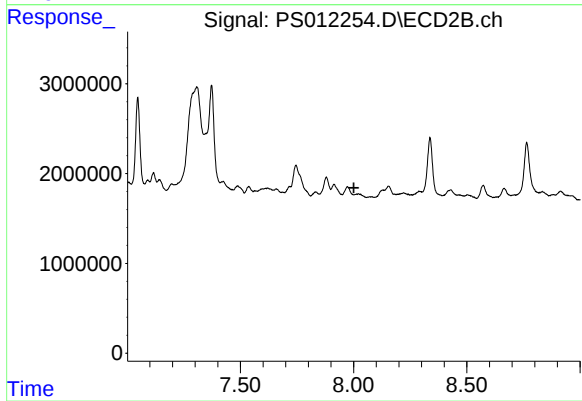

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

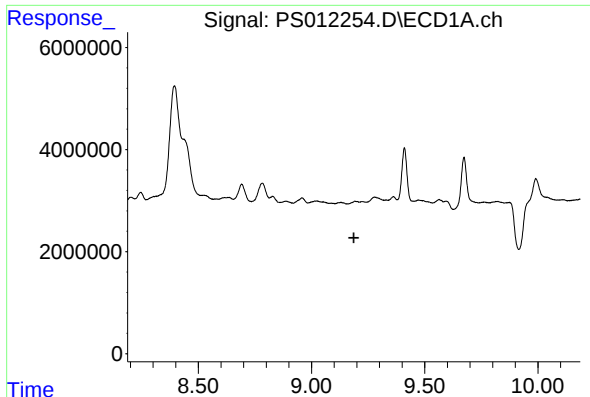

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

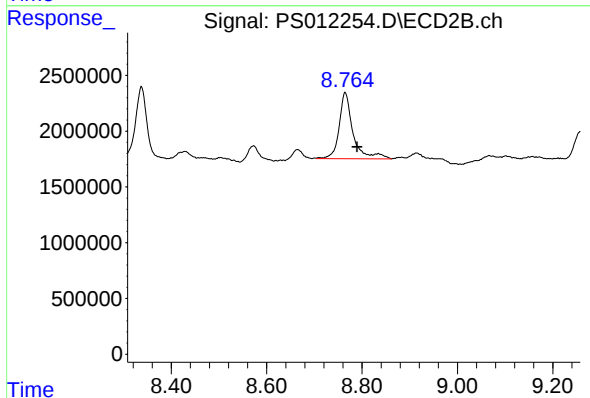


#11 2,4,5-TP (SILVEX)

R.T.: 8.765 min
Delta R.T.: -0.025 min
Response: 12017429
Conc: 4.15 ng/ml

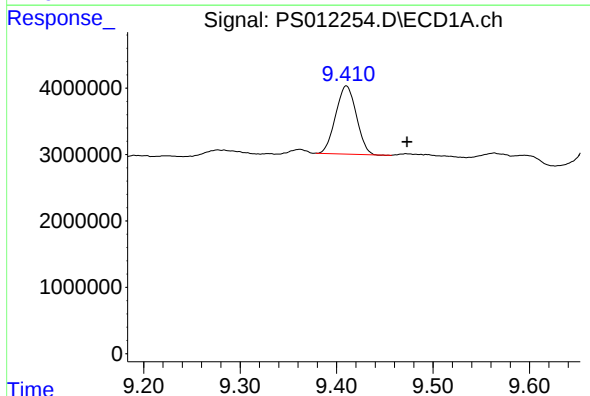


#12 2,4,5-T

R.T.: 9.410 min
Delta R.T.: -0.063 min
Response: 15339881
Conc: 2.50 ng/ml

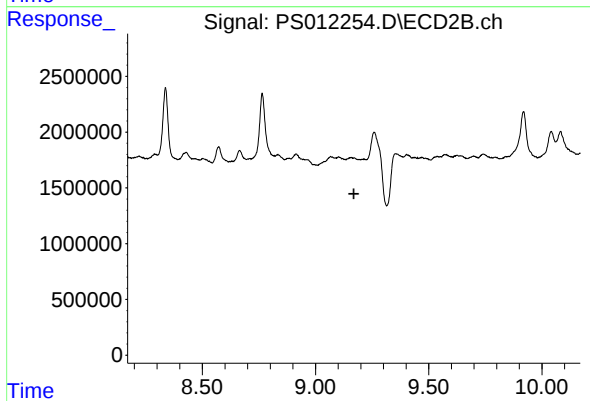

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

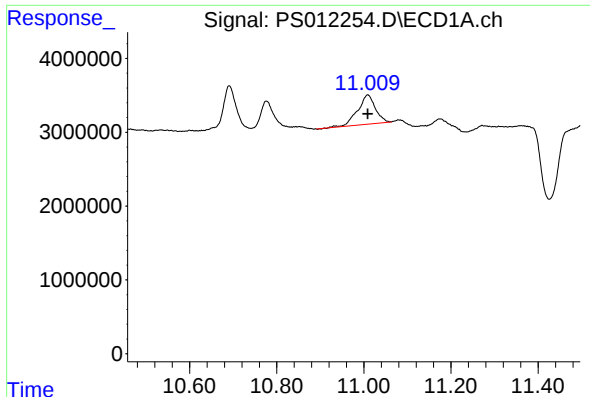

#15 Picloram

R.T.: 11.009 min
Delta R.T.: 0.000 min
Response: 11169286
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

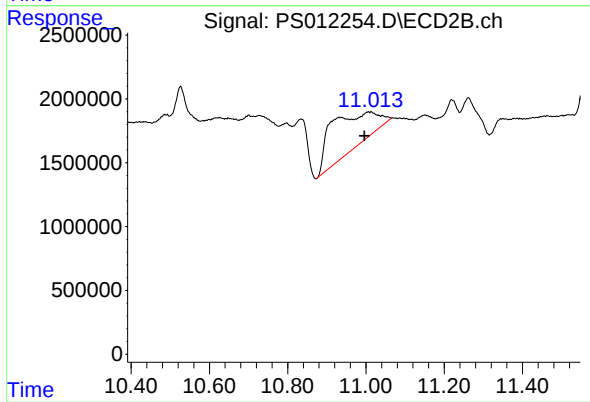

#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.010 min
Response: 22705685
Conc: 5.36 ng/ml