

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 13:50
 Operator : DD\AJ
 Sample : PB131595TB
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 15:50:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	303.8E6	173.9E6	280.263	329.524
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	56283143	N.D.	69.571
3) T	4-Nitroph...	7.107	0.000	8136861	0	15.279	N.D. #
5) T	DICAMBA	7.394	7.046	6898326	10761796	1.639	4.990 #
6) T	MCP	7.567	0.000	5403014	0	1.677	N.D. #
7) T	MCPA	7.685	0.000	337.0E6	0	72.129	N.D. #
8) T	DICHLORPROP	0.000	7.736	0	9175902	N.D.	16.217
9) T	2,4-D	8.395	0.000	103.6E6	0	90.947	N.D. #
11) T	2,4,5-TP ...	0.000	8.760	0	11791801	N.D.	4.074
12) T	2,4,5-T	9.408	0.000	17960491	0	2.928	N.D. #
15) T	Picloram	0.000	11.014	0	7943165	N.D.	1.874
16) T	DCPA	0.000	10.934	0	6740758	N.D.	1.855



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 13:50
Operator : DD\AJ
Sample : PB131595TB
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 15:50:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

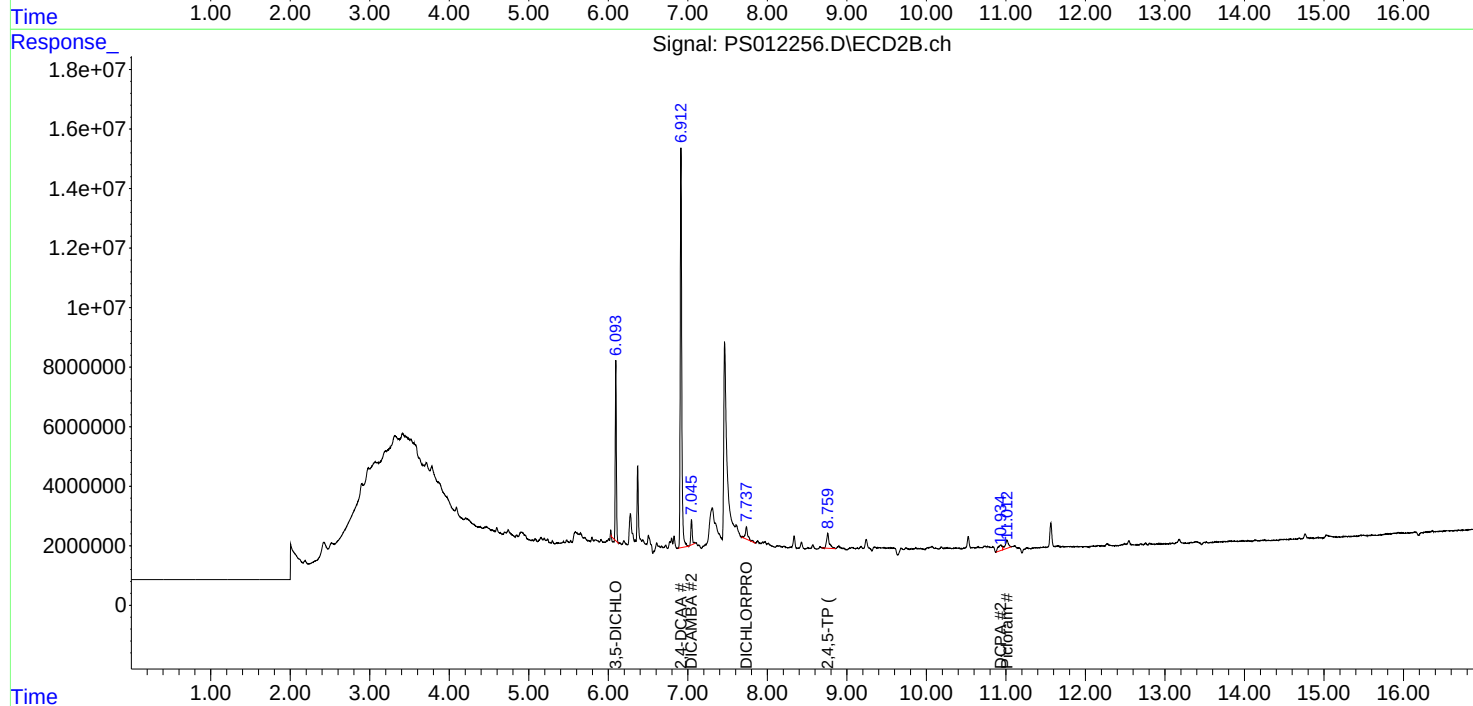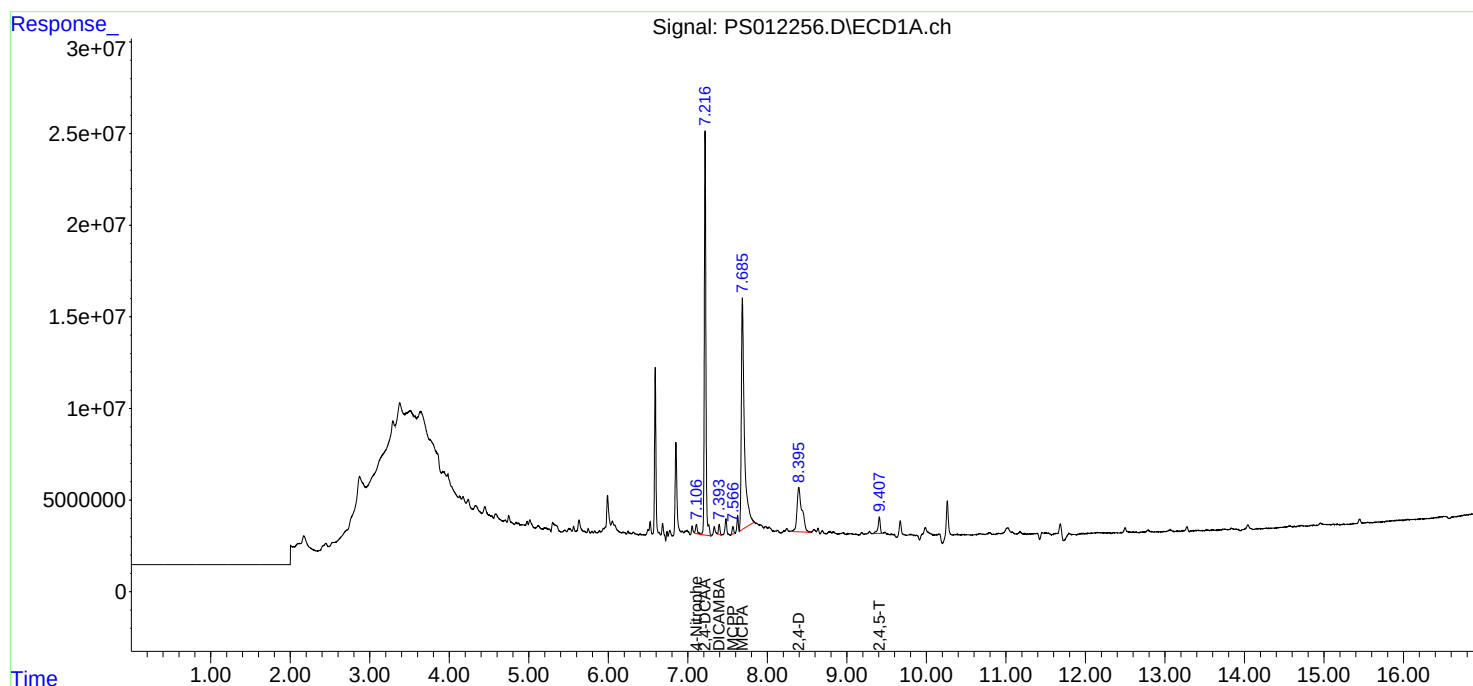


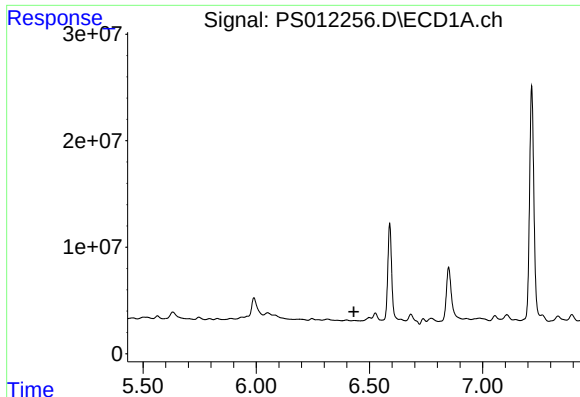

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

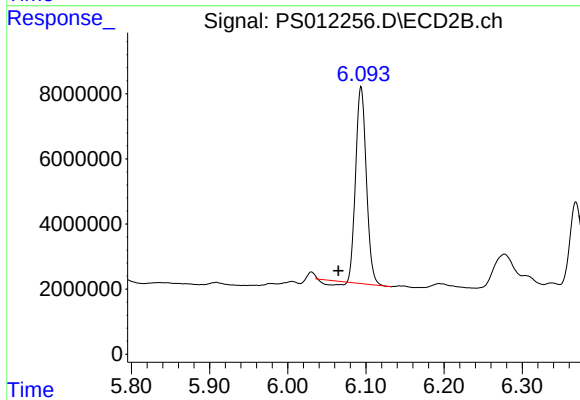


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 56283143
Conc: 69.57 ng/ml

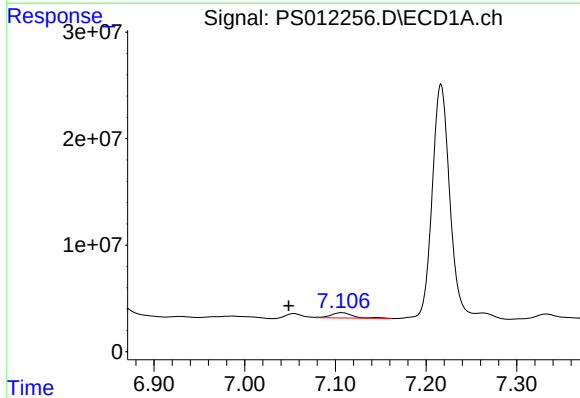


#3 4-Nitrophenol

R.T.: 7.107 min
Delta R.T.: 0.058 min
Response: 8136861
Conc: 15.28 ng/ml

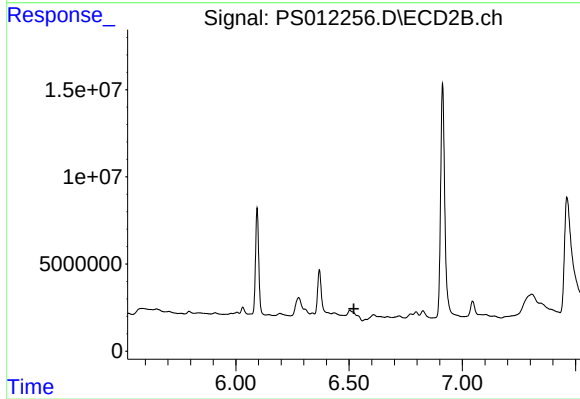

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

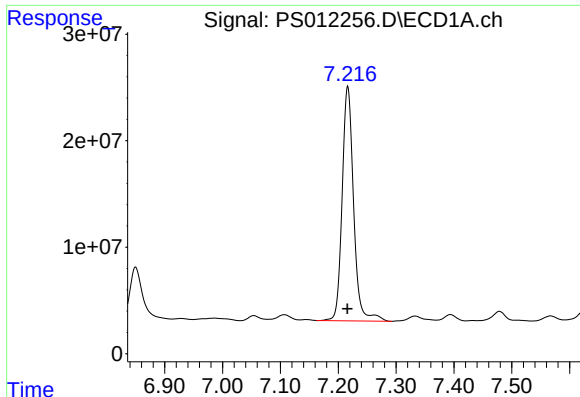

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 303775635
Conc: 280.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

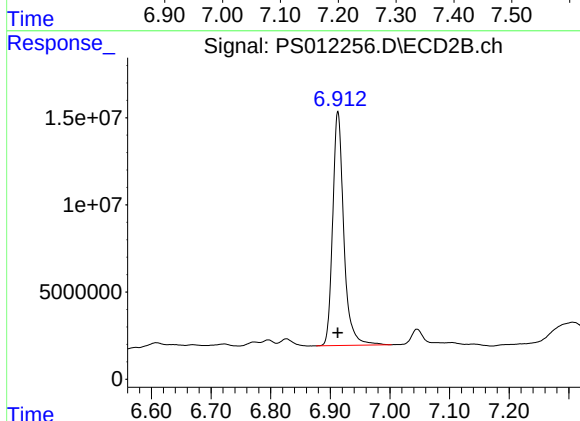


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 173858497
Conc: 329.52 ng/ml

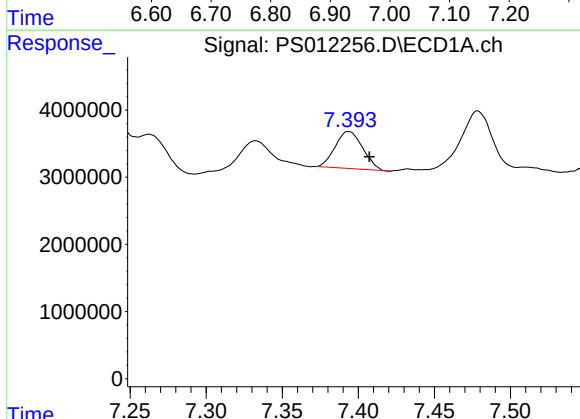


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.014 min
Response: 6898326
Conc: 1.64 ng/ml

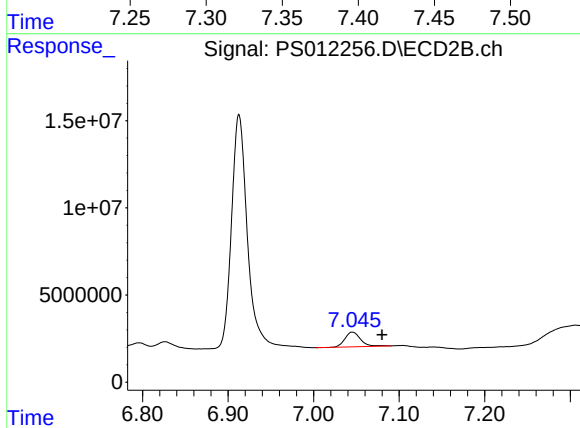

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.035 min
Response: 10761796
Conc: 4.99 ng/ml

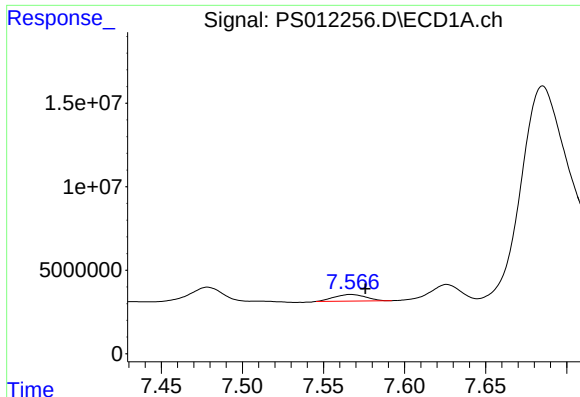

#6 MCPP


R.T.: 7.567 min
Delta R.T.: -0.009 min
Response: 5403014
Conc: 1.68 ug/ml

Instrument :
ECD_S
ClientSampleId :

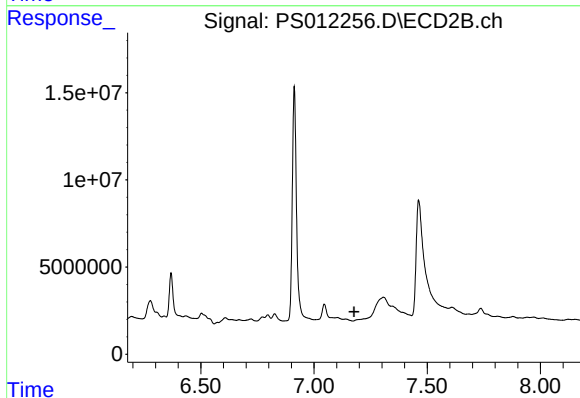


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

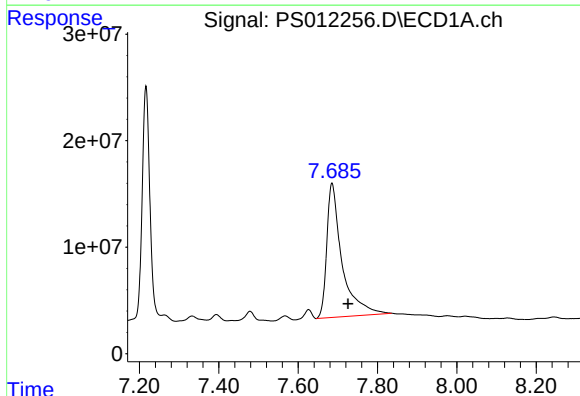


#7 MCPA

R.T.: 7.685 min
Delta R.T.: -0.041 min
Response: 337014984
Conc: 72.13 ug/ml

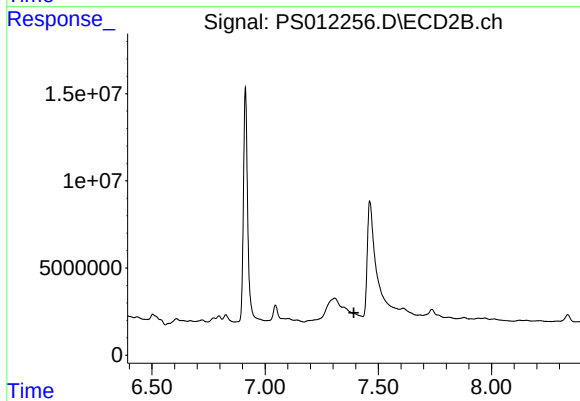

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

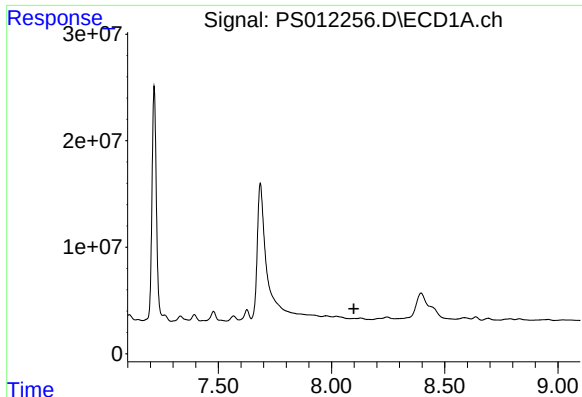

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

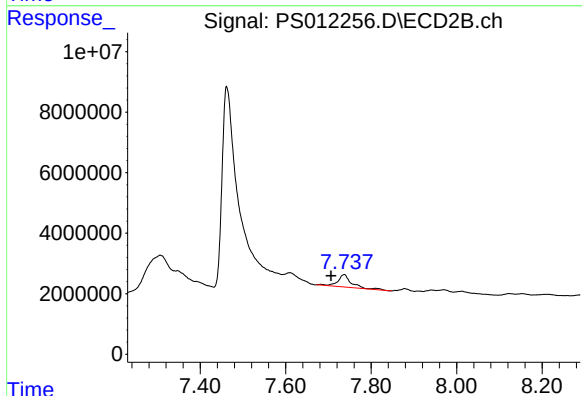


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.031 min
Response: 9175902
Conc: 16.22 ng/ml

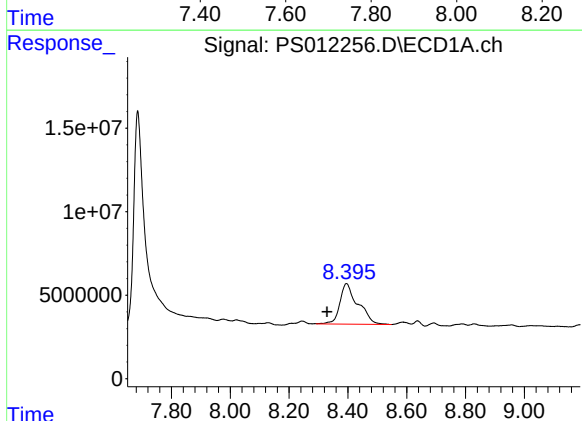


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.066 min
Response: 103584559
Conc: 90.95 ng/ml

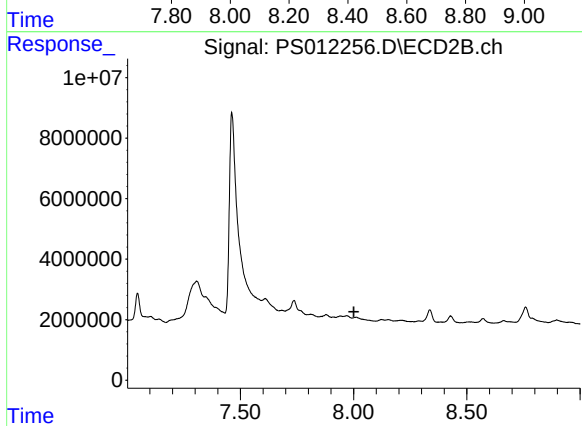

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

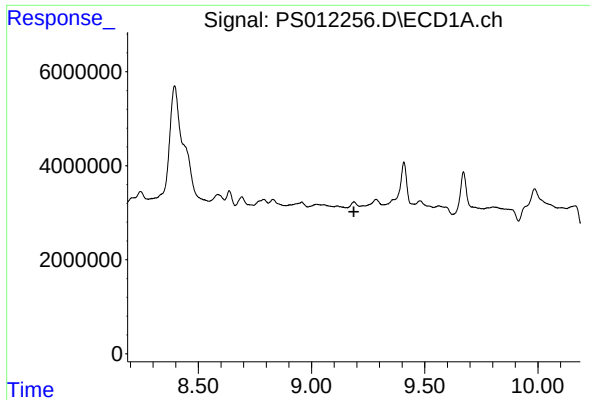

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

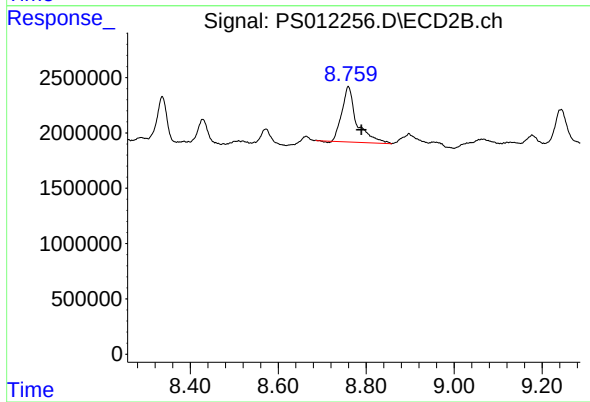


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: -0.030 min
Response: 11791801
Conc: 4.07 ng/ml

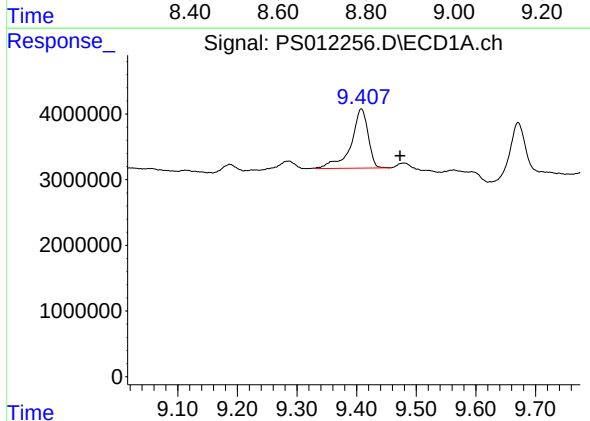


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: -0.065 min
Response: 17960491
Conc: 2.93 ng/ml

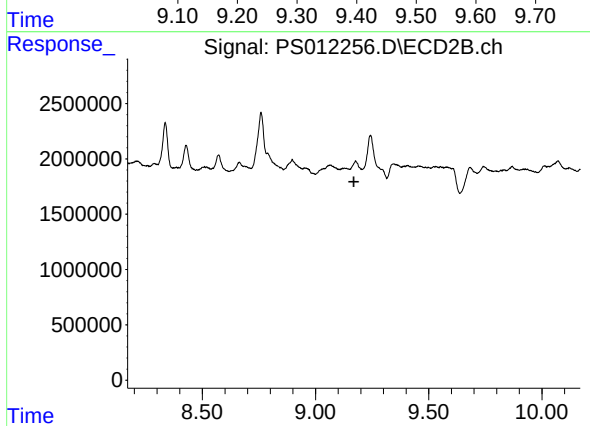

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

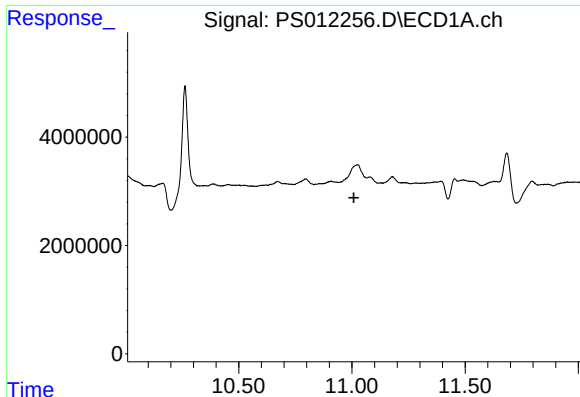

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

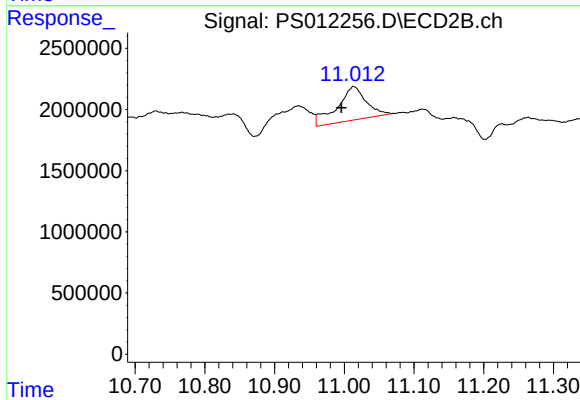


#15 Picloram

R.T.: 11.014 min
Delta R.T.: 0.018 min
Response: 7943165
Conc: 1.87 ng/ml

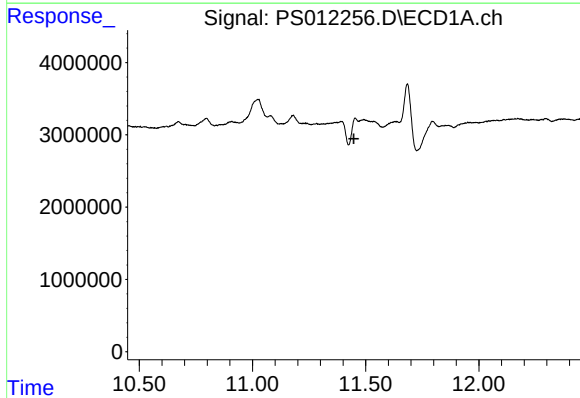

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.448 min
Response: 0
Conc: N.D.

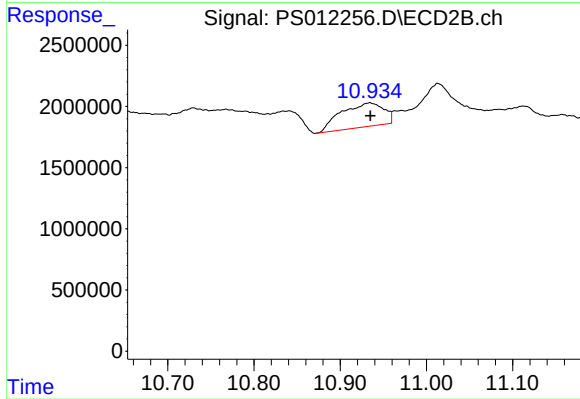

#16 DCPA

R.T.: 10.934 min
Delta R.T.: 0.000 min
Response: 6740758
Conc: 1.85 ng/ml