

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
 Data File : PS012264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2020 16:53
 Operator : DD\AJ
 Sample : L3976-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 15 17:56:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 15 06:03:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.913	324.3E6	187.8E6	299.223	356.039
Target Compounds							
2) T	3,5-DICHL...	0.000	6.094	0	60581570	N.D.	74.885
3) T	4-Nitroph...	7.053	0.000	3138623	0	5.894	N.D. #
5) T	DICAMBA	7.394	7.046	7589003	12191883	1.804	5.653 #
6) T	MCP	7.626	0.000	13267746	0	4.118	N.D. #
7) T	MCPA	7.689	0.000	276.8E6	0	59.236	N.D. #
8) T	DICHLORPROP	0.000	7.737	0	8916366	N.D.	15.759
9) T	2,4-D	8.395	0.000	98418510	0	86.411	N.D. #
11) T	2,4,5-TP ...	0.000	8.760	0	12610759	N.D.	4.357
12) T	2,4,5-T	9.409	0.000	18556426	0	3.026	N.D. #
14) T	DINOSEB	0.000	10.071	0	7064685	N.D.	3.402
15) T	Picloram	11.001	11.016	9833160	18634710	1.335	4.396 #
16) T	DCPA	11.455	0.000	3148297	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091520\
Data File : PS012264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2020 16:53
Operator : DD\AJ
Sample : L3976-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 15 17:56:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091420.M
Quant Title : 8080.M
QLast Update : Tue Sep 15 06:03:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

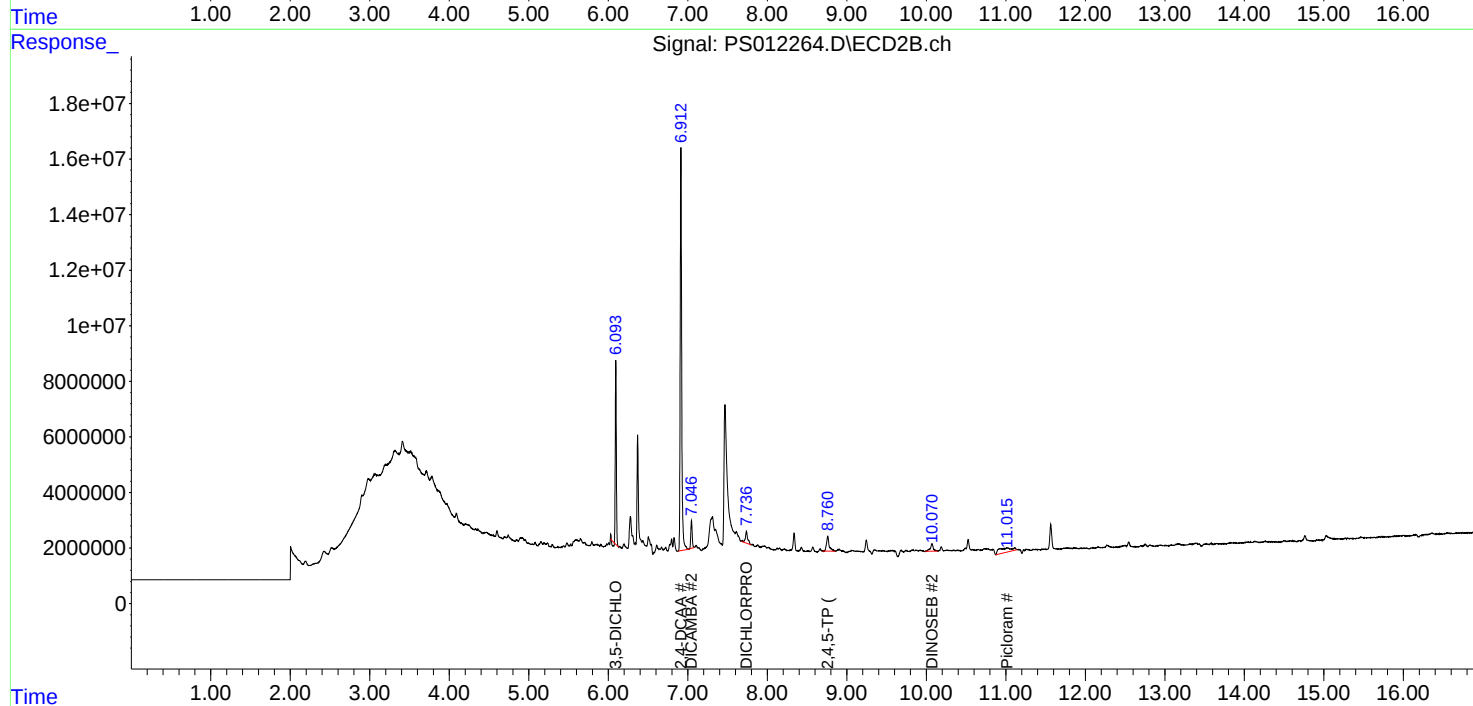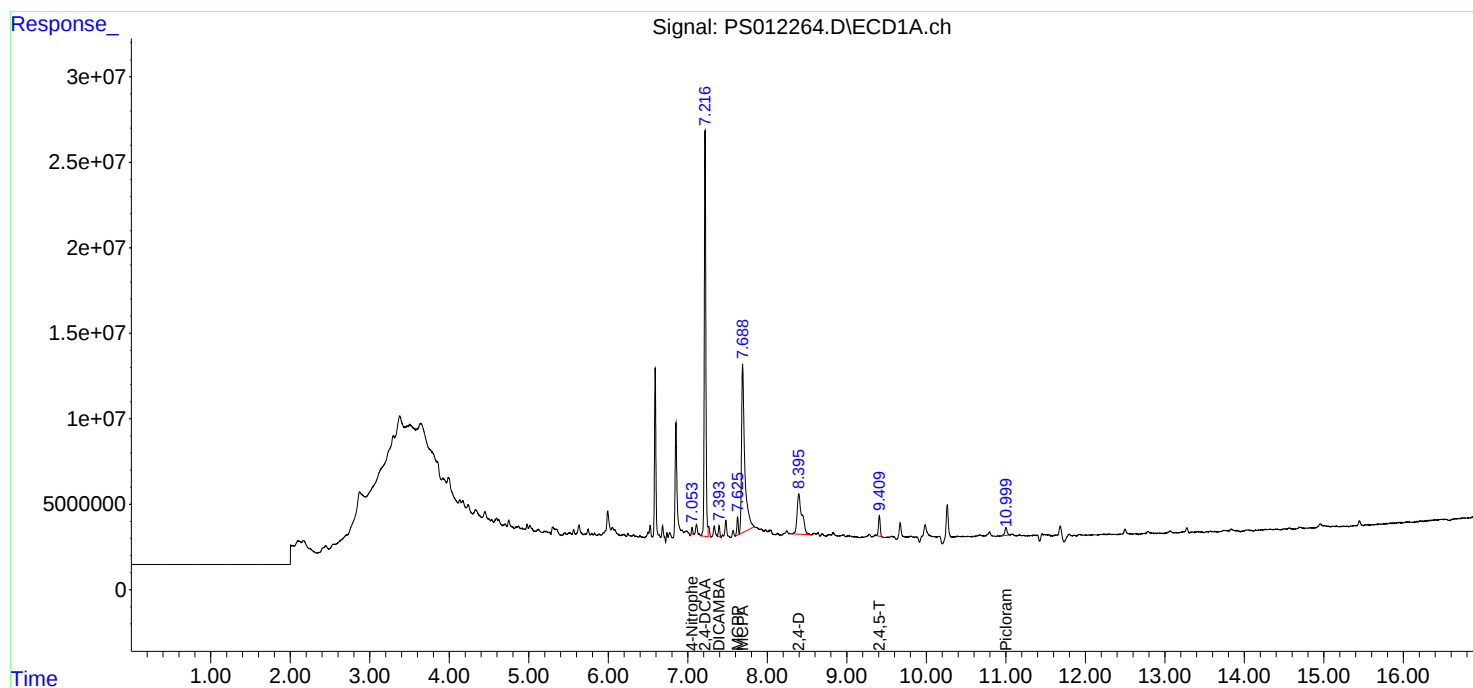


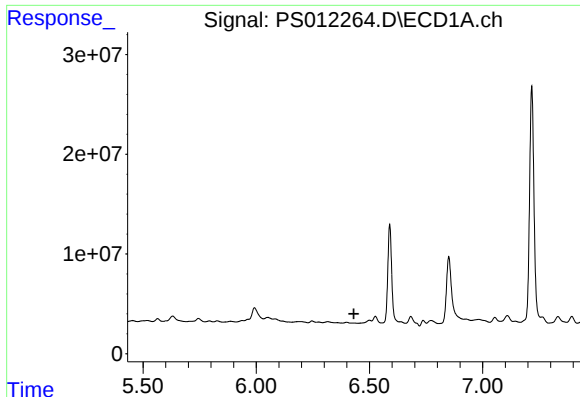

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

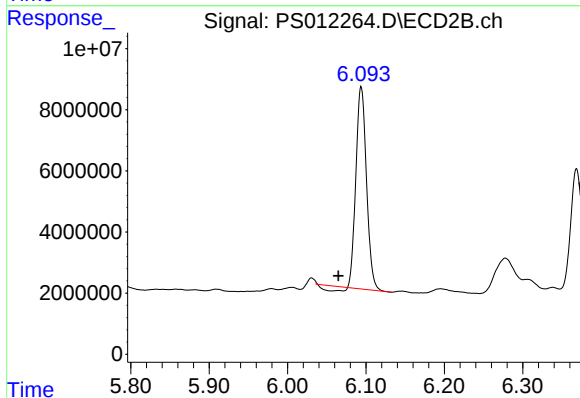


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 60581570
Conc: 74.88 ng/ml

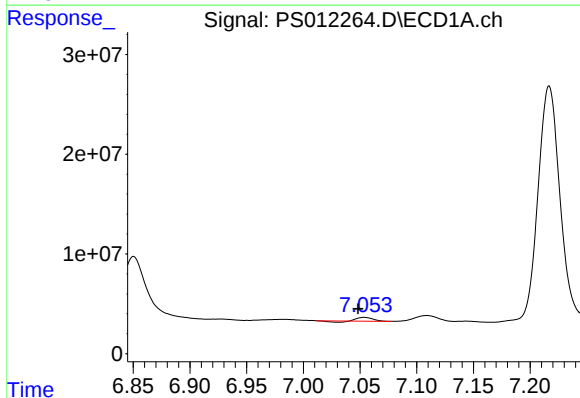


#3 4-Nitrophenol

R.T.: 7.053 min
Delta R.T.: 0.005 min
Response: 3138623
Conc: 5.89 ng/ml

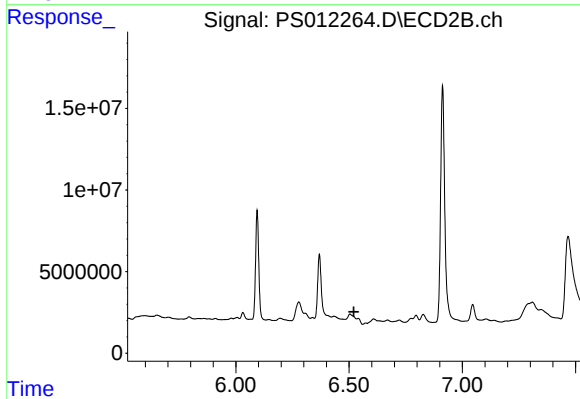

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.522 min
Response: 0
Conc: N.D.

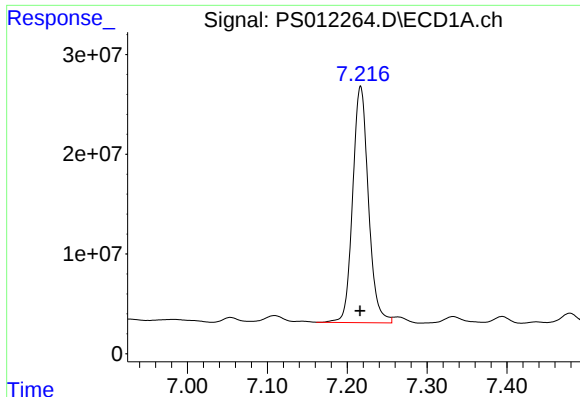

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 324326996
Conc: 299.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

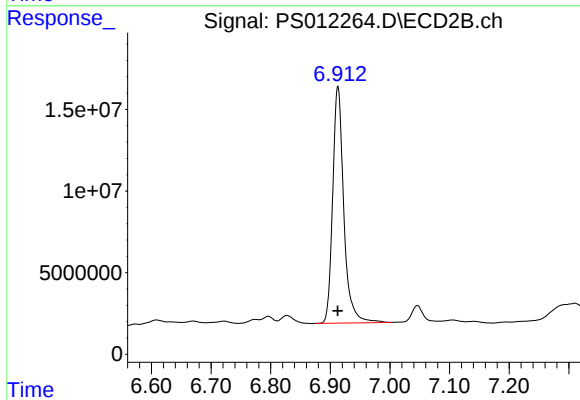


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 187848180
Conc: 356.04 ng/ml

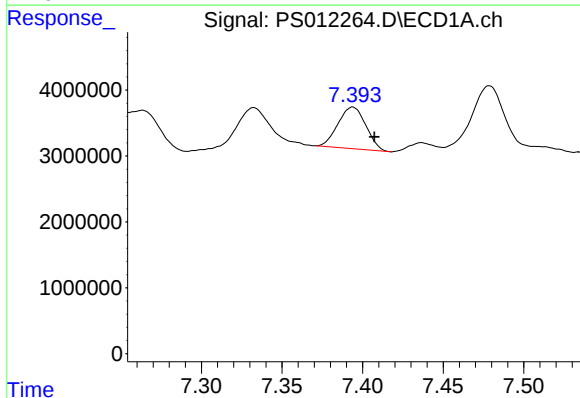


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: -0.013 min
Response: 7589003
Conc: 1.80 ng/ml

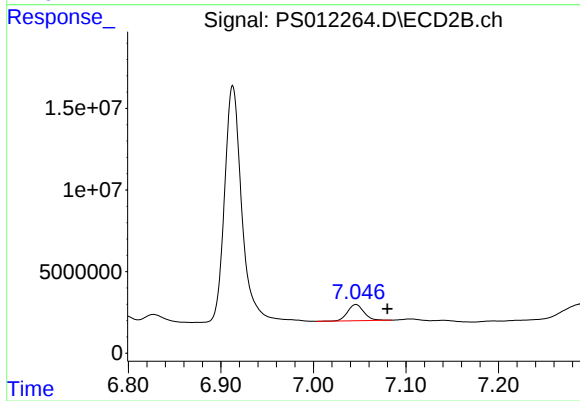

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 12191883
Conc: 5.65 ng/ml

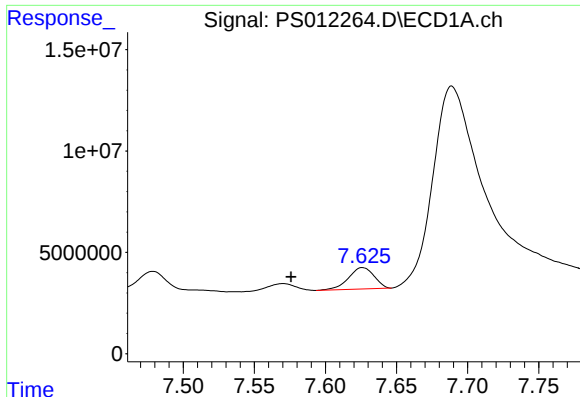

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.050 min
Response: 13267746
Conc: 4.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

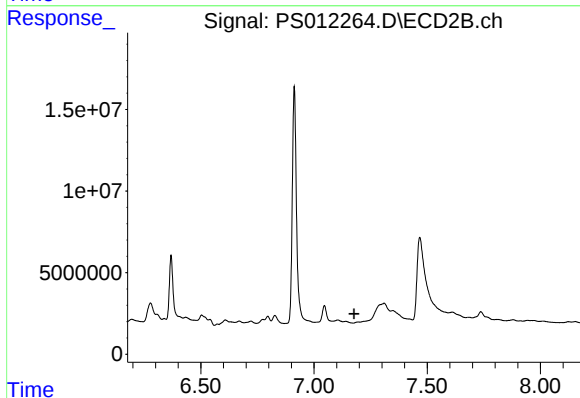


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.177 min
Response: 0
Conc: N.D.

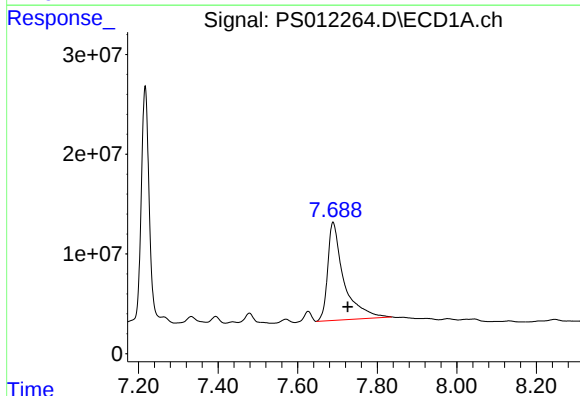


#7 MCPA

R.T.: 7.689 min
Delta R.T.: -0.037 min
Response: 276772336
Conc: 59.24 ug/ml

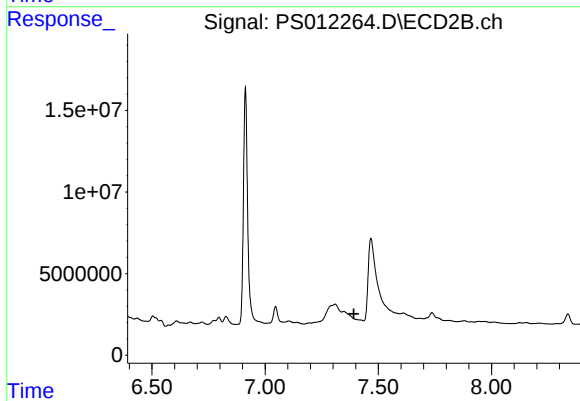

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

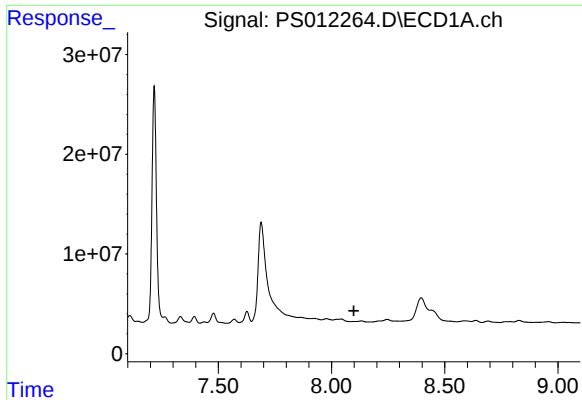

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

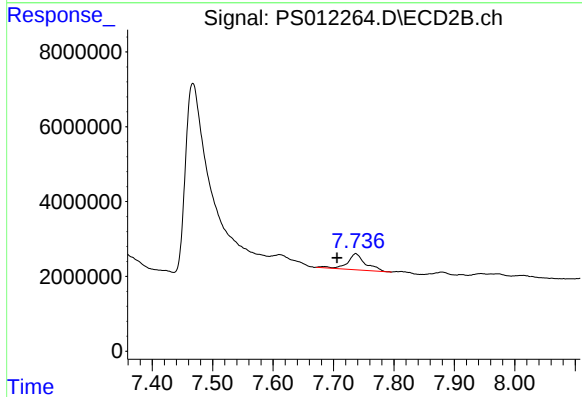


#8 DICHLORPROP

R.T.: 7.737 min
Delta R.T.: 0.031 min
Response: 8916366
Conc: 15.76 ng/ml

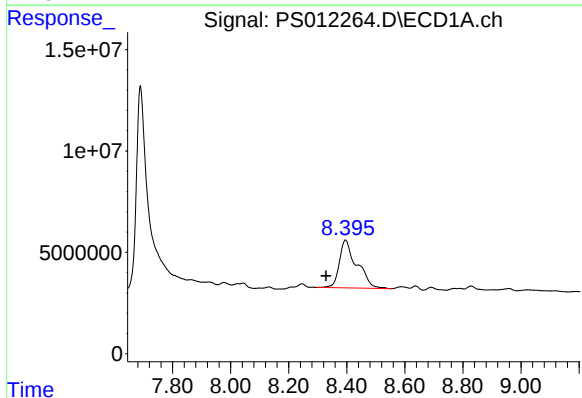


#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.066 min
Response: 98418510
Conc: 86.41 ng/ml

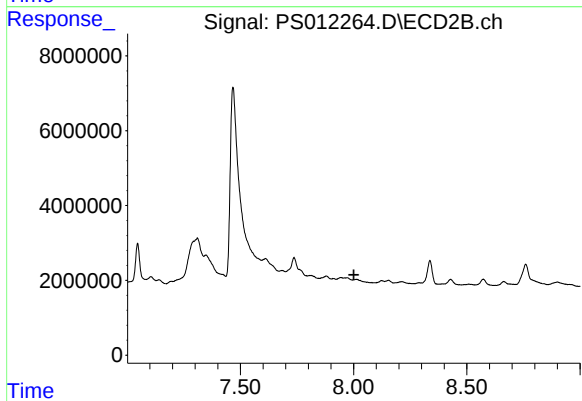

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

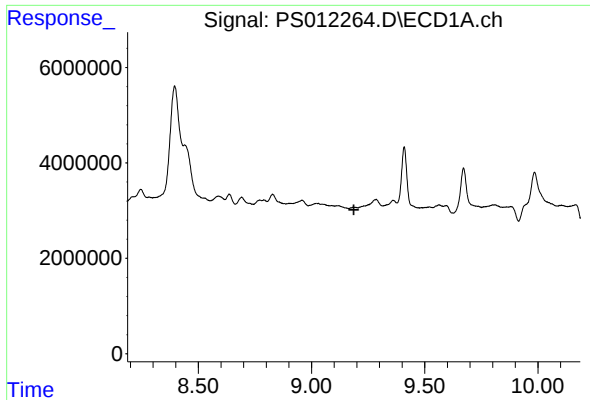

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

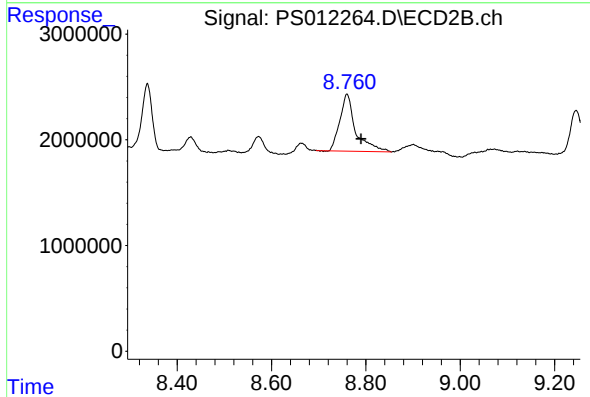


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: -0.029 min
Response: 12610759
Conc: 4.36 ng/ml

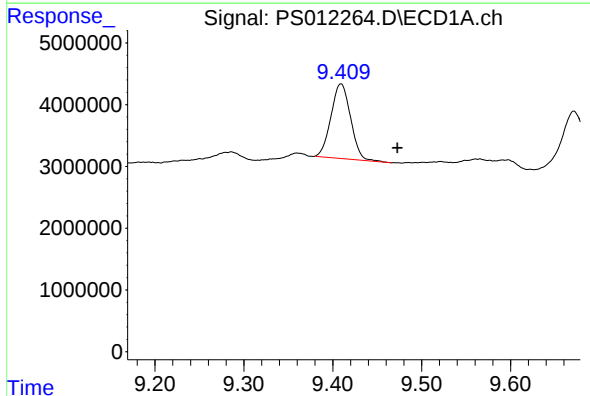


#12 2,4,5-T

R.T.: 9.409 min
Delta R.T.: -0.064 min
Response: 18556426
Conc: 3.03 ng/ml

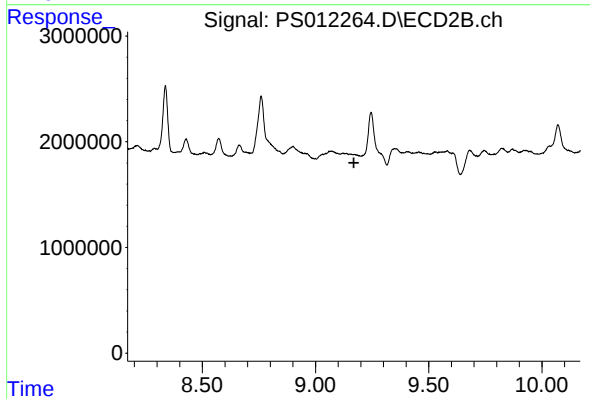

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

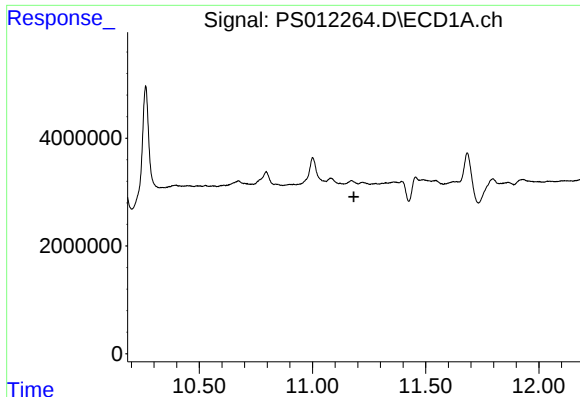

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

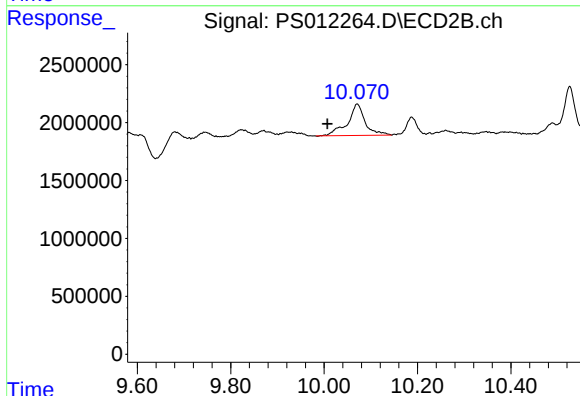


#14 DINOSEB

R.T.: 10.071 min
Delta R.T.: 0.064 min
Response: 7064685
Conc: 3.40 ng/ml

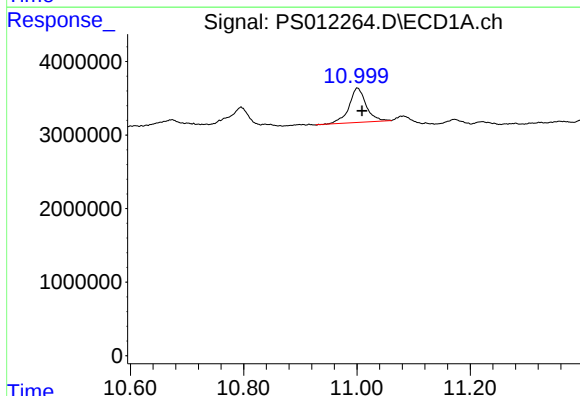

#15 Picloram

R.T.: 11.001 min
Delta R.T.: -0.008 min
Response: 9833160
Conc: 1.34 ng/ml

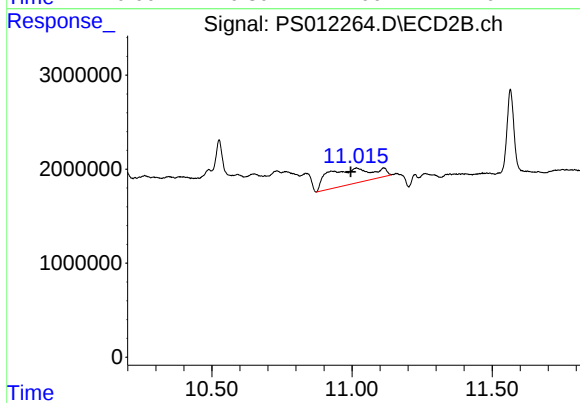

#15 Picloram

R.T.: 11.016 min
Delta R.T.: 0.020 min
Response: 18634710
Conc: 4.40 ng/ml